

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071625\
 Data File : PP073845.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2025 10:34
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 11:36:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.522f	3.812f	390661	63820	0.285	0.035 #
2)	SA Decachlor...	10.169	8.773	72065	361668	0.066	0.273 #
Target Compounds							
3)	L1 AR-1016-1	5.647	4.858	73586	94932	1.549	1.392
4)	L1 AR-1016-2	5.668	4.864	148930	41095	2.091	0.403 #
5)	L1 AR-1016-3	5.728	5.037	241762	327174	5.537	6.047
6)	L1 AR-1016-4	5.824	5.091	55724	679302	1.550	15.481 #
7)	L1 AR-1016-5	6.125	5.315	629422	245924	20.090	4.506 #
8)	L2 AR-1221-1	4.675	3.985	78615	65151	4.400	2.409 #
9)	L2 AR-1221-2	4.754	4.072	282284	74026	20.903	3.636 #
10)	L2 AR-1221-3	4.863	4.160	109480	50820	2.631	0.827 #
11)	L3 AR-1232-1	4.863	4.160	109480	50820	3.353	1.090 #
12)	L3 AR-1232-2	5.376	4.864	136242	41095	8.382	0.862 #
13)	L3 AR-1232-3	5.668	5.037	148930	327174	4.514	13.072 #
14)	L3 AR-1232-4	5.824	5.132	55724	113886	3.389	5.259 #
15)	L3 AR-1232-5	5.886	5.315	219266	245924	20.743	10.899 #
16)	L4 AR-1242-1	5.628	4.858	114905	94932	3.009	1.643 #
17)	L4 AR-1242-2	5.668	4.864	148930	41095	2.487	0.475 #
18)	L4 AR-1242-3	5.728	5.037	241762	327174	6.602	7.121
19)	L4 AR-1242-4	5.824	5.132	55724	113886	1.734	2.573 #
20)	L4 AR-1242-5	6.558	5.641	115341	522392	3.523	9.456 #
21)	L5 AR-1248-1	5.628	4.858	114905	94932	3.722	2.115 #
22)	L5 AR-1248-2	5.886	5.091	219266	679302	5.492	11.039 #
23)	L5 AR-1248-3	6.125	5.132	629422	113886	14.173	1.778 #
24)	L5 AR-1248-4	6.502	5.315	205619	245924	3.733	3.263
25)	L5 AR-1248-5	6.558	5.678	115341	894506	2.144	11.992 #
26)	L6 AR-1254-1	6.502	5.641	205619	522392	3.837	4.502
27)	L6 AR-1254-2	6.695	5.821	3789522	6687870	45.499	66.464 #
28)	L6 AR-1254-3	7.066	6.218	3772148	3296338	42.704	21.343 #
29)	L6 AR-1254-4	7.329	6.445	563098	428007	7.158	4.526 #
30)	L6 AR-1254-5	7.778	6.844	431.0E6	771.1E6	5849.373	5778.442
31)	L7 AR-1260-1	7.231	6.356	266065	39460	4.513	0.404 #
32)	L7 AR-1260-2	7.466	6.524	675.9E6	6278823	7052.493	51.115 #
33)	L7 AR-1260-3	7.778f	6.651	431.0E6	-144334	5898.138	N.D. #
34)	L7 AR-1260-4	8.057	7.130	96541	70676	1.478	0.790 #
35)	L7 AR-1260-5	8.382	7.396	69140	180525	0.458	0.803 #
36)	L8 AR-1262-1	8.057	6.844f	96541	771.1E6	1.109	5221.034 #
37)	L8 AR-1262-2	8.382	7.130	69140	70676	0.349	0.553 #
38)	L8 AR-1262-3	8.693	7.681	593626	817547	4.722	7.170 #
39)	L8 AR-1262-4	8.791	7.711	1011089	323284	10.841	1.757 #
40)	L8 AR-1262-5	9.436	8.193f	191038	22102	3.014	0.262 #
41)	L9 AR-1268-1	8.693	7.681	593626	817547	2.659	2.660

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071625\
Data File : PP073845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2025 10:34
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 11:36:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.791	7.711	1011089	323284	5.307	1.217 #
43)	L9 AR-1268-3	9.013	7.948	2284112	80343	13.795	0.356 #
44)	L9 AR-1268-4	9.436	8.193f	191038	22102	2.747	0.238 #
45)	L9 AR-1268-5	9.885f	8.531	493070	99601	1.070	0.162 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071625\
Data File : PP073845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2025 10:34
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 11:36:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

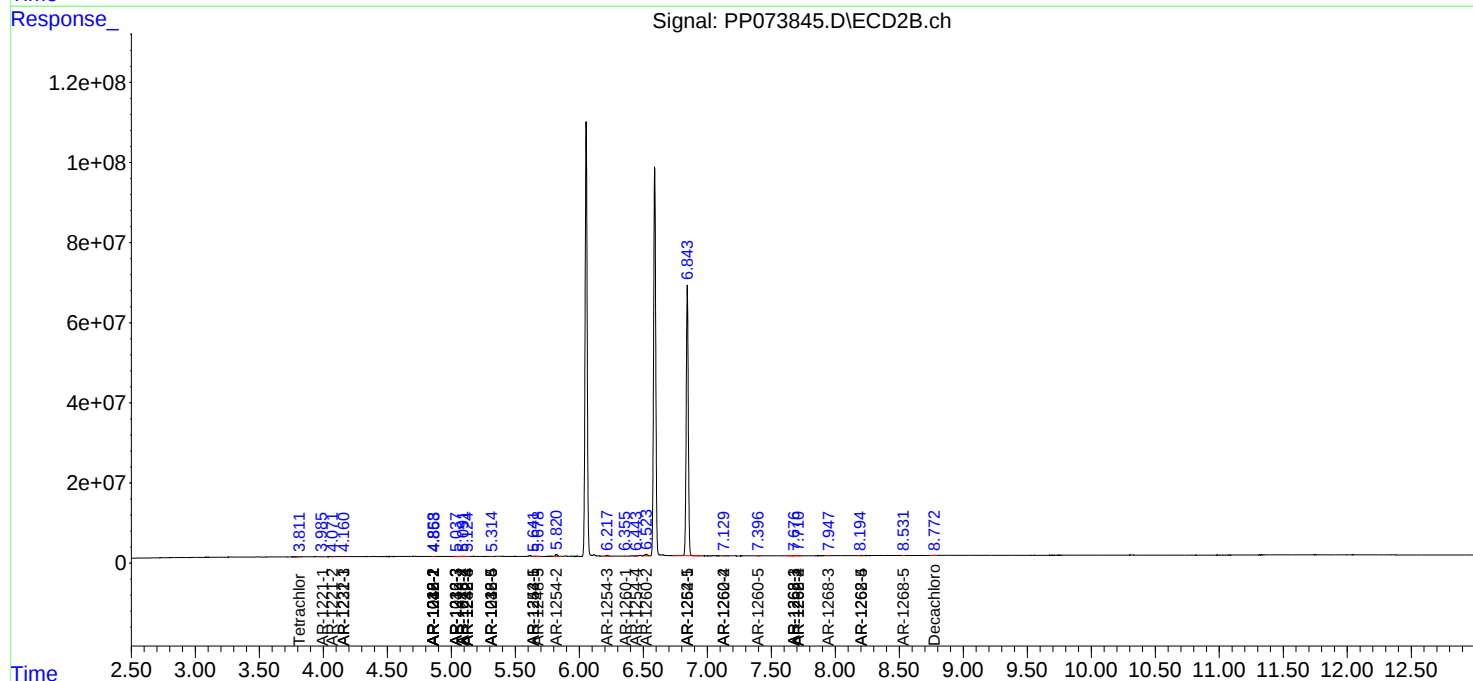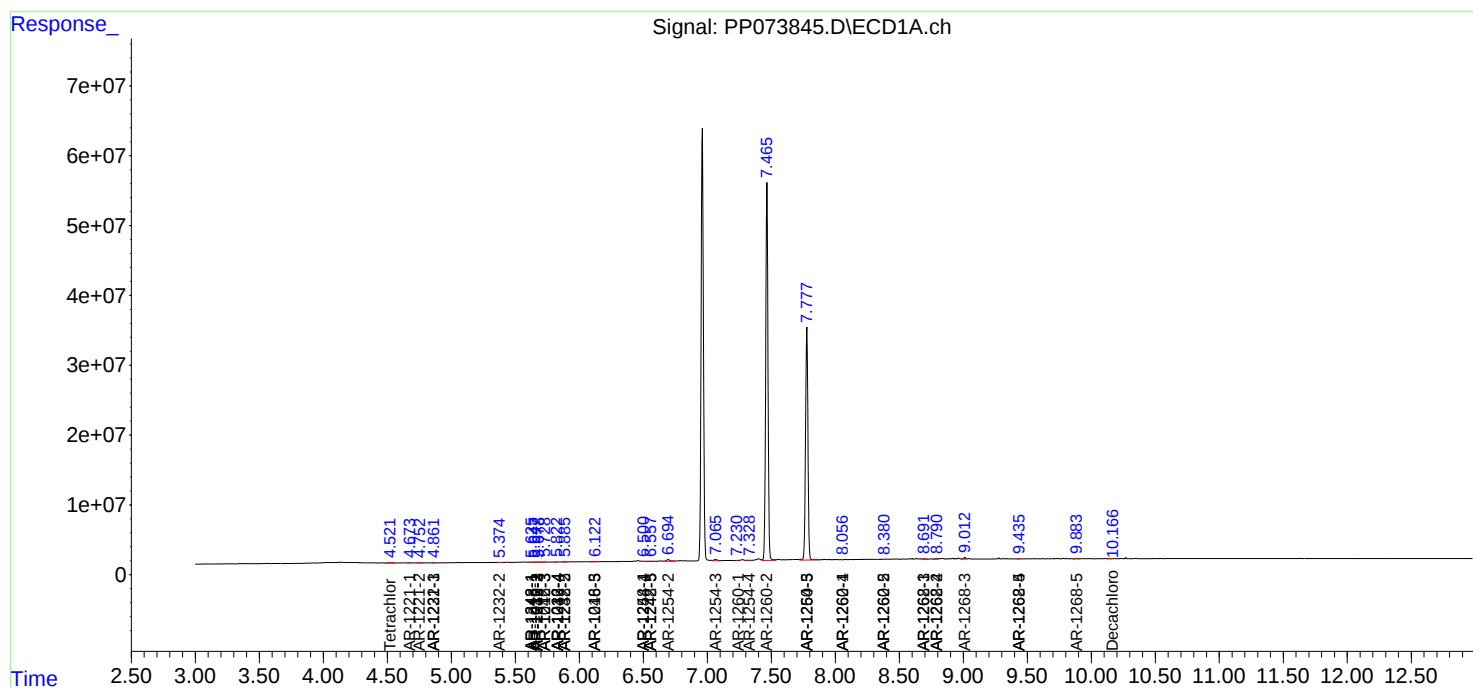


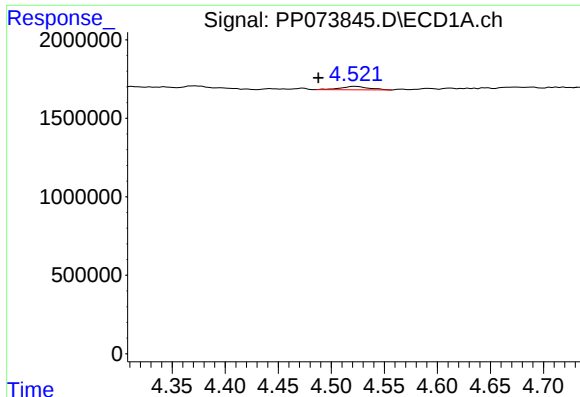

#1 Tetrachloro-m-xylene


R.T.: 4.522 min
Delta R.T.: 0.034 min
Response: 390661
Conc: 0.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

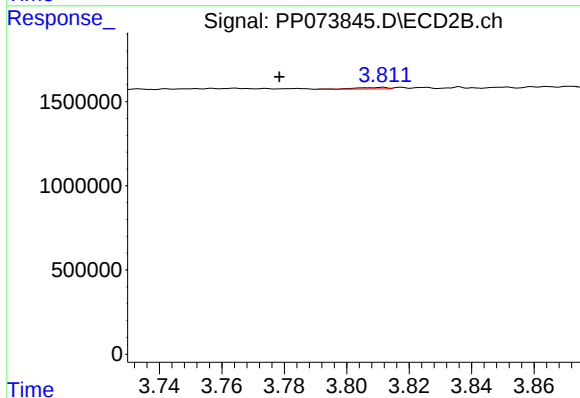


#1 Tetrachloro-m-xylene

R.T.: 3.812 min
Delta R.T.: 0.033 min
Response: 63820
Conc: 0.03 ng/ml

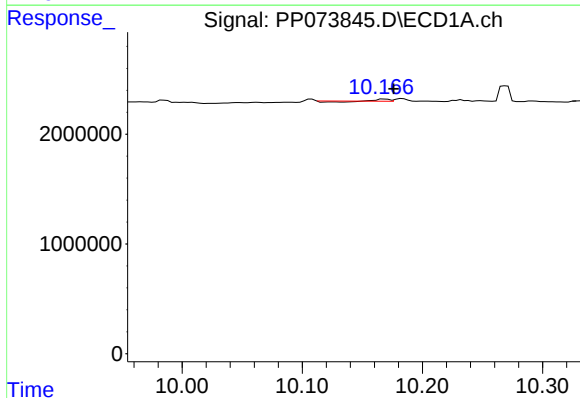


#2 Decachlorobiphenyl

R.T.: 10.169 min
Delta R.T.: -0.007 min
Response: 72065
Conc: 0.07 ng/ml

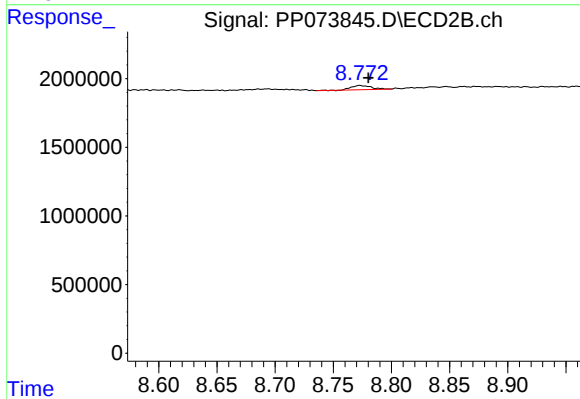

#2 Decachlorobiphenyl


R.T.: 8.773 min
Delta R.T.: -0.007 min
Response: 361668
Conc: 0.27 ng/ml

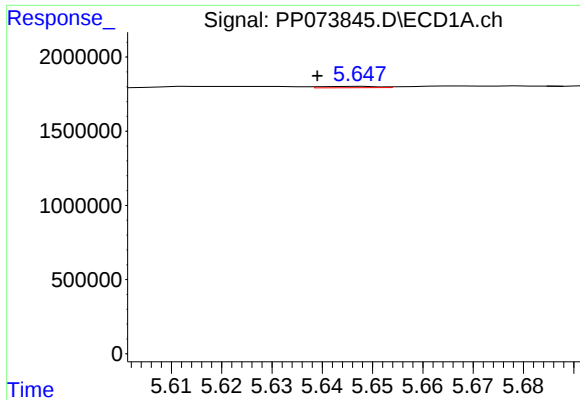

#3 AR-1016-1


R.T.: 5.647 min
Delta R.T.: 0.008 min
Response: 73586
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

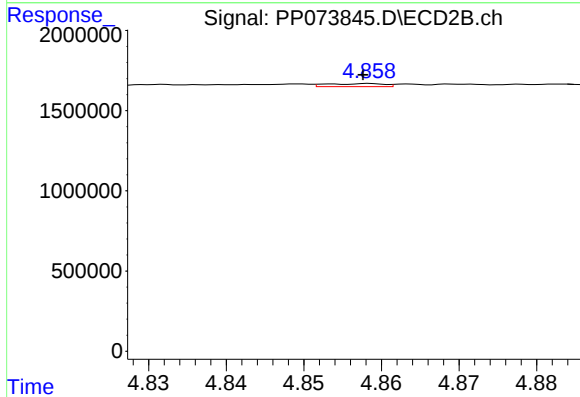


#3 AR-1016-1

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 94932
Conc: 1.39 ng/ml

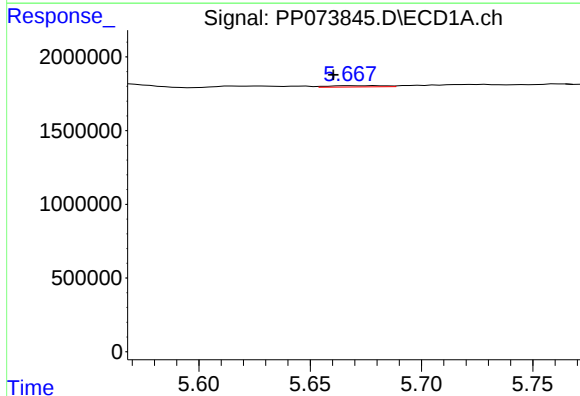


#4 AR-1016-2

R.T.: 5.668 min
Delta R.T.: 0.008 min
Response: 148930
Conc: 2.09 ng/ml

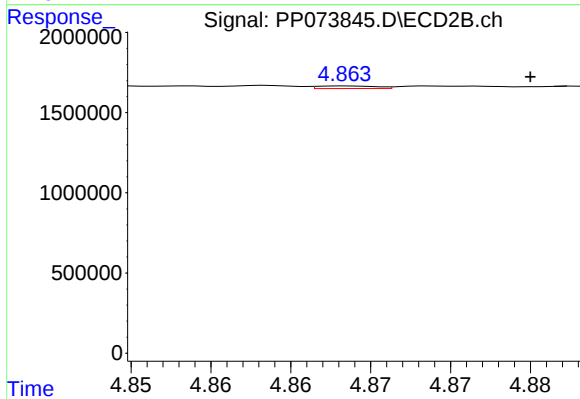

#4 AR-1016-2


R.T.: 4.864 min
Delta R.T.: -0.011 min
Response: 41095
Conc: 0.40 ng/ml

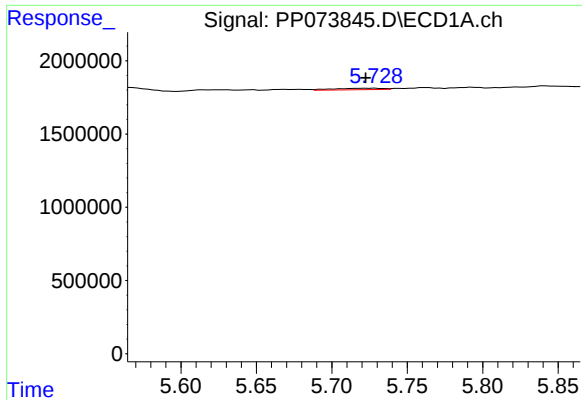

#5 AR-1016-3


R.T.: 5.728 min
Delta R.T.: 0.006 min
Response: 241762
Conc: 5.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

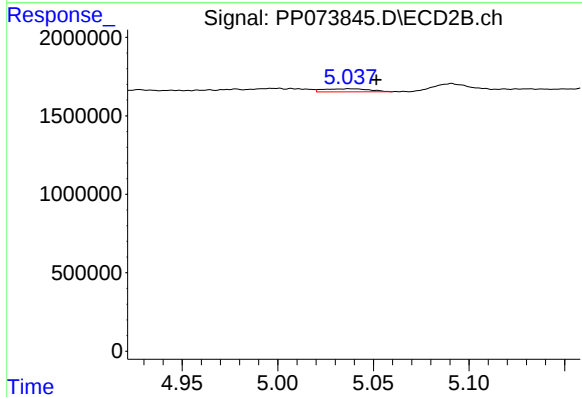


#5 AR-1016-3

R.T.: 5.037 min
Delta R.T.: -0.014 min
Response: 327174
Conc: 6.05 ng/ml

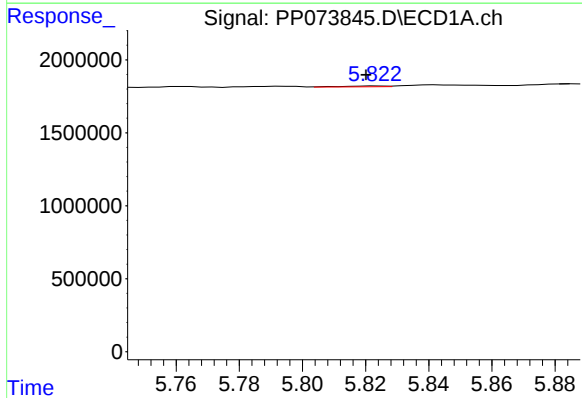


#6 AR-1016-4

R.T.: 5.824 min
Delta R.T.: 0.004 min
Response: 55724
Conc: 1.55 ng/ml

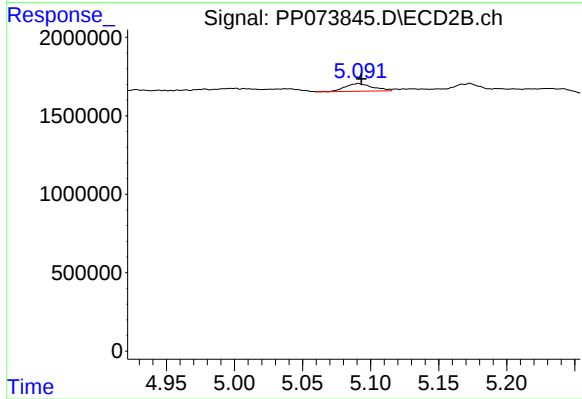

#6 AR-1016-4


R.T.: 5.091 min
Delta R.T.: -0.002 min
Response: 679302
Conc: 15.48 ng/ml

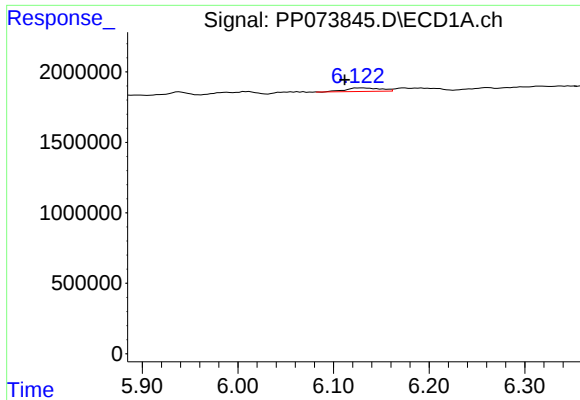

#7 AR-1016-5


R.T.: 6.125 min
Delta R.T.: 0.013 min
Response: 629422
Conc: 20.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

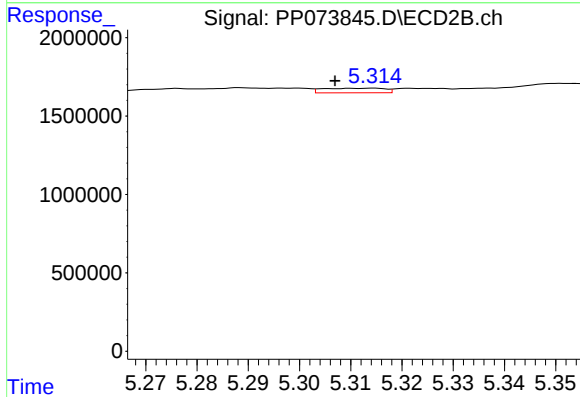


#7 AR-1016-5

R.T.: 5.315 min
Delta R.T.: 0.008 min
Response: 245924
Conc: 4.51 ng/ml

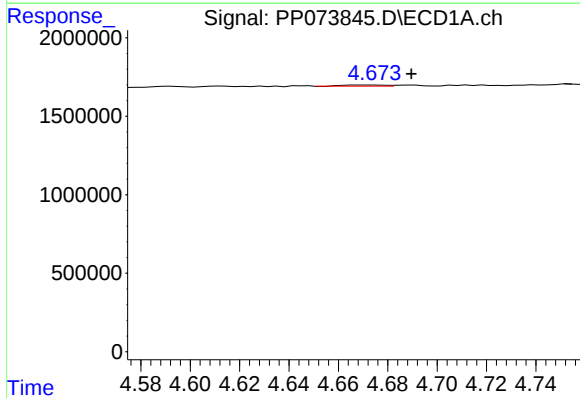


#8 AR-1221-1

R.T.: 4.675 min
Delta R.T.: -0.015 min
Response: 78615
Conc: 4.40 ng/ml

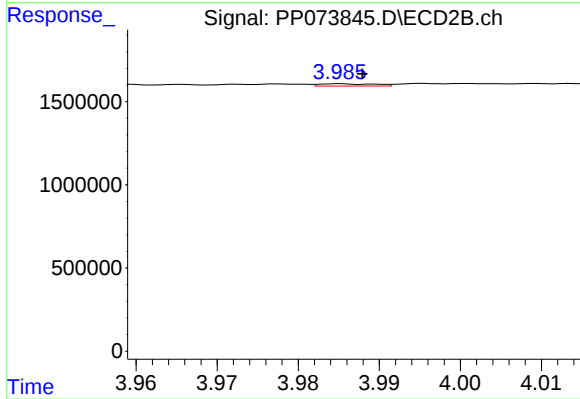

#8 AR-1221-1


R.T.: 3.985 min
Delta R.T.: -0.003 min
Response: 65151
Conc: 2.41 ng/ml

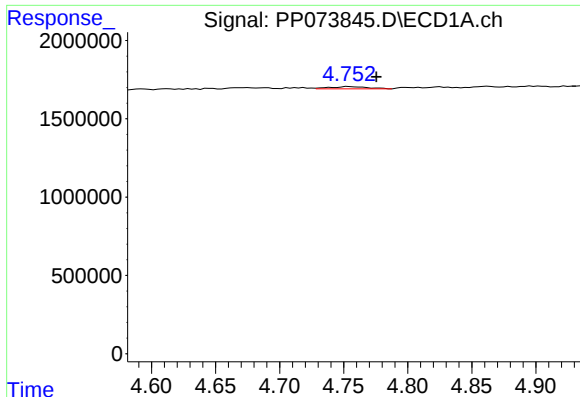

#9 AR-1221-2


R.T.: 4.754 min
Delta R.T.: -0.022 min
Response: 282284
Conc: 20.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

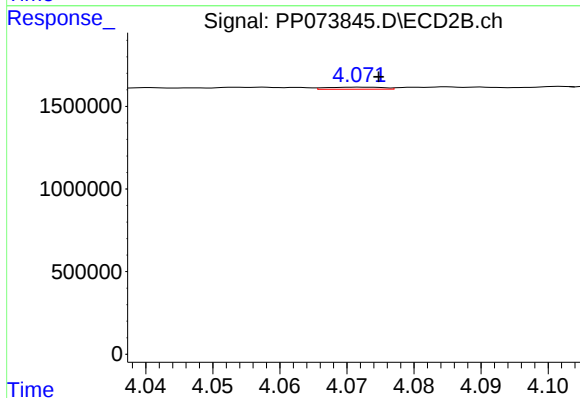


#9 AR-1221-2

R.T.: 4.072 min
Delta R.T.: -0.003 min
Response: 74026
Conc: 3.64 ng/ml

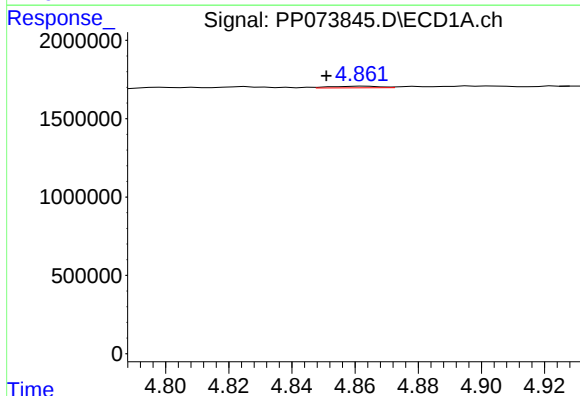


#10 AR-1221-3

R.T.: 4.863 min
Delta R.T.: 0.012 min
Response: 109480
Conc: 2.63 ng/ml

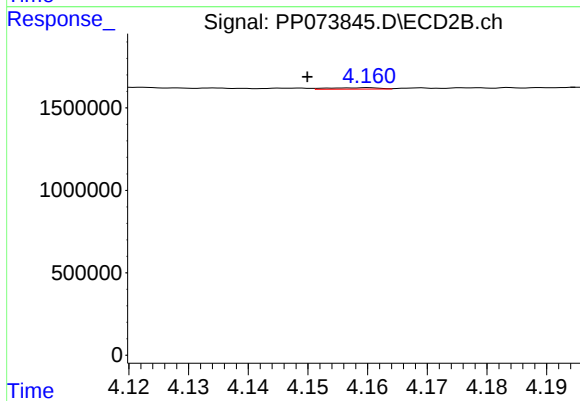

#10 AR-1221-3


R.T.: 4.160 min
Delta R.T.: 0.010 min
Response: 50820
Conc: 0.83 ng/ml

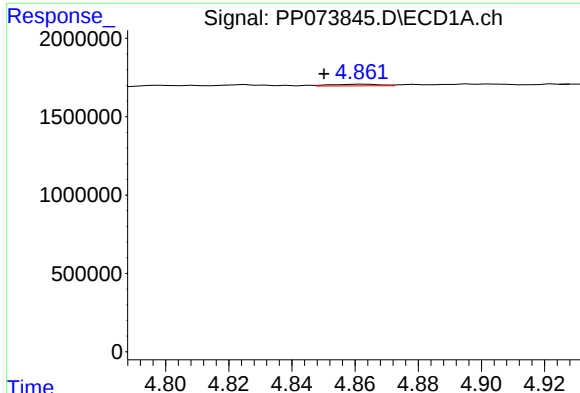

#11 AR-1232-1


R.T.: 4.863 min
Delta R.T.: 0.013 min
Response: 109480
Conc: 3.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

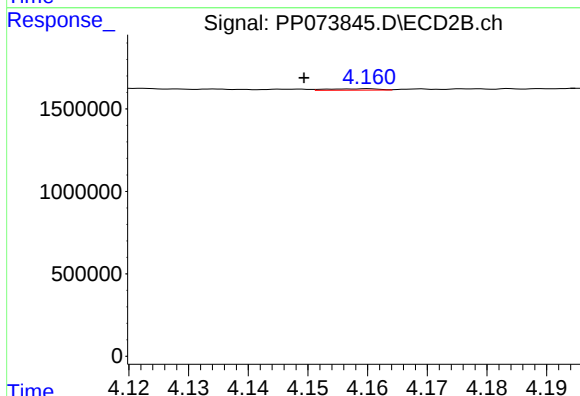


#11 AR-1232-1

R.T.: 4.160 min
Delta R.T.: 0.011 min
Response: 50820
Conc: 1.09 ng/ml

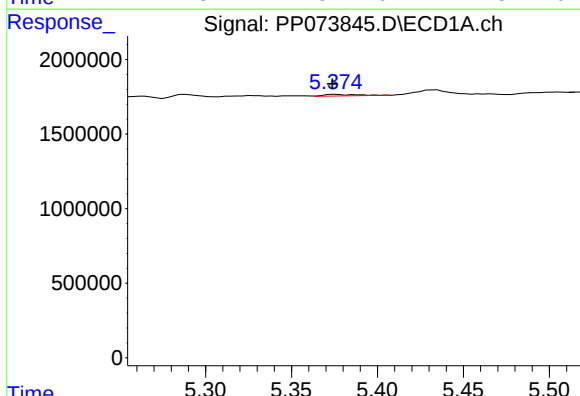


#12 AR-1232-2

R.T.: 5.376 min
Delta R.T.: 0.002 min
Response: 136242
Conc: 8.38 ng/ml

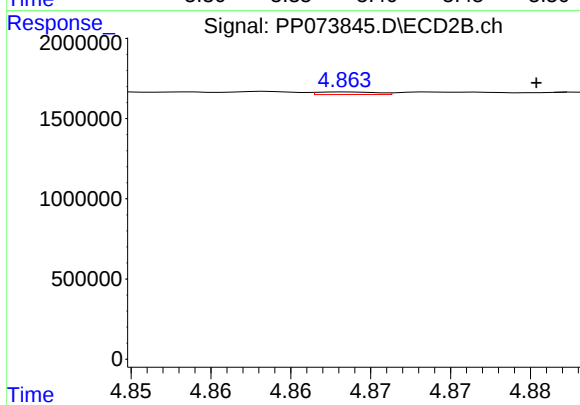

#12 AR-1232-2


R.T.: 4.864 min
Delta R.T.: -0.012 min
Response: 41095
Conc: 0.86 ng/ml

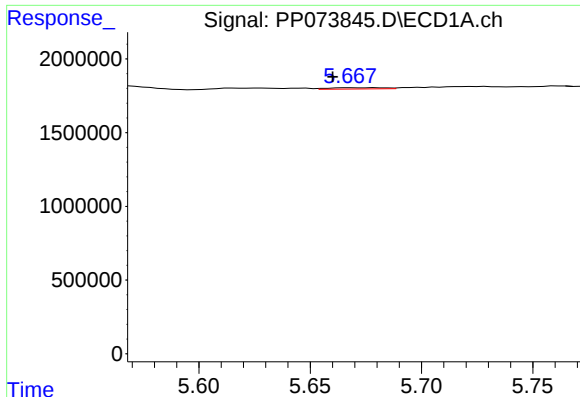

#13 AR-1232-3


R.T.: 5.668 min
Delta R.T.: 0.008 min
Response: 148930
Conc: 4.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

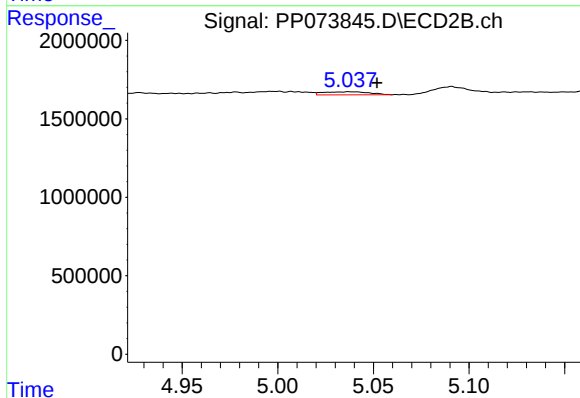


#13 AR-1232-3

R.T.: 5.037 min
Delta R.T.: -0.015 min
Response: 327174
Conc: 13.07 ng/ml

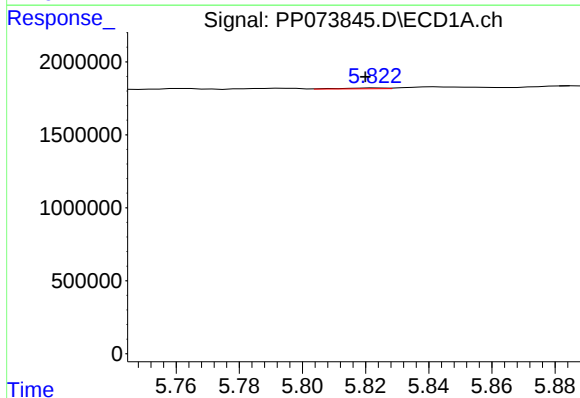


#14 AR-1232-4

R.T.: 5.824 min
Delta R.T.: 0.004 min
Response: 55724
Conc: 3.39 ng/ml

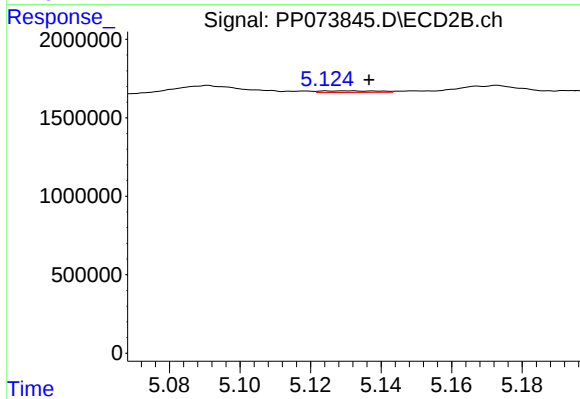

#14 AR-1232-4


R.T.: 5.132 min
Delta R.T.: -0.004 min
Response: 113886
Conc: 5.26 ng/ml

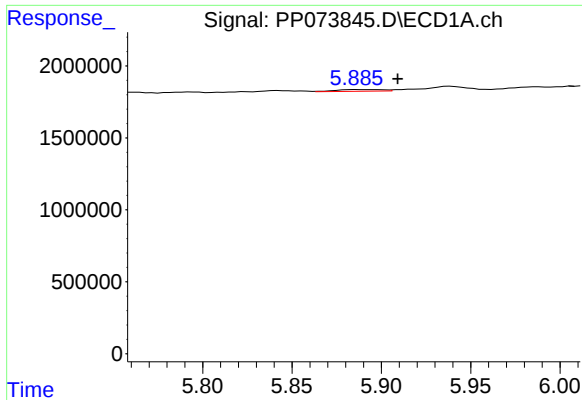

#15 AR-1232-5


R.T.: 5.886 min
Delta R.T.: -0.023 min
Response: 219266
Conc: 20.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

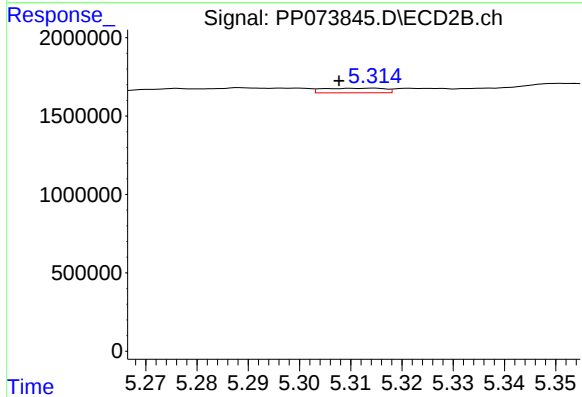


#15 AR-1232-5

R.T.: 5.315 min
Delta R.T.: 0.007 min
Response: 245924
Conc: 10.90 ng/ml

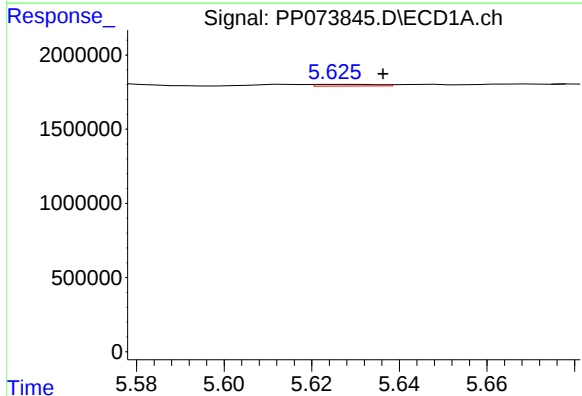


#16 AR-1242-1

R.T.: 5.628 min
Delta R.T.: -0.008 min
Response: 114905
Conc: 3.01 ng/ml

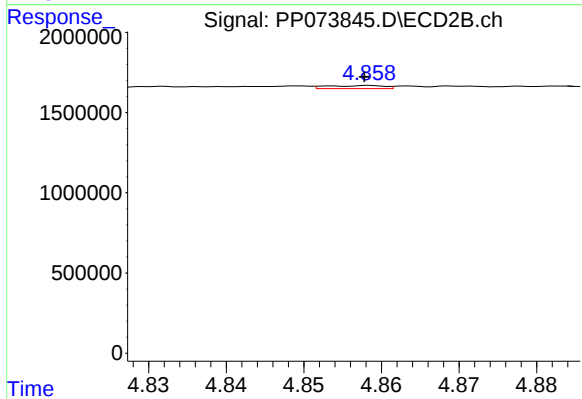

#16 AR-1242-1


R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 94932
Conc: 1.64 ng/ml

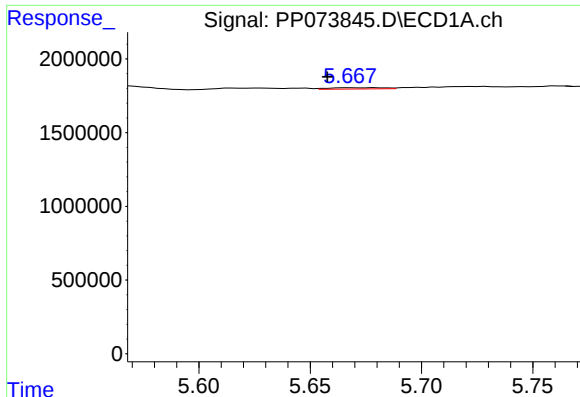

#17 AR-1242-2


R.T.: 5.668 min
Delta R.T.: 0.010 min
Response: 148930
Conc: 2.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

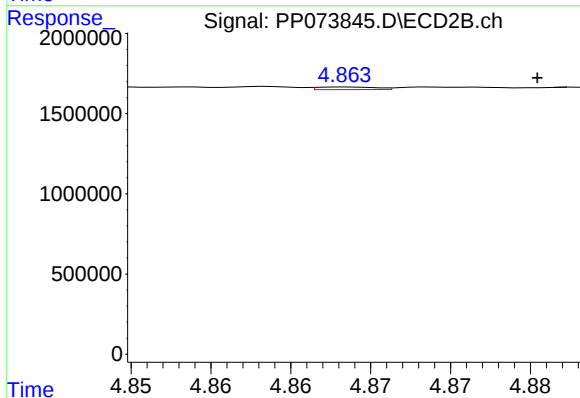


#17 AR-1242-2

R.T.: 4.864 min
Delta R.T.: -0.012 min
Response: 41095
Conc: 0.48 ng/ml

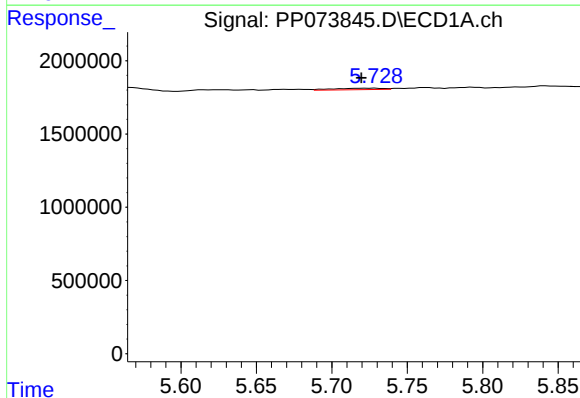


#18 AR-1242-3

R.T.: 5.728 min
Delta R.T.: 0.009 min
Response: 241762
Conc: 6.60 ng/ml

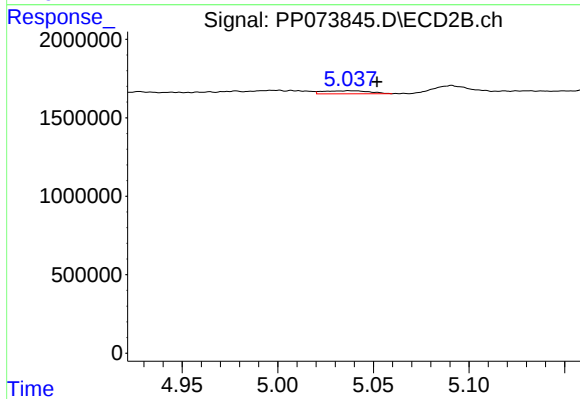

#18 AR-1242-3


R.T.: 5.037 min
Delta R.T.: -0.015 min
Response: 327174
Conc: 7.12 ng/ml

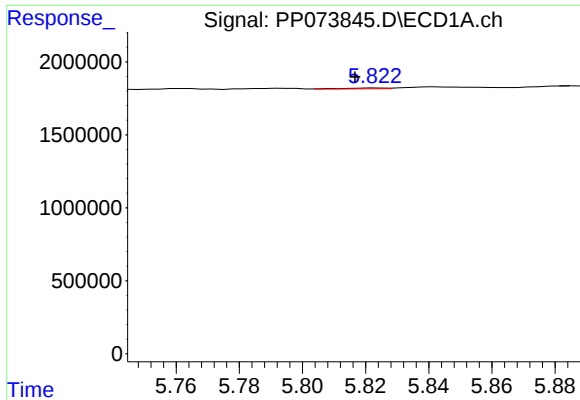

#19 AR-1242-4


R.T.: 5.824 min
Delta R.T.: 0.007 min
Response: 55724
Conc: 1.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

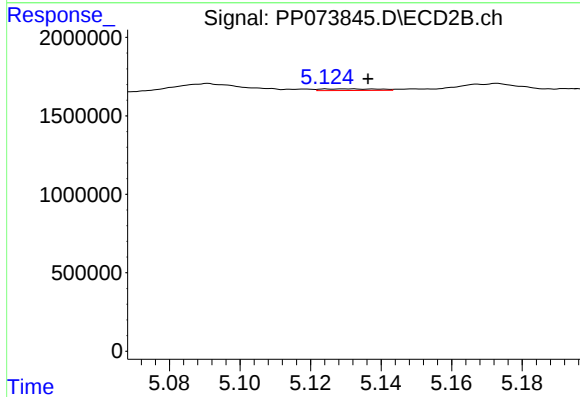


#19 AR-1242-4

R.T.: 5.132 min
Delta R.T.: -0.004 min
Response: 113886
Conc: 2.57 ng/ml

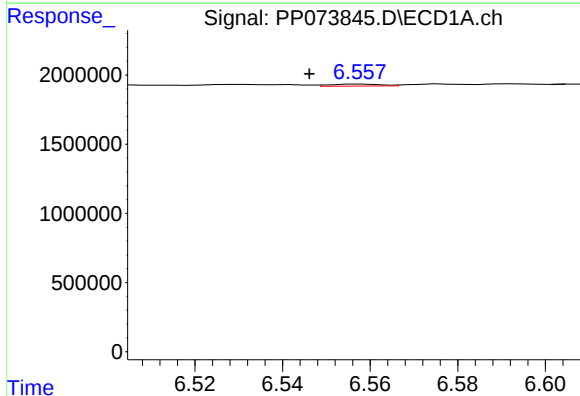


#20 AR-1242-5

R.T.: 6.558 min
Delta R.T.: 0.012 min
Response: 115341
Conc: 3.52 ng/ml

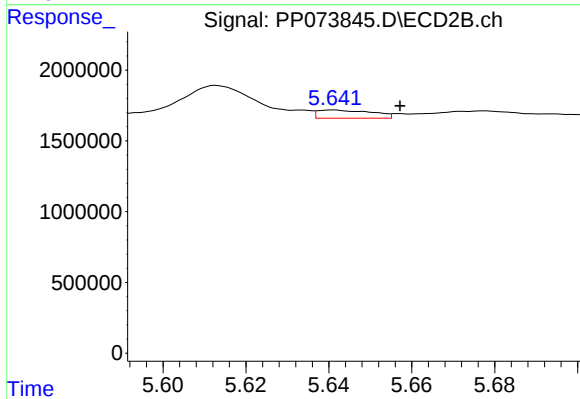

#20 AR-1242-5


R.T.: 5.641 min
Delta R.T.: -0.016 min
Response: 522392
Conc: 9.46 ng/ml

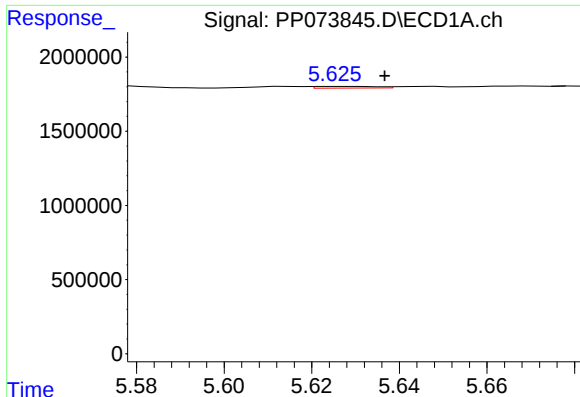

#21 AR-1248-1


R.T.: 5.628 min
Delta R.T.: -0.009 min
Response: 114905
Conc: 3.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

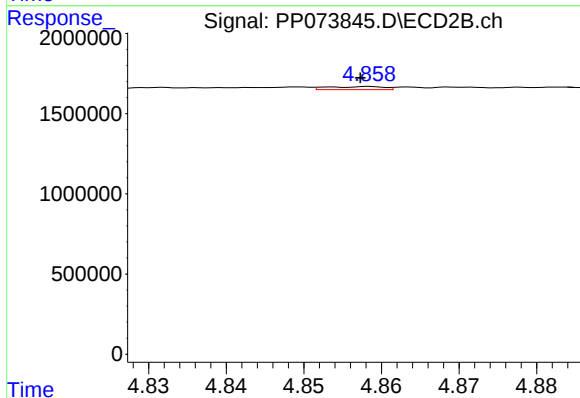


#21 AR-1248-1

R.T.: 4.858 min
Delta R.T.: 0.001 min
Response: 94932
Conc: 2.11 ng/ml

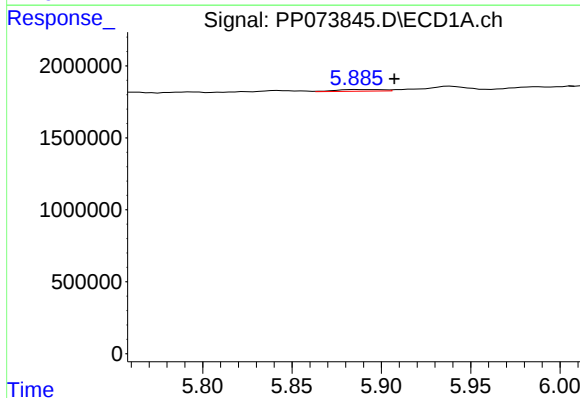


#22 AR-1248-2

R.T.: 5.886 min
Delta R.T.: -0.021 min
Response: 219266
Conc: 5.49 ng/ml

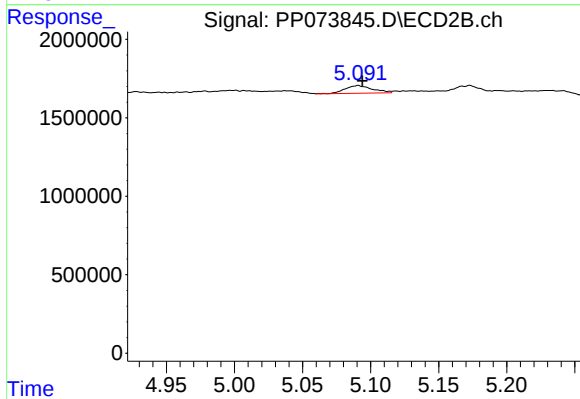

#22 AR-1248-2


R.T.: 5.091 min
Delta R.T.: -0.003 min
Response: 679302
Conc: 11.04 ng/ml

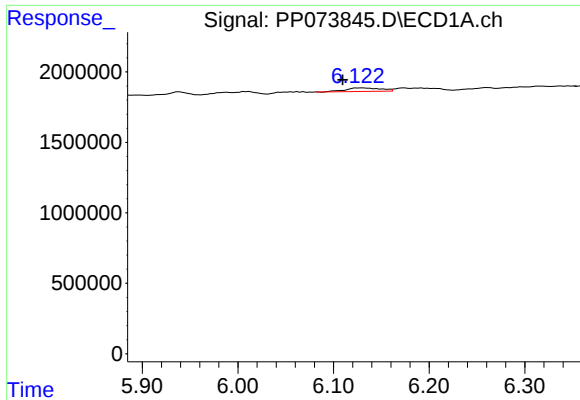

#23 AR-1248-3


R.T.: 6.125 min
Delta R.T.: 0.015 min
Response: 629422
Conc: 14.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

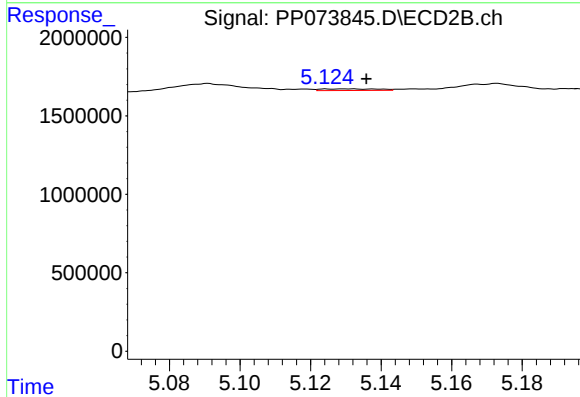


#23 AR-1248-3

R.T.: 5.132 min
Delta R.T.: -0.004 min
Response: 113886
Conc: 1.78 ng/ml

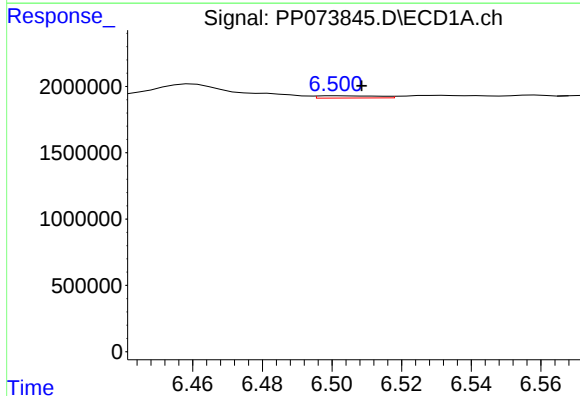


#24 AR-1248-4

R.T.: 6.502 min
Delta R.T.: -0.007 min
Response: 205619
Conc: 3.73 ng/ml

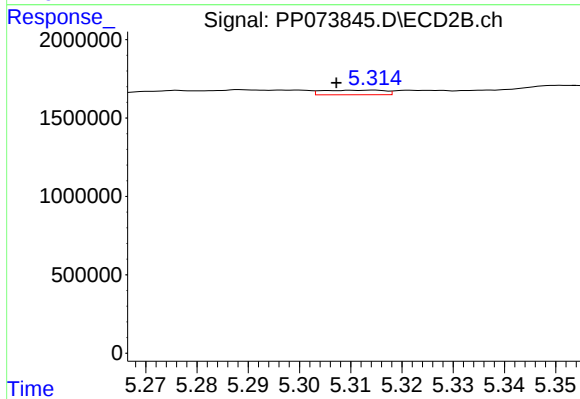

#24 AR-1248-4


R.T.: 5.315 min
Delta R.T.: 0.007 min
Response: 245924
Conc: 3.26 ng/ml

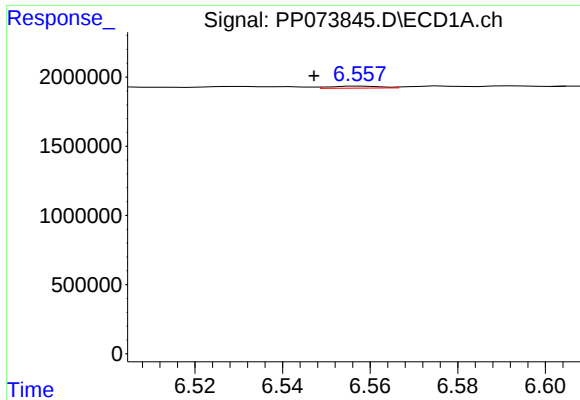

#25 AR-1248-5


R.T.: 6.558 min
Delta R.T.: 0.011 min
Response: 115341
Conc: 2.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

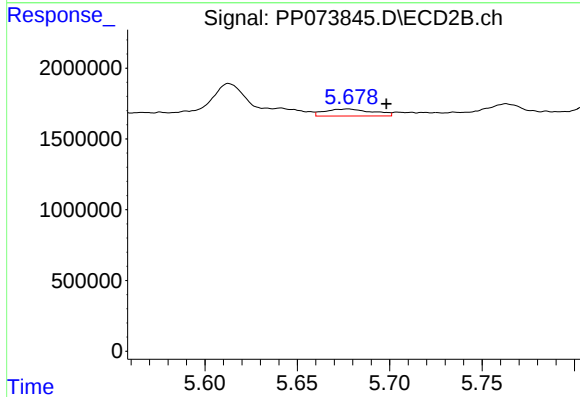


#25 AR-1248-5

R.T.: 5.678 min
Delta R.T.: -0.021 min
Response: 894506
Conc: 11.99 ng/ml

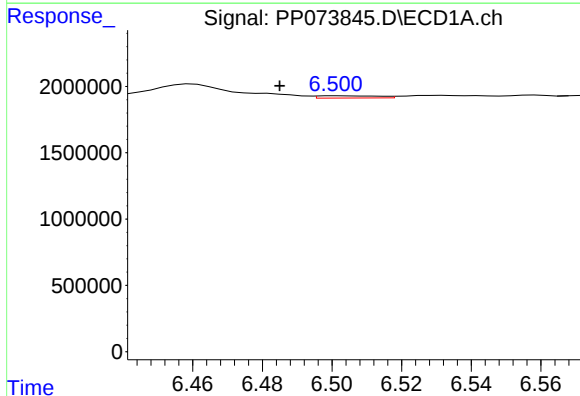


#26 AR-1254-1

R.T.: 6.502 min
Delta R.T.: 0.017 min
Response: 205619
Conc: 3.84 ng/ml

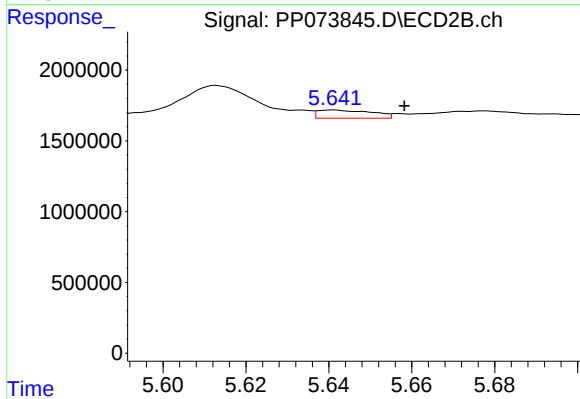

#26 AR-1254-1


R.T.: 5.641 min
Delta R.T.: -0.017 min
Response: 522392
Conc: 4.50 ng/ml

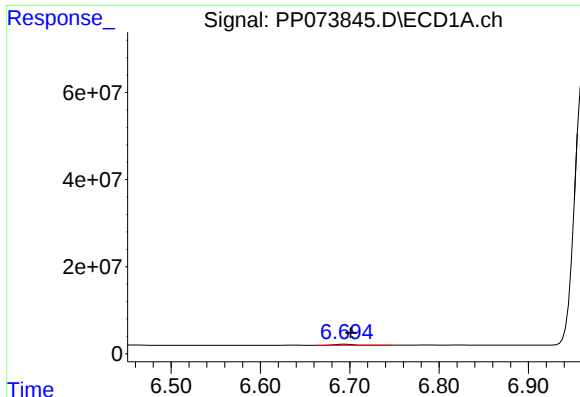

#27 AR-1254-2


R.T.: 6.695 min
Delta R.T.: -0.006 min
Response: 3789522
Conc: 45.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

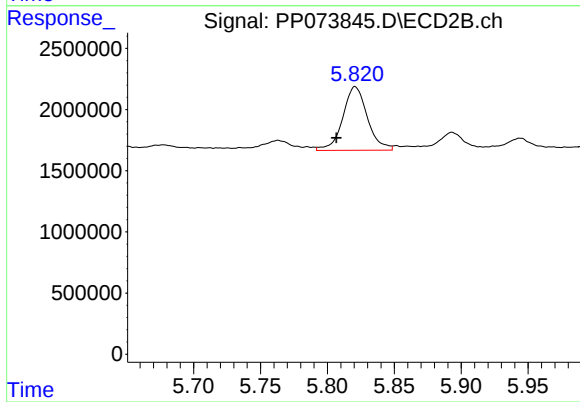


#27 AR-1254-2

R.T.: 5.821 min
Delta R.T.: 0.014 min
Response: 6687870
Conc: 66.46 ng/ml

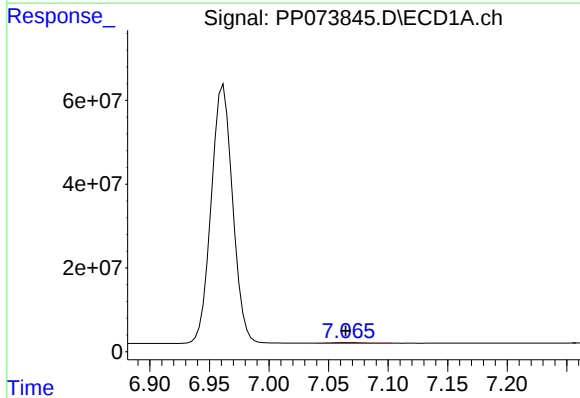


#28 AR-1254-3

R.T.: 7.066 min
Delta R.T.: 0.002 min
Response: 3772148
Conc: 42.70 ng/ml

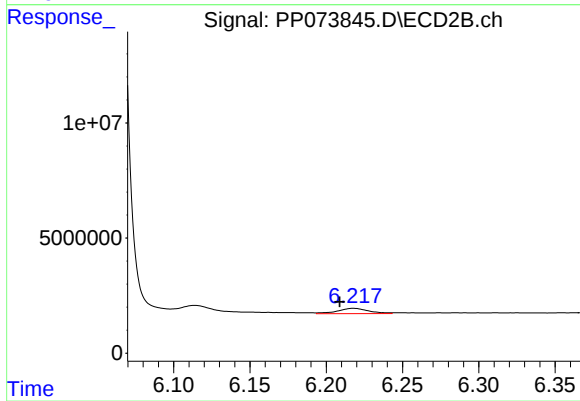

#28 AR-1254-3


R.T.: 6.218 min
Delta R.T.: 0.009 min
Response: 3296338
Conc: 21.34 ng/ml

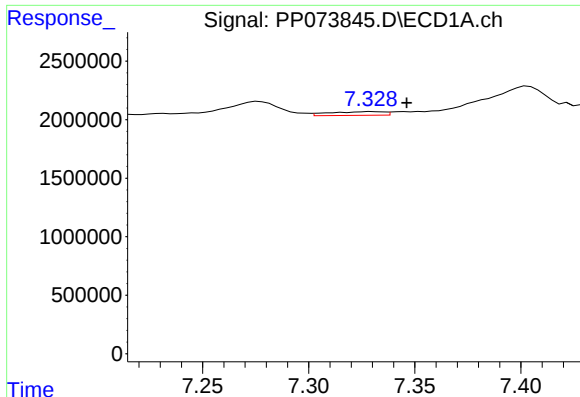

#29 AR-1254-4


R.T.: 7.329 min
Delta R.T.: -0.017 min
Response: 563098
Conc: 7.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

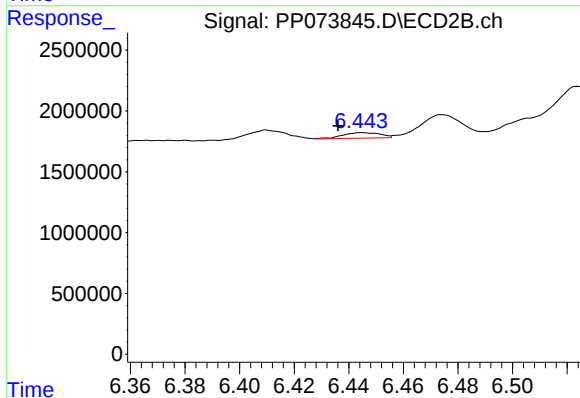


#29 AR-1254-4

R.T.: 6.445 min
Delta R.T.: 0.009 min
Response: 428007
Conc: 4.53 ng/ml

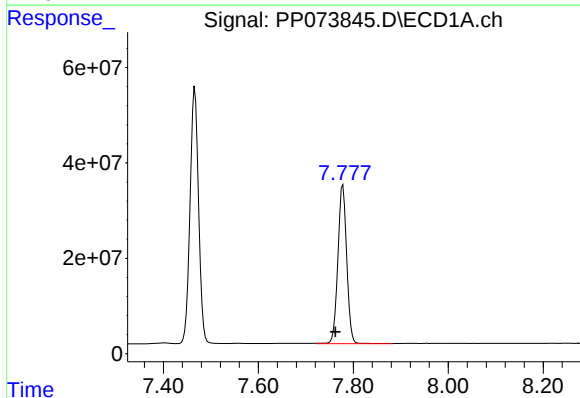


#30 AR-1254-5

R.T.: 7.778 min
Delta R.T.: 0.016 min
Response: 430980677
Conc: 5849.37 ng/ml

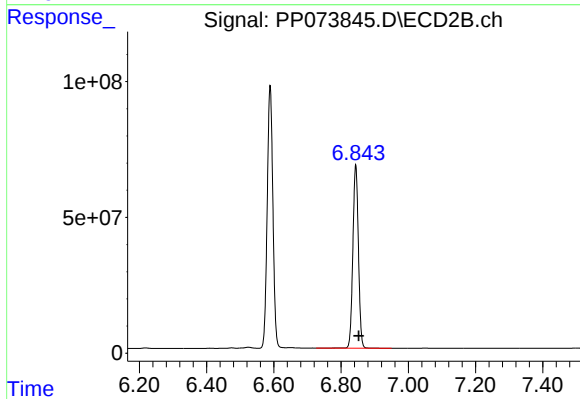

#30 AR-1254-5


R.T.: 6.844 min
Delta R.T.: -0.009 min
Response: 771103326
Conc: 5778.44 ng/ml

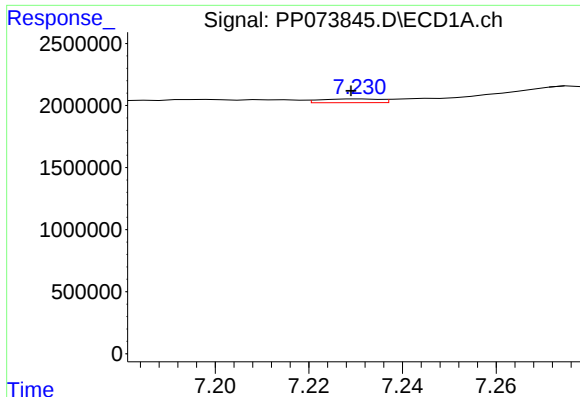

#31 AR-1260-1


R.T.: 7.231 min
Delta R.T.: 0.002 min
Response: 266065
Conc: 4.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

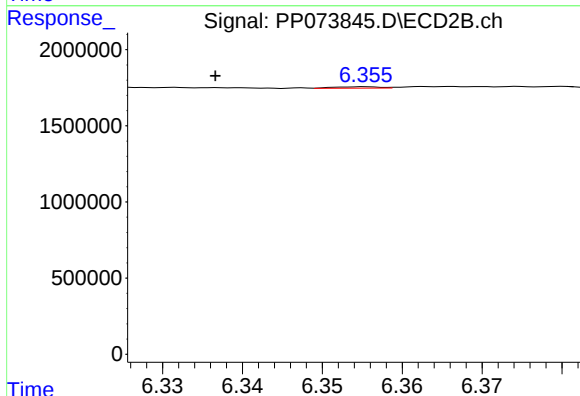


#31 AR-1260-1

R.T.: 6.356 min
Delta R.T.: 0.019 min
Response: 39460
Conc: 0.40 ng/ml

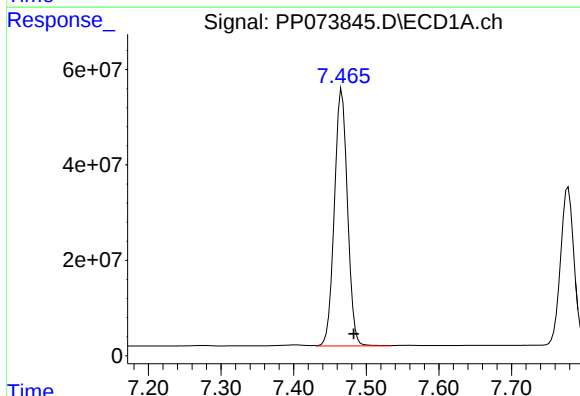


#32 AR-1260-2

R.T.: 7.466 min
Delta R.T.: -0.016 min
Response: 675909940
Conc: 7052.49 ng/ml

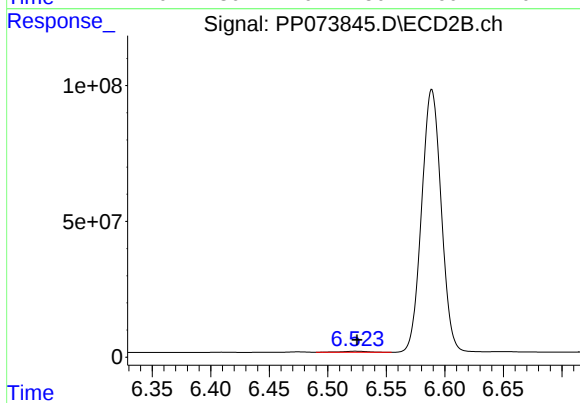

#32 AR-1260-2


R.T.: 6.524 min
Delta R.T.: 0.000 min
Response: 6278823
Conc: 51.11 ng/ml

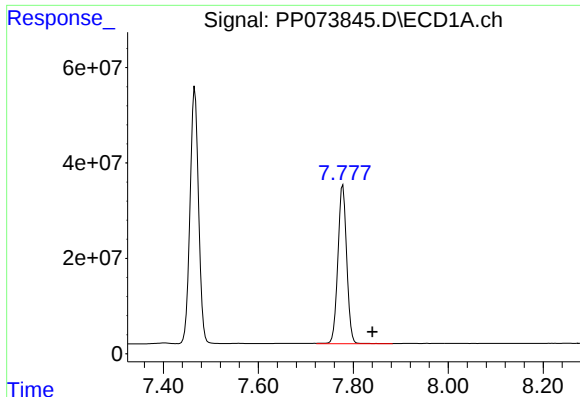

#33 AR-1260-3


R.T.: 7.778 min
Delta R.T.: -0.062 min
Response: 430980677
Conc: 5898.14 ng/m

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

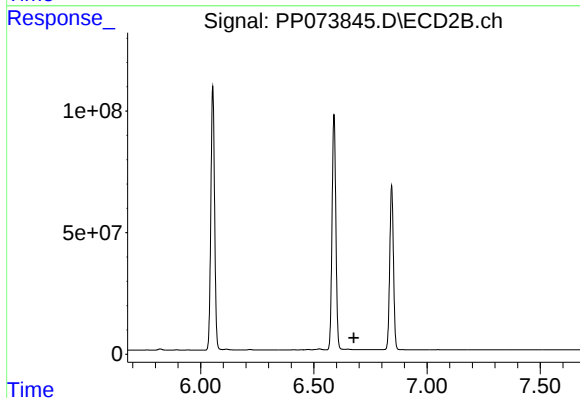


#33 AR-1260-3

R.T.: 6.651 min
Delta R.T.: -0.026 min
Response: -144334
Conc: N.D.

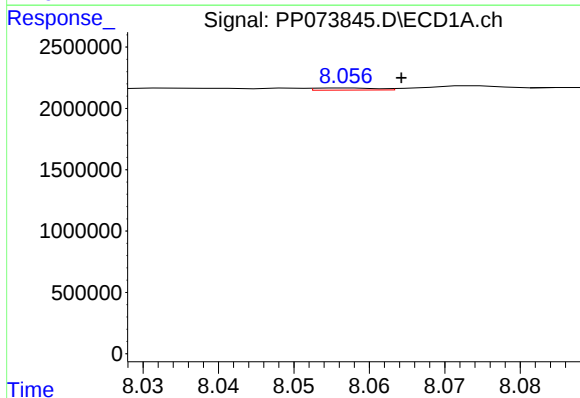


#34 AR-1260-4

R.T.: 8.057 min
Delta R.T.: -0.007 min
Response: 96541
Conc: 1.48 ng/ml

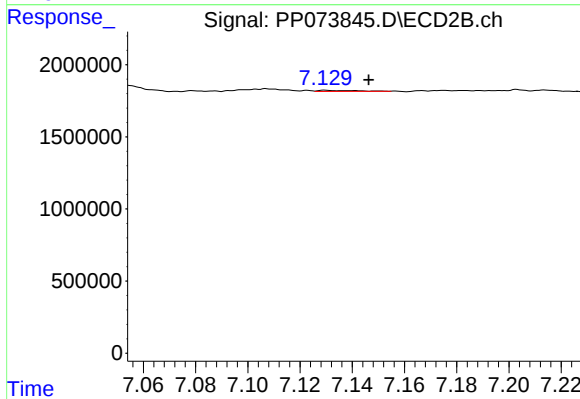

#34 AR-1260-4


R.T.: 7.130 min
Delta R.T.: -0.017 min
Response: 70676
Conc: 0.79 ng/ml

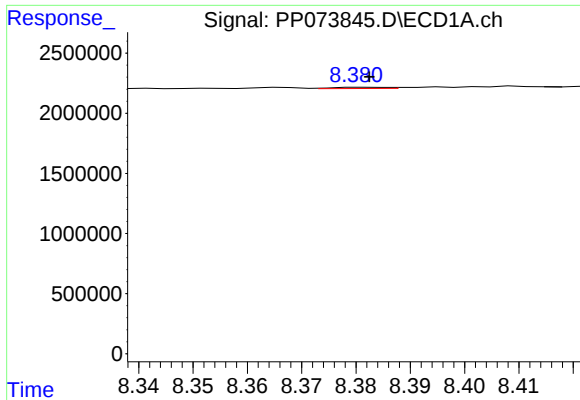

#35 AR-1260-5


R.T.: 8.382 min
Delta R.T.: 0.000 min
Response: 69140
Conc: 0.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

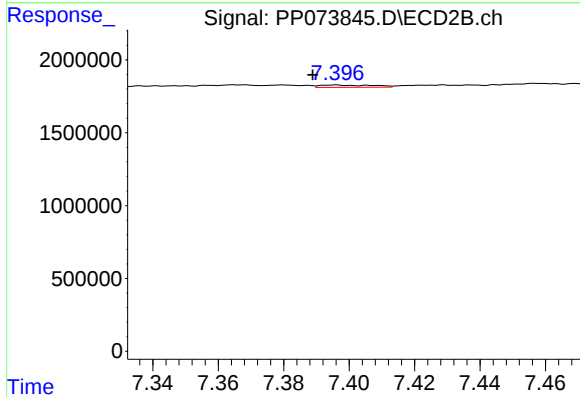


#35 AR-1260-5

R.T.: 7.396 min
Delta R.T.: 0.007 min
Response: 180525
Conc: 0.80 ng/ml

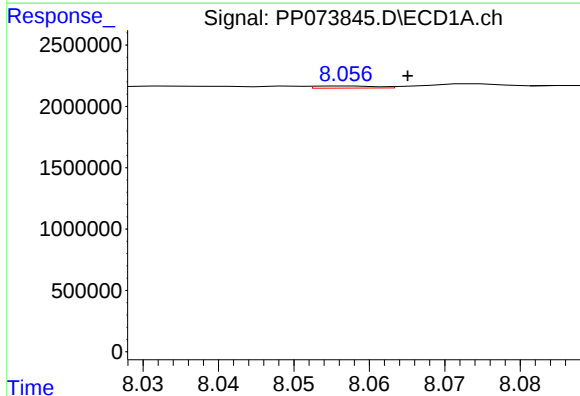


#36 AR-1262-1

R.T.: 8.057 min
Delta R.T.: -0.008 min
Response: 96541
Conc: 1.11 ng/ml

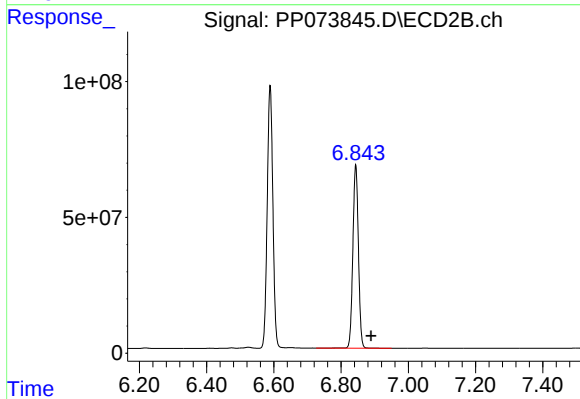

#36 AR-1262-1


R.T.: 6.844 min
Delta R.T.: -0.046 min
Response: 771103326
Conc: 5221.03 ng/ml

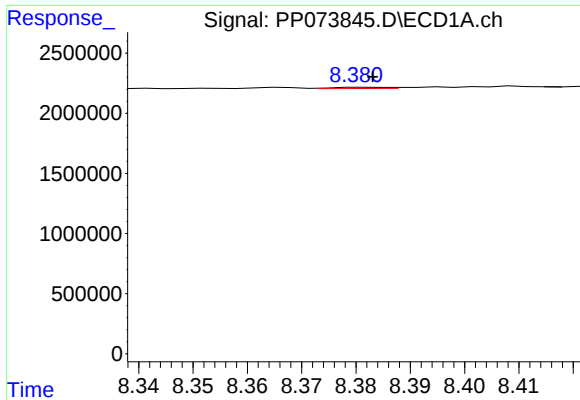

#37 AR-1262-2


R.T.: 8.382 min
Delta R.T.: -0.001 min
Response: 69140
Conc: 0.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

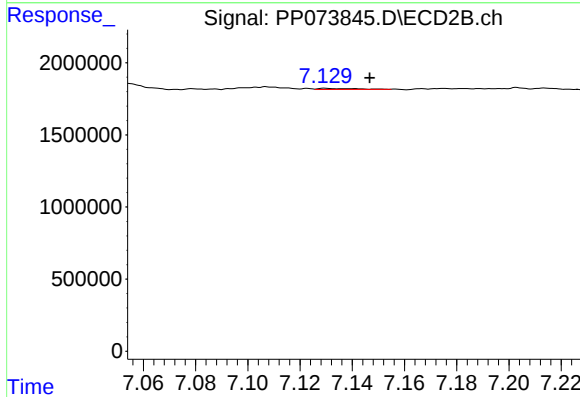


#37 AR-1262-2

R.T.: 7.130 min
Delta R.T.: -0.017 min
Response: 70676
Conc: 0.55 ng/ml

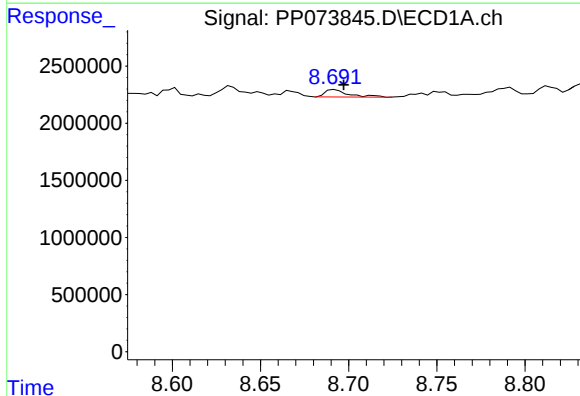


#38 AR-1262-3

R.T.: 8.693 min
Delta R.T.: -0.005 min
Response: 593626
Conc: 4.72 ng/ml

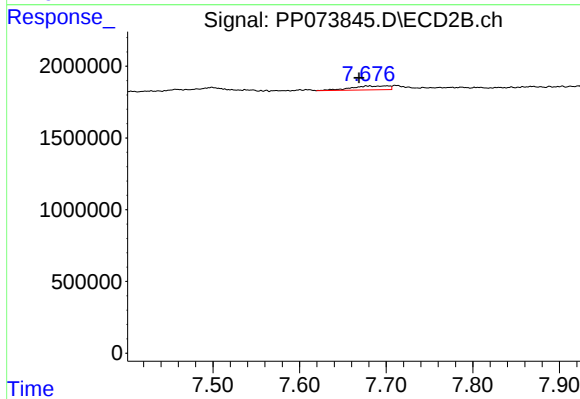

#38 AR-1262-3


R.T.: 7.681 min
Delta R.T.: 0.012 min
Response: 817547
Conc: 7.17 ng/ml

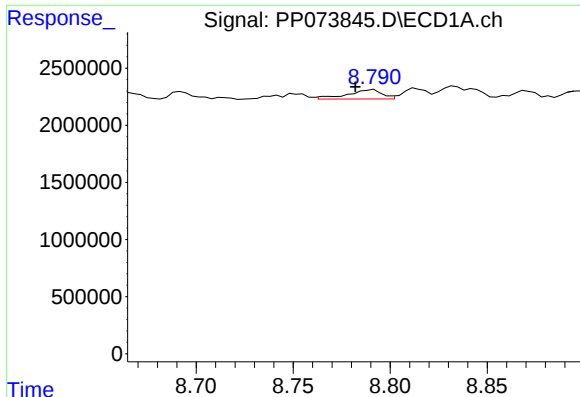

#39 AR-1262-4


R.T.: 8.791 min
Delta R.T.: 0.009 min
Response: 1011089
Conc: 10.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

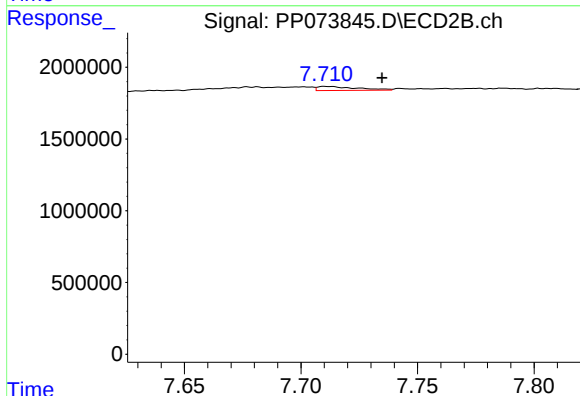


#39 AR-1262-4

R.T.: 7.711 min
Delta R.T.: -0.024 min
Response: 323284
Conc: 1.76 ng/ml

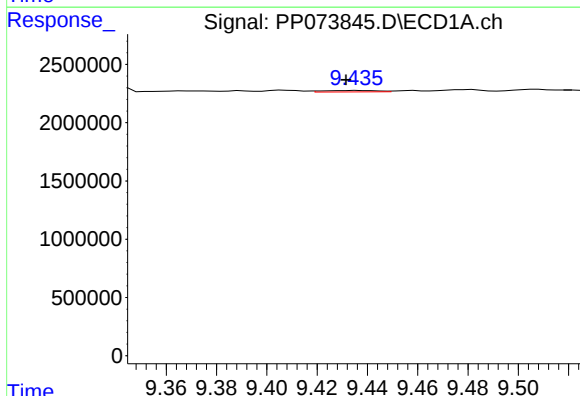


#40 AR-1262-5

R.T.: 9.436 min
Delta R.T.: 0.004 min
Response: 191038
Conc: 3.01 ng/ml

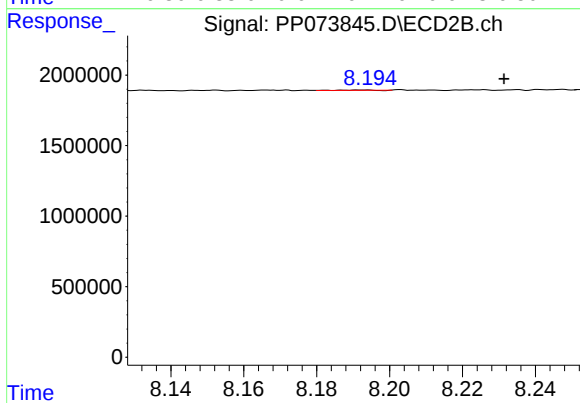

#40 AR-1262-5


R.T.: 8.193 min
Delta R.T.: -0.039 min
Response: 22102
Conc: 0.26 ng/ml

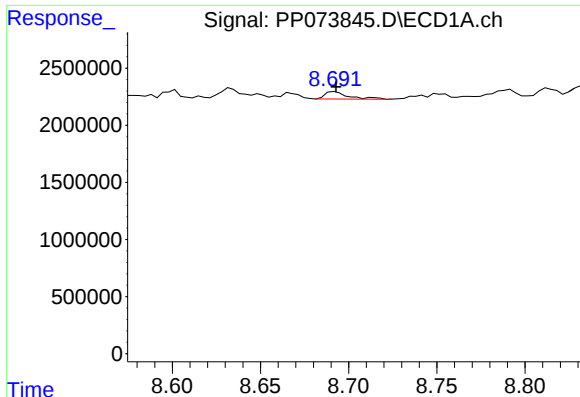

#41 AR-1268-1


R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 593626
Conc: 2.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

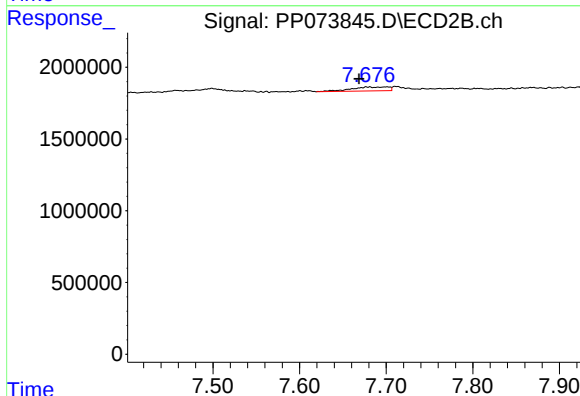


#41 AR-1268-1

R.T.: 7.681 min
Delta R.T.: 0.012 min
Response: 817547
Conc: 2.66 ng/ml

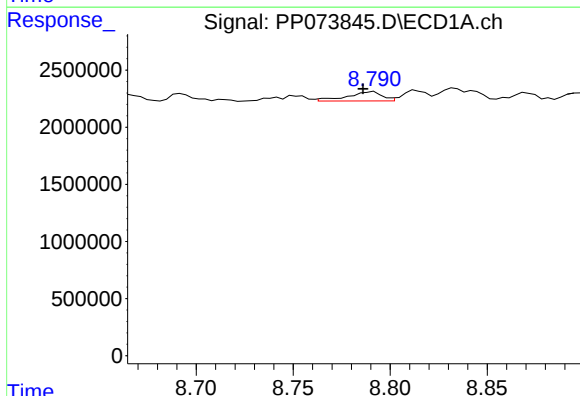


#42 AR-1268-2

R.T.: 8.791 min
Delta R.T.: 0.005 min
Response: 1011089
Conc: 5.31 ng/ml

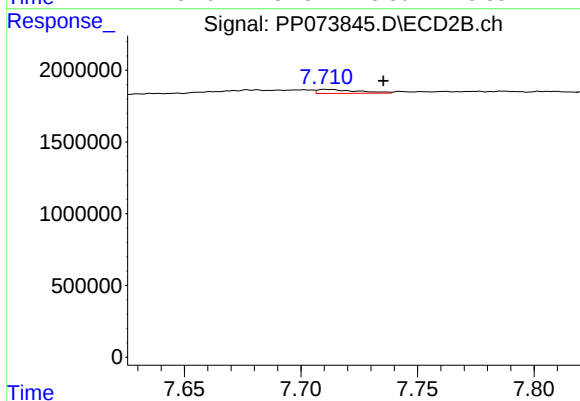

#42 AR-1268-2


R.T.: 7.711 min
Delta R.T.: -0.024 min
Response: 323284
Conc: 1.22 ng/ml

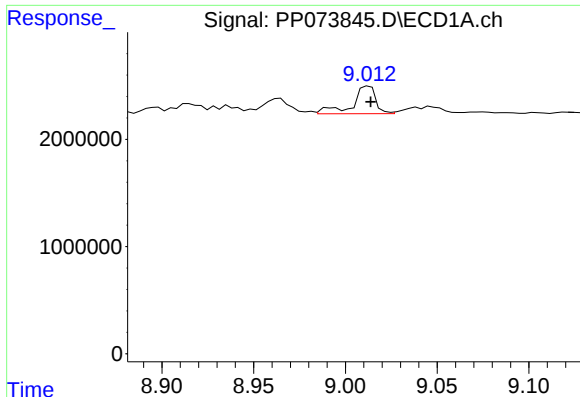

#43 AR-1268-3


R.T.: 9.013 min
Delta R.T.: -0.001 min
Response: 2284112
Conc: 13.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

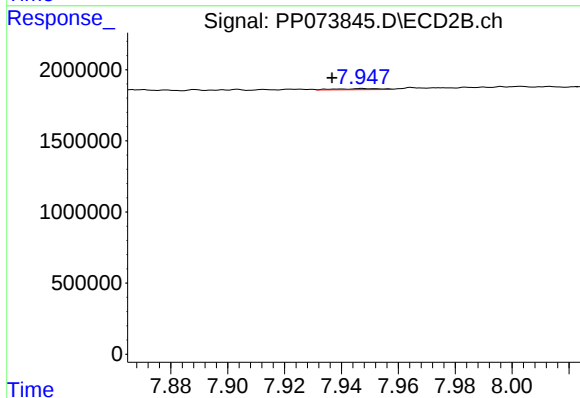


#43 AR-1268-3

R.T.: 7.948 min
Delta R.T.: 0.011 min
Response: 80343
Conc: 0.36 ng/ml

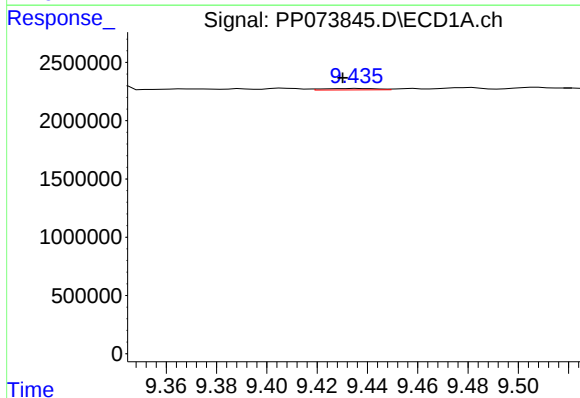


#44 AR-1268-4

R.T.: 9.436 min
Delta R.T.: 0.005 min
Response: 191038
Conc: 2.75 ng/ml

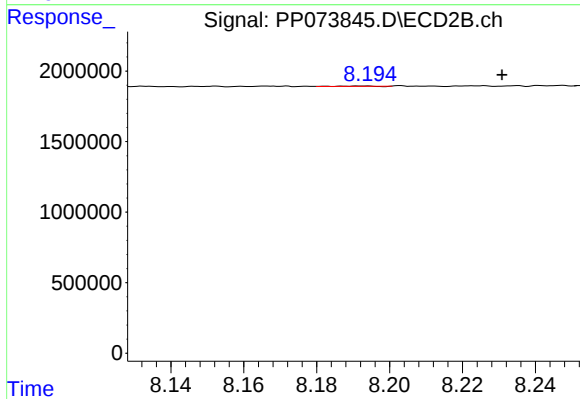

#44 AR-1268-4


R.T.: 8.193 min
Delta R.T.: -0.038 min
Response: 22102
Conc: 0.24 ng/ml

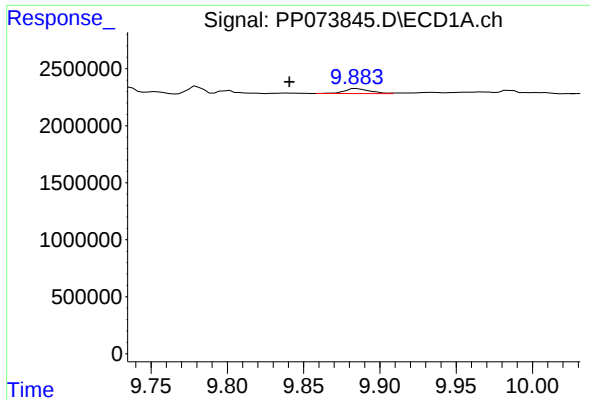

#45 AR-1268-5

R.T.: 9.885 min
Delta R.T.: 0.045 min
Response: 493070
Conc: 1.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

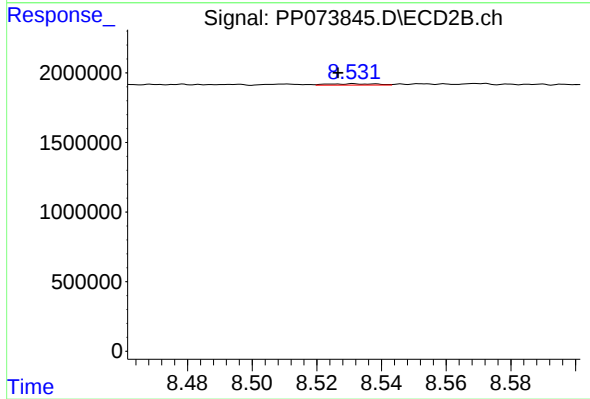

#45 AR-1268-5

R.T.: 8.531 min
Delta R.T.: 0.005 min
Response: 99601
Conc: 0.16 ng/ml