

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071625\
 Data File : PP073863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2025 17:45
 Operator : YP\AJ
 Sample : Q2611-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EO-02-071525

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/17/2025
 Supervised By :mohammad ahmed 07/18/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:49:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.485	3.778	25488511	38459662	18.611m	20.876
2) SA Decachlor...	10.171	8.775	21920154	27164753	20.091	20.530

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071625\
Data File : PP073863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2025 17:45
Operator : YP\AJ
Sample : Q2611-01
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
EO-02-071525


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/17/2025
Supervised By :mohammad ahmed 07/18/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:49:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

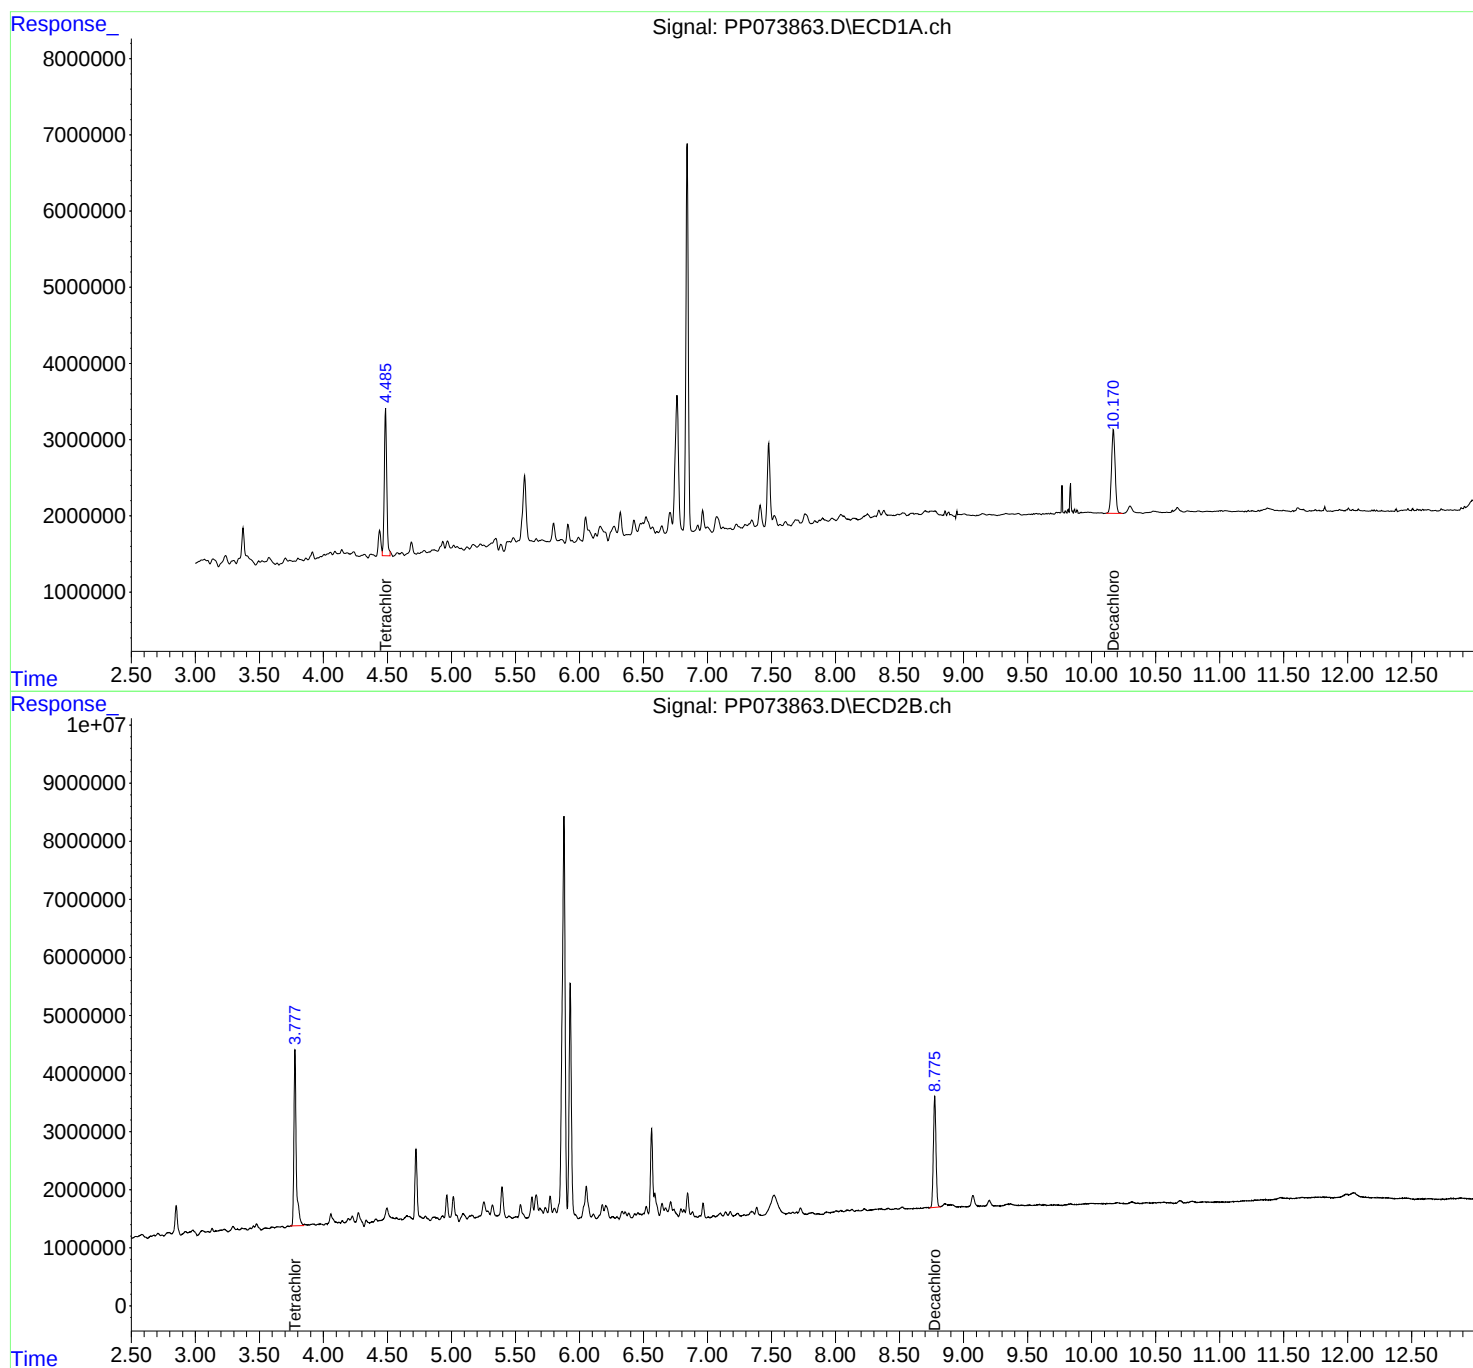

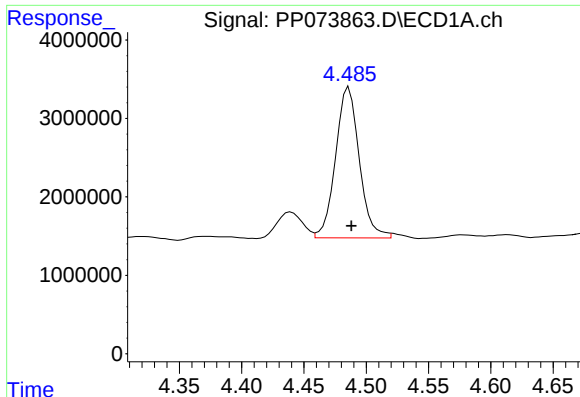


#1 Tetrachloro-m-xylene

R.T.: 4.485 min
Delta R.T.: -0.003 min
Response: 25488511
Conc: 18.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
EO-02-071525


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/17/2025
Supervised By :mohammad ahmed 07/18/2025

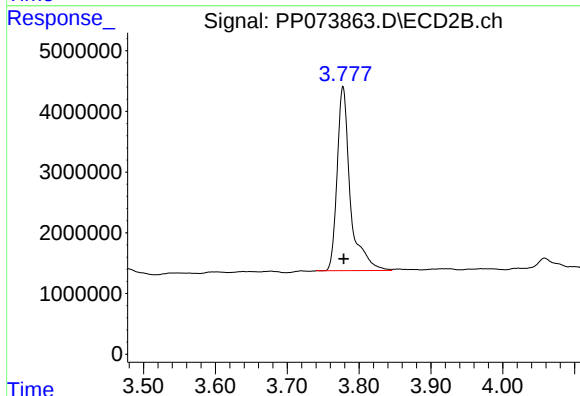


#1 Tetrachloro-m-xylene

R.T.: 3.778 min
Delta R.T.: 0.000 min
Response: 38459662
Conc: 20.88 ng/ml

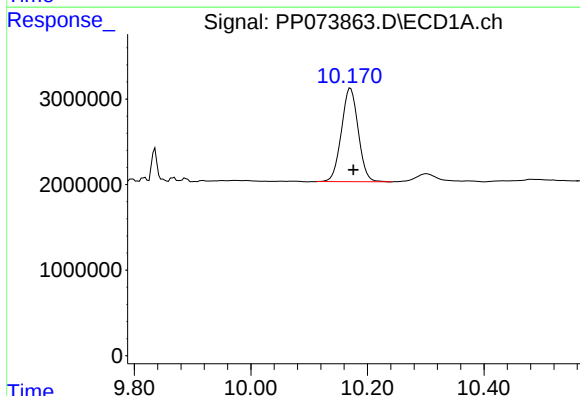

#2 Decachlorobiphenyl

R.T.: 10.171 min
Delta R.T.: -0.005 min
Response: 21920154
Conc: 20.09 ng/ml

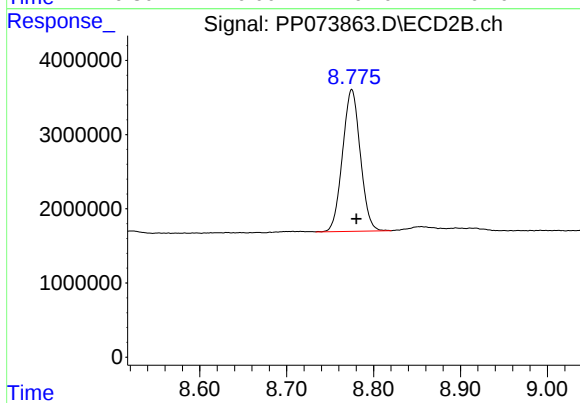

#2 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: -0.005 min
Response: 27164753
Conc: 20.53 ng/ml