

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071725\
 Data File : PP073890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2025 10:53
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 06:36:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.467	3.813f	76146	83154	0.056	0.045
2)	SA Decachlor...	10.169	8.783	56770	79587	0.052	0.060
Target Compounds							
3)	L1 AR-1016-1	5.624	4.854	245482	160234	5.167	2.350 #
4)	L1 AR-1016-2	5.668	4.888	271311	317515	3.810	3.116
5)	L1 AR-1016-3	5.734	5.041	208433	182604	4.774	3.375 #
6)	L1 AR-1016-4	5.832	5.089	201991	649189	5.619	14.794 #
7)	L1 AR-1016-5	6.130	5.294	518309	303411	16.543	5.559 #
8)	L2 AR-1221-1	4.676	3.999	45216	207876	2.531	7.686 #
9)	L2 AR-1221-2	4.759	4.067	170205	77810	12.604	3.822 #
10)	L2 AR-1221-3	4.850	4.166	74603	67553	1.793	1.099 #
11)	L3 AR-1232-1	4.850	4.166	74603	67553	2.285	1.449 #
12)	L3 AR-1232-2	5.351	4.888	135747	317515	8.351	6.662
13)	L3 AR-1232-3	5.668	5.041	271311	182604	8.223	7.296
14)	L3 AR-1232-4	5.832	5.129	201991	104857	12.283	4.842 #
15)	L3 AR-1232-5	5.886	5.294	179369	303411	16.969	13.447
16)	L4 AR-1242-1	5.624	4.854	245482	160234	6.428	2.774 #
17)	L4 AR-1242-2	5.668	4.888	271311	317515	4.531	3.673
18)	L4 AR-1242-3	5.734	5.041	208433	182604	5.692	3.974 #
19)	L4 AR-1242-4	5.832	5.129	201991	104857	6.286	2.369 #
20)	L4 AR-1242-5	6.545	5.699f	133401	32263	4.075	0.584 #
21)	L5 AR-1248-1	5.624	4.854	245482	160234	7.952	3.569 #
22)	L5 AR-1248-2	5.886	5.089	179369	649189	4.493	10.550 #
23)	L5 AR-1248-3	6.130	5.129	518309	104857	11.671	1.637 #
24)	L5 AR-1248-4	6.520	5.294	244688	303411	4.442	4.025
25)	L5 AR-1248-5	6.545	5.699	133401	32263	2.480	0.433 #
26)	L6 AR-1254-1	6.459	5.699f	2347127	32263	43.798	0.278 #
27)	L6 AR-1254-2	6.694	5.820	3153523	5150050	37.862	51.181 #
28)	L6 AR-1254-3	7.069	6.218	3290624	2875628	37.253	18.619 #
29)	L6 AR-1254-4	7.354	6.445	612271	484039	7.783	5.119 #
30)	L6 AR-1254-5	7.778	6.843	358.6E6	636.9E6	4867.286	4772.832
31)	L7 AR-1260-1	7.221	6.334	1241945	86646	21.064	0.888 #
32)	L7 AR-1260-2	7.466	6.523	578.8E6	4947334	6039.632	40.275 #
33)	L7 AR-1260-3	7.853	6.650	889076	-970228	12.167	N.D. #
34)	L7 AR-1260-4	8.046	7.178	209435	95079	3.207	1.063 #
35)	L7 AR-1260-5	8.400	7.381	447077	224967	2.964	1.001 #
36)	L8 AR-1262-1	8.046	6.932f	209435	149341	2.407	1.011 #
37)	L8 AR-1262-2	8.400	7.178	447077	95079	2.258	0.744 #
38)	L8 AR-1262-3	8.704	7.667	77598	102388	0.617	0.898 #
39)	L8 AR-1262-4	8.775	7.732	90144	29271	0.967	0.159 #
40)	L8 AR-1262-5	9.427	8.183f	53870	98328	0.850	1.165 #
41)	L9 AR-1268-1	8.704	7.667	77598	102388	0.348	0.333

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071725\
 Data File : PP073890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2025 10:53
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 06:36:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.775	7.732	90144	29271	0.473	0.110 #
43) L9	AR-1268-3	9.005	7.944	110791	163166	0.669	0.723
44) L9	AR-1268-4	9.427	8.183f	53870	98328	0.775	1.058 #
45) L9	AR-1268-5	9.874	8.535	62892	49227	0.136	0.080 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071725\
Data File : PP073890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2025 10:53
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 06:36:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

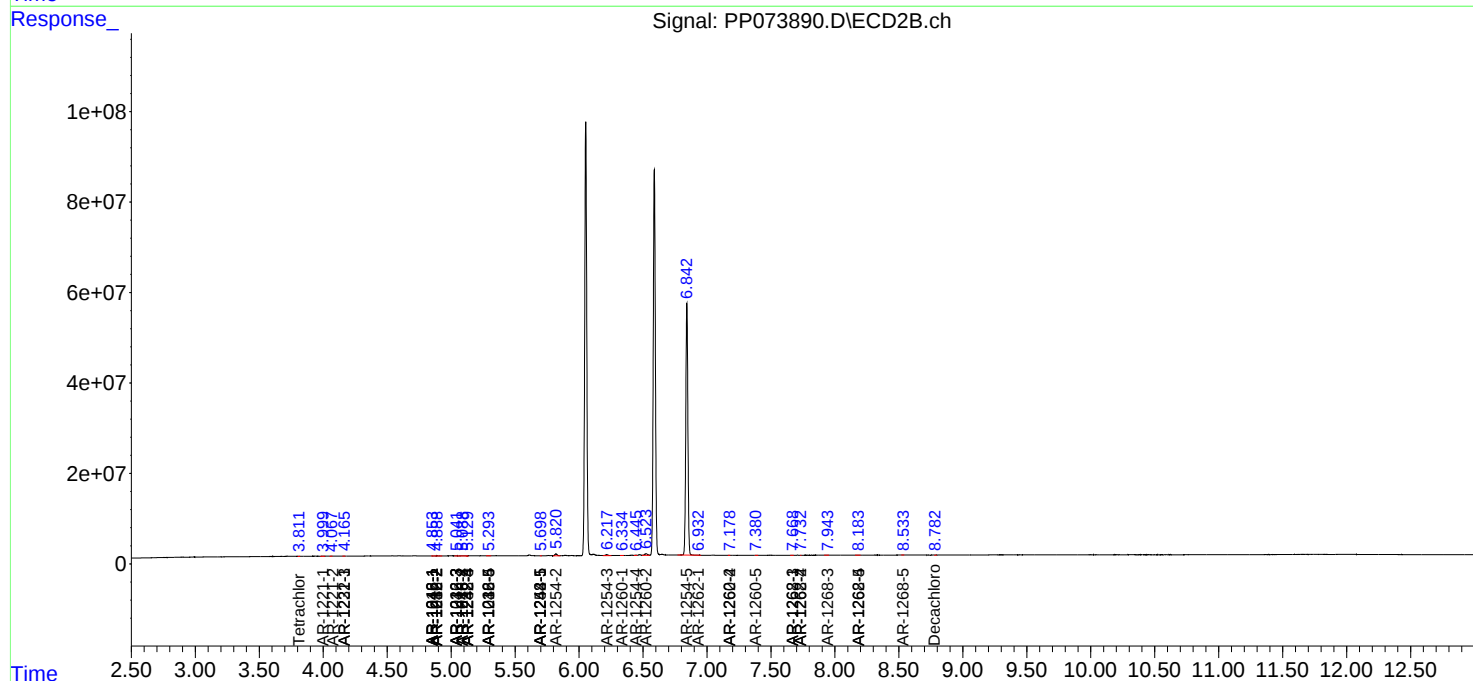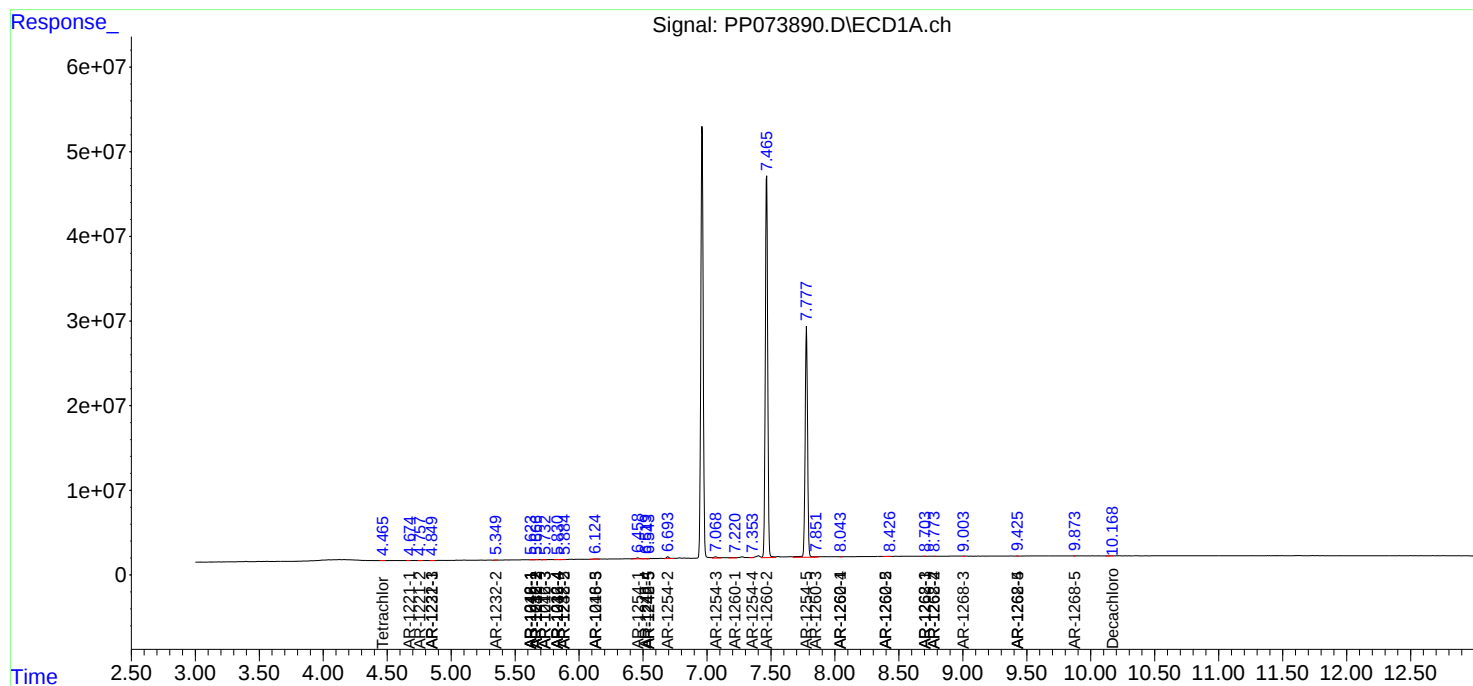


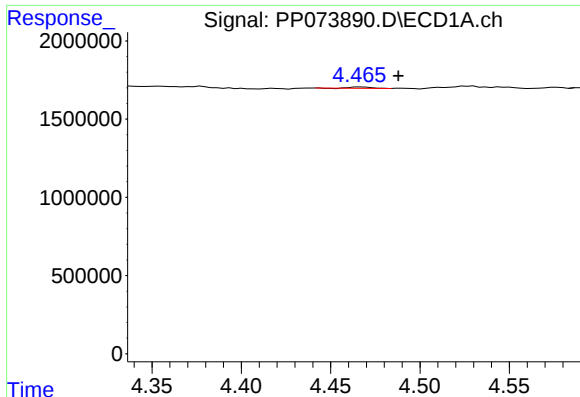

#1 Tetrachloro-m-xylene


R.T.: 4.467 min
Delta R.T.: -0.021 min
Response: 76146
Conc: 0.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

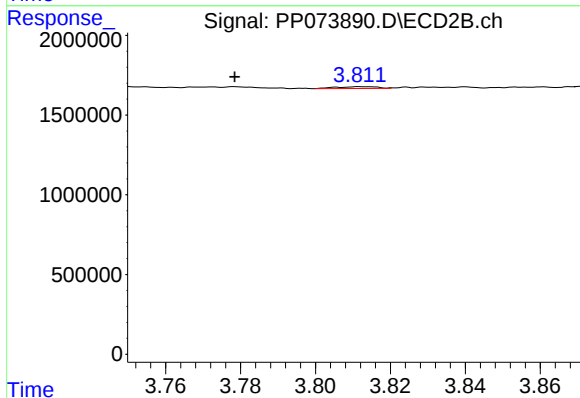


#1 Tetrachloro-m-xylene

R.T.: 3.813 min
Delta R.T.: 0.034 min
Response: 83154
Conc: 0.05 ng/ml

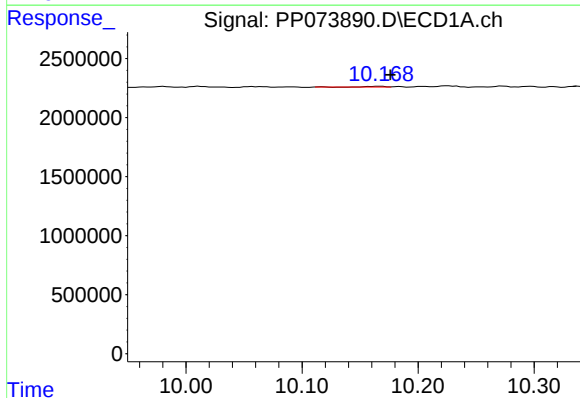


#2 Decachlorobiphenyl

R.T.: 10.169 min
Delta R.T.: -0.007 min
Response: 56770
Conc: 0.05 ng/ml

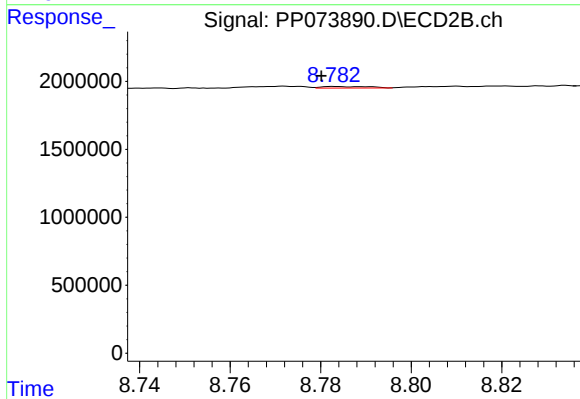

#2 Decachlorobiphenyl


R.T.: 8.783 min
Delta R.T.: 0.003 min
Response: 79587
Conc: 0.06 ng/ml

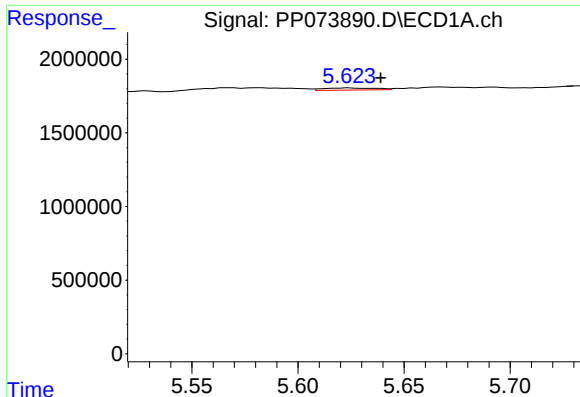

#3 AR-1016-1


R.T.: 5.624 min
Delta R.T.: -0.015 min
Response: 245482
Conc: 5.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

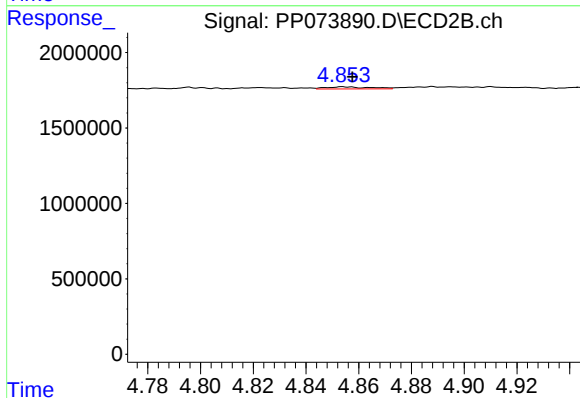


#3 AR-1016-1

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 160234
Conc: 2.35 ng/ml

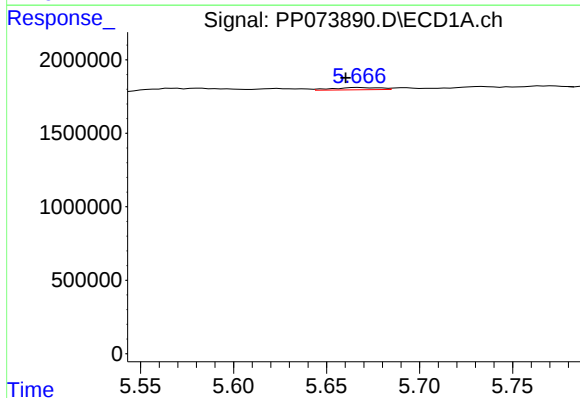


#4 AR-1016-2

R.T.: 5.668 min
Delta R.T.: 0.007 min
Response: 271311
Conc: 3.81 ng/ml

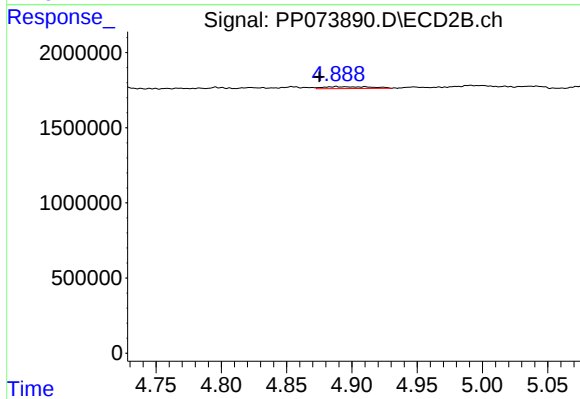

#4 AR-1016-2


R.T.: 4.888 min
Delta R.T.: 0.013 min
Response: 317515
Conc: 3.12 ng/ml

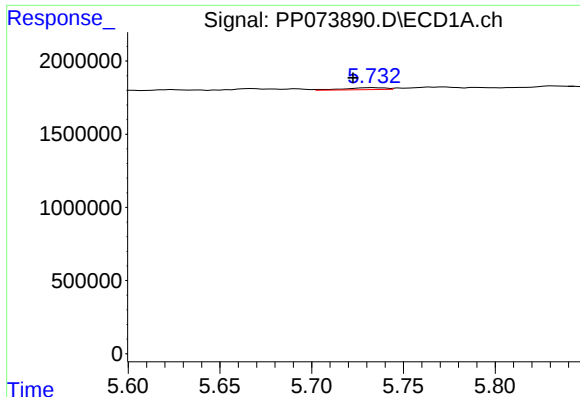

#5 AR-1016-3


R.T.: 5.734 min
Delta R.T.: 0.011 min
Response: 208433
Conc: 4.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

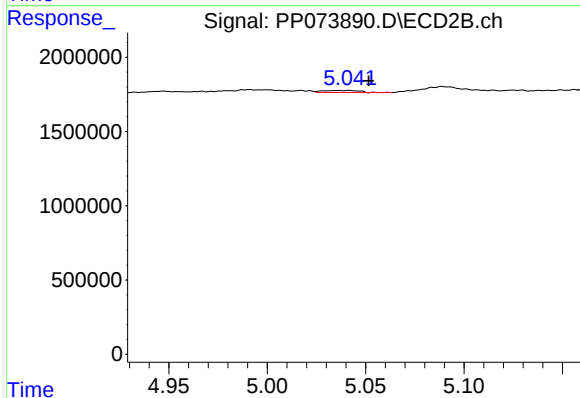


#5 AR-1016-3

R.T.: 5.041 min
Delta R.T.: -0.010 min
Response: 182604
Conc: 3.37 ng/ml

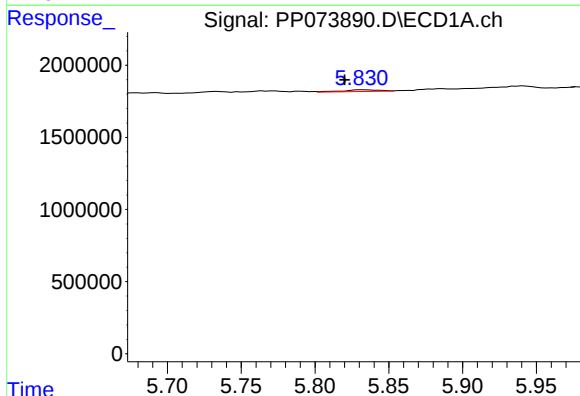


#6 AR-1016-4

R.T.: 5.832 min
Delta R.T.: 0.012 min
Response: 201991
Conc: 5.62 ng/ml

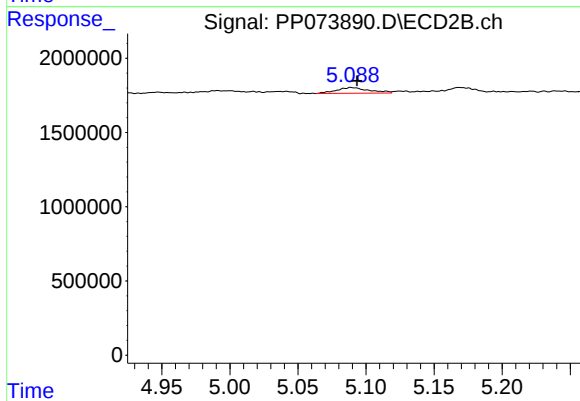

#6 AR-1016-4


R.T.: 5.089 min
Delta R.T.: -0.004 min
Response: 649189
Conc: 14.79 ng/ml

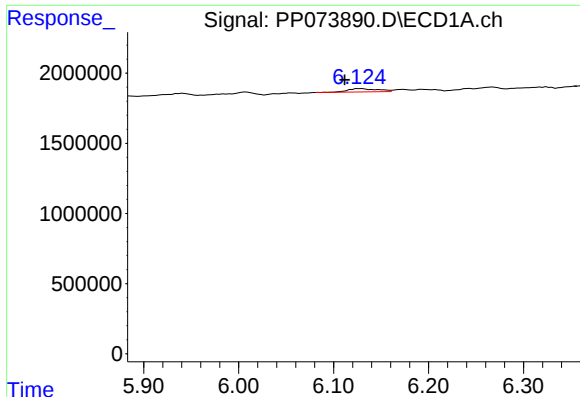

#7 AR-1016-5


R.T.: 6.130 min
Delta R.T.: 0.018 min
Response: 518309
Conc: 16.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

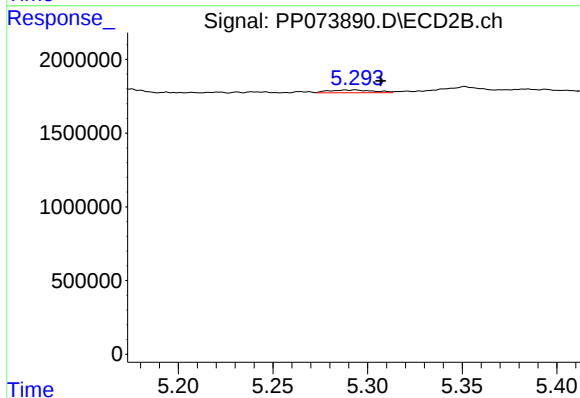


#7 AR-1016-5

R.T.: 5.294 min
Delta R.T.: -0.013 min
Response: 303411
Conc: 5.56 ng/ml

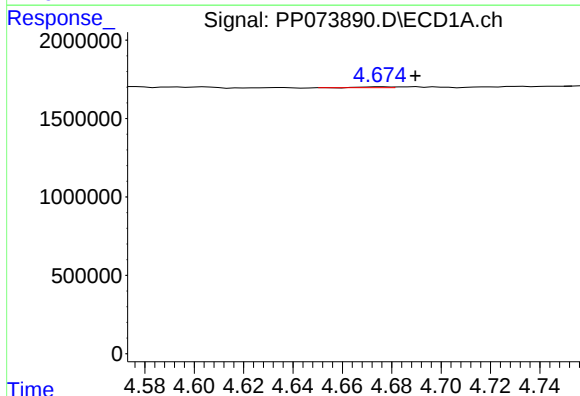


#8 AR-1221-1

R.T.: 4.676 min
Delta R.T.: -0.014 min
Response: 45216
Conc: 2.53 ng/ml

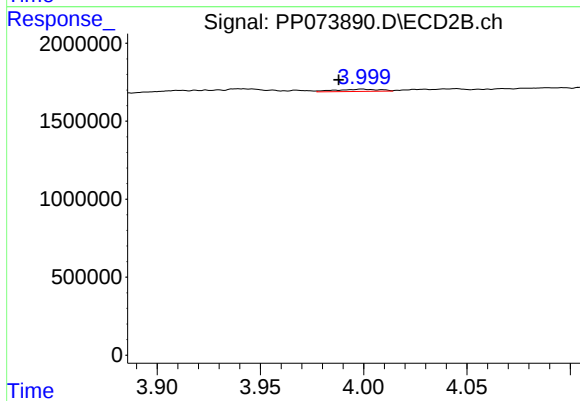

#8 AR-1221-1


R.T.: 3.999 min
Delta R.T.: 0.011 min
Response: 207876
Conc: 7.69 ng/ml

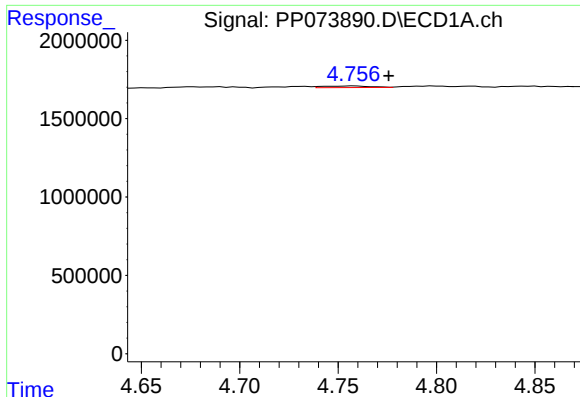

#9 AR-1221-2


R.T.: 4.759 min
Delta R.T.: -0.017 min
Response: 170205
Conc: 12.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

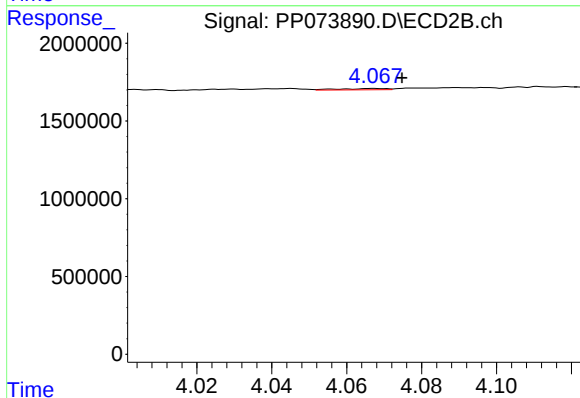


#9 AR-1221-2

R.T.: 4.067 min
Delta R.T.: -0.007 min
Response: 77810
Conc: 3.82 ng/ml

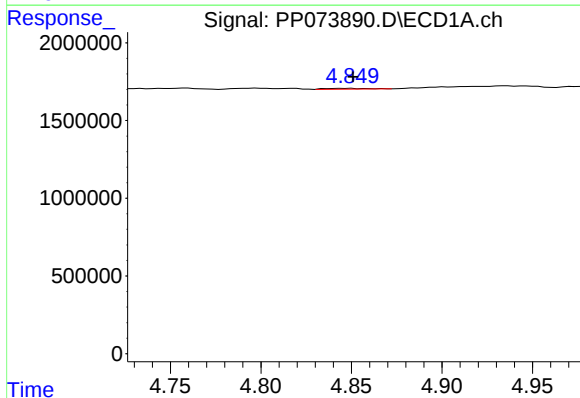


#10 AR-1221-3

R.T.: 4.850 min
Delta R.T.: 0.000 min
Response: 74603
Conc: 1.79 ng/ml

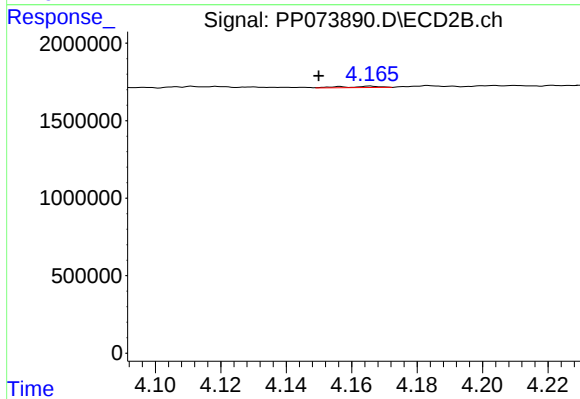

#10 AR-1221-3


R.T.: 4.166 min
Delta R.T.: 0.016 min
Response: 67553
Conc: 1.10 ng/ml

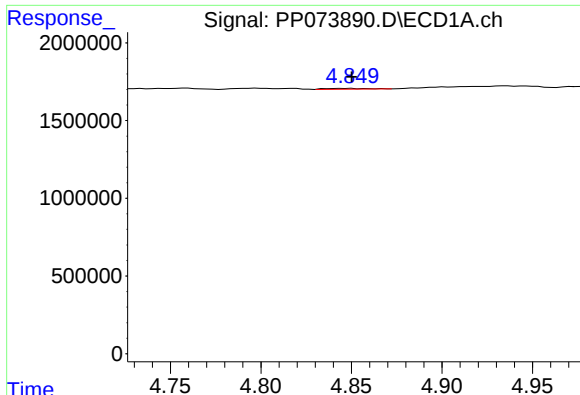

#11 AR-1232-1


R.T.: 4.850 min
Delta R.T.: 0.000 min
Response: 74603
Conc: 2.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

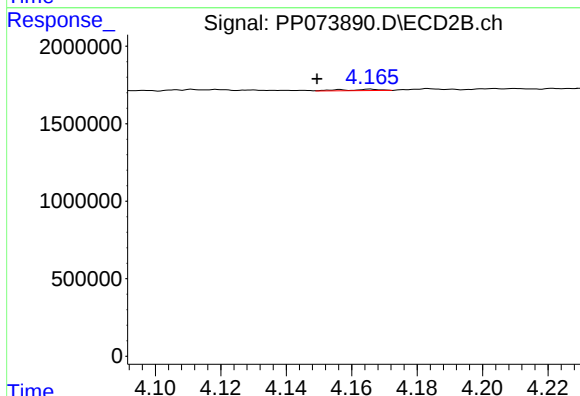


#11 AR-1232-1

R.T.: 4.166 min
Delta R.T.: 0.016 min
Response: 67553
Conc: 1.45 ng/ml

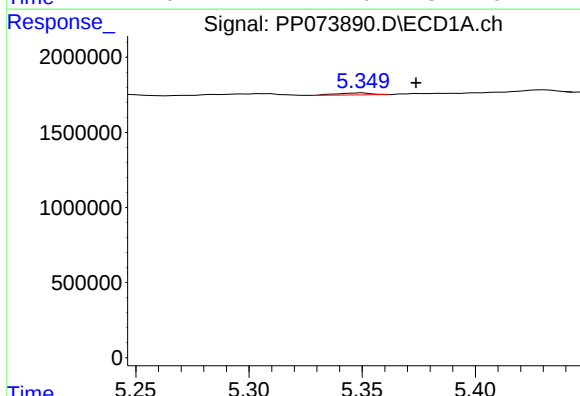


#12 AR-1232-2

R.T.: 5.351 min
Delta R.T.: -0.023 min
Response: 135747
Conc: 8.35 ng/ml

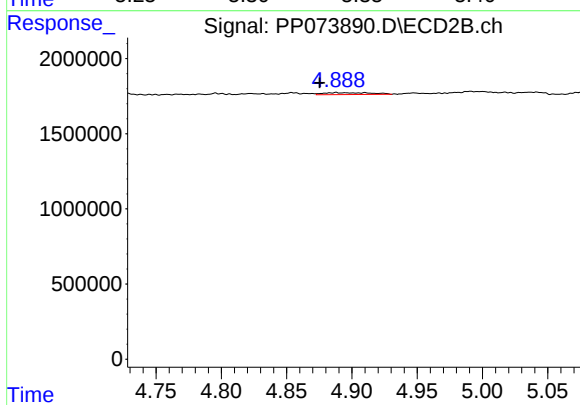

#12 AR-1232-2


R.T.: 4.888 min
Delta R.T.: 0.013 min
Response: 317515
Conc: 6.66 ng/ml

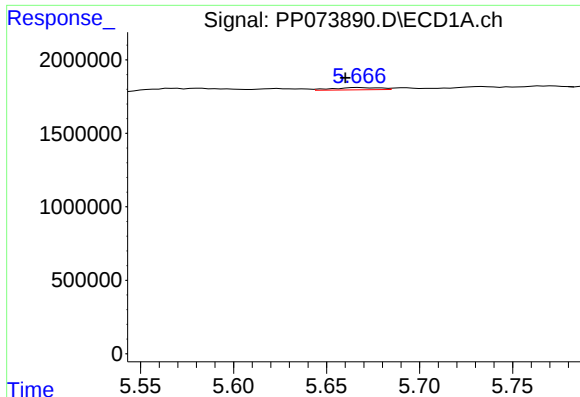

#13 AR-1232-3


R.T.: 5.668 min
Delta R.T.: 0.007 min
Response: 271311
Conc: 8.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

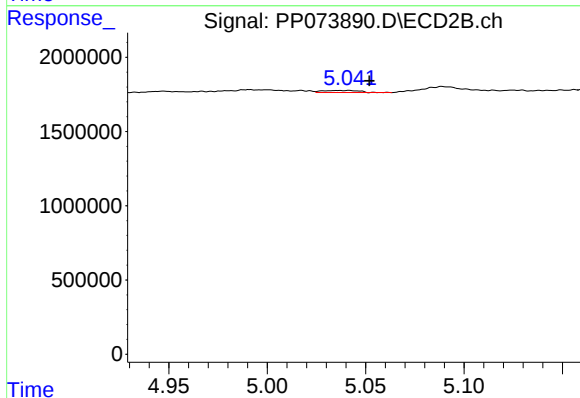


#13 AR-1232-3

R.T.: 5.041 min
Delta R.T.: -0.011 min
Response: 182604
Conc: 7.30 ng/ml

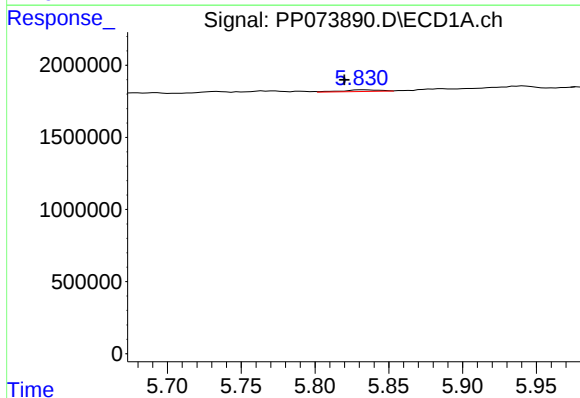


#14 AR-1232-4

R.T.: 5.832 min
Delta R.T.: 0.012 min
Response: 201991
Conc: 12.28 ng/ml

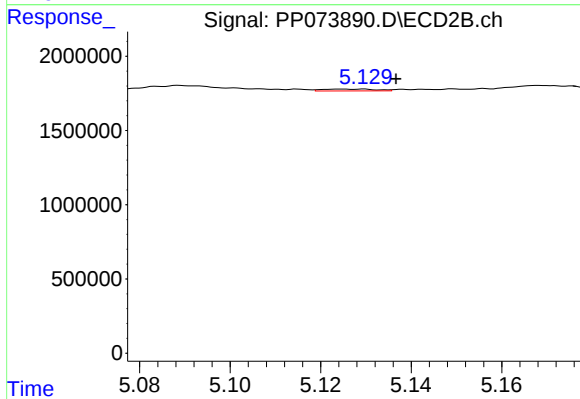

#14 AR-1232-4


R.T.: 5.129 min
Delta R.T.: -0.008 min
Response: 104857
Conc: 4.84 ng/ml

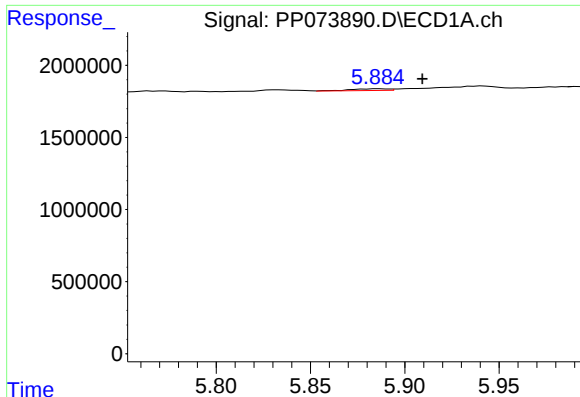

#15 AR-1232-5


R.T.: 5.886 min
Delta R.T.: -0.023 min
Response: 179369
Conc: 16.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

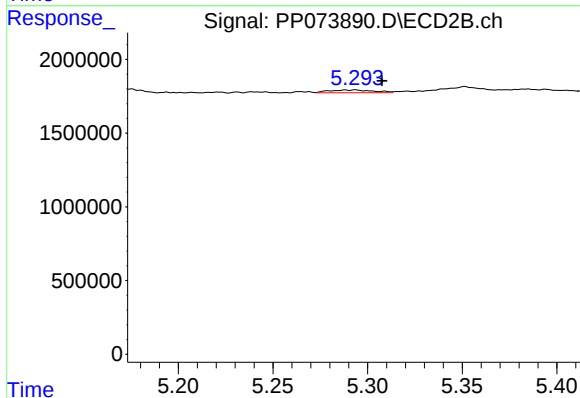


#15 AR-1232-5

R.T.: 5.294 min
Delta R.T.: -0.014 min
Response: 303411
Conc: 13.45 ng/ml

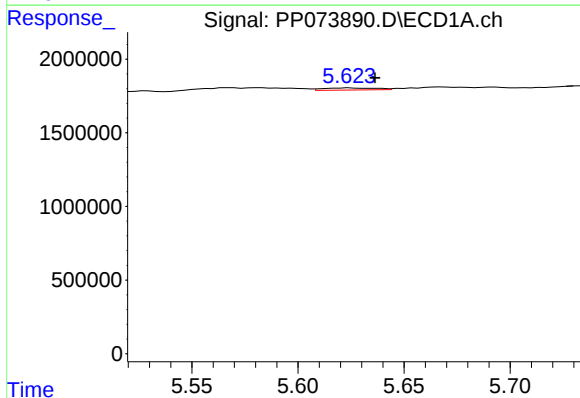


#16 AR-1242-1

R.T.: 5.624 min
Delta R.T.: -0.012 min
Response: 245482
Conc: 6.43 ng/ml

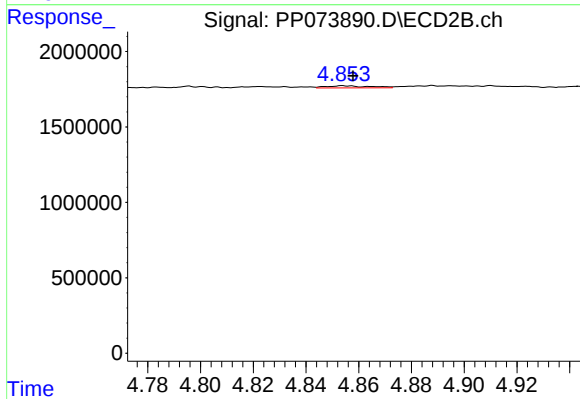

#16 AR-1242-1


R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 160234
Conc: 2.77 ng/ml

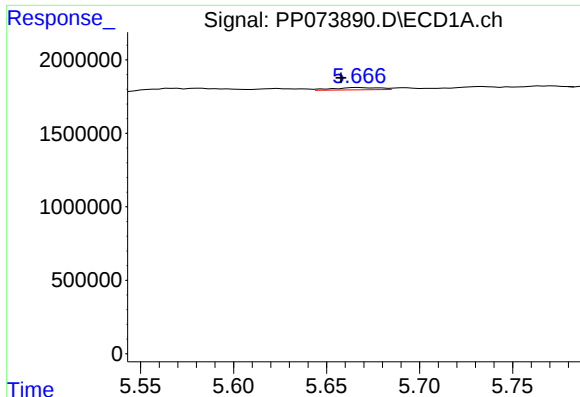

#17 AR-1242-2


R.T.: 5.668 min
Delta R.T.: 0.010 min
Response: 271311
Conc: 4.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

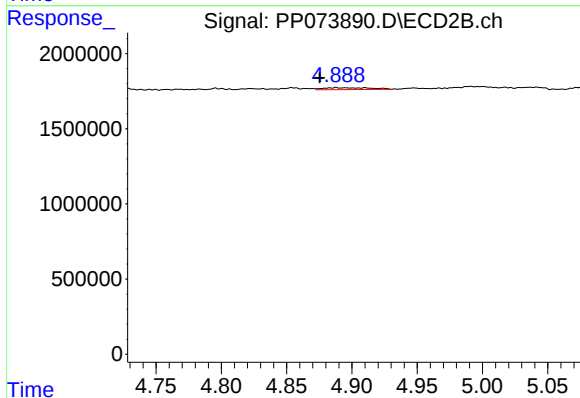


#17 AR-1242-2

R.T.: 4.888 min
Delta R.T.: 0.013 min
Response: 317515
Conc: 3.67 ng/ml

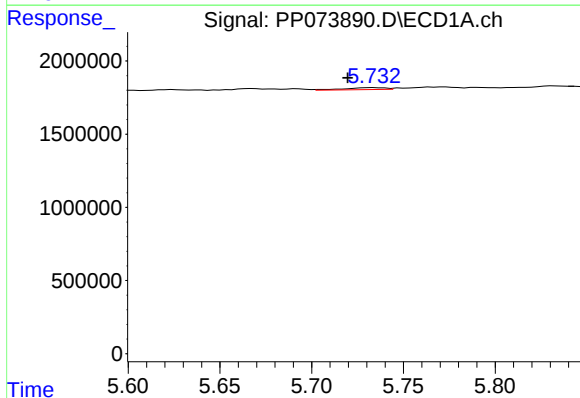


#18 AR-1242-3

R.T.: 5.734 min
Delta R.T.: 0.014 min
Response: 208433
Conc: 5.69 ng/ml

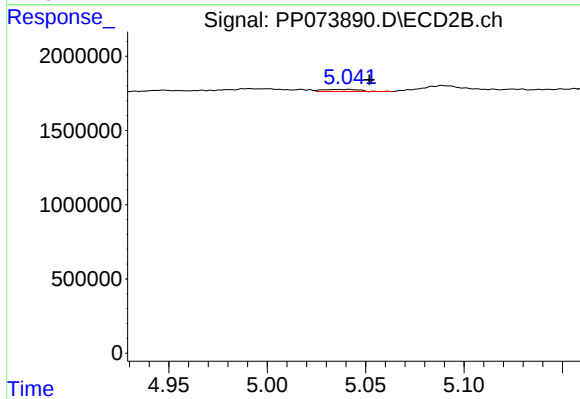

#18 AR-1242-3


R.T.: 5.041 min
Delta R.T.: -0.011 min
Response: 182604
Conc: 3.97 ng/ml

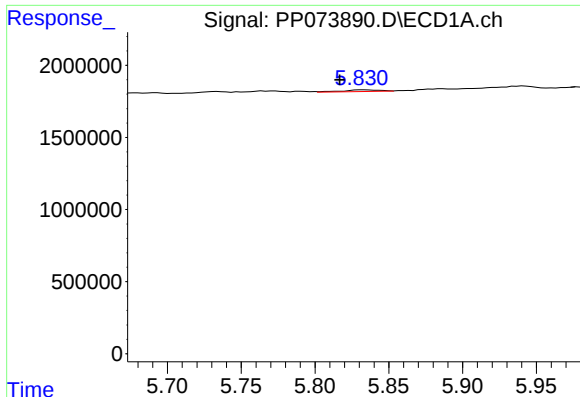

#19 AR-1242-4


R.T.: 5.832 min
Delta R.T.: 0.015 min
Response: 201991
Conc: 6.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

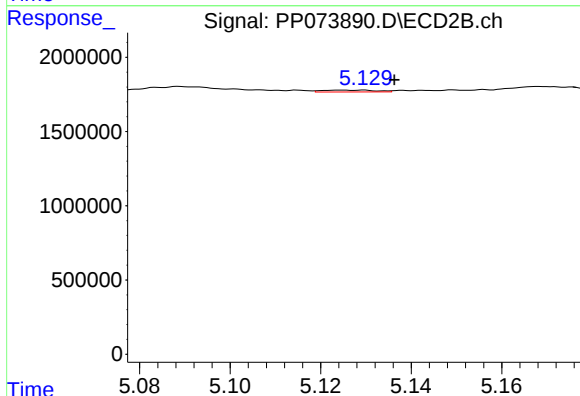


#19 AR-1242-4

R.T.: 5.129 min
Delta R.T.: -0.007 min
Response: 104857
Conc: 2.37 ng/ml

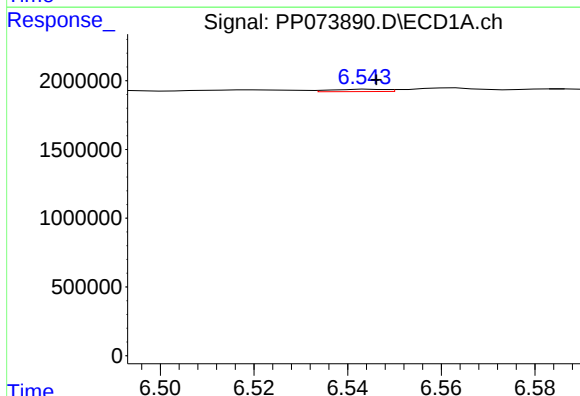


#20 AR-1242-5

R.T.: 6.545 min
Delta R.T.: -0.001 min
Response: 133401
Conc: 4.07 ng/ml

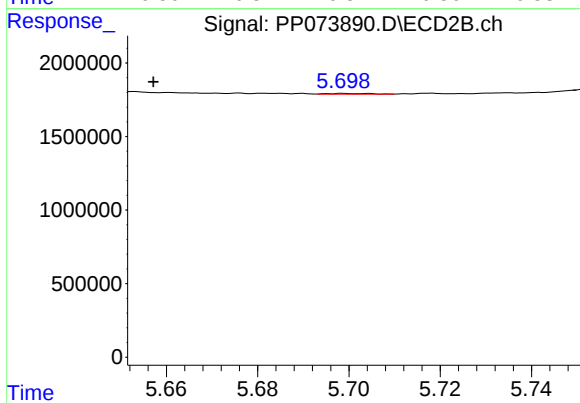

#20 AR-1242-5


R.T.: 5.699 min
Delta R.T.: 0.042 min
Response: 32263
Conc: 0.58 ng/ml

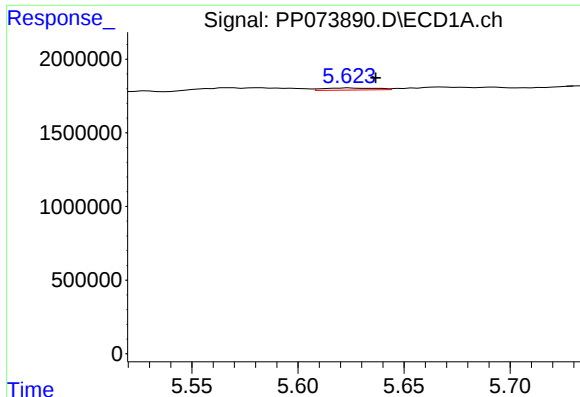

#21 AR-1248-1


R.T.: 5.624 min
Delta R.T.: -0.012 min
Response: 245482
Conc: 7.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

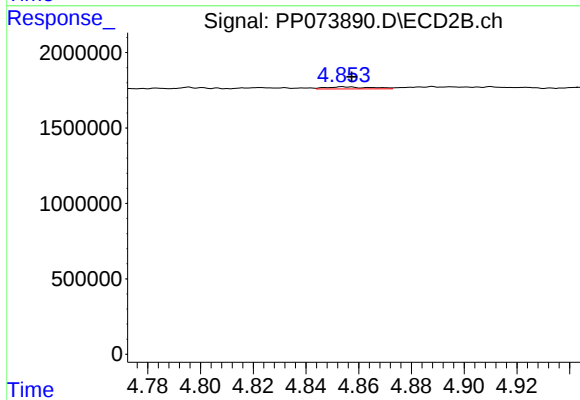


#21 AR-1248-1

R.T.: 4.854 min
Delta R.T.: -0.003 min
Response: 160234
Conc: 3.57 ng/ml

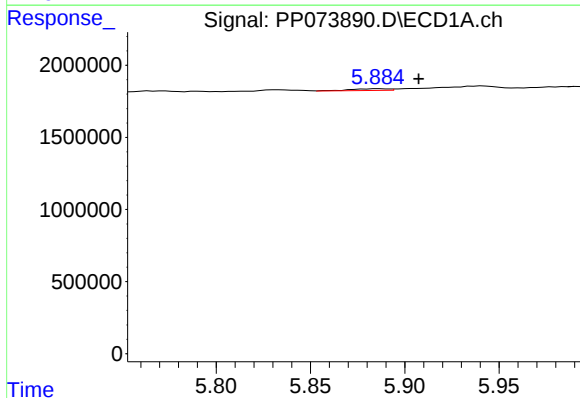


#22 AR-1248-2

R.T.: 5.886 min
Delta R.T.: -0.021 min
Response: 179369
Conc: 4.49 ng/ml

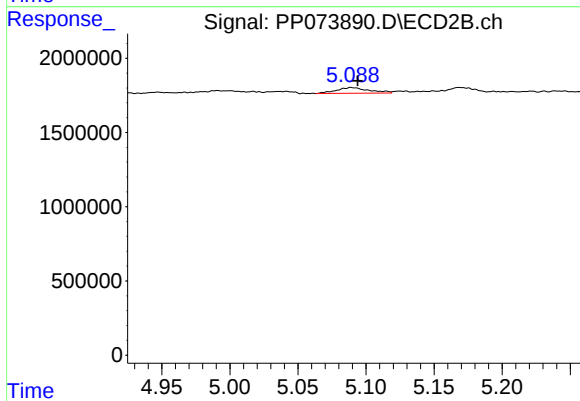

#22 AR-1248-2


R.T.: 5.089 min
Delta R.T.: -0.005 min
Response: 649189
Conc: 10.55 ng/ml

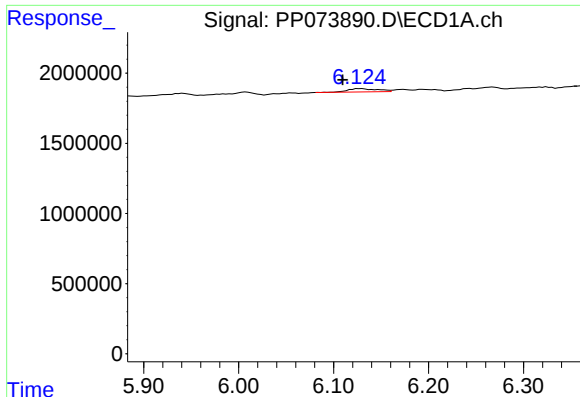

#23 AR-1248-3


R.T.: 6.130 min
Delta R.T.: 0.020 min
Response: 518309
Conc: 11.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

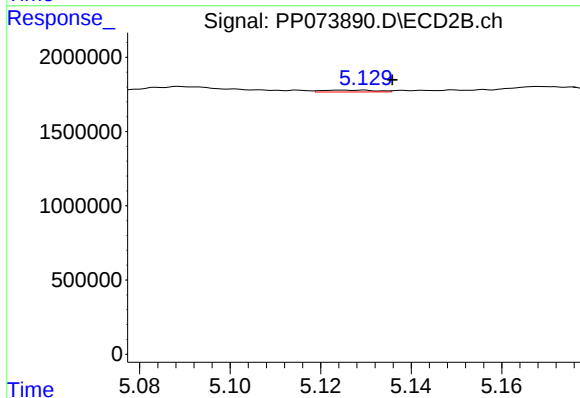


#23 AR-1248-3

R.T.: 5.129 min
Delta R.T.: -0.007 min
Response: 104857
Conc: 1.64 ng/ml

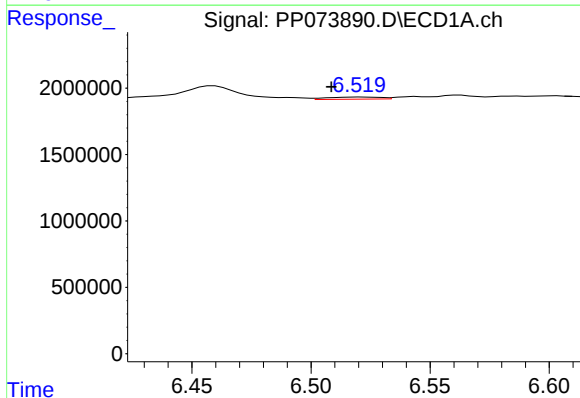


#24 AR-1248-4

R.T.: 6.520 min
Delta R.T.: 0.012 min
Response: 244688
Conc: 4.44 ng/ml

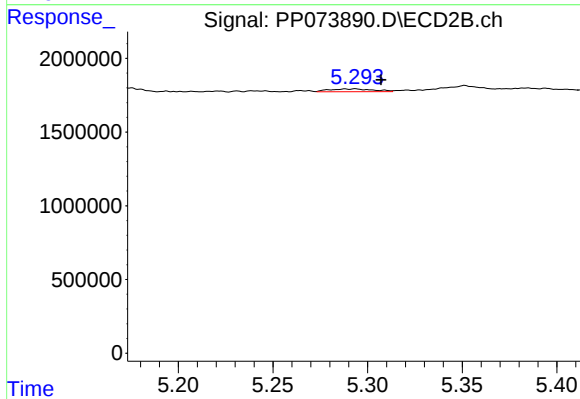

#24 AR-1248-4


R.T.: 5.294 min
Delta R.T.: -0.014 min
Response: 303411
Conc: 4.03 ng/ml

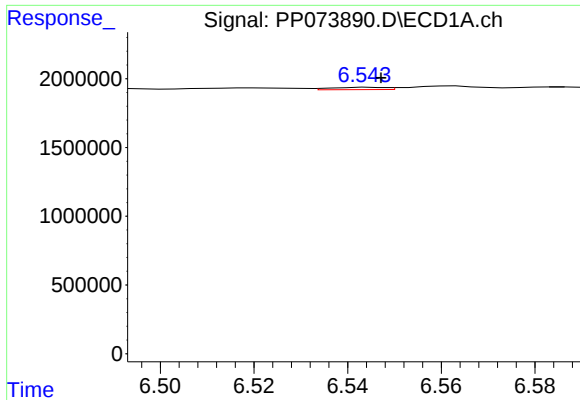

#25 AR-1248-5


R.T.: 6.545 min
Delta R.T.: -0.002 min
Response: 133401
Conc: 2.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

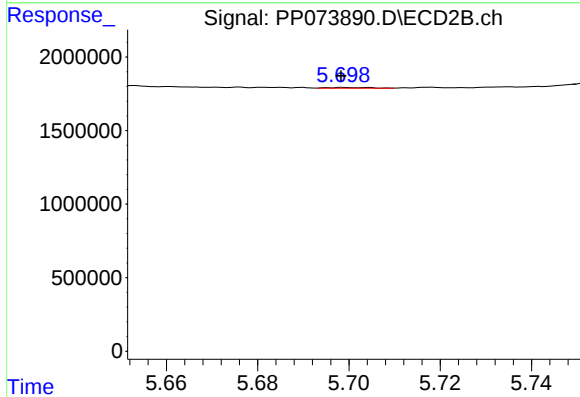


#25 AR-1248-5

R.T.: 5.699 min
Delta R.T.: 0.000 min
Response: 32263
Conc: 0.43 ng/ml

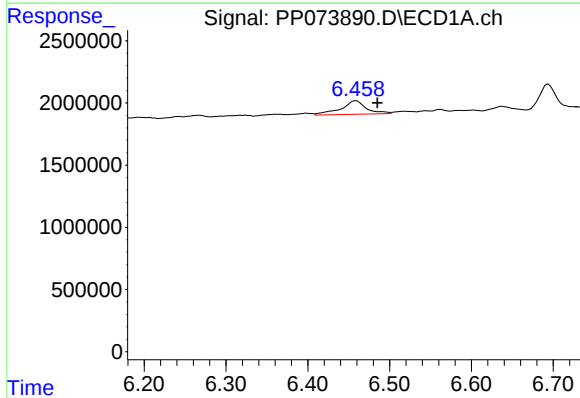


#26 AR-1254-1

R.T.: 6.459 min
Delta R.T.: -0.026 min
Response: 2347127
Conc: 43.80 ng/ml

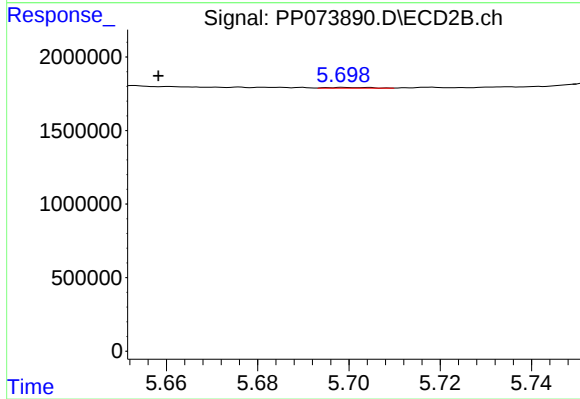

#26 AR-1254-1


R.T.: 5.699 min
Delta R.T.: 0.040 min
Response: 32263
Conc: 0.28 ng/ml

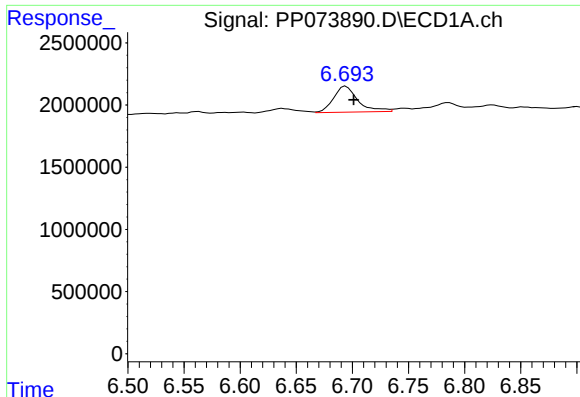

#27 AR-1254-2


R.T.: 6.694 min
Delta R.T.: -0.007 min
Response: 3153523
Conc: 37.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

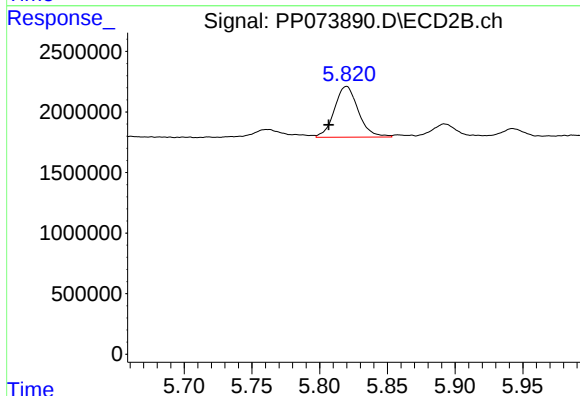


#27 AR-1254-2

R.T.: 5.820 min
Delta R.T.: 0.013 min
Response: 5150050
Conc: 51.18 ng/ml

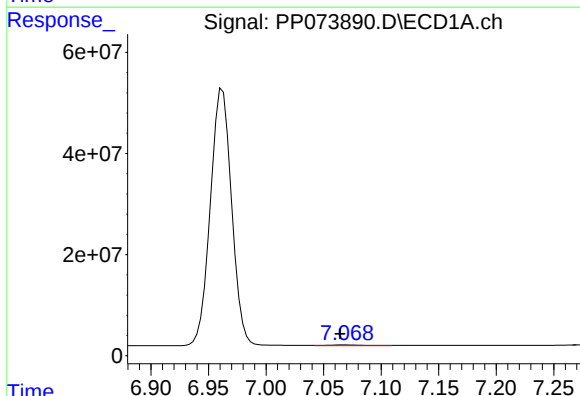


#28 AR-1254-3

R.T.: 7.069 min
Delta R.T.: 0.005 min
Response: 3290624
Conc: 37.25 ng/ml

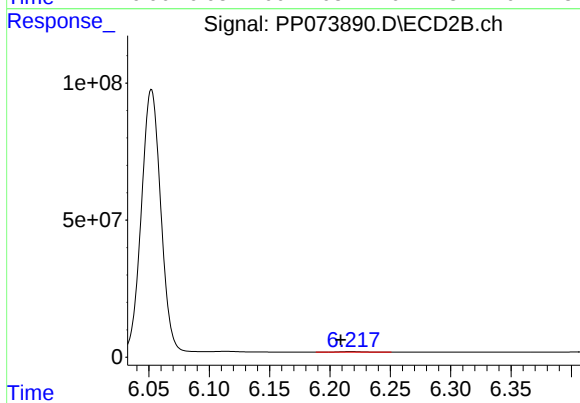

#28 AR-1254-3


R.T.: 6.218 min
Delta R.T.: 0.009 min
Response: 2875628
Conc: 18.62 ng/ml

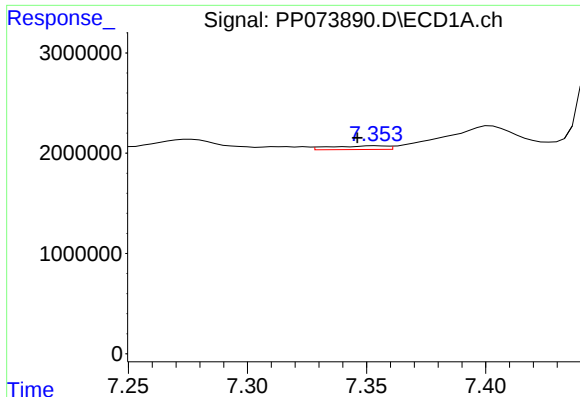

#29 AR-1254-4


R.T.: 7.354 min
Delta R.T.: 0.008 min
Response: 612271
Conc: 7.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

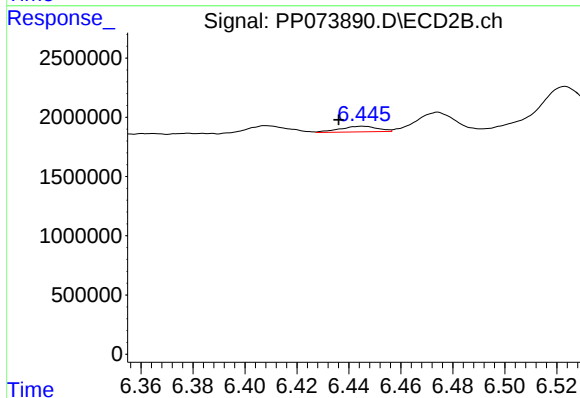


#29 AR-1254-4

R.T.: 6.445 min
Delta R.T.: 0.009 min
Response: 484039
Conc: 5.12 ng/ml

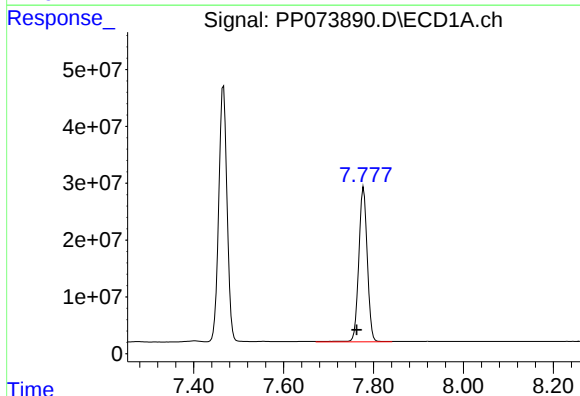


#30 AR-1254-5

R.T.: 7.778 min
Delta R.T.: 0.016 min
Response: 358620667
Conc: 4867.29 ng/ml

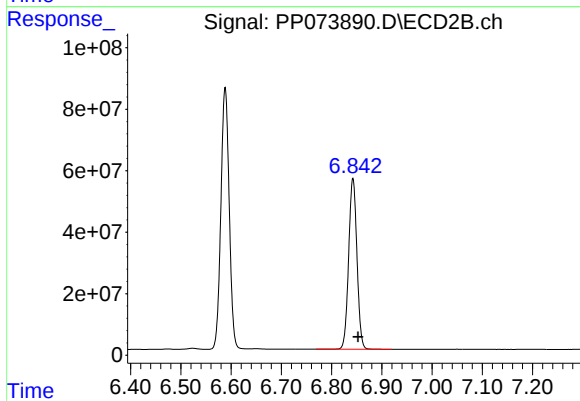

#30 AR-1254-5


R.T.: 6.843 min
Delta R.T.: -0.010 min
Response: 636909947
Conc: 4772.83 ng/ml

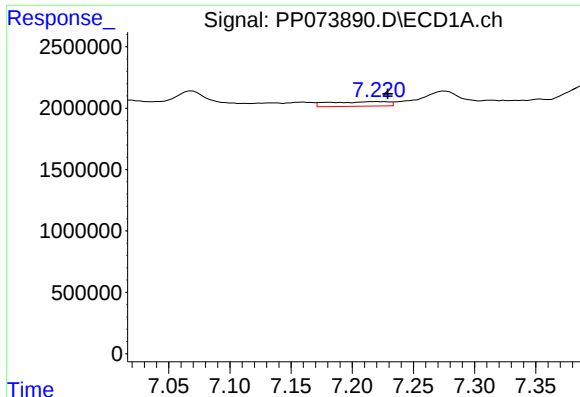

#31 AR-1260-1


R.T.: 7.221 min
Delta R.T.: -0.008 min
Response: 1241945
Conc: 21.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

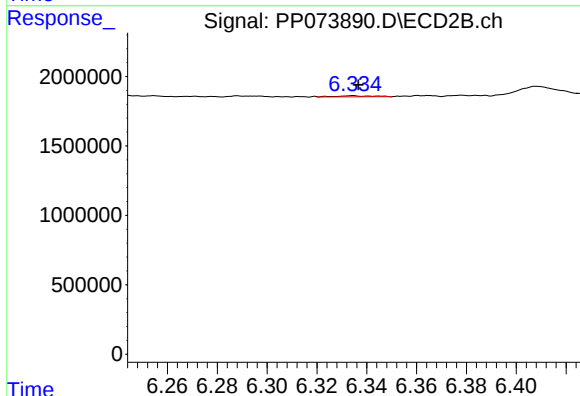


#31 AR-1260-1

R.T.: 6.334 min
Delta R.T.: -0.002 min
Response: 86646
Conc: 0.89 ng/ml

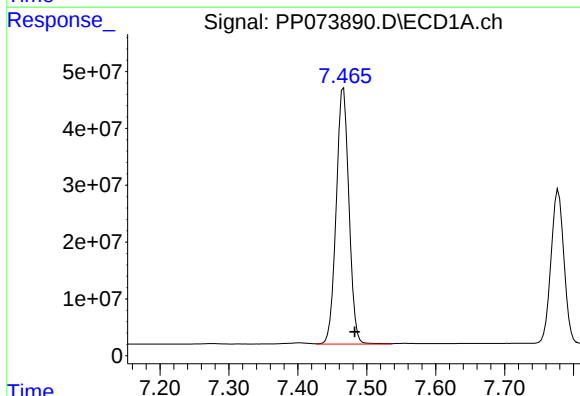


#32 AR-1260-2

R.T.: 7.466 min
Delta R.T.: -0.017 min
Response: 578837527
Conc: 6039.63 ng/ml

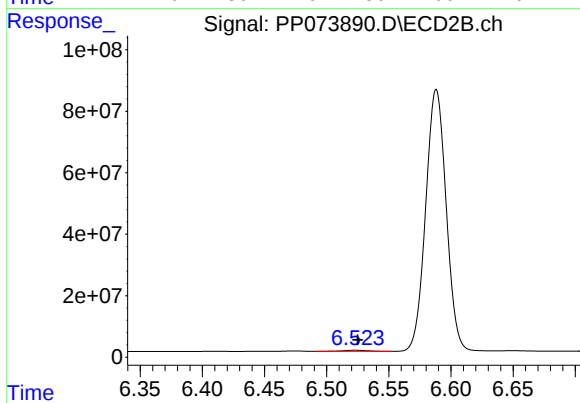

#32 AR-1260-2


R.T.: 6.523 min
Delta R.T.: -0.002 min
Response: 4947334
Conc: 40.28 ng/ml

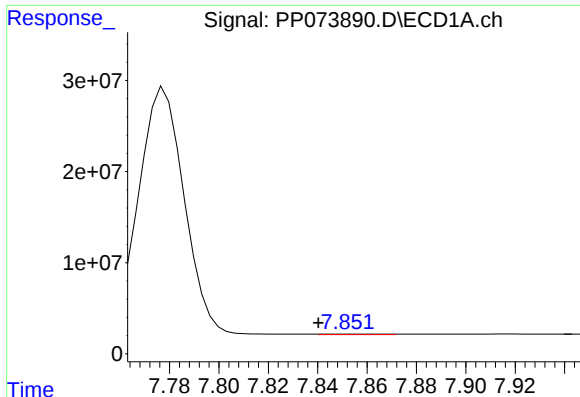

#33 AR-1260-3


R.T.: 7.853 min
Delta R.T.: 0.012 min
Response: 889076
Conc: 12.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

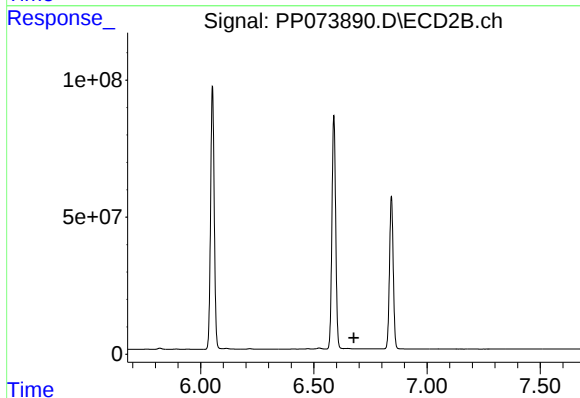


#33 AR-1260-3

R.T.: 6.650 min
Delta R.T.: -0.027 min
Response: -970228
Conc: N.D.

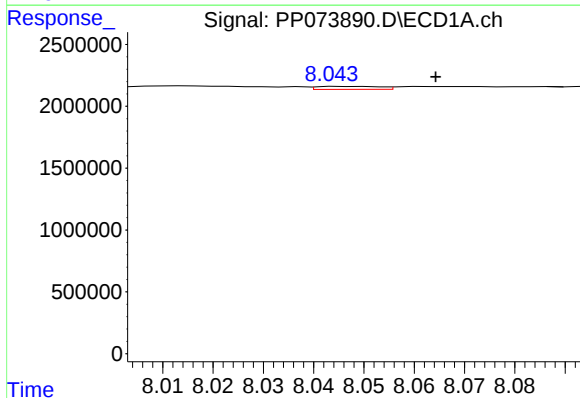


#34 AR-1260-4

R.T.: 8.046 min
Delta R.T.: -0.018 min
Response: 209435
Conc: 3.21 ng/ml

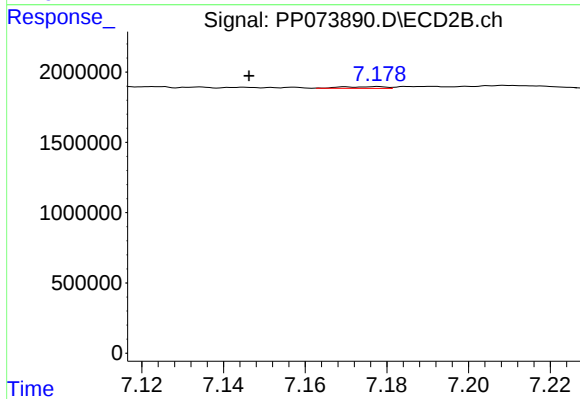

#34 AR-1260-4


R.T.: 7.178 min
Delta R.T.: 0.031 min
Response: 95079
Conc: 1.06 ng/ml

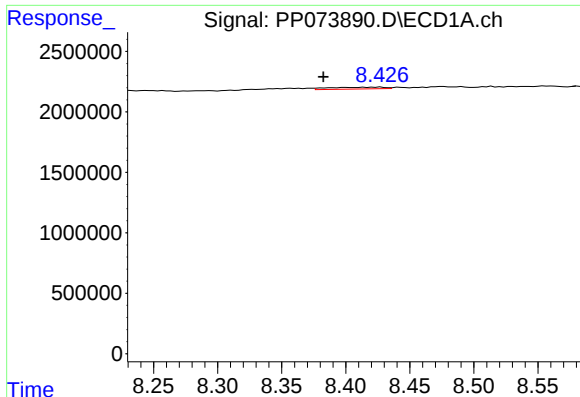

#35 AR-1260-5


R.T.: 8.400 min
Delta R.T.: 0.017 min
Response: 447077
Conc: 2.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

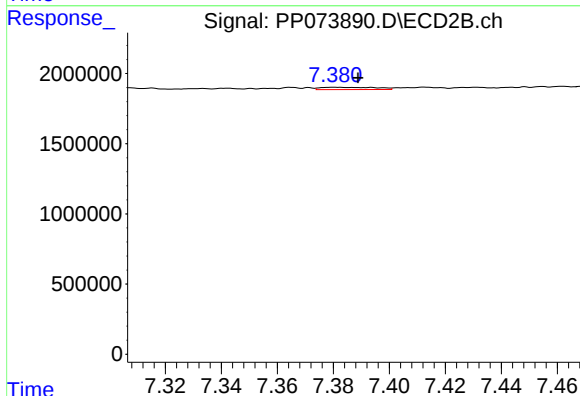


#35 AR-1260-5

R.T.: 7.381 min
Delta R.T.: -0.008 min
Response: 224967
Conc: 1.00 ng/ml

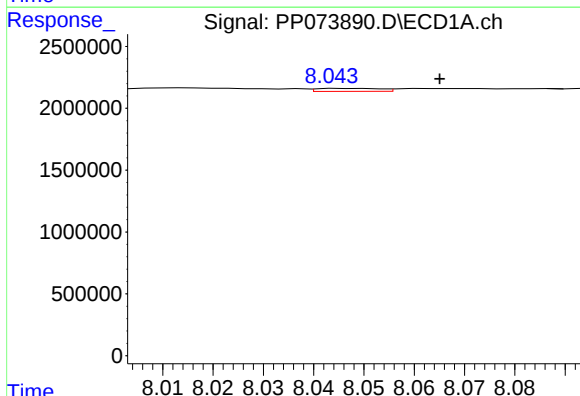


#36 AR-1262-1

R.T.: 8.046 min
Delta R.T.: -0.019 min
Response: 209435
Conc: 2.41 ng/ml

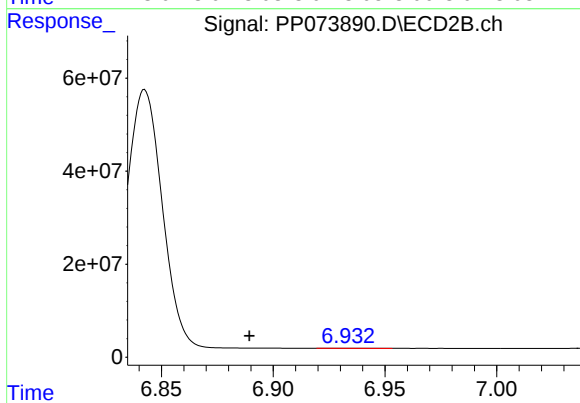

#36 AR-1262-1


R.T.: 6.932 min
Delta R.T.: 0.043 min
Response: 149341
Conc: 1.01 ng/ml

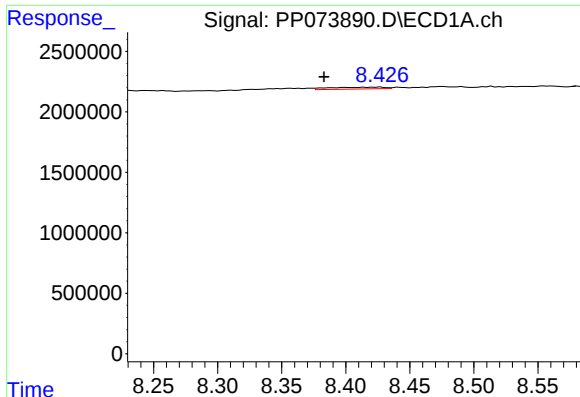

#37 AR-1262-2


R.T.: 8.400 min
Delta R.T.: 0.017 min
Response: 447077
Conc: 2.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

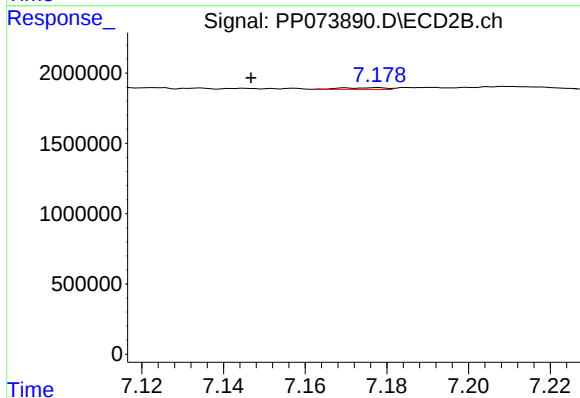


#37 AR-1262-2

R.T.: 7.178 min
Delta R.T.: 0.031 min
Response: 95079
Conc: 0.74 ng/ml

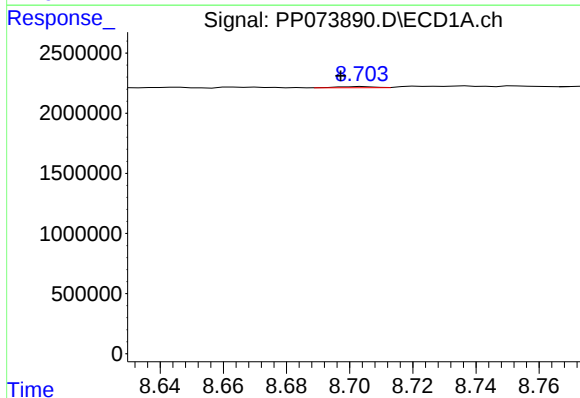


#38 AR-1262-3

R.T.: 8.704 min
Delta R.T.: 0.007 min
Response: 77598
Conc: 0.62 ng/ml

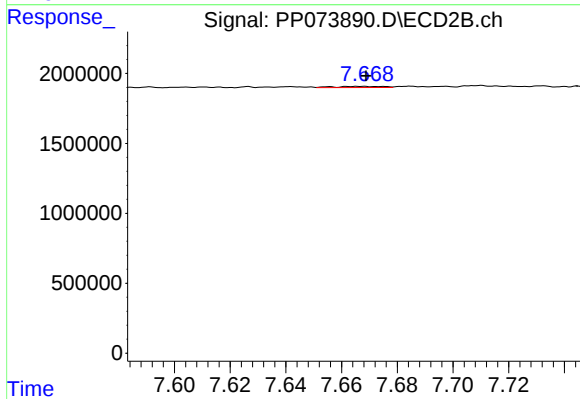

#38 AR-1262-3


R.T.: 7.667 min
Delta R.T.: -0.002 min
Response: 102388
Conc: 0.90 ng/ml

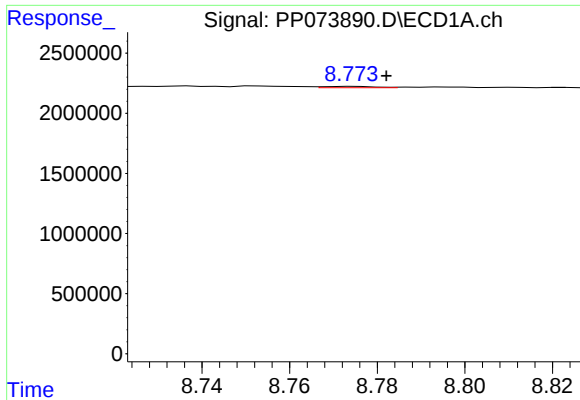

#39 AR-1262-4


R.T.: 8.775 min
Delta R.T.: -0.007 min
Response: 90144
Conc: 0.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

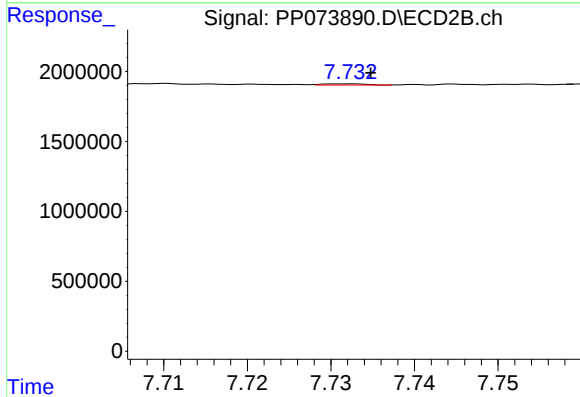


#39 AR-1262-4

R.T.: 7.732 min
Delta R.T.: -0.003 min
Response: 29271
Conc: 0.16 ng/ml

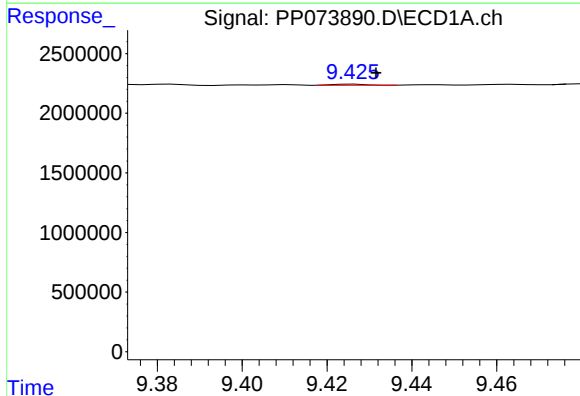


#40 AR-1262-5

R.T.: 9.427 min
Delta R.T.: -0.005 min
Response: 53870
Conc: 0.85 ng/ml

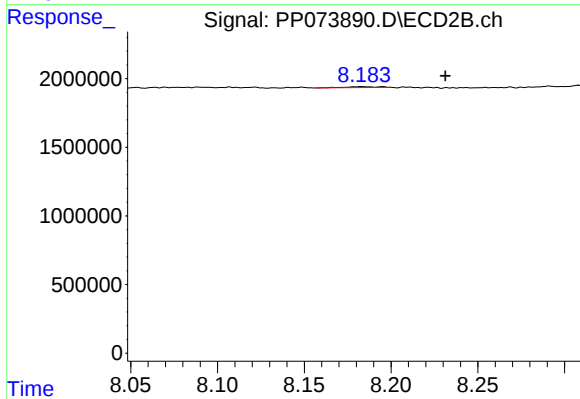

#40 AR-1262-5


R.T.: 8.183 min
Delta R.T.: -0.048 min
Response: 98328
Conc: 1.16 ng/ml

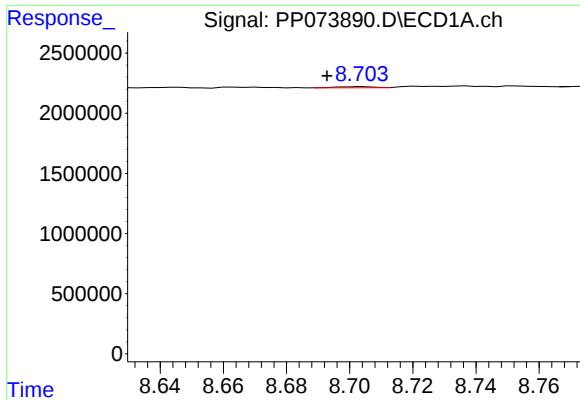

#41 AR-1268-1


R.T.: 8.704 min
Delta R.T.: 0.012 min
Response: 77598
Conc: 0.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

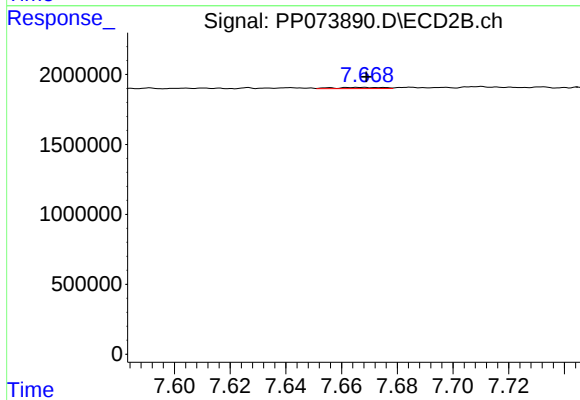


#41 AR-1268-1

R.T.: 7.667 min
Delta R.T.: -0.002 min
Response: 102388
Conc: 0.33 ng/ml

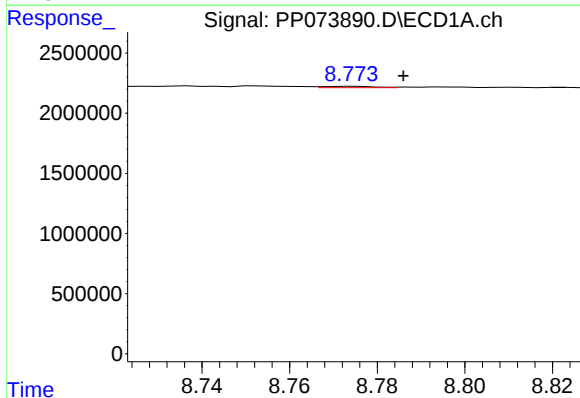


#42 AR-1268-2

R.T.: 8.775 min
Delta R.T.: -0.011 min
Response: 90144
Conc: 0.47 ng/ml

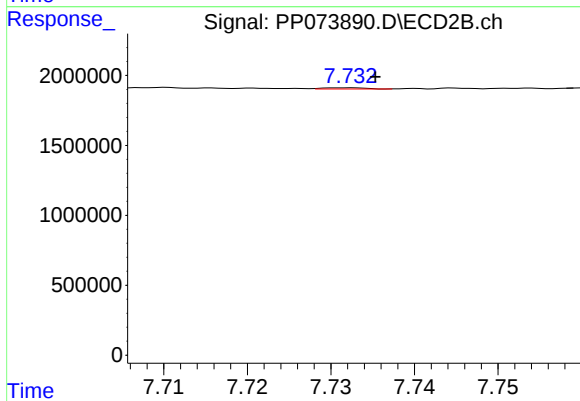

#42 AR-1268-2


R.T.: 7.732 min
Delta R.T.: -0.003 min
Response: 29271
Conc: 0.11 ng/ml

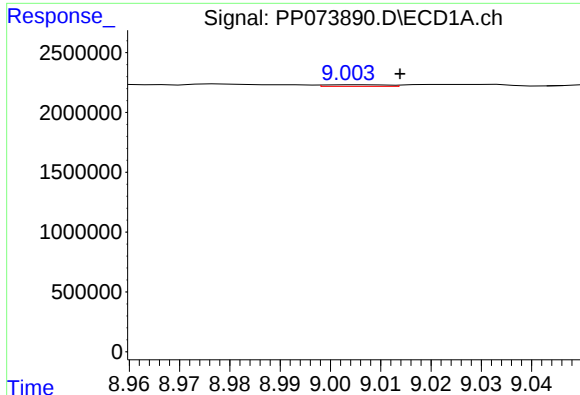

#43 AR-1268-3


R.T.: 9.005 min
Delta R.T.: -0.009 min
Response: 110791
Conc: 0.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

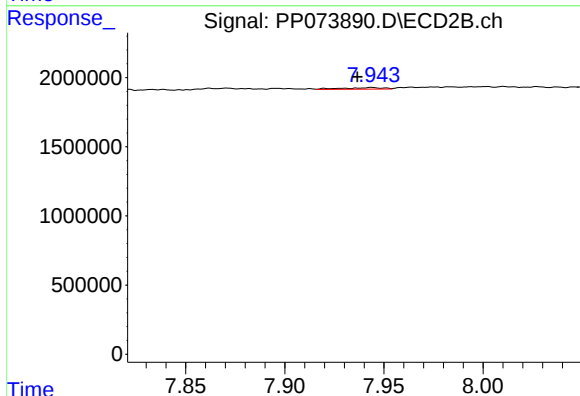


#43 AR-1268-3

R.T.: 7.944 min
Delta R.T.: 0.007 min
Response: 163166
Conc: 0.72 ng/ml

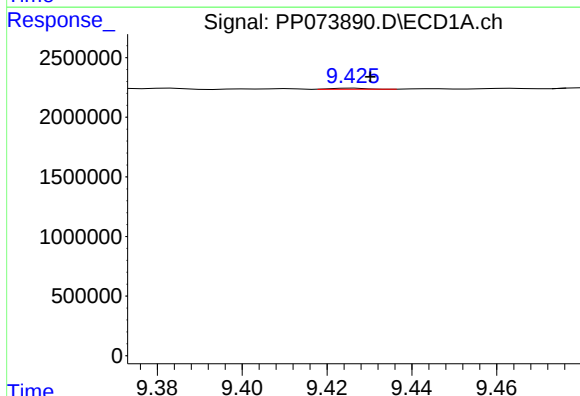


#44 AR-1268-4

R.T.: 9.427 min
Delta R.T.: -0.004 min
Response: 53870
Conc: 0.77 ng/ml

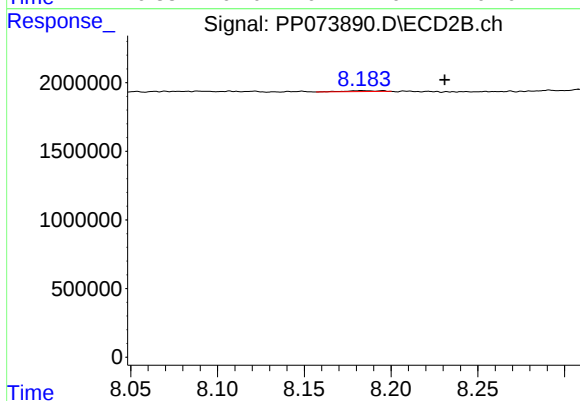

#44 AR-1268-4


R.T.: 8.183 min
Delta R.T.: -0.048 min
Response: 98328
Conc: 1.06 ng/ml

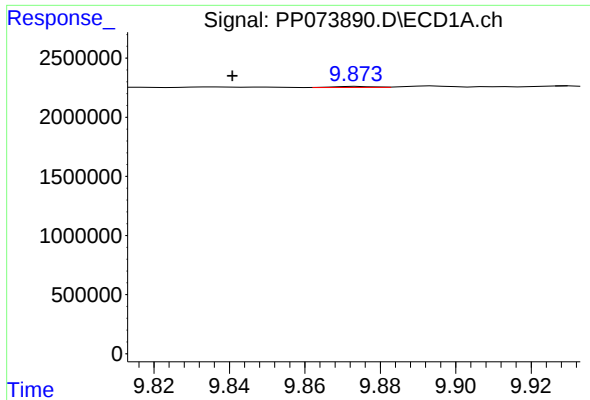

#45 AR-1268-5

R.T.: 9.874 min
Delta R.T.: 0.033 min
Response: 62892
Conc: 0.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

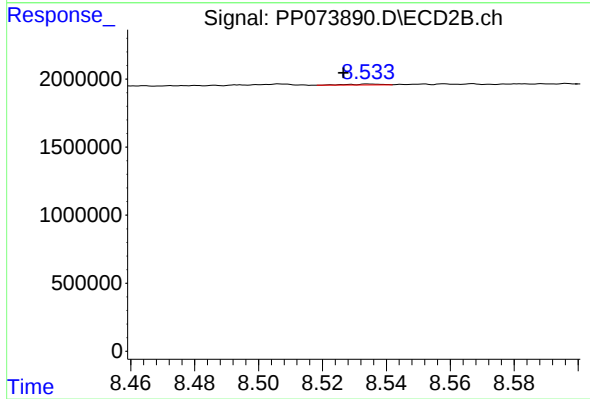

#45 AR-1268-5

R.T.: 8.535 min
Delta R.T.: 0.008 min
Response: 49227
Conc: 0.08 ng/ml