

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD P\Data\PP071818\
 Data File : PP026771.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2018 9:48
 Operator : EI\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 14:54:40 2018
 Quant Method : Z:\bestpcbsrv\HPCHEM1\ECD_P\methods\PP071318.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 13 23:16:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
Target Compounds						
10) T Pentachlo...	14.332	0.000	16730234	0	2.474	N.D. #
15) T Picloram	17.594	0.000	24270264	0	6.366	N.D. #
16) T DCPA	18.200	0.000	10750647	0	2.939	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD P\Data\PP071818\
Data File : PP026771.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2018 9:48
Operator : EI\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 14:54:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071318.M
Quant Title : 8080.M
QLast Update : Fri Jul 13 23:16:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

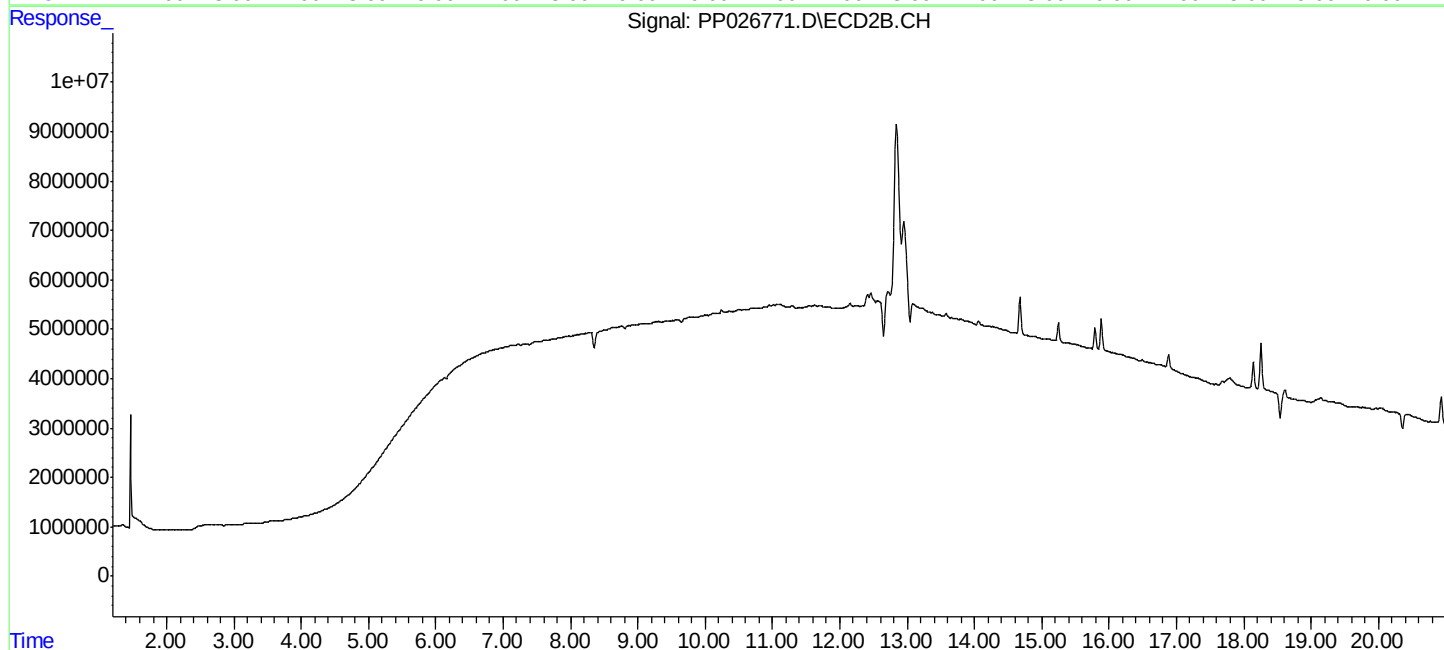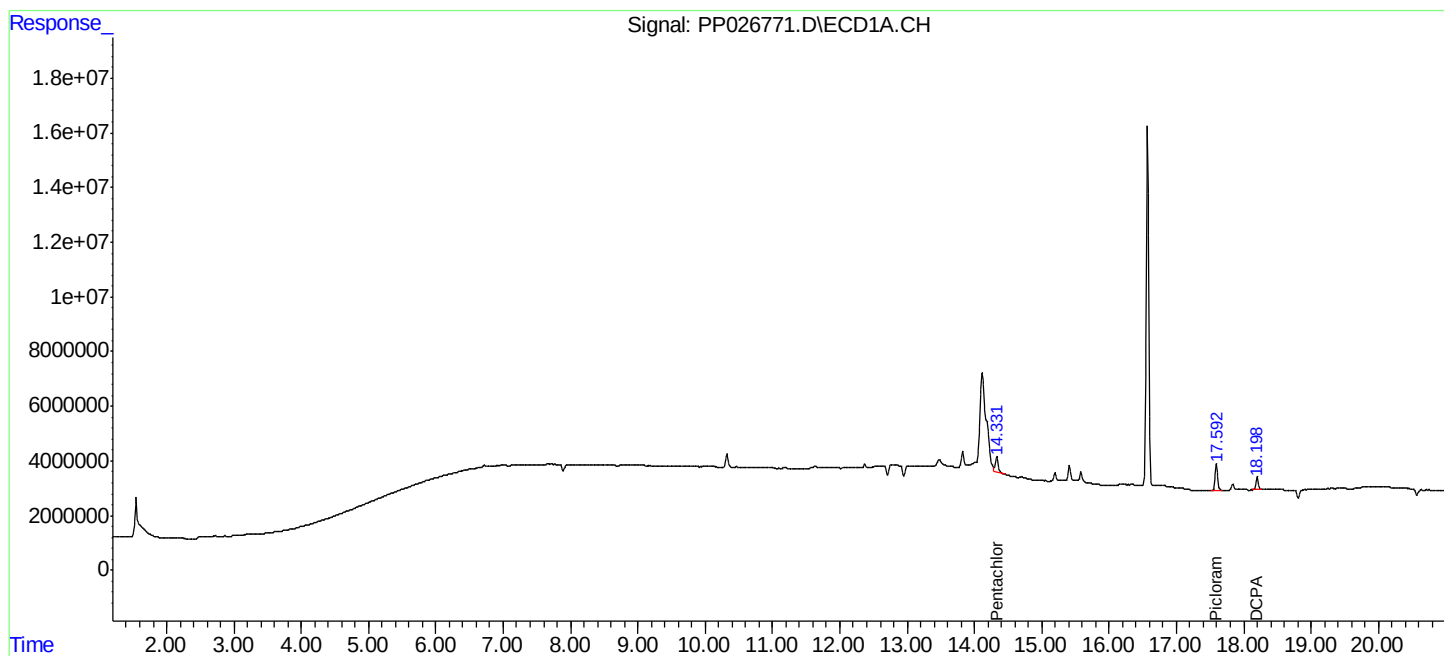


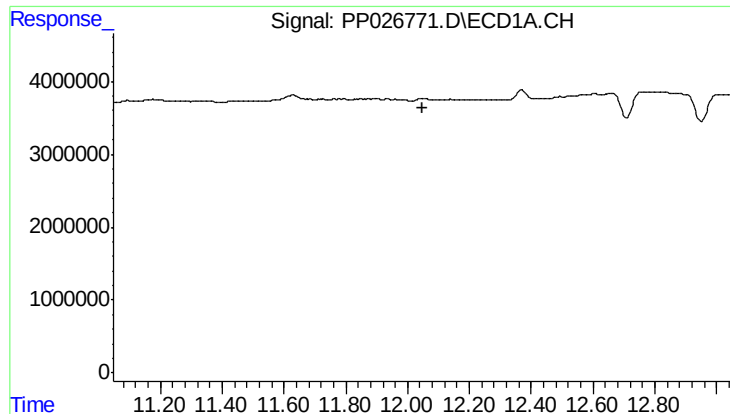

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 12.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

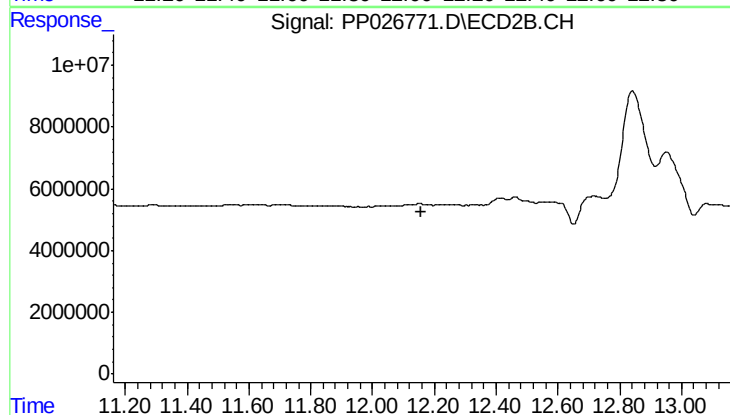


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 12.158 min
Response: 0
Conc: N.D.

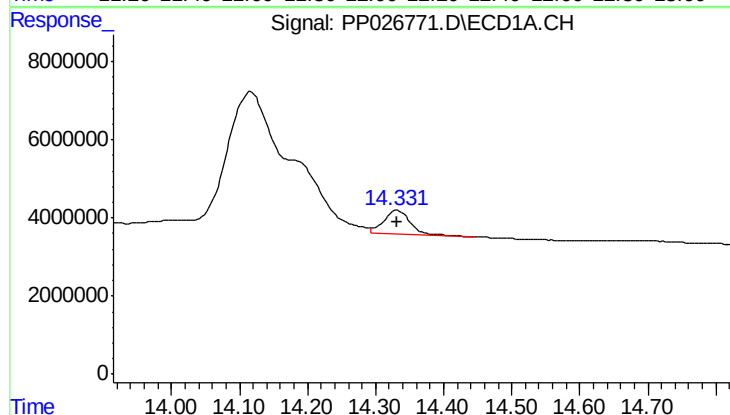


#10 Pentachlorophenol

R.T.: 14.332 min
Delta R.T.: 0.001 min
Response: 16730234
Conc: 2.47 ng/ml

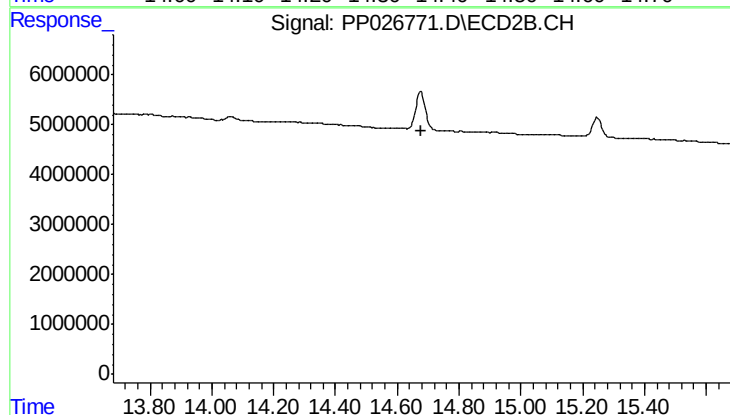

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 14.680 min
Response: 0
Conc: N.D.

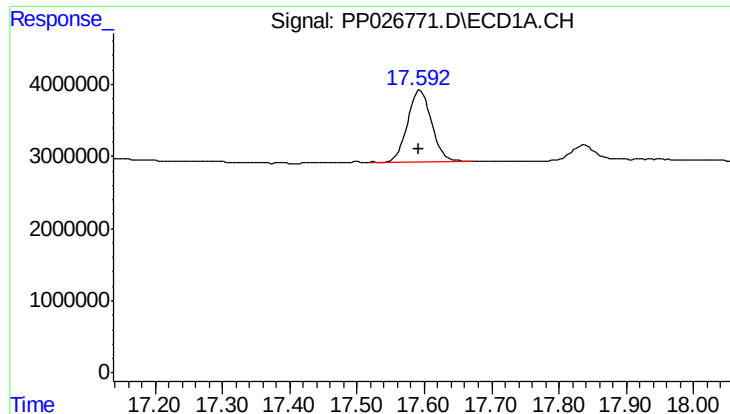

#15 Picloram


R.T.: 17.594 min
Delta R.T.: 0.003 min
Response: 24270264
Conc: 6.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

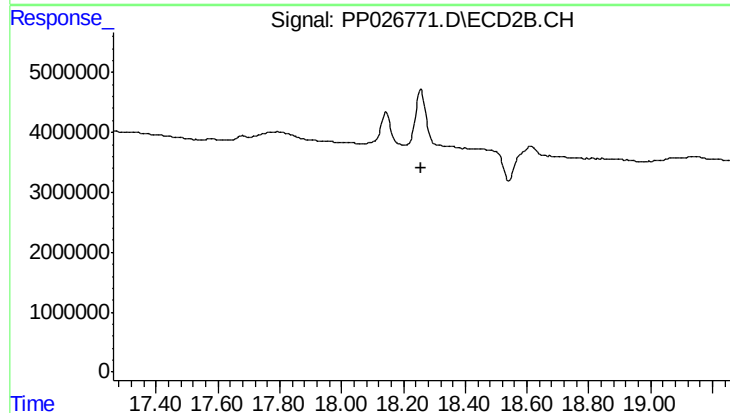


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.258 min
Response: 0
Conc: N.D.

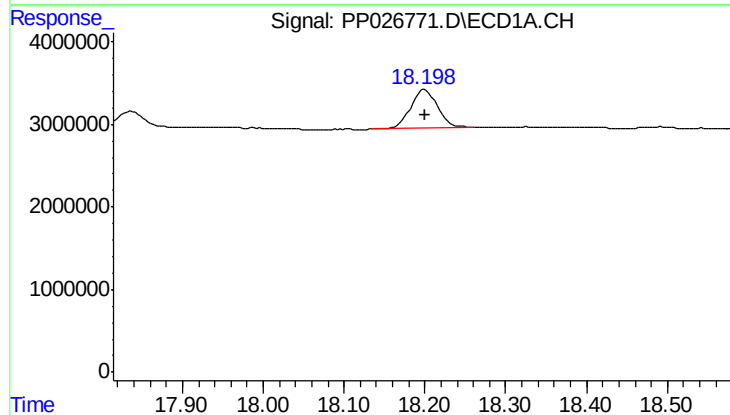

#16 DCPA

R.T.: 18.200 min
Delta R.T.: 0.000 min
Response: 10750647
Conc: 2.94 ng/ml

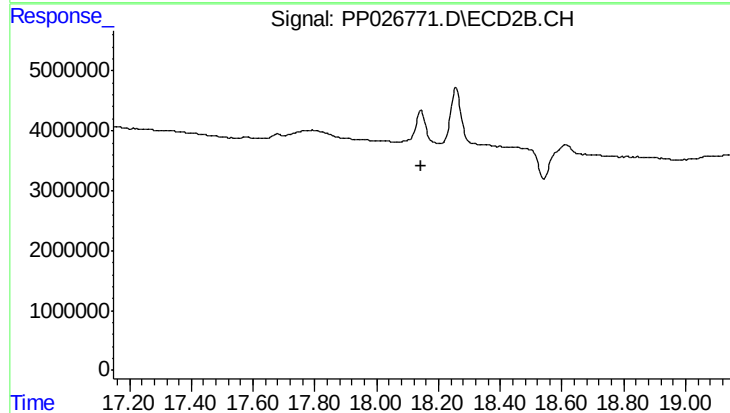

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.145 min
Response: 0
Conc: N.D.