

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071825\
 Data File : PP073950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2025 19:33
 Operator : YP\AJ
 Sample : Q2633-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FIBER-GLASS-TANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 23:18:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.487	3.776	25001629	37075388	18.256	20.125
2) SA Decachlor...	10.169	8.771	18849117	26692828	17.276	20.174

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071825\
Data File : PP073950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2025 19:33
Operator : YP\AJ
Sample : Q2633-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FIBER-GLASS-TANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 23:18:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

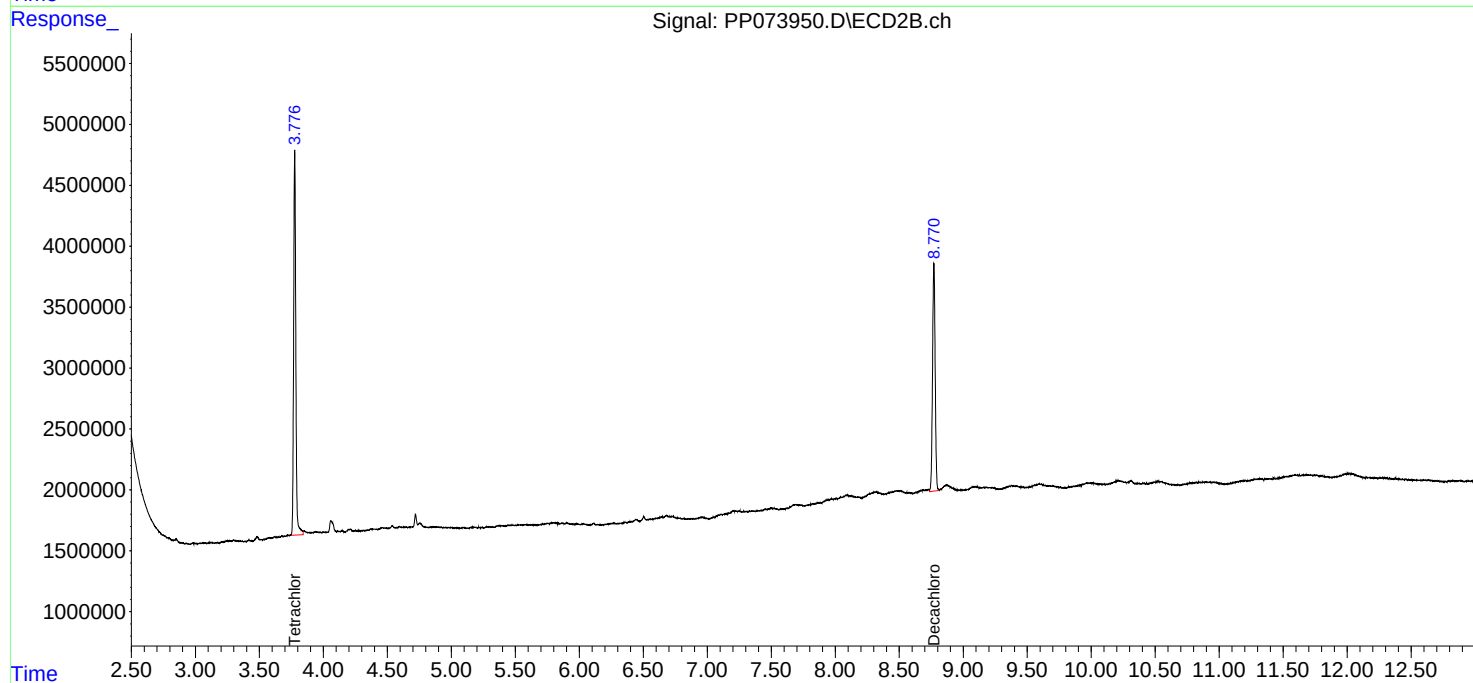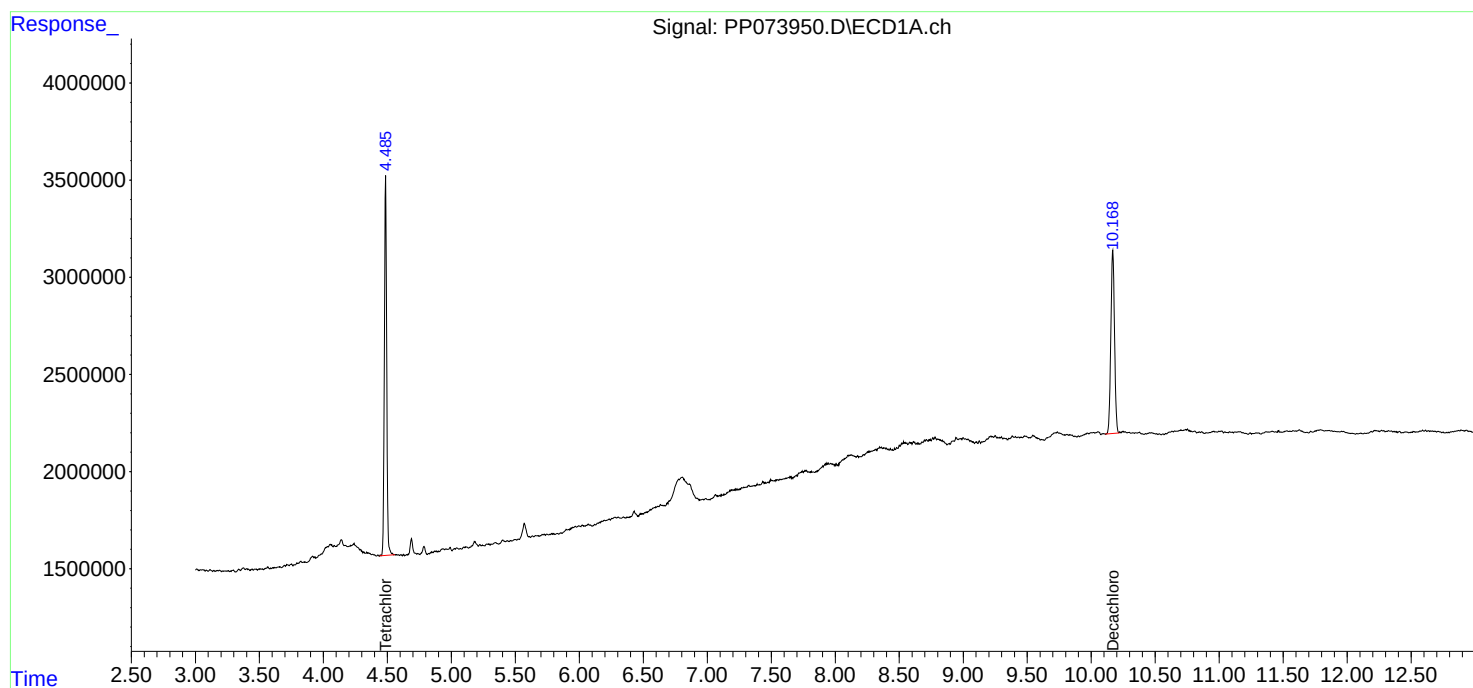


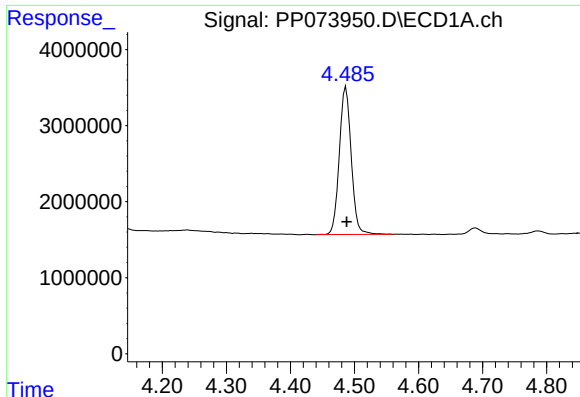

#1 Tetrachloro-m-xylene


R.T.: 4.487 min
Delta R.T.: -0.001 min
Response: 25001629
Conc: 18.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
FIBER-GLASS-TANK

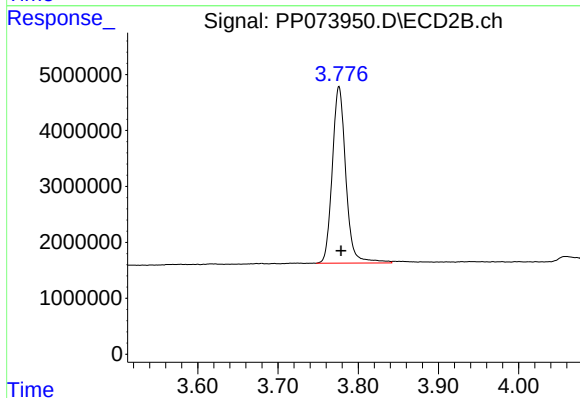


#1 Tetrachloro-m-xylene

R.T.: 3.776 min
Delta R.T.: -0.002 min
Response: 37075388
Conc: 20.12 ng/ml

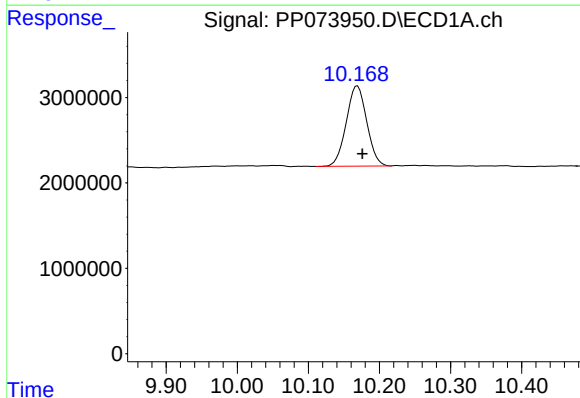

#2 Decachlorobiphenyl

R.T.: 10.169 min
Delta R.T.: -0.007 min
Response: 18849117
Conc: 17.28 ng/ml

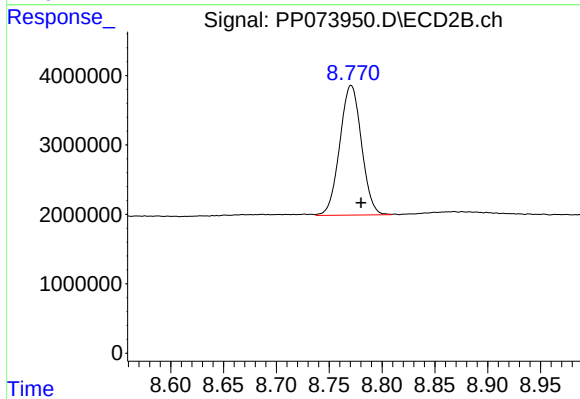

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.009 min
Response: 26692828
Conc: 20.17 ng/ml