

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071921\
 Data File : PP037359.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jul 2021 12:49
 Operator : DD\AJ
 Sample : M3051-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-41257-59

Manual Integrations
 APPROVED

mohammad
 7/20/2021 11:44:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 05:48:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.959	3.950	445923	252587	9.811	9.231
2) SA Decachlor...	10.991	9.244	591762	332138	12.854m	11.932

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071921\
Data File : PP037359.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2021 12:49
Operator : DD\AJ
Sample : M3051-10
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-41257-59


Manual Integrations
APPROVED

mohammad
7/20/2021 11:44:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 05:48:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

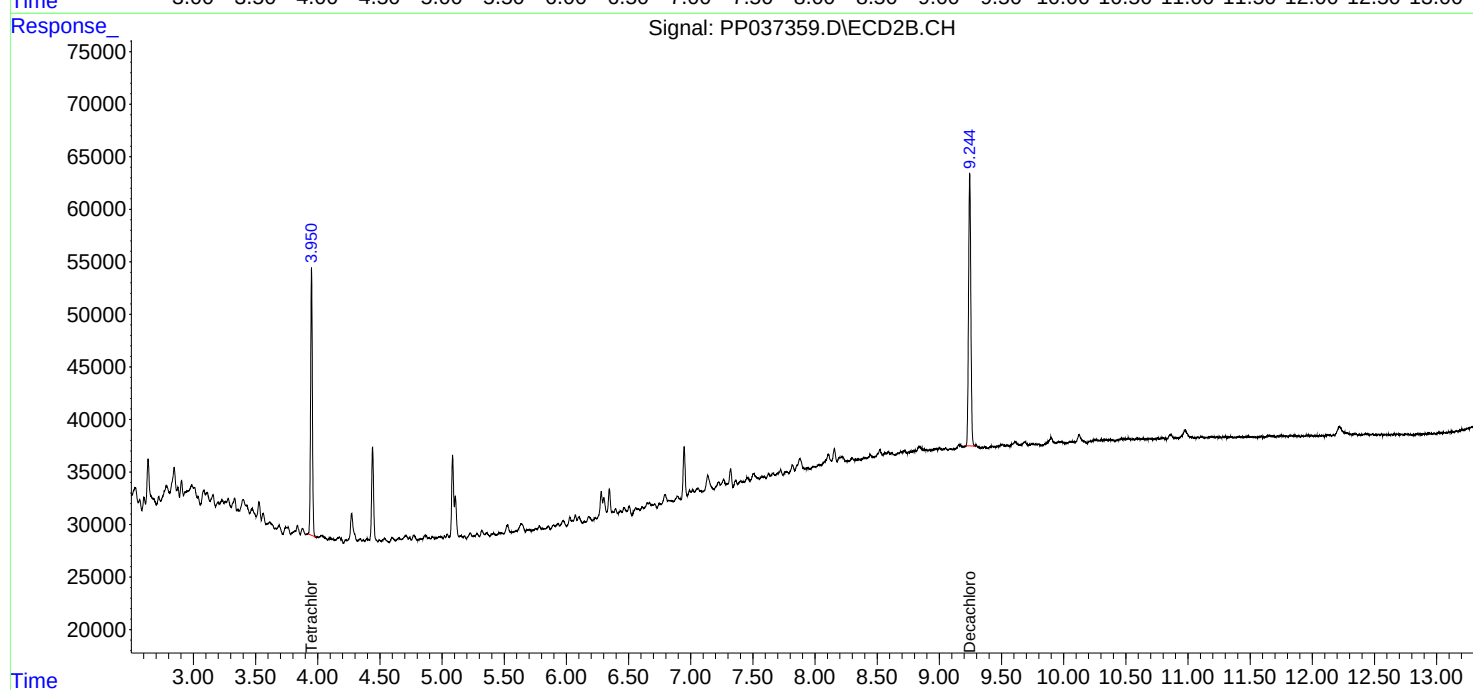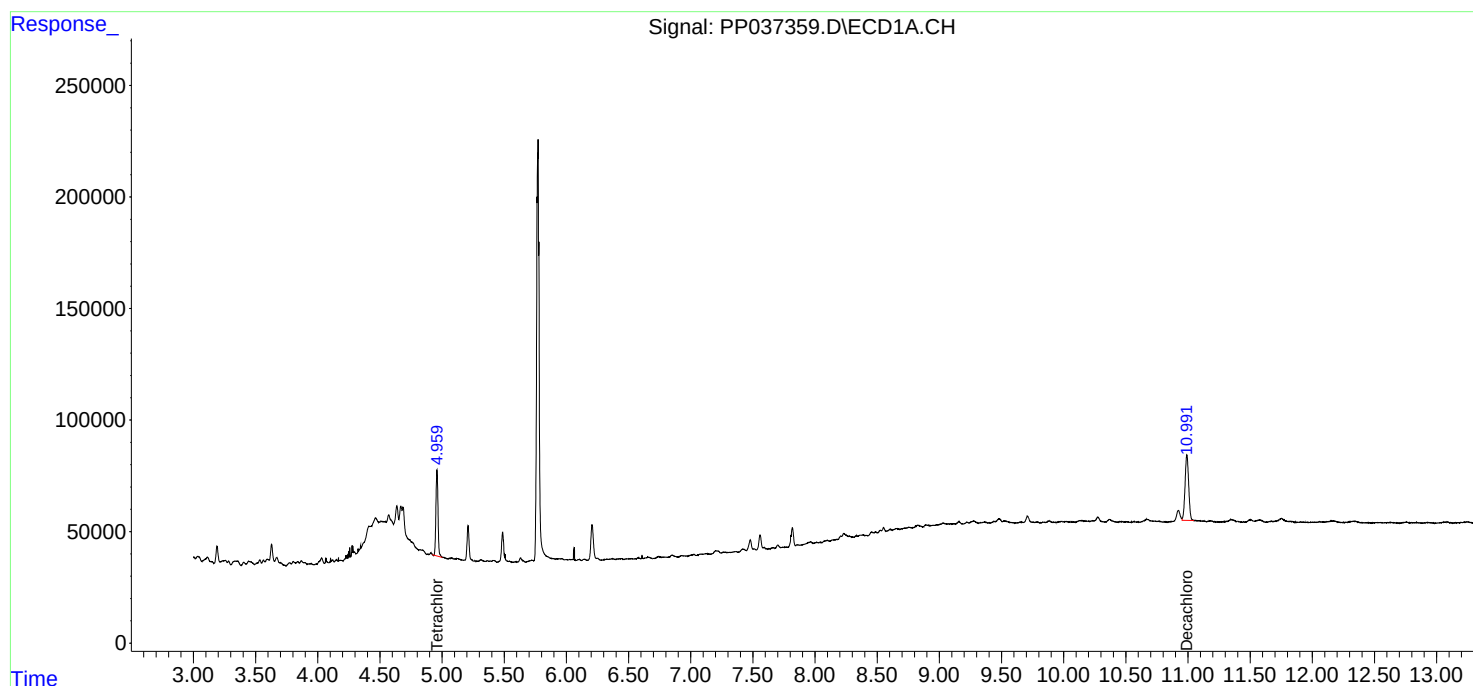

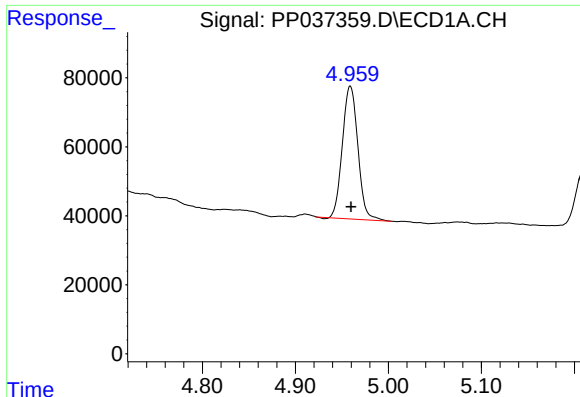


#1 Tetrachloro-m-xylene

R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 445923
Conc: 9.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-41257-59


Manual Integrations
APPROVED

mohammad
7/20/2021 11:44:32 AM

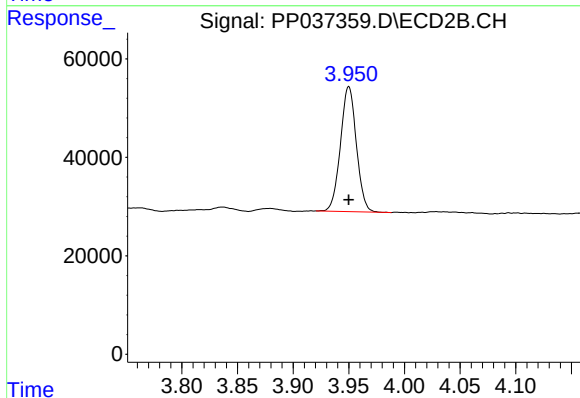


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 252587
Conc: 9.23 ng/ml

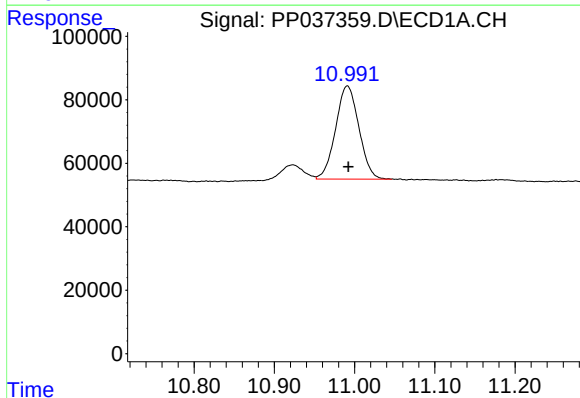

#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: -0.001 min
Response: 591762
Conc: 12.85 ng/ml m

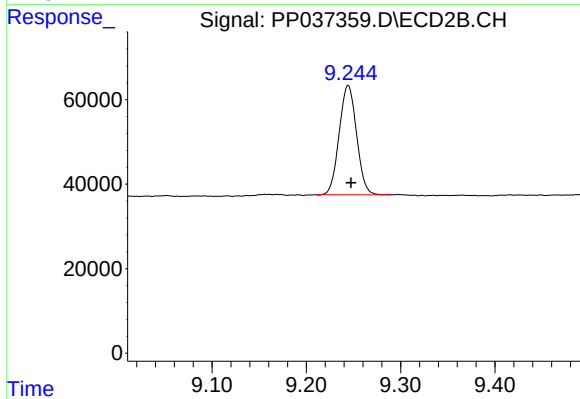

#2 Decachlorobiphenyl

R.T.: 9.244 min
Delta R.T.: -0.003 min
Response: 332138
Conc: 11.93 ng/ml