

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071921\
 Data File : PP037398.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2021 00:24
 Operator : DD\AJ
 Sample : M3067-01 5X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RW-3

Manual Integrations
 APPROVED

mohammad
 7/20/2021 11:44:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 06:12:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.957	3.947	65839	62048	1.449m	2.267 #
2) SA Decachlor...	10.992	9.241	60321	49027	1.310	1.761 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071921\
Data File : PP037398.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2021 00:24
Operator : DD\AJ
Sample : M3067-01 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RW-3


Manual Integrations
APPROVED

mohammad
7/20/2021 11:44:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 06:12:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

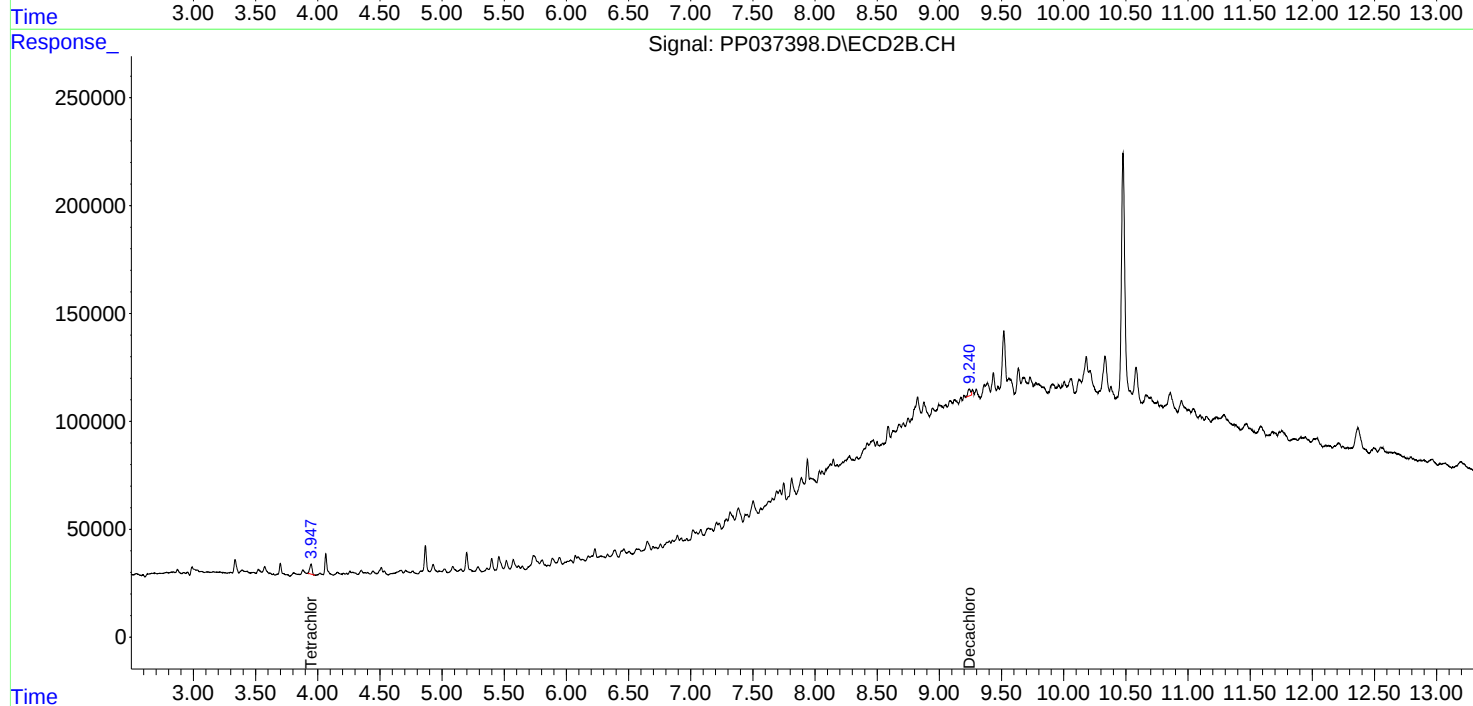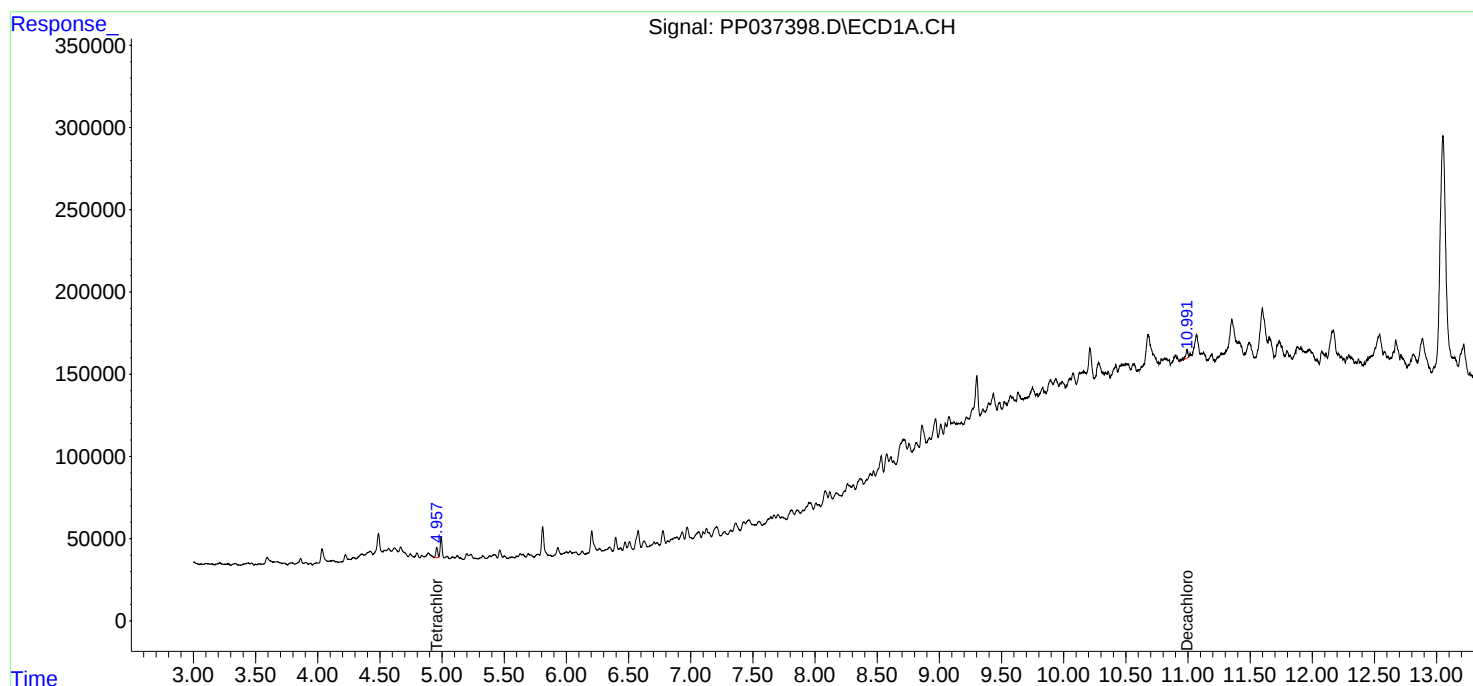

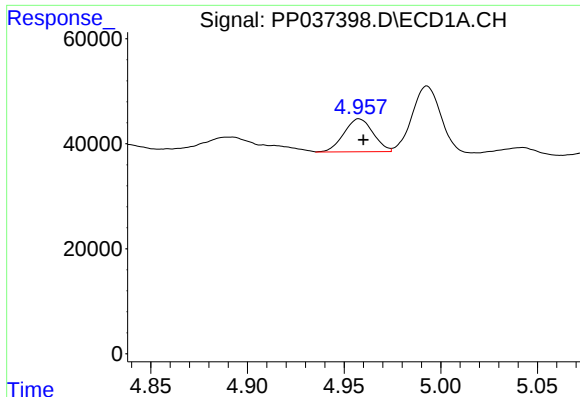


#1 Tetrachloro-m-xylene

R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 65839
Conc: 1.45 ng/ml m

Instrument :
ECD_P
ClientSampleId :
RW-3


Manual Integrations
APPROVED

mohammad
7/20/2021 11:44:54 AM

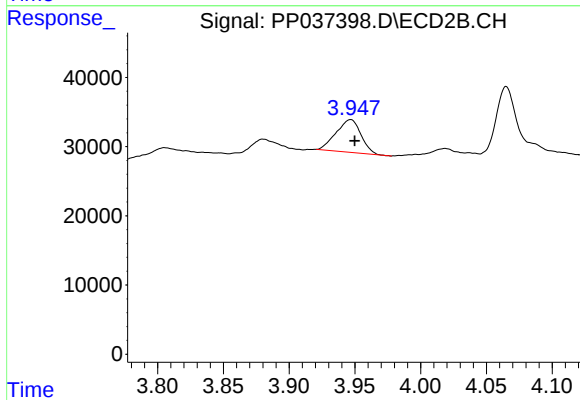


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.003 min
Response: 62048
Conc: 2.27 ng/ml

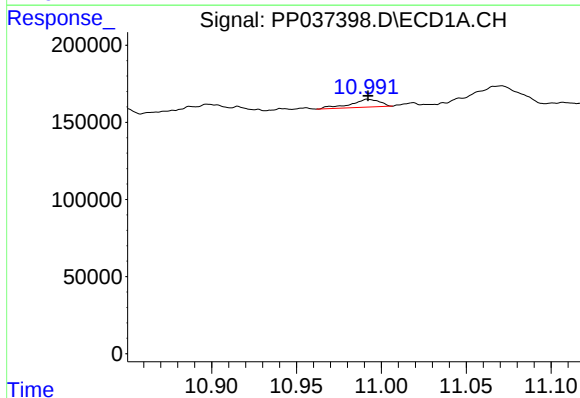

#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: 0.000 min
Response: 60321
Conc: 1.31 ng/ml

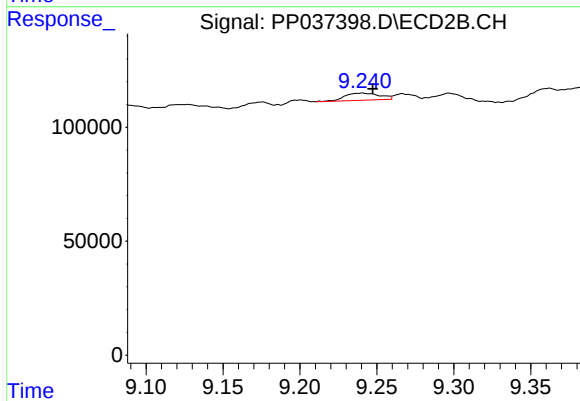

#2 Decachlorobiphenyl

R.T.: 9.241 min
Delta R.T.: -0.007 min
Response: 49027
Conc: 1.76 ng/ml