

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071922\
 Data File : PP049593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2022 13:52
 Operator : YP\AJ
 Sample : N3761-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-40049

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
 Supervised By :mohammad ahmed 07/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 16:27:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.600	34362016	58887789	23.679	24.092
2) SA Decachlor...	10.104	8.569	34194712	27989766	24.176	24.034
Target Compounds						
26) L6 AR-1254-1	6.384	5.469	17214821	31672400	273.333m	249.722
27) L6 AR-1254-2	6.604	5.616	28835014	28016168	295.979m	253.469
28) L6 AR-1254-3	6.974	6.019	25932528	35931598	250.985	220.745
29) L6 AR-1254-4	7.261	6.246	13873239	14465113	173.298	149.499
30) L6 AR-1254-5	7.681	6.661	10130397	13869370	113.976m	104.662

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071922\
Data File : PP049593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2022 13:52
Operator : YP\AJ
Sample : N3761-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-40049


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 16:27:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

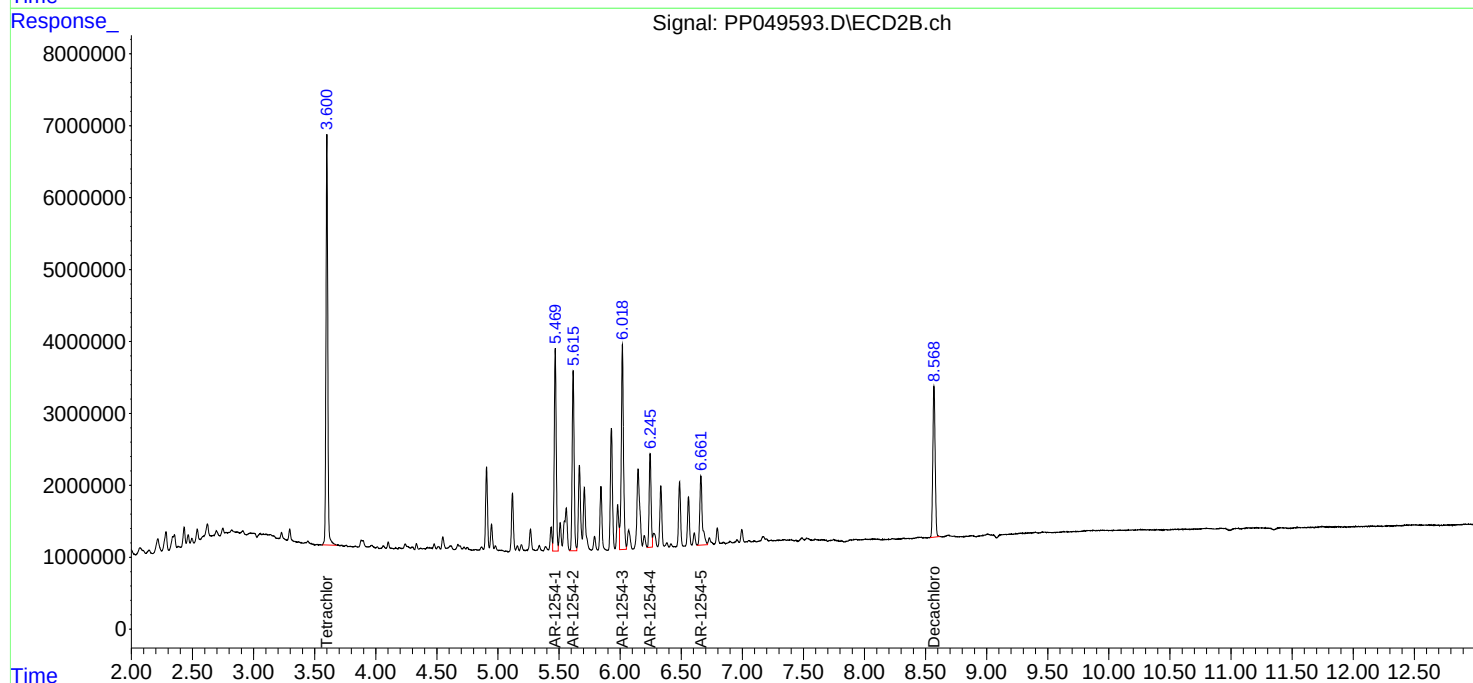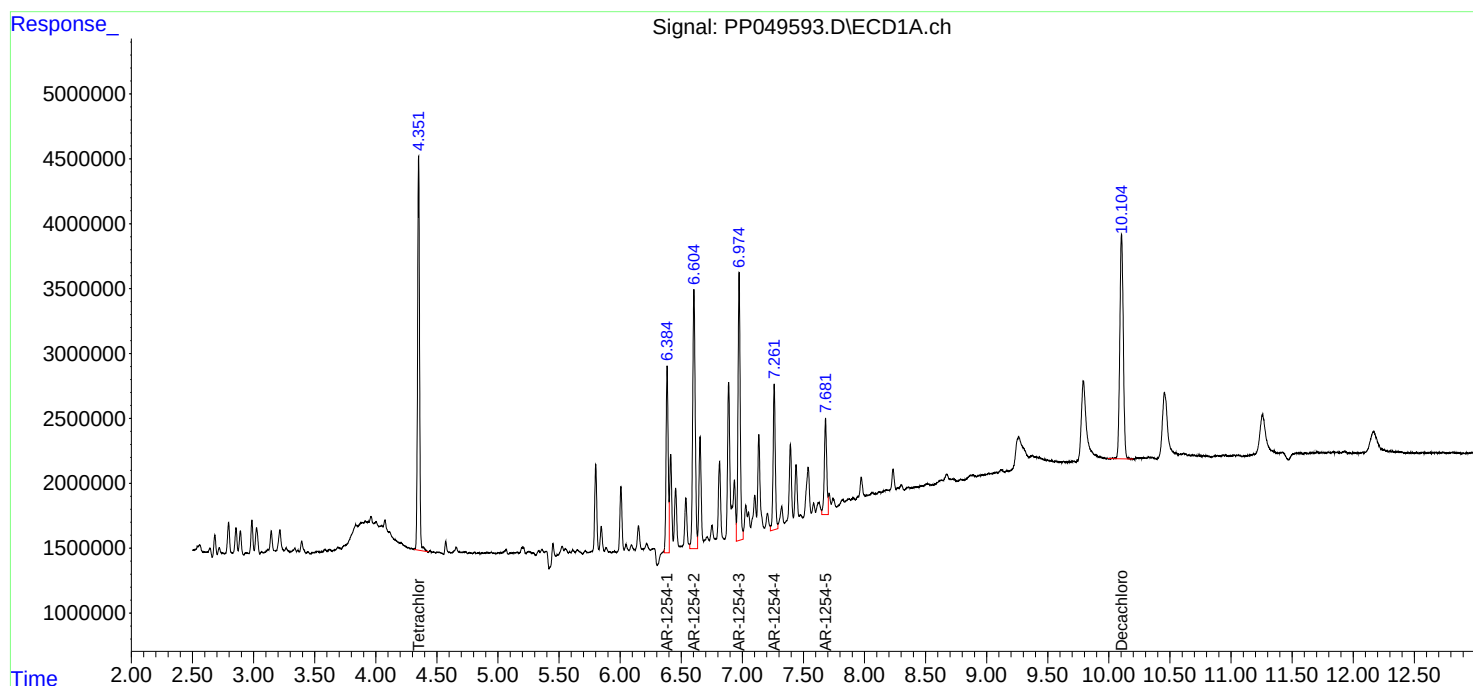

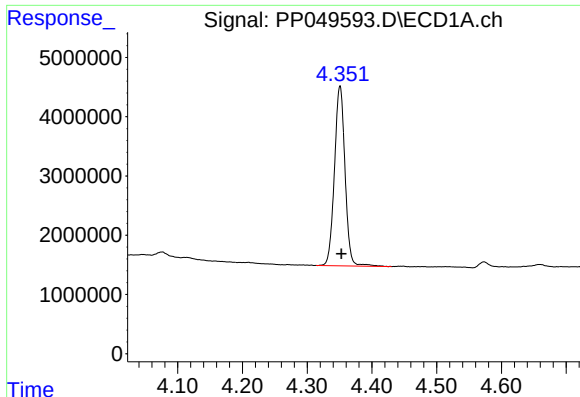


#1 Tetrachloro-m-xylene

R.T.: 4.351 min
Delta R.T.: -0.002 min
Response: 34362016
Conc: 23.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40049


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

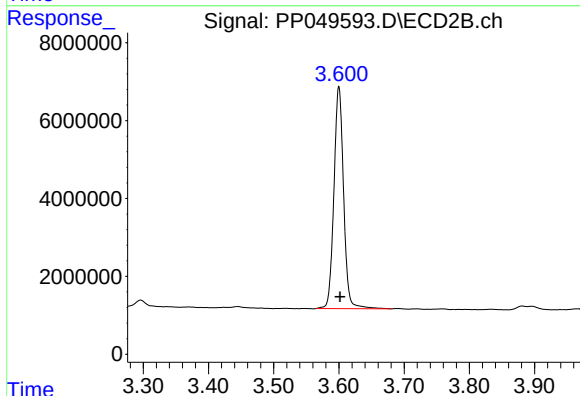


#1 Tetrachloro-m-xylene

R.T.: 3.600 min
Delta R.T.: -0.002 min
Response: 58887789
Conc: 24.09 ng/ml

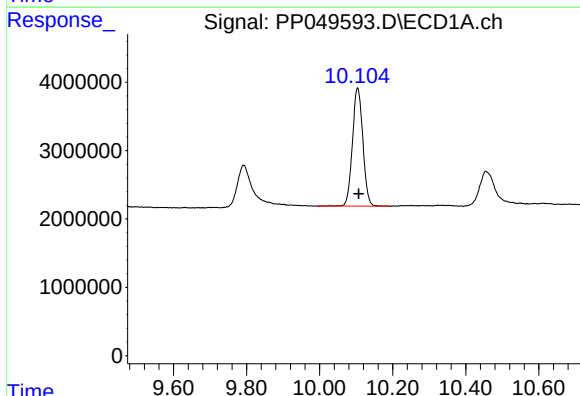


#2 Decachlorobiphenyl

R.T.: 10.104 min
Delta R.T.: -0.003 min
Response: 34194712
Conc: 24.18 ng/ml

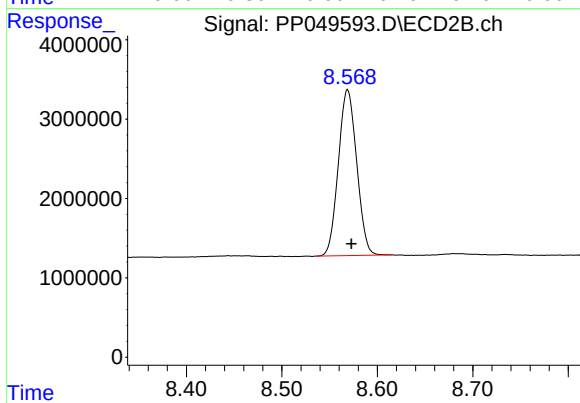

#2 Decachlorobiphenyl

R.T.: 8.569 min
Delta R.T.: -0.004 min
Response: 27989766
Conc: 24.03 ng/ml

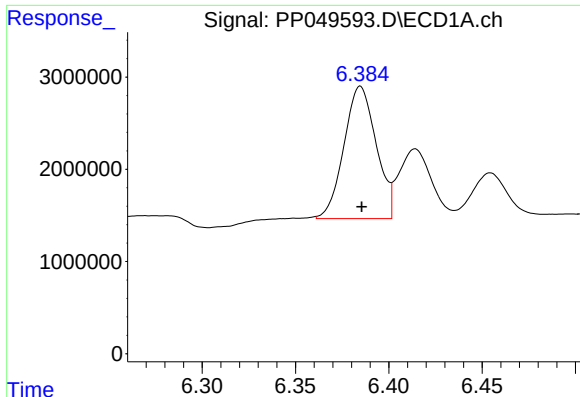


#26 AR-1254-1

R.T.: 6.384 min
Delta R.T.: -0.001 min
Response: 17214821
Conc: 273.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40049


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

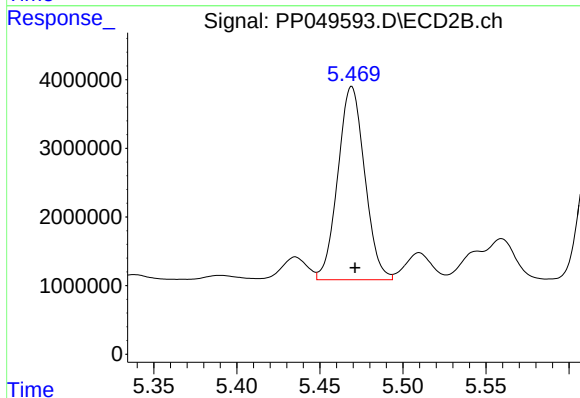


#26 AR-1254-1

R.T.: 5.469 min
Delta R.T.: -0.002 min
Response: 31672400
Conc: 249.72 ng/ml

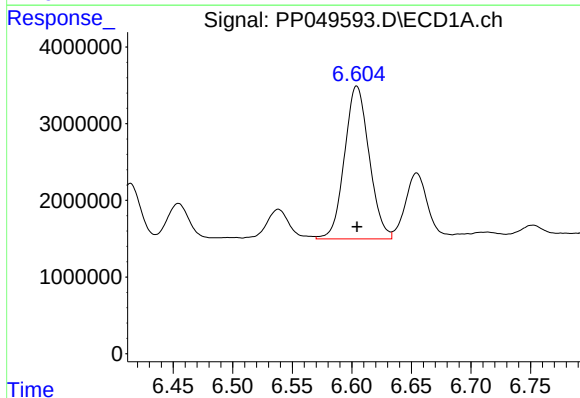


#27 AR-1254-2

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 28835014
Conc: 295.98 ng/ml m

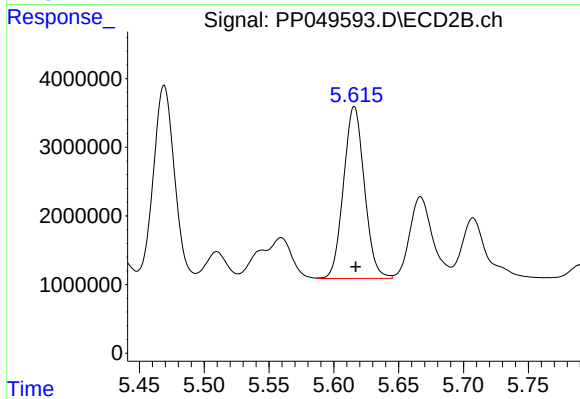

#27 AR-1254-2

R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 28016168
Conc: 253.47 ng/ml

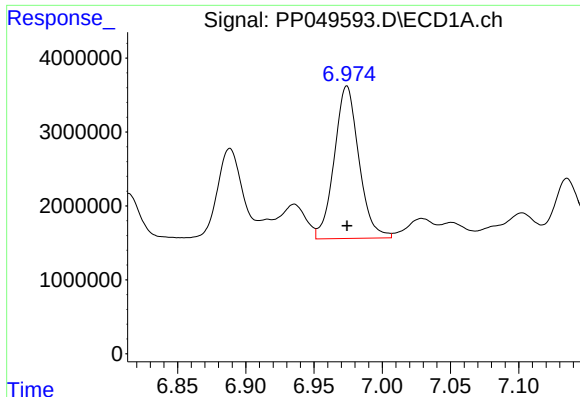


#28 AR-1254-3

R.T.: 6.974 min
Delta R.T.: 0.000 min
Response: 25932528
Conc: 250.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40049


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

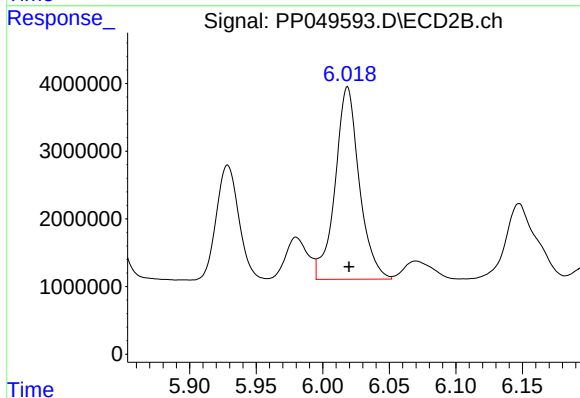


#28 AR-1254-3

R.T.: 6.019 min
Delta R.T.: -0.001 min
Response: 35931598
Conc: 220.74 ng/ml

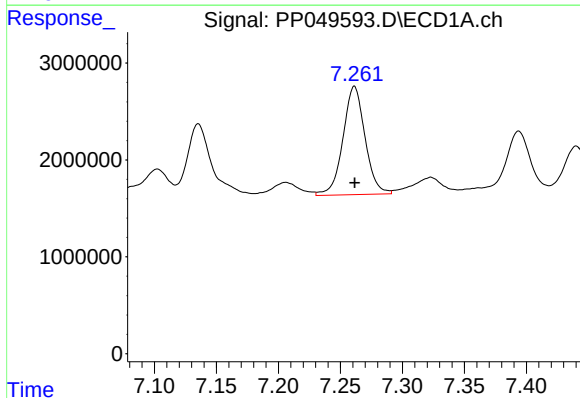


#29 AR-1254-4

R.T.: 7.261 min
Delta R.T.: 0.000 min
Response: 13873239
Conc: 173.30 ng/ml

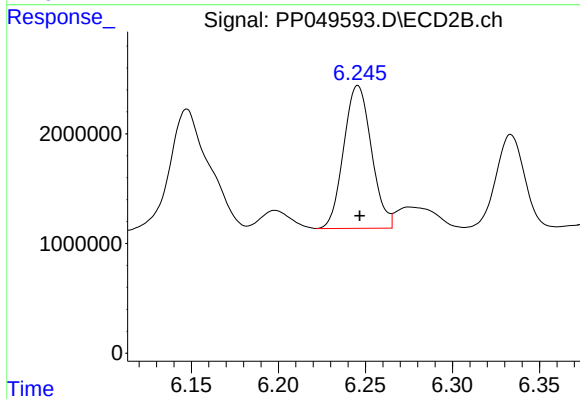

#29 AR-1254-4

R.T.: 6.246 min
Delta R.T.: -0.001 min
Response: 14465113
Conc: 149.50 ng/ml

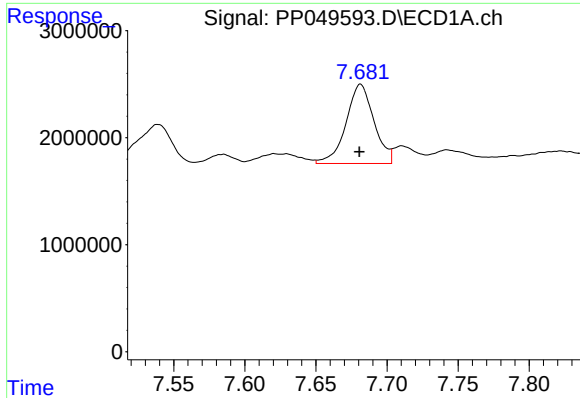


#30 AR-1254-5

R.T.: 7.681 min
Delta R.T.: 0.000 min
Response: 10130397
Conc: 113.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40049

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

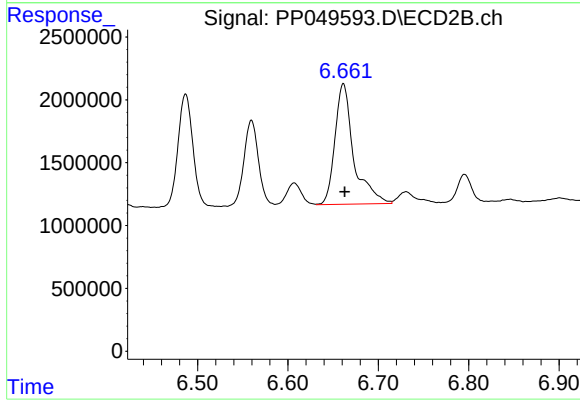

#30 AR-1254-5

R.T.: 6.661 min
Delta R.T.: -0.002 min
Response: 13869370
Conc: 104.66 ng/ml