

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071922\
 Data File : PP049595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2022 14:25
 Operator : YP\AJ
 Sample : N3761-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-40051

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
 Supervised By :mohammad ahmed 07/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 16:28:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.601	29427718	48458652	20.279	19.825
2) SA Decachlor...	10.108	8.571	32689524	24050117	23.112	20.651
Target Compounds						
26) L6 AR-1254-1	6.387	5.469	912672	2489534	14.491m	19.629m#
27) L6 AR-1254-2	6.605	5.617	1670301	2093433	17.145	18.940
28) L6 AR-1254-3	6.976	6.020	1709648	3041184	16.547	18.683
29) L6 AR-1254-4	7.263	6.247	1672680	2424393	20.894	25.056
30) L6 AR-1254-5	7.682	6.663	2078783	3245611	23.388m	24.492

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071922\
Data File : PP049595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2022 14:25
Operator : YP\AJ
Sample : N3761-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-40051


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 16:28:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

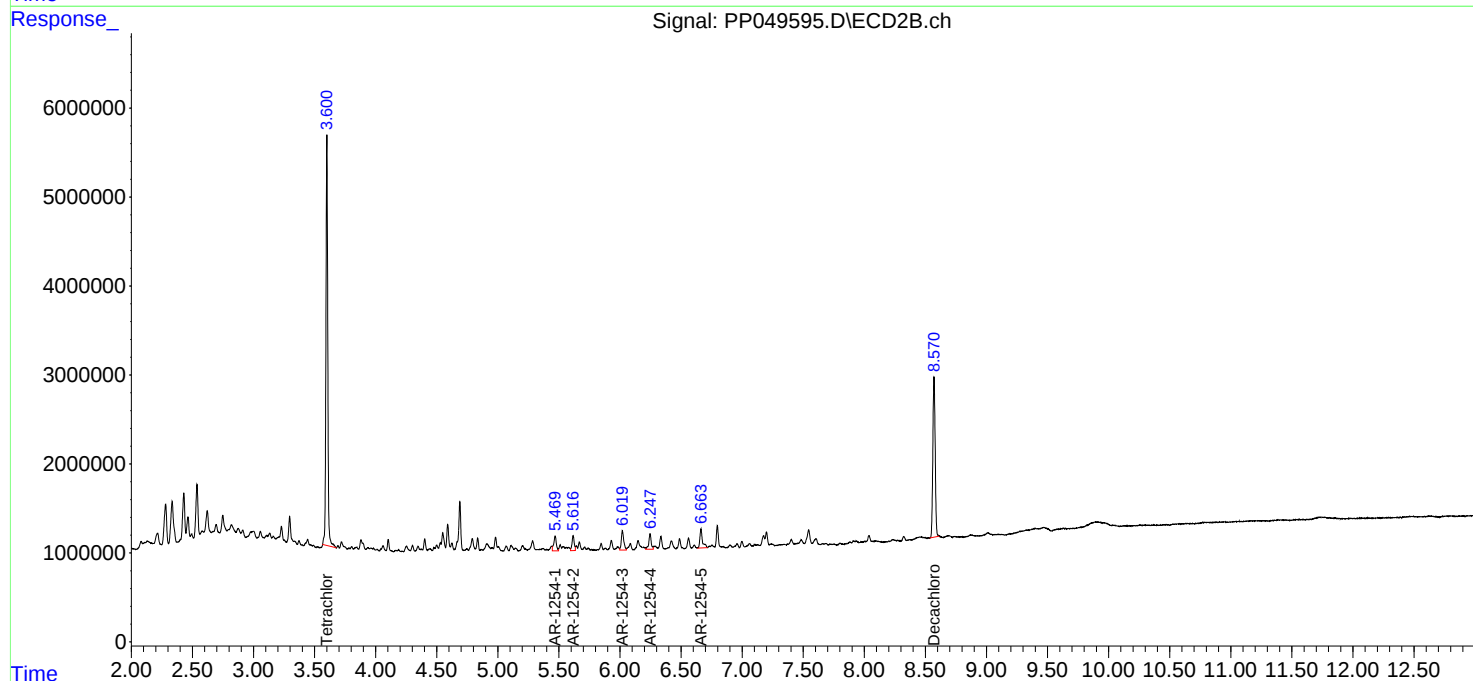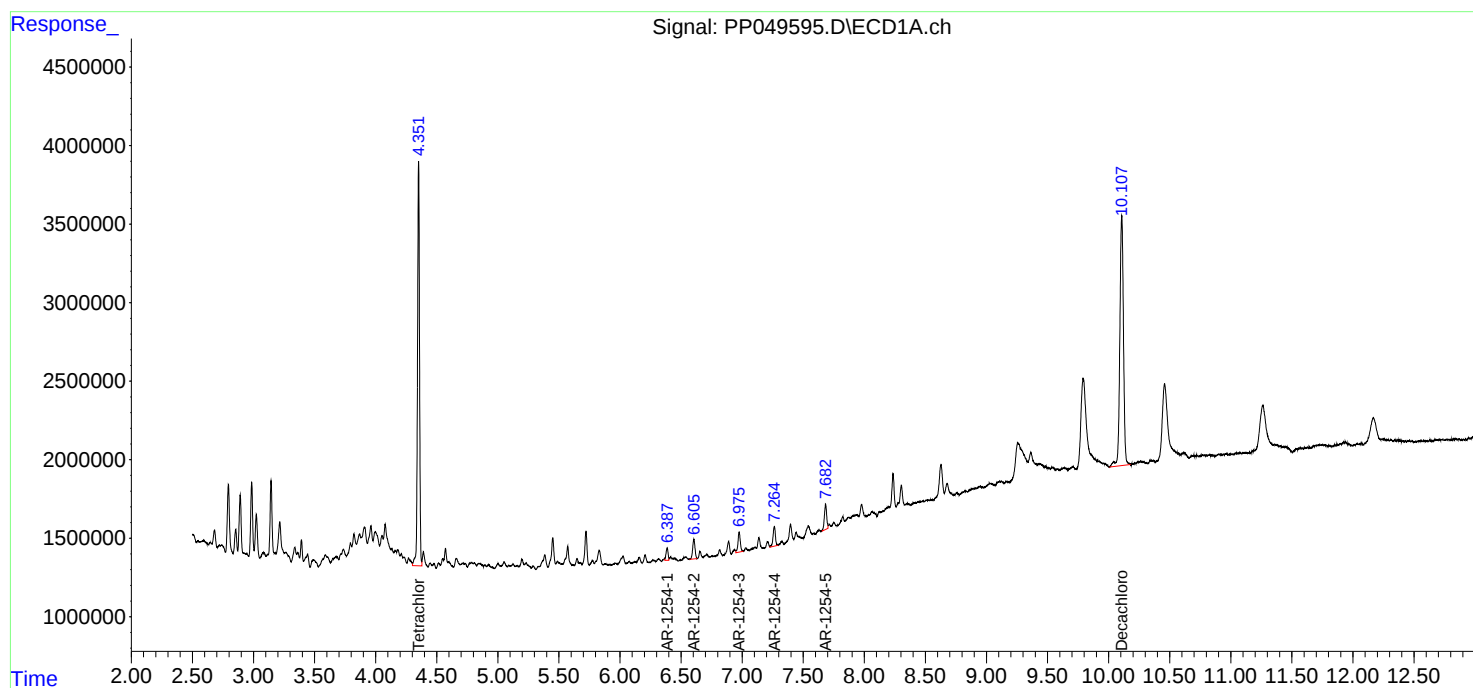

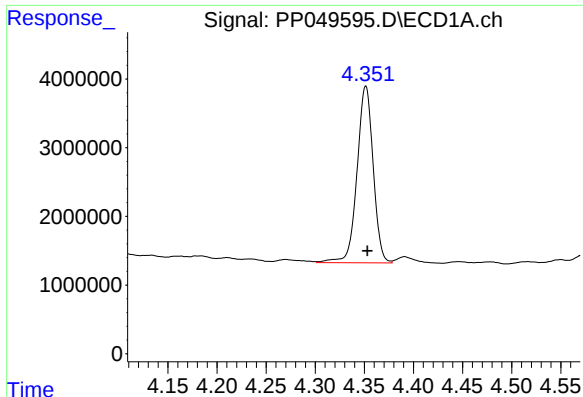


#1 Tetrachloro-m-xylene

R.T.: 4.351 min
Delta R.T.: -0.002 min
Response: 29427718
Conc: 20.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40051


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

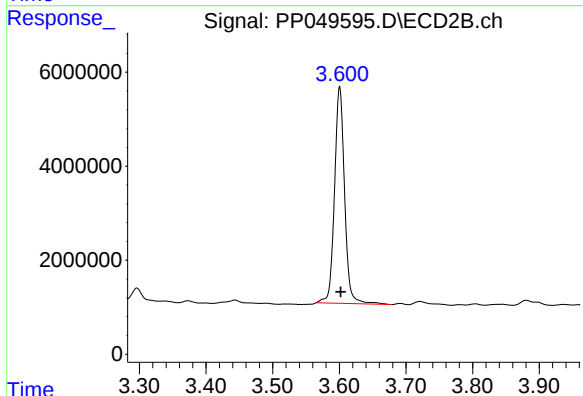


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.001 min
Response: 48458652
Conc: 19.82 ng/ml

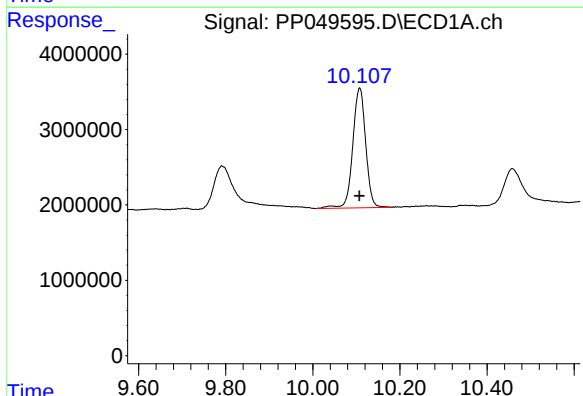


#2 Decachlorobiphenyl

R.T.: 10.108 min
Delta R.T.: 0.000 min
Response: 32689524
Conc: 23.11 ng/ml

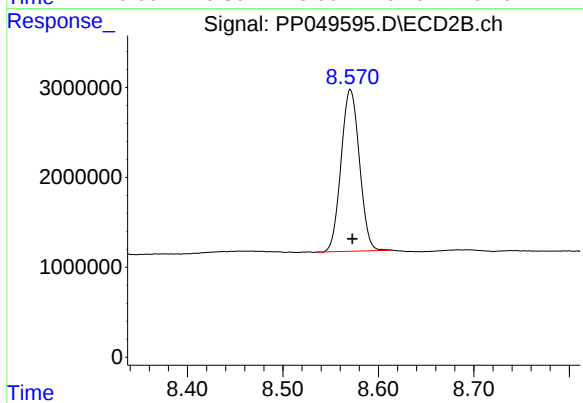

#2 Decachlorobiphenyl

R.T.: 8.571 min
Delta R.T.: -0.002 min
Response: 24050117
Conc: 20.65 ng/ml

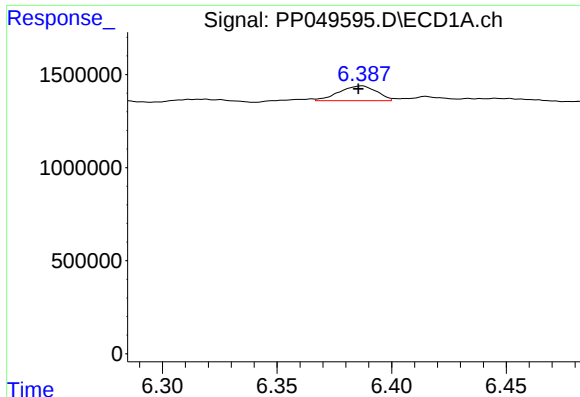


#26 AR-1254-1

R.T.: 6.387 min
Delta R.T.: 0.001 min
Response: 912672
Conc: 14.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40051


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

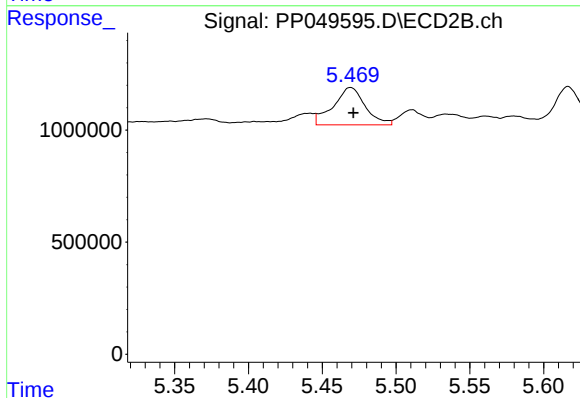


#26 AR-1254-1

R.T.: 5.469 min
Delta R.T.: -0.002 min
Response: 2489534
Conc: 19.63 ng/ml m

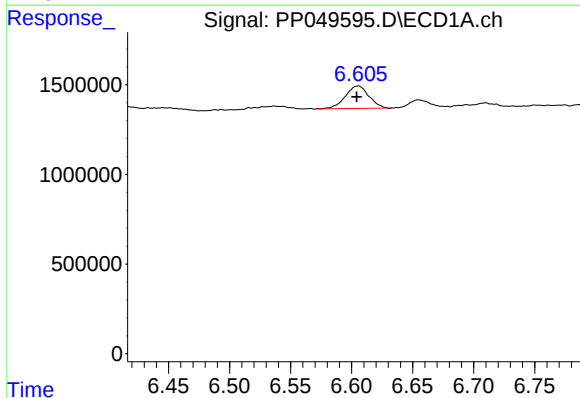


#27 AR-1254-2

R.T.: 6.605 min
Delta R.T.: 0.000 min
Response: 1670301
Conc: 17.14 ng/ml

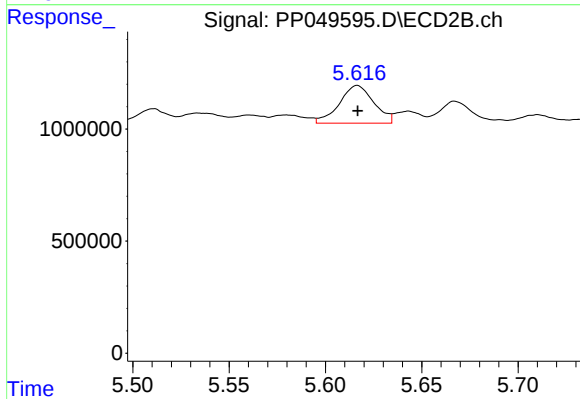

#27 AR-1254-2

R.T.: 5.617 min
Delta R.T.: 0.000 min
Response: 2093433
Conc: 18.94 ng/ml

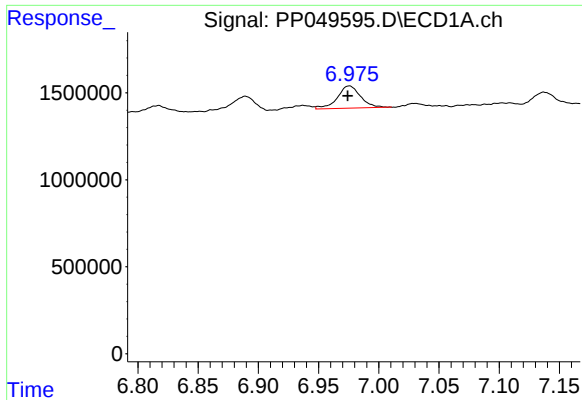


#28 AR-1254-3

R.T.: 6.976 min
Delta R.T.: 0.001 min
Response: 1709648
Conc: 16.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40051


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

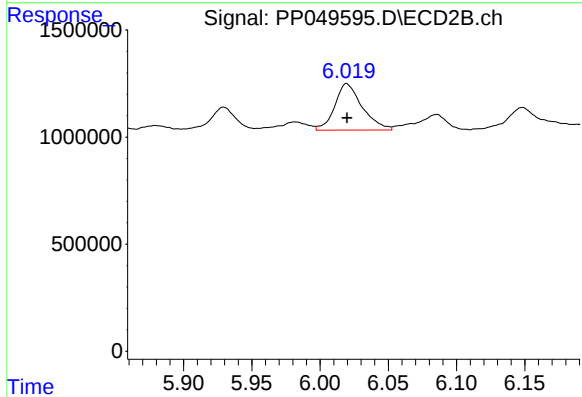


#28 AR-1254-3

R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 3041184
Conc: 18.68 ng/ml

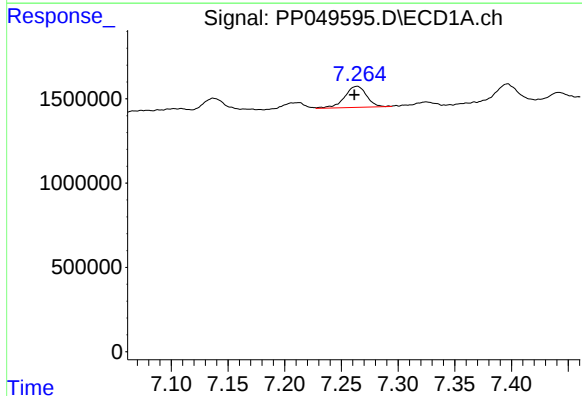


#29 AR-1254-4

R.T.: 7.263 min
Delta R.T.: 0.002 min
Response: 1672680
Conc: 20.89 ng/ml

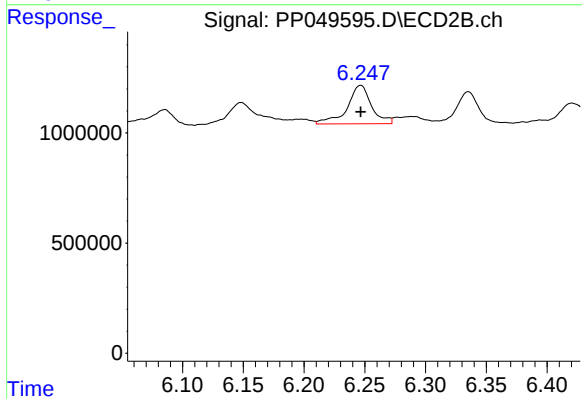

#29 AR-1254-4

R.T.: 6.247 min
Delta R.T.: 0.000 min
Response: 2424393
Conc: 25.06 ng/ml

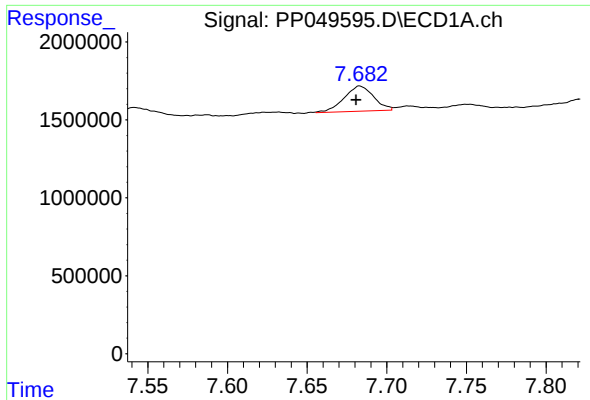


#30 AR-1254-5

R.T.: 7.682 min
Delta R.T.: 0.002 min
Response: 2078783
Conc: 23.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40051

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 07/20/2022
Supervised By :mohammad ahmed 07/20/2022

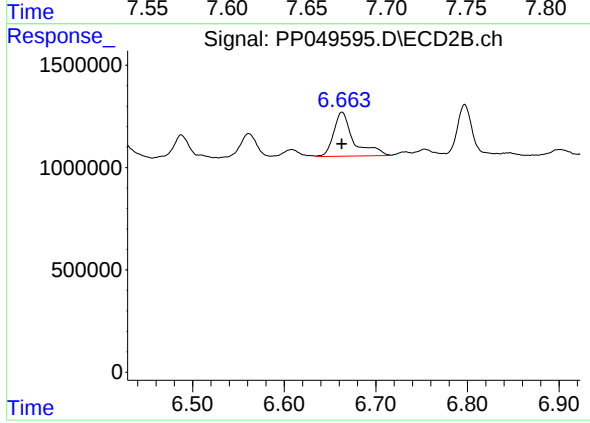

#30 AR-1254-5

R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 3245611
Conc: 24.49 ng/ml