

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071924\
 Data File : PP066444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2024 18:09
 Operator : YP\AJ
 Sample : P3306-01 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 52-E

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2024
 Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 00:58:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 07:20:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.019	1443953	4321804	0.820	2.263m#
2) SA Decachlor...	10.799	9.211	3917334	1553227	2.232m	1.217m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071924\
Data File : PP066444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2024 18:09
Operator : YP\AJ
Sample : P3306-01 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
52-E


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 00:58:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 07:20:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

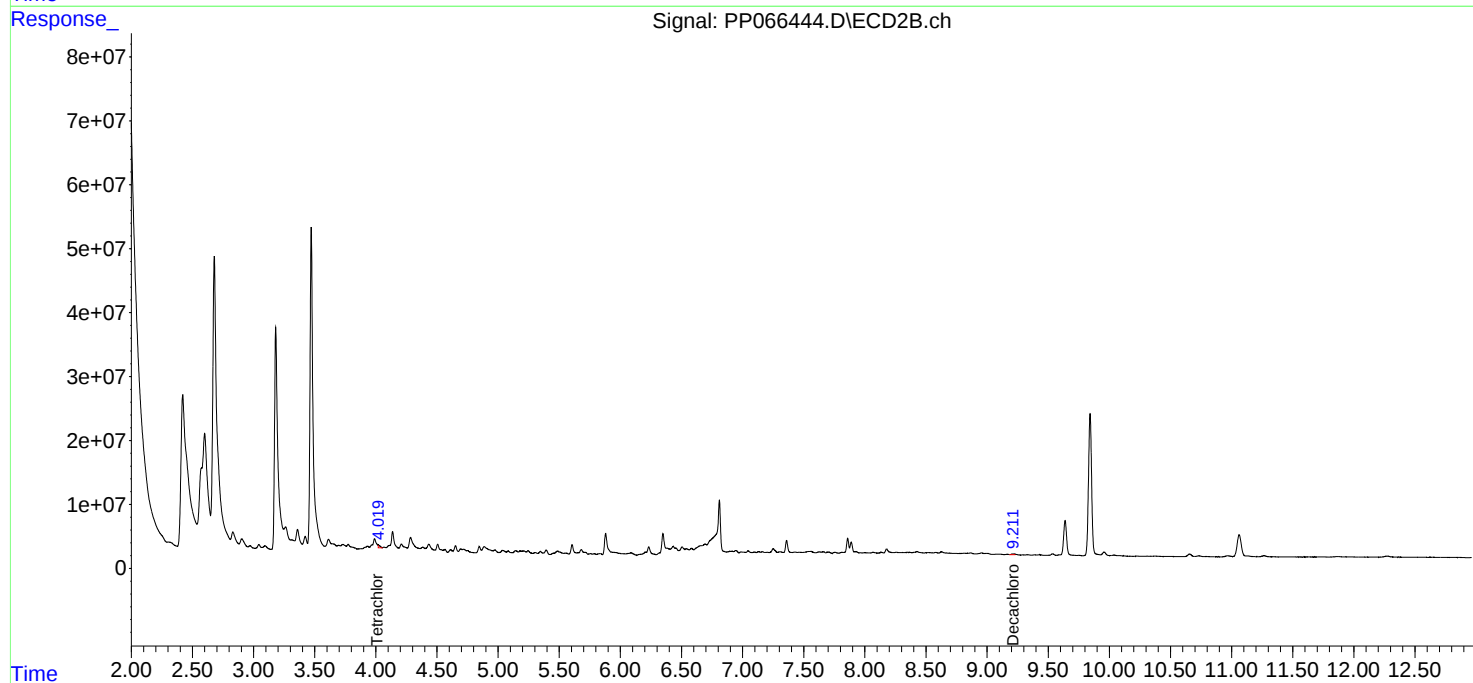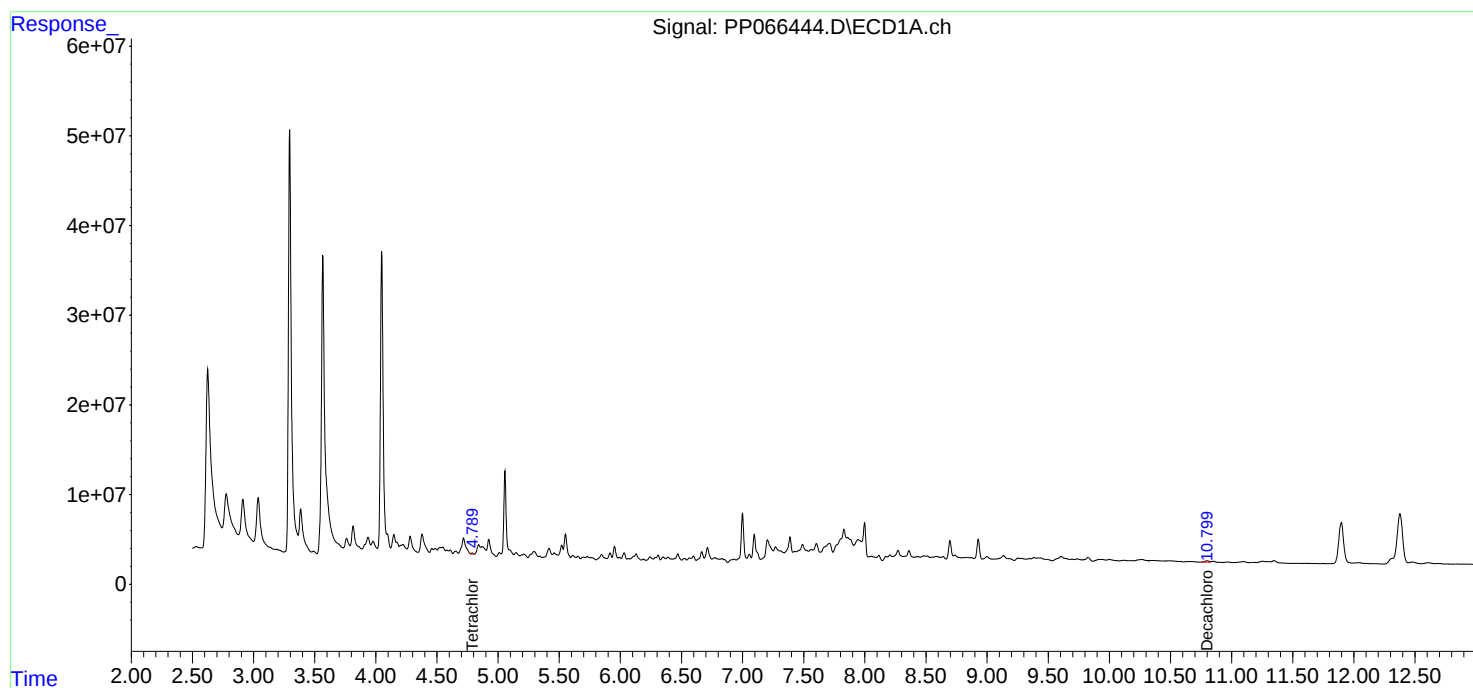

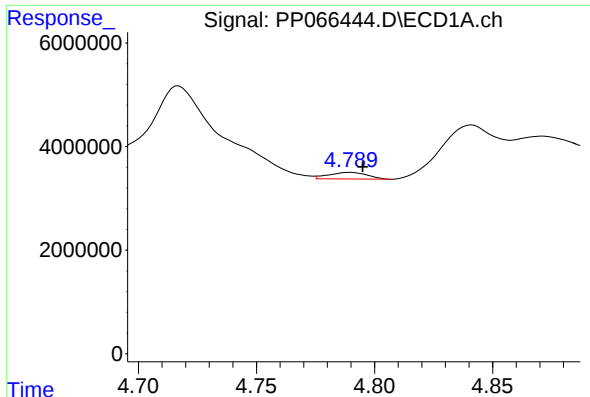


#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: -0.005 min
Response: 1443953
Conc: 0.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
52-E


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

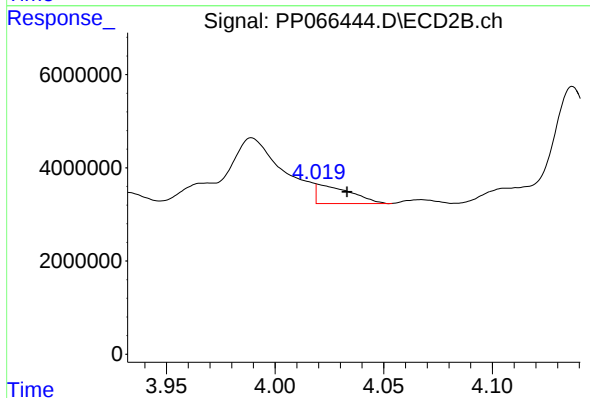


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.014 min
Response: 4321804
Conc: 2.26 ng/ml m

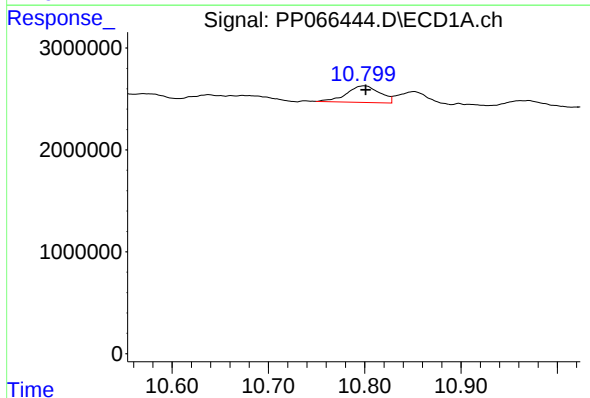

#2 Decachlorobiphenyl

R.T.: 10.799 min
Delta R.T.: -0.002 min
Response: 3917334
Conc: 2.23 ng/ml m

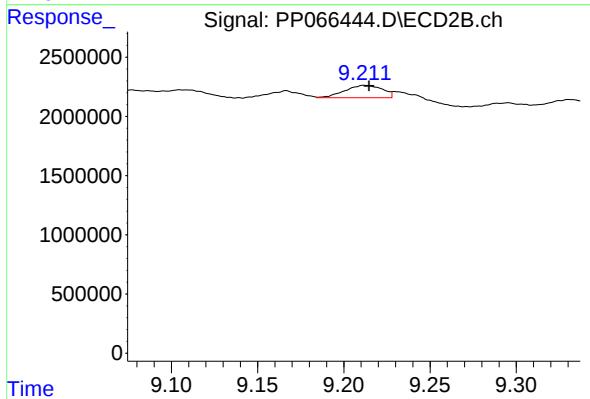

#2 Decachlorobiphenyl

R.T.: 9.211 min
Delta R.T.: -0.004 min
Response: 1553227
Conc: 1.22 ng/ml m