

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071924\
 Data File : PP066446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2024 18:42
 Operator : YP\AJ
 Sample : P3306-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 617-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2024
 Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 01:03:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 07:20:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.798	4.041	28526964	32665843	16.192	17.106
2) SA Decachlor...	10.831f	9.238	27958403	15146783	15.929m	11.871m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071924\
Data File : PP066446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2024 18:42
Operator : YP\AJ
Sample : P3306-04
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
617-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 01:03:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 07:20:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

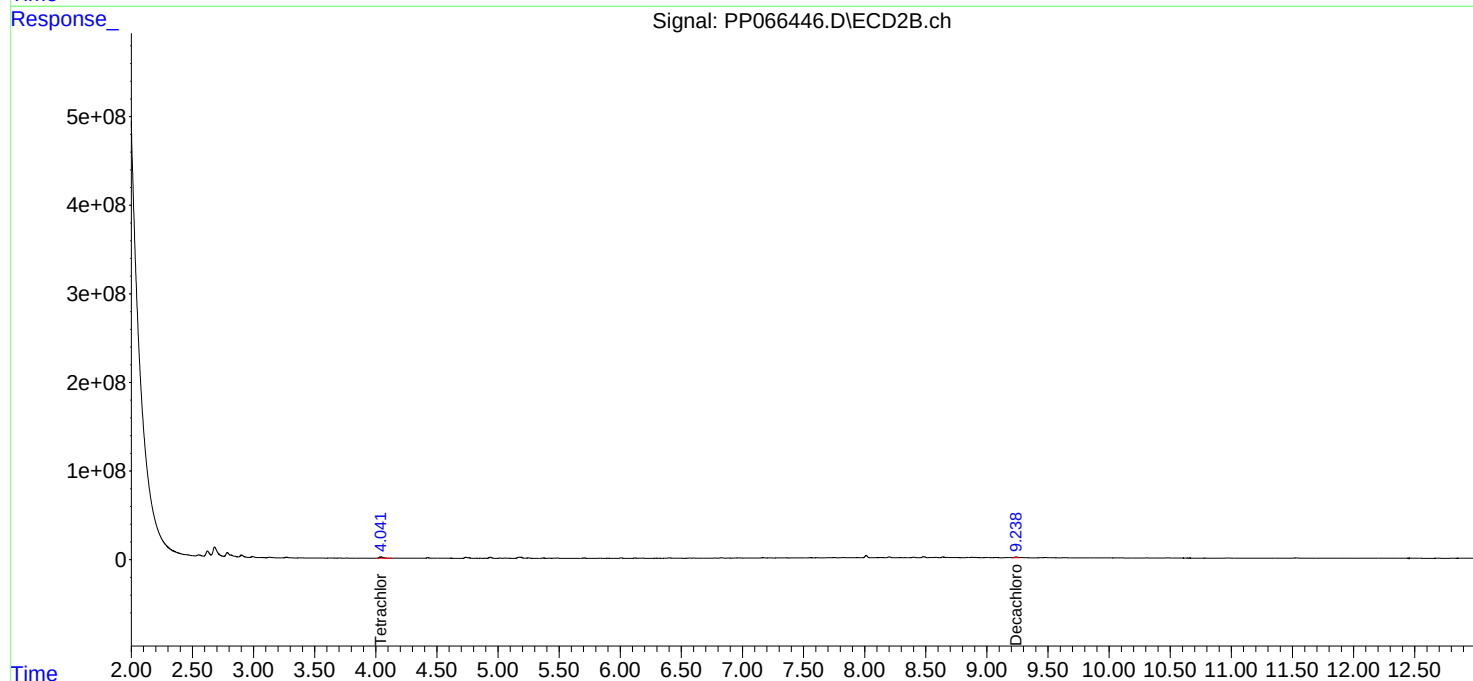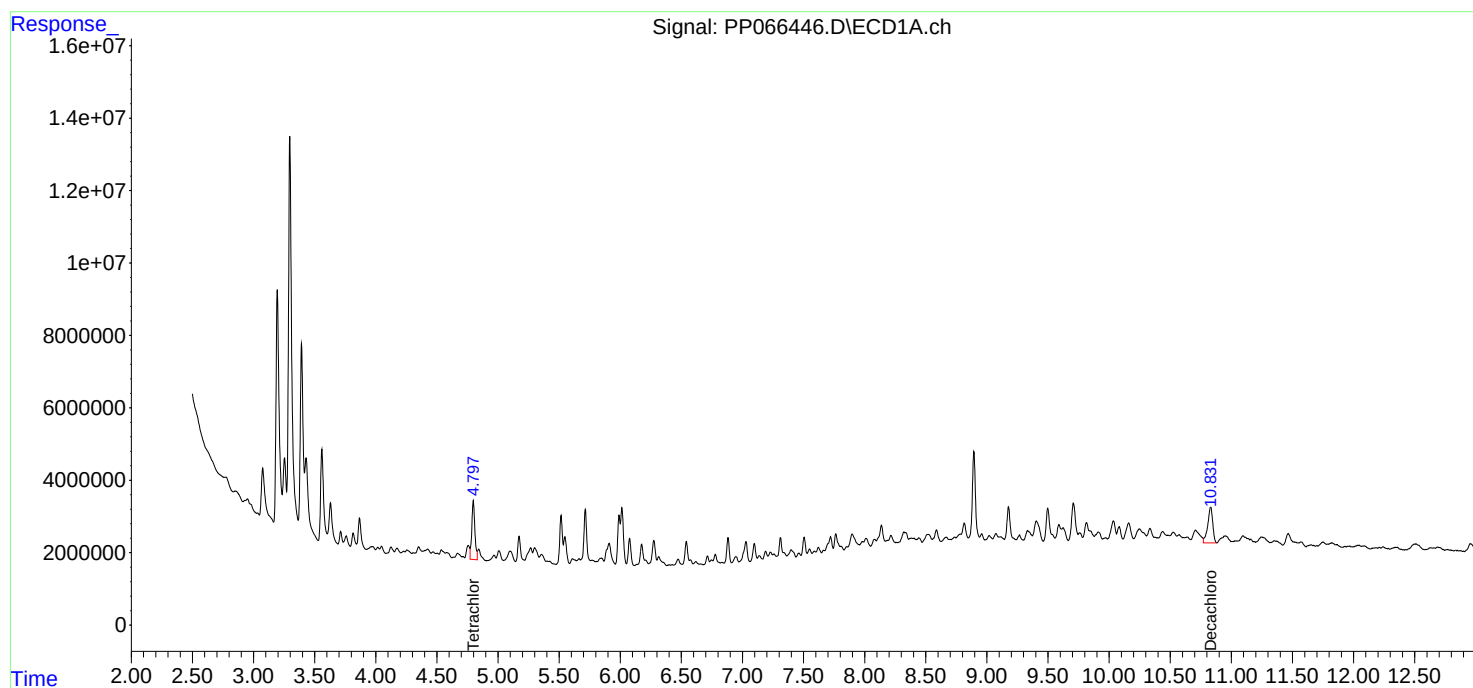

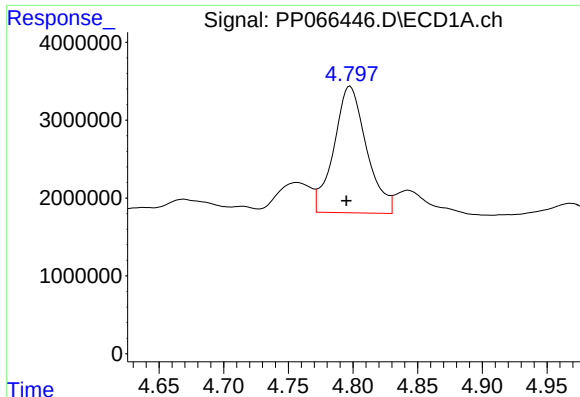


#1 Tetrachloro-m-xylene

R.T.: 4.798 min
Delta R.T.: 0.003 min
Response: 28526964
Conc: 16.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
617-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

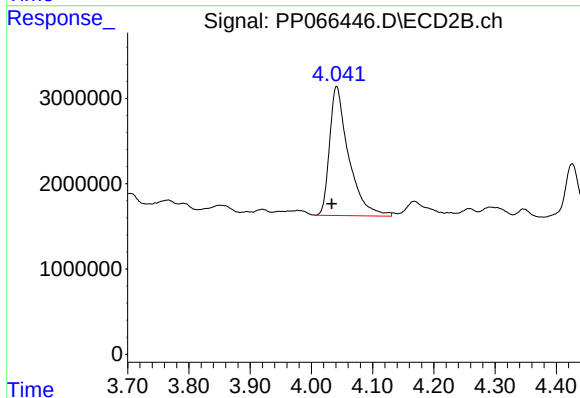


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: 0.008 min
Response: 32665843
Conc: 17.11 ng/ml

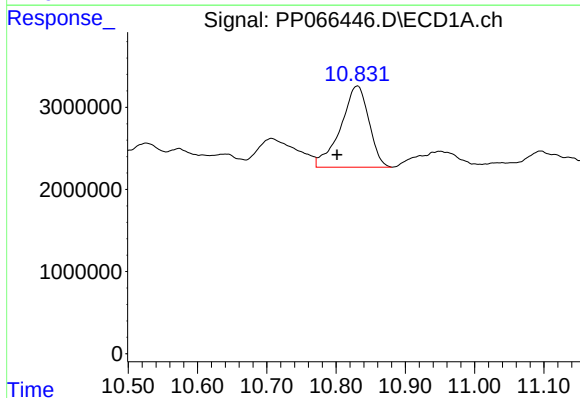

#2 Decachlorobiphenyl

R.T.: 10.831 min
Delta R.T.: 0.030 min
Response: 27958403
Conc: 15.93 ng/ml m

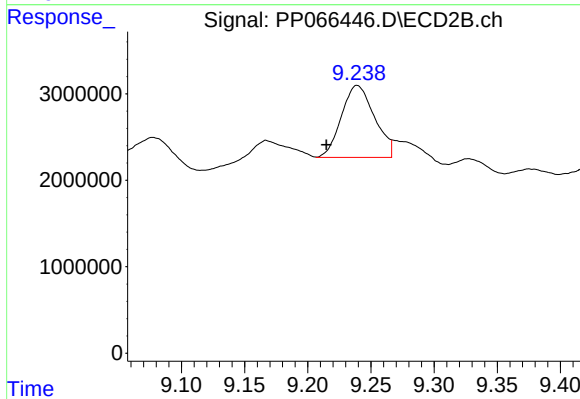

#2 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.024 min
Response: 15146783
Conc: 11.87 ng/ml m