

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072018\
 Data File : PP026806.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2018 9:37
 Operator : EI\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 14:14:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071318.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 13 23:16:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) T	DICHLORPROP	13.540	0.000	70550324	0	234.550	N.D.	#
------	-------------	--------	-------	----------	---	---------	------	---



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072018\
Data File : PP026806.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2018 9:37
Operator : EI\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 14:14:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071318.M
Quant Title : 8080.M
QLast Update : Fri Jul 13 23:16:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25 μ m

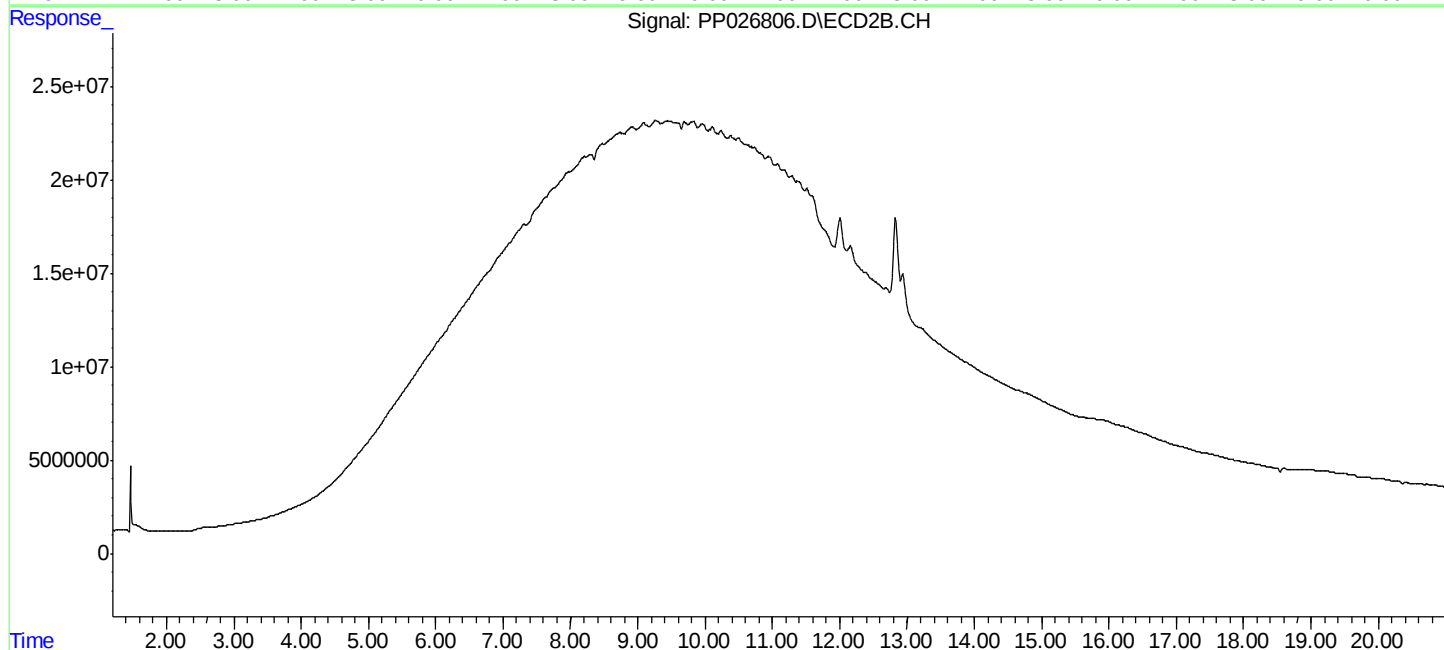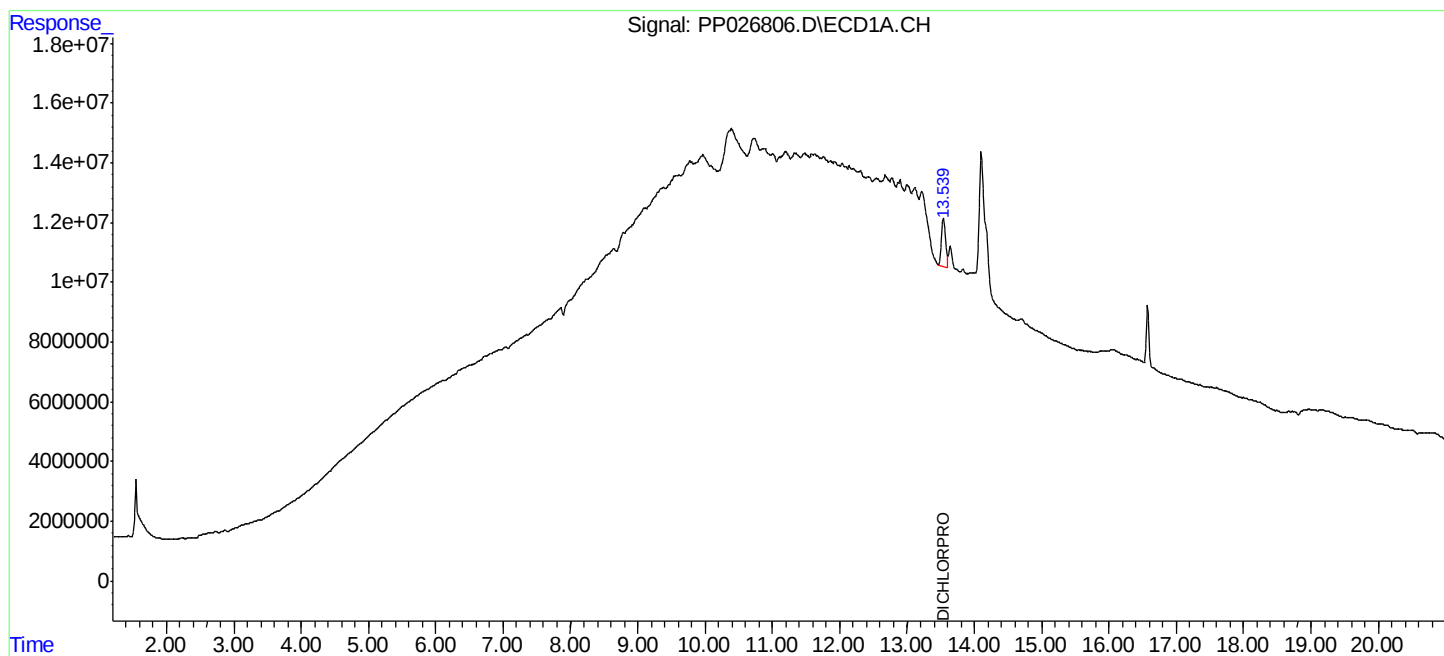


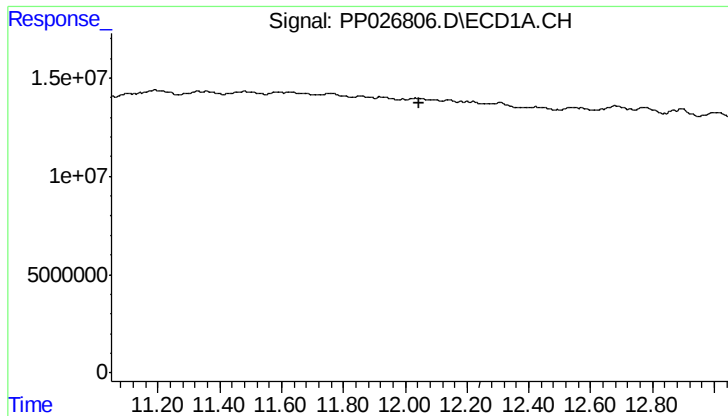

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 12.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

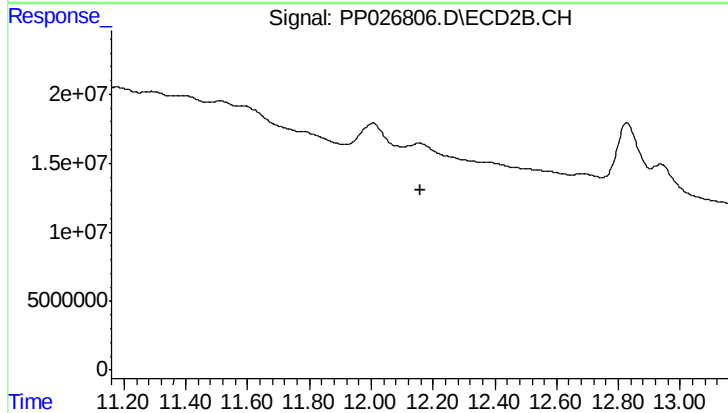


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 12.158 min
Response: 0
Conc: N.D.

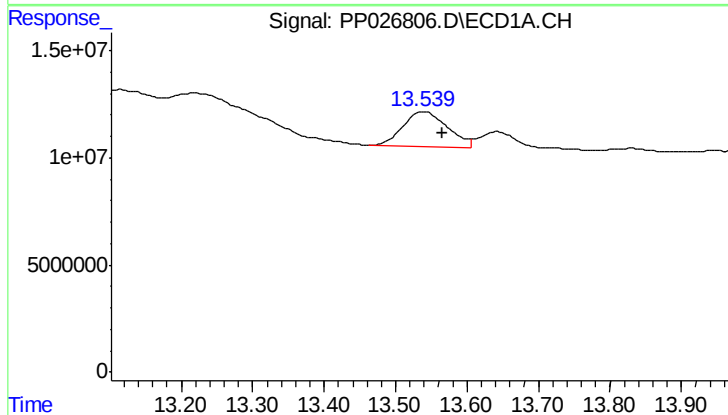

#8 DICHLORPROP

R.T.: 13.540 min
Delta R.T.: -0.025 min
Response: 70550324
Conc: 234.55 ng/ml

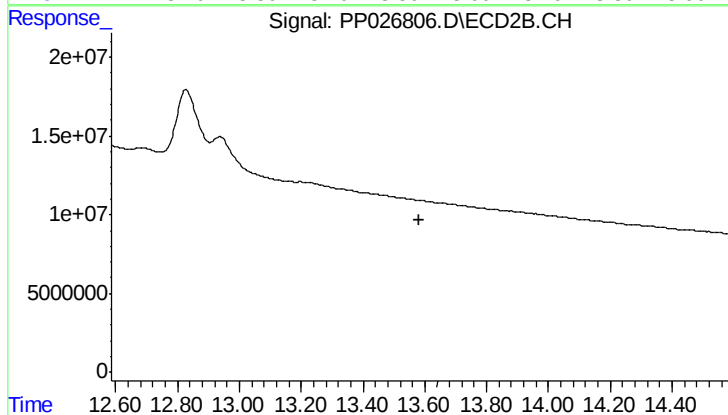

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 13.584 min
Response: 0
Conc: N.D.