

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072021\
 Data File : PP037432.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2021 16:09
 Operator : DD\AJ
 Sample : M3093-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20210528-COM-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 16:35:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.958	3.948	992405	581804	21.835	21.261
2) SA Decachlor...	10.989	9.241	775785	440544	16.852	15.827

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072021\
Data File : PP037432.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2021 16:09
Operator : DD\AJ
Sample : M3093-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20210528-COM-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 16:35:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

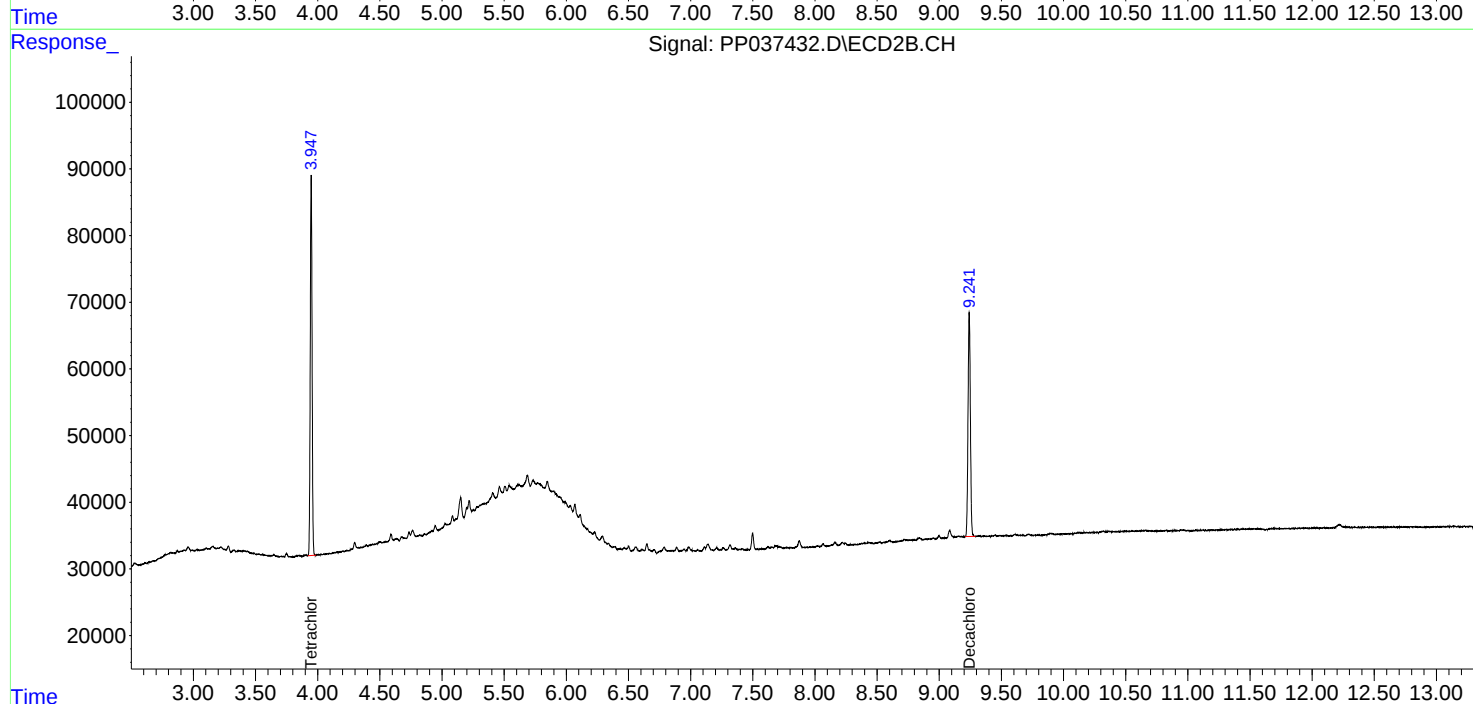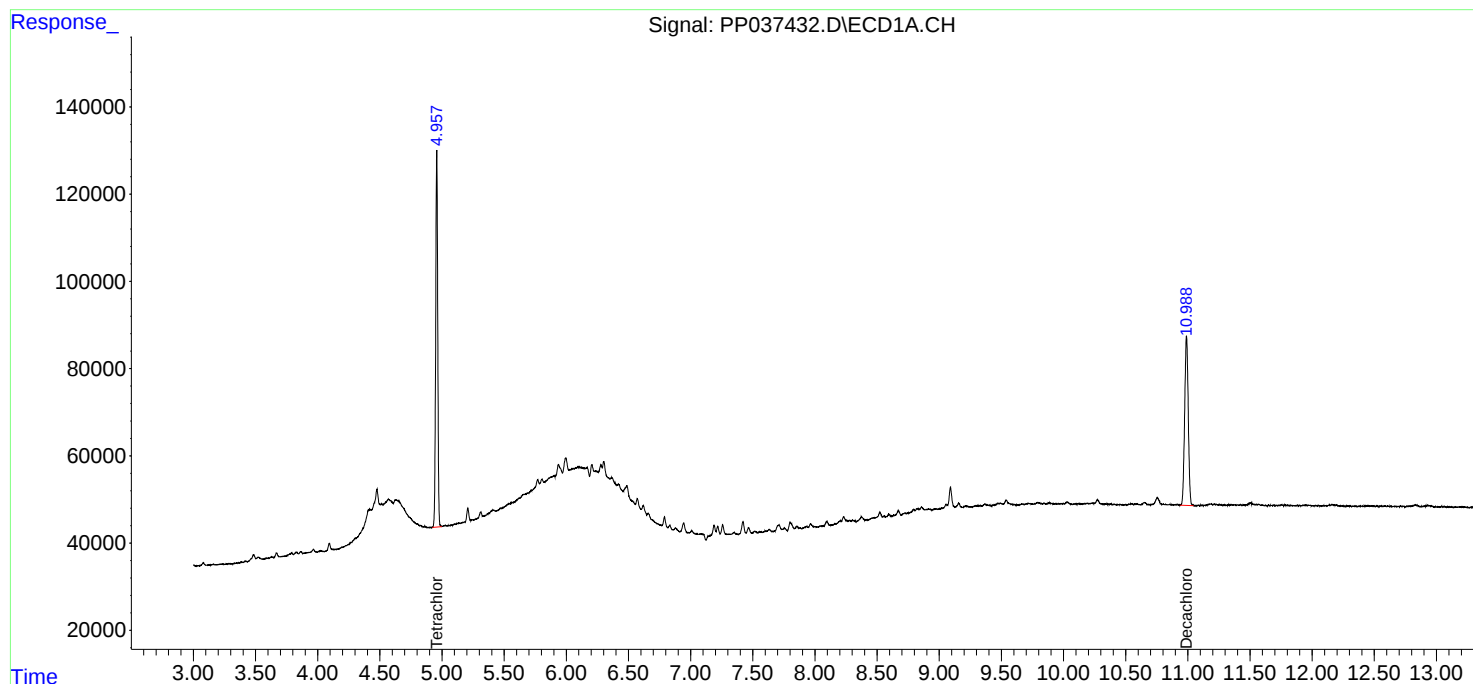


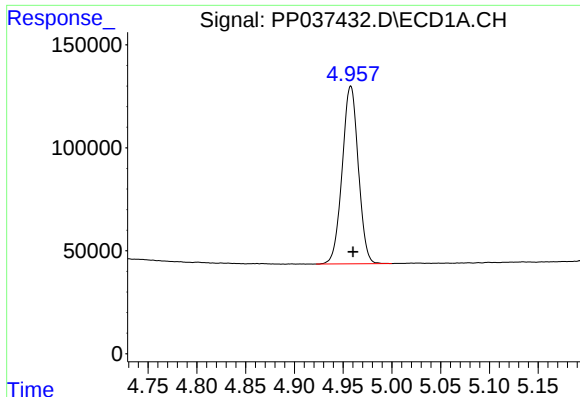

#1 Tetrachloro-m-xylene


R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 992405
Conc: 21.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
20210528-COM-1

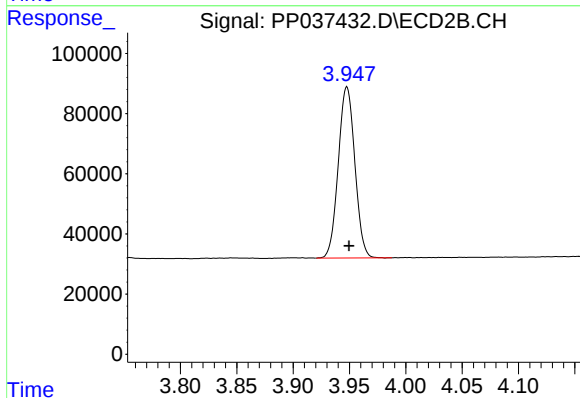


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 581804
Conc: 21.26 ng/ml

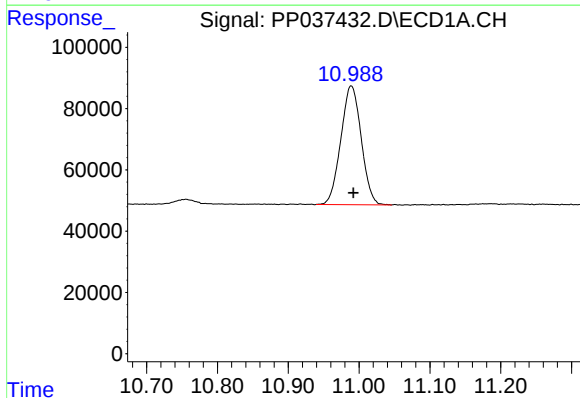

#2 Decachlorobiphenyl

R.T.: 10.989 min
Delta R.T.: -0.003 min
Response: 775785
Conc: 16.85 ng/ml

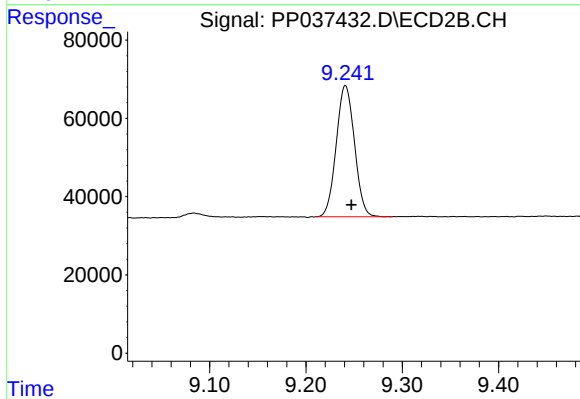

#2 Decachlorobiphenyl

R.T.: 9.241 min
Delta R.T.: -0.006 min
Response: 440544
Conc: 15.83 ng/ml