

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072121\
 Data File : PP037521.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2021 2:09
 Operator : DD\AJ
 Sample : M3076-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:43:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.957	3.947	960632	554984	21.136	20.281
2)	SA Decachlor...	10.986	9.238	791843	413732	17.201	14.864
Target Compounds							
8)	L2 AR-1221-1	5.207	0.000	99211	0	187.060	N.D. #
9)	L2 AR-1221-2	5.309	0.000	14523	0	35.847	N.D. #
20)	L4 AR-1242-5	7.280f	0.000	24386	0	23.449	N.D. #
24)	L5 AR-1248-4	7.194f	0.000	28235	0	14.938	N.D. #
25)	L5 AR-1248-5	7.280f	0.000	24386	0	13.029	N.D. #
26)	L6 AR-1254-1	7.194	0.000	28235	0	15.717	N.D. #
28)	L6 AR-1254-3	7.817f	0.000	10897	0	3.535	N.D. #
30)	L6 AR-1254-5	8.545f	0.000	15426	0	6.164	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072121\
Data File : PP037521.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2021 2:09
Operator : DD\AJ
Sample : M3076-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 02:43:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

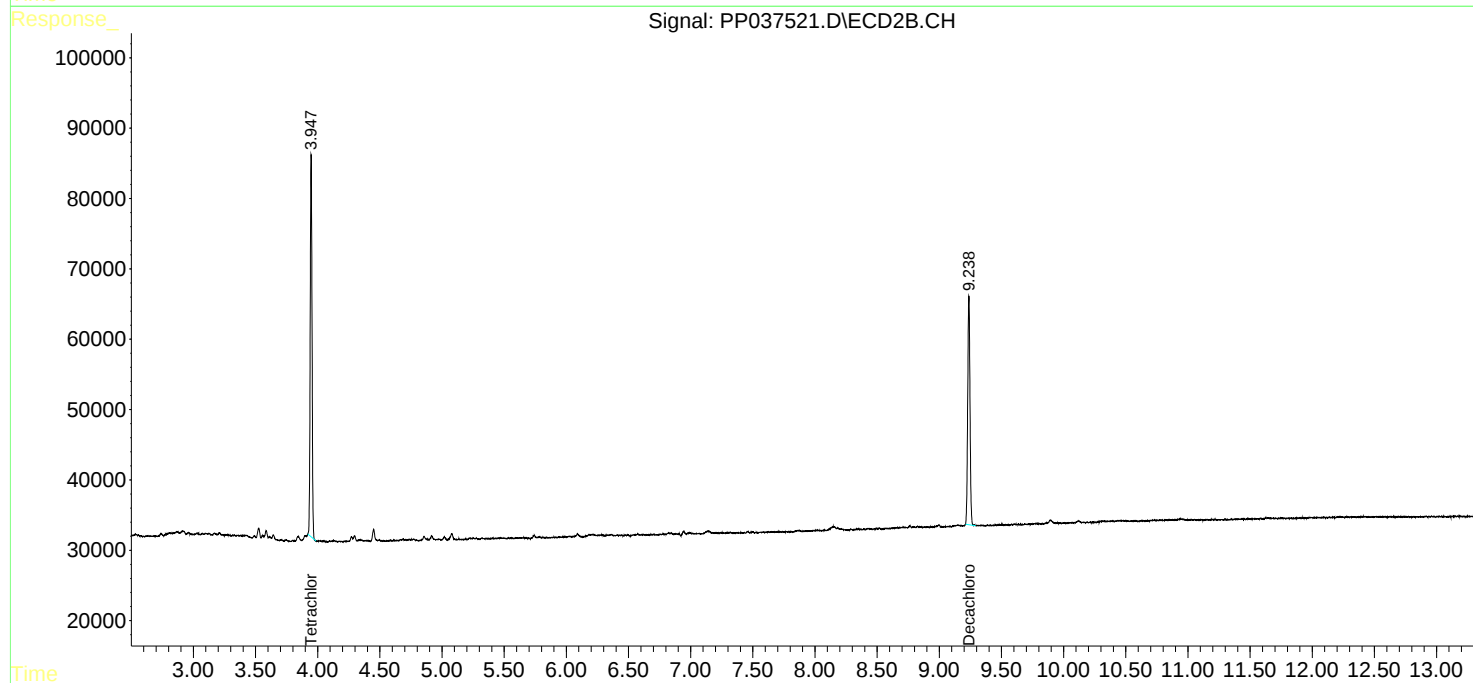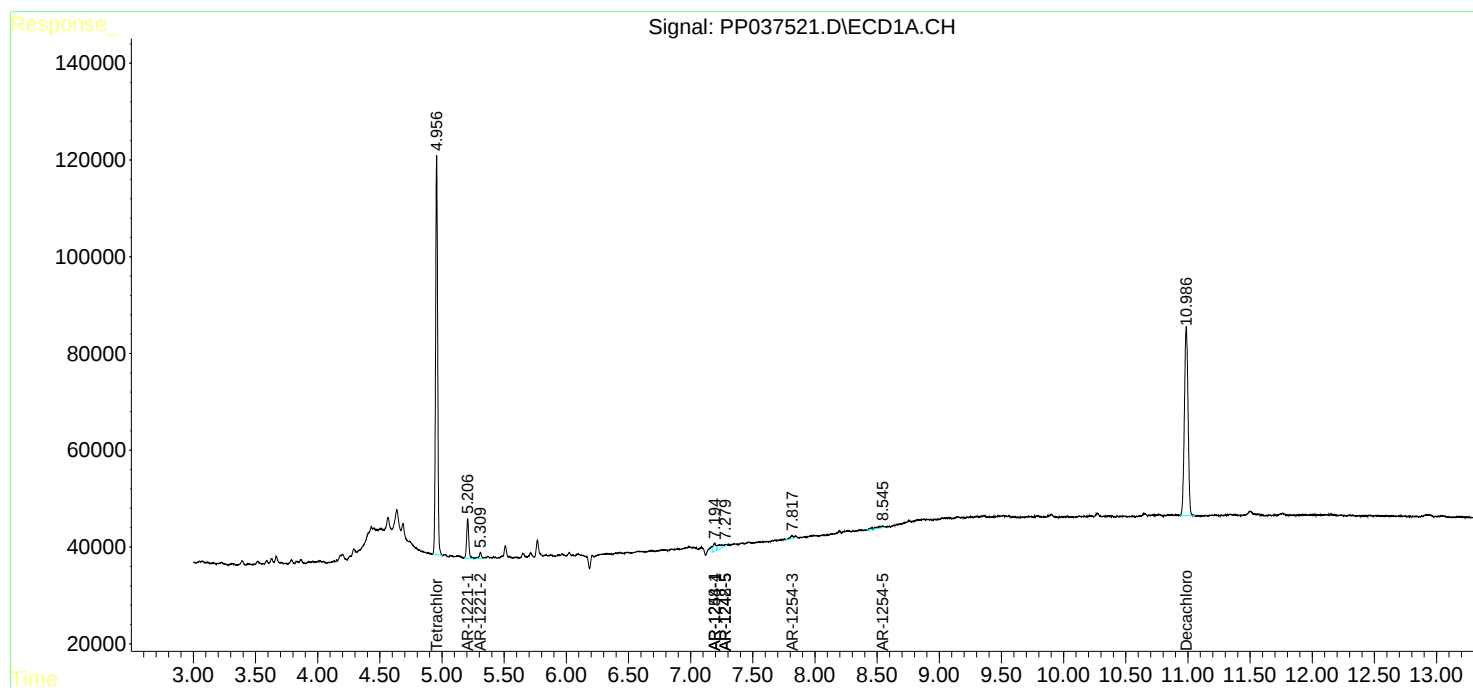


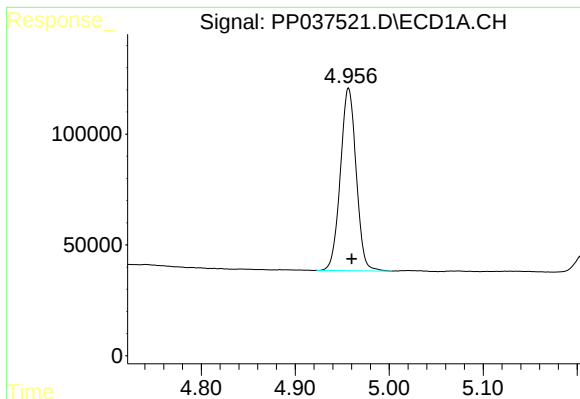

#1 Tetrachloro-m-xylene


R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 960632
Conc: 21.14 ng/ml

Instrument :
ECD_P
ClientSampleId :

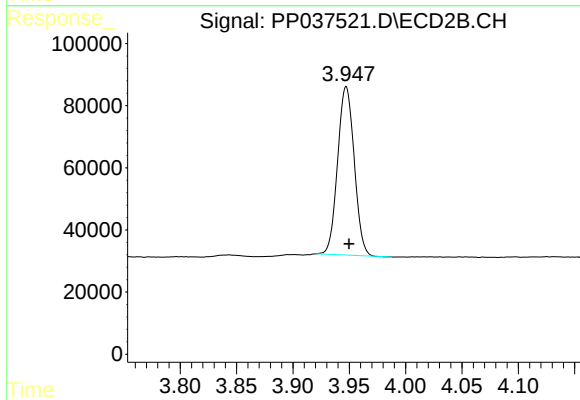


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.003 min
Response: 554984
Conc: 20.28 ng/ml

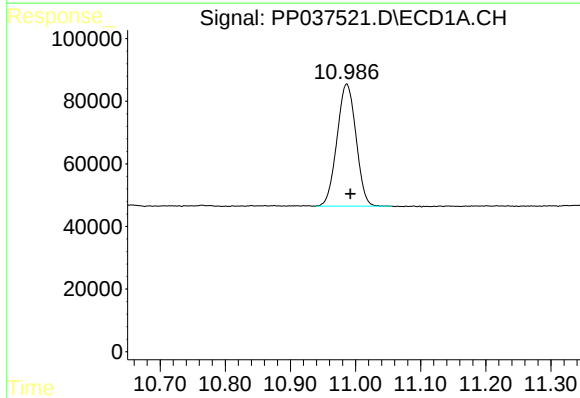


#2 Decachlorobiphenyl

R.T.: 10.986 min
Delta R.T.: -0.006 min
Response: 791843
Conc: 17.20 ng/ml

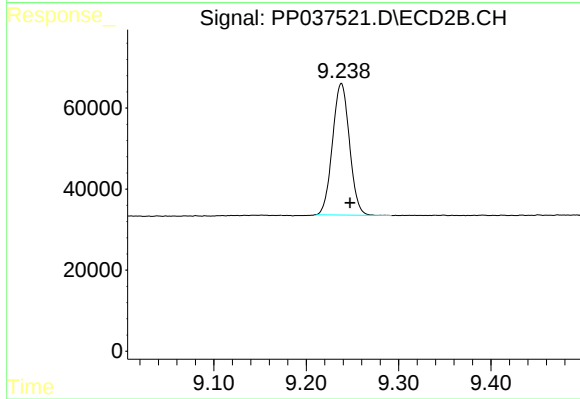

#2 Decachlorobiphenyl


R.T.: 9.238 min
Delta R.T.: -0.009 min
Response: 413732
Conc: 14.86 ng/ml

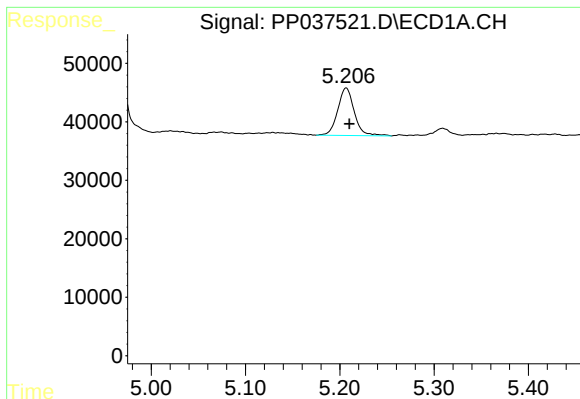

#8 AR-1221-1


R.T.: 5.207 min
Delta R.T.: -0.004 min
Response: 99211
Conc: 187.06 ng/ml

Instrument :
ECD_P
ClientSampleId :

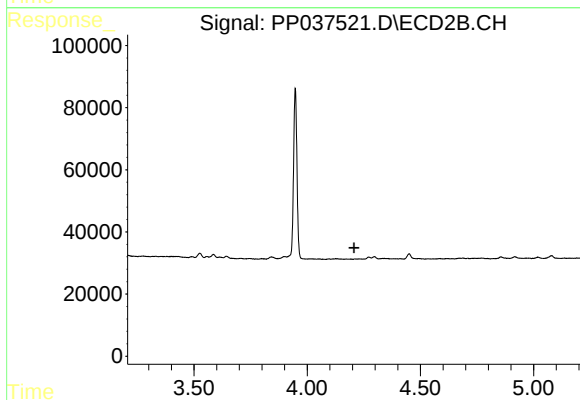


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

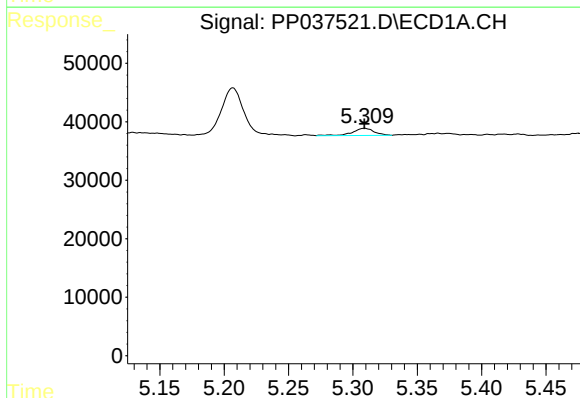


#9 AR-1221-2

R.T.: 5.309 min
Delta R.T.: 0.000 min
Response: 14523
Conc: 35.85 ng/ml

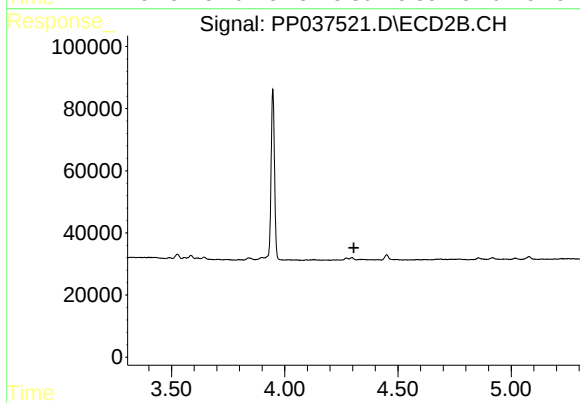

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.305 min
Response: 0
Conc: N.D.

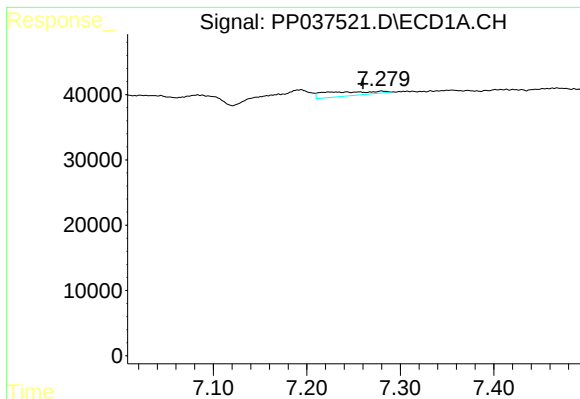

#20 AR-1242-5


R.T.: 7.280 min
Delta R.T.: 0.020 min
Response: 24386
Conc: 23.45 ng/ml

Instrument :
ECD_P
ClientSampleId :

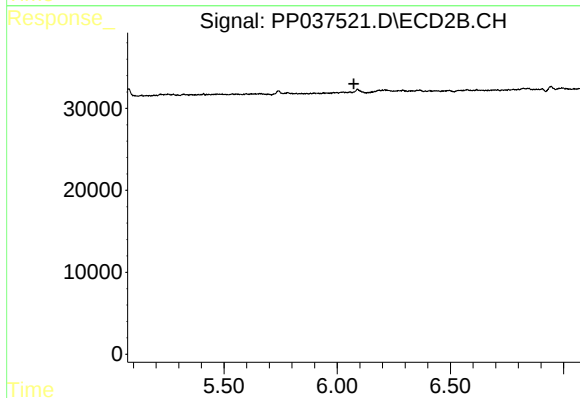


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

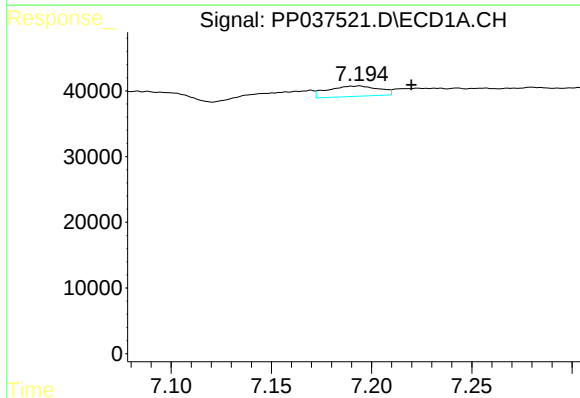


#24 AR-1248-4

R.T.: 7.194 min
Delta R.T.: -0.026 min
Response: 28235
Conc: 14.94 ng/ml

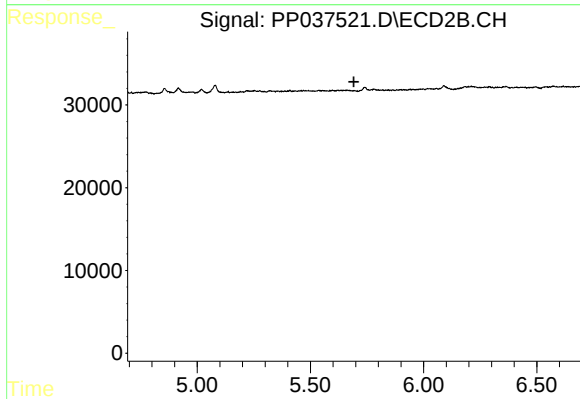

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.692 min
Response: 0
Conc: N.D.

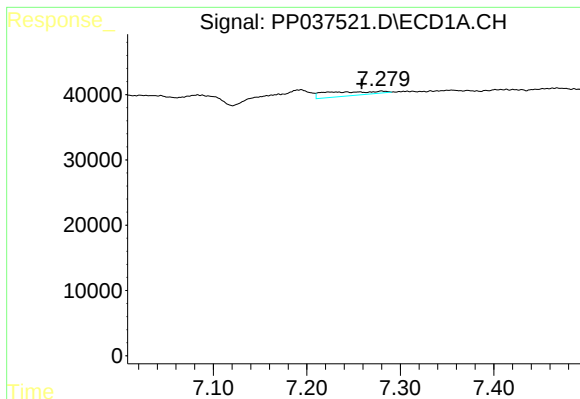

#25 AR-1248-5


R.T.: 7.280 min
Delta R.T.: 0.021 min
Response: 24386
Conc: 13.03 ng/ml

Instrument :
ECD_P
ClientSampleId :

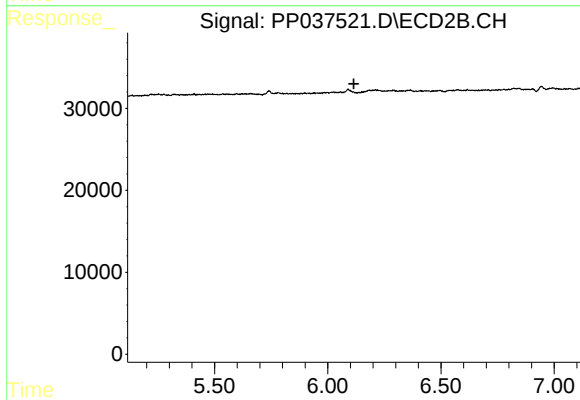


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

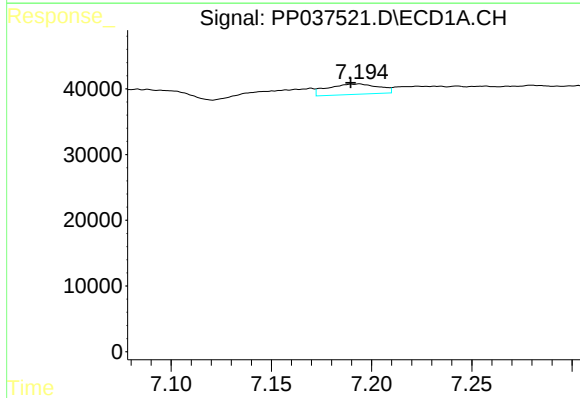


#26 AR-1254-1

R.T.: 7.194 min
Delta R.T.: 0.004 min
Response: 28235
Conc: 15.72 ng/ml

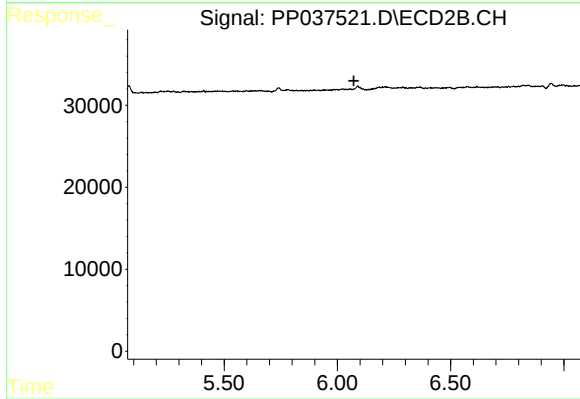

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

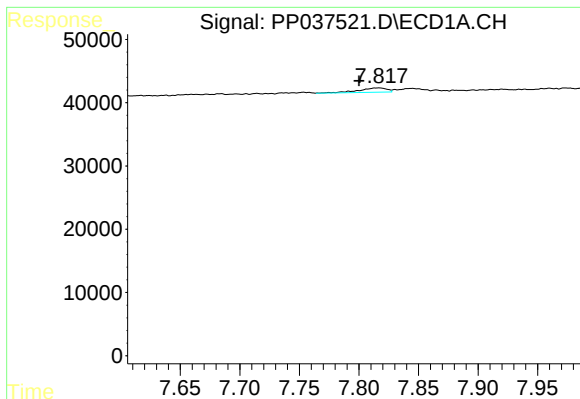

#28 AR-1254-3


R.T.: 7.817 min
Delta R.T.: 0.017 min
Response: 10897
Conc: 3.53 ng/ml

Instrument :
ECD_P
ClientSampleId :

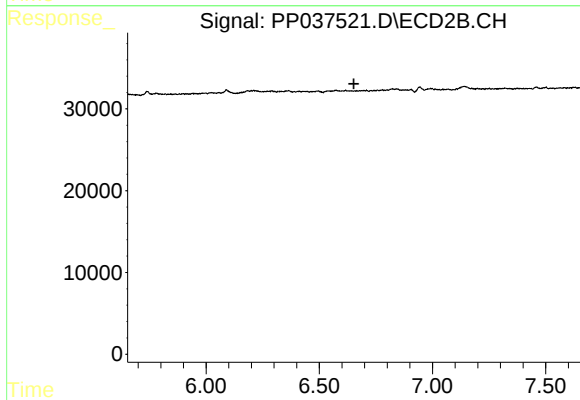


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

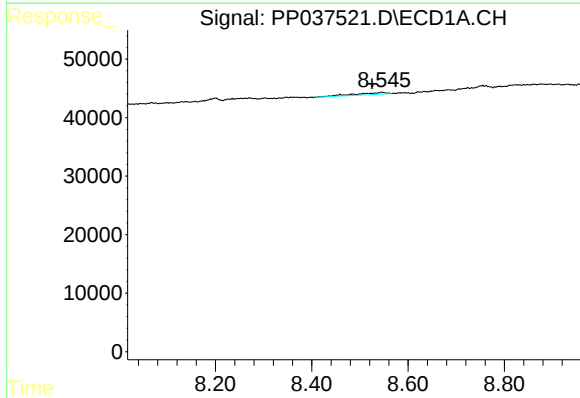

#30 AR-1254-5

R.T.: 8.545 min
Delta R.T.: 0.020 min
Response: 15426
Conc: 6.16 ng/ml

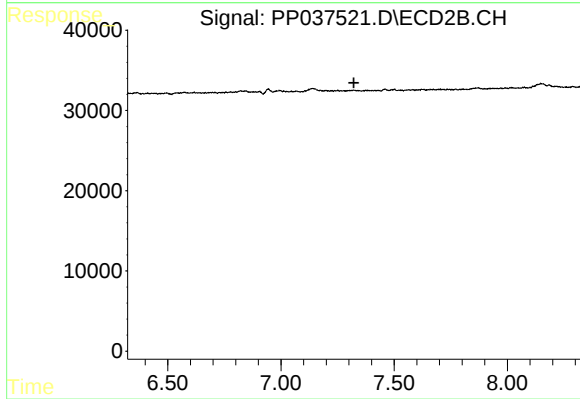

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.322 min
Response: 0
Conc: N.D.