

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072121\
 Data File : PP037535.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2021 6:22
 Operator : DD\AJ
 Sample : M3099-03 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 06:48:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.957	3.948	74558	47434	1.640	1.733
2) SA Decachlor...	10.987	9.242	73036	32873	1.587	1.181 #
Target Compounds						
30) L6 AR-1254-5	8.533	0.000	11754	0	4.697	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072121\
Data File : PP037535.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2021 6:22
Operator : DD\AJ
Sample : M3099-03 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 06:48:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

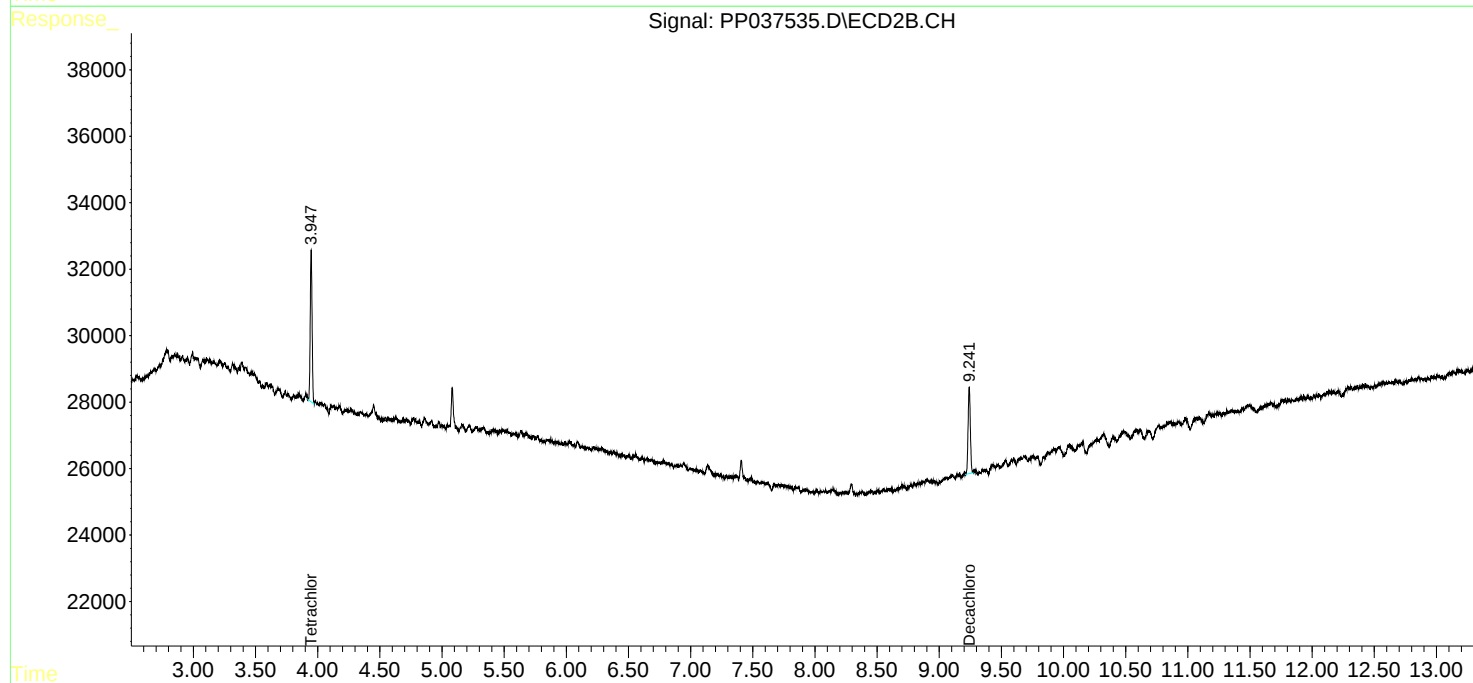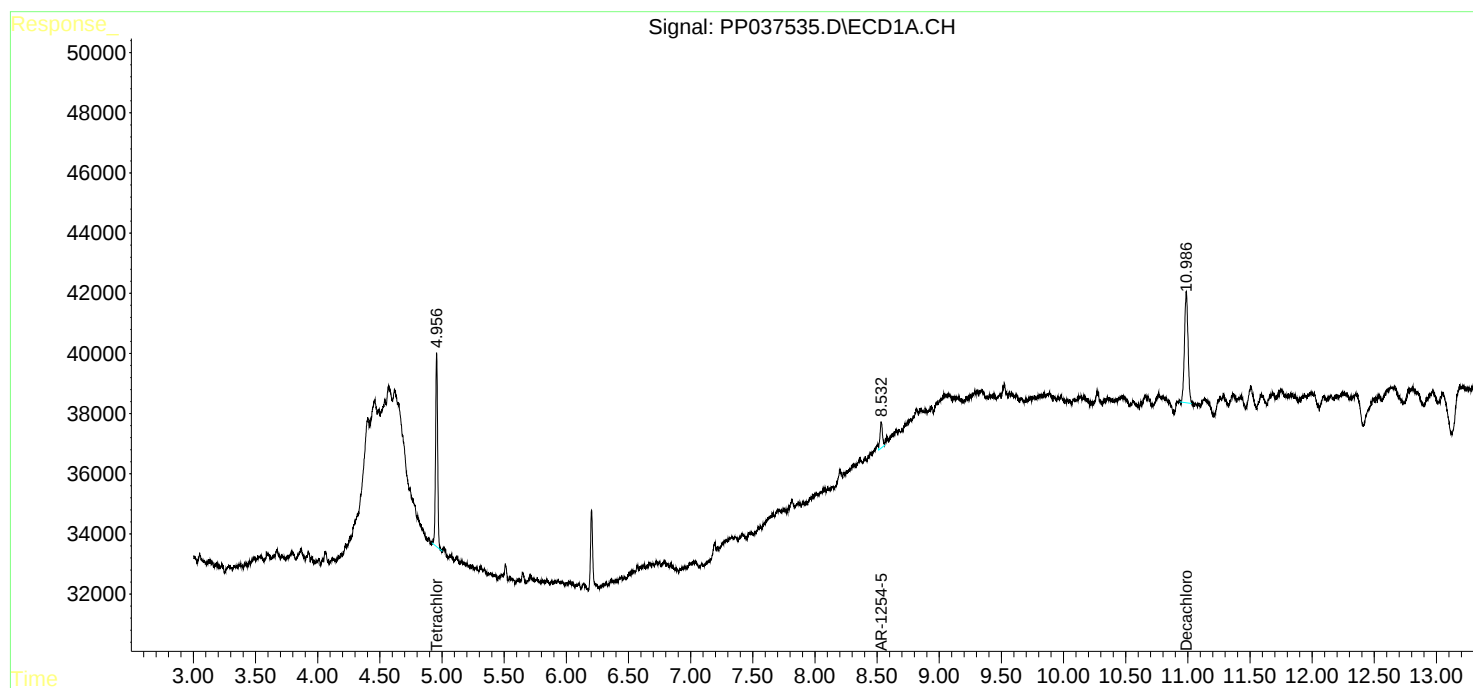


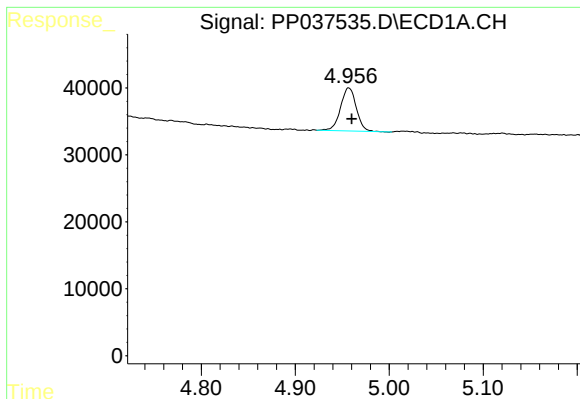

#1 Tetrachloro-m-xylene


R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 74558
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

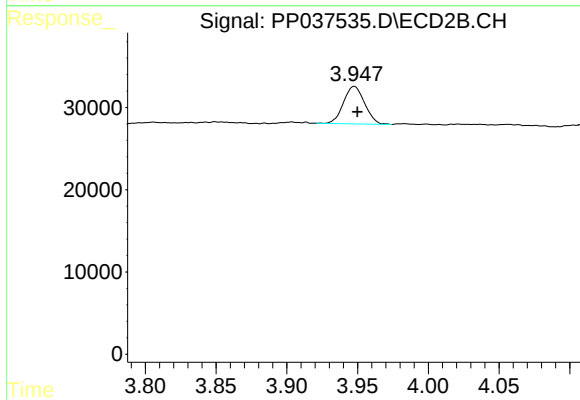


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 47434
Conc: 1.73 ng/ml

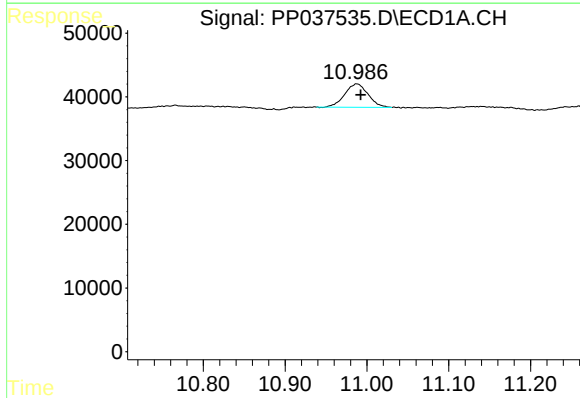


#2 Decachlorobiphenyl

R.T.: 10.987 min
Delta R.T.: -0.005 min
Response: 73036
Conc: 1.59 ng/ml

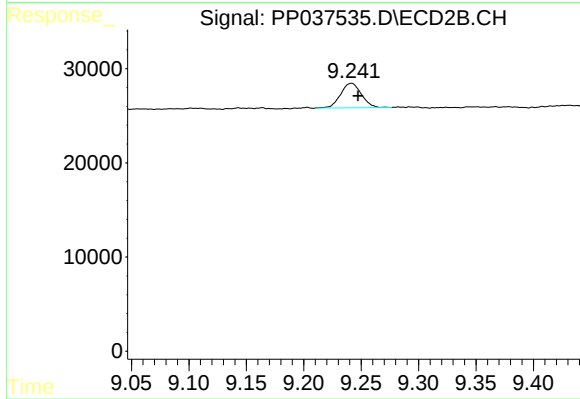

#2 Decachlorobiphenyl


R.T.: 9.242 min
Delta R.T.: -0.006 min
Response: 32873
Conc: 1.18 ng/ml

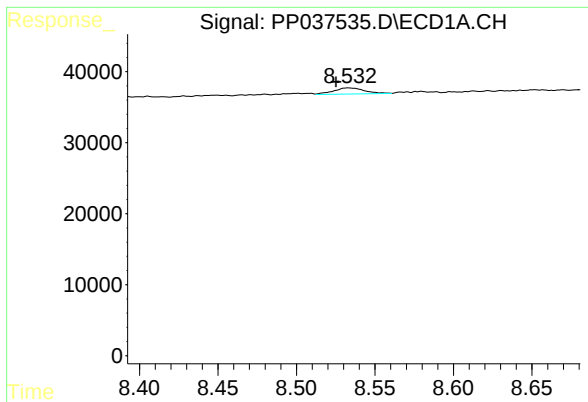

#30 AR-1254-5

R.T.: 8.533 min
Delta R.T.: 0.008 min
Response: 11754
Conc: 4.70 ng/ml

Instrument :
ECD_P
ClientSampleId :

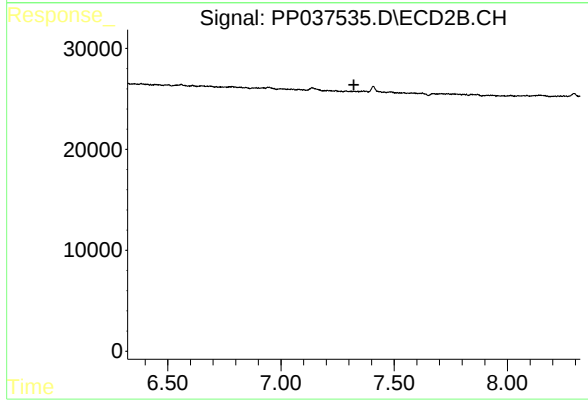

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.322 min
Response: 0
Conc: N.D.