

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072121\
 Data File : PP037484.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jul 2021 15:25
 Operator : DD\AJ
 Sample : M3070-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 01-A-01-B-01-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 16:06:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.958	3.948	1054122	606160	23.193	22.152
2) SA Decachlor...	10.992	9.241	1023981	545026	22.243m	19.581m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072121\
Data File : PP037484.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jul 2021 15:25
Operator : DD\AJ
Sample : M3070-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 16:06:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

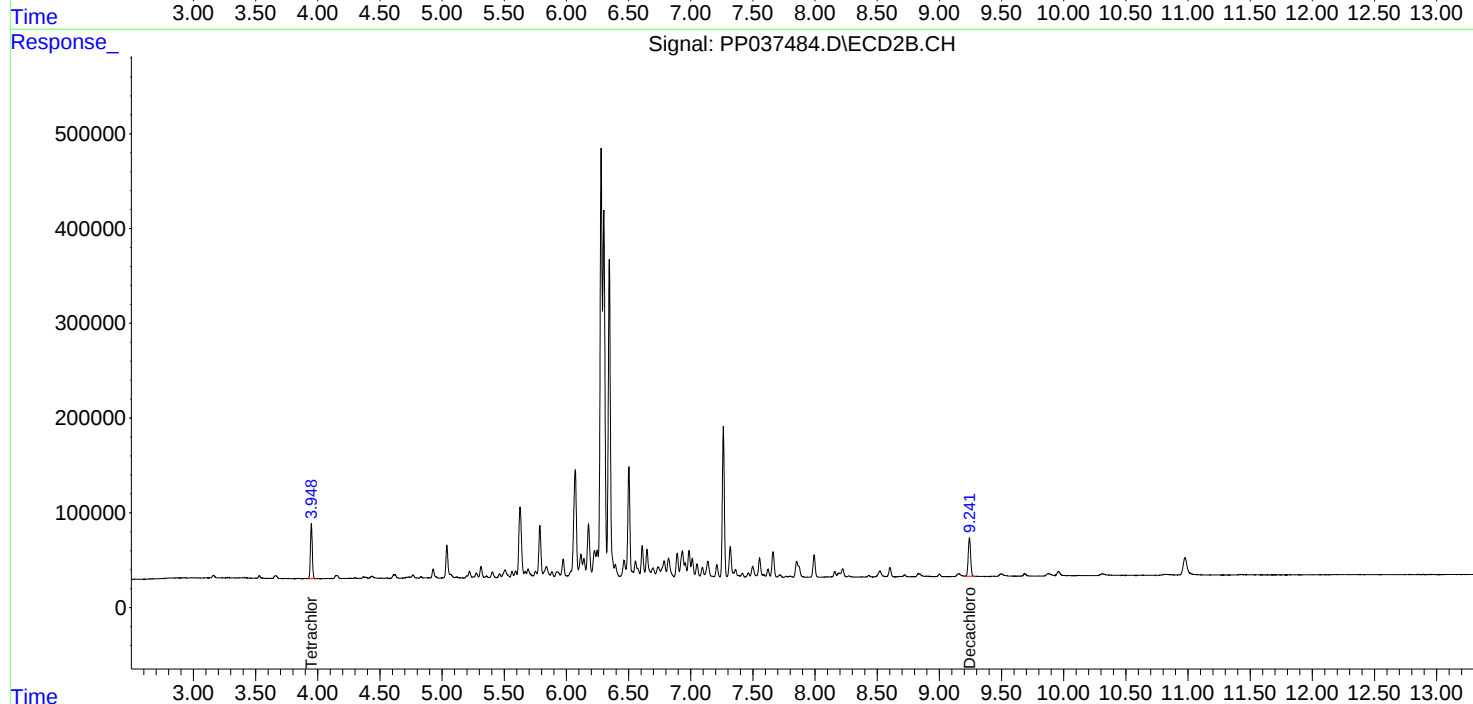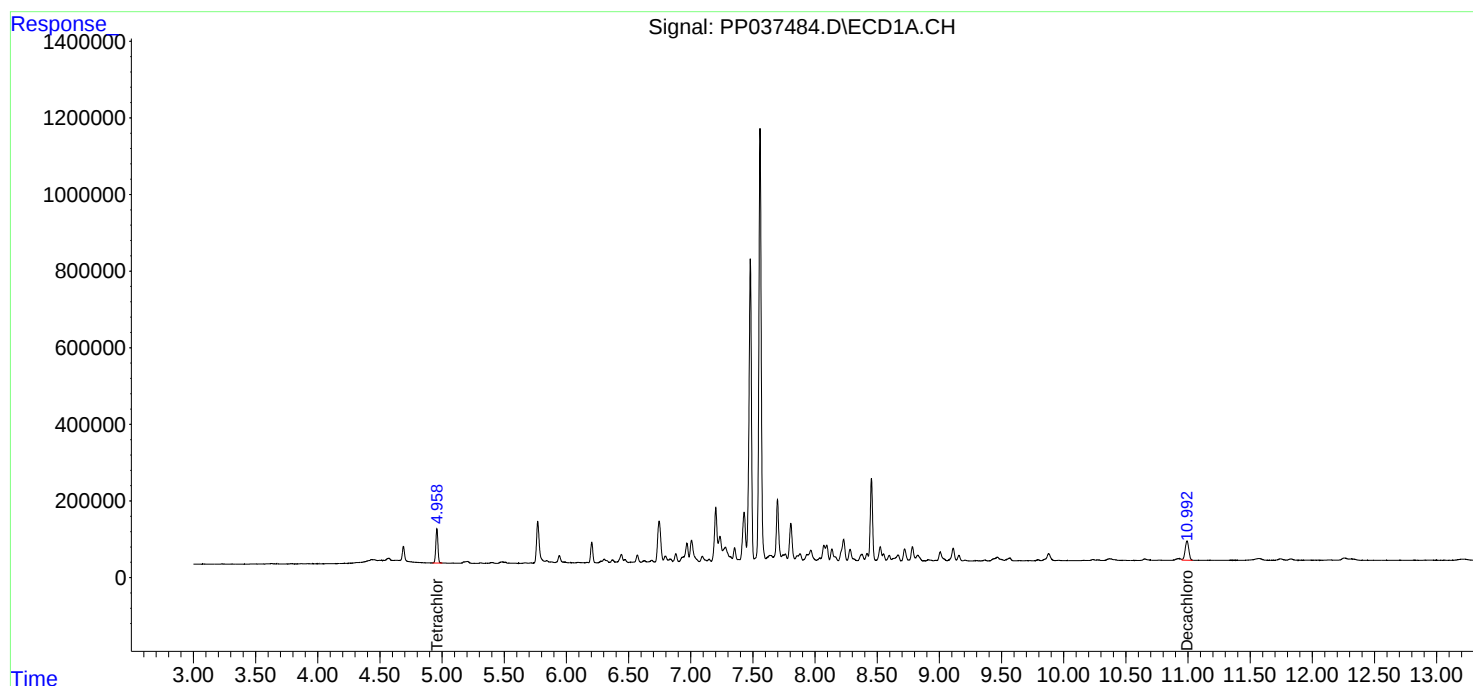


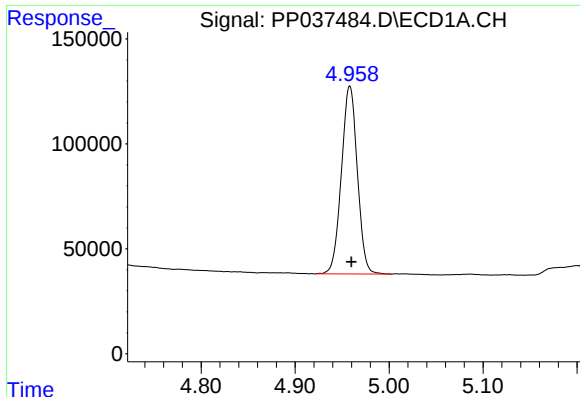

#1 Tetrachloro-m-xylene


R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 1054122
Conc: 23.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C

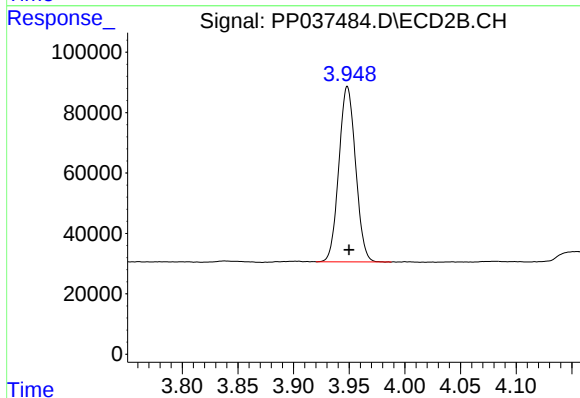


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 606160
Conc: 22.15 ng/ml

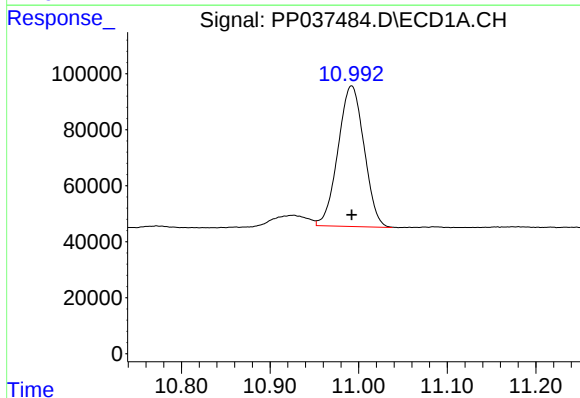

#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: 0.000 min
Response: 1023981
Conc: 22.24 ng/ml m

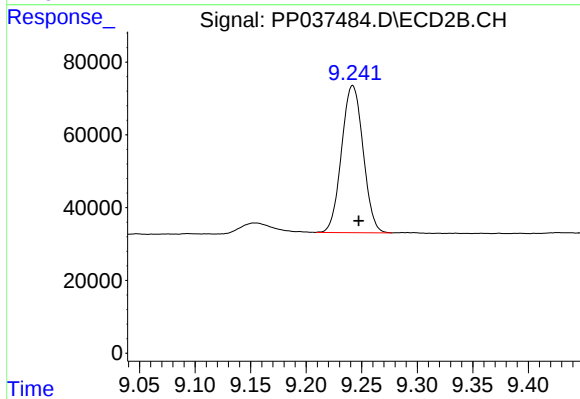

#2 Decachlorobiphenyl

R.T.: 9.241 min
Delta R.T.: -0.006 min
Response: 545026
Conc: 19.58 ng/ml m