

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072121\
 Data File : PP037537.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2021 6:56
 Operator : DD\AJ
 Sample : M3100-01 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC260356LOK-END-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 06:55:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.956	3.946	67233	46506	1.479	1.700
2) SA Decachlor...	10.983	9.237	73021	35009	1.586	1.258

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072121\
Data File : PP037537.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2021 6:56
Operator : DD\AJ
Sample : M3100-01 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BC260356LOK-END-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 06:55:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

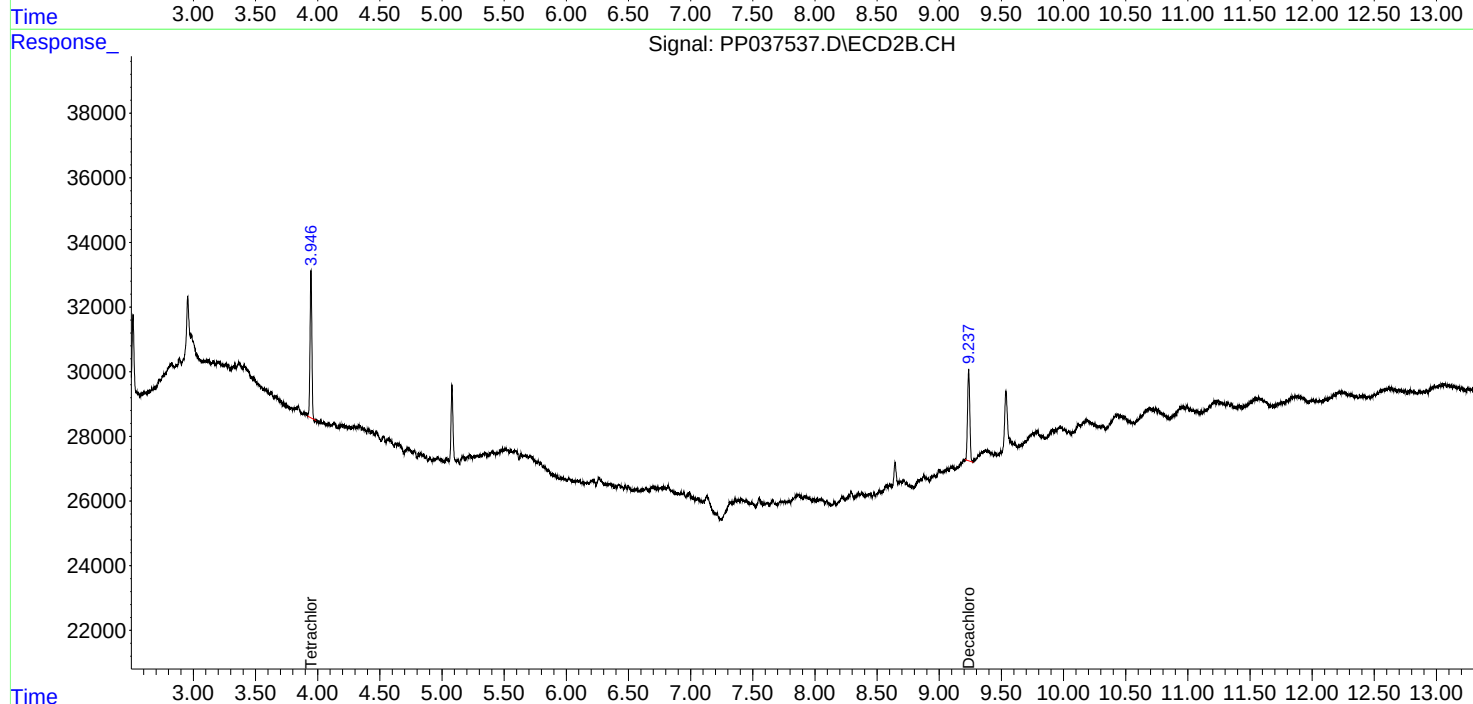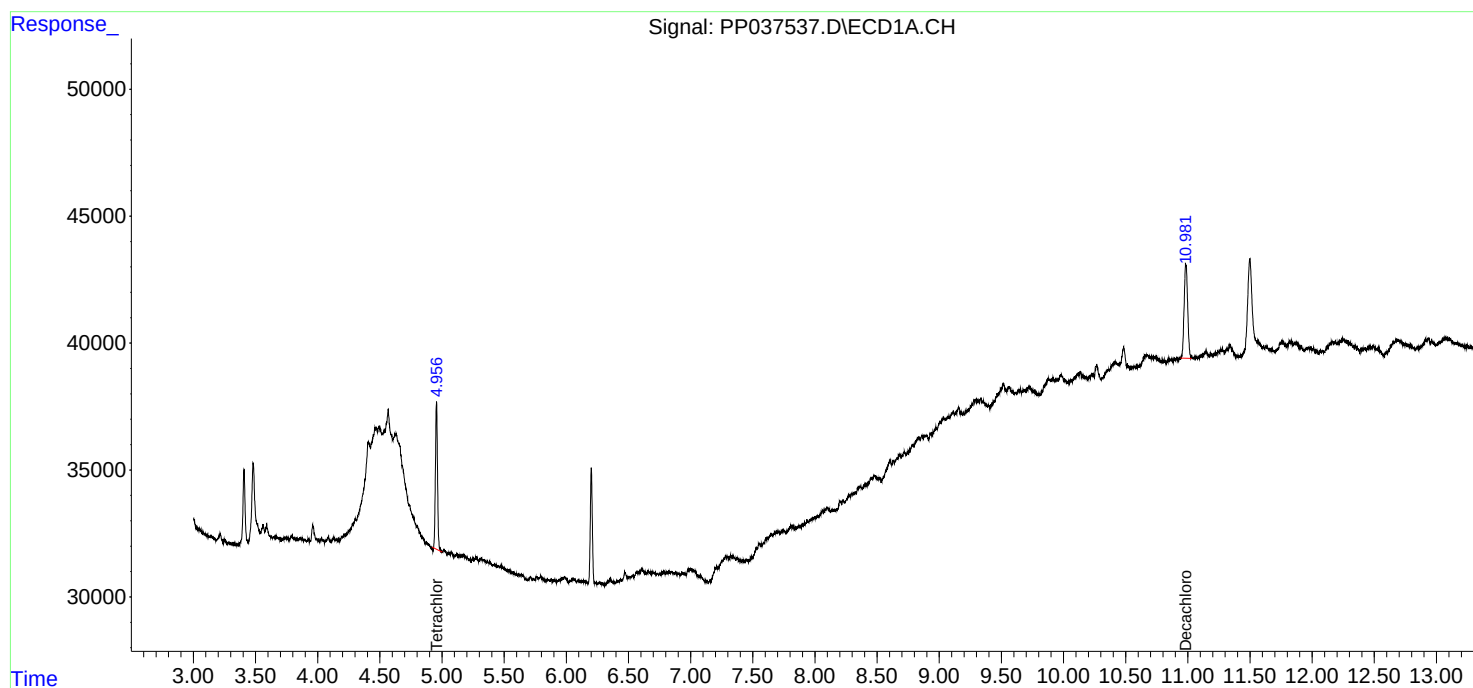


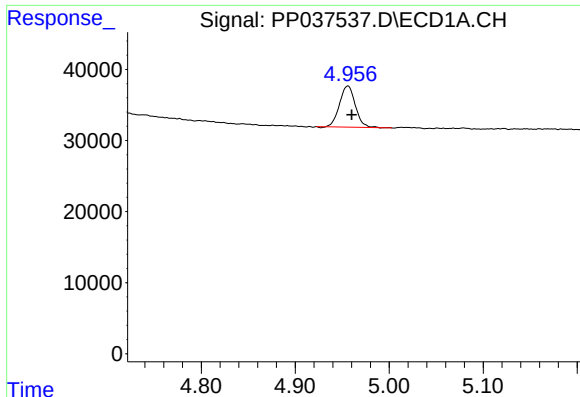

#1 Tetrachloro-m-xylene


R.T.: 4.956 min
Delta R.T.: -0.004 min
Response: 67233
Conc: 1.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC260356LOK-END-1-1

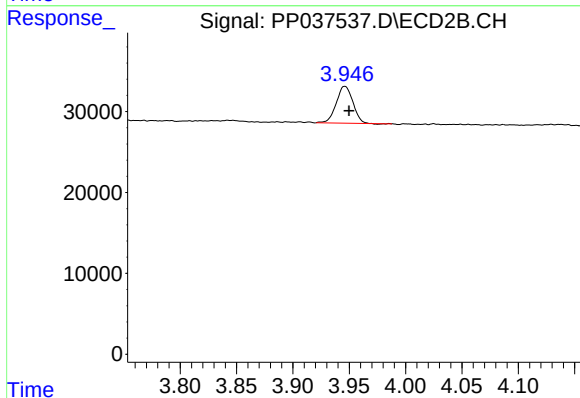


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 46506
Conc: 1.70 ng/ml

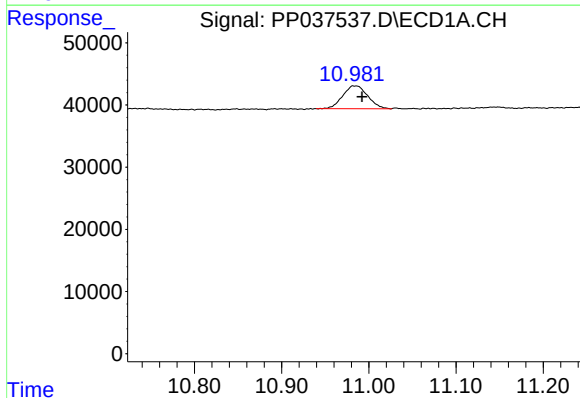

#2 Decachlorobiphenyl

R.T.: 10.983 min
Delta R.T.: -0.009 min
Response: 73021
Conc: 1.59 ng/ml

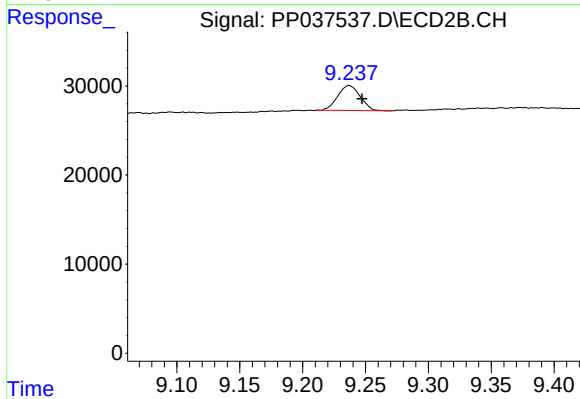

#2 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: -0.010 min
Response: 35009
Conc: 1.26 ng/ml