

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072122\
 Data File : PP049691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 11:00
 Operator : YP\AJ
 Sample : N3774-05DL 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 34072DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2022
 Supervised By :Ankita Jodhani 07/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 15:57:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.601	15594576	26065742	10.746	10.664
2) SA Decachlor...	10.103	8.567	16884209	13352361	11.937	11.465
Target Compounds						
16) L4 AR-1242-1	5.529	4.674	31652940	44010005	707.976m	627.473
17) L4 AR-1242-2	5.551	4.692	40008772	59198860	634.555m	599.933
18) L4 AR-1242-3	5.613	4.867	26826443	33409642	689.971	640.199
19) L4 AR-1242-4	5.714	4.950	24012905	38340274	744.347	731.520
20) L4 AR-1242-5	6.453	5.469	13979701	29758752	406.489	468.163

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072122\
Data File : PP049691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 11:00
Operator : YP\AJ
Sample : N3774-05DL 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
34072DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 15:57:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

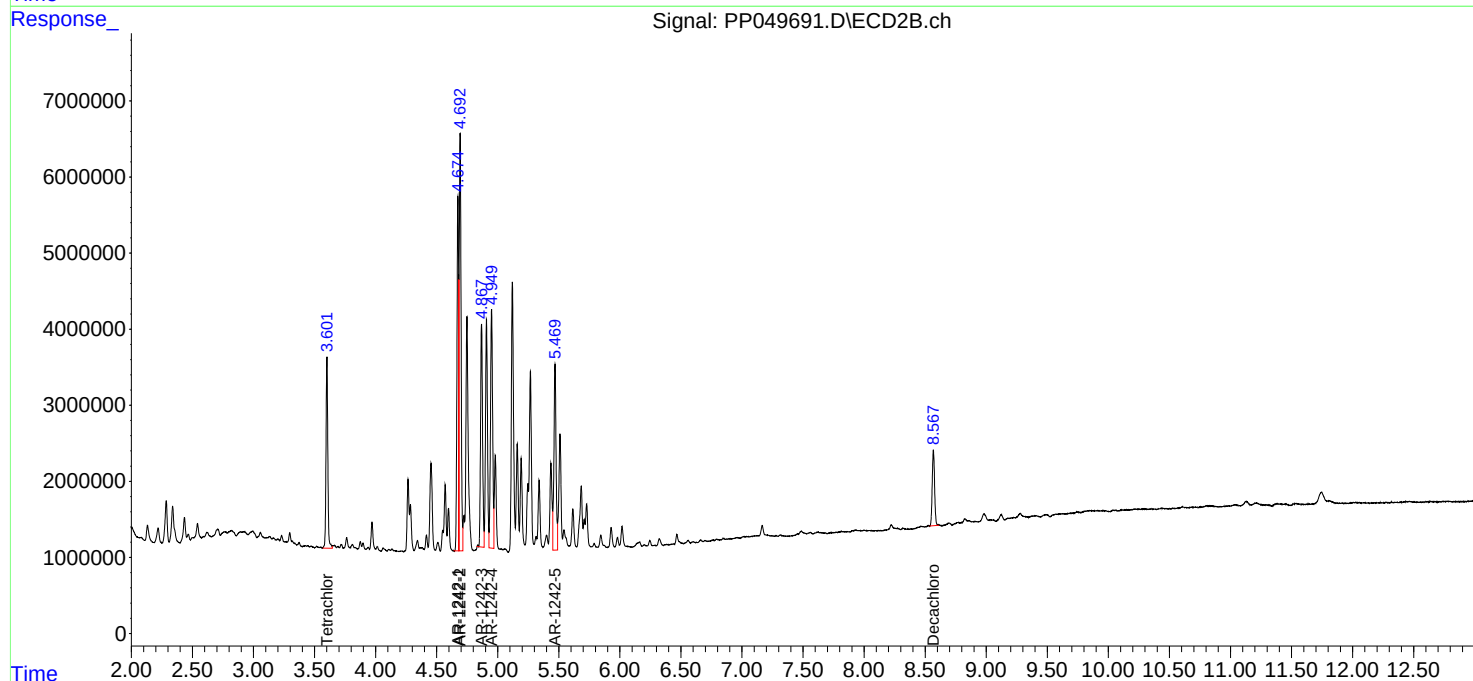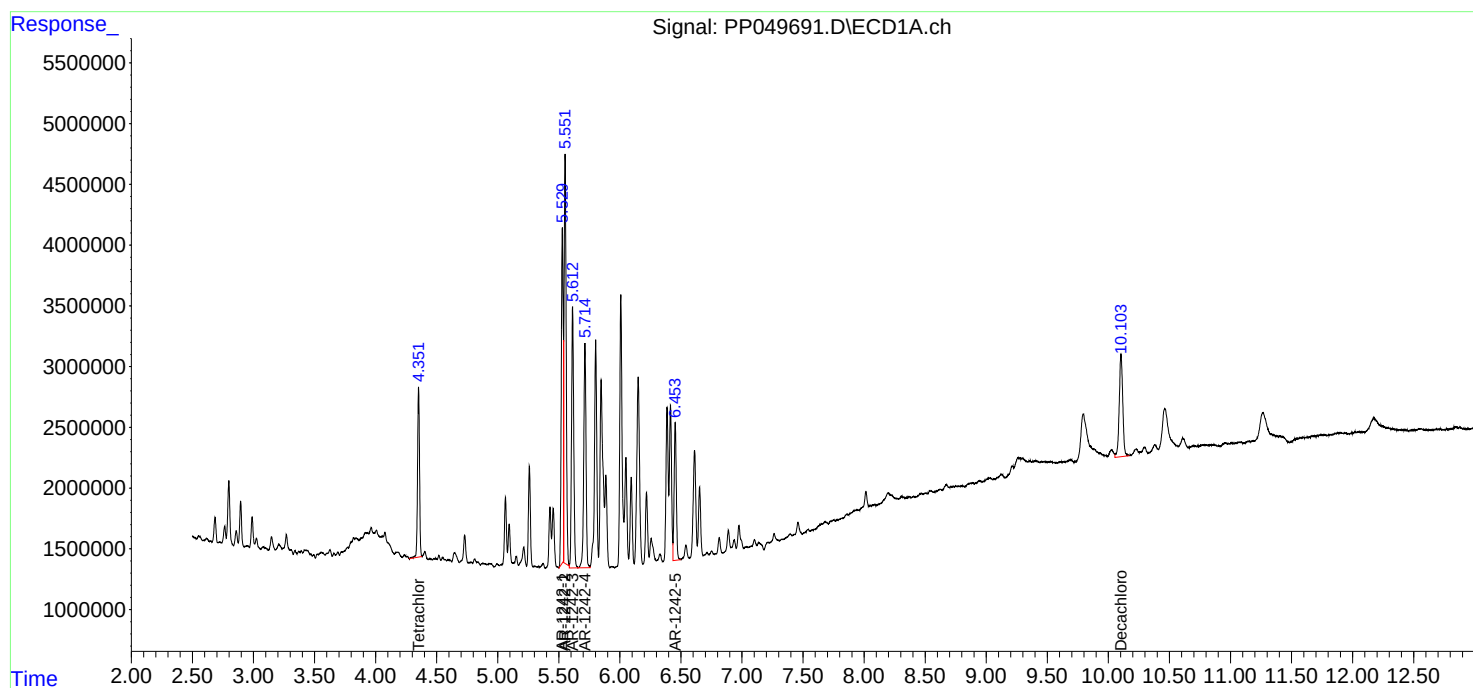

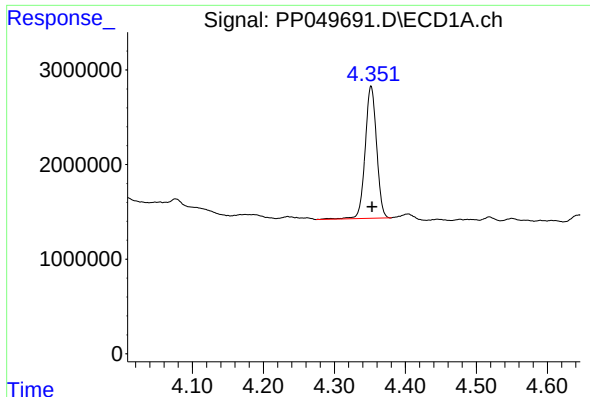


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: -0.001 min
Response: 15594576
Conc: 10.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
34072DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

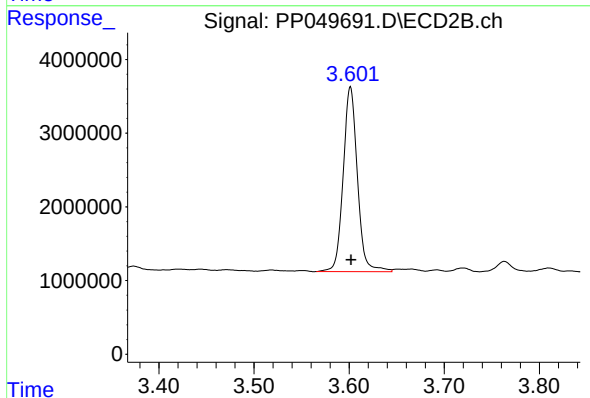


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 26065742
Conc: 10.66 ng/ml

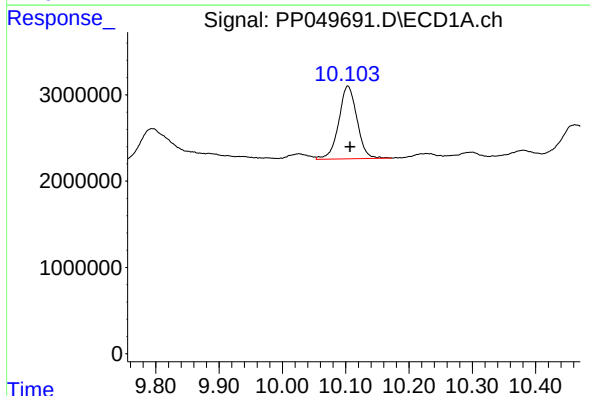


#2 Decachlorobiphenyl

R.T.: 10.103 min
Delta R.T.: -0.004 min
Response: 16884209
Conc: 11.94 ng/ml

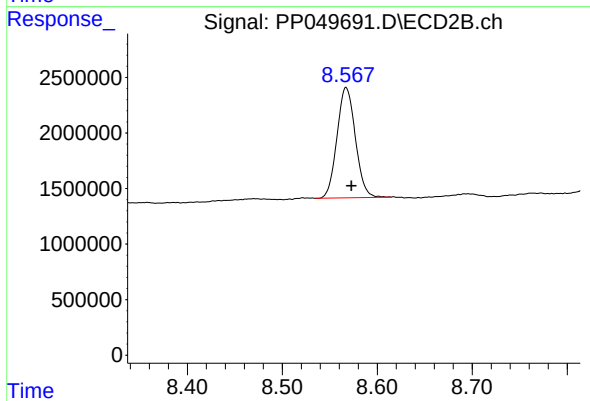

#2 Decachlorobiphenyl

R.T.: 8.567 min
Delta R.T.: -0.005 min
Response: 13352361
Conc: 11.47 ng/ml

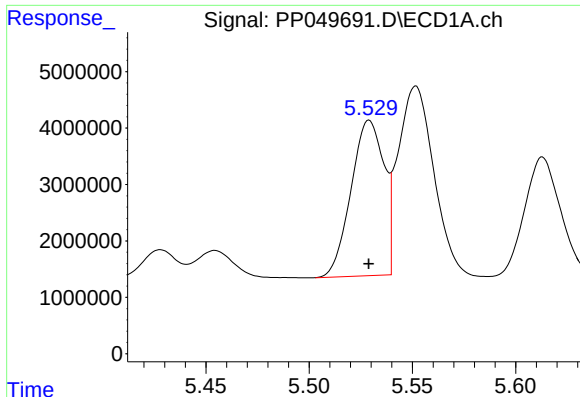


#16 AR-1242-1

R.T.: 5.529 min
Delta R.T.: 0.000 min
Response: 31652940
Conc: 707.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
34072DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

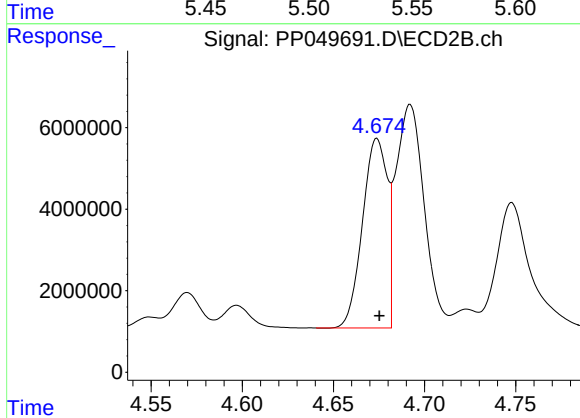


#16 AR-1242-1

R.T.: 4.674 min
Delta R.T.: -0.001 min
Response: 44010005
Conc: 627.47 ng/ml

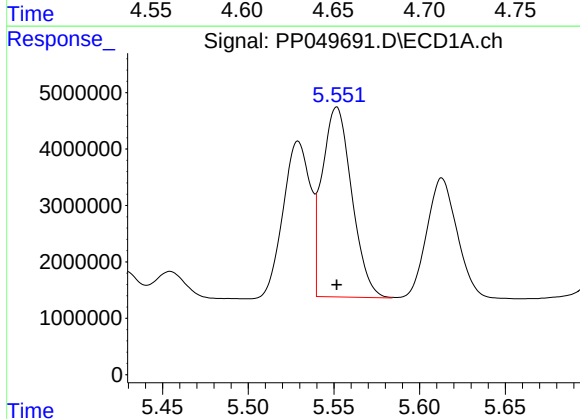


#17 AR-1242-2

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 40008772
Conc: 634.55 ng/ml m

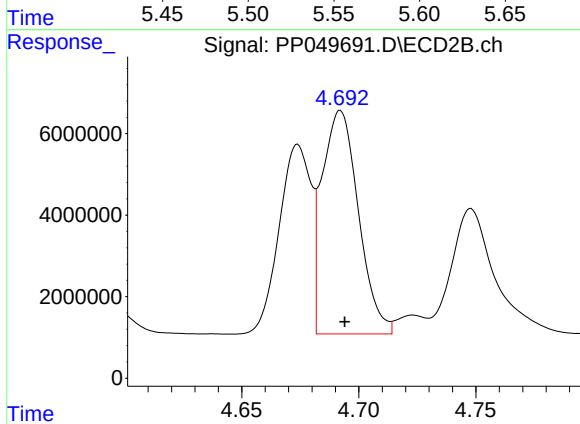

#17 AR-1242-2

R.T.: 4.692 min
Delta R.T.: -0.002 min
Response: 59198860
Conc: 599.93 ng/ml

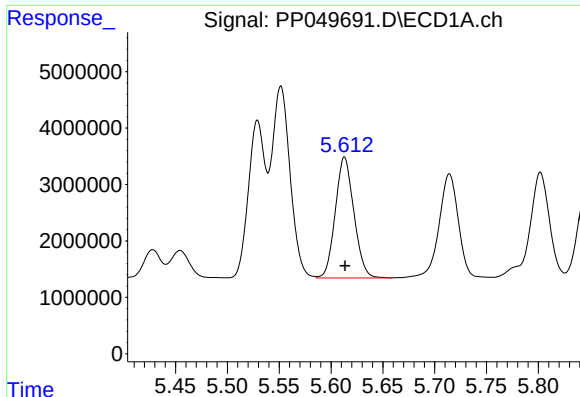


#18 AR-1242-3

R.T.: 5.613 min
Delta R.T.: 0.000 min
Response: 26826443
Conc: 689.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
34072DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

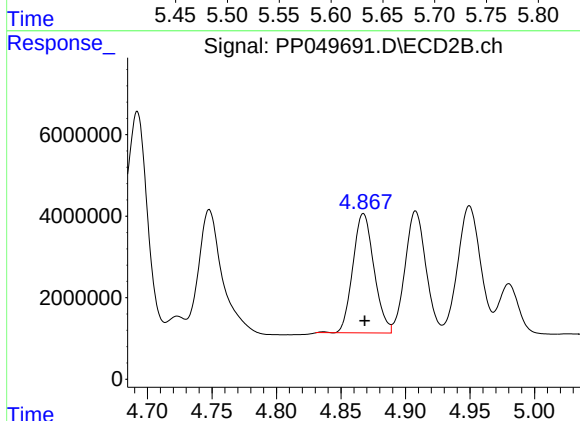


#18 AR-1242-3

R.T.: 4.867 min
Delta R.T.: 0.000 min
Response: 33409642
Conc: 640.20 ng/ml

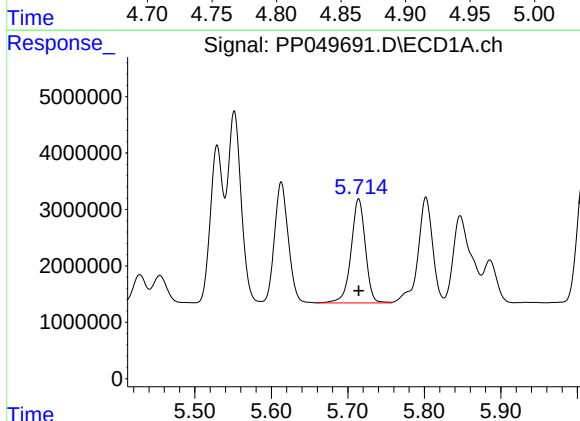


#19 AR-1242-4

R.T.: 5.714 min
Delta R.T.: 0.000 min
Response: 24012905
Conc: 744.35 ng/ml

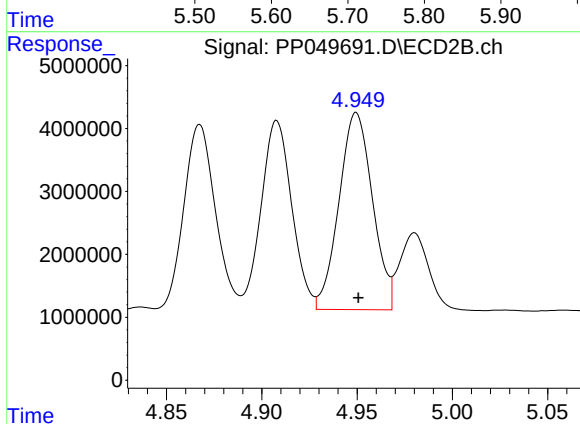

#19 AR-1242-4

R.T.: 4.950 min
Delta R.T.: -0.001 min
Response: 38340274
Conc: 731.52 ng/ml

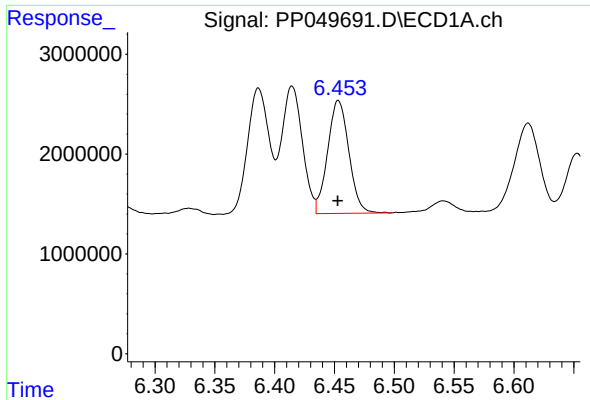


#20 AR-1242-5

R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 13979701
Conc: 406.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
34072DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

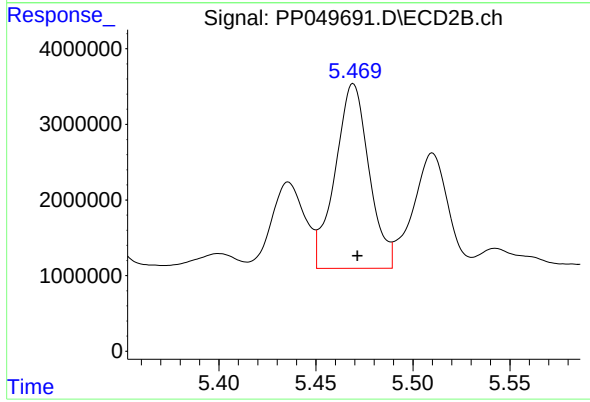

#20 AR-1242-5

R.T.: 5.469 min
Delta R.T.: -0.002 min
Response: 29758752
Conc: 468.16 ng/ml