

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 10:13
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:46:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.519f	3.807f	950114	108701	0.694	0.059 #
2)	SA Decachlor...	10.169	0.000	432679	0	0.397	N.D. #
Target Compounds							
3)	L1 AR-1016-1	5.620	4.854	118969	1873750	2.504	27.485 #
4)	L1 AR-1016-2	5.684	4.879	131961	500141	1.853	4.909 #
5)	L1 AR-1016-3	5.725	5.034	149515	2014166	3.424	37.226 #
6)	L1 AR-1016-4	5.813	5.089	53441	2443227	1.487	55.679 #
7)	L1 AR-1016-5	6.128	5.316	1137200	795586	36.297	14.576 #
8)	L2 AR-1221-1	4.694	3.994	40362	94155	2.259	3.481 #
9)	L2 AR-1221-2	4.799	4.082	99033	272200	7.333	13.369 #
10)	L2 AR-1221-3	4.855	4.149	191235	89995	4.596	1.465 #
11)	L3 AR-1232-1	4.855	4.149	191235	89995	5.857	1.931 #
12)	L3 AR-1232-2	5.373	4.879	67456	500141	4.150	10.494 #
13)	L3 AR-1232-3	5.684	5.034	131961	2014166	4.000	80.473 #
14)	L3 AR-1232-4	5.813	5.169	53441	3293587	3.250	152.085 #
15)	L3 AR-1232-5	5.893	5.316	203382	795586	19.241	35.260 #
16)	L4 AR-1242-1	5.620	4.854	118969	1873750	3.115	32.438 #
17)	L4 AR-1242-2	5.684	4.879	131961	500141	2.204	5.785 #
18)	L4 AR-1242-3	5.725	5.034	149515	2014166	4.083	43.837 #
19)	L4 AR-1242-4	5.813	5.169	53441	3293587	1.663	74.409 #
20)	L4 AR-1242-5	6.539	5.673	1184465	9669280	36.181	175.033 #
21)	L5 AR-1248-1	5.620	4.854	118969	1873750	3.854	41.736 #
22)	L5 AR-1248-2	5.893	5.089	203382	2443227	5.094	39.704 #
23)	L5 AR-1248-3	6.128	5.169	1137200	3293587	25.607	51.410 #
24)	L5 AR-1248-4	6.516	5.316	585082	795586	10.622	10.555
25)	L5 AR-1248-5	6.539	5.715	1184465	677697	22.020	9.086 #
26)	L6 AR-1254-1	6.482	5.673	4584386	9669280	85.546	83.334
27)	L6 AR-1254-2	6.694	5.818	7294143	12609767	87.576	125.316 #
28)	L6 AR-1254-3	7.064	6.216	11956841	7518519	135.363	48.680 #
29)	L6 AR-1254-4	7.327	6.444	2416834	817685	30.722	8.647 #
30)	L6 AR-1254-5	7.778	6.842	679.9E6	1100.6E6	9227.489	8247.558
31)	L7 AR-1260-1	7.238	6.341	2722453	248498	46.174	2.547 #
32)	L7 AR-1260-2	7.467	6.521	1138.9E6	8972359	11882.923	73.042 #
33)	L7 AR-1260-3	7.849	6.648	1435228	-1305051	19.642	N.D. #
34)	L7 AR-1260-4	8.070	7.182f	949027	326962	14.533	3.657 #
35)	L7 AR-1260-5	8.396	7.394	433468	220923	2.873	0.983 #
36)	L8 AR-1262-1	8.070	6.929f	949027	161047	10.905	1.090 #
37)	L8 AR-1262-2	8.396	7.182	433468	326962	2.189	2.558
38)	L8 AR-1262-3	8.692	7.686	130849	6329246	1.041	55.510 #
39)	L8 AR-1262-4	8.782	7.686f	238231	6329246	2.554	34.389 #
40)	L8 AR-1262-5	9.418	8.211	211877	42205	3.342	0.500 #
41)	L9 AR-1268-1	8.692	7.686	130849	6329246	0.586	20.591 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 10:13
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:46:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.782	7.686f	238231	6329246	1.251	23.822 #
43) L9	AR-1268-3	9.024	7.939	228613	77748	1.381	0.345 #
44) L9	AR-1268-4	9.418	8.211	211877	42205	3.047	0.454 #
45) L9	AR-1268-5	9.877f	8.542	602853	29138	1.308	0.047 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
Data File : PP073977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 10:13
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:46:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

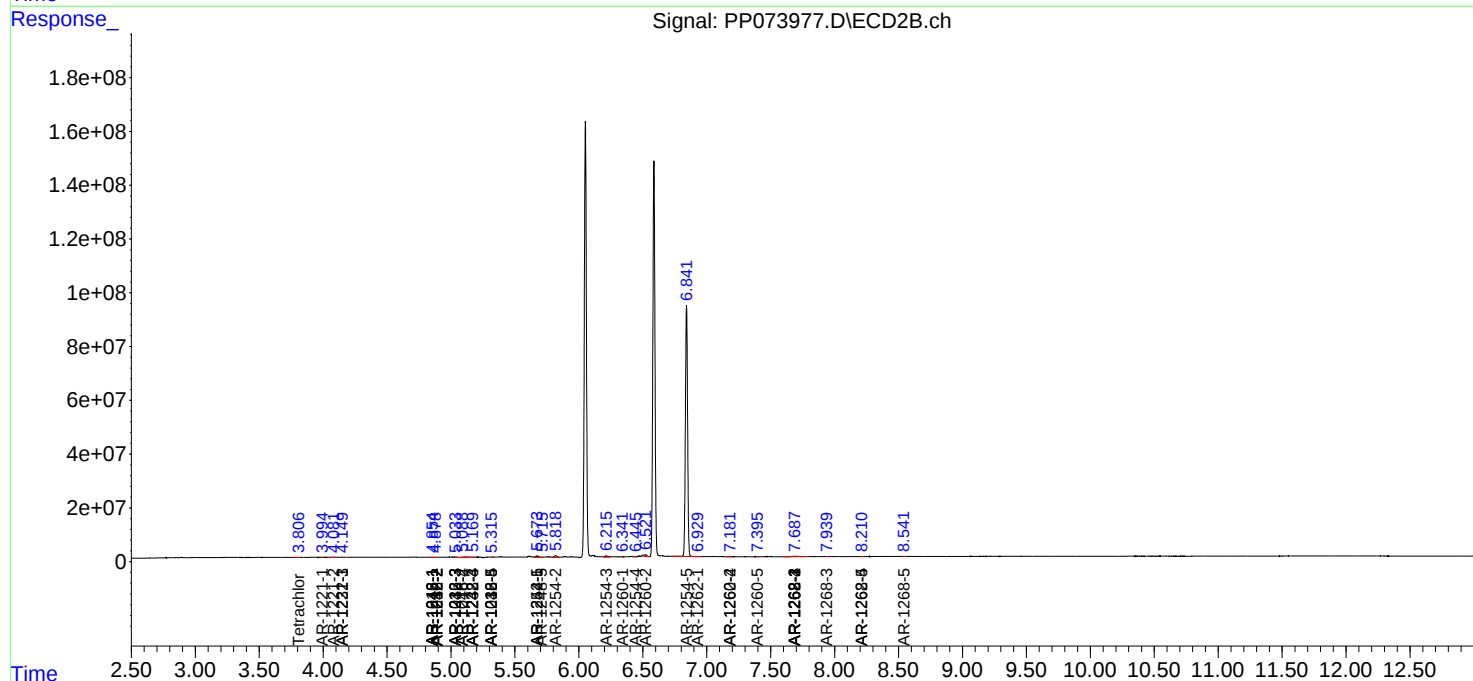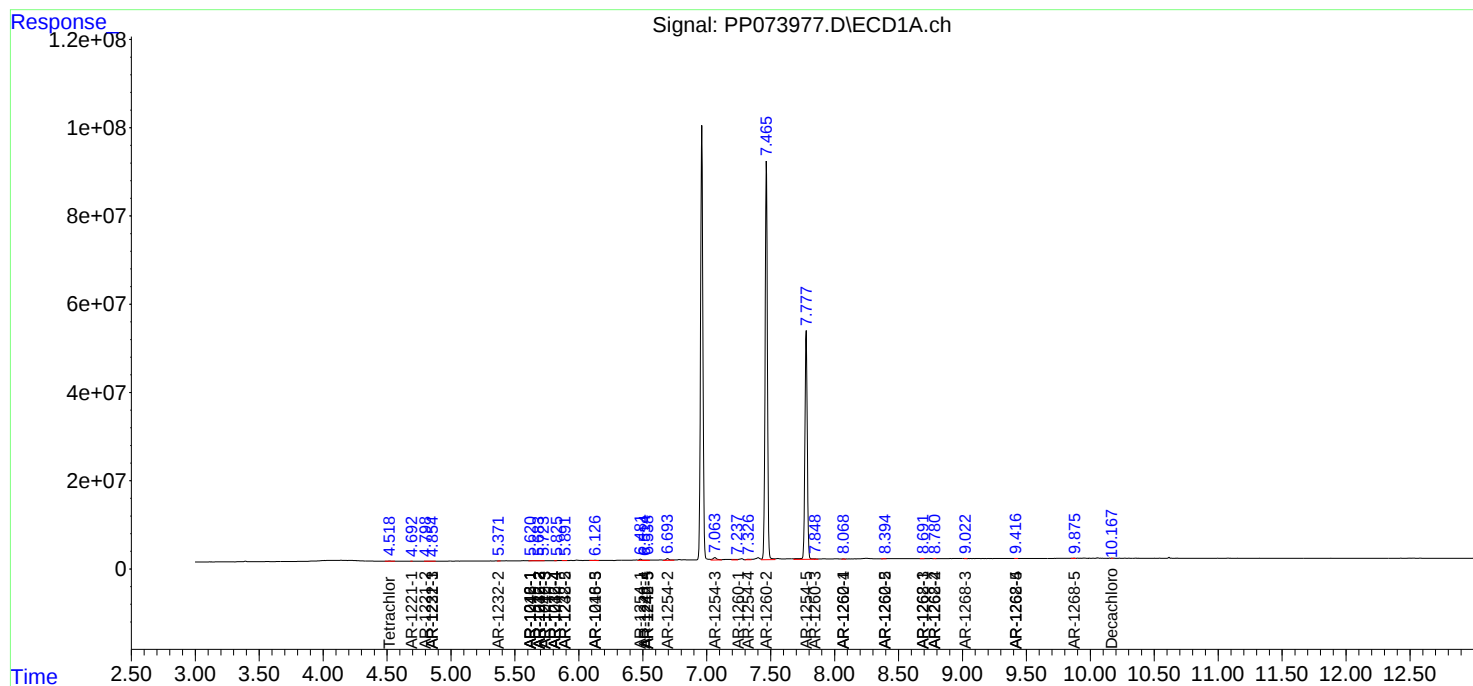


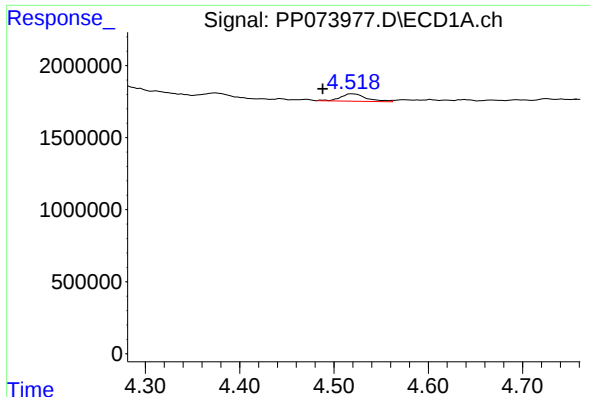

#1 Tetrachloro-m-xylene


R.T.: 4.519 min
Delta R.T.: 0.031 min
Response: 950114
Conc: 0.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

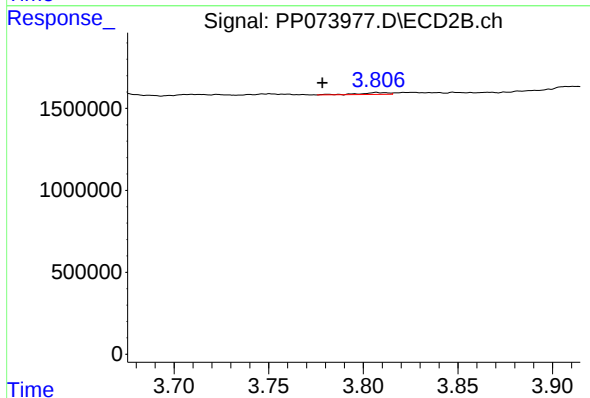


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.029 min
Response: 108701
Conc: 0.06 ng/ml

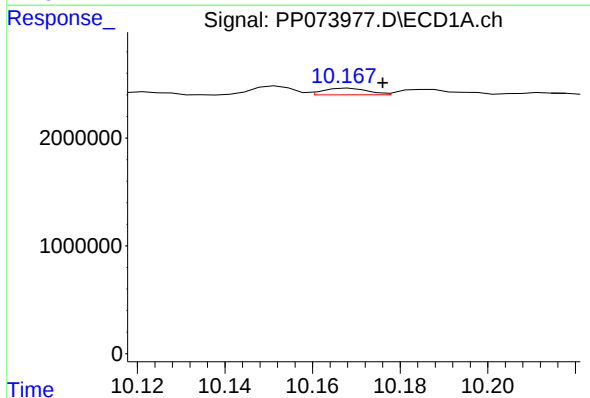


#2 Decachlorobiphenyl

R.T.: 10.169 min
Delta R.T.: -0.007 min
Response: 432679
Conc: 0.40 ng/ml

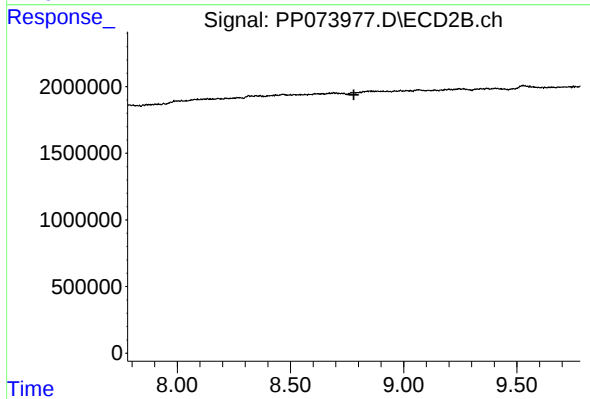

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T.: 8.780 min
Response: 0
Conc: N.D.

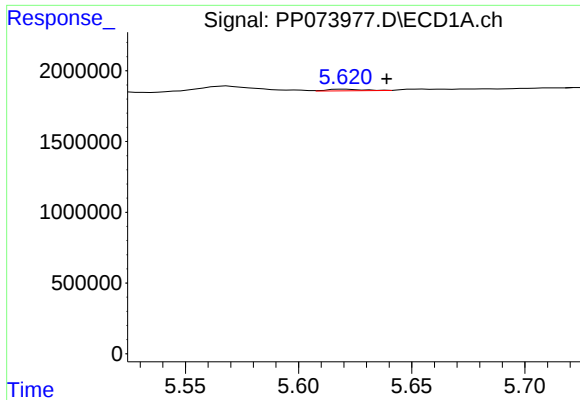

#3 AR-1016-1


R.T.: 5.620 min
Delta R.T.: -0.019 min
Response: 118969
Conc: 2.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

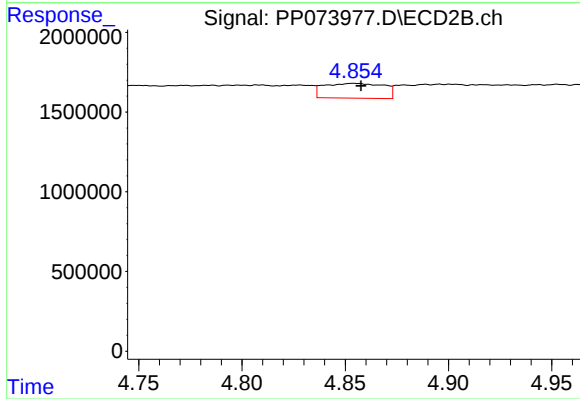


#3 AR-1016-1

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 1873750
Conc: 27.48 ng/ml

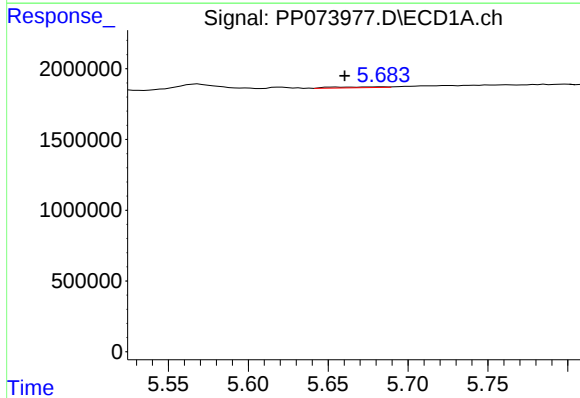


#4 AR-1016-2

R.T.: 5.684 min
Delta R.T.: 0.024 min
Response: 131961
Conc: 1.85 ng/ml

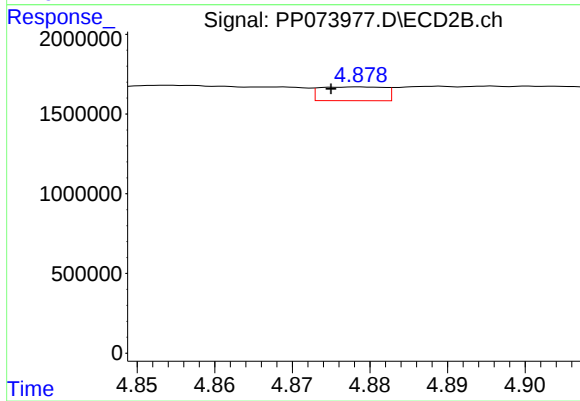

#4 AR-1016-2


R.T.: 4.879 min
Delta R.T.: 0.004 min
Response: 500141
Conc: 4.91 ng/ml

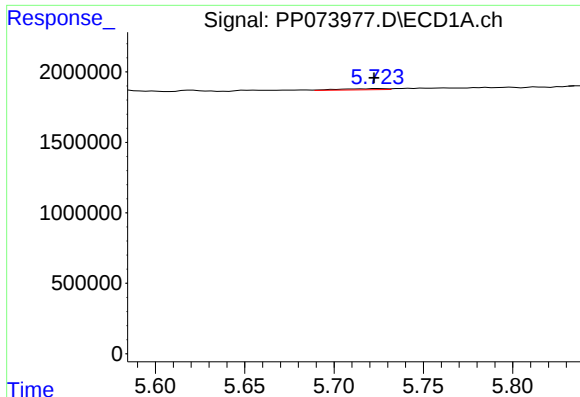

#5 AR-1016-3


R.T.: 5.725 min
Delta R.T.: 0.003 min
Response: 149515
Conc: 3.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

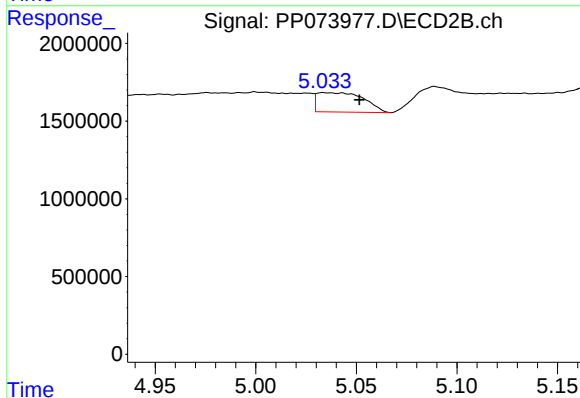


#5 AR-1016-3

R.T.: 5.034 min
Delta R.T.: -0.018 min
Response: 2014166
Conc: 37.23 ng/ml

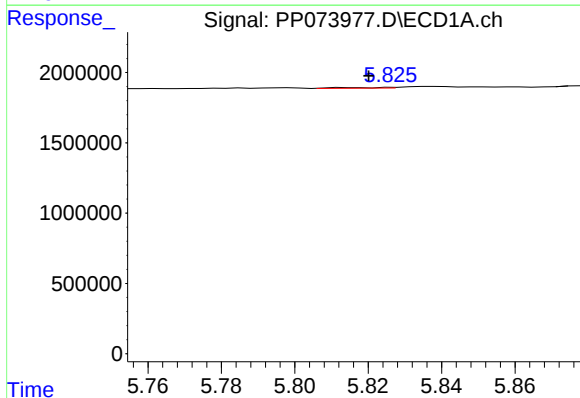


#6 AR-1016-4

R.T.: 5.813 min
Delta R.T.: -0.007 min
Response: 53441
Conc: 1.49 ng/ml

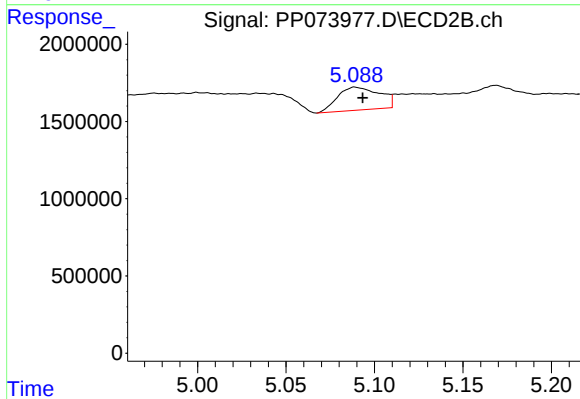

#6 AR-1016-4


R.T.: 5.089 min
Delta R.T.: -0.004 min
Response: 2443227
Conc: 55.68 ng/ml

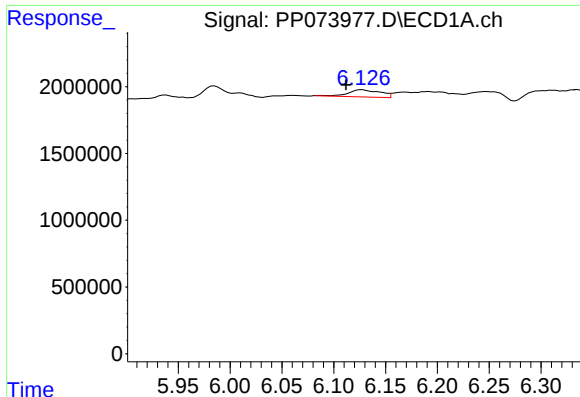

#7 AR-1016-5


R.T.: 6.128 min
Delta R.T.: 0.016 min
Response: 1137200
Conc: 36.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

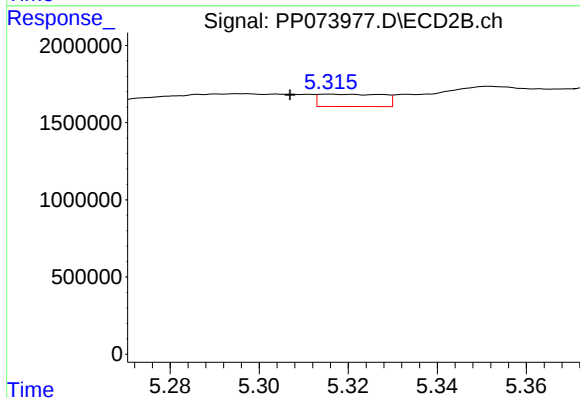


#7 AR-1016-5

R.T.: 5.316 min
Delta R.T.: 0.009 min
Response: 795586
Conc: 14.58 ng/ml

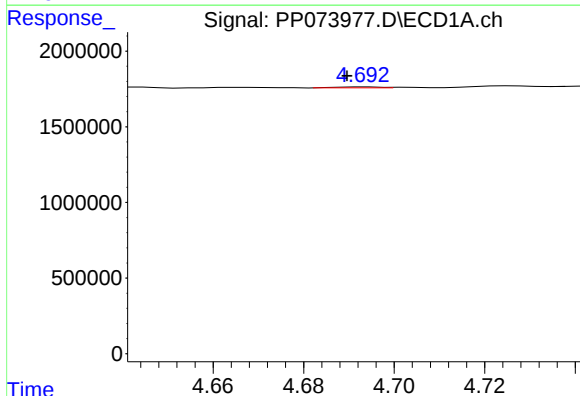


#8 AR-1221-1

R.T.: 4.694 min
Delta R.T.: 0.004 min
Response: 40362
Conc: 2.26 ng/ml

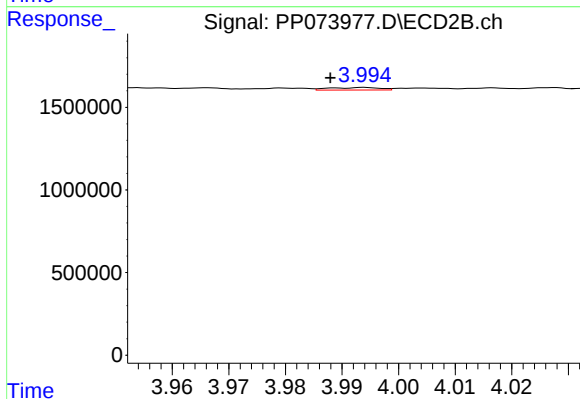

#8 AR-1221-1


R.T.: 3.994 min
Delta R.T.: 0.006 min
Response: 94155
Conc: 3.48 ng/ml

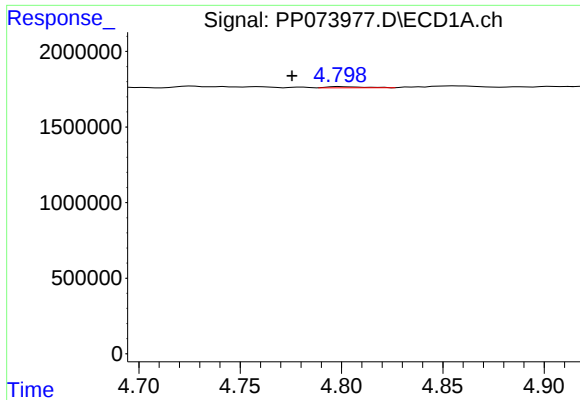

#9 AR-1221-2


R.T.: 4.799 min
Delta R.T.: 0.024 min
Response: 99033
Conc: 7.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

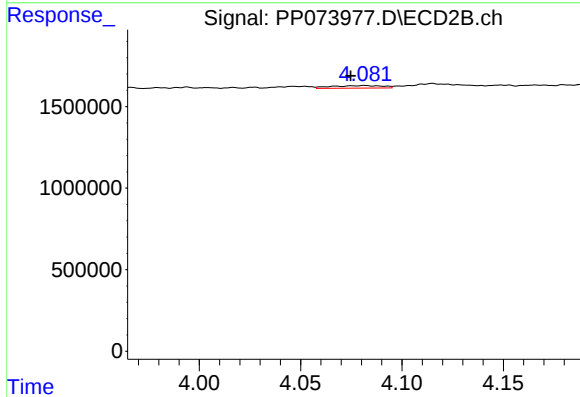


#9 AR-1221-2

R.T.: 4.082 min
Delta R.T.: 0.007 min
Response: 272200
Conc: 13.37 ng/ml

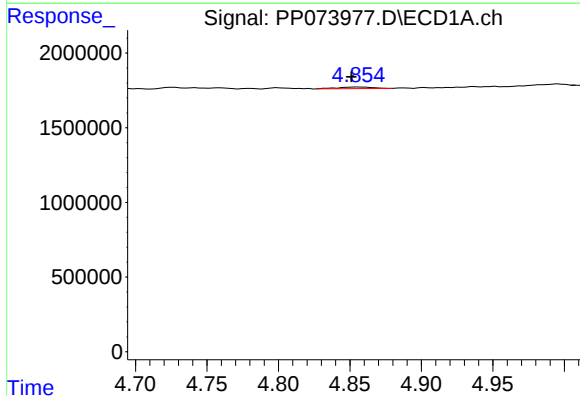


#10 AR-1221-3

R.T.: 4.855 min
Delta R.T.: 0.005 min
Response: 191235
Conc: 4.60 ng/ml

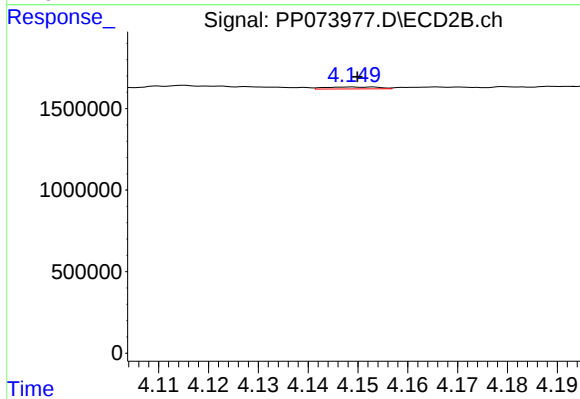

#10 AR-1221-3


R.T.: 4.149 min
Delta R.T.: -0.001 min
Response: 89995
Conc: 1.46 ng/ml

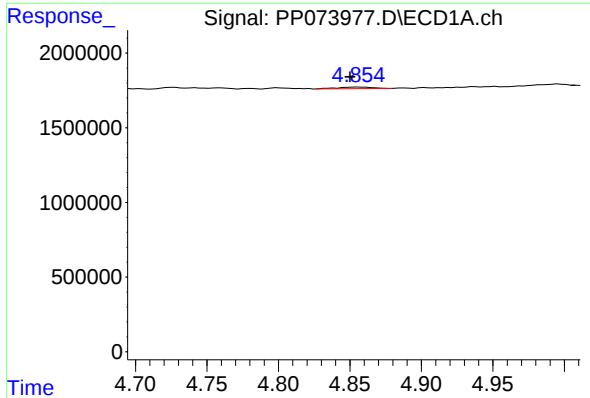

#11 AR-1232-1


R.T.: 4.855 min
Delta R.T.: 0.005 min
Response: 191235
Conc: 5.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

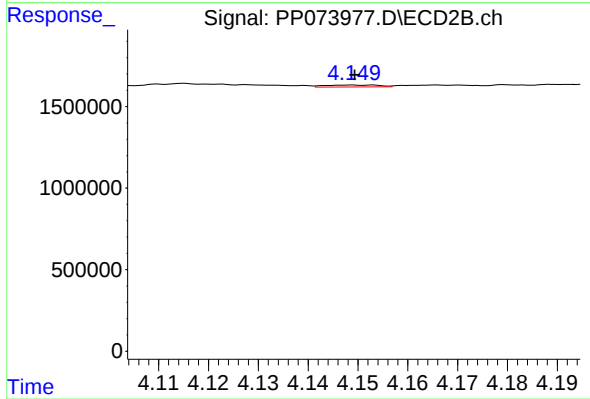


#11 AR-1232-1

R.T.: 4.149 min
Delta R.T.: 0.000 min
Response: 89995
Conc: 1.93 ng/ml

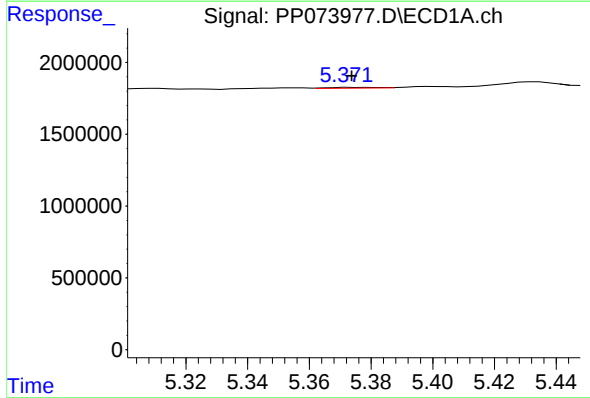


#12 AR-1232-2

R.T.: 5.373 min
Delta R.T.: 0.000 min
Response: 67456
Conc: 4.15 ng/ml

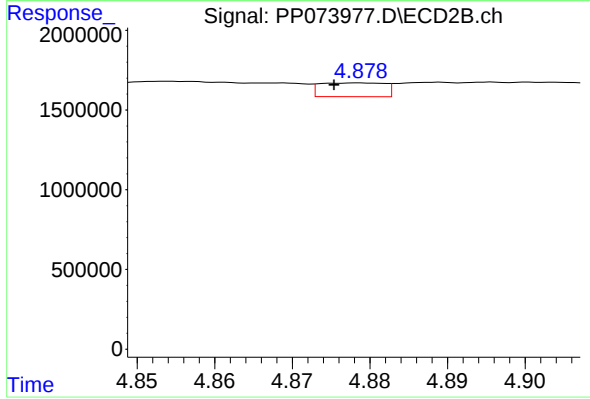

#12 AR-1232-2


R.T.: 4.879 min
Delta R.T.: 0.003 min
Response: 500141
Conc: 10.49 ng/ml

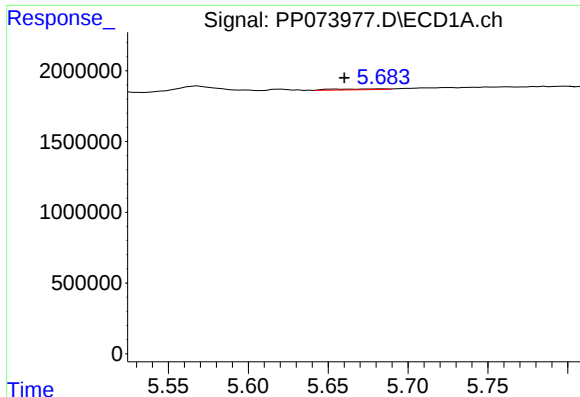

#13 AR-1232-3


R.T.: 5.684 min
Delta R.T.: 0.024 min
Response: 131961
Conc: 4.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

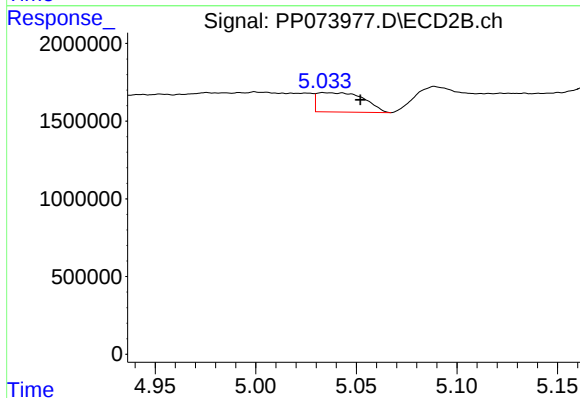


#13 AR-1232-3

R.T.: 5.034 min
Delta R.T.: -0.018 min
Response: 2014166
Conc: 80.47 ng/ml

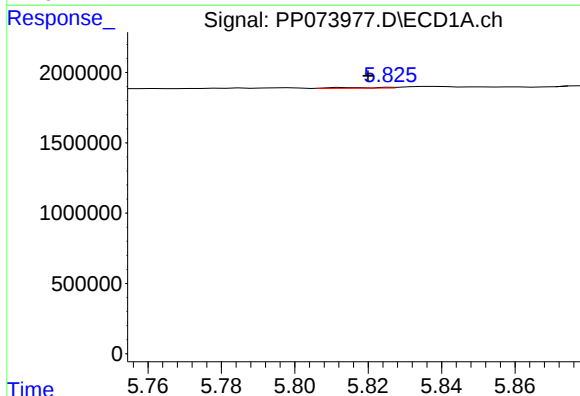


#14 AR-1232-4

R.T.: 5.813 min
Delta R.T.: -0.006 min
Response: 53441
Conc: 3.25 ng/ml

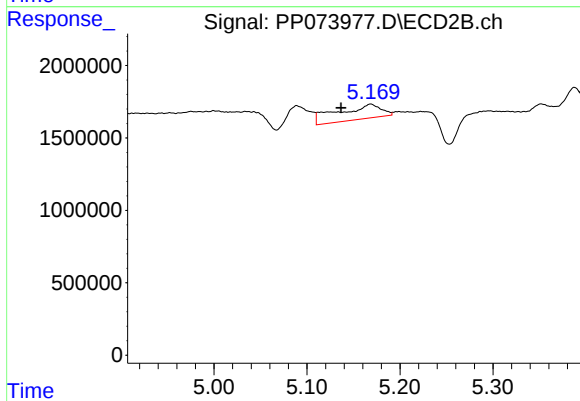

#14 AR-1232-4


R.T.: 5.169 min
Delta R.T.: 0.032 min
Response: 3293587
Conc: 152.08 ng/ml

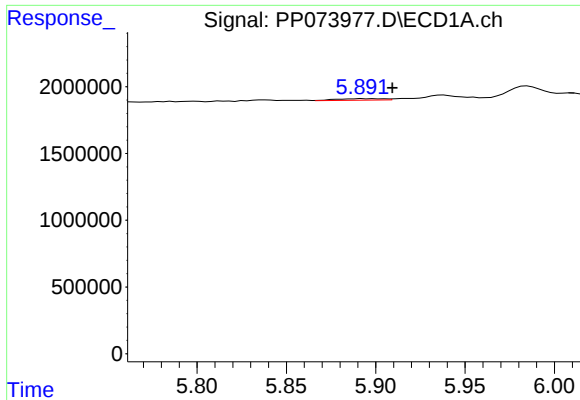

#15 AR-1232-5


R.T.: 5.893 min
Delta R.T.: -0.017 min
Response: 203382
Conc: 19.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

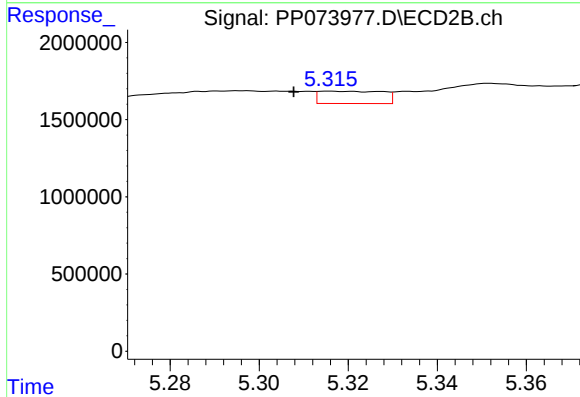


#15 AR-1232-5

R.T.: 5.316 min
Delta R.T.: 0.008 min
Response: 795586
Conc: 35.26 ng/ml

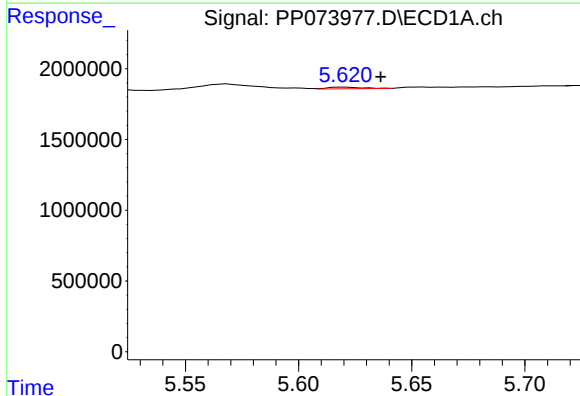


#16 AR-1242-1

R.T.: 5.620 min
Delta R.T.: -0.016 min
Response: 118969
Conc: 3.12 ng/ml

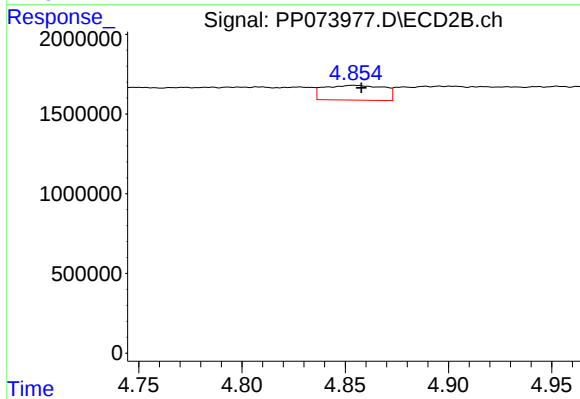

#16 AR-1242-1


R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 1873750
Conc: 32.44 ng/ml

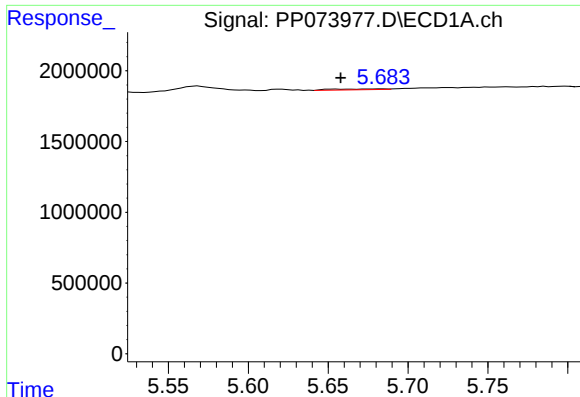

#17 AR-1242-2


R.T.: 5.684 min
Delta R.T.: 0.026 min
Response: 131961
Conc: 2.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

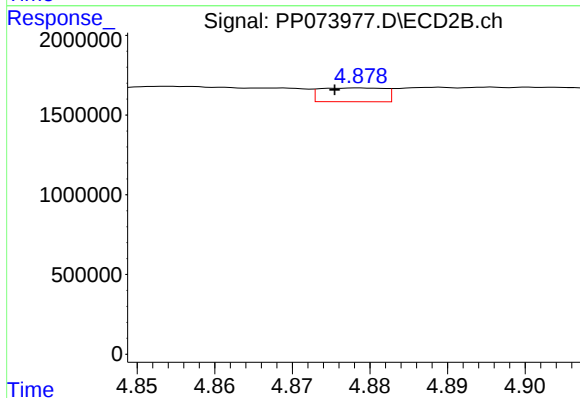


#17 AR-1242-2

R.T.: 4.879 min
Delta R.T.: 0.003 min
Response: 500141
Conc: 5.79 ng/ml

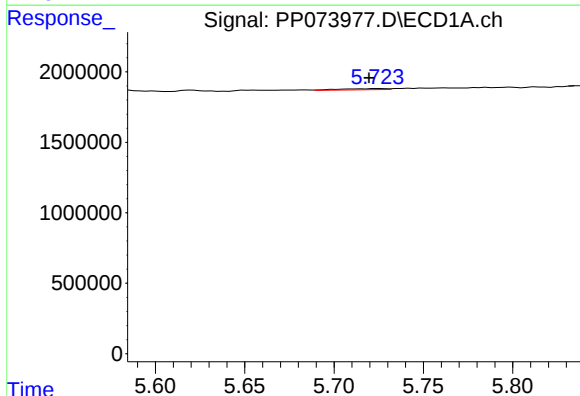


#18 AR-1242-3

R.T.: 5.725 min
Delta R.T.: 0.006 min
Response: 149515
Conc: 4.08 ng/ml

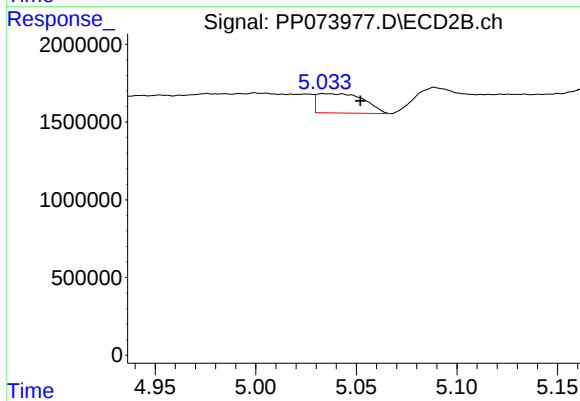

#18 AR-1242-3


R.T.: 5.034 min
Delta R.T.: -0.018 min
Response: 2014166
Conc: 43.84 ng/ml

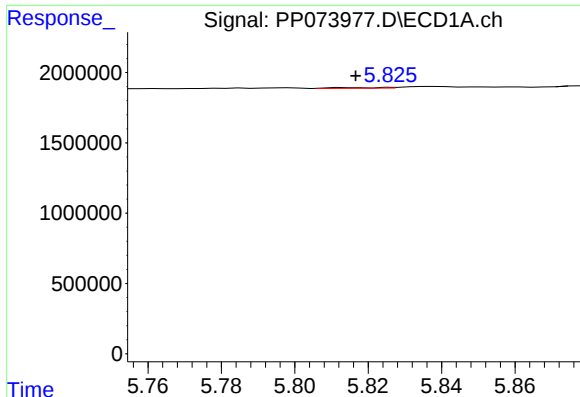

#19 AR-1242-4


R.T.: 5.813 min
Delta R.T.: -0.003 min
Response: 53441
Conc: 1.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

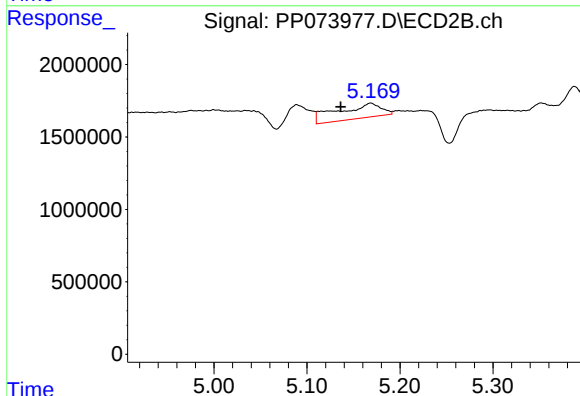


#19 AR-1242-4

R.T.: 5.169 min
Delta R.T.: 0.032 min
Response: 3293587
Conc: 74.41 ng/ml

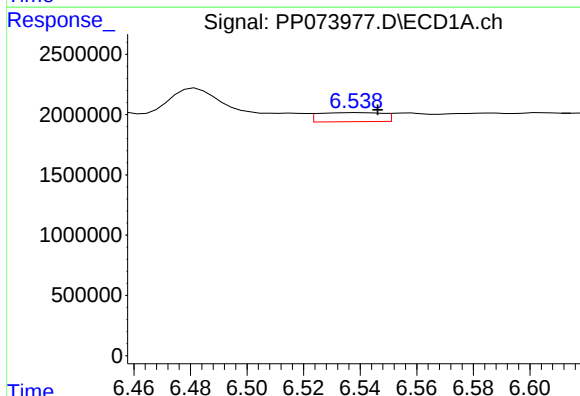


#20 AR-1242-5

R.T.: 6.539 min
Delta R.T.: -0.007 min
Response: 1184465
Conc: 36.18 ng/ml

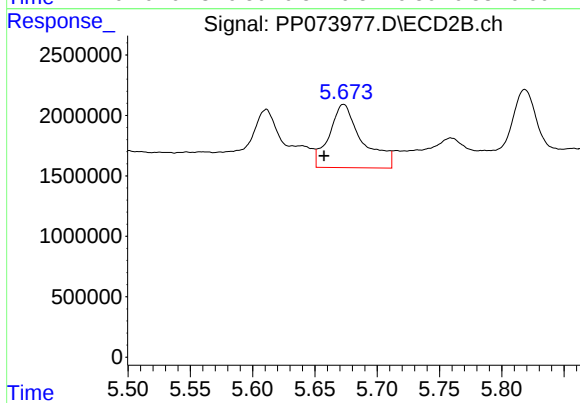

#20 AR-1242-5


R.T.: 5.673 min
Delta R.T.: 0.016 min
Response: 9669280
Conc: 175.03 ng/ml

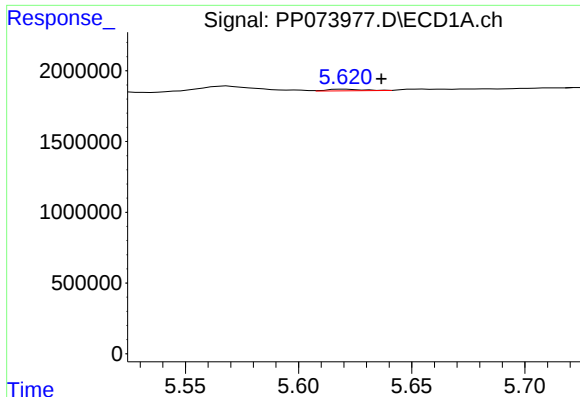

#21 AR-1248-1


R.T.: 5.620 min
Delta R.T.: -0.016 min
Response: 118969
Conc: 3.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

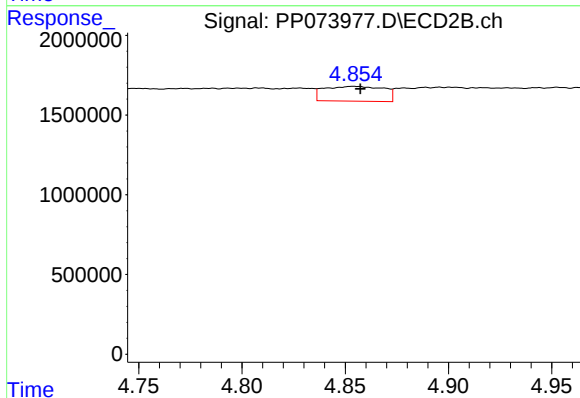


#21 AR-1248-1

R.T.: 4.854 min
Delta R.T.: -0.003 min
Response: 1873750
Conc: 41.74 ng/ml

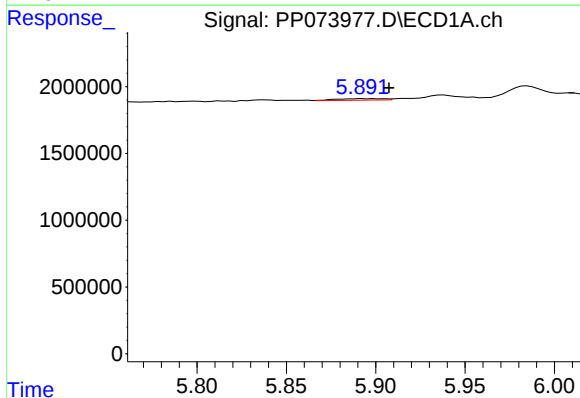


#22 AR-1248-2

R.T.: 5.893 min
Delta R.T.: -0.015 min
Response: 203382
Conc: 5.09 ng/ml

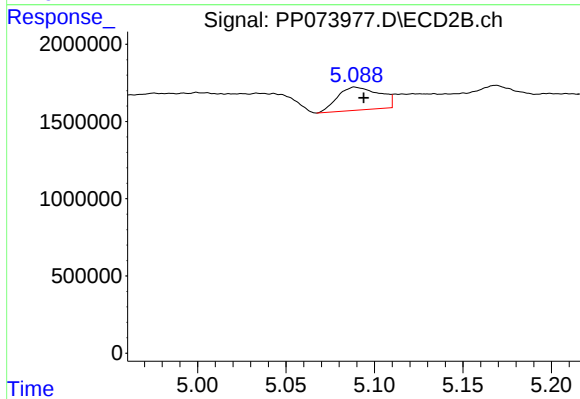

#22 AR-1248-2


R.T.: 5.089 min
Delta R.T.: -0.005 min
Response: 2443227
Conc: 39.70 ng/ml

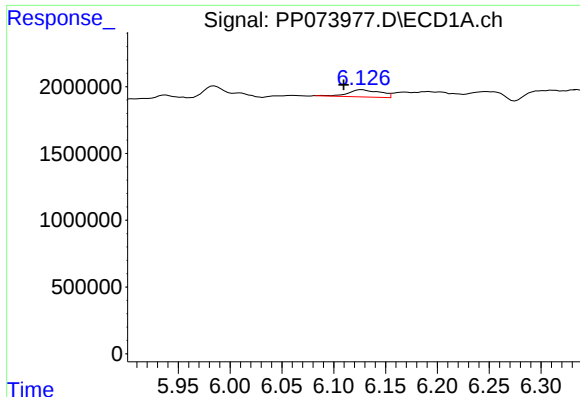

#23 AR-1248-3


R.T.: 6.128 min
Delta R.T.: 0.018 min
Response: 1137200
Conc: 25.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

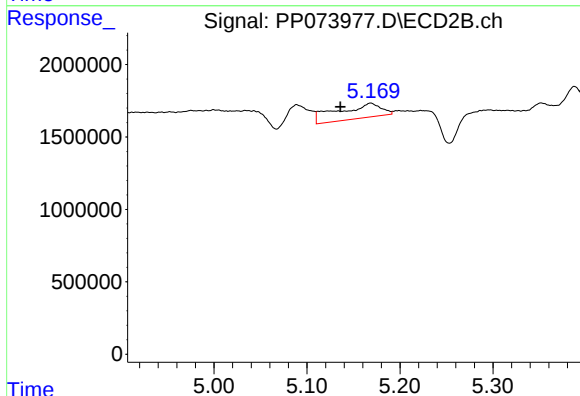


#23 AR-1248-3

R.T.: 5.169 min
Delta R.T.: 0.033 min
Response: 3293587
Conc: 51.41 ng/ml

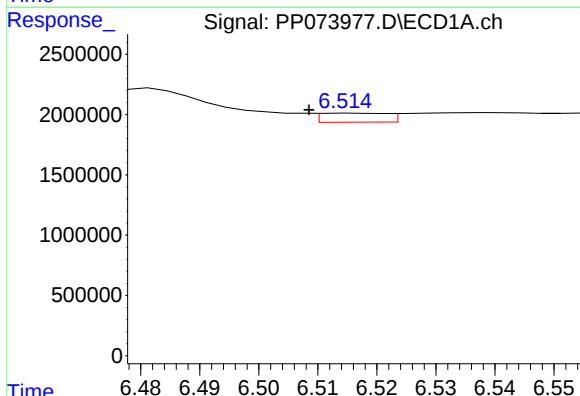


#24 AR-1248-4

R.T.: 6.516 min
Delta R.T.: 0.007 min
Response: 585082
Conc: 10.62 ng/ml

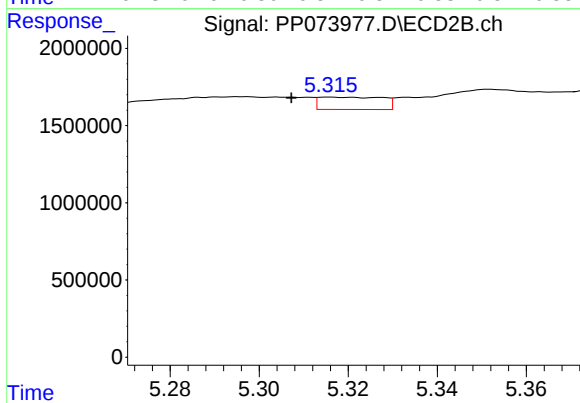

#24 AR-1248-4


R.T.: 5.316 min
Delta R.T.: 0.008 min
Response: 795586
Conc: 10.55 ng/ml

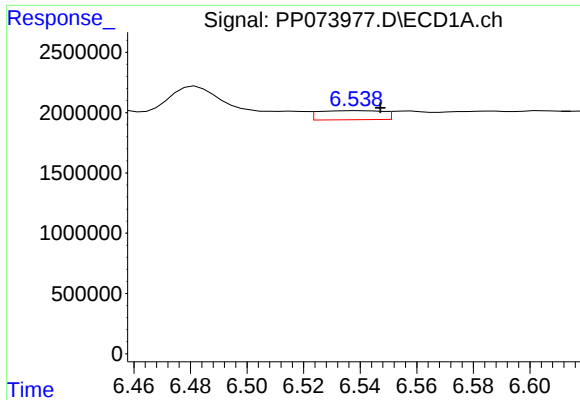

#25 AR-1248-5


R.T.: 6.539 min
Delta R.T.: -0.008 min
Response: 1184465
Conc: 22.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

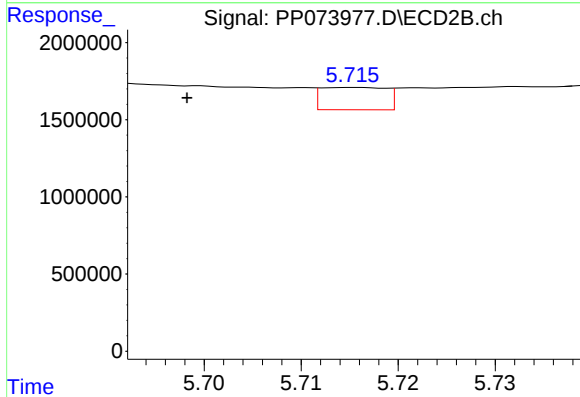


#25 AR-1248-5

R.T.: 5.715 min
Delta R.T.: 0.017 min
Response: 677697
Conc: 9.09 ng/ml

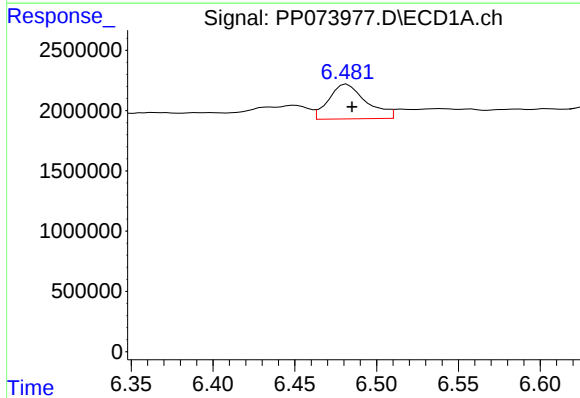


#26 AR-1254-1

R.T.: 6.482 min
Delta R.T.: -0.003 min
Response: 4584386
Conc: 85.55 ng/ml

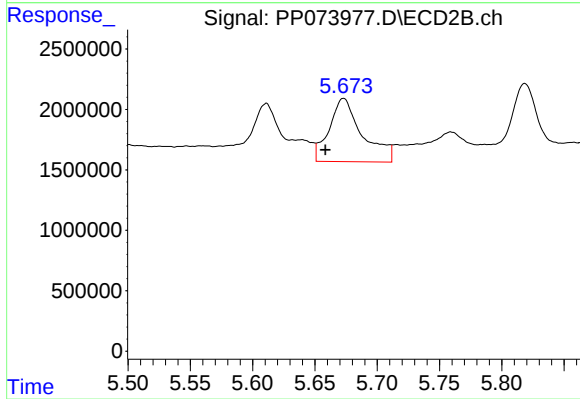

#26 AR-1254-1


R.T.: 5.673 min
Delta R.T.: 0.015 min
Response: 9669280
Conc: 83.33 ng/ml

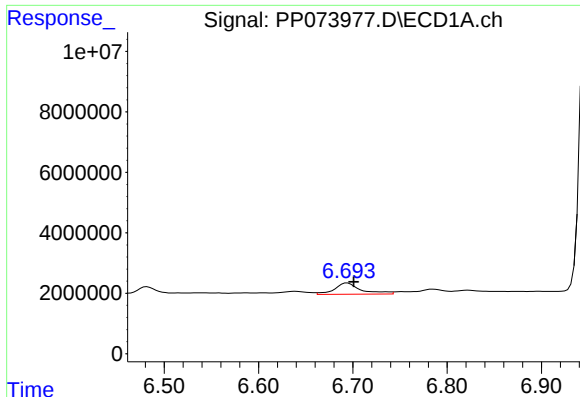

#27 AR-1254-2


R.T.: 6.694 min
Delta R.T.: -0.007 min
Response: 7294143
Conc: 87.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

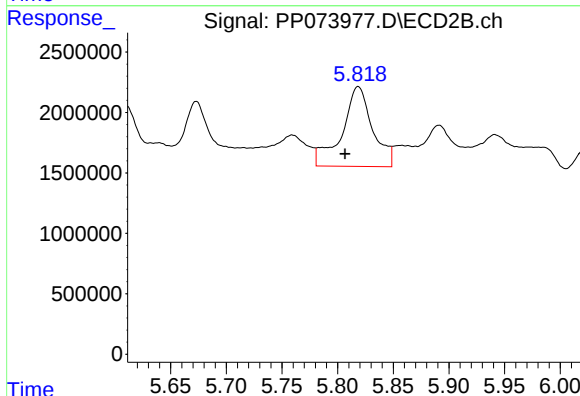


#27 AR-1254-2

R.T.: 5.818 min
Delta R.T.: 0.012 min
Response: 12609767
Conc: 125.32 ng/ml

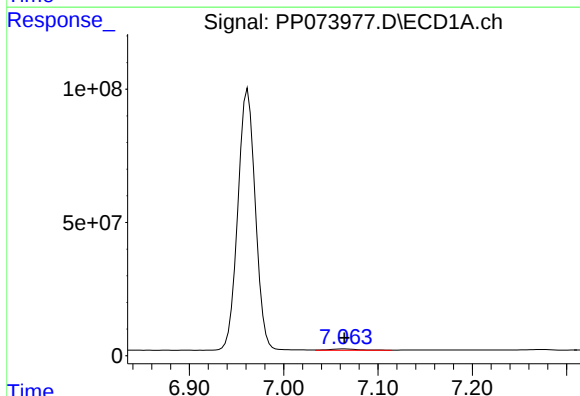


#28 AR-1254-3

R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 11956841
Conc: 135.36 ng/ml

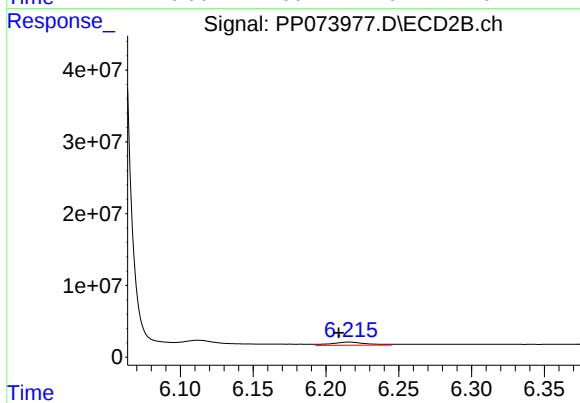

#28 AR-1254-3


R.T.: 6.216 min
Delta R.T.: 0.007 min
Response: 7518519
Conc: 48.68 ng/ml

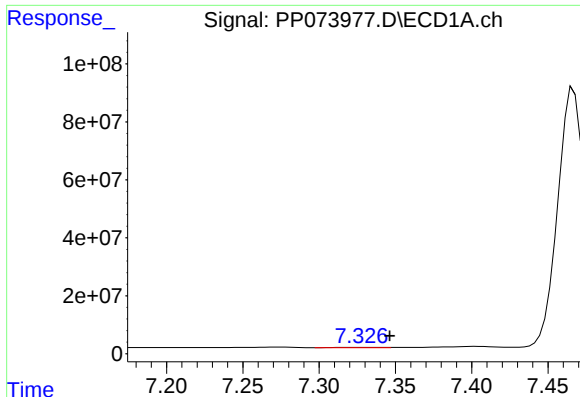

#29 AR-1254-4


R.T.: 7.327 min
Delta R.T.: -0.019 min
Response: 2416834
Conc: 30.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

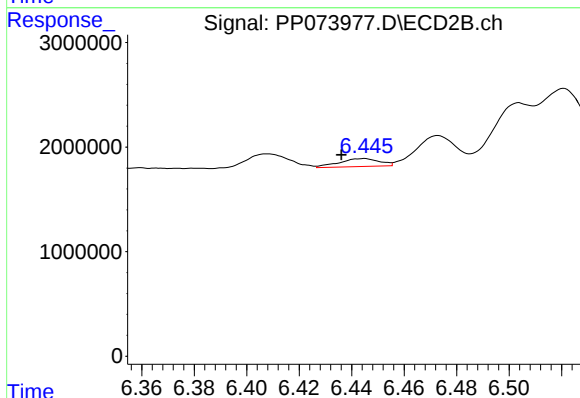


#29 AR-1254-4

R.T.: 6.444 min
Delta R.T.: 0.008 min
Response: 817685
Conc: 8.65 ng/ml

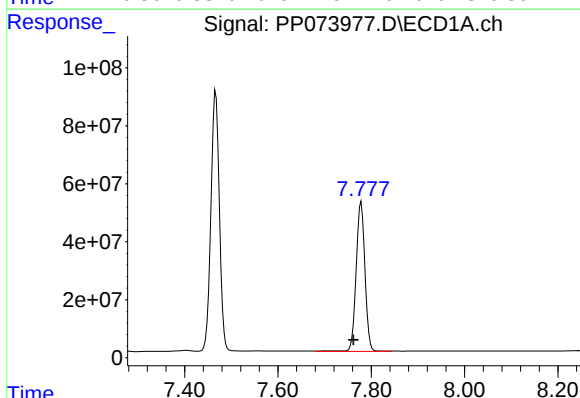


#30 AR-1254-5

R.T.: 7.778 min
Delta R.T.: 0.016 min
Response: 679879622
Conc: 9227.49 ng/ml

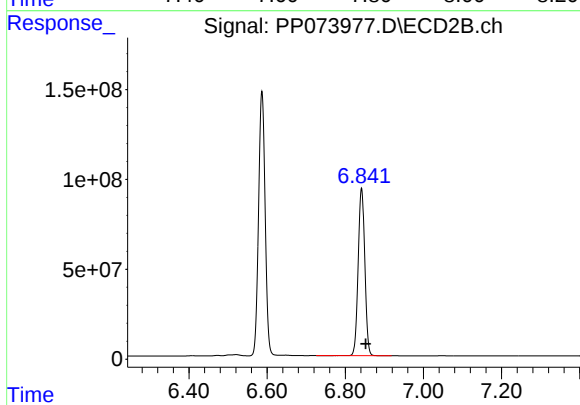

#30 AR-1254-5


R.T.: 6.842 min
Delta R.T.: -0.011 min
Response: 1100594272
Conc: 8247.56 ng/ml

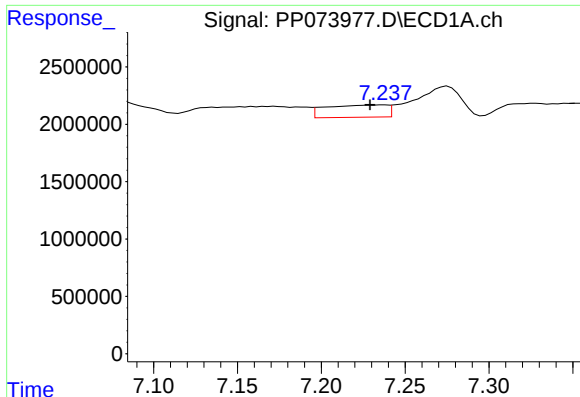

#31 AR-1260-1


R.T.: 7.238 min
Delta R.T.: 0.009 min
Response: 2722453
Conc: 46.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

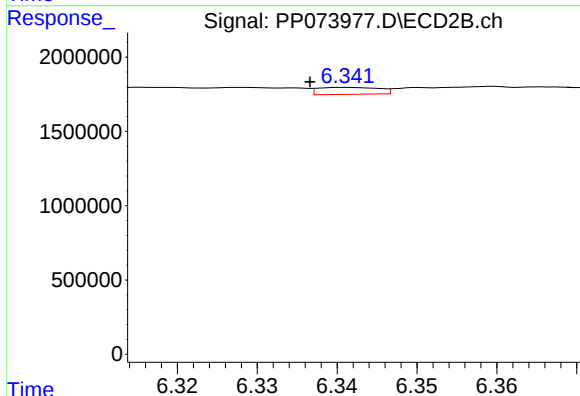


#31 AR-1260-1

R.T.: 6.341 min
Delta R.T.: 0.005 min
Response: 248498
Conc: 2.55 ng/ml

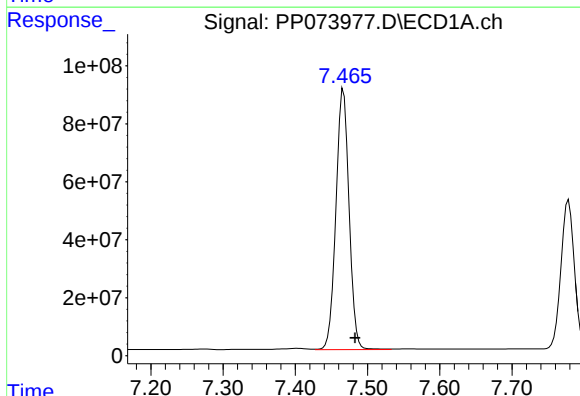


#32 AR-1260-2

R.T.: 7.467 min
Delta R.T.: -0.016 min
Response: 1138857644
Conc: 11882.92 ng/ml

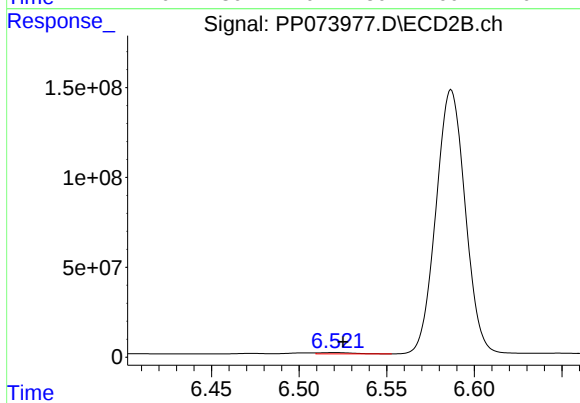

#32 AR-1260-2


R.T.: 6.521 min
Delta R.T.: -0.004 min
Response: 8972359
Conc: 73.04 ng/ml

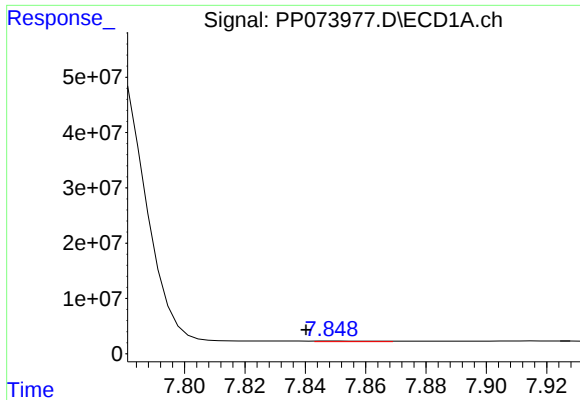

#33 AR-1260-3


R.T.: 7.849 min
Delta R.T.: 0.009 min
Response: 1435228
Conc: 19.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

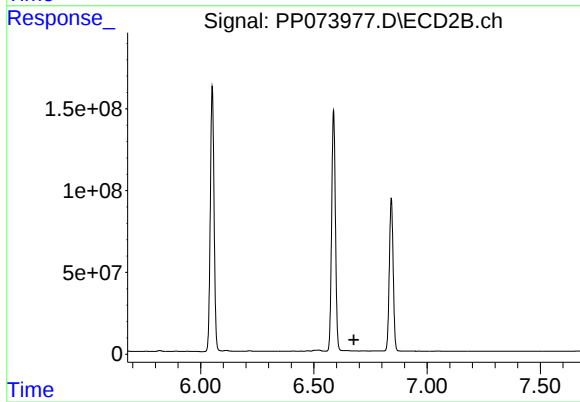


#33 AR-1260-3

R.T.: 6.648 min
Delta R.T.: -0.029 min
Response: -1305051
Conc: N.D.

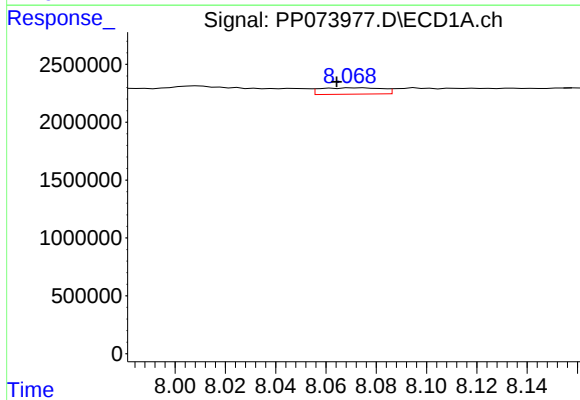


#34 AR-1260-4

R.T.: 8.070 min
Delta R.T.: 0.006 min
Response: 949027
Conc: 14.53 ng/ml

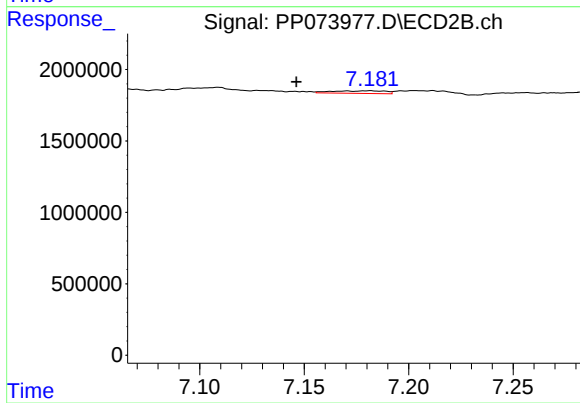

#34 AR-1260-4


R.T.: 7.182 min
Delta R.T.: 0.035 min
Response: 326962
Conc: 3.66 ng/ml

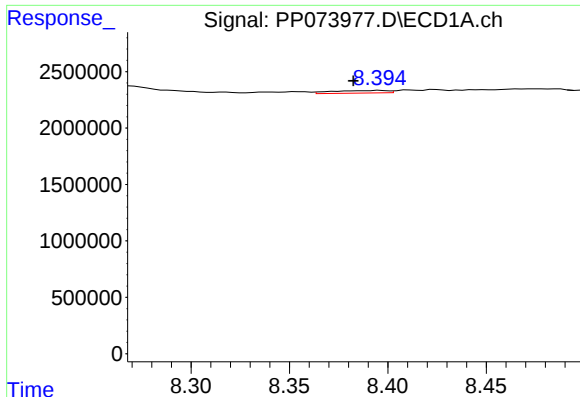

#35 AR-1260-5


R.T.: 8.396 min
Delta R.T.: 0.014 min
Response: 433468
Conc: 2.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

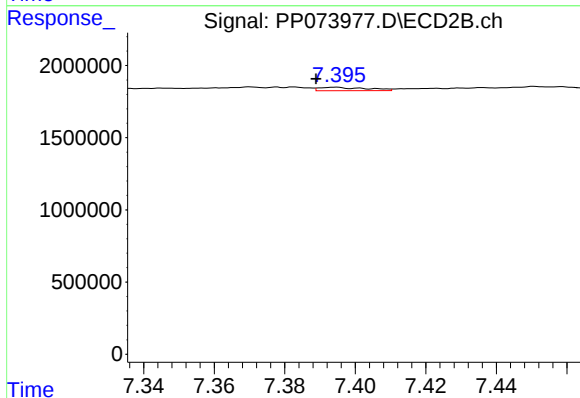


#35 AR-1260-5

R.T.: 7.394 min
Delta R.T.: 0.005 min
Response: 220923
Conc: 0.98 ng/ml

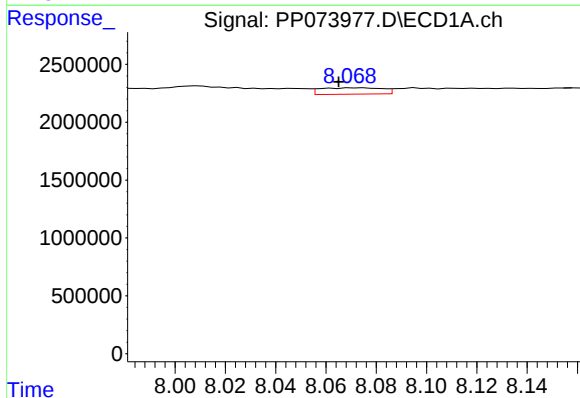


#36 AR-1262-1

R.T.: 8.070 min
Delta R.T.: 0.005 min
Response: 949027
Conc: 10.90 ng/ml

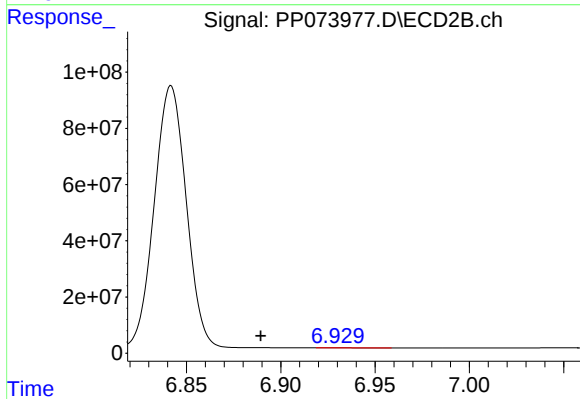

#36 AR-1262-1


R.T.: 6.929 min
Delta R.T.: 0.039 min
Response: 161047
Conc: 1.09 ng/ml

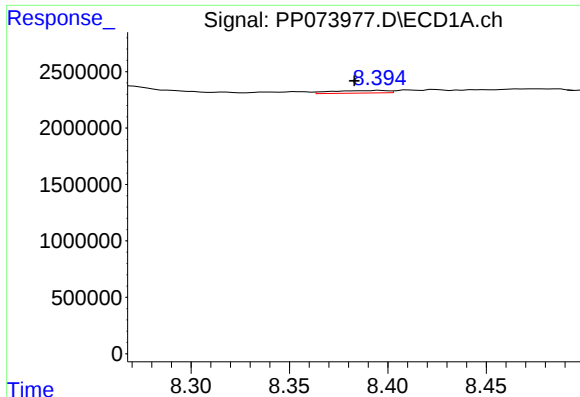

#37 AR-1262-2


R.T.: 8.396 min
Delta R.T.: 0.013 min
Response: 433468
Conc: 2.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

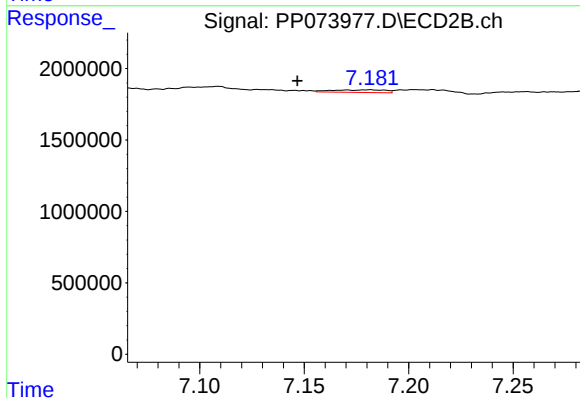


#37 AR-1262-2

R.T.: 7.182 min
Delta R.T.: 0.035 min
Response: 326962
Conc: 2.56 ng/ml

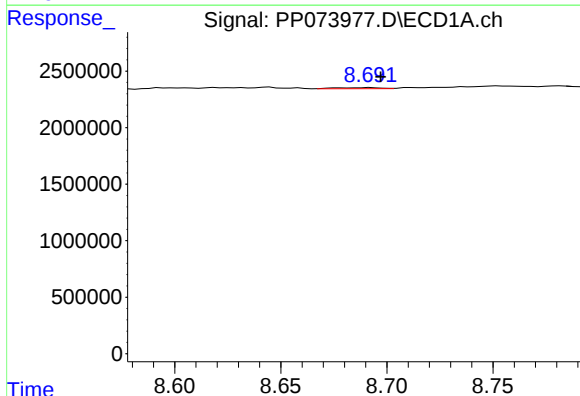


#38 AR-1262-3

R.T.: 8.692 min
Delta R.T.: -0.005 min
Response: 130849
Conc: 1.04 ng/ml

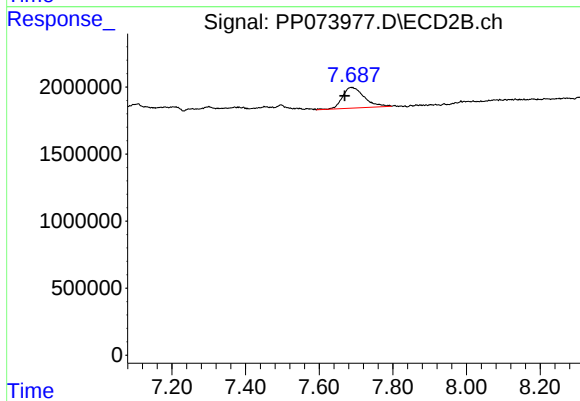

#38 AR-1262-3


R.T.: 7.686 min
Delta R.T.: 0.018 min
Response: 6329246
Conc: 55.51 ng/ml

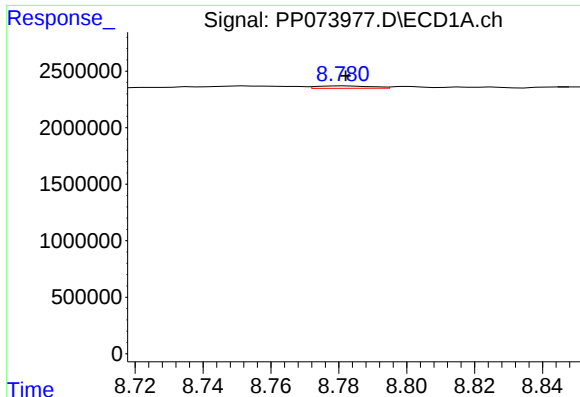

#39 AR-1262-4


R.T.: 8.782 min
Delta R.T.: 0.000 min
Response: 238231
Conc: 2.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

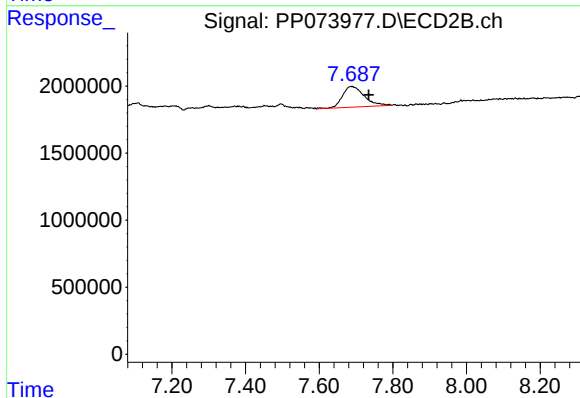


#39 AR-1262-4

R.T.: 7.686 min
Delta R.T.: -0.048 min
Response: 6329246
Conc: 34.39 ng/ml

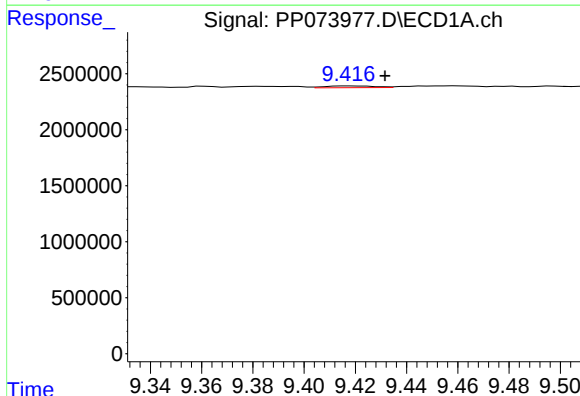


#40 AR-1262-5

R.T.: 9.418 min
Delta R.T.: -0.014 min
Response: 211877
Conc: 3.34 ng/ml

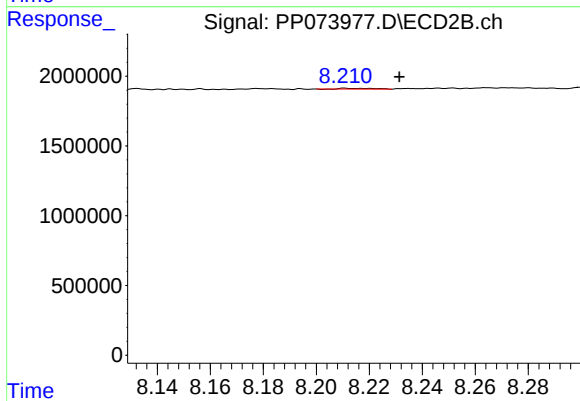

#40 AR-1262-5


R.T.: 8.211 min
Delta R.T.: -0.020 min
Response: 42205
Conc: 0.50 ng/ml

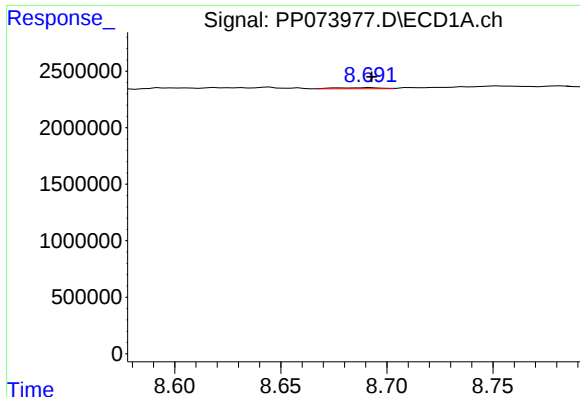

#41 AR-1268-1


R.T.: 8.692 min
Delta R.T.: 0.000 min
Response: 130849
Conc: 0.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

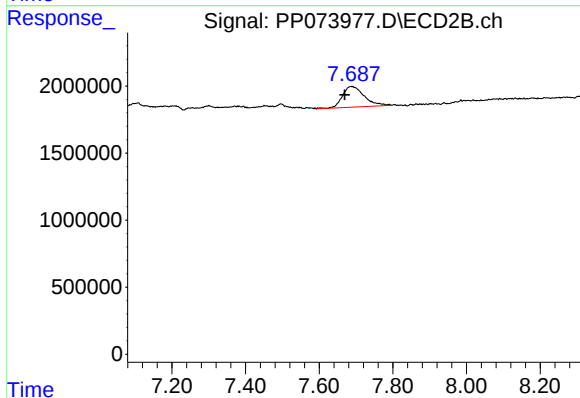


#41 AR-1268-1

R.T.: 7.686 min
Delta R.T.: 0.018 min
Response: 6329246
Conc: 20.59 ng/ml

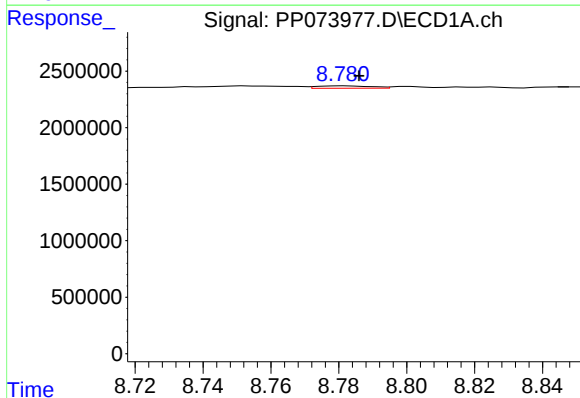


#42 AR-1268-2

R.T.: 8.782 min
Delta R.T.: -0.004 min
Response: 238231
Conc: 1.25 ng/ml

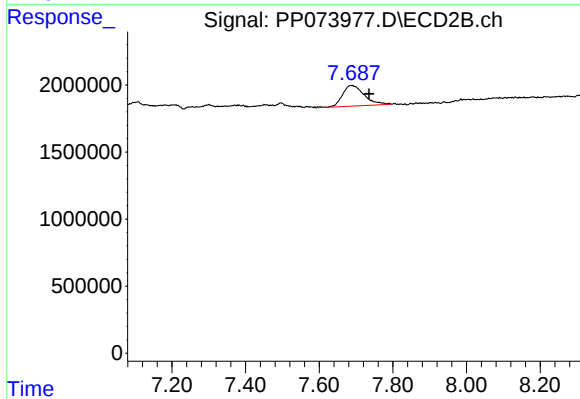

#42 AR-1268-2


R.T.: 7.686 min
Delta R.T.: -0.049 min
Response: 6329246
Conc: 23.82 ng/ml

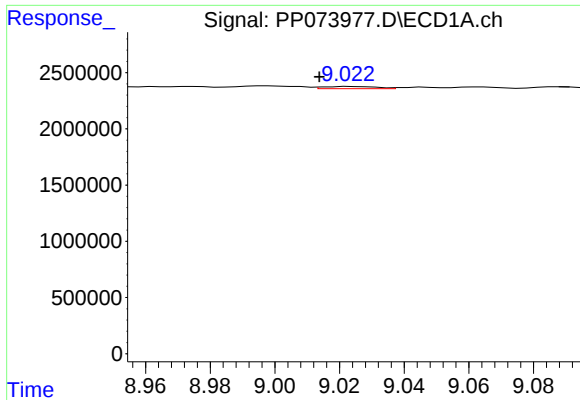

#43 AR-1268-3


R.T.: 9.024 min
Delta R.T.: 0.010 min
Response: 228613
Conc: 1.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

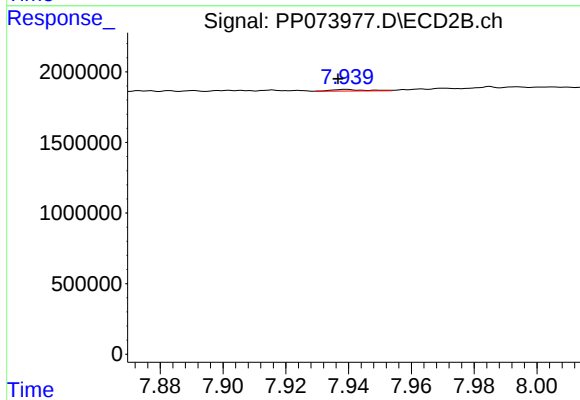


#43 AR-1268-3

R.T.: 7.939 min
Delta R.T.: 0.002 min
Response: 77748
Conc: 0.34 ng/ml

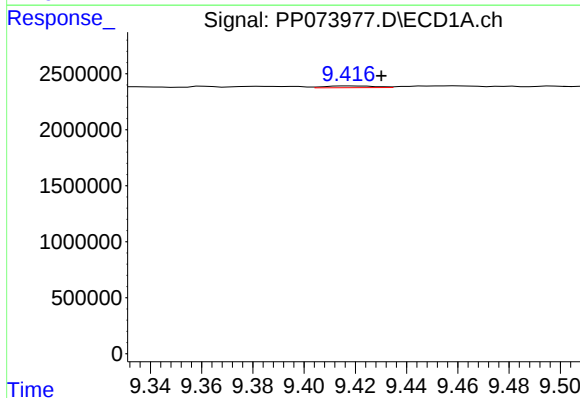


#44 AR-1268-4

R.T.: 9.418 min
Delta R.T.: -0.013 min
Response: 211877
Conc: 3.05 ng/ml

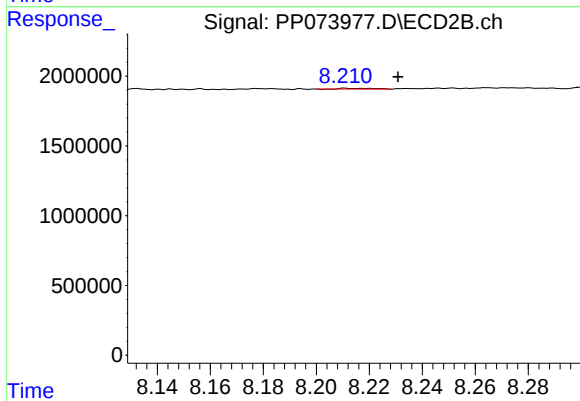

#44 AR-1268-4


R.T.: 8.211 min
Delta R.T.: -0.020 min
Response: 42205
Conc: 0.45 ng/ml

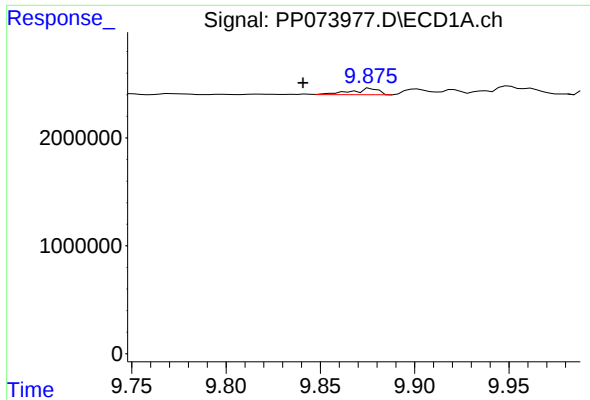

#45 AR-1268-5

R.T.: 9.877 min
Delta R.T.: 0.036 min
Response: 602853
Conc: 1.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

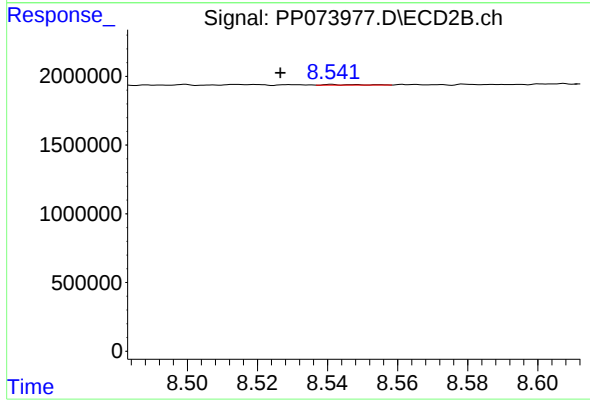

#45 AR-1268-5

R.T.: 8.542 min
Delta R.T.: 0.015 min
Response: 29138
Conc: 0.05 ng/ml