

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 14:13
 Operator : YP\AJ
 Sample : Q2634-01 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 J2315

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:51:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.479	3.773	1621321	2074709	1.184m	1.126m
2) SA Decachlor...	10.163	8.771	1585015	2111252	1.453	1.596

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
Data File : PP073986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 14:13
Operator : YP\AJ
Sample : Q2634-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
J2315


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:51:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

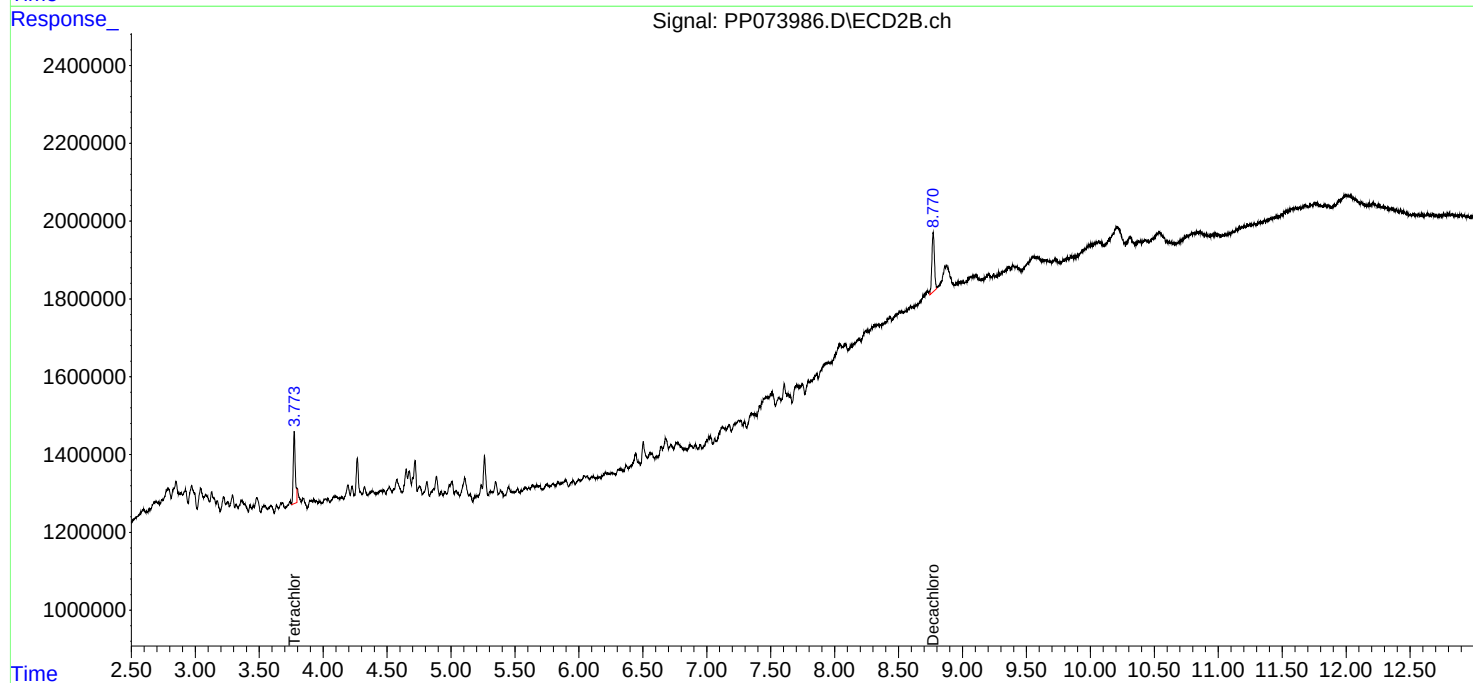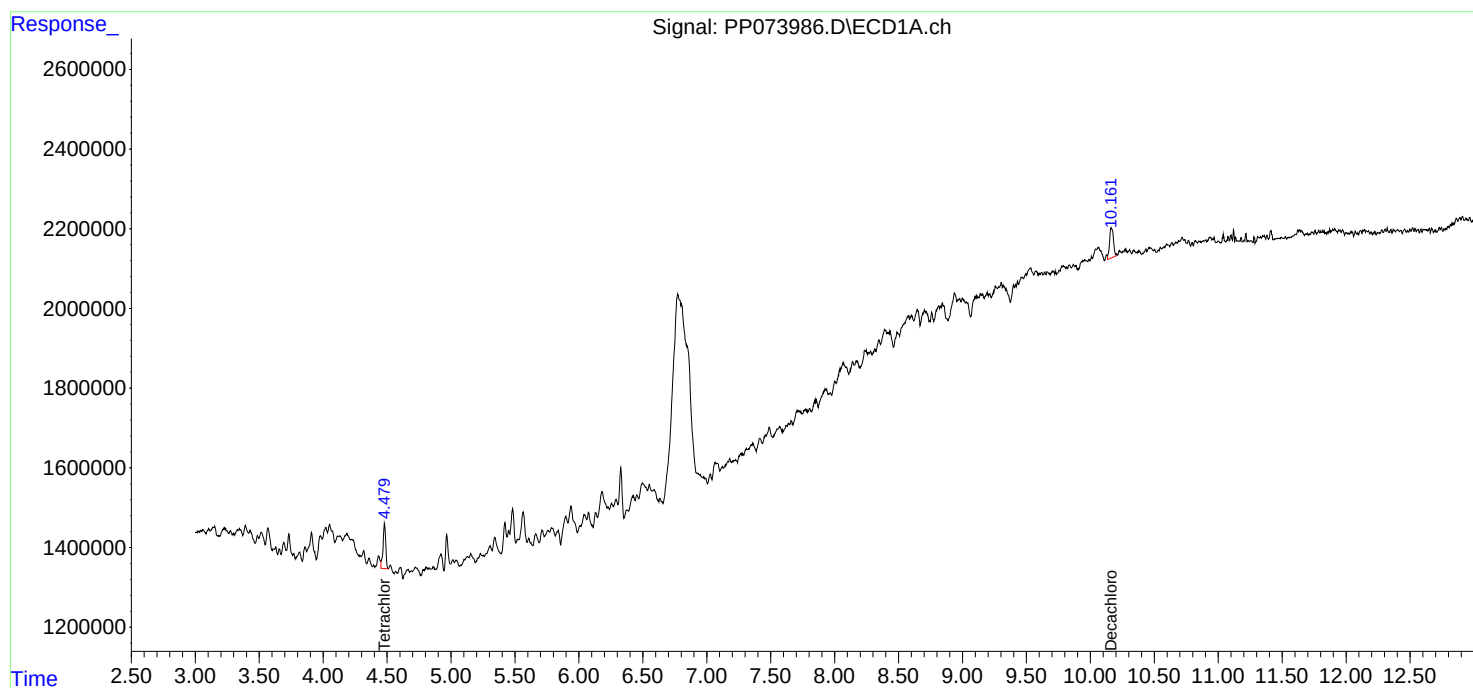

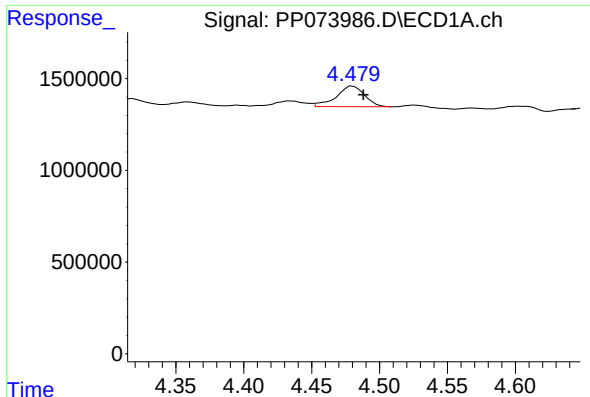


#1 Tetrachloro-m-xylene

R.T.: 4.479 min
Delta R.T.: -0.009 min
Response: 1621321
Conc: 1.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
J2315


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

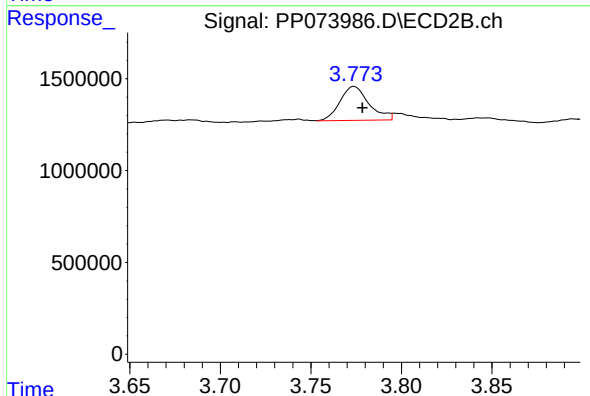


#1 Tetrachloro-m-xylene

R.T.: 3.773 min
Delta R.T.: -0.005 min
Response: 2074709
Conc: 1.13 ng/ml m

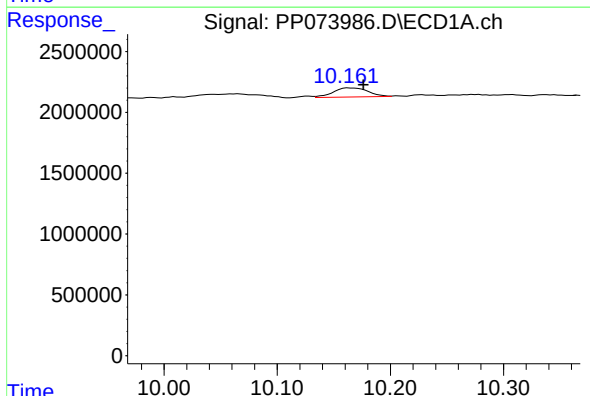

#2 Decachlorobiphenyl

R.T.: 10.163 min
Delta R.T.: -0.013 min
Response: 1585015
Conc: 1.45 ng/ml

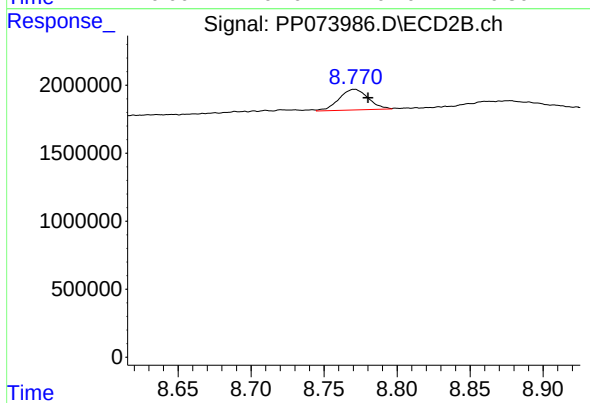

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.009 min
Response: 2111252
Conc: 1.60 ng/ml