

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
 Data File : PP037545.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2021 9:47
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 14:32:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
20)	L4	AR-1242-5	7.255	6.091f	7992	108174	7.685 158.921 #
24)	L5	AR-1248-4	7.232	0.000	14626	0	7.738 N.D. #
25)	L5	AR-1248-5	7.255	6.091f	7992	108174	4.270 101.979 #
26)	L6	AR-1254-1	7.194	6.091f	265940	108174	148.033 72.866 #
28)	L6	AR-1254-3	7.816f	0.000	60314	0	19.563 N.D. #
29)	L6	AR-1254-4	8.071f	0.000	13688	0	6.026 N.D. #
32)	L7	AR-1260-2	8.206f	0.000	27301	0	9.814 N.D. #
38)	L8	AR-1262-3	0.000	8.143f	0	83705	N.D. 59.451 #
41)	L9	AR-1268-1	0.000	8.143f	0	83705	N.D. 21.004 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
Data File : PP037545.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2021 9:47
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 14:32:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

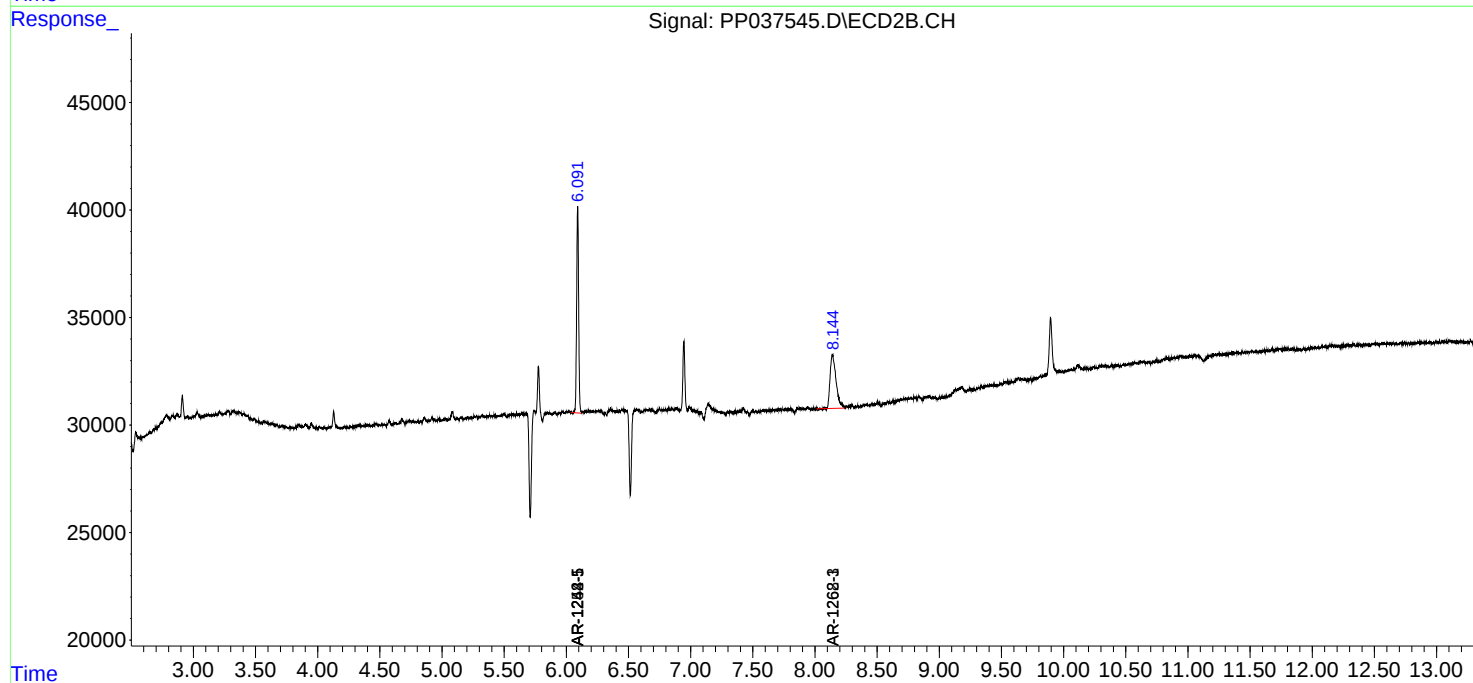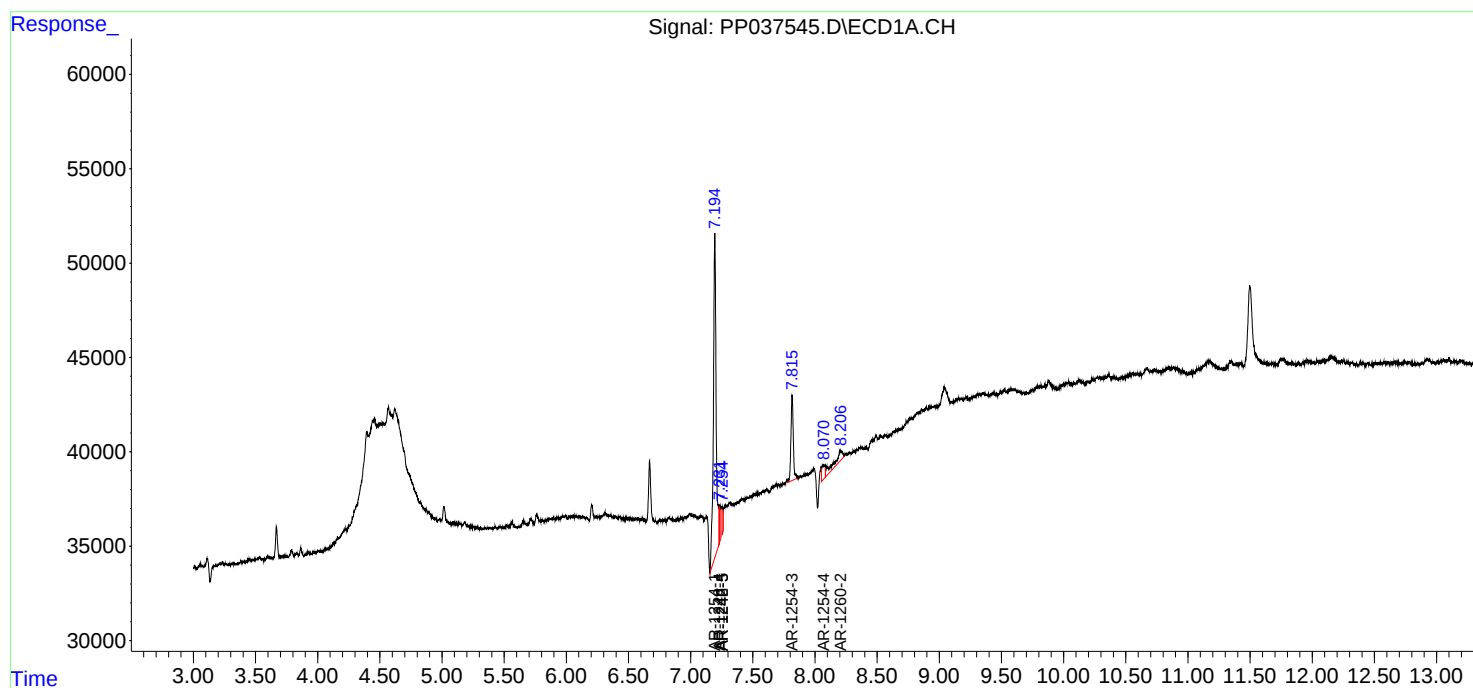


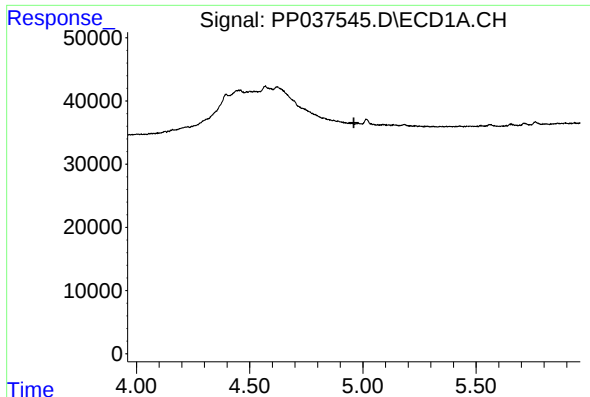

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

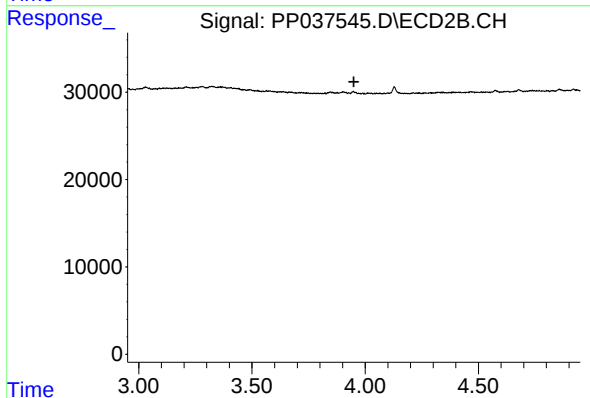


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.950 min
Response: 0
Conc: N.D.

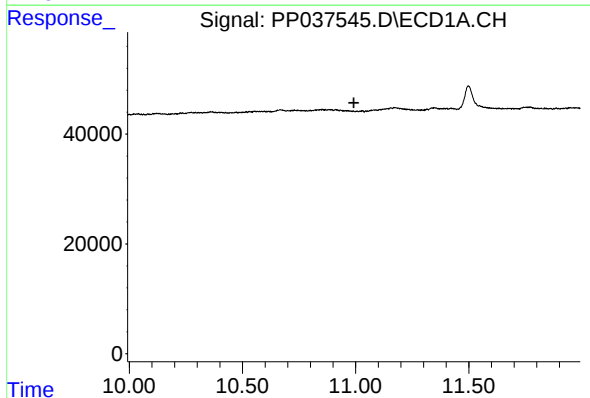


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 10.992 min
Response: 0
Conc: N.D.

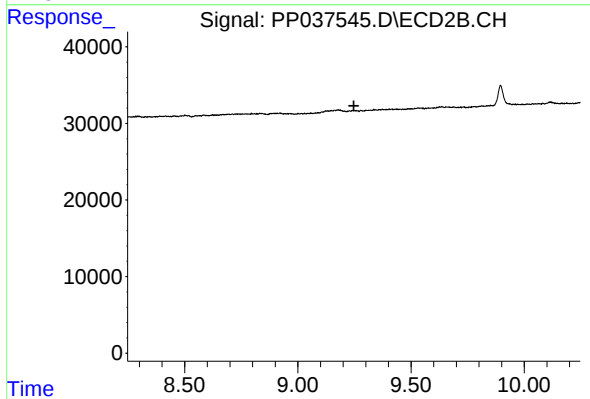

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T.: 9.247 min
Response: 0
Conc: N.D.

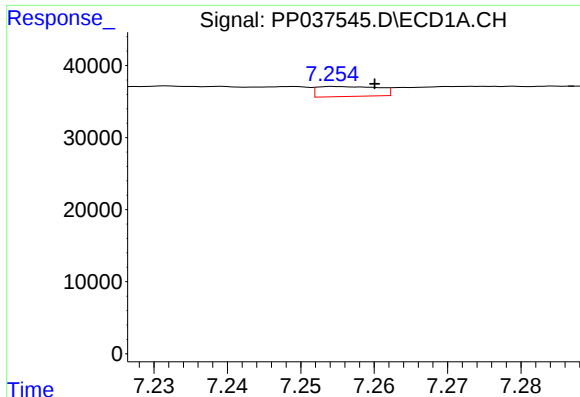

#20 AR-1242-5


R.T.: 7.255 min
Delta R.T.: -0.005 min
Response: 7992
Conc: 7.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

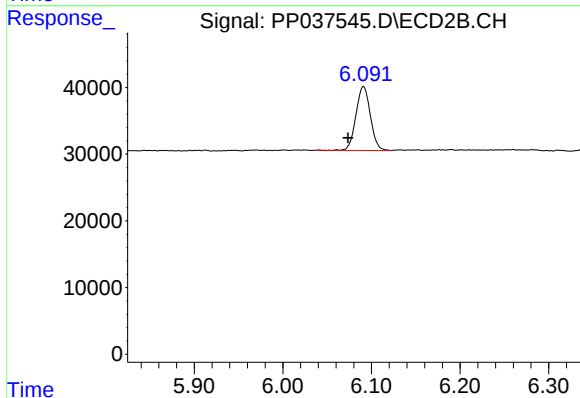


#20 AR-1242-5

R.T.: 6.091 min
Delta R.T.: 0.018 min
Response: 108174
Conc: 158.92 ng/ml

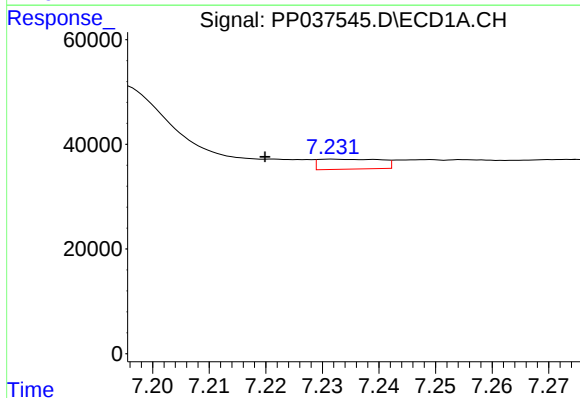


#24 AR-1248-4

R.T.: 7.232 min
Delta R.T.: 0.012 min
Response: 14626
Conc: 7.74 ng/ml

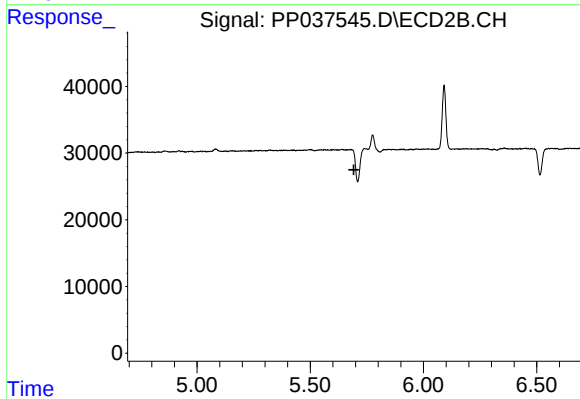

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.692 min
Response: 0
Conc: N.D.

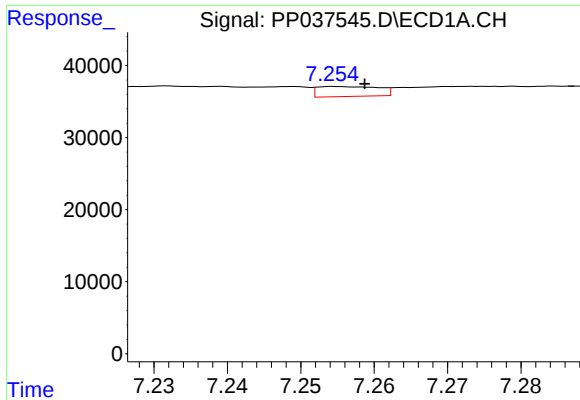

#25 AR-1248-5


R.T.: 7.255 min
Delta R.T.: -0.004 min
Response: 7992
Conc: 4.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

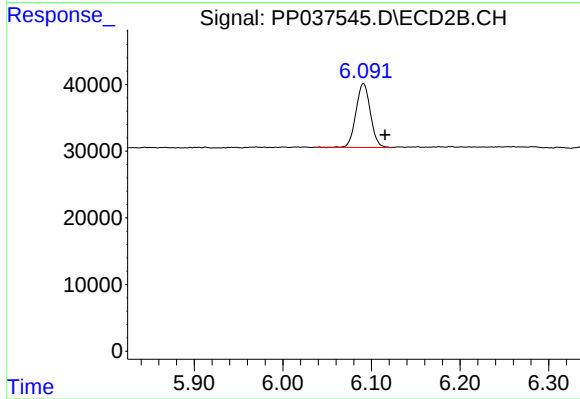


#25 AR-1248-5

R.T.: 6.091 min
Delta R.T.: -0.024 min
Response: 108174
Conc: 101.98 ng/ml

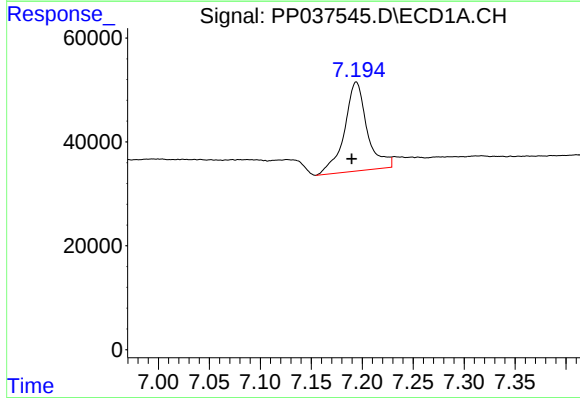


#26 AR-1254-1

R.T.: 7.194 min
Delta R.T.: 0.005 min
Response: 265940
Conc: 148.03 ng/ml

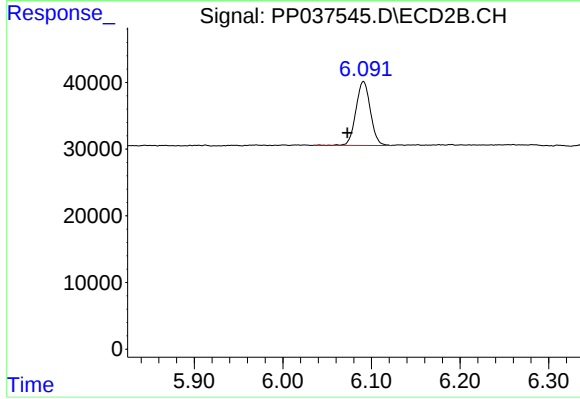

#26 AR-1254-1


R.T.: 6.091 min
Delta R.T.: 0.018 min
Response: 108174
Conc: 72.87 ng/ml

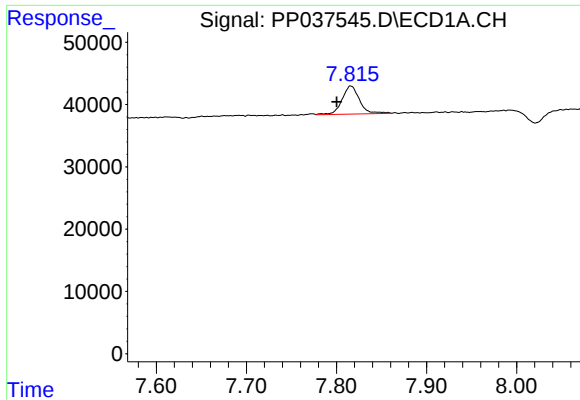

#28 AR-1254-3


R.T.: 7.816 min
Delta R.T.: 0.015 min
Response: 60314
Conc: 19.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

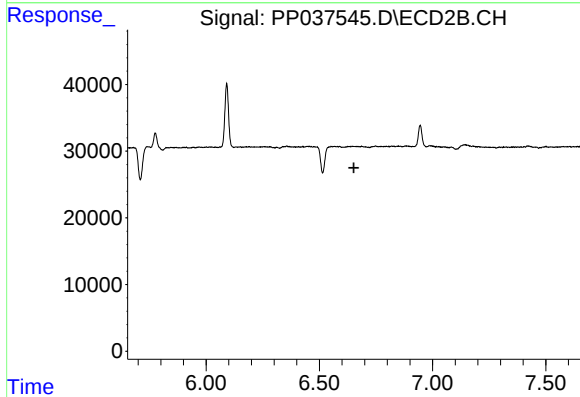


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

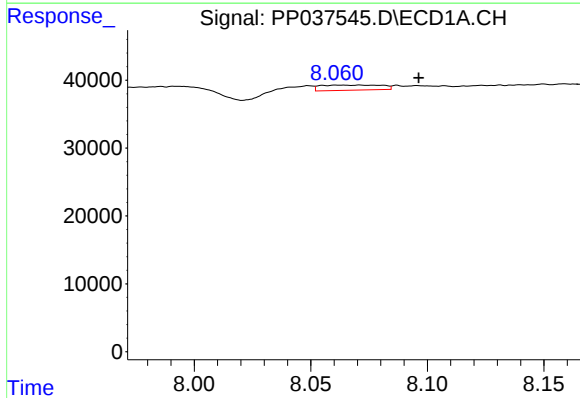


#29 AR-1254-4

R.T.: 8.071 min
Delta R.T.: -0.025 min
Response: 13688
Conc: 6.03 ng/ml

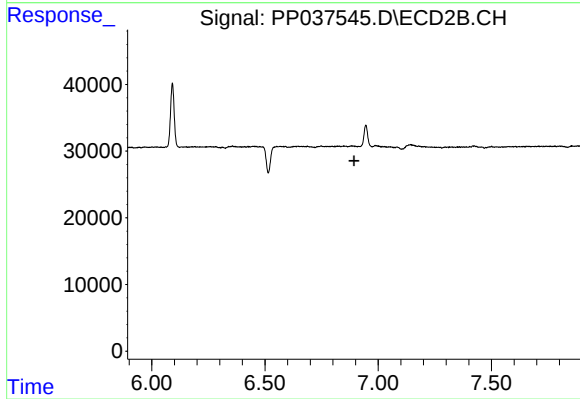

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.893 min
Response: 0
Conc: N.D.

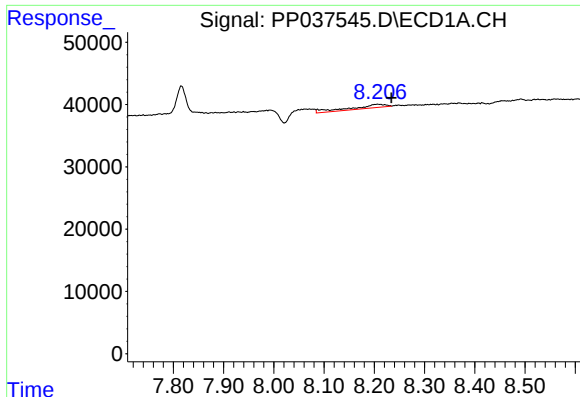

#32 AR-1260-2


R.T.: 8.206 min
Delta R.T.: -0.027 min
Response: 27301
Conc: 9.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

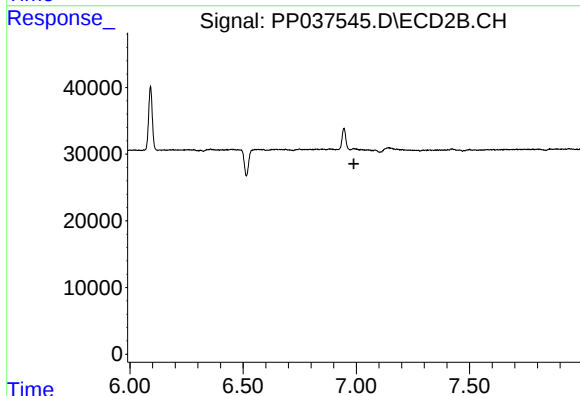


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

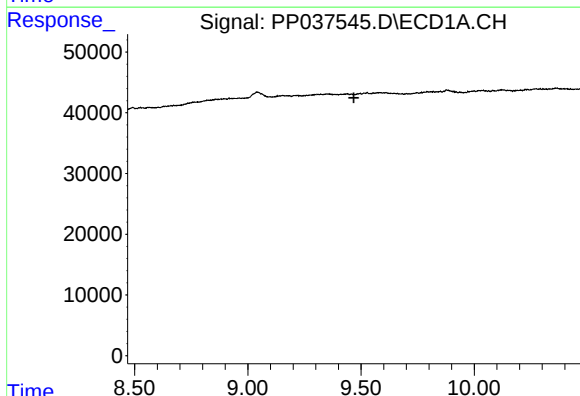


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.469 min
Response: 0
Conc: N.D.

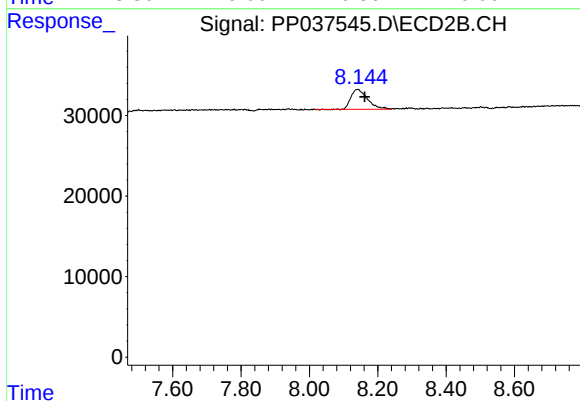

#38 AR-1262-3


R.T.: 8.143 min
Delta R.T.: -0.019 min
Response: 83705
Conc: 59.45 ng/ml

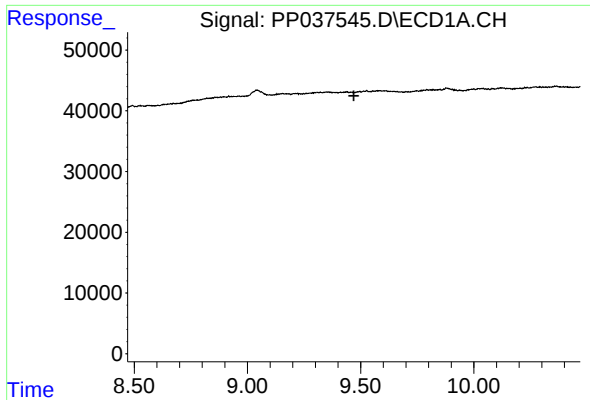

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

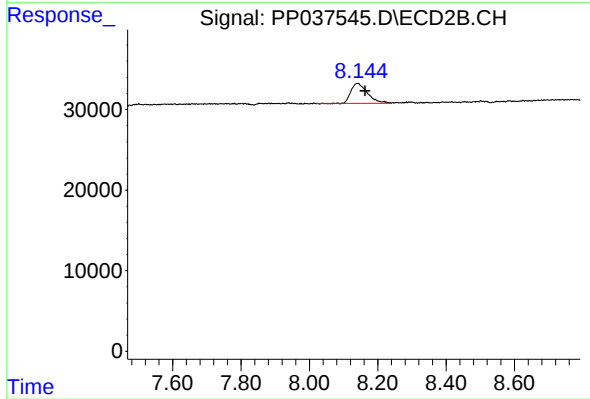

#41 AR-1268-1

R.T.: 8.143 min
Delta R.T.: -0.021 min
Response: 83705
Conc: 21.00 ng/ml