

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
 Data File : PP037567.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2021 16:53
 Operator : DD\AJ
 Sample : M3117-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NJ-CLEAN-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:49:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.957	3.947	971099	583372	21.367	21.319
2)	SA Decachlor...	10.985	9.237	891825	418902	19.373	15.050
Target Compounds							
8)	L2 AR-1221-1	5.206	0.000	48447	0	91.345	N.D. #
9)	L2 AR-1221-2	5.310	0.000	12656	0	31.240	N.D. #
24)	L5 AR-1248-4	7.195f	0.000	2943	0	1.557	N.D. #
26)	L6 AR-1254-1	7.195	0.000	2943	0	1.638	N.D. #
28)	L6 AR-1254-3	7.813	0.000	14254	0	4.623	N.D. #
30)	L6 AR-1254-5	8.546f	7.315	36554	19553	14.607	10.430 #
32)	L7 AR-1260-2	8.226	0.000	23878	0	8.584	N.D. #
36)	L8 AR-1262-1	0.000	7.315	0	19553	N.D.	18.830 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
Data File : PP037567.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2021 16:53
Operator : DD\AJ
Sample : M3117-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
NJ-CLEAN-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:49:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

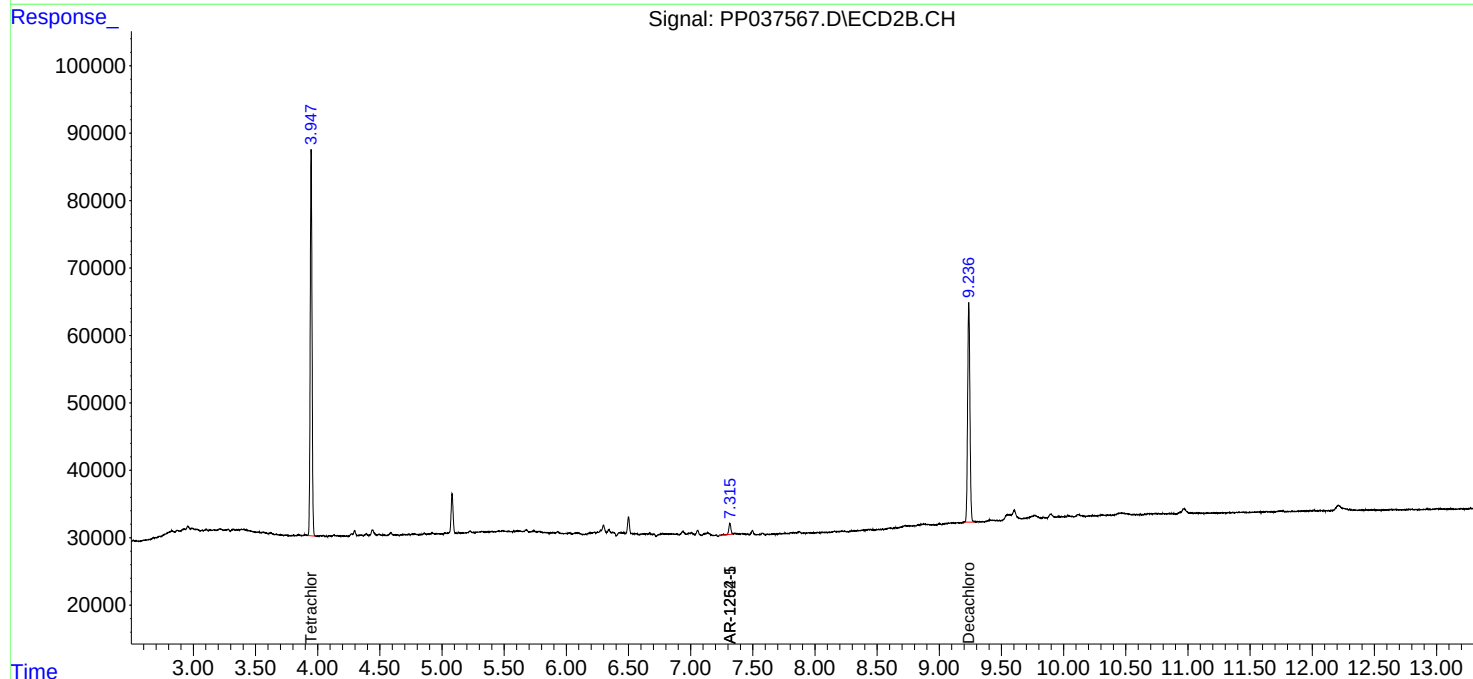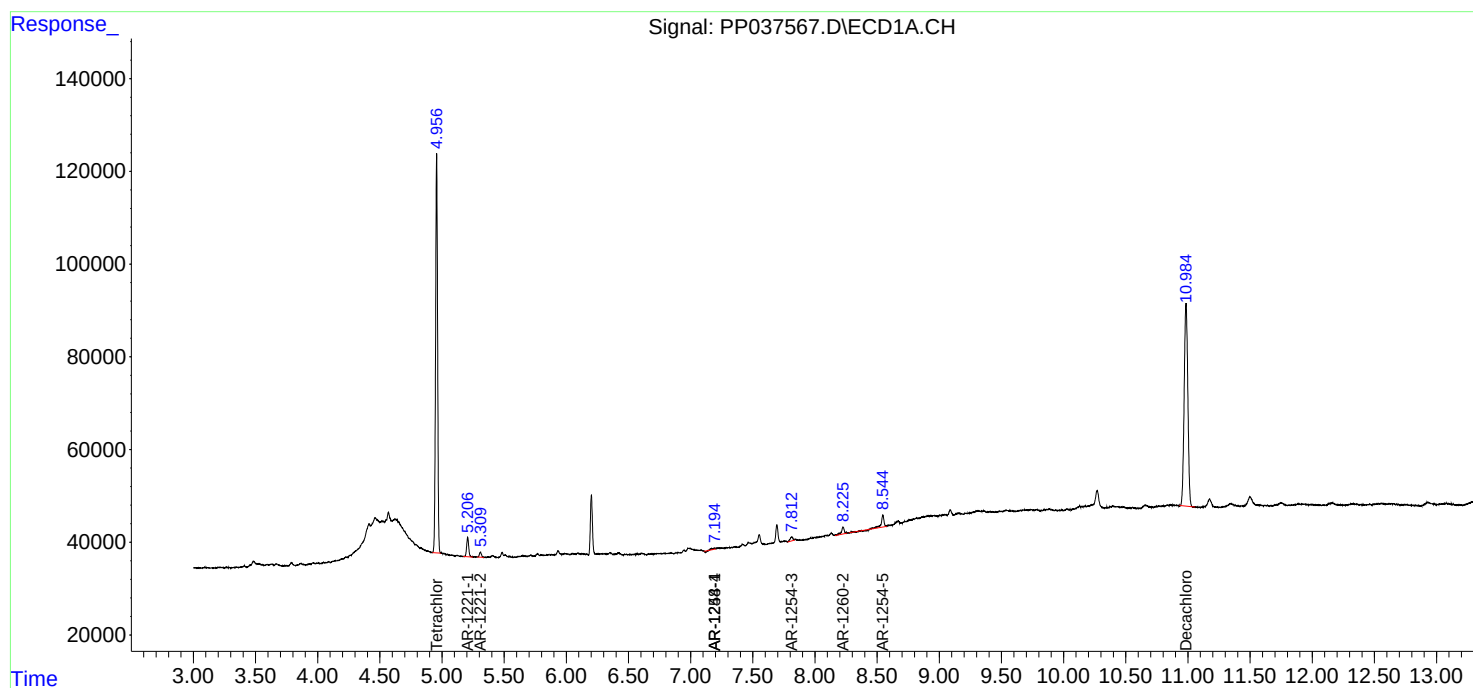


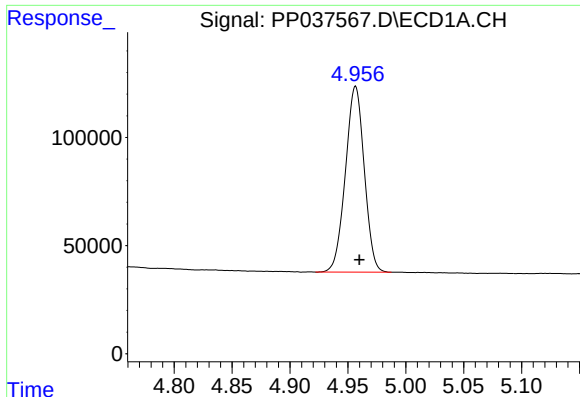

#1 Tetrachloro-m-xylene


R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 971099
Conc: 21.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
NJ-CLEAN-7

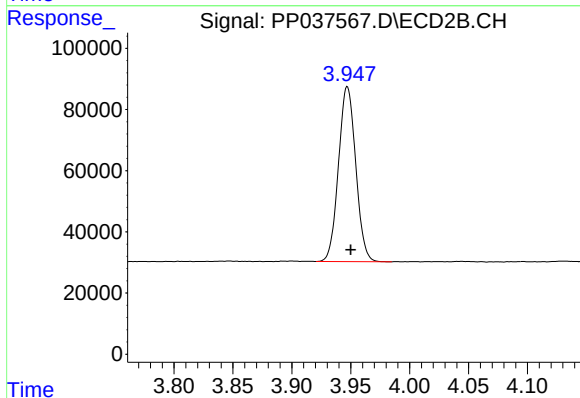


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.003 min
Response: 583372
Conc: 21.32 ng/ml

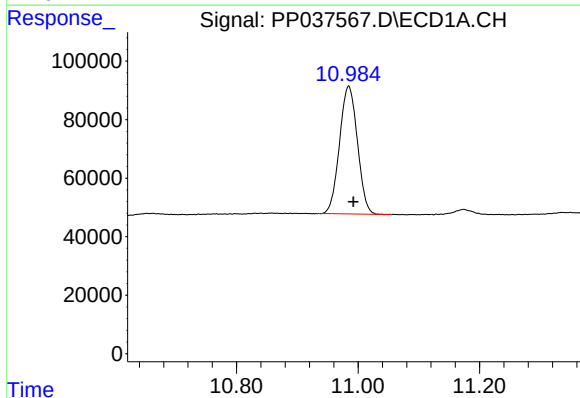


#2 Decachlorobiphenyl

R.T.: 10.985 min
Delta R.T.: -0.008 min
Response: 891825
Conc: 19.37 ng/ml

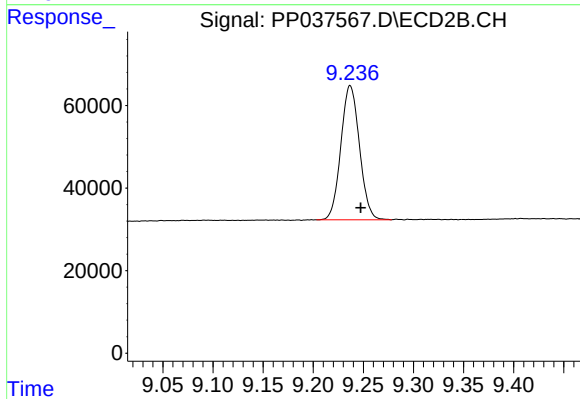

#2 Decachlorobiphenyl


R.T.: 9.237 min
Delta R.T.: -0.010 min
Response: 418902
Conc: 15.05 ng/ml

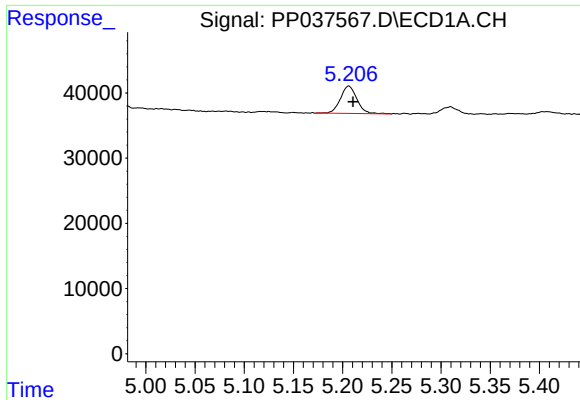

#8 AR-1221-1


R.T.: 5.206 min
Delta R.T.: -0.004 min
Response: 48447
Conc: 91.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
NJ-CLEAN-7

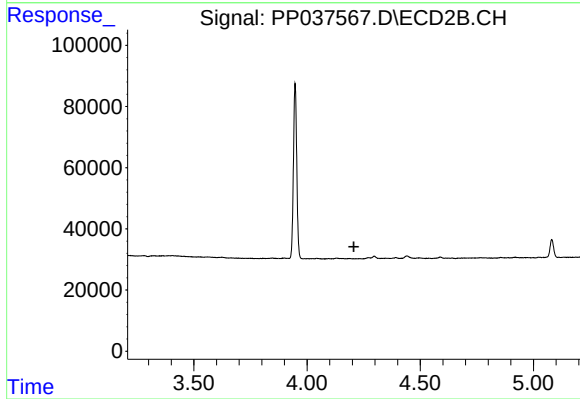


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

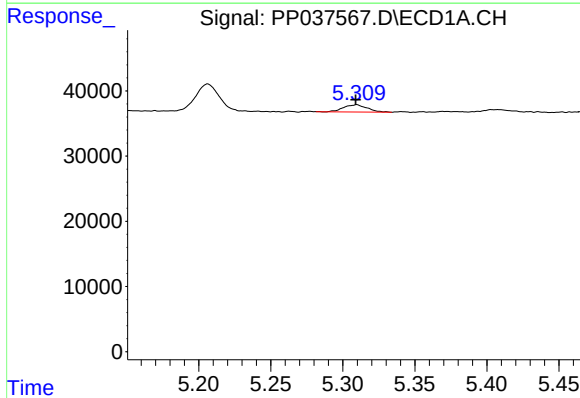


#9 AR-1221-2

R.T.: 5.310 min
Delta R.T.: 0.000 min
Response: 12656
Conc: 31.24 ng/ml

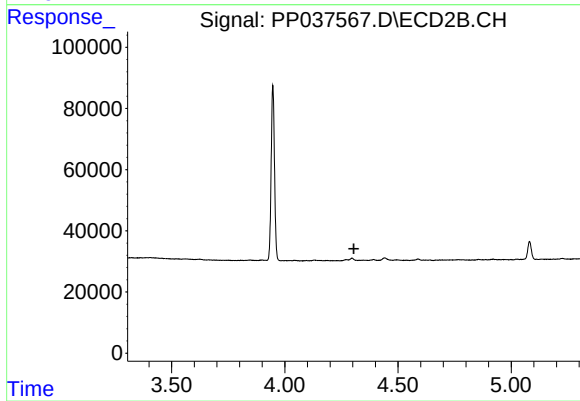

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.305 min
Response: 0
Conc: N.D.

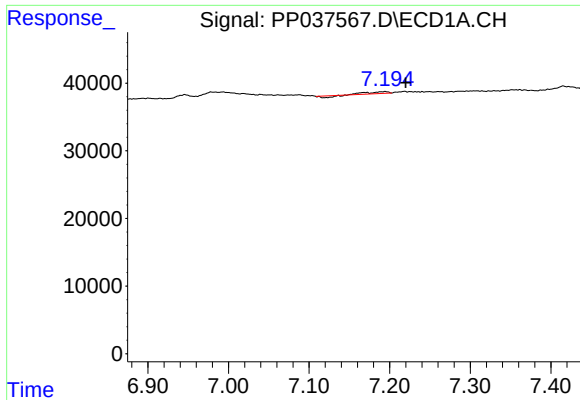

#24 AR-1248-4


R.T.: 7.195 min
Delta R.T.: -0.025 min
Response: 2943
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
NJ-CLEAN-7

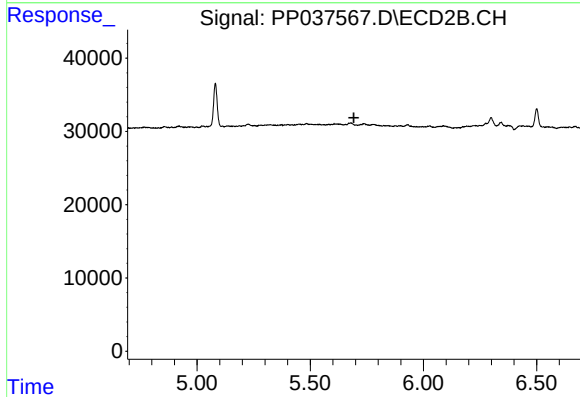


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.692 min
Response: 0
Conc: N.D.

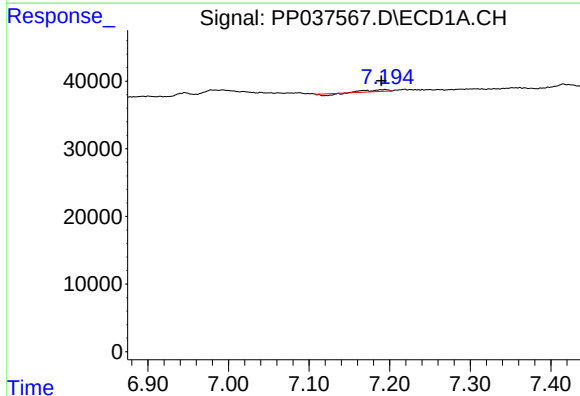


#26 AR-1254-1

R.T.: 7.195 min
Delta R.T.: 0.005 min
Response: 2943
Conc: 1.64 ng/ml

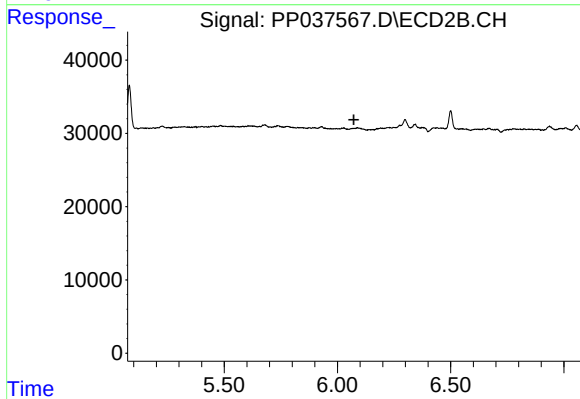

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

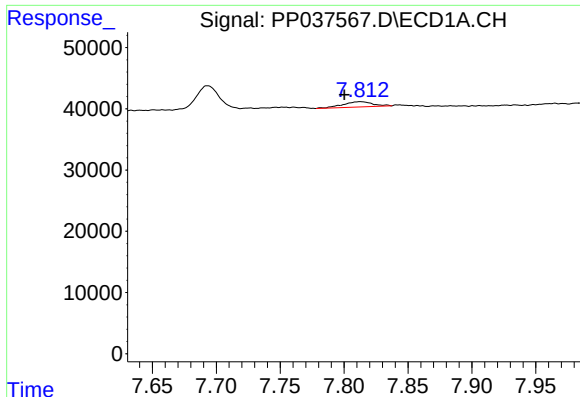

#28 AR-1254-3


R.T.: 7.813 min
Delta R.T.: 0.013 min
Response: 14254
Conc: 4.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
NJ-CLEAN-7

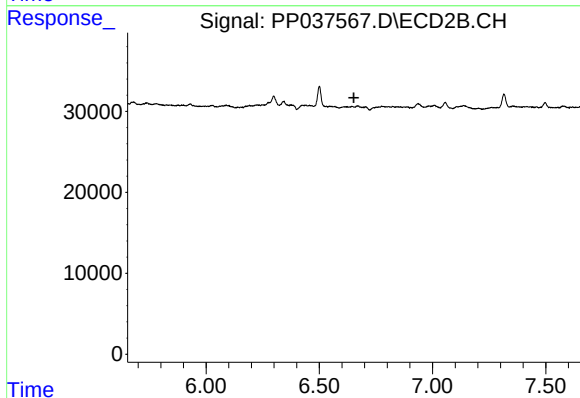


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

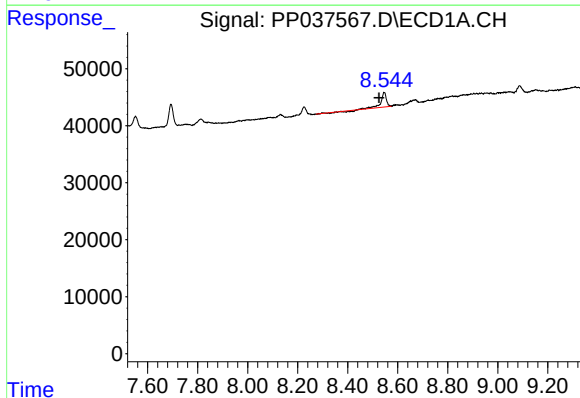


#30 AR-1254-5

R.T.: 8.546 min
Delta R.T.: 0.021 min
Response: 36554
Conc: 14.61 ng/ml

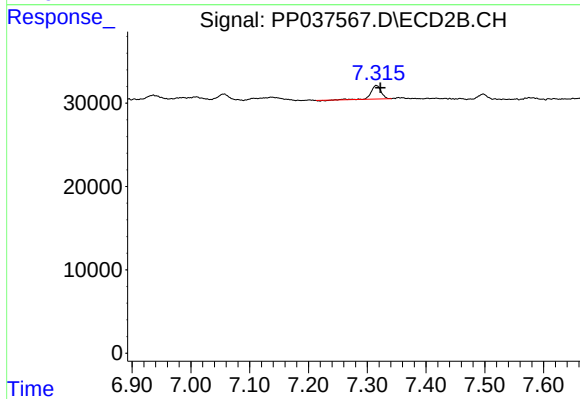

#30 AR-1254-5


R.T.: 7.315 min
Delta R.T.: -0.007 min
Response: 19553
Conc: 10.43 ng/ml

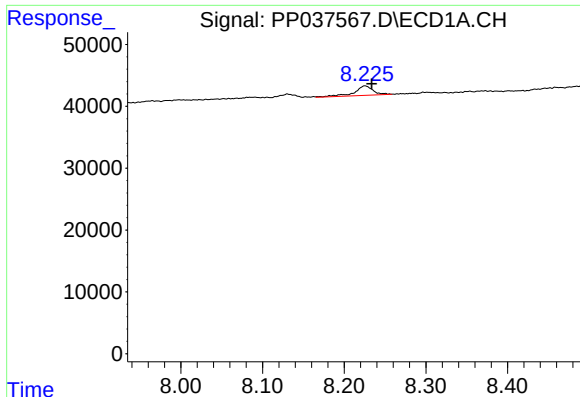

#32 AR-1260-2


R.T.: 8.226 min
Delta R.T.: -0.008 min
Response: 23878
Conc: 8.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
NJ-CLEAN-7

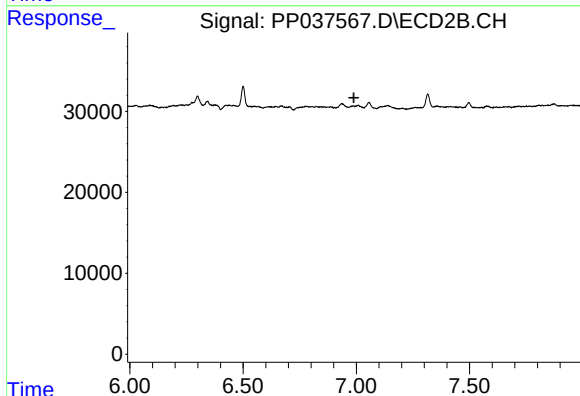


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

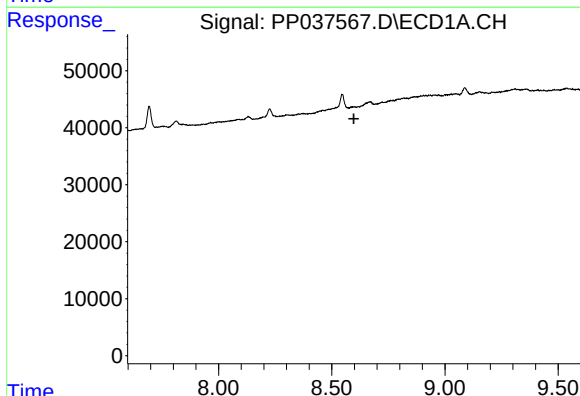

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.598 min
Response: 0
Conc: N.D.

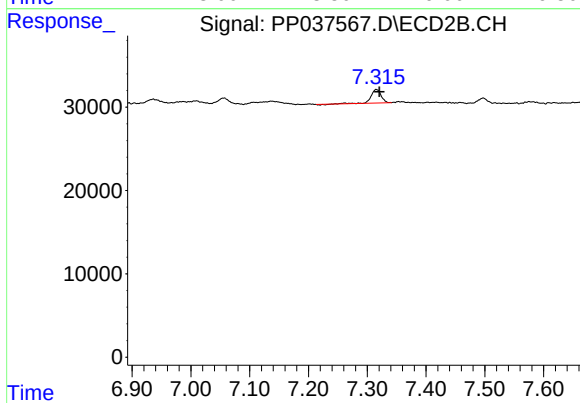

#36 AR-1262-1

R.T.: 7.315 min
Delta R.T.: -0.006 min
Response: 19553
Conc: 18.83 ng/ml