

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
 Data File : PP037593.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 00:46
 Operator : DD\AJ
 Sample : PB137881TB
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB137881TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 03:04:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.955	3.946	906044	530350	19.935	19.381
2)	SA Decachlor...	10.982	9.236	860920	460661	18.701	16.550
Target Compounds							
8)	L2 AR-1221-1	5.205	0.000	22883	0	43.144	N.D. #
9)	L2 AR-1221-2	5.309	0.000	11512	0	28.415	N.D. #
24)	L5 AR-1248-4	7.193f	0.000	9897	0	5.236	N.D. #
26)	L6 AR-1254-1	7.193	0.000	9897	0	5.509	N.D. #
28)	L6 AR-1254-3	7.812	0.000	7349	0	2.384	N.D. #
30)	L6 AR-1254-5	8.525	0.000	8624	0	3.446	N.D. #
32)	L7 AR-1260-2	8.261f	0.000	2596	0	0.933	N.D. #
44)	L9 AR-1268-4	10.264f	0.000	27085	0	11.839	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
Data File : PP037593.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 00:46
Operator : DD\AJ
Sample : PB137881TB
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB137881TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 03:04:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

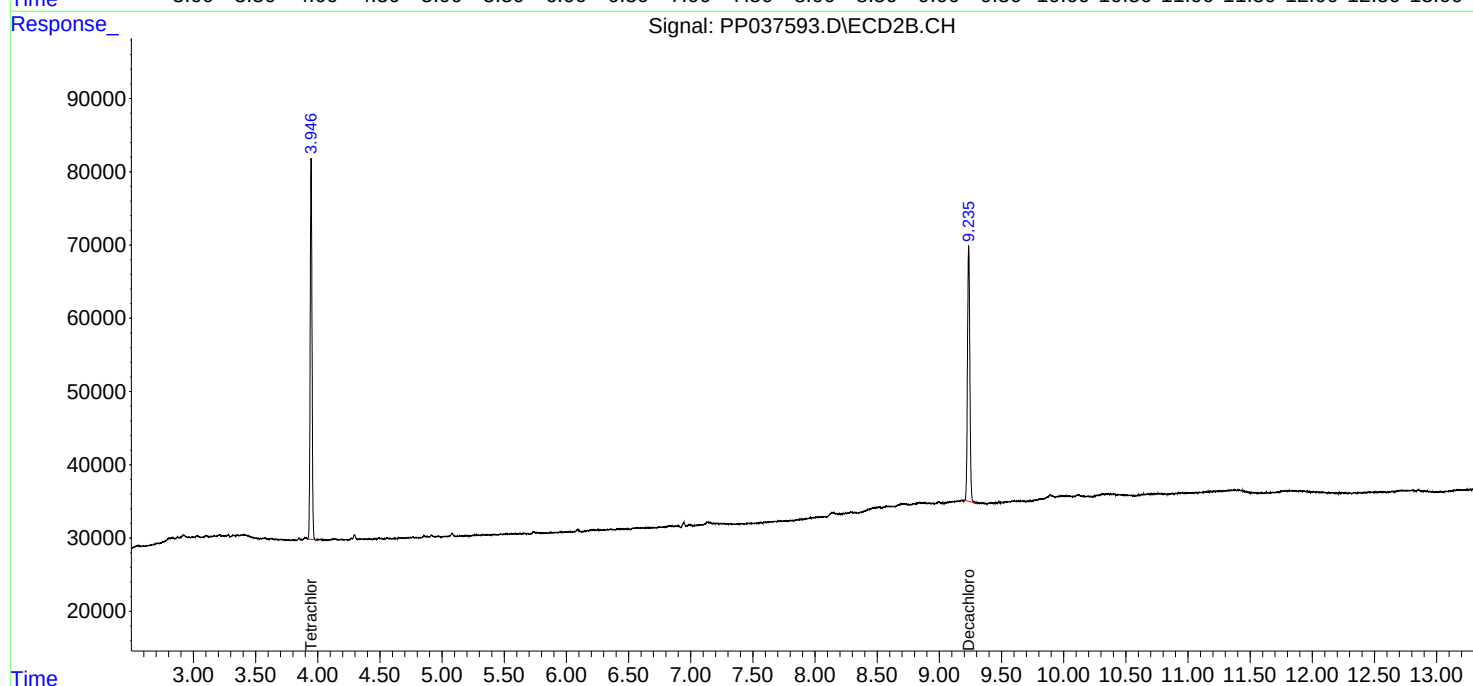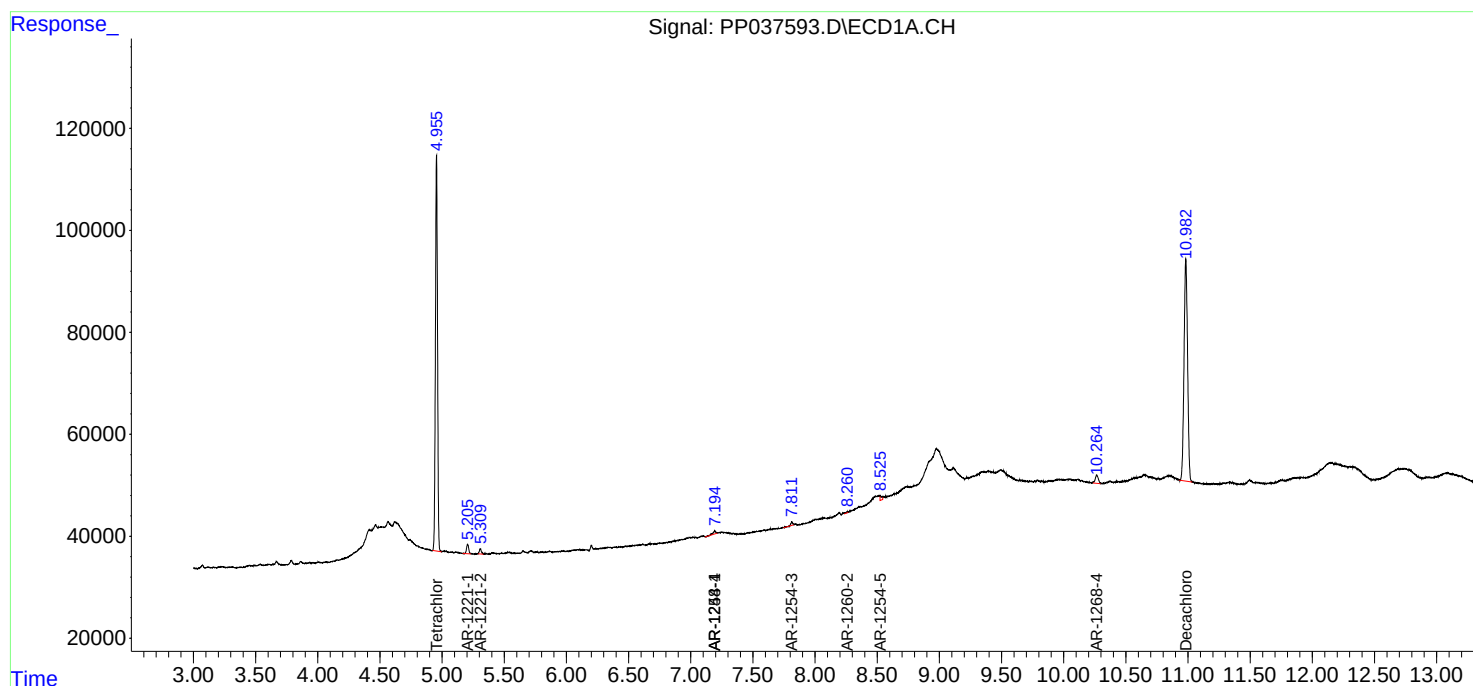


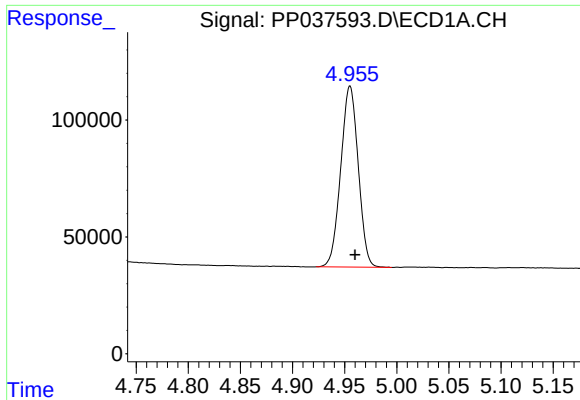

#1 Tetrachloro-m-xylene


R.T.: 4.955 min
Delta R.T.: -0.005 min
Response: 906044
Conc: 19.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB137881TB

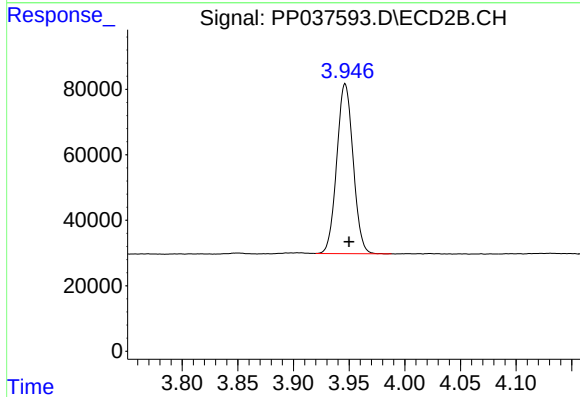


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.003 min
Response: 530350
Conc: 19.38 ng/ml

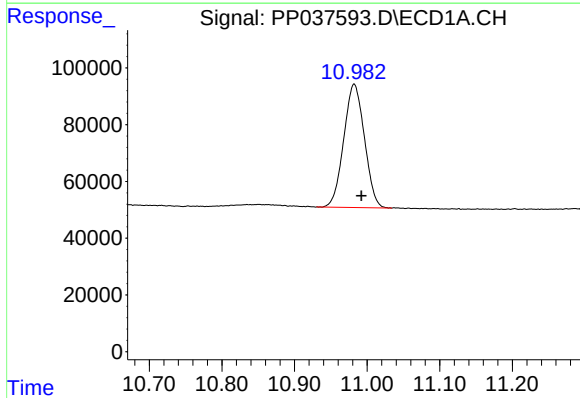


#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.010 min
Response: 860920
Conc: 18.70 ng/ml

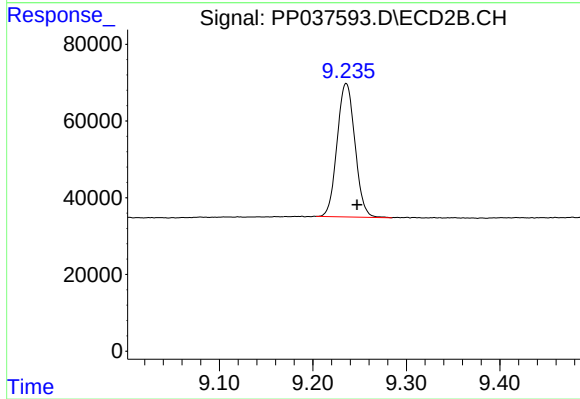

#2 Decachlorobiphenyl


R.T.: 9.236 min
Delta R.T.: -0.012 min
Response: 460661
Conc: 16.55 ng/ml

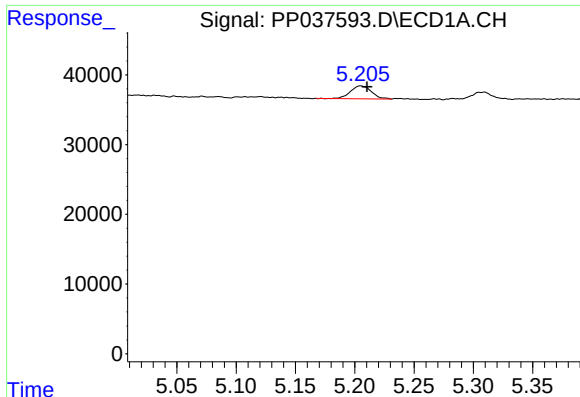

#8 AR-1221-1


R.T.: 5.205 min
Delta R.T.: -0.005 min
Response: 22883
Conc: 43.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB137881TB

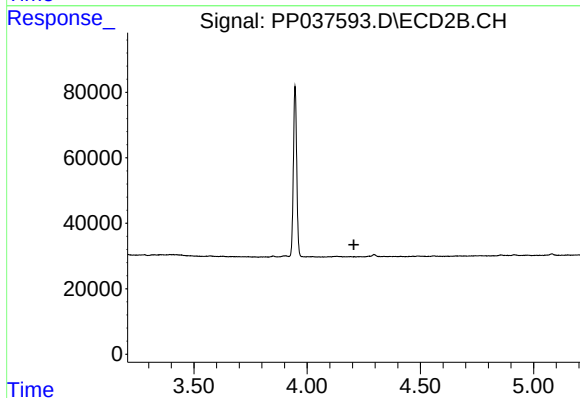


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

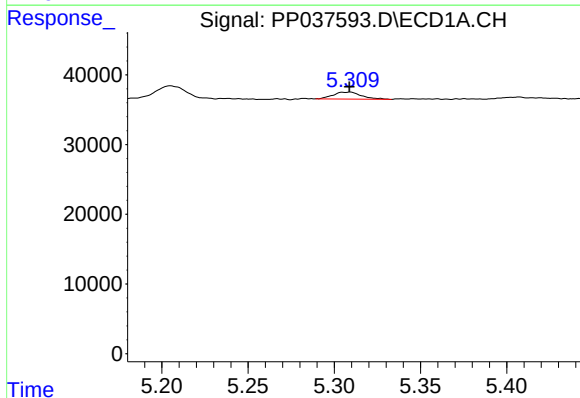


#9 AR-1221-2

R.T.: 5.309 min
Delta R.T.: 0.000 min
Response: 11512
Conc: 28.42 ng/ml

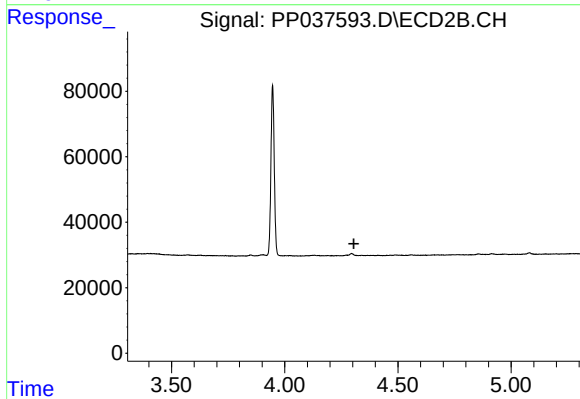

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.305 min
Response: 0
Conc: N.D.

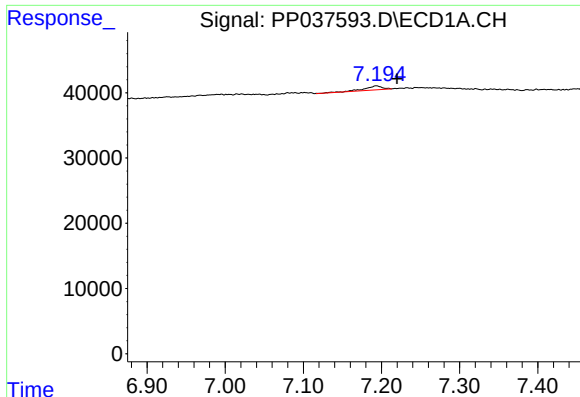

#24 AR-1248-4


R.T.: 7.193 min
Delta R.T.: -0.026 min
Response: 9897
Conc: 5.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB137881TB

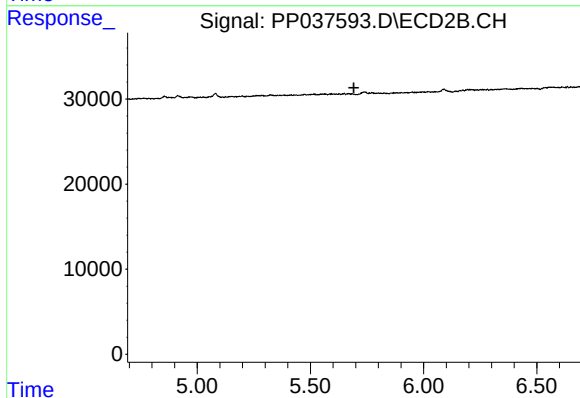


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.692 min
Response: 0
Conc: N.D.

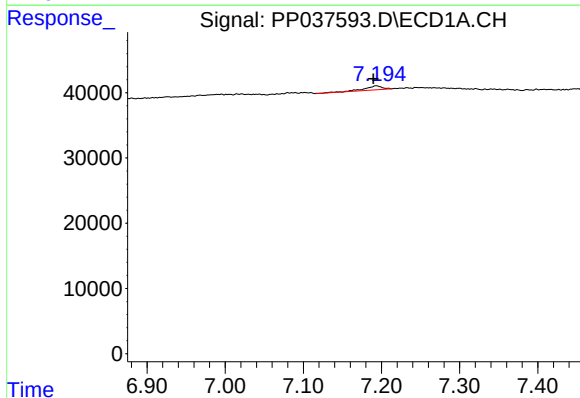


#26 AR-1254-1

R.T.: 7.193 min
Delta R.T.: 0.004 min
Response: 9897
Conc: 5.51 ng/ml

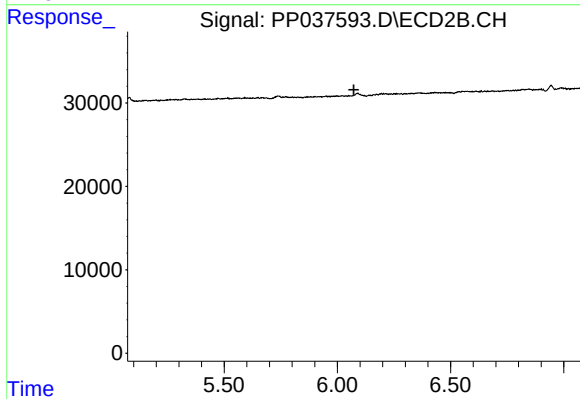

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

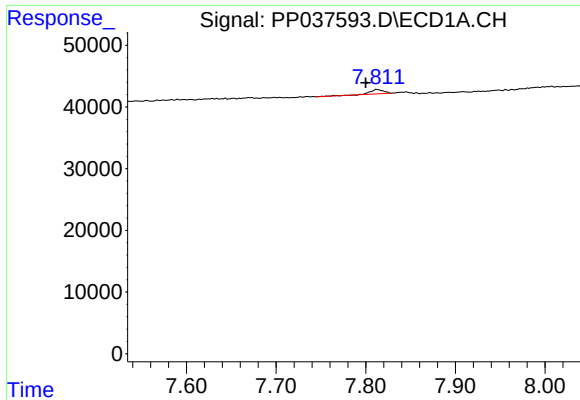

#28 AR-1254-3


R.T.: 7.812 min
Delta R.T.: 0.012 min
Response: 7349
Conc: 2.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB137881TB

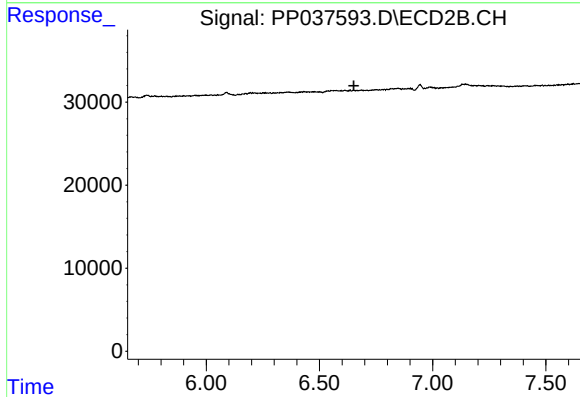


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

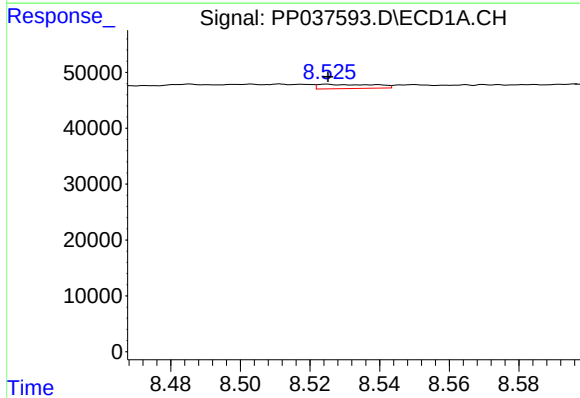


#30 AR-1254-5

R.T.: 8.525 min
Delta R.T.: 0.000 min
Response: 8624
Conc: 3.45 ng/ml

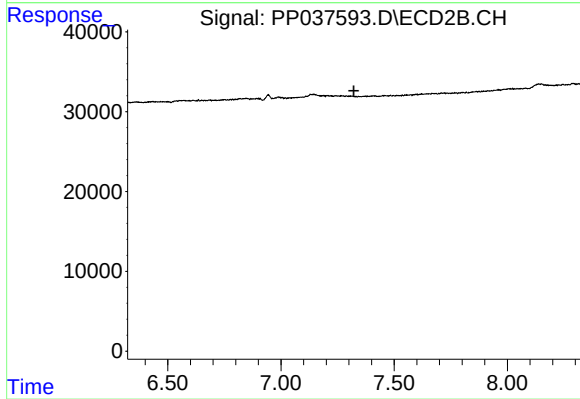

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.322 min
Response: 0
Conc: N.D.

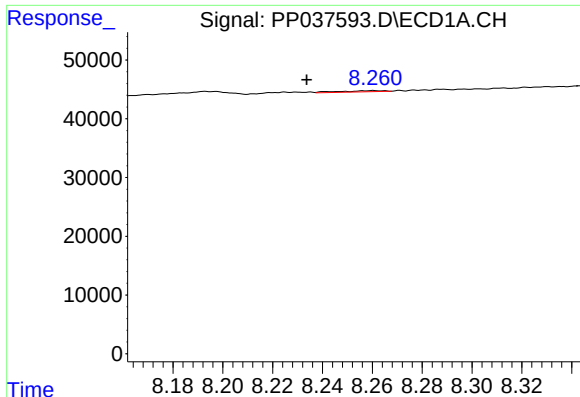

#32 AR-1260-2


R.T.: 8.261 min
Delta R.T.: 0.027 min
Response: 2596
Conc: 0.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB137881TB

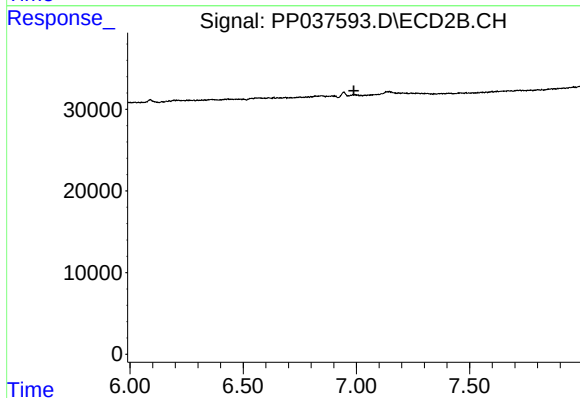


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

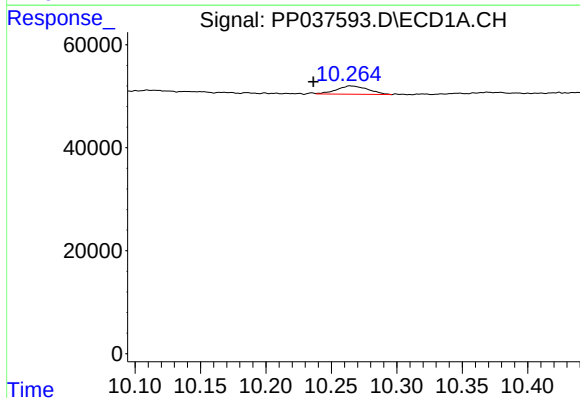

#44 AR-1268-4

R.T.: 10.264 min
Delta R.T.: 0.028 min
Response: 27085
Conc: 11.84 ng/ml

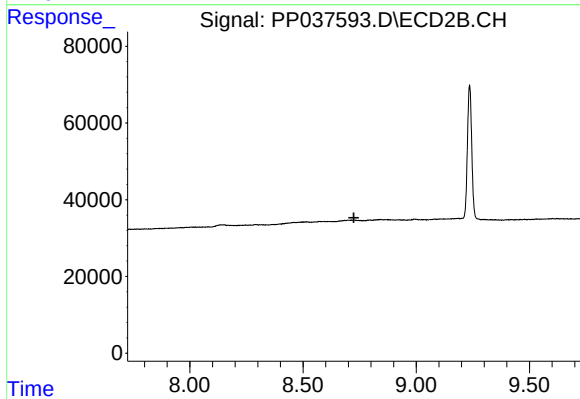

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.725 min
Response: 0
Conc: N.D.