

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
 Data File : PP037550.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2021 11:11
 Operator : DD\AJ
 Sample : M3059-03DL 40X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 01-A-01-B-01-CDL

Manual Integrations
 APPROVED

mohammad
 7/23/2021 4:27:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 14:34:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.956	3.948	23373	14662	0.514m	0.536
2) SA Decachlor...	10.989	9.240	24682	13741	0.536	0.494
Target Compounds						
26) L6 AR-1254-1	7.187	6.067	1492493	1323079	830.780	891.219
27) L6 AR-1254-2	7.417	6.228	2147554	952425	772.036	733.197
28) L6 AR-1254-3	7.799	6.647	1919305	1391425	622.541	652.018
29) L6 AR-1254-4	8.094	6.887	1023975	619834	450.804	456.858
30) L6 AR-1254-5	8.523	7.317	709462	479985	283.513	256.042

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
Data File : PP037550.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2021 11:11
Operator : DD\AJ
Sample : M3059-03DL 40X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleID :
01-A-01-B-01-CDL


Manual Integrations
APPROVED

mohammad
7/23/2021 4:27:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 14:34:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

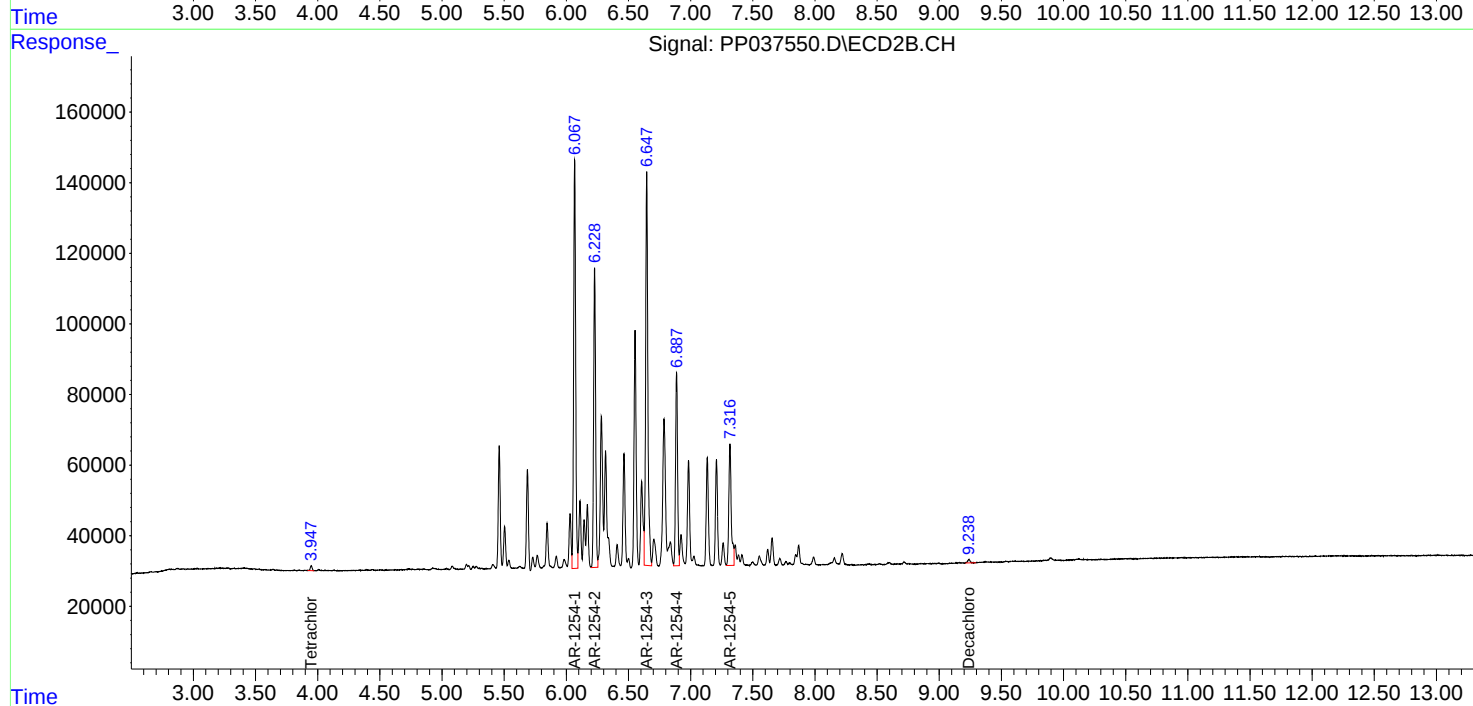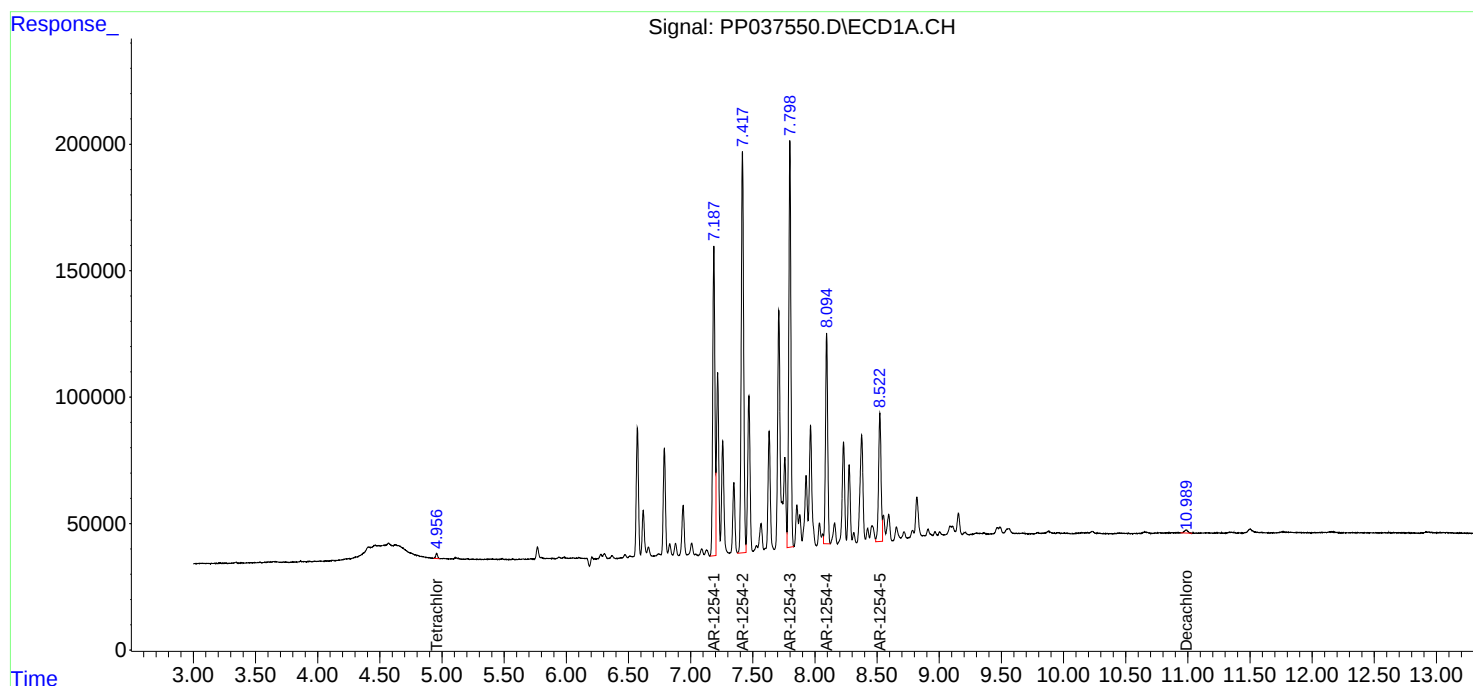

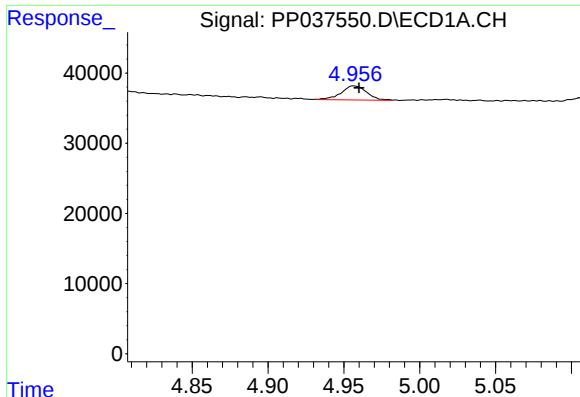


#1 Tetrachloro-m-xylene

R.T.: 4.956 min
Delta R.T.: -0.004 min
Response: 23373
Conc: 0.51 ng/ml m

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-CDL


Manual Integrations
APPROVED

mohammad
7/23/2021 4:27:50 PM

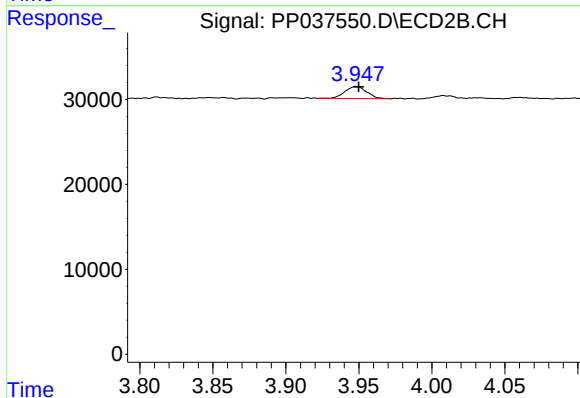


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 14662
Conc: 0.54 ng/ml

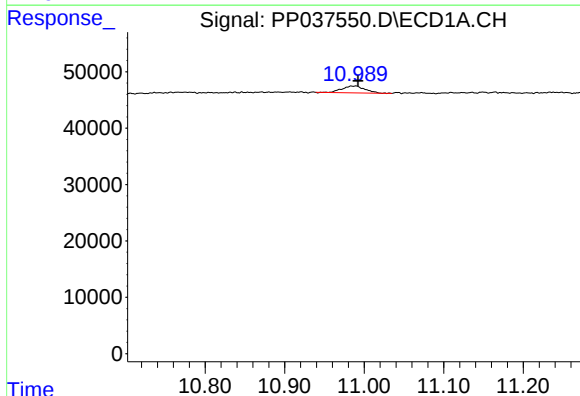


#2 Decachlorobiphenyl

R.T.: 10.989 min
Delta R.T.: -0.003 min
Response: 24682
Conc: 0.54 ng/ml

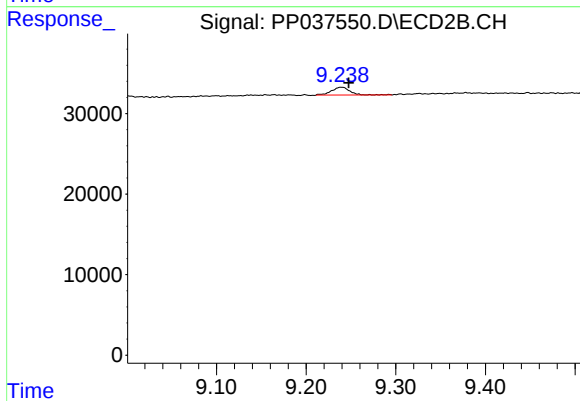

#2 Decachlorobiphenyl

R.T.: 9.240 min
Delta R.T.: -0.008 min
Response: 13741
Conc: 0.49 ng/ml

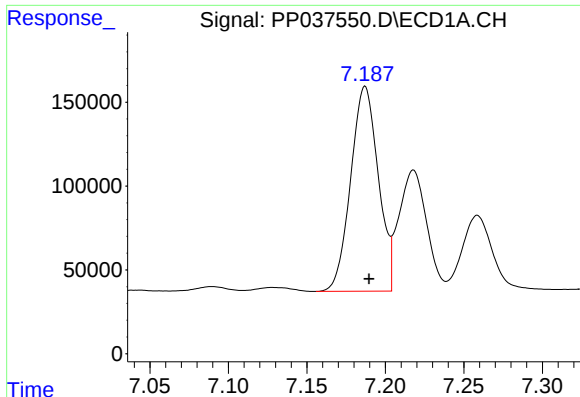


#26 AR-1254-1

R.T.: 7.187 min
Delta R.T.: -0.002 min
Response: 1492493
Conc: 830.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-CDL


Manual Integrations
APPROVED

mohammad
7/23/2021 4:27:50 PM

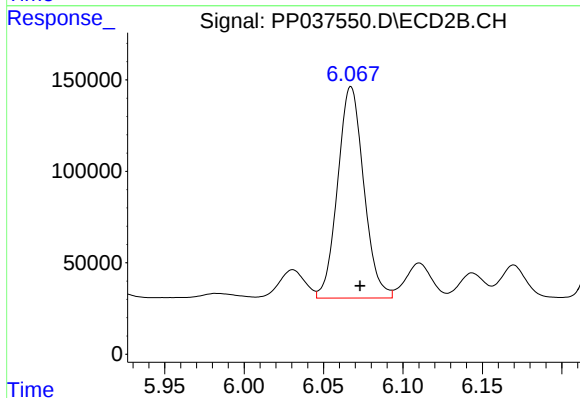


#26 AR-1254-1

R.T.: 6.067 min
Delta R.T.: -0.006 min
Response: 1323079
Conc: 891.22 ng/ml

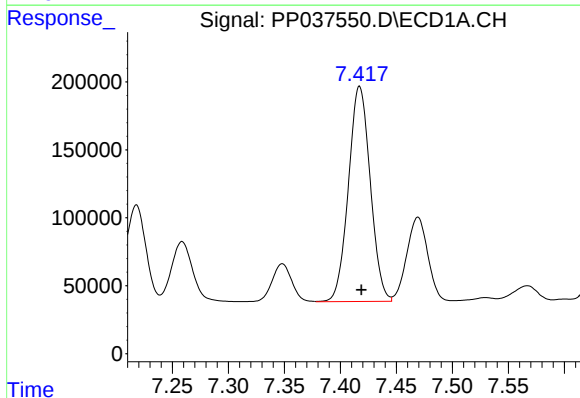


#27 AR-1254-2

R.T.: 7.417 min
Delta R.T.: -0.002 min
Response: 2147554
Conc: 772.04 ng/ml

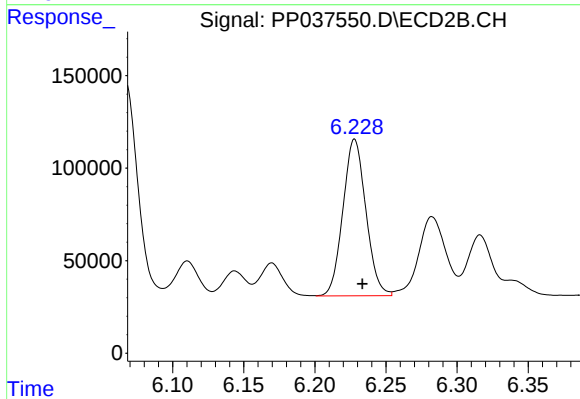

#27 AR-1254-2

R.T.: 6.228 min
Delta R.T.: -0.006 min
Response: 952425
Conc: 733.20 ng/ml

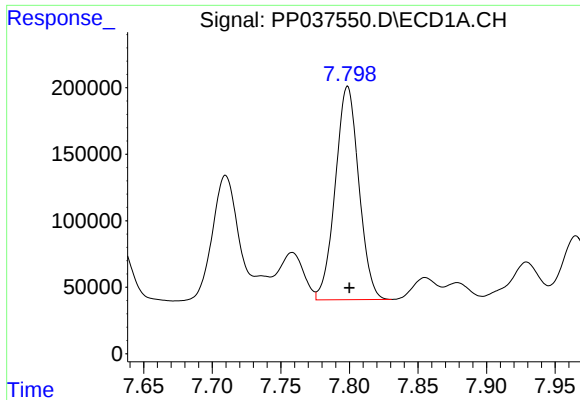


#28 AR-1254-3

R.T.: 7.799 min
Delta R.T.: -0.001 min
Response: 1919305
Conc: 622.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-CDL


Manual Integrations
APPROVED

mohammad
7/23/2021 4:27:50 PM

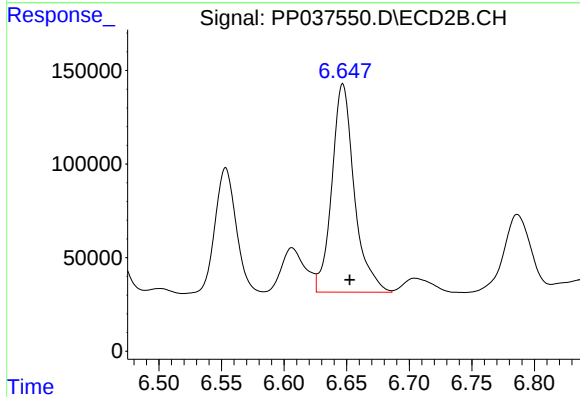


#28 AR-1254-3

R.T.: 6.647 min
Delta R.T.: -0.005 min
Response: 1391425
Conc: 652.02 ng/ml

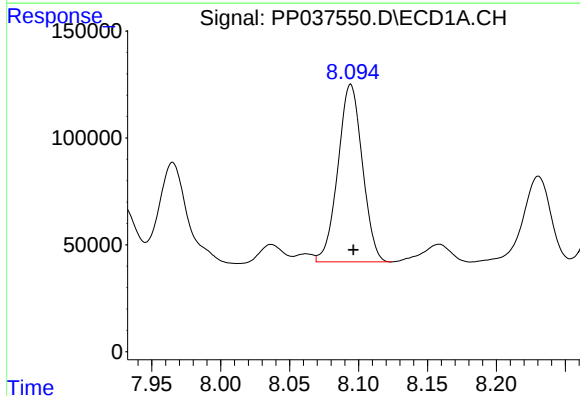


#29 AR-1254-4

R.T.: 8.094 min
Delta R.T.: -0.002 min
Response: 1023975
Conc: 450.80 ng/ml

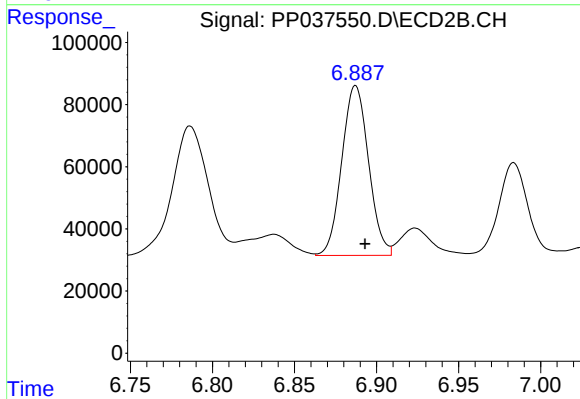

#29 AR-1254-4

R.T.: 6.887 min
Delta R.T.: -0.006 min
Response: 619834
Conc: 456.86 ng/ml

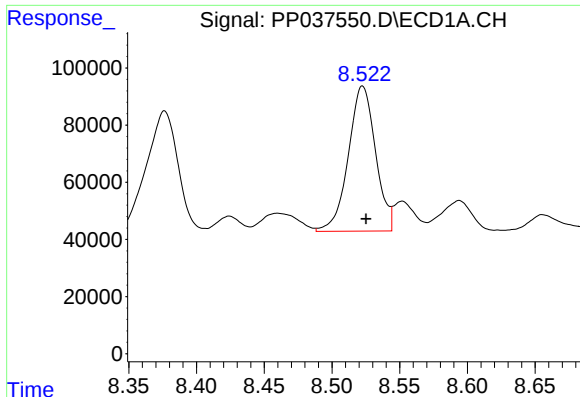


#30 AR-1254-5

R.T.: 8.523 min
Delta R.T.: -0.003 min
Response: 709462
Conc: 283.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-CDL

Manual Integrations
APPROVED

mohammad
7/23/2021 4:27:50 PM

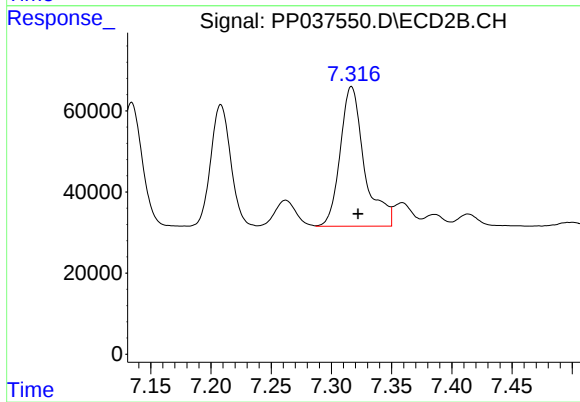

#30 AR-1254-5

R.T.: 7.317 min
Delta R.T.: -0.006 min
Response: 479985
Conc: 256.04 ng/ml