

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
 Data File : PP037594.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 1:03
 Operator : DD\AJ
 Sample : M3114-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20210594-AMENDED-COM-8-SPLP

Manual Integrations
 APPROVED

mohammad
 7/23/2021 4:28:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 03:05:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.955	3.946	815055	483322	17.933	17.663m
2) SA Decachlor...	10.982	9.237	842169	445019	18.294	15.988

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072221\
Data File : PP037594.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 1:03
Operator : DD\AJ
Sample : M3114-07
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
20210594-AMENDED-COM-8-SPLP


Manual Integrations
APPROVED

mohammad
7/23/2021 4:28:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 03:05:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

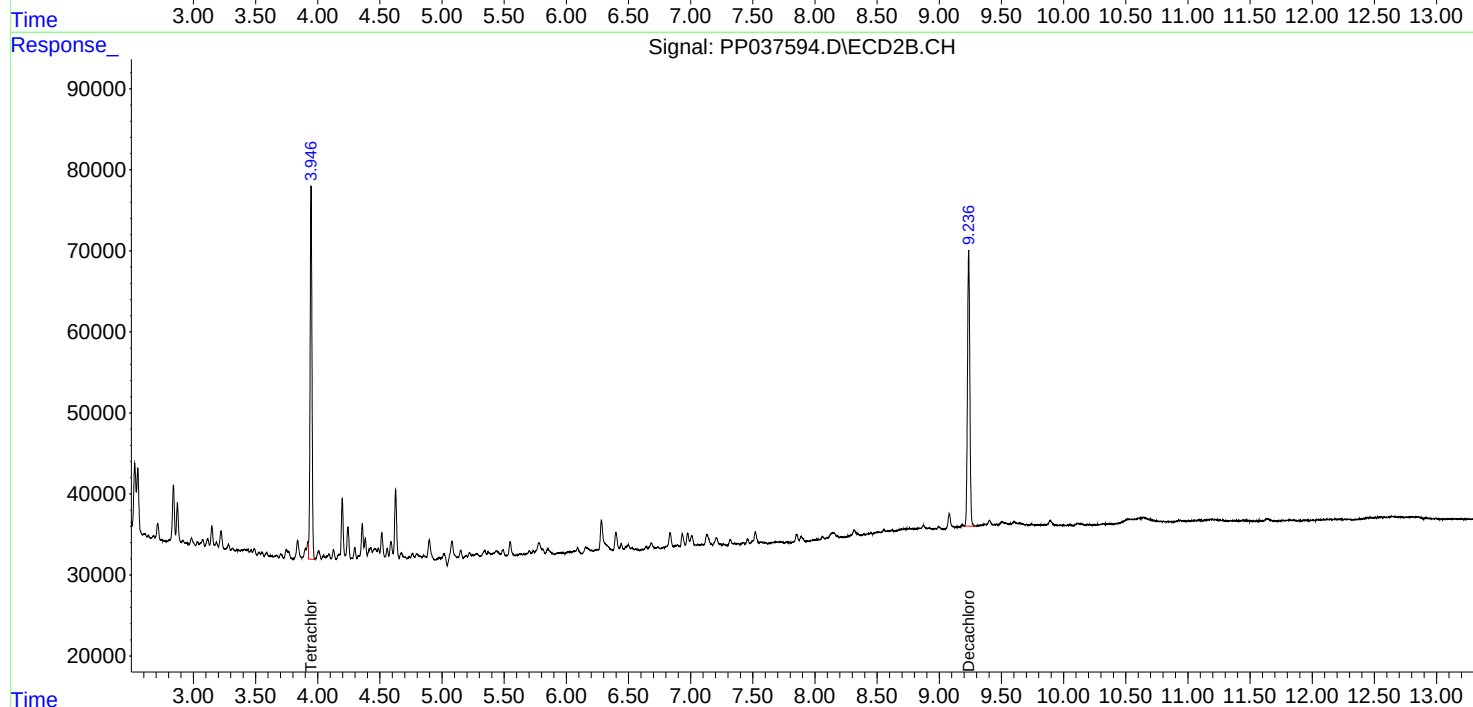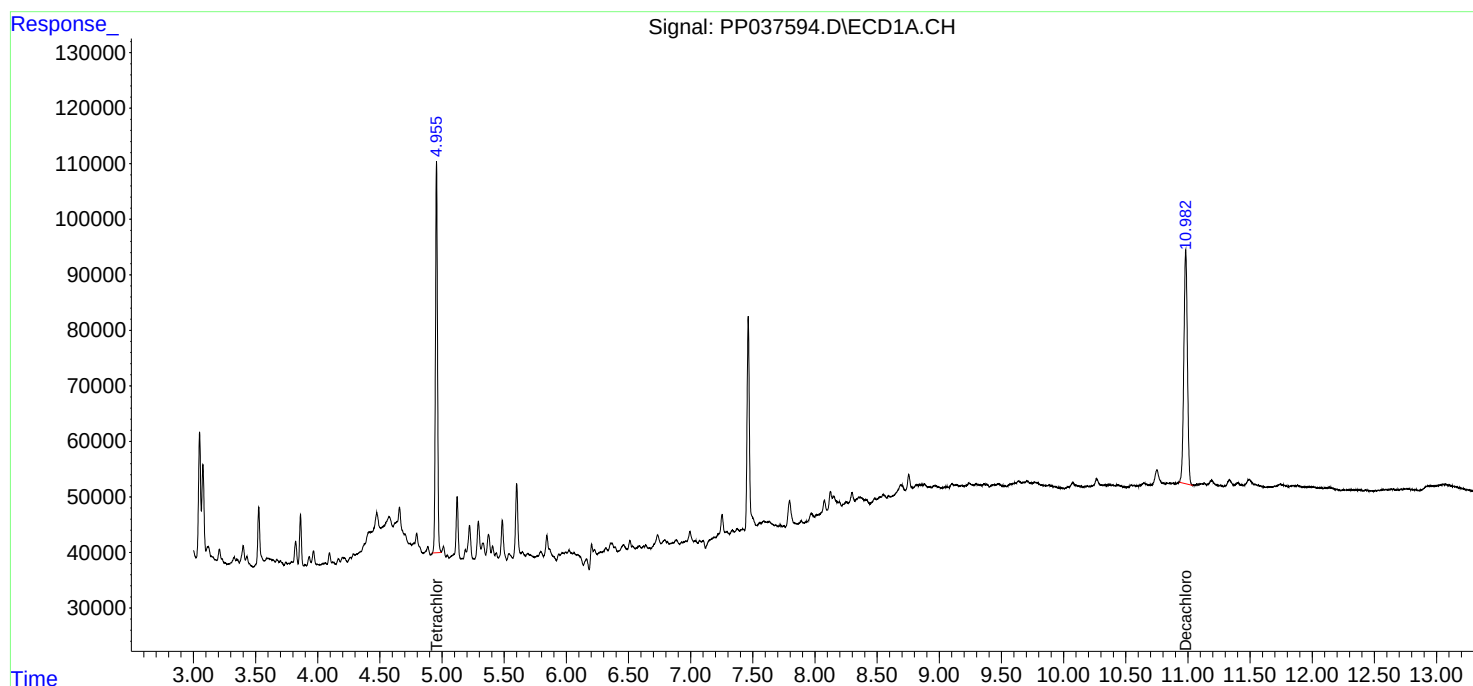

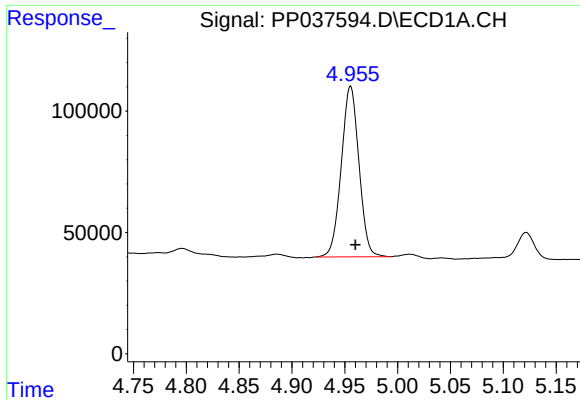


#1 Tetrachloro-m-xylene

R.T.: 4.955 min
Delta R.T.: -0.005 min
Response: 815055
Conc: 17.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
20210594-AMENDED-COM-8-SPLP


Manual Integrations
APPROVED

mohammad
7/23/2021 4:28:17 PM

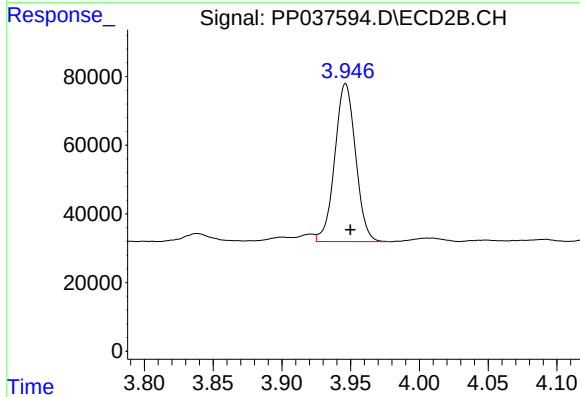


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 483322
Conc: 17.66 ng/ml m

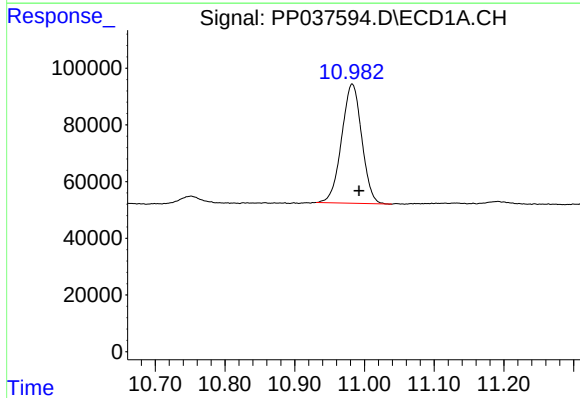

#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.010 min
Response: 842169
Conc: 18.29 ng/ml

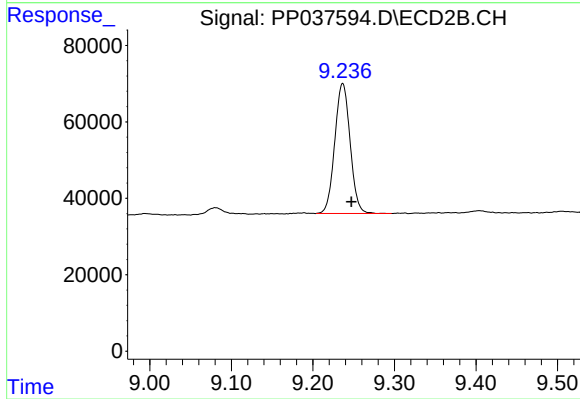

#2 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: -0.011 min
Response: 445019
Conc: 15.99 ng/ml