

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072222\
 Data File : PP049735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2022 15:10
 Operator : YP\AJ
 Sample : N3814-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ENV-DE-3(0-5)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2022
 Supervised By :Ankita Jodhani 07/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:26:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.601	31363828	48408722	21.613m	19.804
2) SA Decachlor...	10.102	8.566	25326317	24270235	17.906	20.840m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072222\
Data File : PP049735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2022 15:10
Operator : YP\AJ
Sample : N3814-04
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
ENV-DE-3(0-5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2022
Supervised By :Ankita Jodhani 07/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:26:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

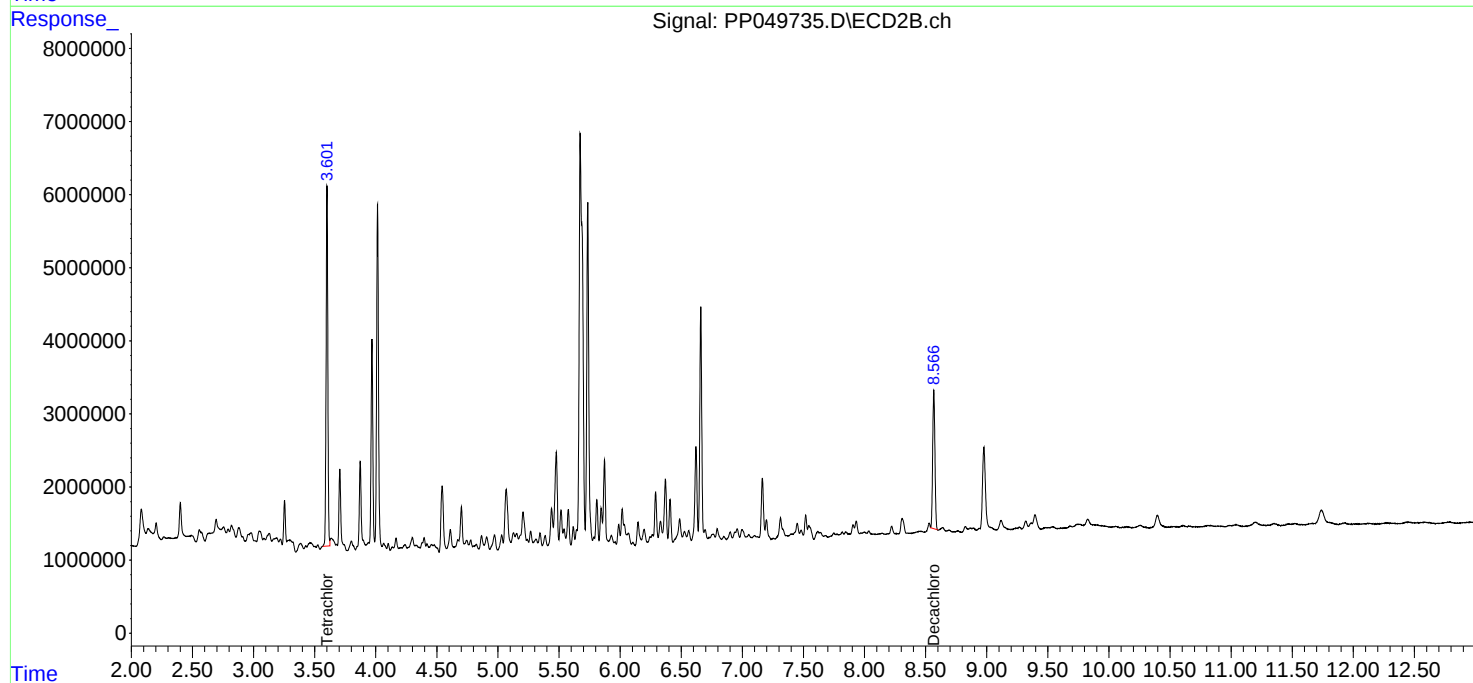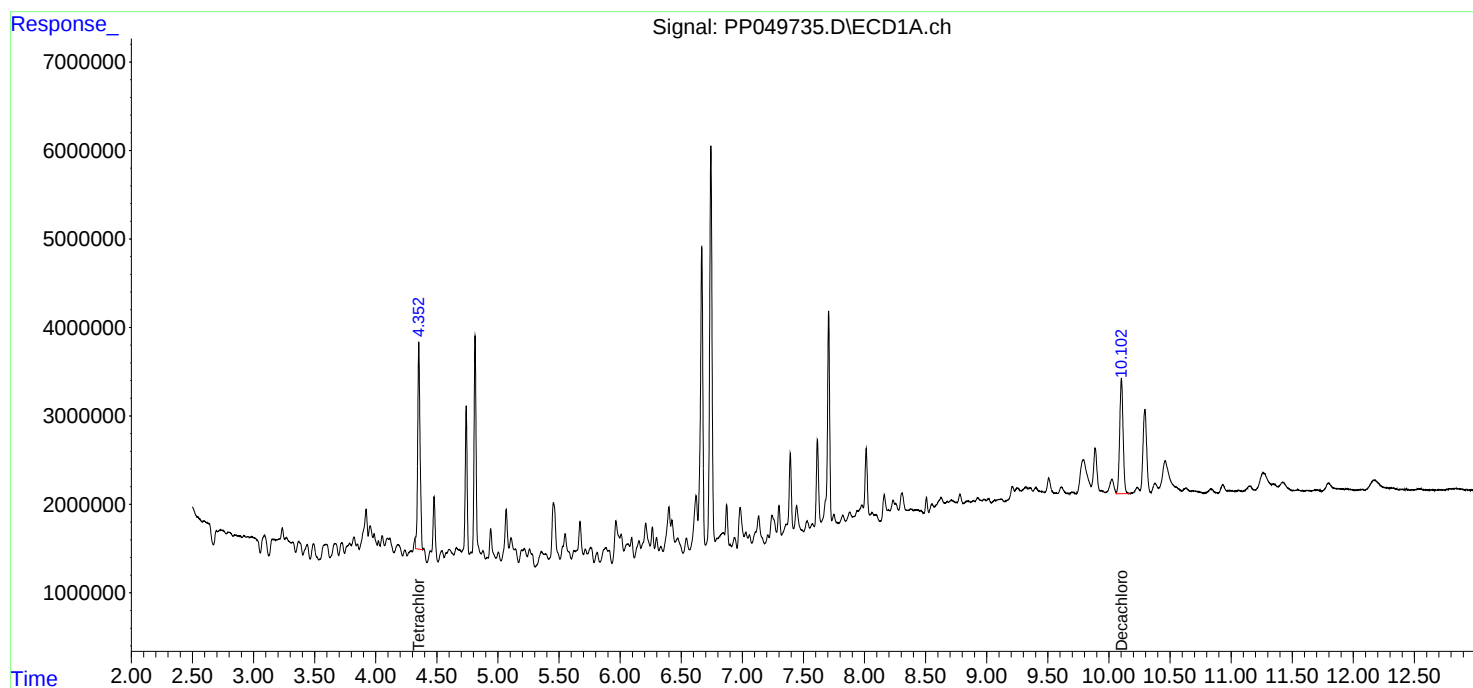

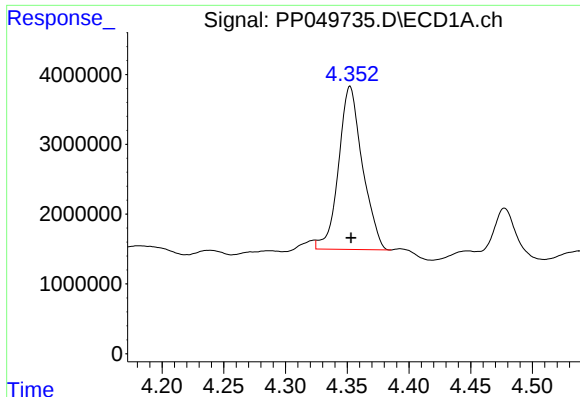

#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: -0.001 min
Response: 31363828
Conc: 21.61 ng/ml

Instrument :

ECD_P


ClientSampleId :

ENV-DE-3(0-5)

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/25/2022
Supervised By :Ankita Jodhani 07/25/2022

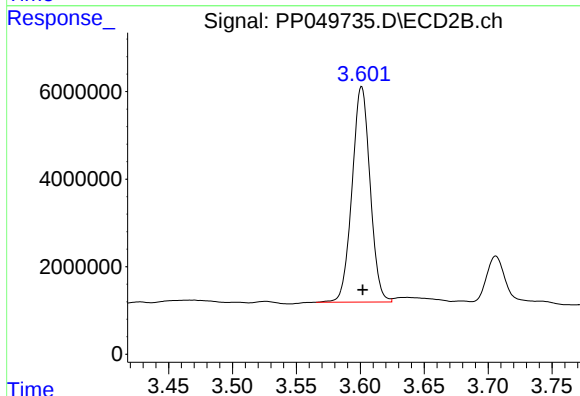


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 48408722
Conc: 19.80 ng/ml

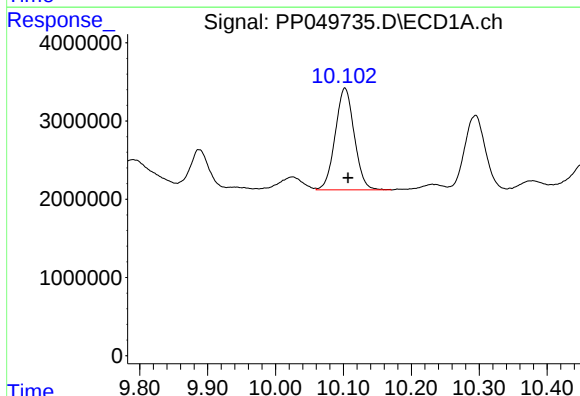

#2 Decachlorobiphenyl

R.T.: 10.102 min
Delta R.T.: -0.005 min
Response: 25326317
Conc: 17.91 ng/ml

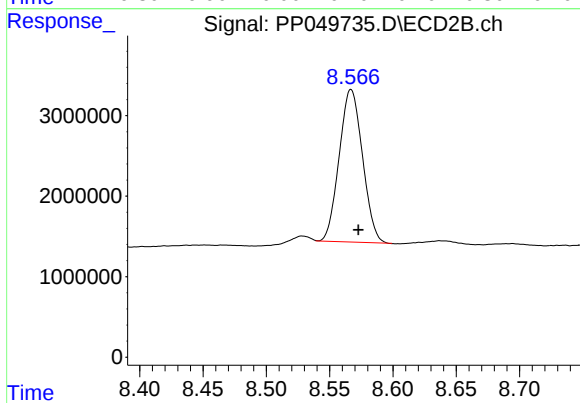

#2 Decachlorobiphenyl

R.T.: 8.566 min
Delta R.T.: -0.006 min
Response: 24270235
Conc: 20.84 ng/ml m