

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072224\
 Data File : PP066456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2024 11:02
 Operator : YP\AJ
 Sample : P3318-01 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-23-00118

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/23/2024
 Supervised By :Ankita Jodhani 07/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 11:52:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 07:20:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.025	1425153	3672644	0.809	1.923m#
2) SA Decachlor...	10.796	9.211	2289288	1867556	1.304m	1.464

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072224\
Data File : PP066456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2024 11:02
Operator : YP\AJ
Sample : P3318-01 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LAW-23-00118


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2024
Supervised By :Ankita Jodhani 07/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 11:52:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 07:20:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

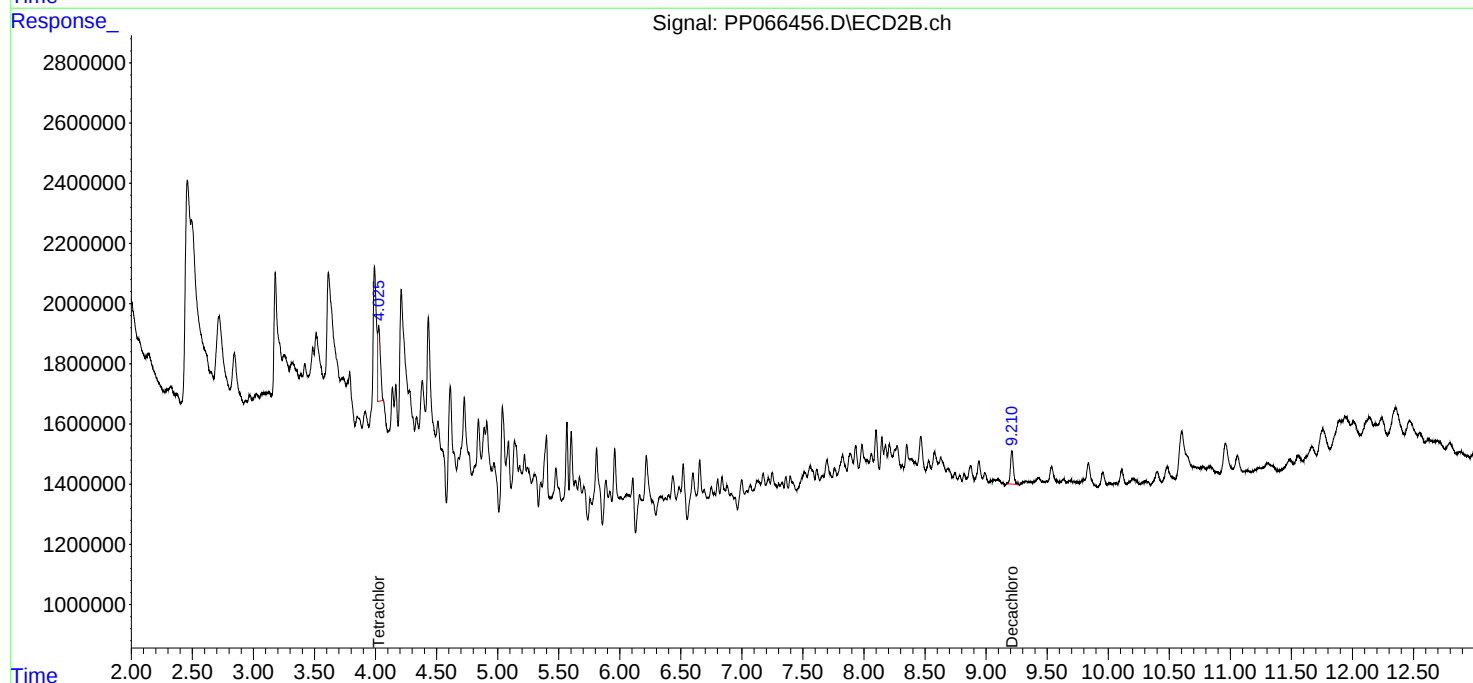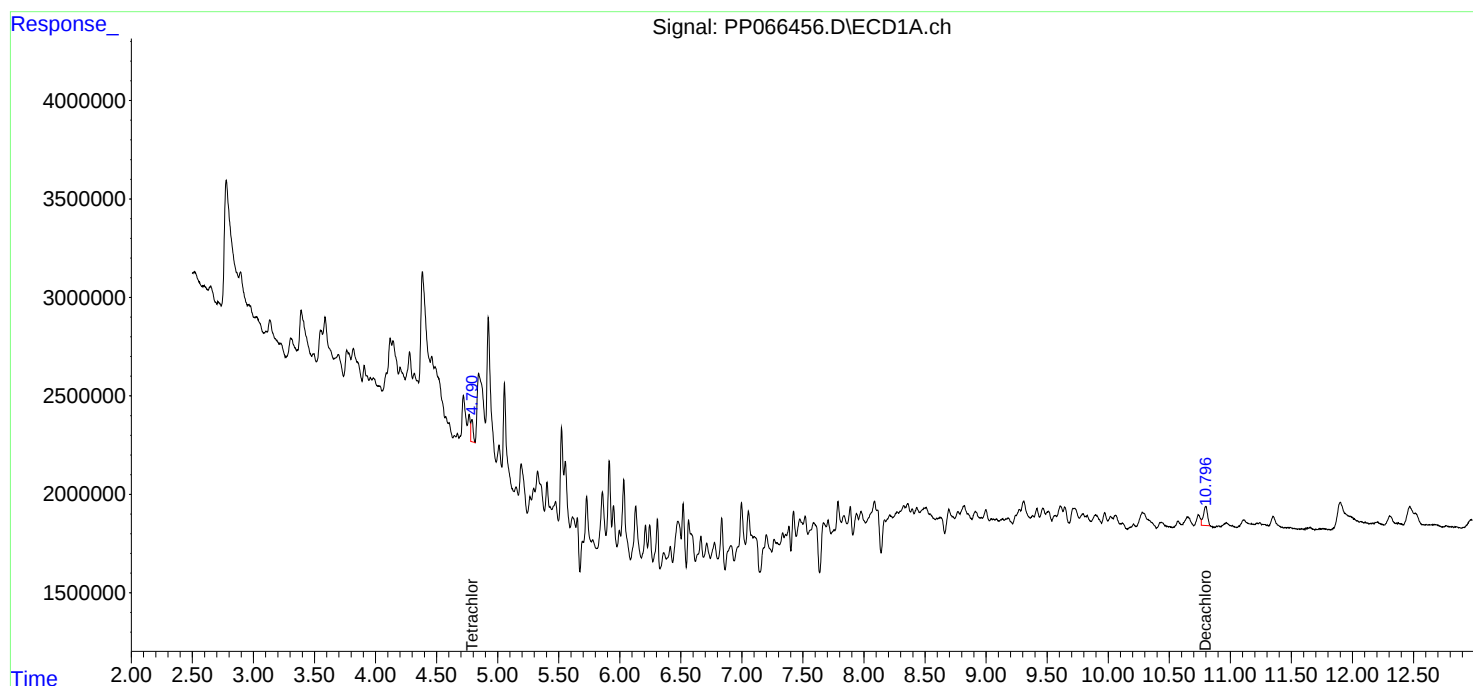

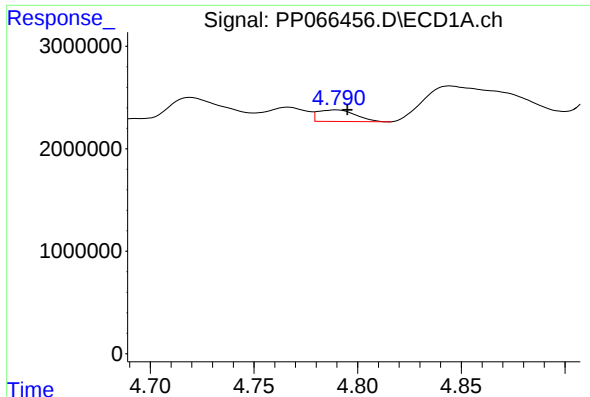

#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: -0.005 min
Response: 1425153
Conc: 0.81 ng/ml

Instrument :

ECD_P


ClientSampleId :

LAW-23-00118

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/23/2024
Supervised By :Ankita Jodhani 07/23/2024

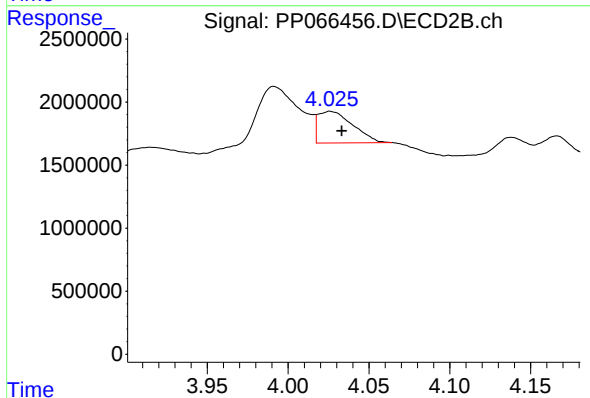


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: -0.008 min
Response: 3672644
Conc: 1.92 ng/ml m

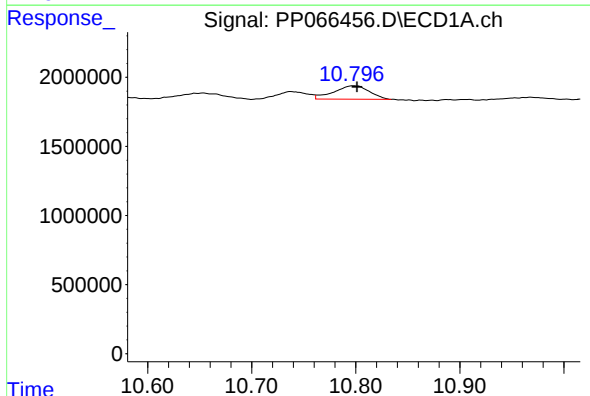

#2 Decachlorobiphenyl

R.T.: 10.796 min
Delta R.T.: -0.005 min
Response: 2289288
Conc: 1.30 ng/ml m

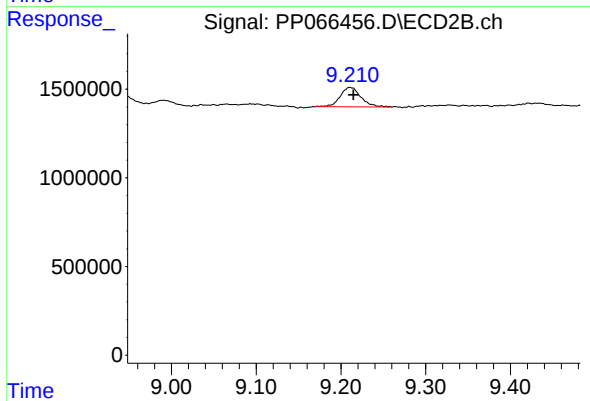

#2 Decachlorobiphenyl

R.T.: 9.211 min
Delta R.T.: -0.004 min
Response: 1867556
Conc: 1.46 ng/ml