

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
 Data File : PP037613.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 11:15
 Operator : DD\AJ
 Sample : PB137862BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 07:22:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.955	3.946	991654	575136	21.819	21.018
2)	SA Decachlor...	10.982	9.234	1007972	566758	21.896	20.361
Target Compounds							
8)	L2 AR-1221-1	5.205	0.000	57532	0	108.475	N.D. #
9)	L2 AR-1221-2	5.307	4.293	12206	13544	30.127	57.533 #
28)	L6 AR-1254-3	7.814	0.000	7873	0	2.554	N.D. #
30)	L6 AR-1254-5	8.505f	0.000	15983	0	6.387	N.D. #
33)	L7 AR-1260-3	8.572f	0.000	14365	0	7.107	N.D. #
35)	L7 AR-1260-5	9.178f	0.000	58169	0	12.606	N.D. #
36)	L8 AR-1262-1	8.572f	0.000	14365	0	4.932	N.D. #
37)	L8 AR-1262-2	9.178f	0.000	58169	0	11.076	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
Data File : PP037613.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 11:15
Operator : DD\AJ
Sample : PB137862BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 07:22:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

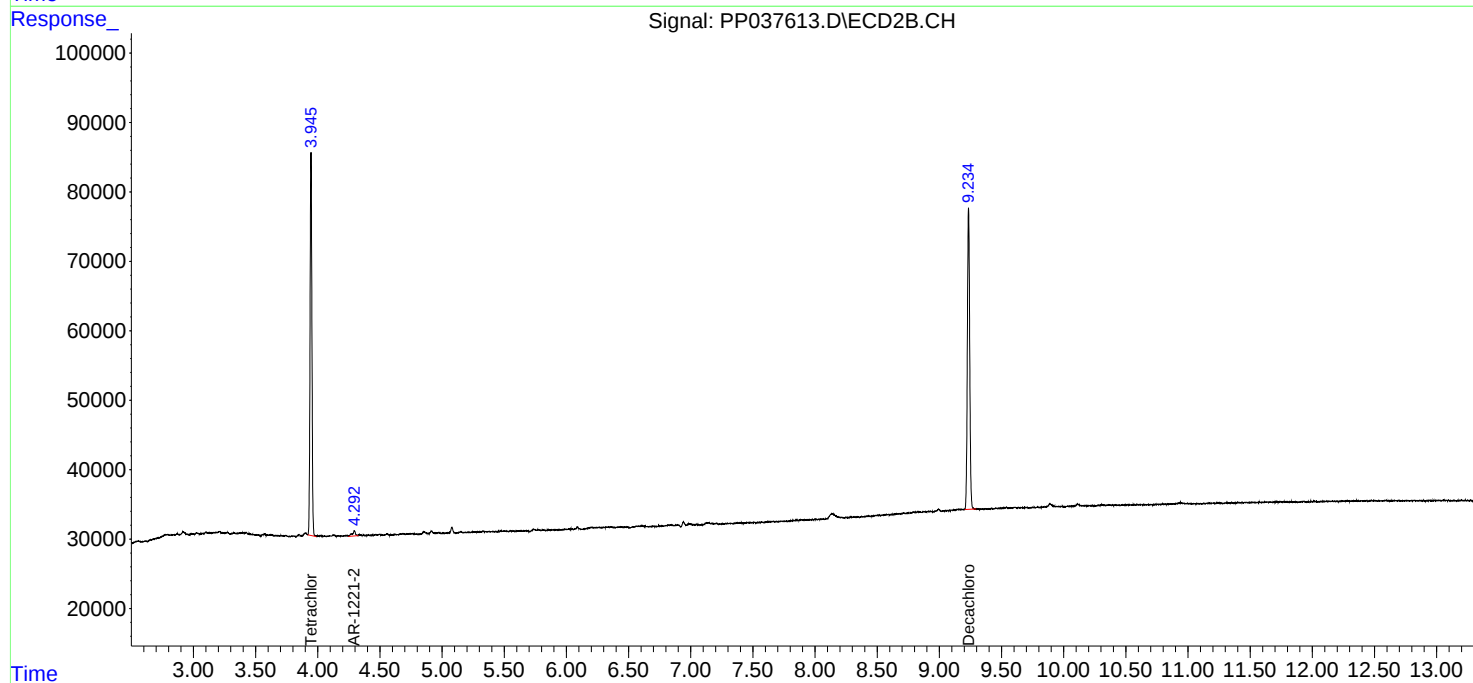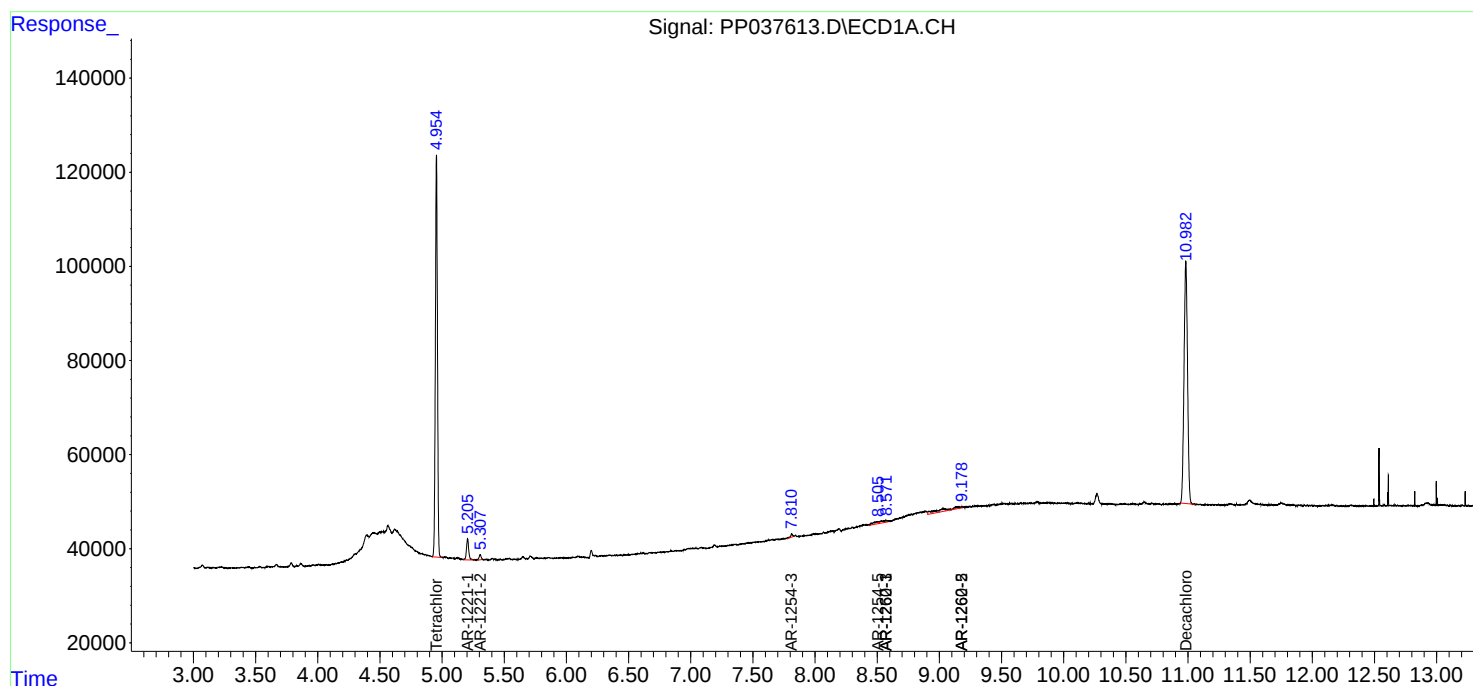


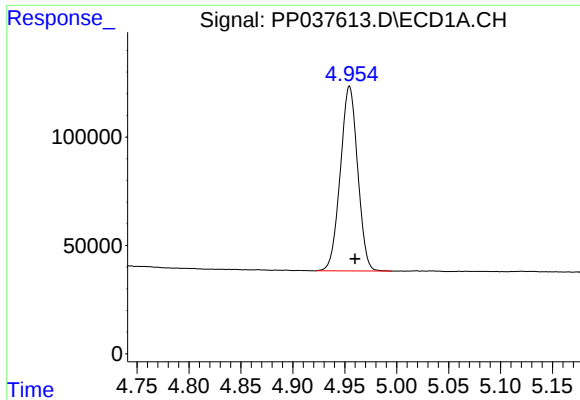

#1 Tetrachloro-m-xylene


R.T.: 4.955 min
Delta R.T.: -0.005 min
Response: 991654
Conc: 21.82 ng/ml

Instrument :
ECD_P
ClientSampleId :

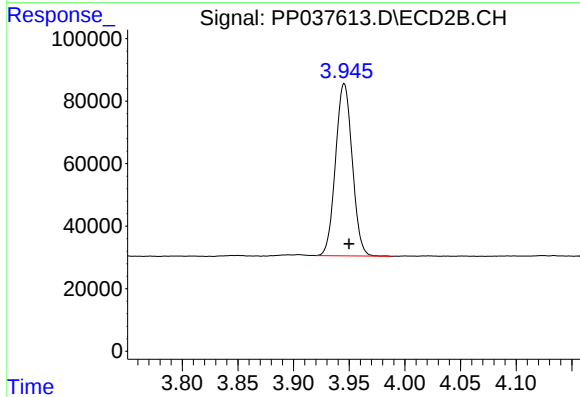


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 575136
Conc: 21.02 ng/ml

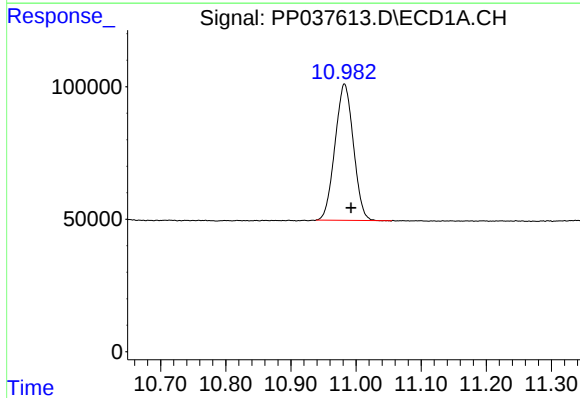


#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.010 min
Response: 1007972
Conc: 21.90 ng/ml

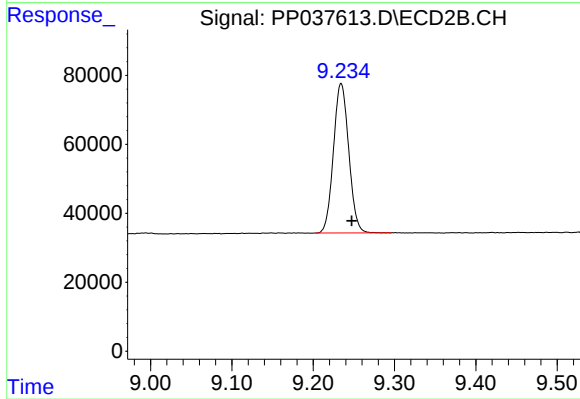

#2 Decachlorobiphenyl


R.T.: 9.234 min
Delta R.T.: -0.013 min
Response: 566758
Conc: 20.36 ng/ml

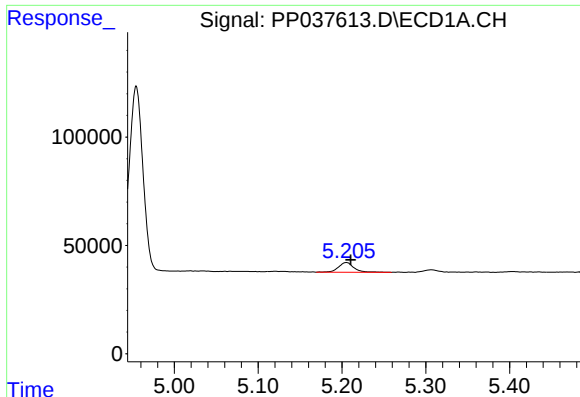

#8 AR-1221-1


R.T.: 5.205 min
Delta R.T.: -0.005 min
Response: 57532
Conc: 108.47 ng/ml

Instrument :
ECD_P
ClientSampleId :

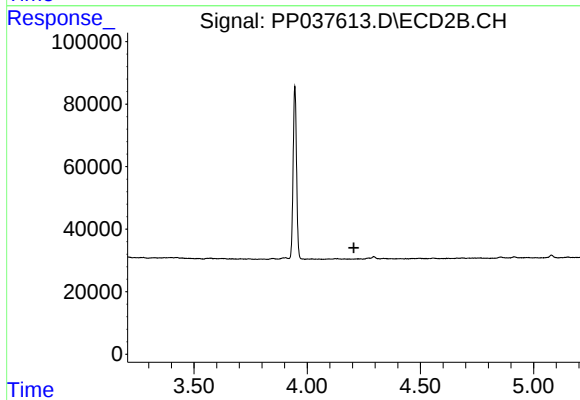


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

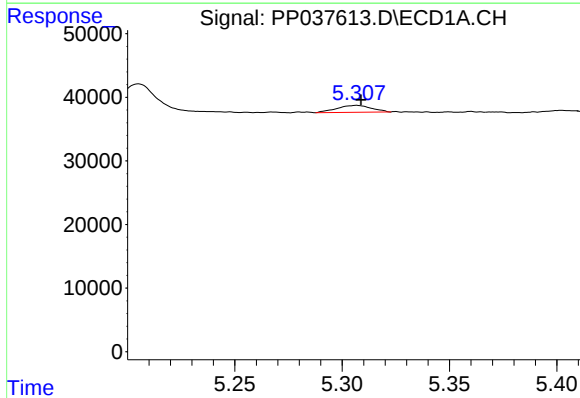


#9 AR-1221-2

R.T.: 5.307 min
Delta R.T.: -0.002 min
Response: 12206
Conc: 30.13 ng/ml

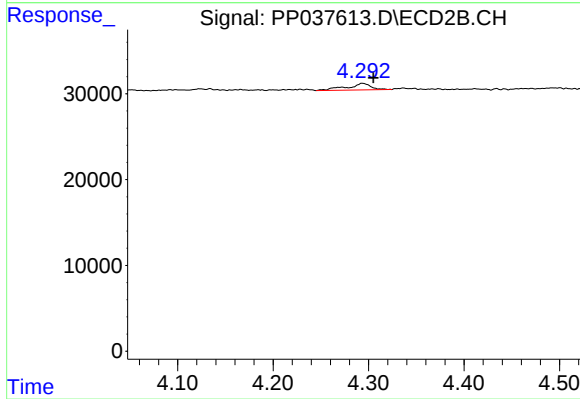

#9 AR-1221-2


R.T.: 4.293 min
Delta R.T.: -0.012 min
Response: 13544
Conc: 57.53 ng/ml

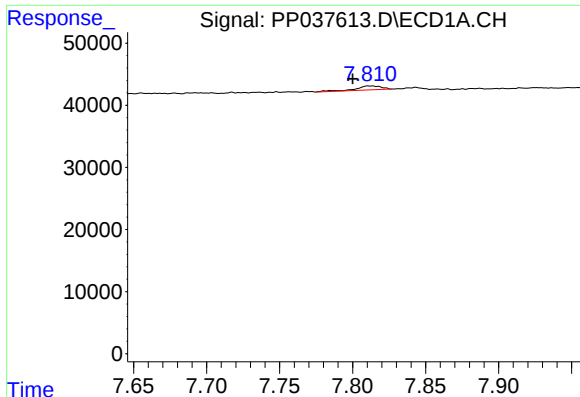

#28 AR-1254-3


R.T.: 7.814 min
Delta R.T.: 0.014 min
Response: 7873
Conc: 2.55 ng/ml

Instrument :
ECD_P
ClientSampleId :

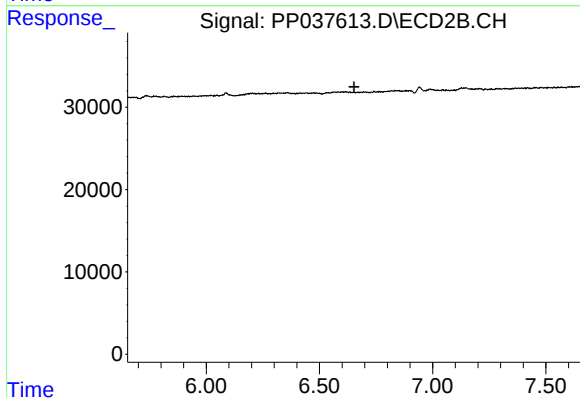


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

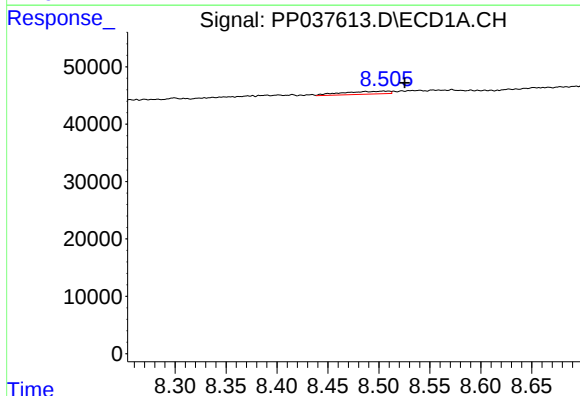


#30 AR-1254-5

R.T.: 8.505 min
Delta R.T.: -0.020 min
Response: 15983
Conc: 6.39 ng/ml

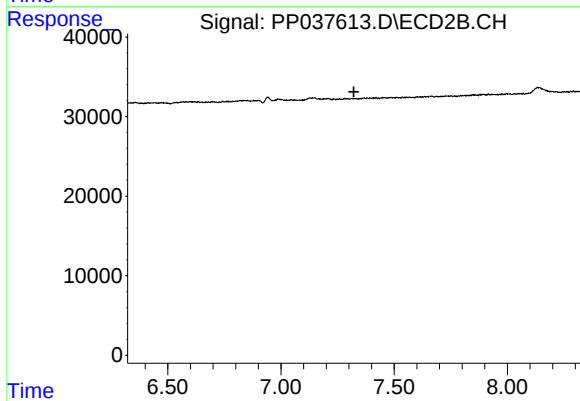

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.322 min
Response: 0
Conc: N.D.

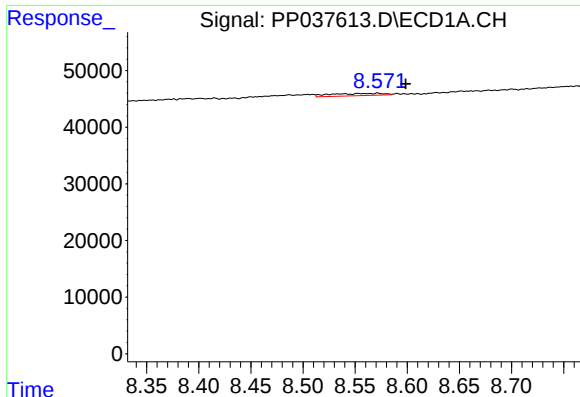

#33 AR-1260-3


R.T.: 8.572 min
Delta R.T.: -0.027 min
Response: 14365
Conc: 7.11 ng/ml

Instrument :
ECD_P
ClientSampleId :

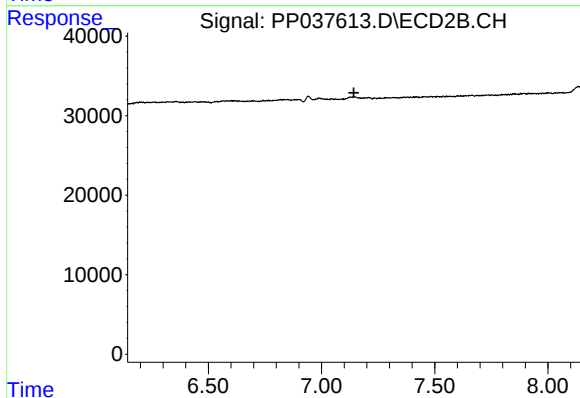


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.143 min
Response: 0
Conc: N.D.

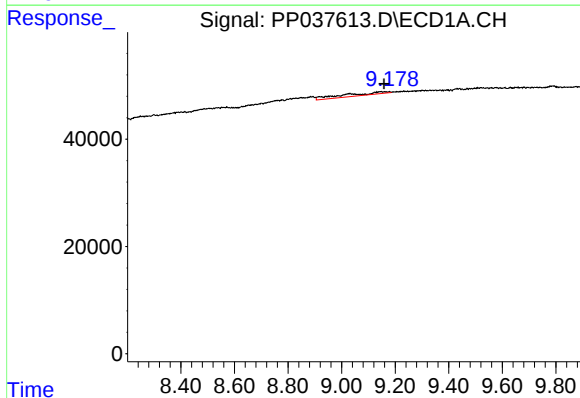


#35 AR-1260-5

R.T.: 9.178 min
Delta R.T.: 0.020 min
Response: 58169
Conc: 12.61 ng/ml

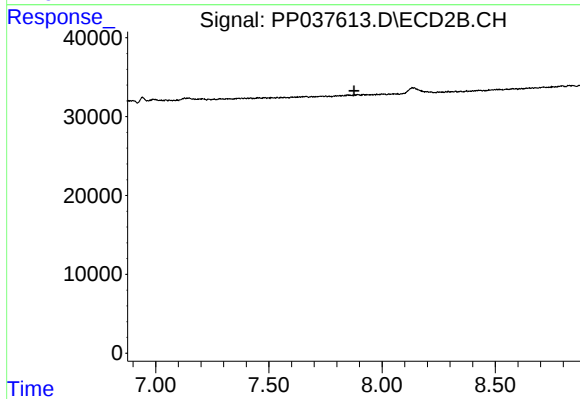

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.876 min
Response: 0
Conc: N.D.

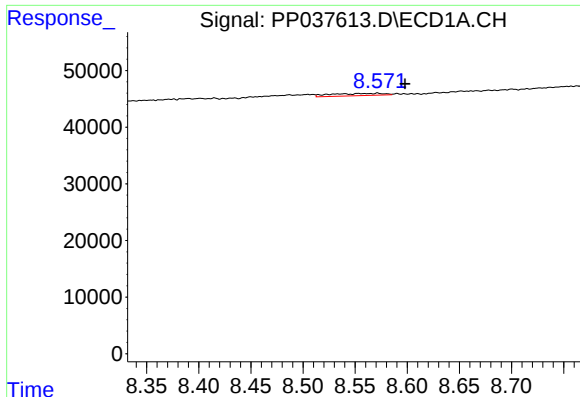

#36 AR-1262-1


R.T.: 8.572 min
Delta R.T.: -0.026 min
Response: 14365
Conc: 4.93 ng/ml

Instrument :
ECD_P
ClientSampleId :

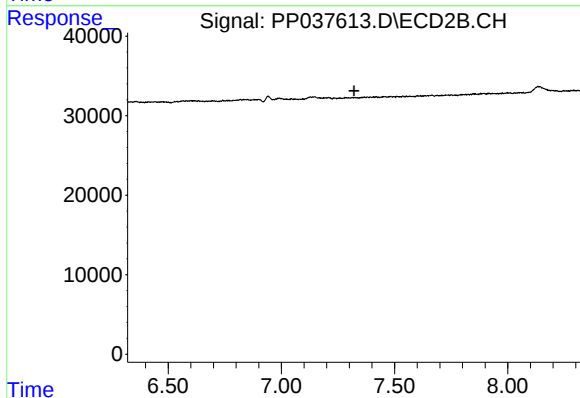


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.321 min
Response: 0
Conc: N.D.

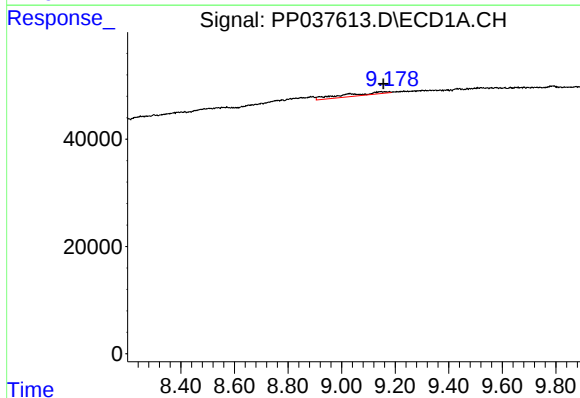

#37 AR-1262-2

R.T.: 9.178 min
Delta R.T.: 0.022 min
Response: 58169
Conc: 11.08 ng/ml

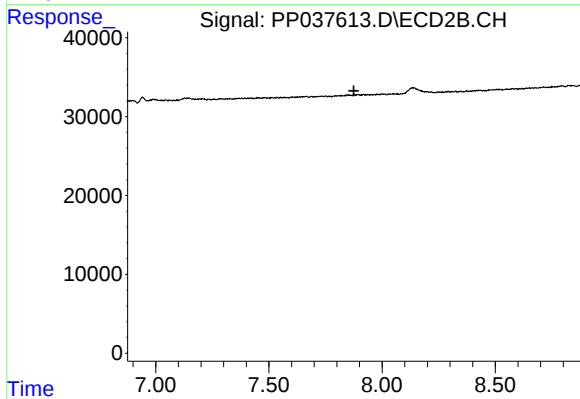

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.875 min
Response: 0
Conc: N.D.