

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
 Data File : PP037621.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 14:14
 Operator : DD\AJ
 Sample : M3138-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VB16085

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 07:26:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.956	3.946	878166	486543	19.322	17.780
2)	SA Decachlor...	10.984	9.236	711038	363377	15.445	13.055
Target Compounds							
8)	L2 AR-1221-1	5.205	0.000	11453	0	21.595	N.D. #
9)	L2 AR-1221-2	5.307	0.000	10311	0	25.450	N.D. #
20)	L4 AR-1242-5	7.235f	0.000	1248	0	1.200	N.D. #
24)	L5 AR-1248-4	7.213	0.000	1968	0	1.041	N.D. #
25)	L5 AR-1248-5	7.235f	0.000	1248	0	0.667	N.D. #
26)	L6 AR-1254-1	7.191	0.000	21448	0	11.939	N.D. #
28)	L6 AR-1254-3	7.811	0.000	12962	0	4.204	N.D. #
32)	L7 AR-1260-2	8.229	0.000	7612	0	2.736	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
Data File : PP037621.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 14:14
Operator : DD\AJ
Sample : M3138-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
VB16085

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 07:26:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

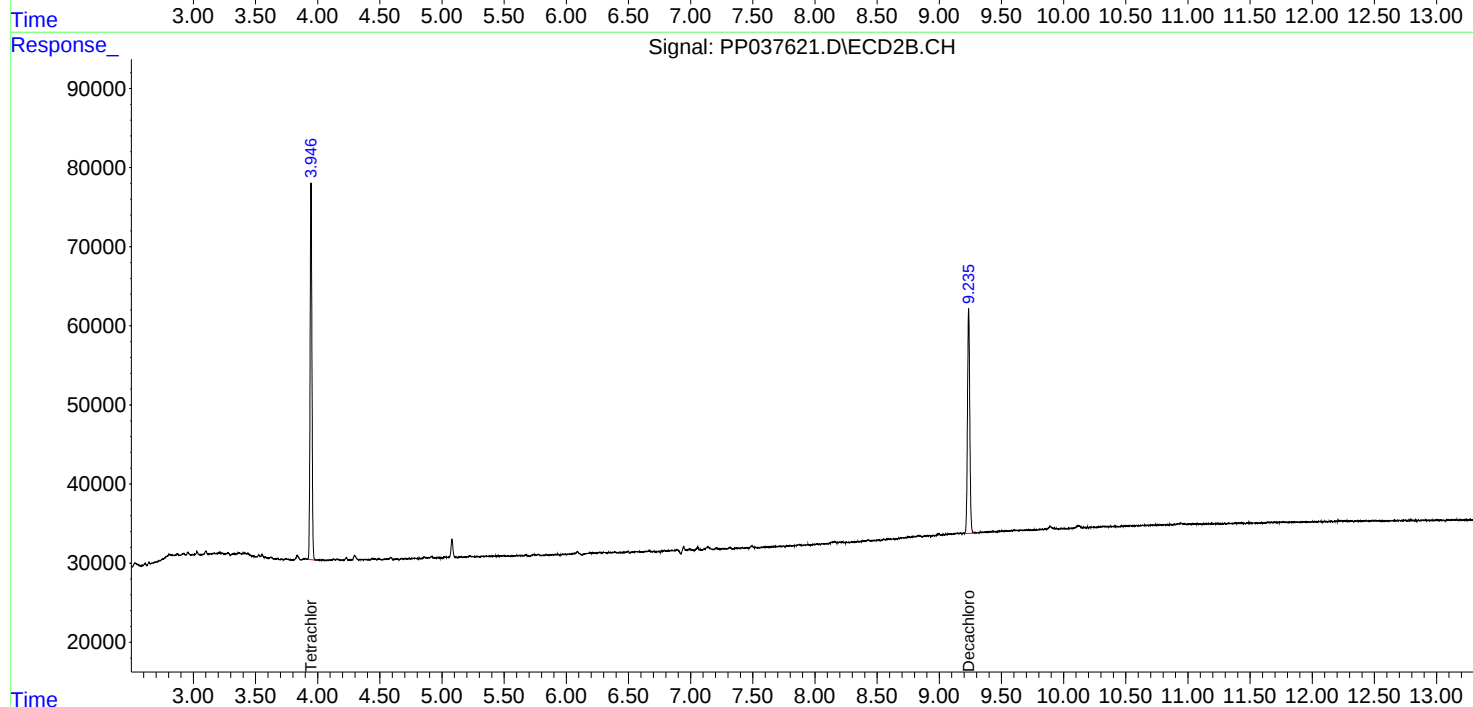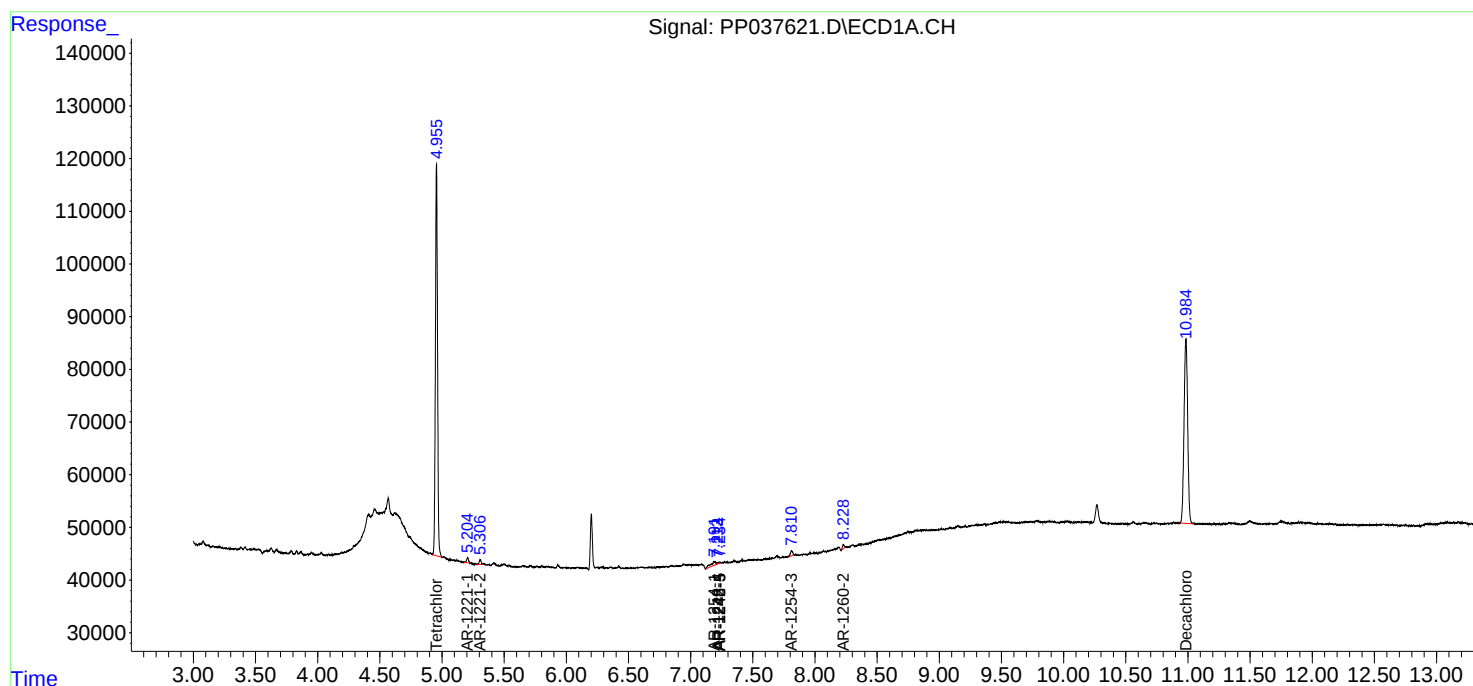


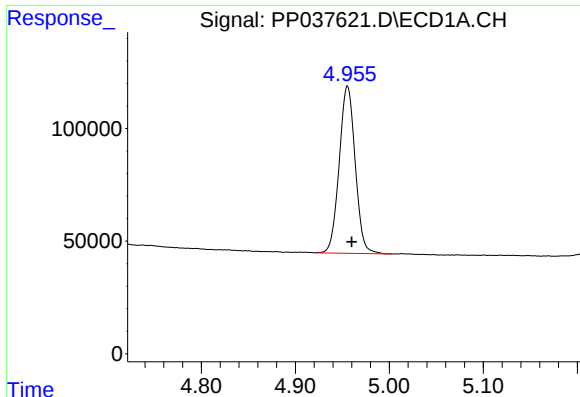

#1 Tetrachloro-m-xylene


R.T.: 4.956 min
Delta R.T.: -0.004 min
Response: 878166
Conc: 19.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
VB16085

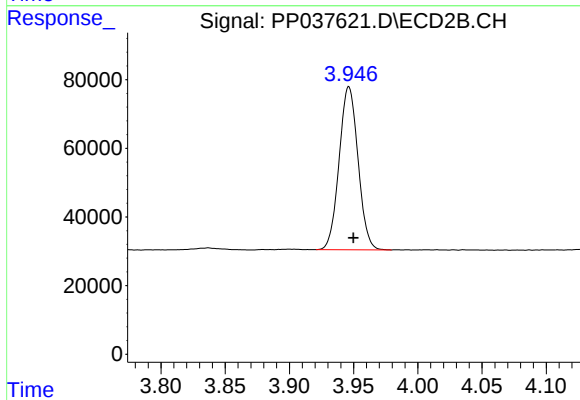


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 486543
Conc: 17.78 ng/ml

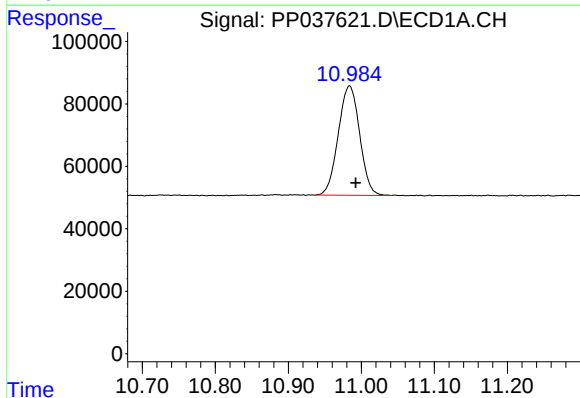


#2 Decachlorobiphenyl

R.T.: 10.984 min
Delta R.T.: -0.008 min
Response: 711038
Conc: 15.45 ng/ml

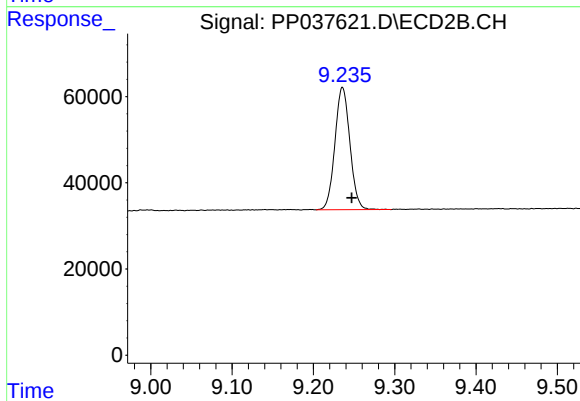

#2 Decachlorobiphenyl


R.T.: 9.236 min
Delta R.T.: -0.012 min
Response: 363377
Conc: 13.05 ng/ml

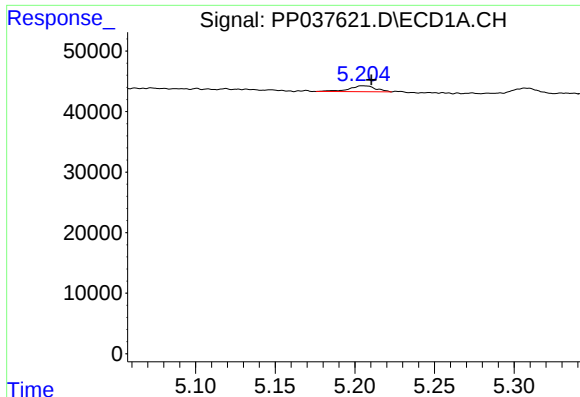

#8 AR-1221-1


R.T.: 5.205 min
Delta R.T.: -0.006 min
Response: 11453
Conc: 21.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
VB16085

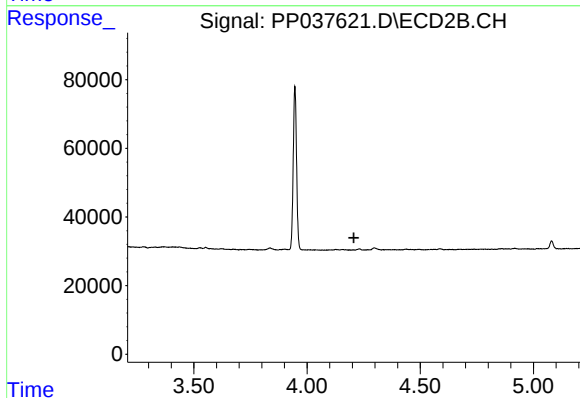


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

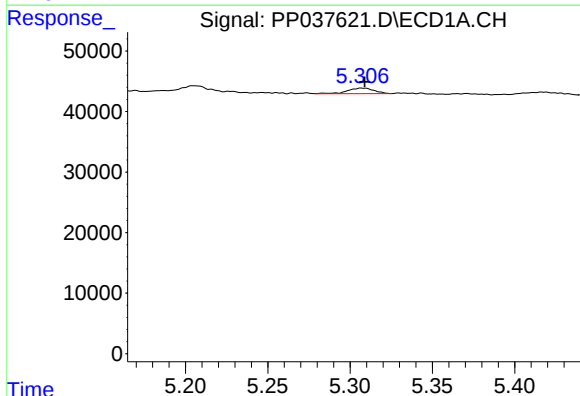


#9 AR-1221-2

R.T.: 5.307 min
Delta R.T.: -0.002 min
Response: 10311
Conc: 25.45 ng/ml

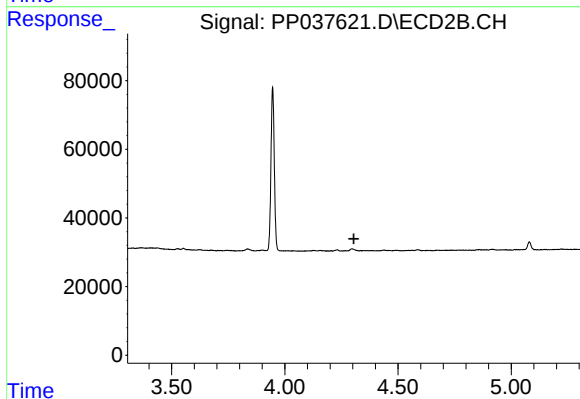

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.305 min
Response: 0
Conc: N.D.

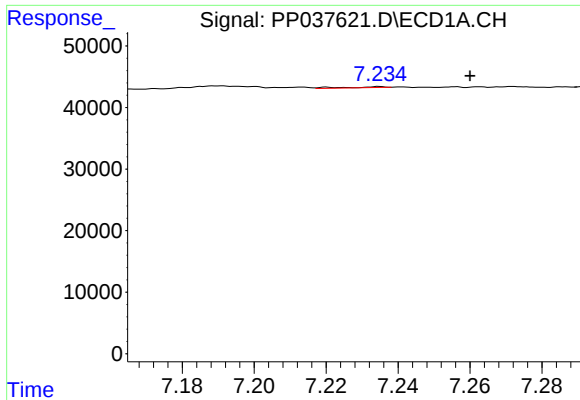

#20 AR-1242-5


R.T.: 7.235 min
Delta R.T.: -0.025 min
Response: 1248
Conc: 1.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
VB16085

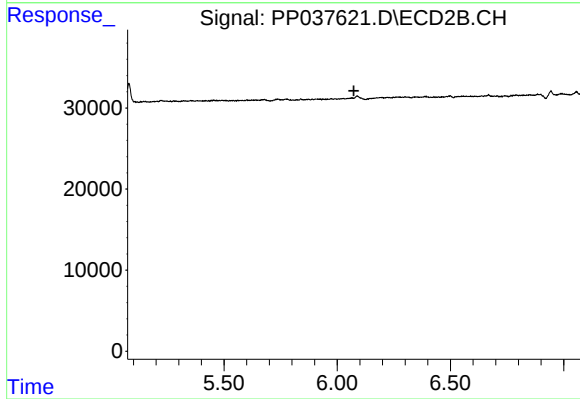


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

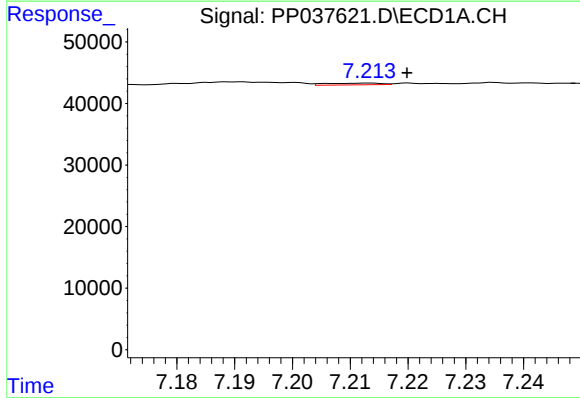


#24 AR-1248-4

R.T.: 7.213 min
Delta R.T.: -0.007 min
Response: 1968
Conc: 1.04 ng/ml

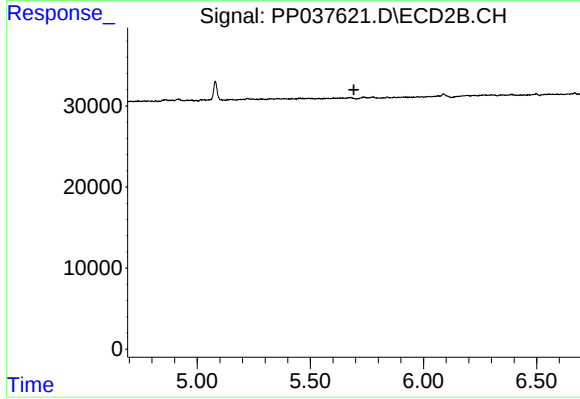

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.692 min
Response: 0
Conc: N.D.

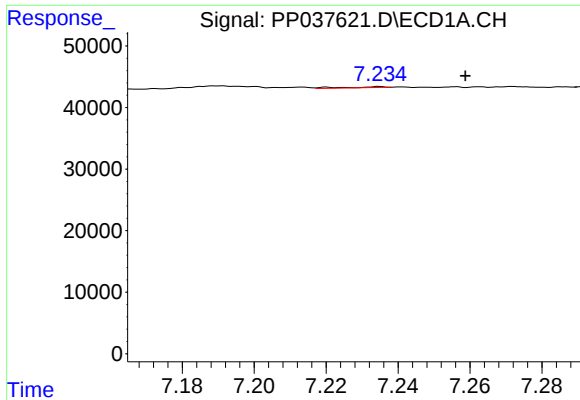

#25 AR-1248-5


R.T.: 7.235 min
Delta R.T.: -0.024 min
Response: 1248
Conc: 0.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
VB16085

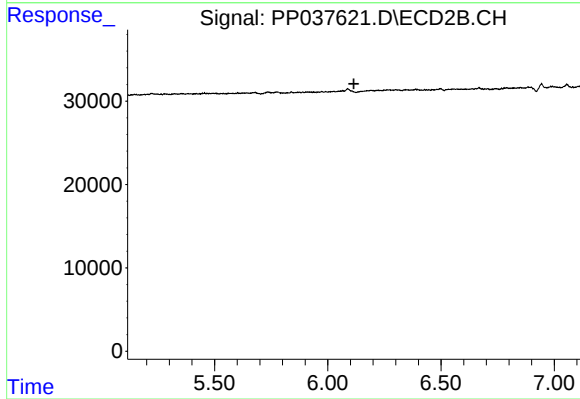


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

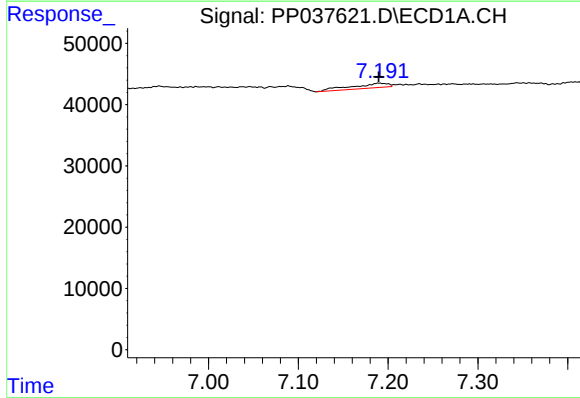


#26 AR-1254-1

R.T.: 7.191 min
Delta R.T.: 0.002 min
Response: 21448
Conc: 11.94 ng/ml

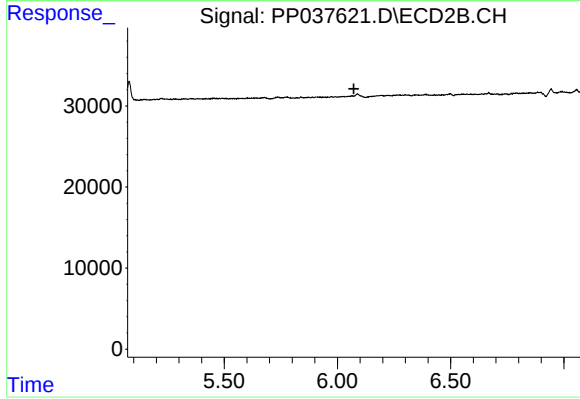

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

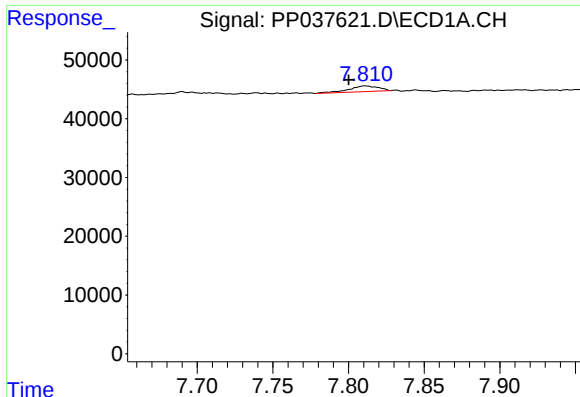

#28 AR-1254-3


R.T.: 7.811 min
Delta R.T.: 0.011 min
Response: 12962
Conc: 4.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
VB16085

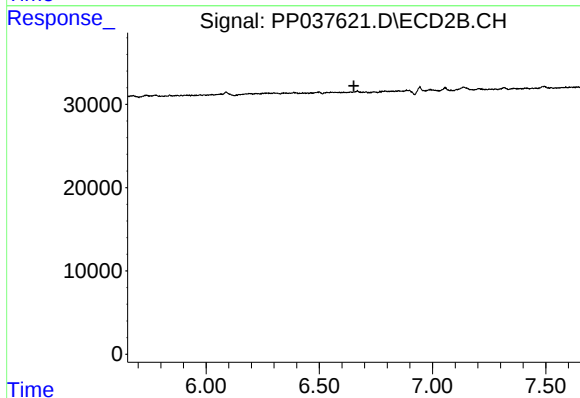


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

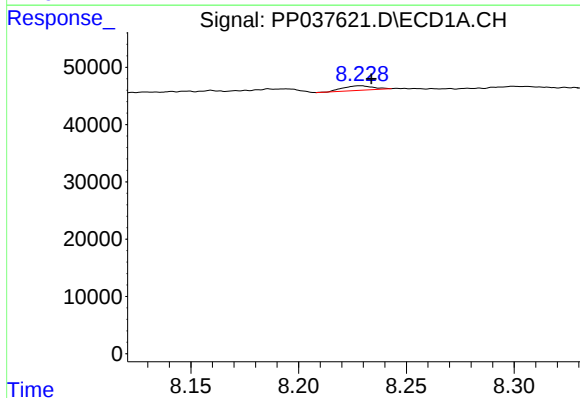

#32 AR-1260-2

R.T.: 8.229 min
Delta R.T.: -0.005 min
Response: 7612
Conc: 2.74 ng/ml

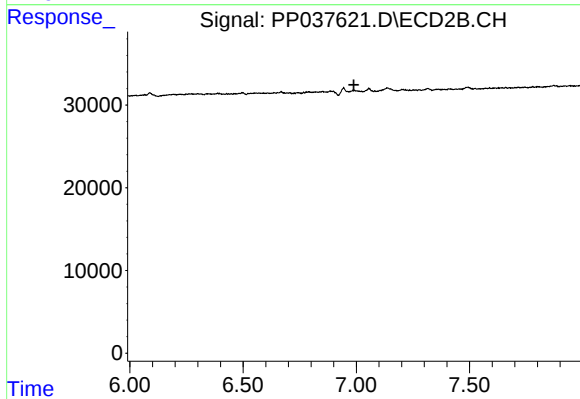

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.