

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
 Data File : PP037634.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 17:57
 Operator : DD\AJ
 Sample : M3152-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VAULT-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 07:32:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.955	3.947	1261324	716100	27.752	26.169
2)	SA Decachlor...	10.982	9.236	1217680	642192	26.451	23.071
Target Compounds							
8)	L2 AR-1221-1	5.206	0.000	72664	0	137.006	N.D. #
9)	L2 AR-1221-2	5.307	4.296	16455	10365	40.617	44.029
24)	L5 AR-1248-4	7.224	0.000	1588	0	0.840	N.D. #
26)	L6 AR-1254-1	7.190	0.000	10148	0	5.649	N.D. #
27)	L6 AR-1254-2	7.424	0.000	16287	0	5.855	N.D. #
28)	L6 AR-1254-3	7.813	0.000	9496	0	3.080	N.D. #
32)	L7 AR-1260-2	8.245	0.000	7241	0	2.603	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
Data File : PP037634.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 17:57
Operator : DD\AJ
Sample : M3152-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
VAULT-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 07:32:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

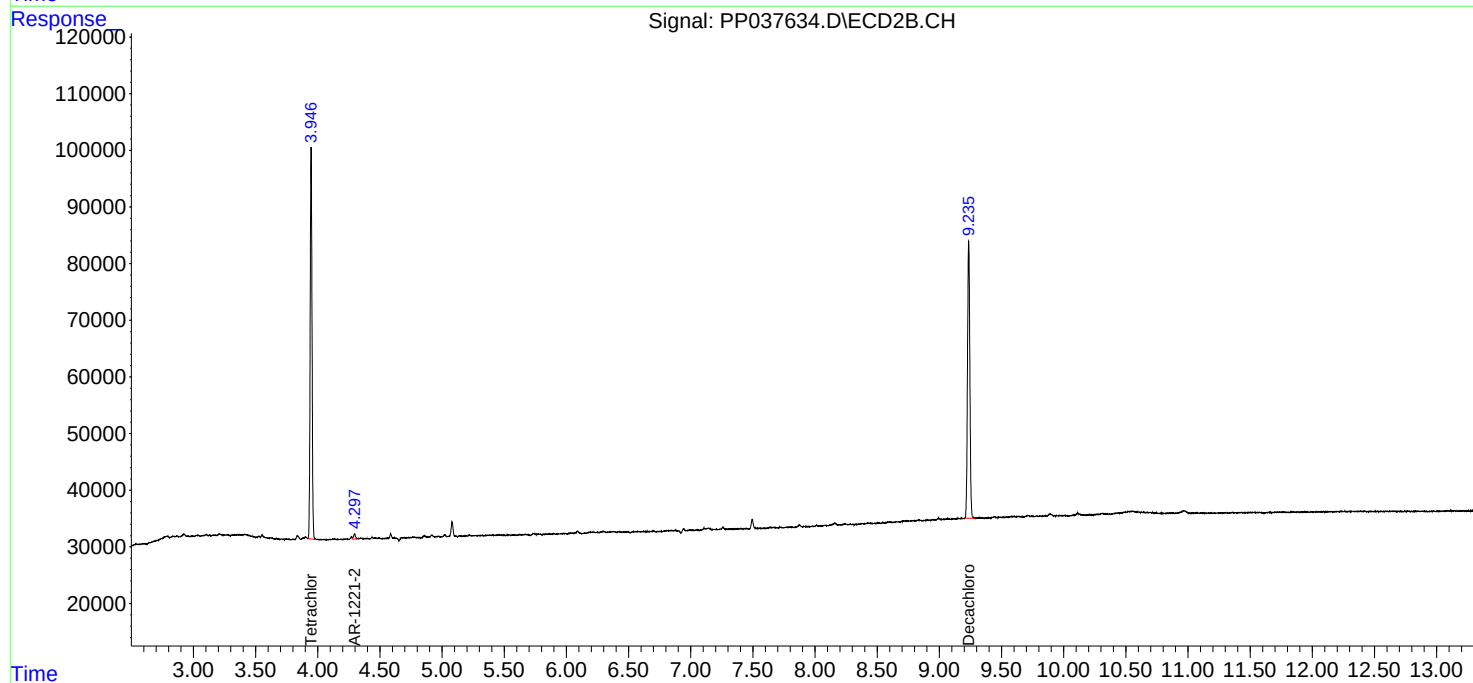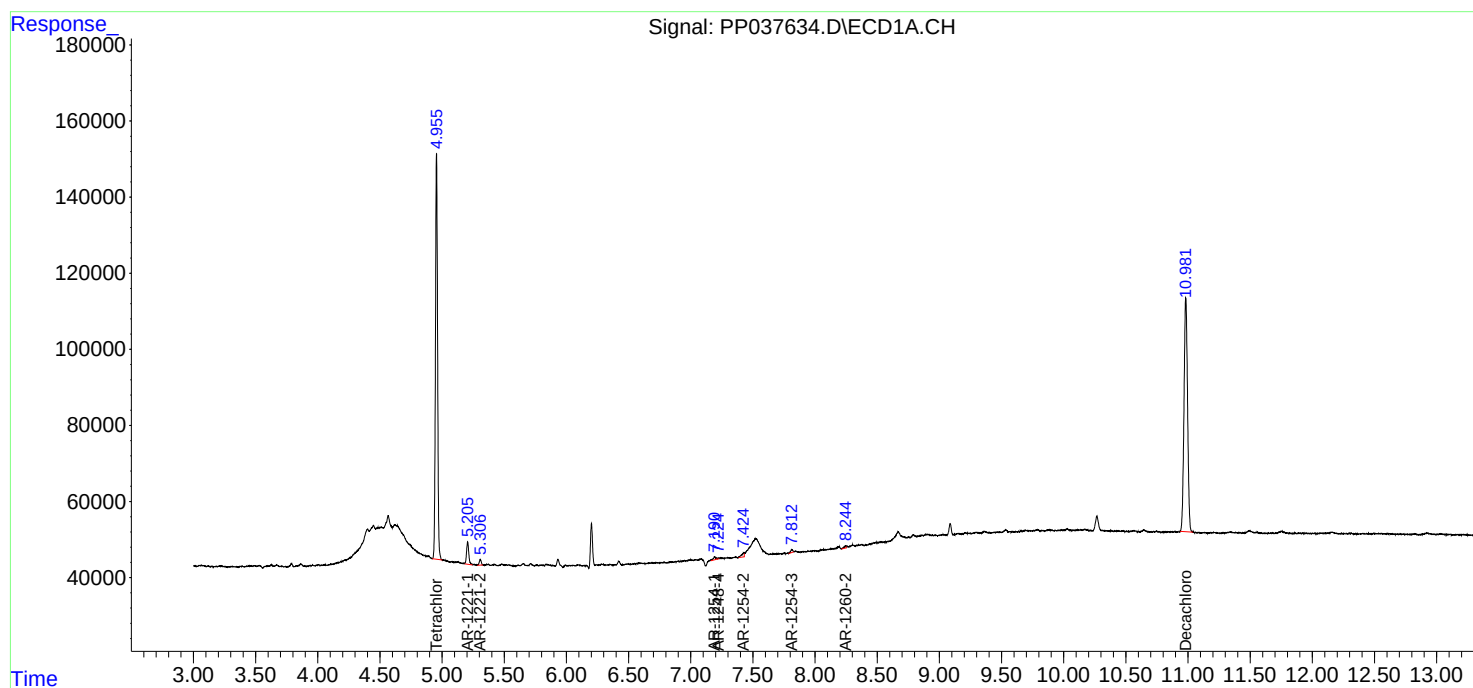


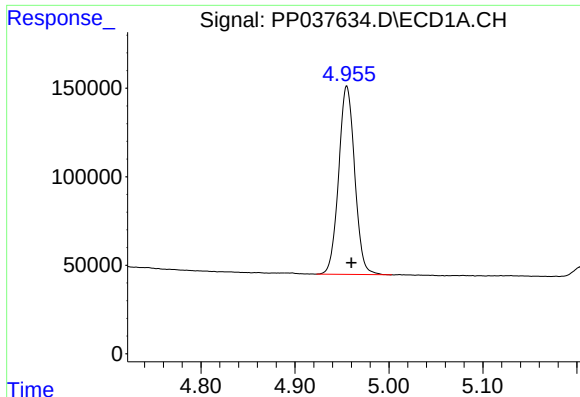

#1 Tetrachloro-m-xylene


R.T.: 4.955 min
Delta R.T.: -0.005 min
Response: 1261324
Conc: 27.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAULT-B

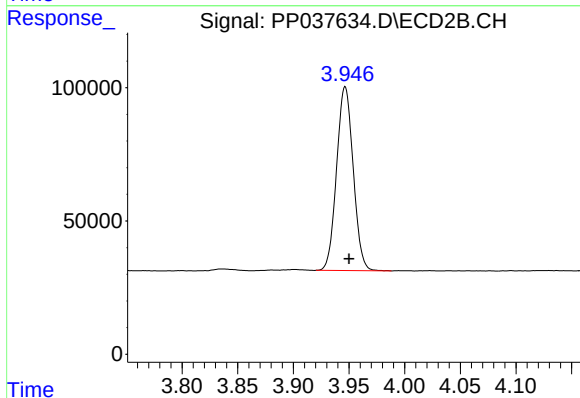


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.003 min
Response: 716100
Conc: 26.17 ng/ml

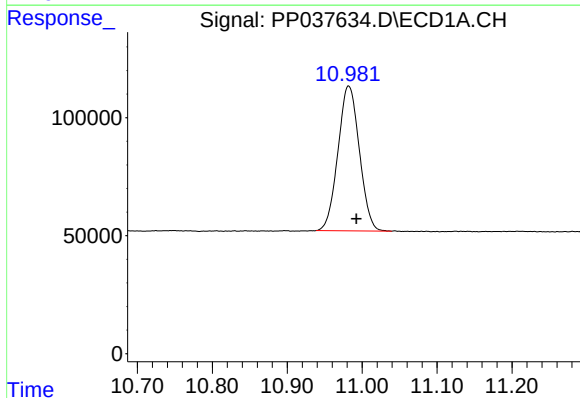


#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.010 min
Response: 1217680
Conc: 26.45 ng/ml

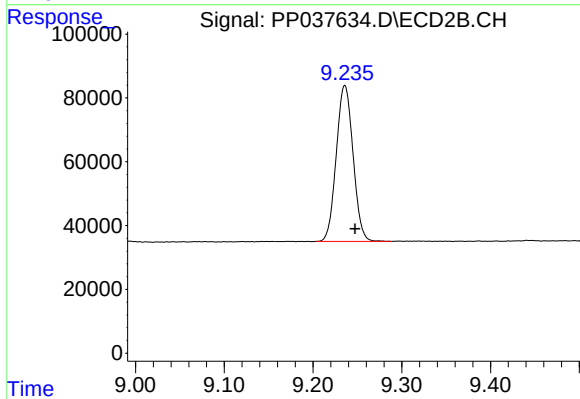

#2 Decachlorobiphenyl


R.T.: 9.236 min
Delta R.T.: -0.011 min
Response: 642192
Conc: 23.07 ng/ml

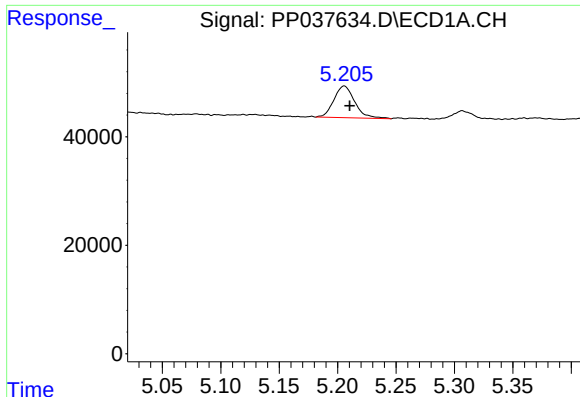

#8 AR-1221-1


R.T.: 5.206 min
Delta R.T.: -0.005 min
Response: 72664
Conc: 137.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAULT-B

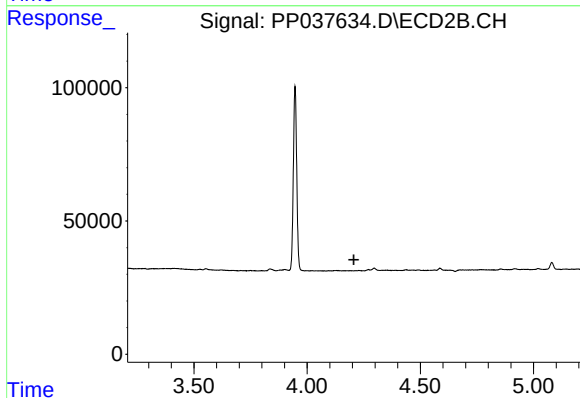


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

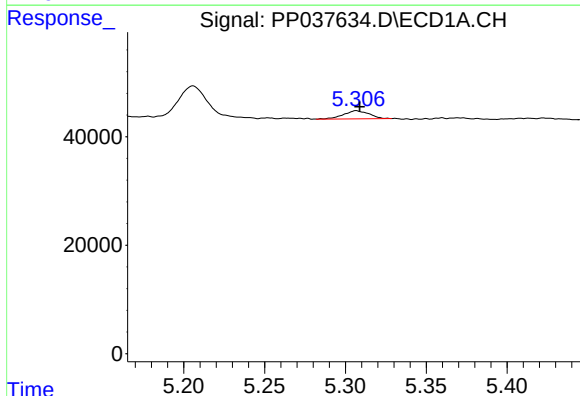


#9 AR-1221-2

R.T.: 5.307 min
Delta R.T.: -0.002 min
Response: 16455
Conc: 40.62 ng/ml

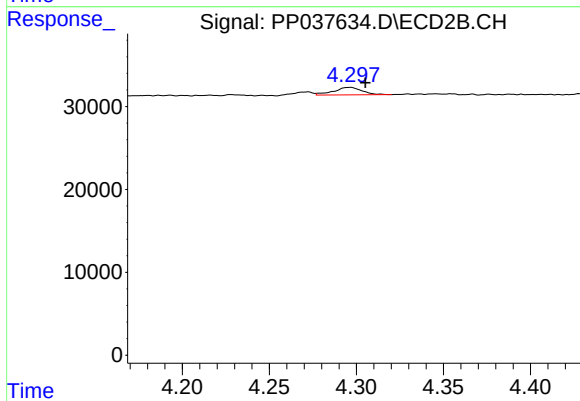

#9 AR-1221-2


R.T.: 4.296 min
Delta R.T.: -0.009 min
Response: 10365
Conc: 44.03 ng/ml

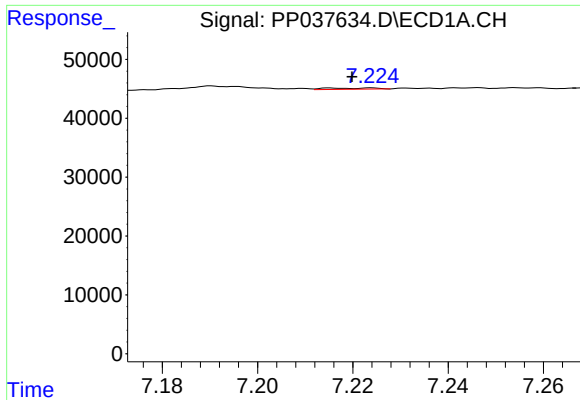

#24 AR-1248-4


R.T.: 7.224 min
Delta R.T.: 0.004 min
Response: 1588
Conc: 0.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAULT-B

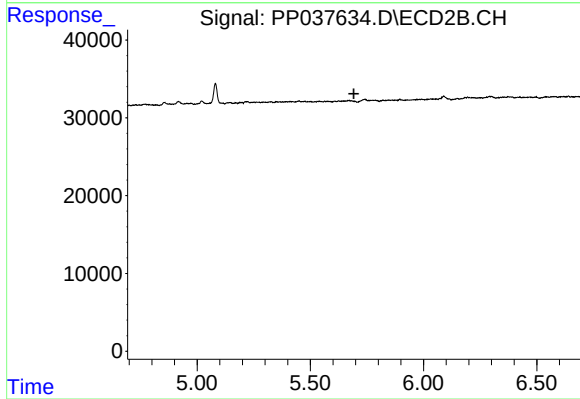


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.692 min
Response: 0
Conc: N.D.

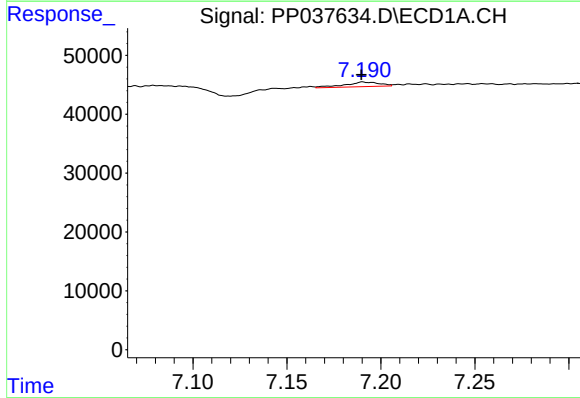


#26 AR-1254-1

R.T.: 7.190 min
Delta R.T.: 0.000 min
Response: 10148
Conc: 5.65 ng/ml

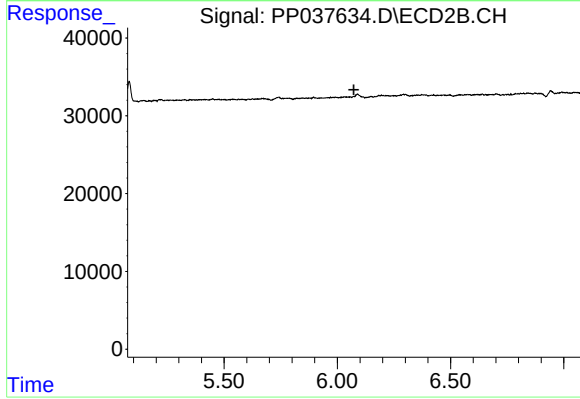

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

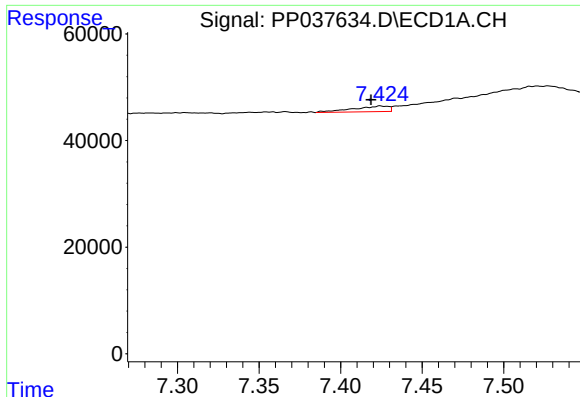

#27 AR-1254-2


R.T.: 7.424 min
Delta R.T.: 0.006 min
Response: 16287
Conc: 5.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAULT-B

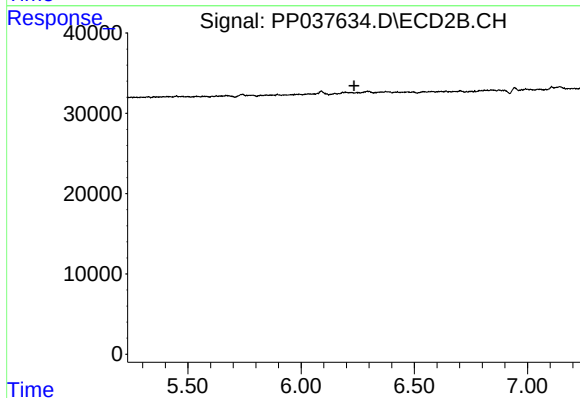


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

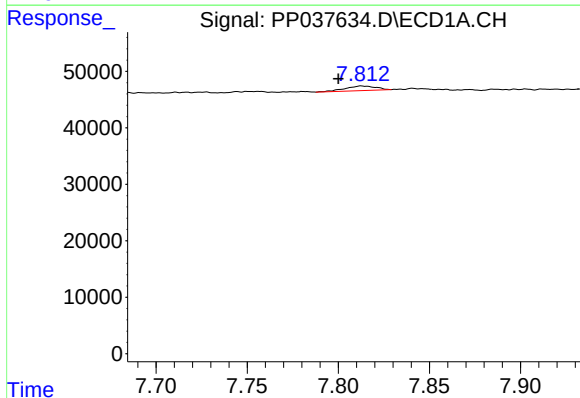


#28 AR-1254-3

R.T.: 7.813 min
Delta R.T.: 0.013 min
Response: 9496
Conc: 3.08 ng/ml

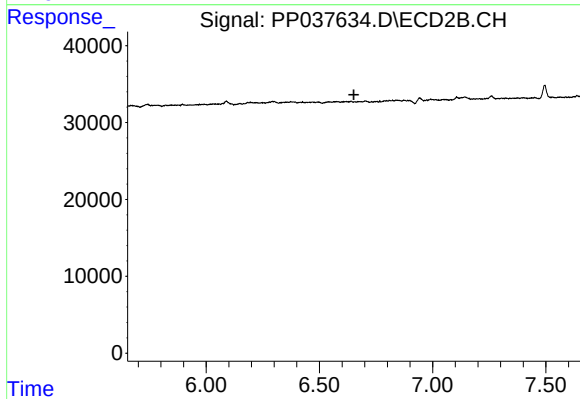

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

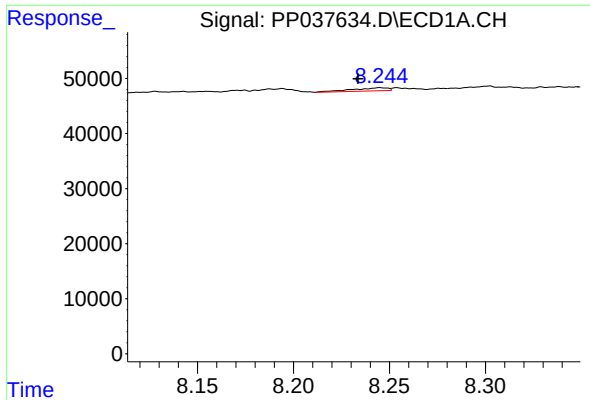

#32 AR-1260-2

R.T.: 8.245 min
Delta R.T.: 0.011 min
Response: 7241
Conc: 2.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAULT-B

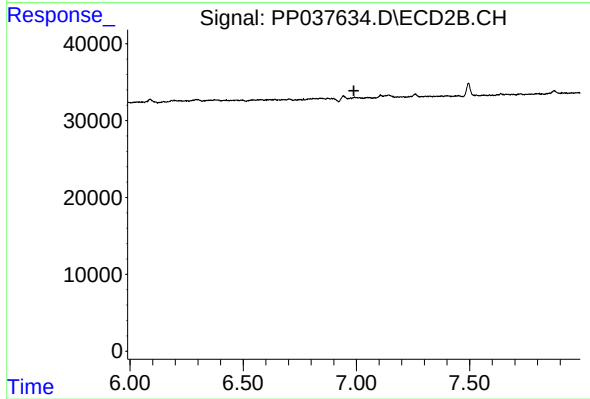

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.