

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
 Data File : PP037617.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 13:07
 Operator : DD\AJ
 Sample : M3133-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PIPE-TRE-1236

Manual Integrations
 APPROVED

mohammad
 7/26/2021 11:56:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 07:24:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.954	3.945	761213	425000	16.749	15.531
2) SA Decachlor...	10.982	9.234	768756	389291	16.699	13.986
Target Compounds						
26) L6 AR-1254-1	7.187	6.063	43244	17227	24.072	11.604m#
27) L6 AR-1254-2	7.413	6.225	54948	17314	19.753	13.328m#
28) L6 AR-1254-3	7.799	6.643	69755	19519	22.626	9.146m#
29) L6 AR-1254-4	8.092	6.883	38602	13543	16.995	9.982m#
30) L6 AR-1254-5	8.520	7.314	53614	28953	21.425	15.445 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
Data File : PP037617.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 13:07
Operator : DD\AJ
Sample : M3133-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
PIPE-TRE-1236


Manual Integrations
APPROVED

mohammad
7/26/2021 11:56:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 07:24:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

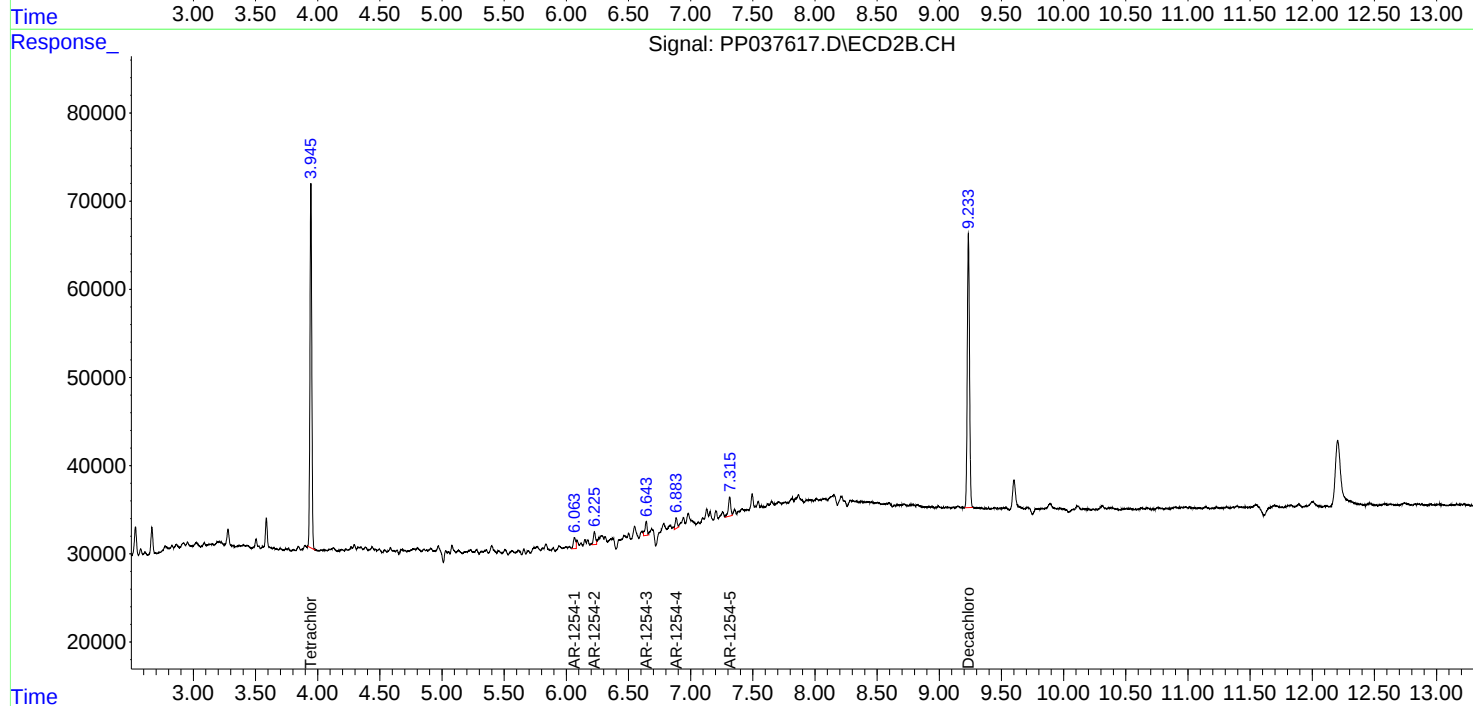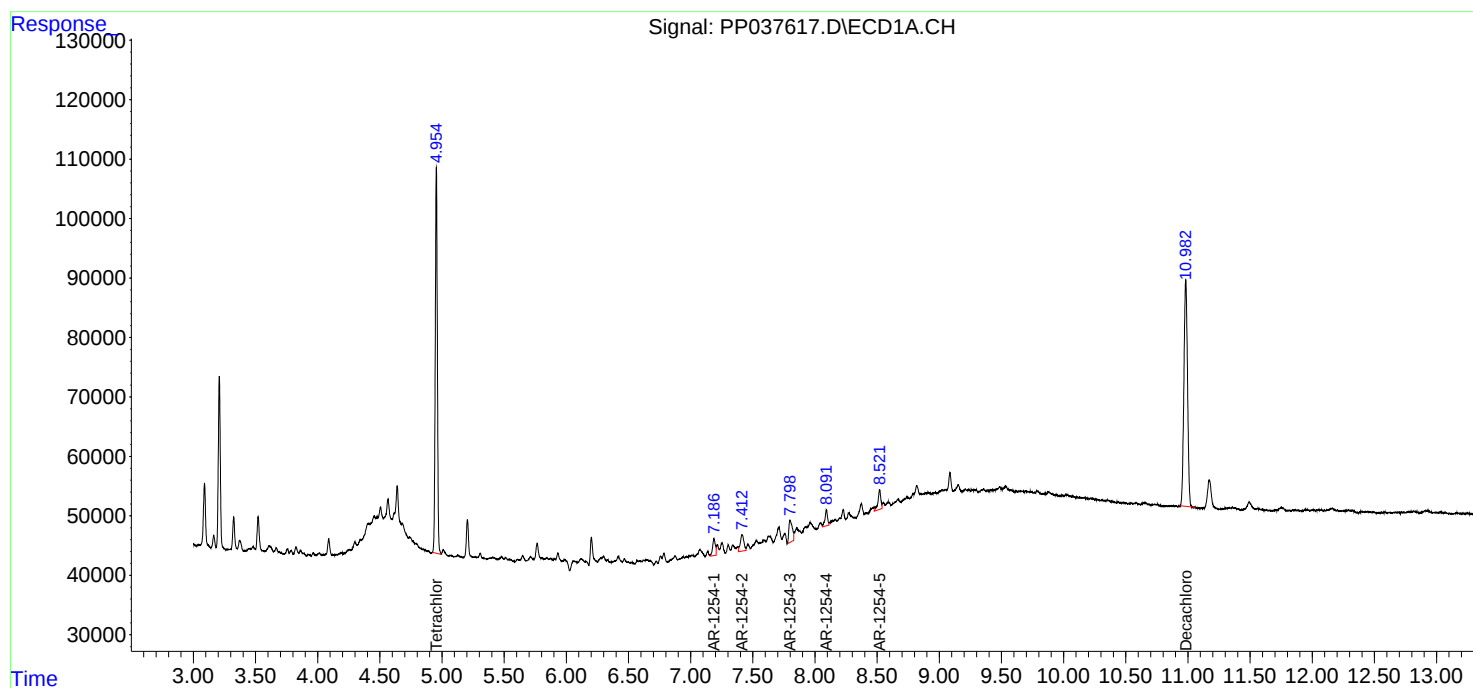

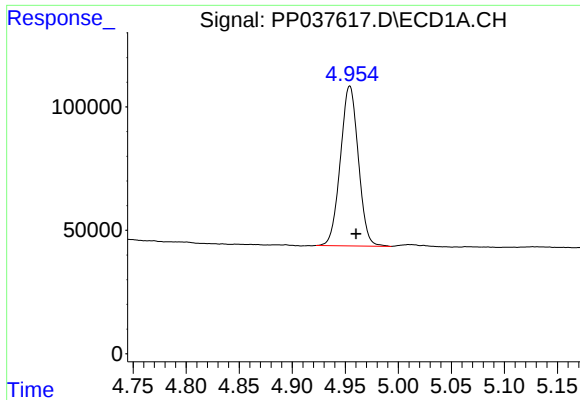


#1 Tetrachloro-m-xylene

R.T.: 4.954 min
Delta R.T.: -0.006 min
Response: 761213
Conc: 16.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPE-TRE-1236


Manual Integrations
APPROVED

mohammad
7/26/2021 11:56:49 AM

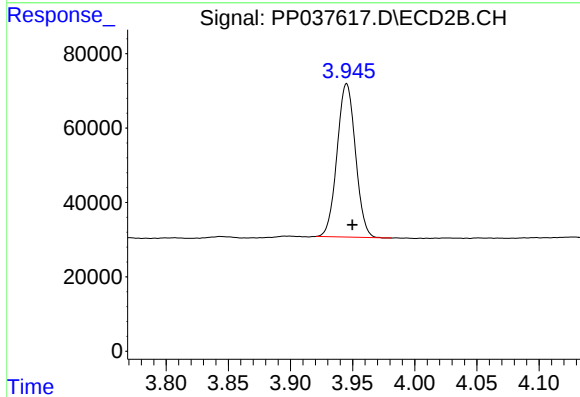


#1 Tetrachloro-m-xylene

R.T.: 3.945 min
Delta R.T.: -0.005 min
Response: 425000
Conc: 15.53 ng/ml

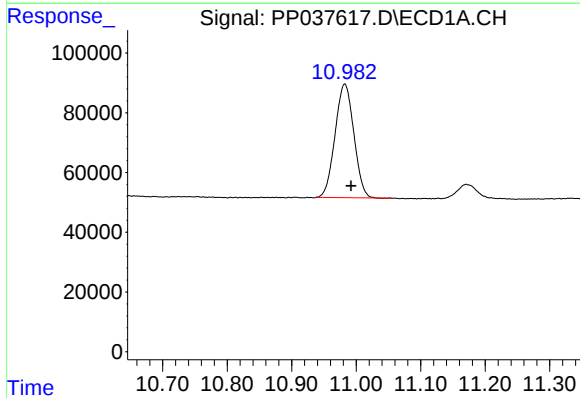


#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.010 min
Response: 768756
Conc: 16.70 ng/ml

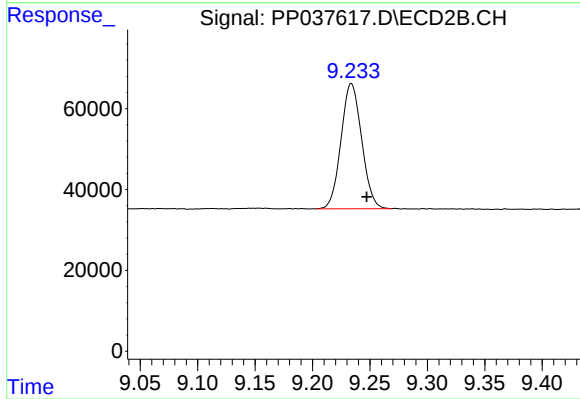

#2 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: -0.014 min
Response: 389291
Conc: 13.99 ng/ml

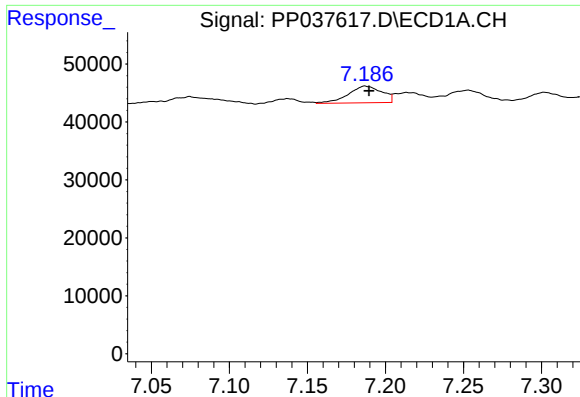


#26 AR-1254-1

R.T.: 7.187 min
Delta R.T.: -0.003 min
Response: 43244
Conc: 24.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPE-TRE-1236


Manual Integrations
APPROVED

mohammad
7/26/2021 11:56:49 AM

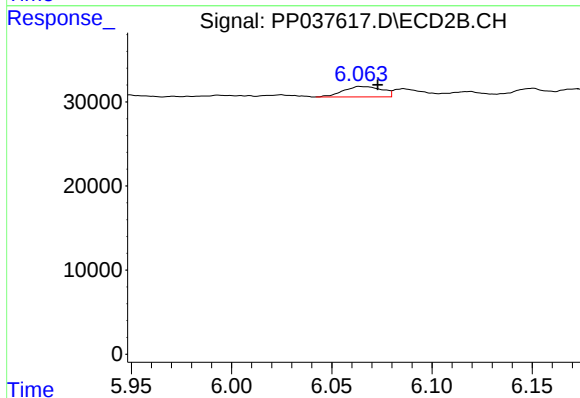


#26 AR-1254-1

R.T.: 6.063 min
Delta R.T.: -0.010 min
Response: 17227
Conc: 11.60 ng/ml m

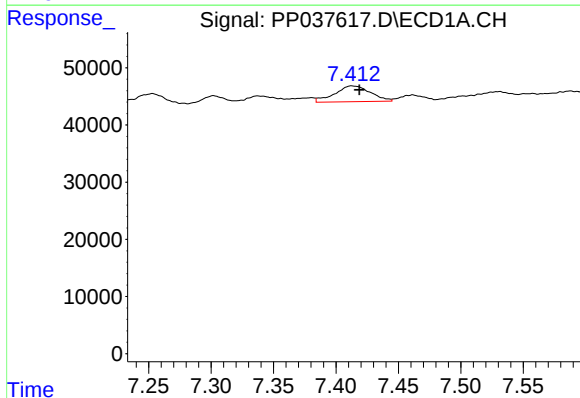


#27 AR-1254-2

R.T.: 7.413 min
Delta R.T.: -0.006 min
Response: 54948
Conc: 19.75 ng/ml

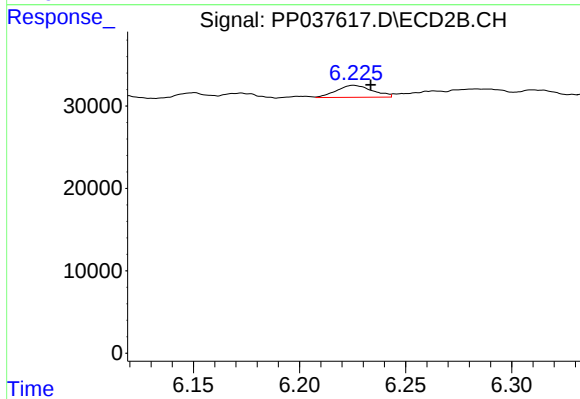

#27 AR-1254-2

R.T.: 6.225 min
Delta R.T.: -0.008 min
Response: 17314
Conc: 13.33 ng/ml m

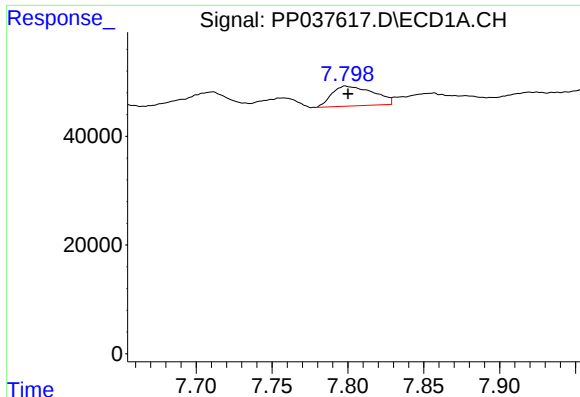


#28 AR-1254-3

R.T.: 7.799 min
Delta R.T.: -0.002 min
Response: 69755
Conc: 22.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPE-TRE-1236


Manual Integrations
APPROVED

mohammad
7/26/2021 11:56:49 AM

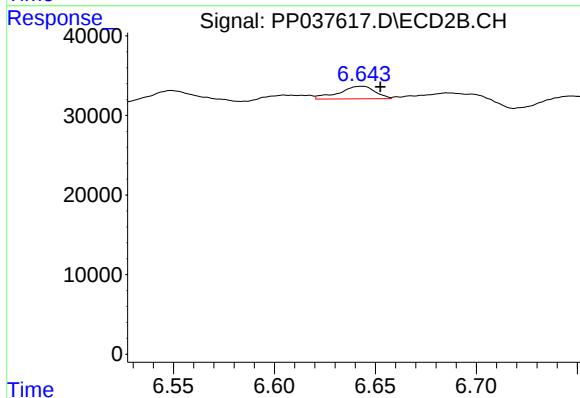


#28 AR-1254-3

R.T.: 6.643 min
Delta R.T.: -0.009 min
Response: 19519
Conc: 9.15 ng/ml m

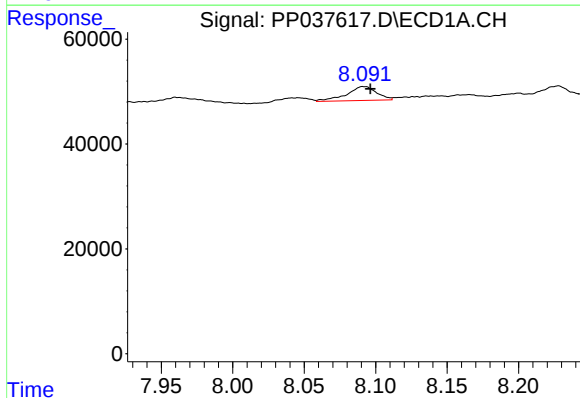


#29 AR-1254-4

R.T.: 8.092 min
Delta R.T.: -0.004 min
Response: 38602
Conc: 16.99 ng/ml

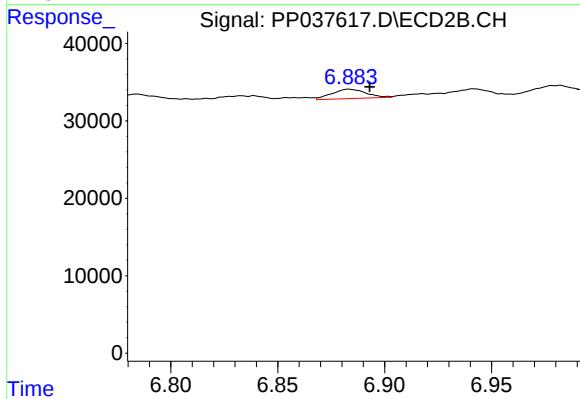

#29 AR-1254-4

R.T.: 6.883 min
Delta R.T.: -0.010 min
Response: 13543
Conc: 9.98 ng/ml m

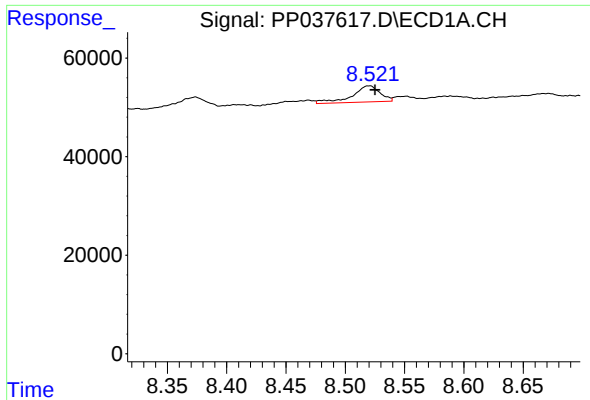


#30 AR-1254-5

R.T.: 8.520 min
Delta R.T.: -0.005 min
Response: 53614
Conc: 21.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPE-TRE-1236

Manual Integrations
APPROVED

mohammad
7/26/2021 11:56:49 AM

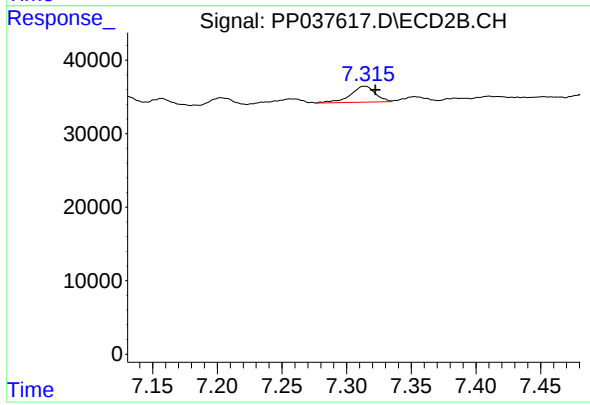

#30 AR-1254-5

R.T.: 7.314 min
Delta R.T.: -0.008 min
Response: 28953
Conc: 15.44 ng/ml