

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
 Data File : PP037644.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 21:21
 Operator : DD\AJ
 Sample : M3142-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JONES-RD-STOCK-PILE

Manual Integrations
 APPROVED

mohammad
 7/26/2021 11:57:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 07:38:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.955	3.946	992792	555866	21.844	20.314
2) SA Decachlor...	10.982	9.234	888314	381959	19.296	13.722m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072321\
Data File : PP037644.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 21:21
Operator : DD\AJ
Sample : M3142-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JONES-RD-STOCK-PILE


Manual Integrations
APPROVED

mohammad
7/26/2021 11:57:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 07:38:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

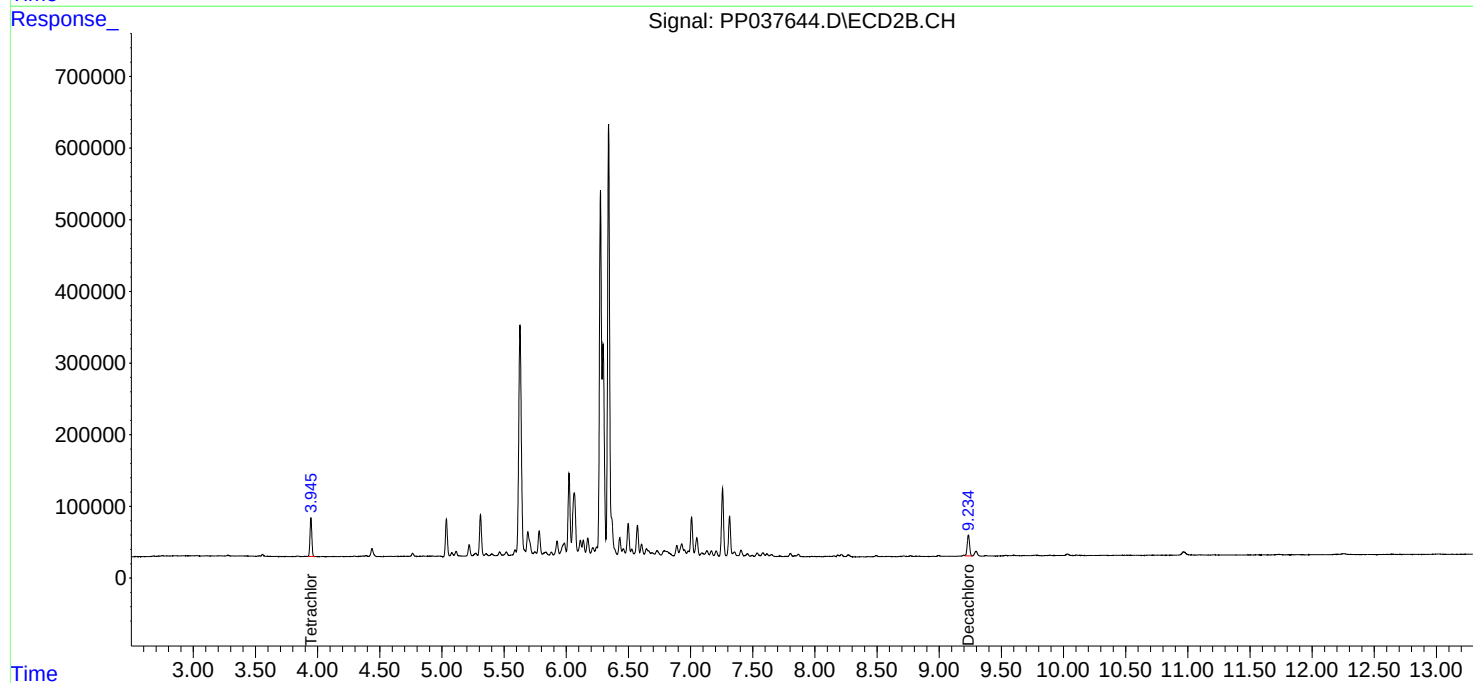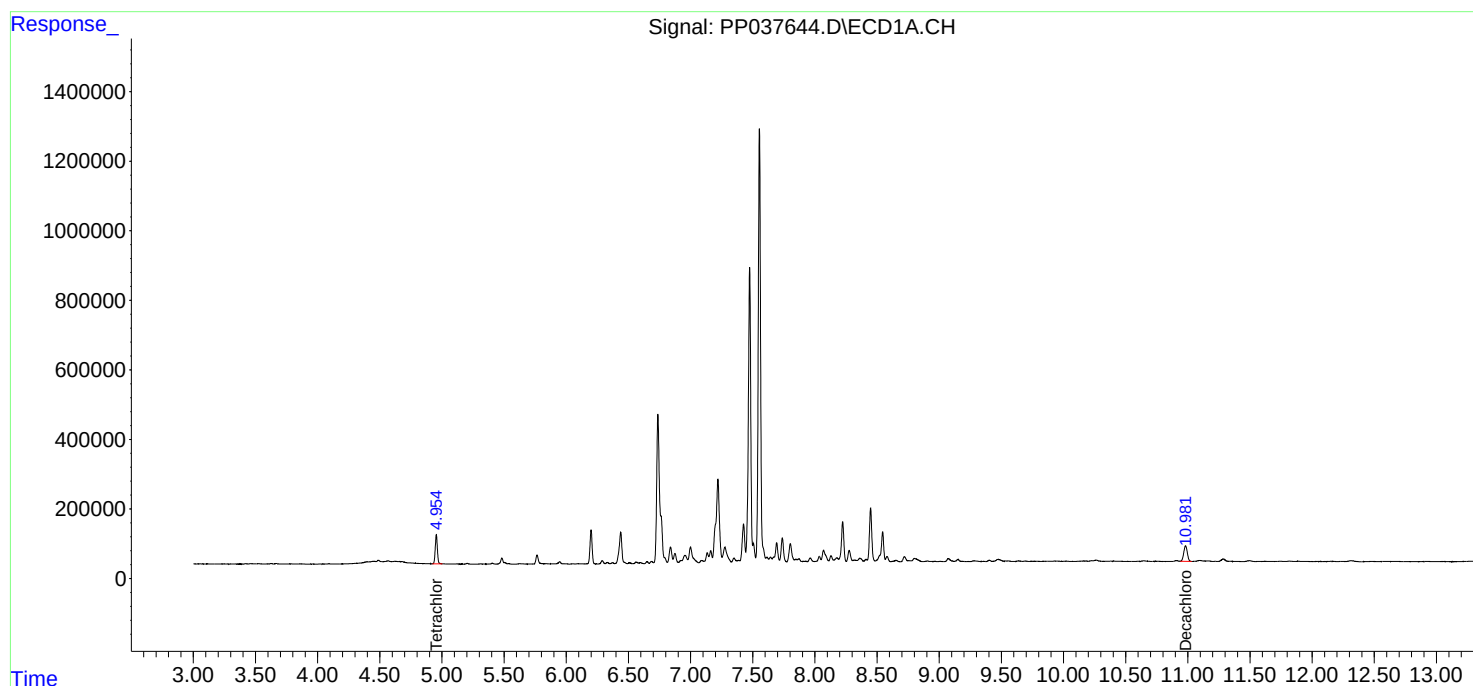

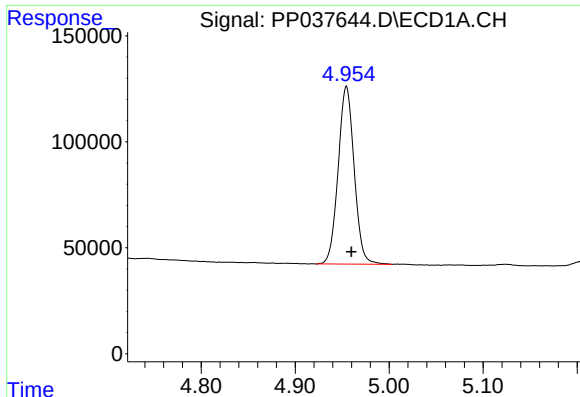


#1 Tetrachloro-m-xylene

R.T.: 4.955 min
Delta R.T.: -0.005 min
Response: 992792
Conc: 21.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
JONES-RD-STOCK-PILE


Manual Integrations
APPROVED

mohammad
7/26/2021 11:57:14 AM

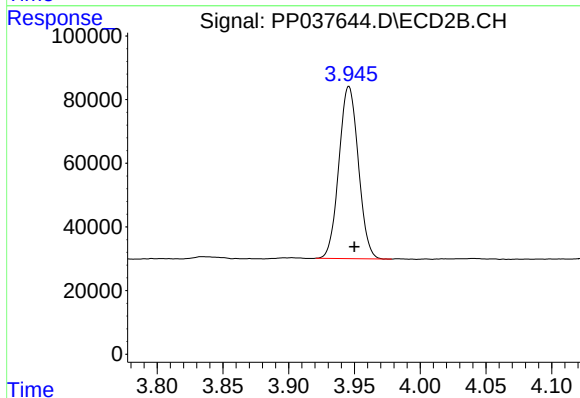


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 555866
Conc: 20.31 ng/ml

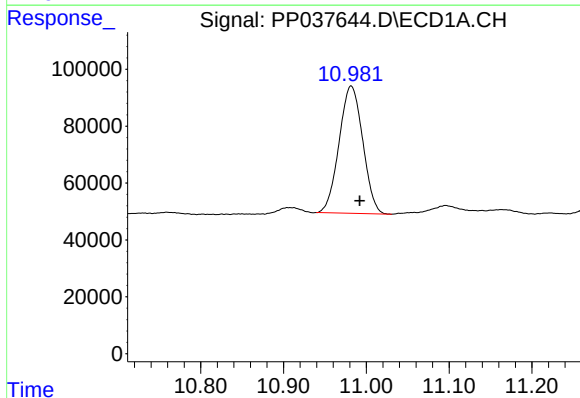

#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.011 min
Response: 888314
Conc: 19.30 ng/ml

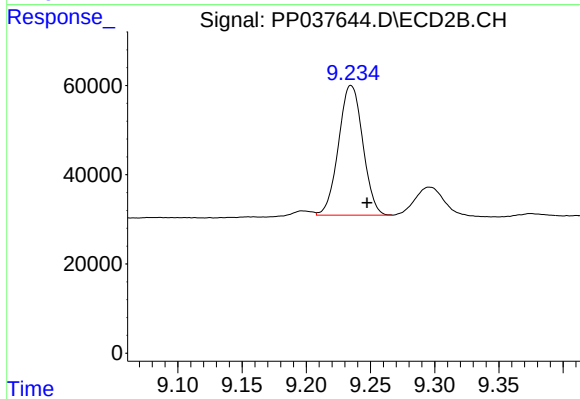

#2 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: -0.013 min
Response: 381959
Conc: 13.72 ng/ml m