

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072324\
 Data File : PP066480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 12:39
 Operator : YP\AJ
 Sample : P3324-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CONRAIL-01-VALVE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 01:49:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 07:20:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.792	4.029	42582041	44081377	24.170	23.085
2) SA Decachlor...	10.794	9.205	41765482	26714586	23.795	20.937
Target Compounds						
3) L1 AR-1016-1	5.972	5.142	55996026	50925693	764.009	812.921
4) L1 AR-1016-2	5.997	5.161	155.9E6	76577291	1425.757	860.381 #
5) L1 AR-1016-3	6.058	5.343	60319169	45356751	893.597	960.760
6) L1 AR-1016-4	6.158	5.381	62931167	30397476	1133.799	796.576 #
7) L1 AR-1016-5	6.454	5.612	64589778	95960484	1161.698	1979.910 #
8) L2 AR-1221-1	4.999	4.241	2538484	8507508	114.335	368.095 #
9) L2 AR-1221-2	5.090	4.334	6035032	3902905	359.551	226.099 #
10) L2 AR-1221-3	5.164	4.412	35851649	37503886	699.835	741.877
11) L3 AR-1232-1	5.164	4.412	35851649	37503886	819.325	878.709
12) L3 AR-1232-2	5.702	5.142	45993992	50925693	1779.981	1726.725
13) L3 AR-1232-3	5.972	5.343	55996026	45356751	1655.804	2036.467
14) L3 AR-1232-4	6.158	5.425	62931167	36971062	2427.773	1838.778
15) L3 AR-1232-5	6.246	5.612	41431766	95960484	1910.991	4505.150 #
16) L4 AR-1242-1	5.972	5.142	55996026	50925693	1008.783	974.261
17) L4 AR-1242-2	5.997	5.161	155.9E6	76577291	1742.285	1060.161 #
18) L4 AR-1242-3	6.058	5.343	60319169	45356751	1098.838	1185.446
19) L4 AR-1242-4	6.158	5.425	62931167	36971062	1374.393	974.081 #
20) L4 AR-1242-5	6.905	5.957	242.7E6	46095878	4878.612	1021.784 #
21) L5 AR-1248-1	5.972	5.142	55996026	50925693	1148.903	1236.052
22) L5 AR-1248-2	6.246	5.381	41431766	30397476	542.758	535.266
23) L5 AR-1248-3	6.454	5.425	64589778	36971062	793.020	626.991
24) L5 AR-1248-4	6.858	5.612	52874635	95960484	567.669	1398.963 #
25) L5 AR-1248-5	6.905	6.000	242.7E6	43407503	2630.113	692.130 #
26) L6 AR-1254-1	6.832	5.957	37426073	46095878	400.193	484.354
27) L6 AR-1254-2	7.058	6.107	42379827	13743216	300.449	165.479 #
28) L6 AR-1254-3	7.420	6.518	13919335	13674902	107.322	109.448
29) L6 AR-1254-4	7.705	6.746	7312038	5435118	79.740	79.432
30) L6 AR-1254-5	8.127	7.168	9021285	3658766	90.763	36.442 #
31) L7 AR-1260-1	7.586	6.667	3474575	3945015	32.845	46.146 #
32) L7 AR-1260-2	7.839	6.834	3968938	1442687	34.450	14.836 #
33) L7 AR-1260-3	8.215	6.994	1934232	2163783	24.370	23.584
34) L7 AR-1260-4	8.441	7.468	-25654	1529391	N.D.	23.533 #
35) L7 AR-1260-5	8.793	7.708	2626880	1880469	16.990	13.377
36) L8 AR-1262-1	8.264	7.279f	1871408	8760743	33.193	184.097 #
37) L8 AR-1262-2	8.793	7.468	2626880	1529391	13.897	16.348
38) L8 AR-1262-3	9.154f	8.001	3304927	808593	25.321	11.302 #
39) L8 AR-1262-4	9.213f	0.000	2558114	0	22.726	N.D. #
40) L8 AR-1262-5	9.954	8.593	1783630	168360	27.393	2.813 #
41) L9 AR-1268-1	9.154f	8.001	3304927	808593	14.133	4.015 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072324\
 Data File : PP066480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 12:39
 Operator : YP\AJ
 Sample : P3324-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CONRAIL-01-VALVE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 01:49:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 07:20:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.213f	0.000	2558114	0	11.989	N.D. #
43) L9	AR-1268-3	9.503	8.263f	6194535	3222485	32.337	19.927 #
44) L9	AR-1268-4	9.954	8.593	1783630	168360	25.574	2.501 #
45) L9	AR-1268-5	10.414	0.000	843977	0	1.380	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072324\
Data File : PP066480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 12:39
Operator : YP\AJ
Sample : P3324-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 01:49:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 07:20:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

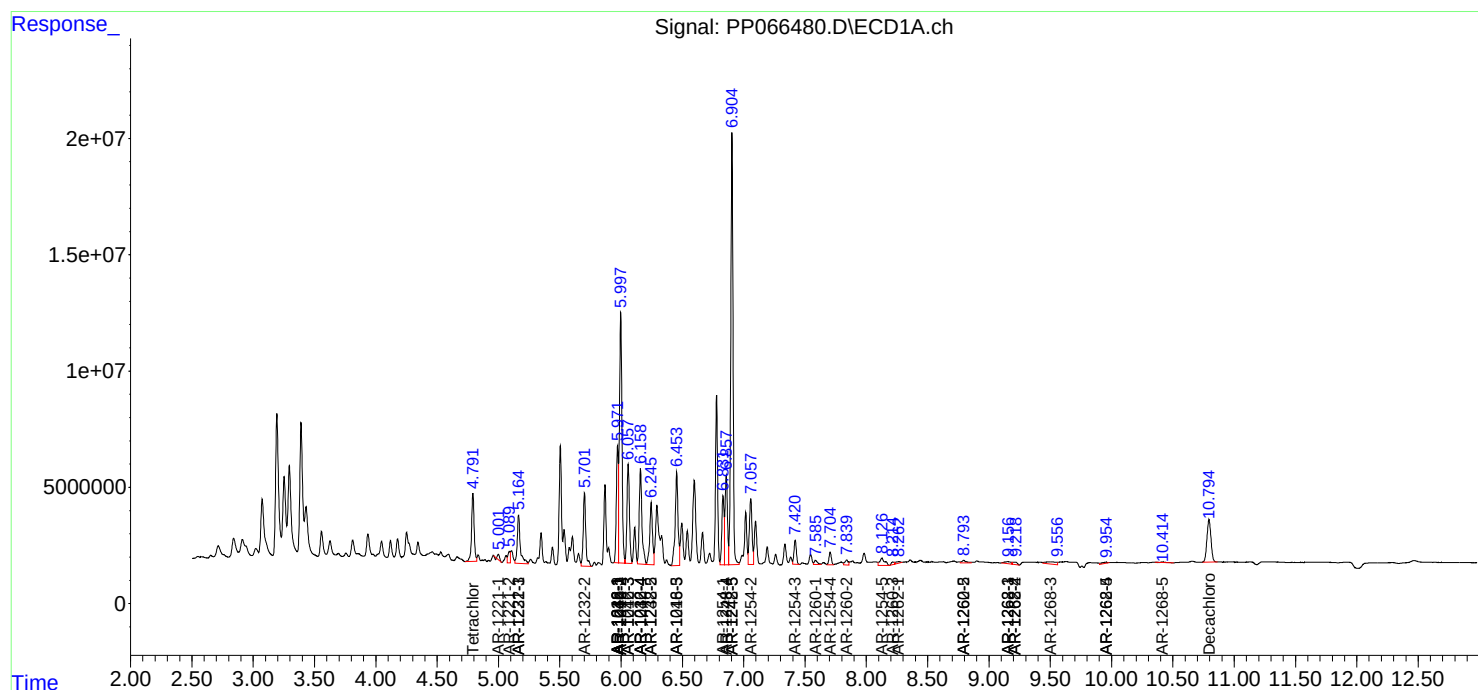


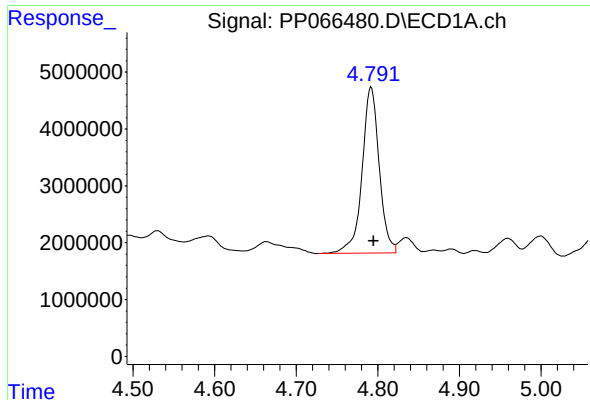

#1 Tetrachloro-m-xylene


R.T.: 4.792 min
Delta R.T.: -0.003 min
Response: 42582041
Conc: 24.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

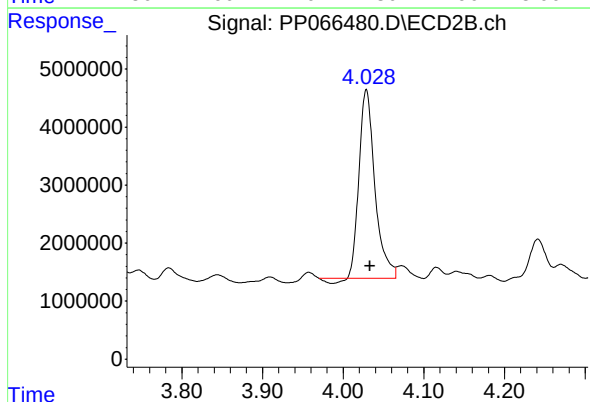


#1 Tetrachloro-m-xylene

R.T.: 4.029 min
Delta R.T.: -0.004 min
Response: 44081377
Conc: 23.08 ng/ml

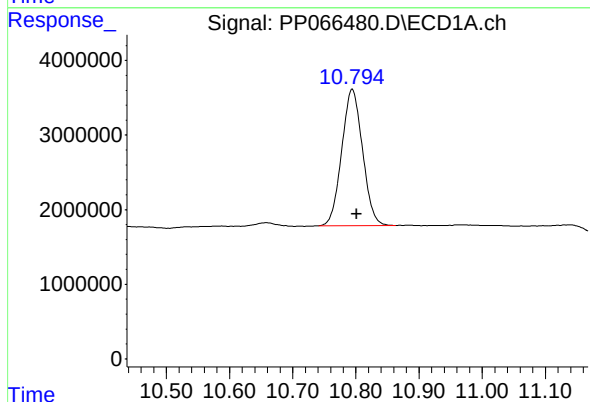


#2 Decachlorobiphenyl

R.T.: 10.794 min
Delta R.T.: -0.007 min
Response: 41765482
Conc: 23.79 ng/ml

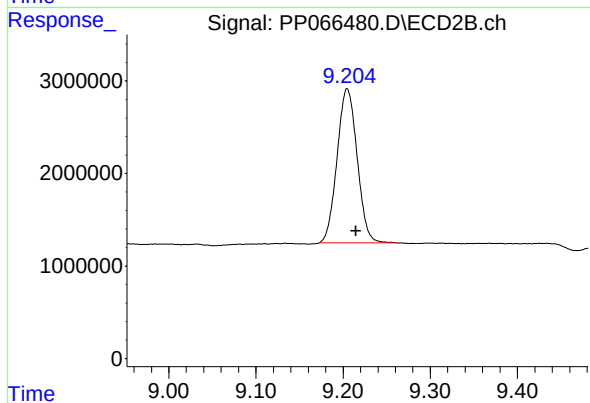

#2 Decachlorobiphenyl


R.T.: 9.205 min
Delta R.T.: -0.010 min
Response: 26714586
Conc: 20.94 ng/ml

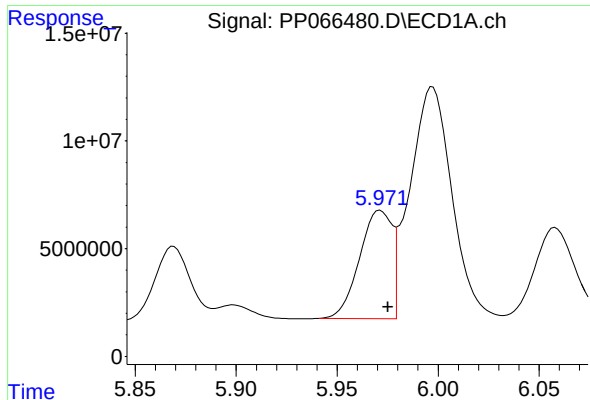

#3 AR-1016-1


R.T.: 5.972 min
Delta R.T.: -0.003 min
Response: 55996026
Conc: 764.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

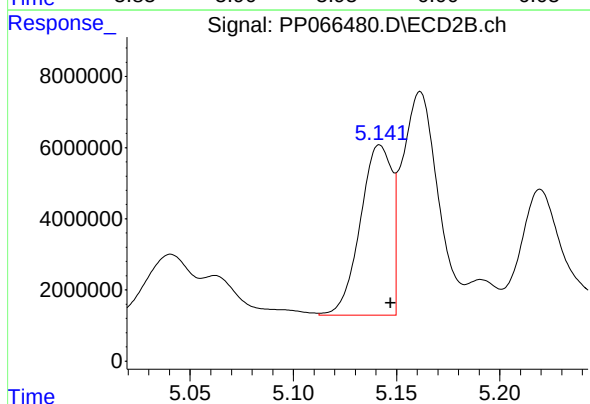


#3 AR-1016-1

R.T.: 5.142 min
Delta R.T.: -0.005 min
Response: 50925693
Conc: 812.92 ng/ml

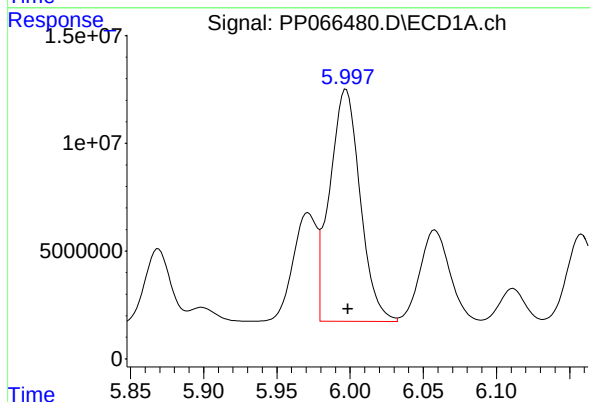


#4 AR-1016-2

R.T.: 5.997 min
Delta R.T.: -0.001 min
Response: 155917413
Conc: 1425.76 ng/ml

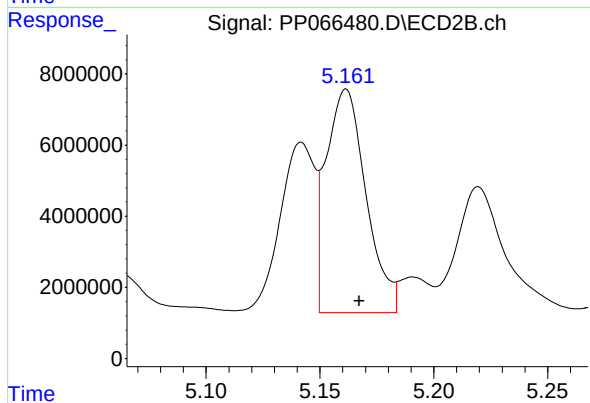

#4 AR-1016-2


R.T.: 5.161 min
Delta R.T.: -0.006 min
Response: 76577291
Conc: 860.38 ng/ml

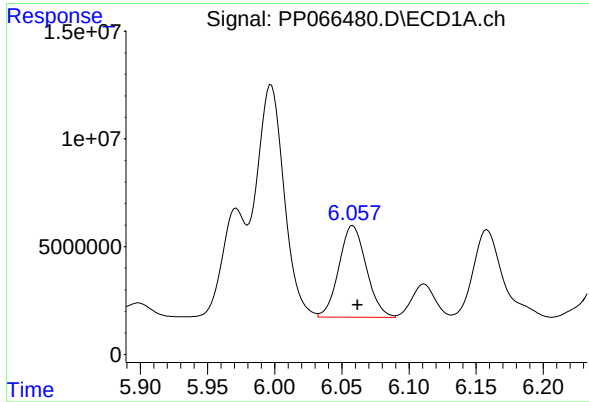

#5 AR-1016-3


R.T.: 6.058 min
Delta R.T.: -0.004 min
Response: 60319169
Conc: 893.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

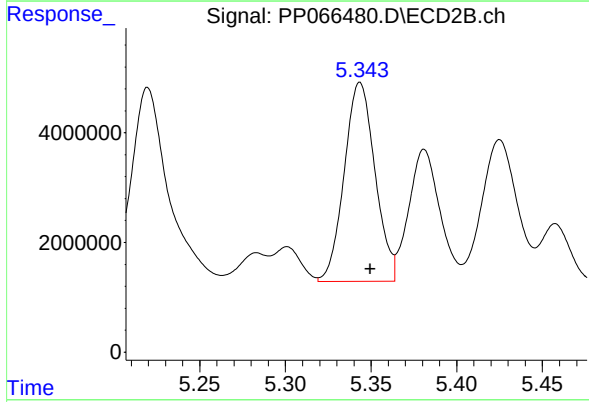


#5 AR-1016-3

R.T.: 5.343 min
Delta R.T.: -0.006 min
Response: 45356751
Conc: 960.76 ng/ml

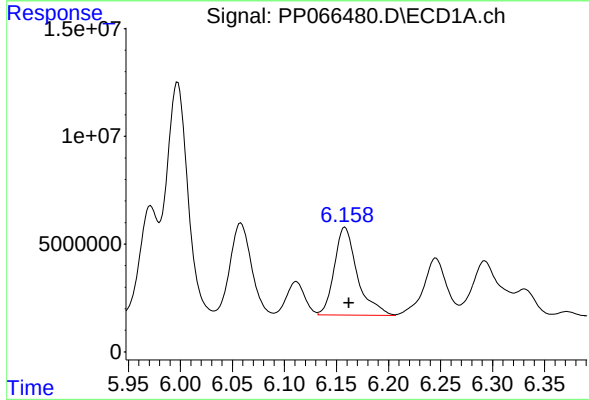


#6 AR-1016-4

R.T.: 6.158 min
Delta R.T.: -0.004 min
Response: 62931167
Conc: 1133.80 ng/ml

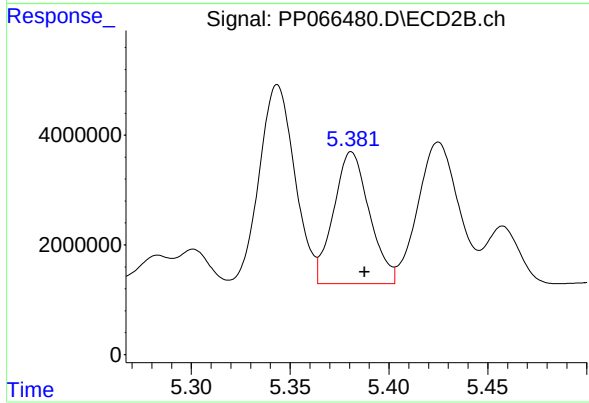

#6 AR-1016-4


R.T.: 5.381 min
Delta R.T.: -0.007 min
Response: 30397476
Conc: 796.58 ng/ml

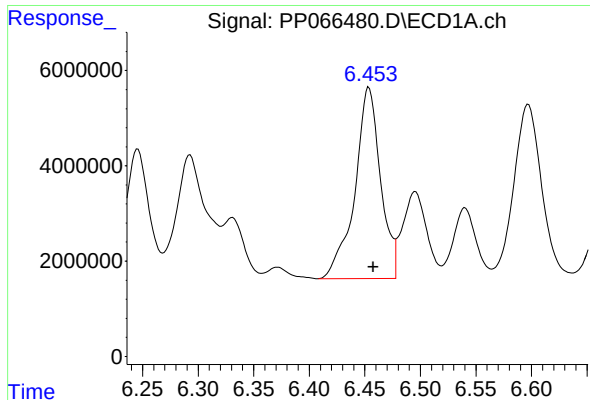

#7 AR-1016-5


R.T.: 6.454 min
Delta R.T.: -0.004 min
Response: 64589778
Conc: 1161.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

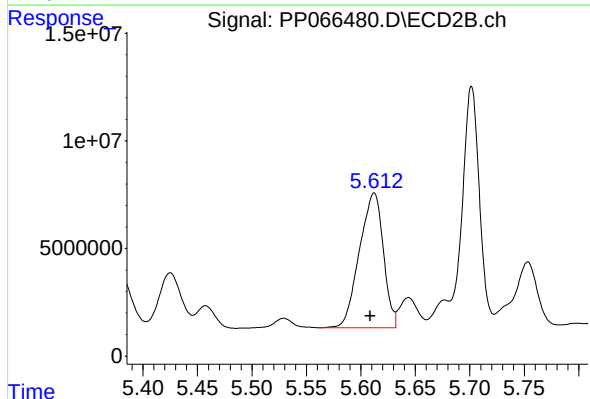


#7 AR-1016-5

R.T.: 5.612 min
Delta R.T.: 0.004 min
Response: 95960484
Conc: 1979.91 ng/ml

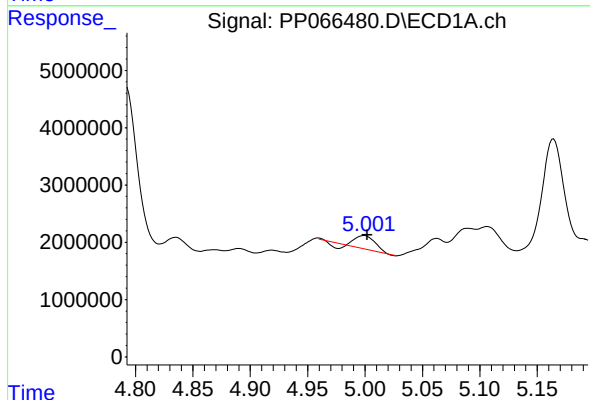


#8 AR-1221-1

R.T.: 4.999 min
Delta R.T.: -0.003 min
Response: 2538484
Conc: 114.34 ng/ml

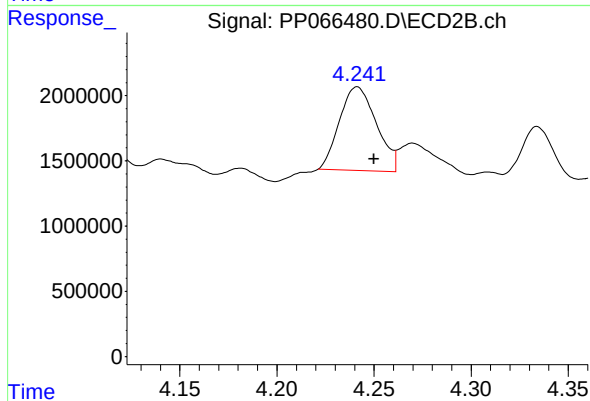

#8 AR-1221-1


R.T.: 4.241 min
Delta R.T.: -0.009 min
Response: 8507508
Conc: 368.09 ng/ml

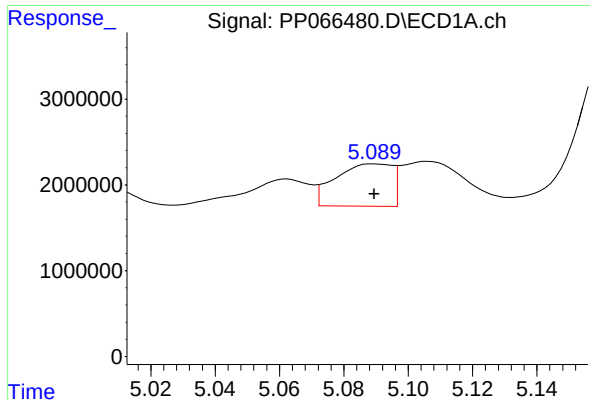

#9 AR-1221-2


R.T.: 5.090 min
Delta R.T.: 0.000 min
Response: 6035032
Conc: 359.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

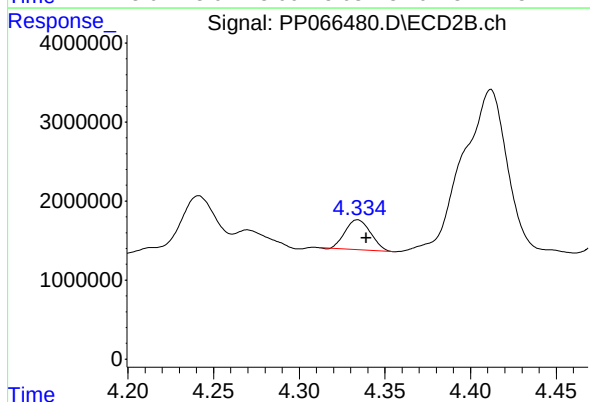


#9 AR-1221-2

R.T.: 4.334 min
Delta R.T.: -0.005 min
Response: 3902905
Conc: 226.10 ng/ml

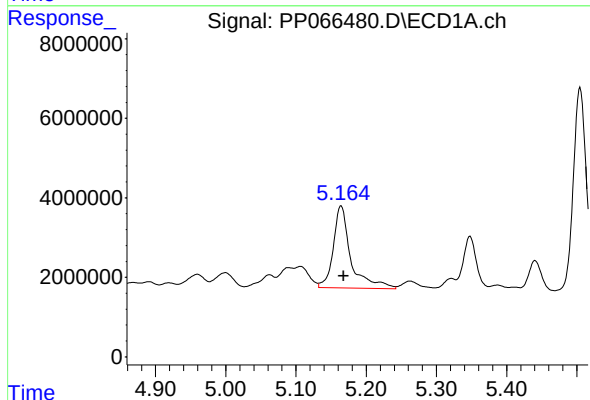


#10 AR-1221-3

R.T.: 5.164 min
Delta R.T.: -0.004 min
Response: 35851649
Conc: 699.83 ng/ml

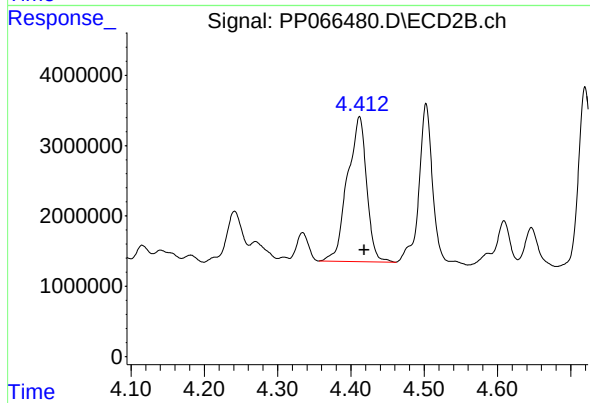

#10 AR-1221-3


R.T.: 4.412 min
Delta R.T.: -0.006 min
Response: 37503886
Conc: 741.88 ng/ml

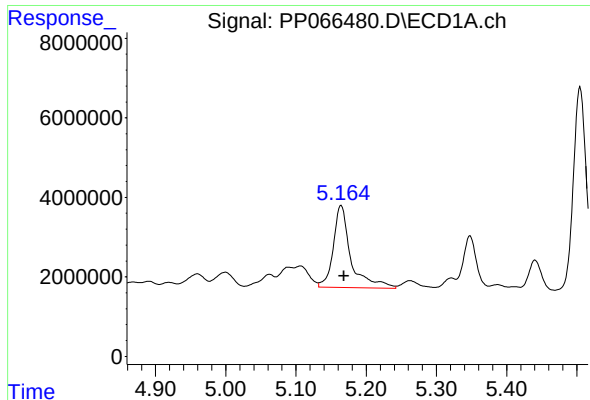

#11 AR-1232-1


R.T.: 5.164 min
Delta R.T.: -0.004 min
Response: 35851649
Conc: 819.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

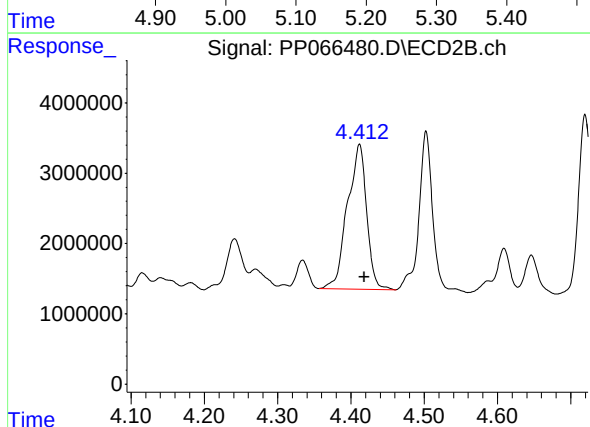


#11 AR-1232-1

R.T.: 4.412 min
Delta R.T.: -0.007 min
Response: 37503886
Conc: 878.71 ng/ml

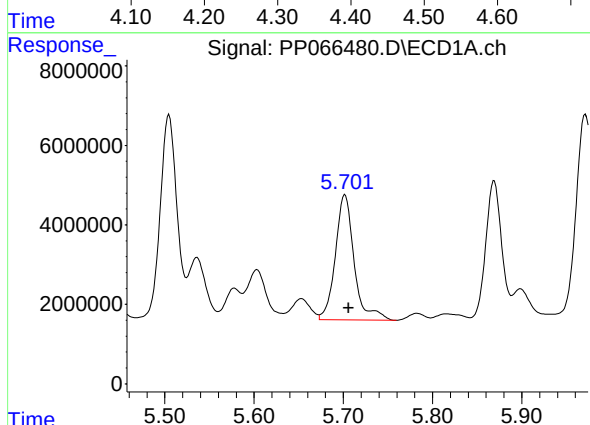


#12 AR-1232-2

R.T.: 5.702 min
Delta R.T.: -0.004 min
Response: 45993992
Conc: 1779.98 ng/ml

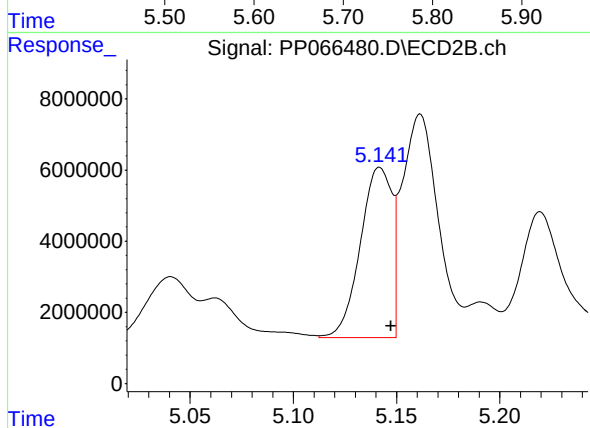

#12 AR-1232-2


R.T.: 5.142 min
Delta R.T.: -0.005 min
Response: 50925693
Conc: 1726.73 ng/ml

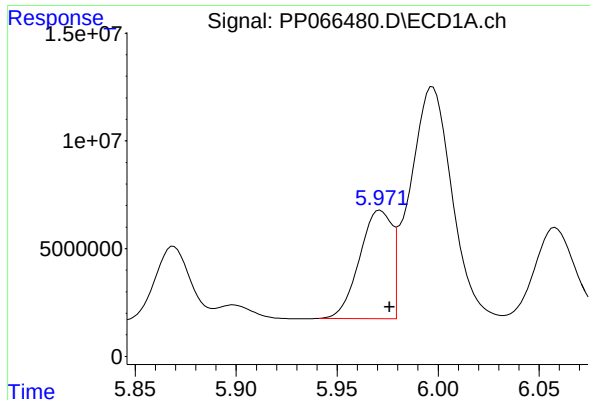

#13 AR-1232-3


R.T.: 5.972 min
Delta R.T.: -0.004 min
Response: 55996026
Conc: 1655.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

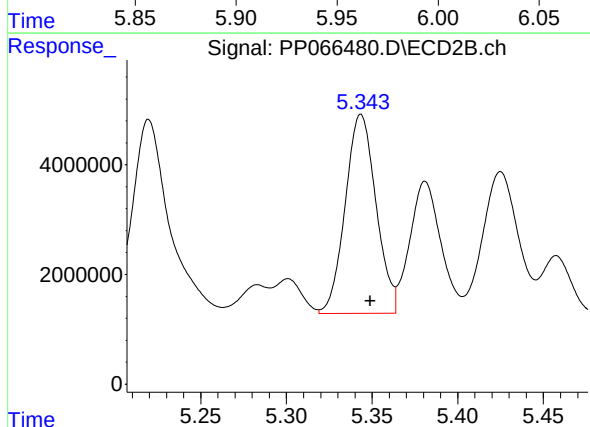


#13 AR-1232-3

R.T.: 5.343 min
Delta R.T.: -0.005 min
Response: 45356751
Conc: 2036.47 ng/ml

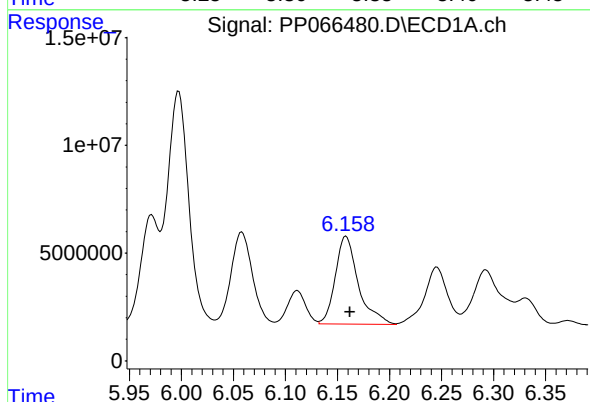


#14 AR-1232-4

R.T.: 6.158 min
Delta R.T.: -0.004 min
Response: 62931167
Conc: 2427.77 ng/ml

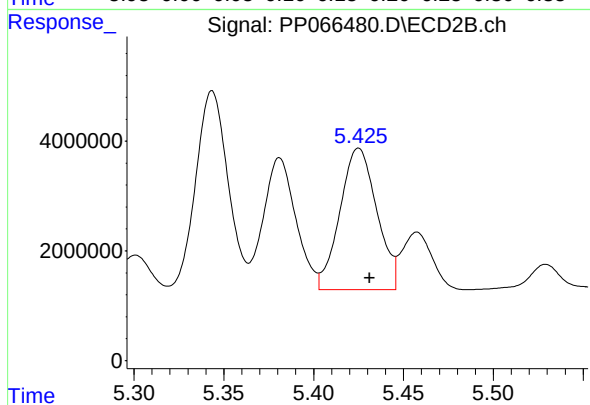

#14 AR-1232-4


R.T.: 5.425 min
Delta R.T.: -0.006 min
Response: 36971062
Conc: 1838.78 ng/ml

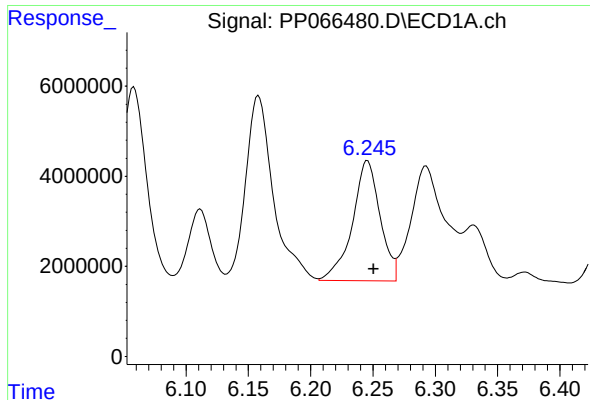

#15 AR-1232-5


R.T.: 6.246 min
Delta R.T.: -0.005 min
Response: 41431766
Conc: 1910.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

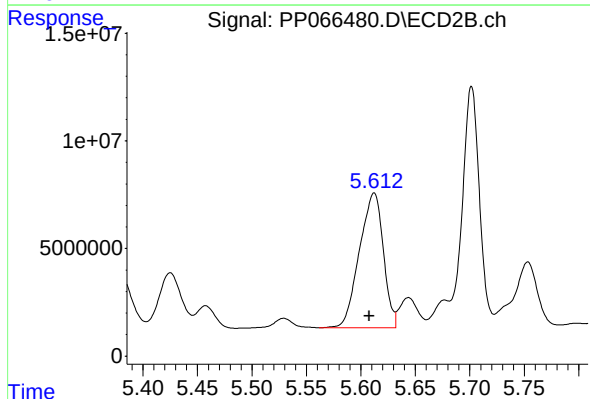


#15 AR-1232-5

R.T.: 5.612 min
Delta R.T.: 0.004 min
Response: 95960484
Conc: 4505.15 ng/ml

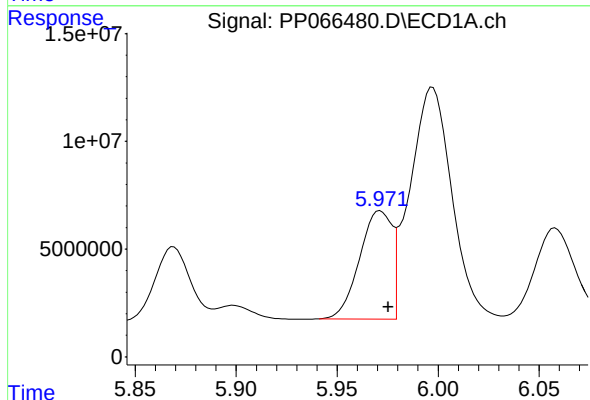


#16 AR-1242-1

R.T.: 5.972 min
Delta R.T.: -0.004 min
Response: 55996026
Conc: 1008.78 ng/ml

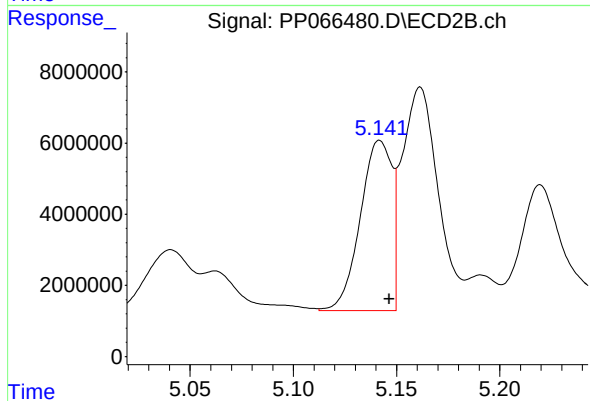

#16 AR-1242-1


R.T.: 5.142 min
Delta R.T.: -0.005 min
Response: 50925693
Conc: 974.26 ng/ml

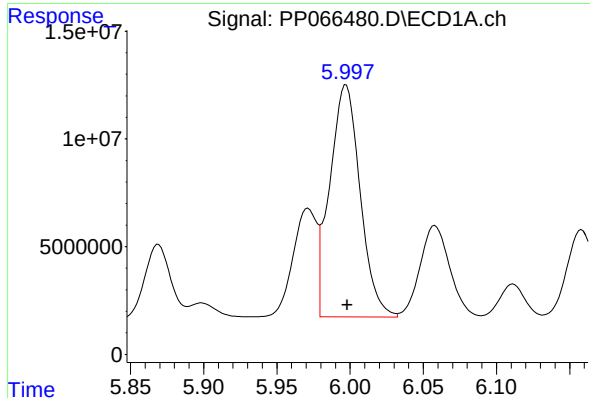

#17 AR-1242-2


R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 155917413
Conc: 1742.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

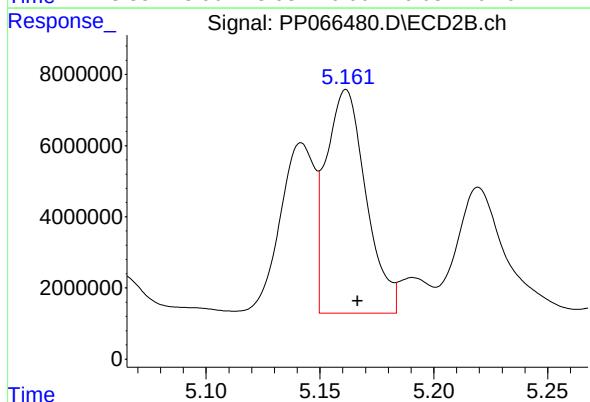


#17 AR-1242-2

R.T.: 5.161 min
Delta R.T.: -0.005 min
Response: 76577291
Conc: 1060.16 ng/ml

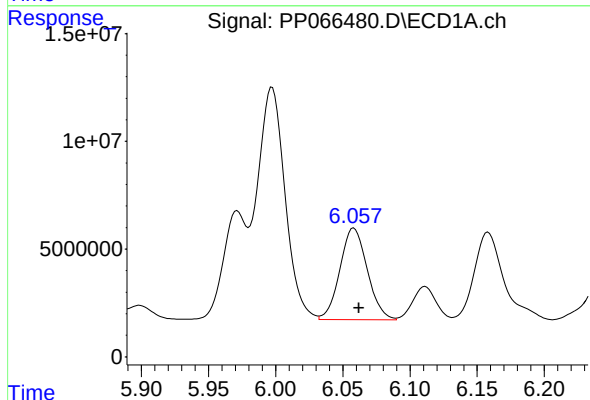


#18 AR-1242-3

R.T.: 6.058 min
Delta R.T.: -0.004 min
Response: 60319169
Conc: 1098.84 ng/ml

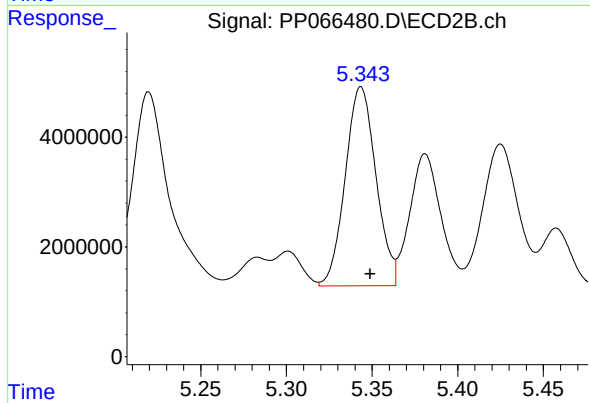

#18 AR-1242-3


R.T.: 5.343 min
Delta R.T.: -0.005 min
Response: 45356751
Conc: 1185.45 ng/ml

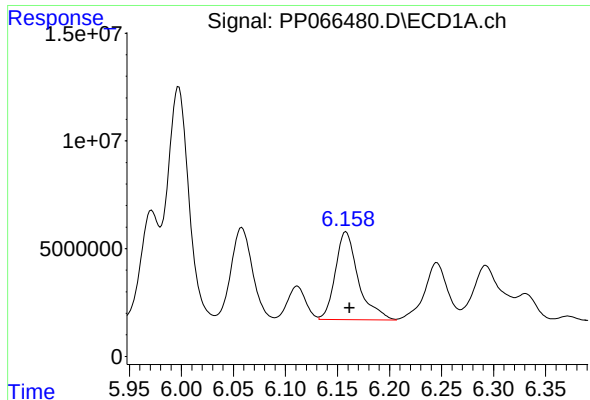

#19 AR-1242-4


R.T.: 6.158 min
Delta R.T.: -0.004 min
Response: 62931167
Conc: 1374.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

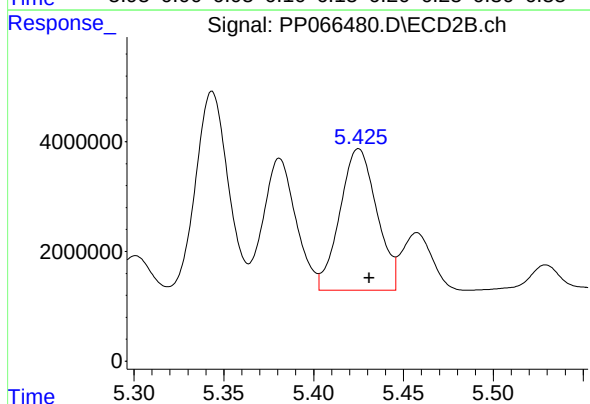


#19 AR-1242-4

R.T.: 5.425 min
Delta R.T.: -0.006 min
Response: 36971062
Conc: 974.08 ng/ml

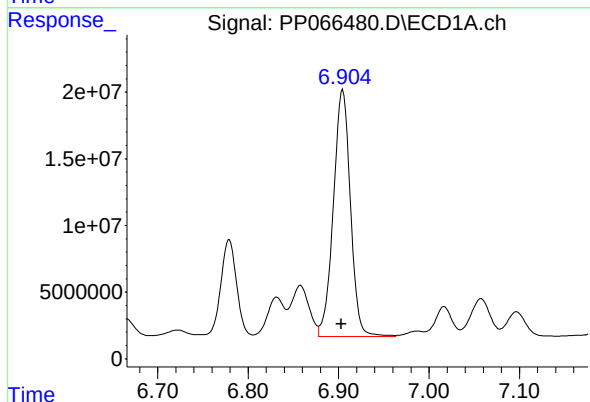


#20 AR-1242-5

R.T.: 6.905 min
Delta R.T.: 0.002 min
Response: 242660647
Conc: 4878.61 ng/ml

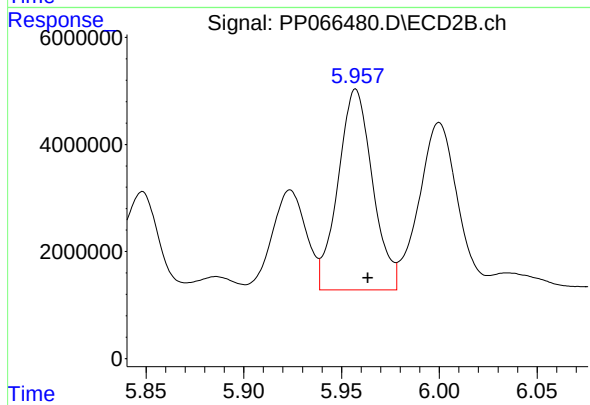

#20 AR-1242-5


R.T.: 5.957 min
Delta R.T.: -0.006 min
Response: 46095878
Conc: 1021.78 ng/ml

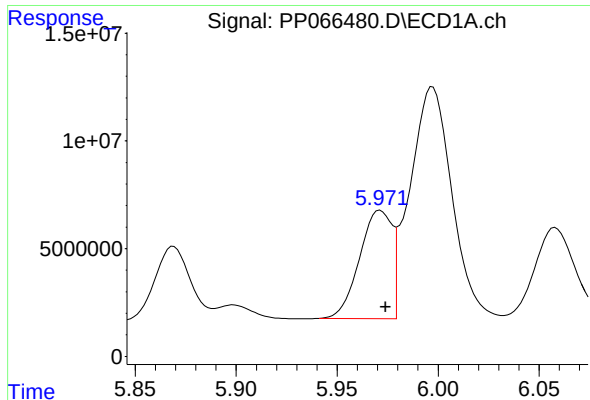

#21 AR-1248-1


R.T.: 5.972 min
Delta R.T.: -0.002 min
Response: 55996026
Conc: 1148.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

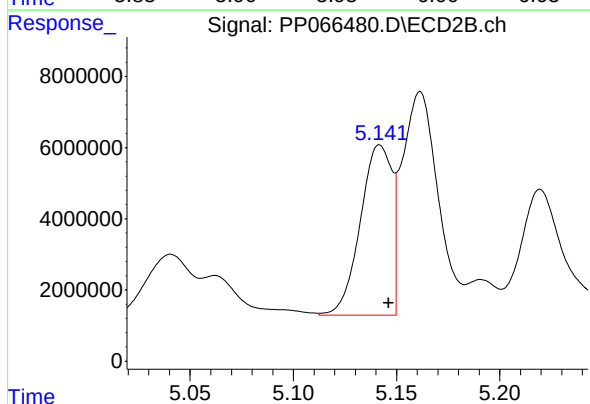


#21 AR-1248-1

R.T.: 5.142 min
Delta R.T.: -0.004 min
Response: 50925693
Conc: 1236.05 ng/ml

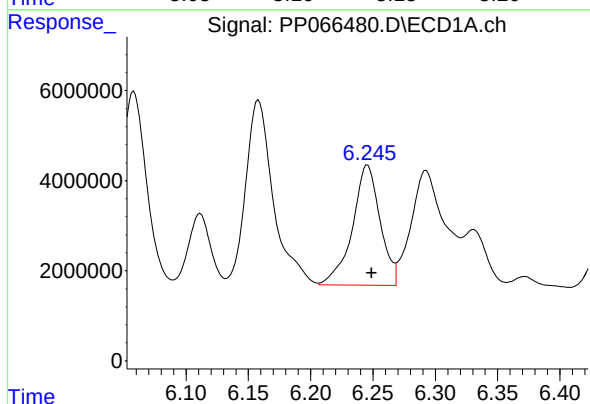


#22 AR-1248-2

R.T.: 6.246 min
Delta R.T.: -0.003 min
Response: 41431766
Conc: 542.76 ng/ml

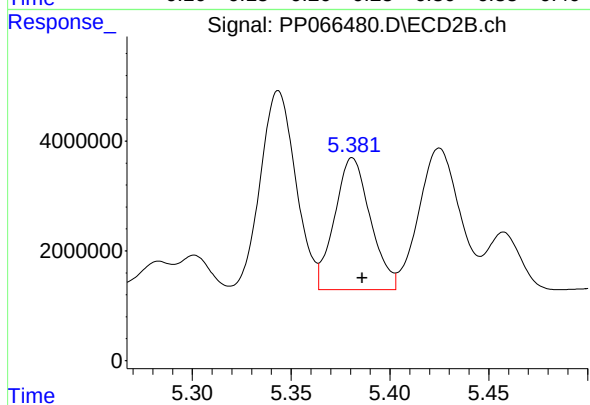

#22 AR-1248-2


R.T.: 5.381 min
Delta R.T.: -0.005 min
Response: 30397476
Conc: 535.27 ng/ml

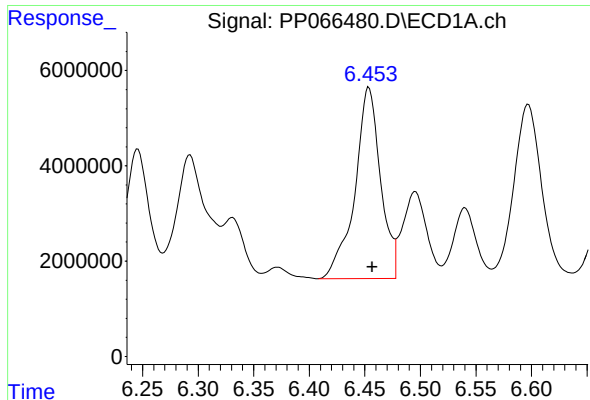

#23 AR-1248-3


R.T.: 6.454 min
Delta R.T.: -0.003 min
Response: 64589778
Conc: 793.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

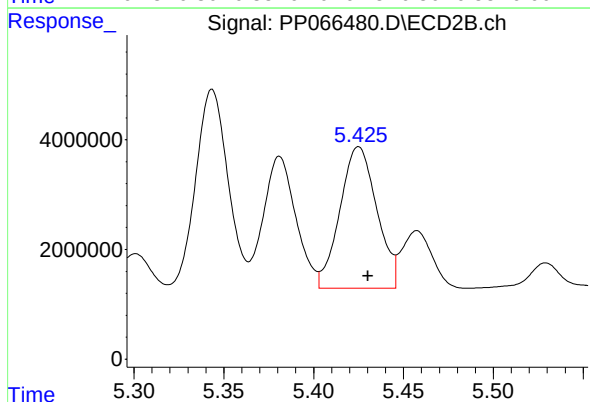


#23 AR-1248-3

R.T.: 5.425 min
Delta R.T.: -0.005 min
Response: 36971062
Conc: 626.99 ng/ml

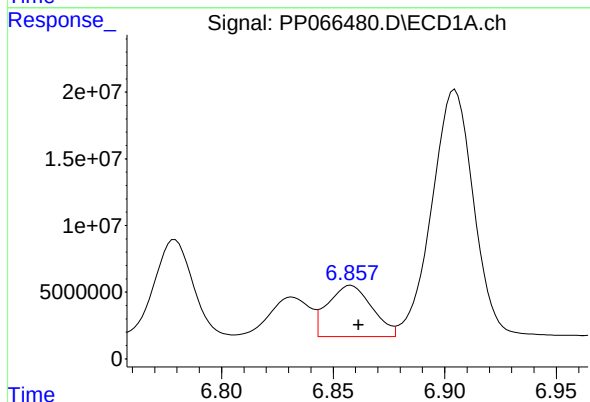


#24 AR-1248-4

R.T.: 6.858 min
Delta R.T.: -0.004 min
Response: 52874635
Conc: 567.67 ng/ml

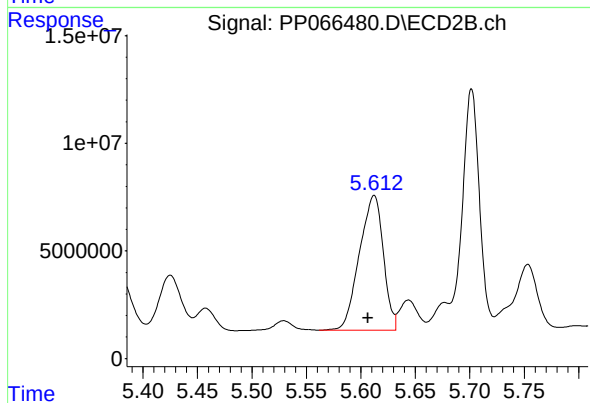

#24 AR-1248-4


R.T.: 5.612 min
Delta R.T.: 0.006 min
Response: 95960484
Conc: 1398.96 ng/ml

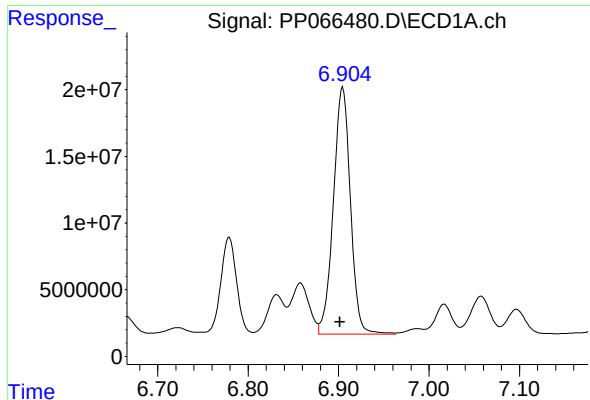

#25 AR-1248-5


R.T.: 6.905 min
Delta R.T.: 0.003 min
Response: 242660647
Conc: 2630.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

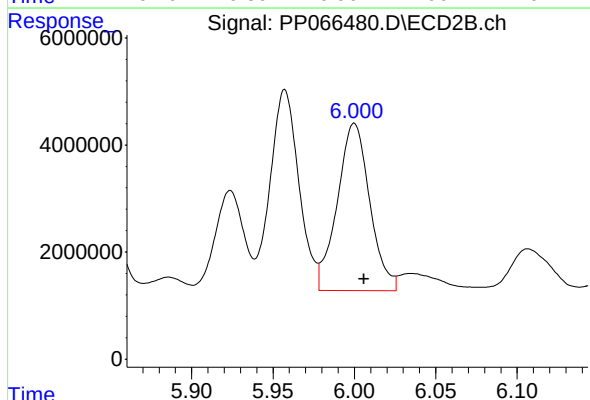


#25 AR-1248-5

R.T.: 6.000 min
Delta R.T.: -0.006 min
Response: 43407503
Conc: 692.13 ng/ml

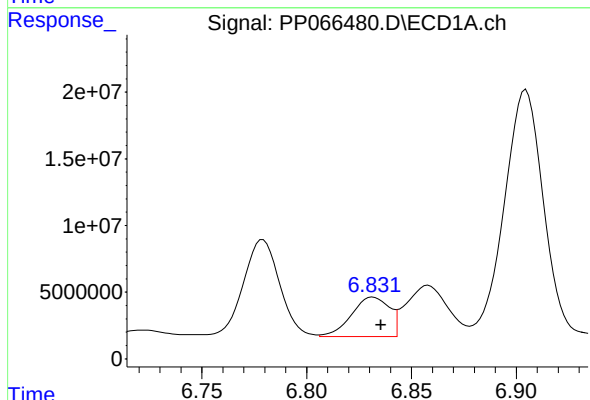


#26 AR-1254-1

R.T.: 6.832 min
Delta R.T.: -0.004 min
Response: 37426073
Conc: 400.19 ng/ml

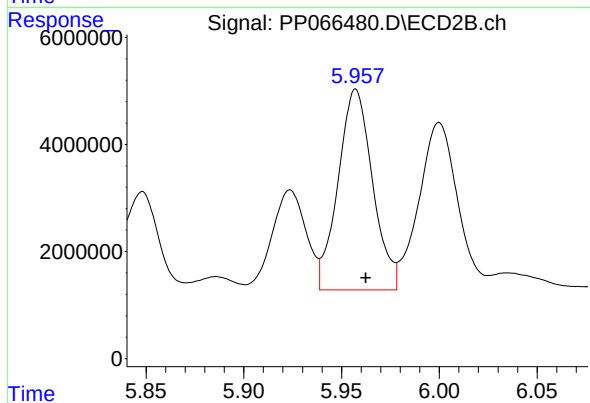

#26 AR-1254-1


R.T.: 5.957 min
Delta R.T.: -0.005 min
Response: 46095878
Conc: 484.35 ng/ml

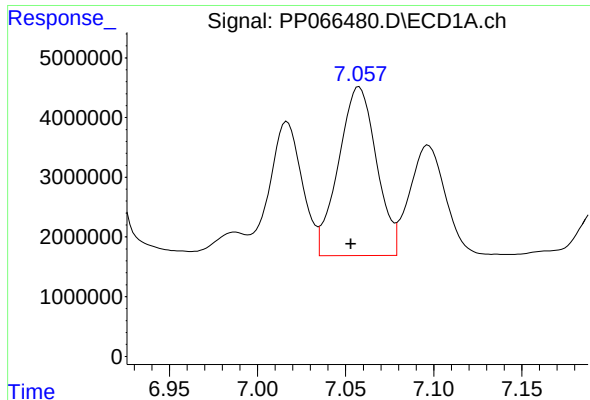

#27 AR-1254-2


R.T.: 7.058 min
Delta R.T.: 0.005 min
Response: 42379827
Conc: 300.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

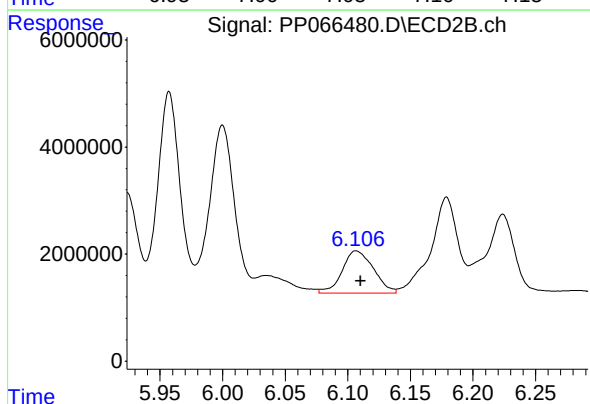


#27 AR-1254-2

R.T.: 6.107 min
Delta R.T.: -0.004 min
Response: 13743216
Conc: 165.48 ng/ml

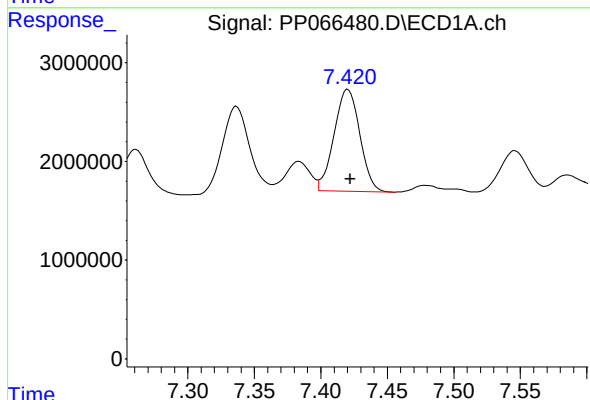


#28 AR-1254-3

R.T.: 7.420 min
Delta R.T.: -0.002 min
Response: 13919335
Conc: 107.32 ng/ml

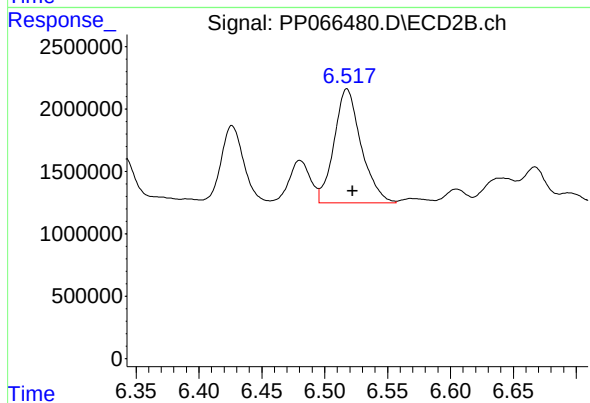

#28 AR-1254-3


R.T.: 6.518 min
Delta R.T.: -0.005 min
Response: 13674902
Conc: 109.45 ng/ml

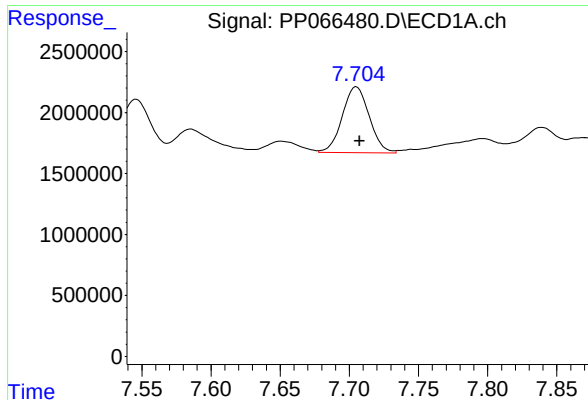

#29 AR-1254-4


R.T.: 7.705 min
Delta R.T.: -0.002 min
Response: 7312038
Conc: 79.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

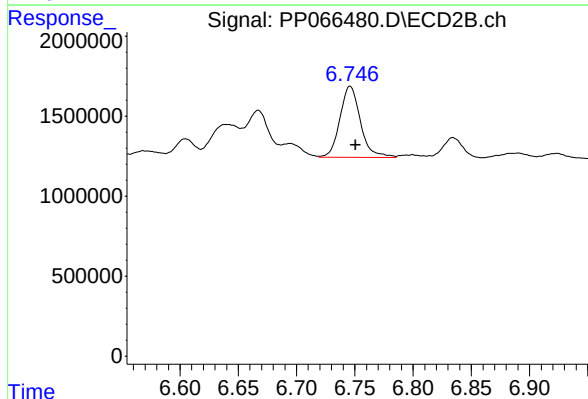


#29 AR-1254-4

R.T.: 6.746 min
Delta R.T.: -0.005 min
Response: 5435118
Conc: 79.43 ng/ml

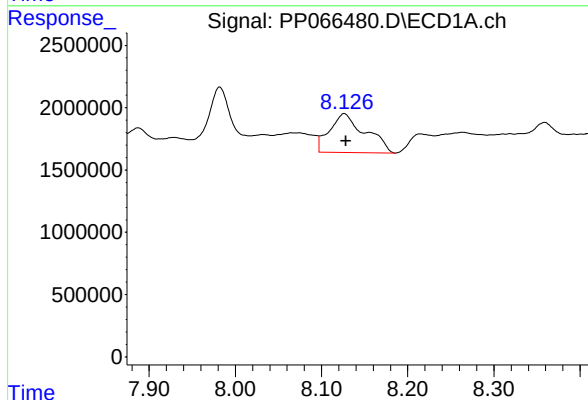


#30 AR-1254-5

R.T.: 8.127 min
Delta R.T.: -0.002 min
Response: 9021285
Conc: 90.76 ng/ml

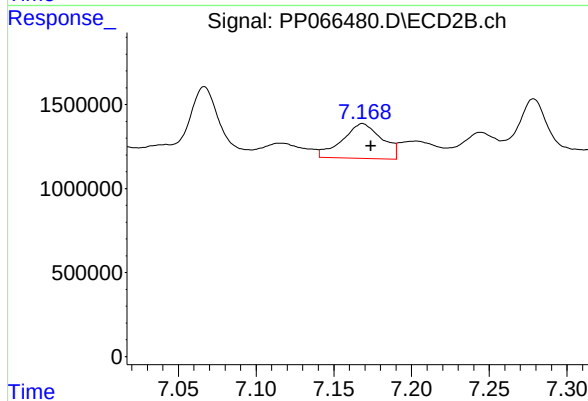

#30 AR-1254-5


R.T.: 7.168 min
Delta R.T.: -0.005 min
Response: 3658766
Conc: 36.44 ng/ml

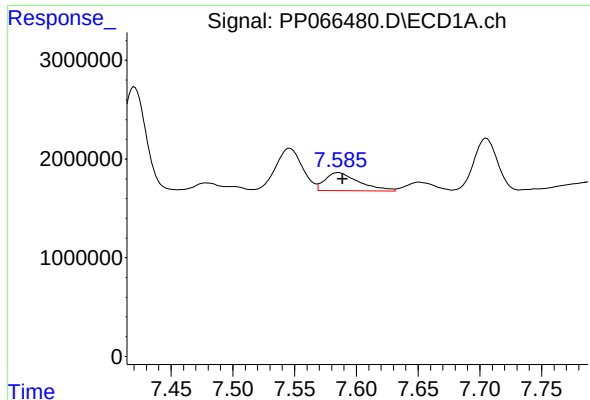

#31 AR-1260-1


R.T.: 7.586 min
Delta R.T.: -0.003 min
Response: 3474575
Conc: 32.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

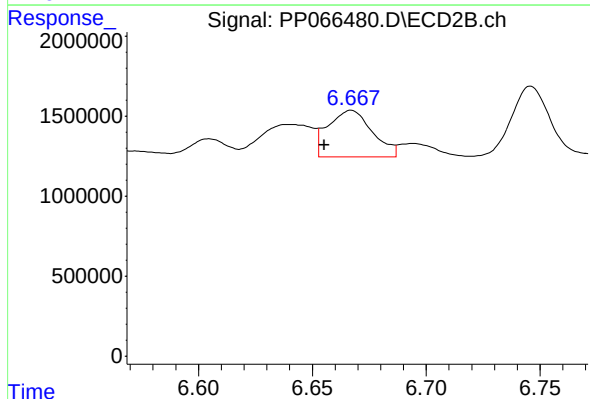


#31 AR-1260-1

R.T.: 6.667 min
Delta R.T.: 0.012 min
Response: 3945015
Conc: 46.15 ng/ml

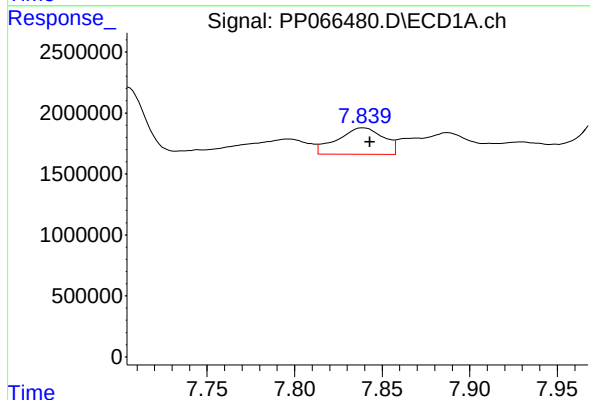


#32 AR-1260-2

R.T.: 7.839 min
Delta R.T.: -0.004 min
Response: 3968938
Conc: 34.45 ng/ml

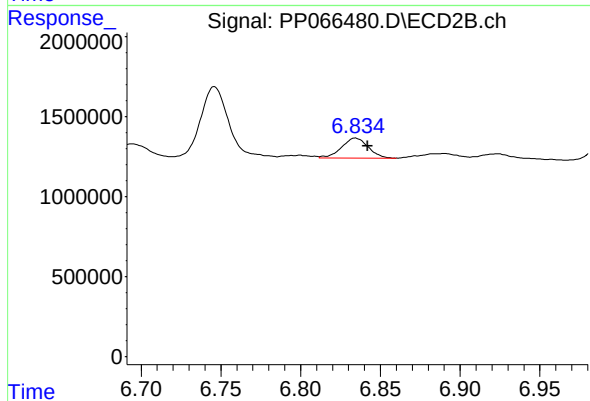

#32 AR-1260-2


R.T.: 6.834 min
Delta R.T.: -0.008 min
Response: 1442687
Conc: 14.84 ng/ml

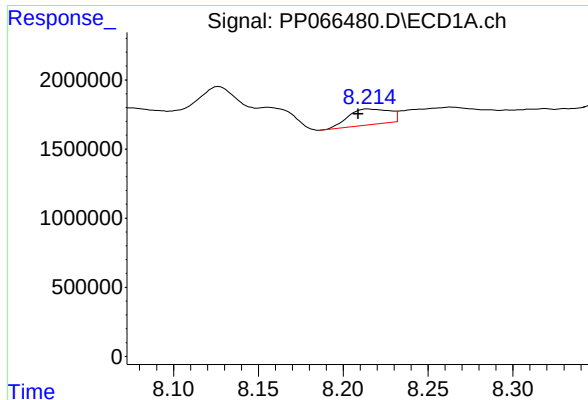

#33 AR-1260-3


R.T.: 8.215 min
Delta R.T.: 0.006 min
Response: 1934232
Conc: 24.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

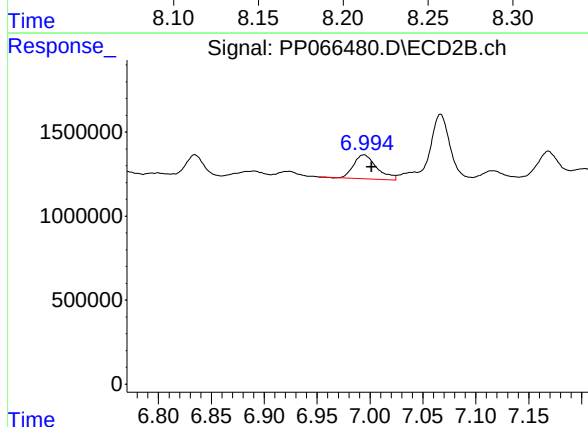


#33 AR-1260-3

R.T.: 6.994 min
Delta R.T.: -0.007 min
Response: 2163783
Conc: 23.58 ng/ml

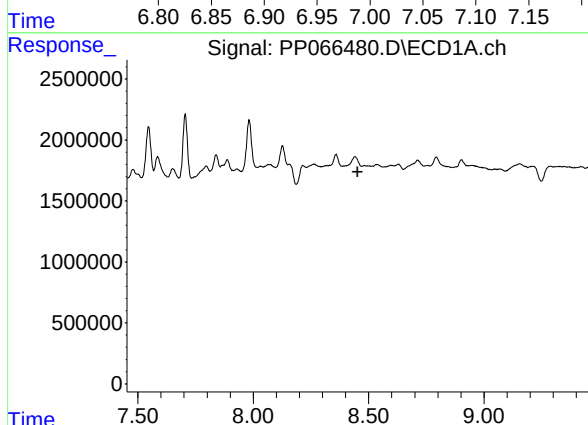


#34 AR-1260-4

R.T.: 8.441 min
Delta R.T.: -0.011 min
Response: -25654
Conc: N.D.

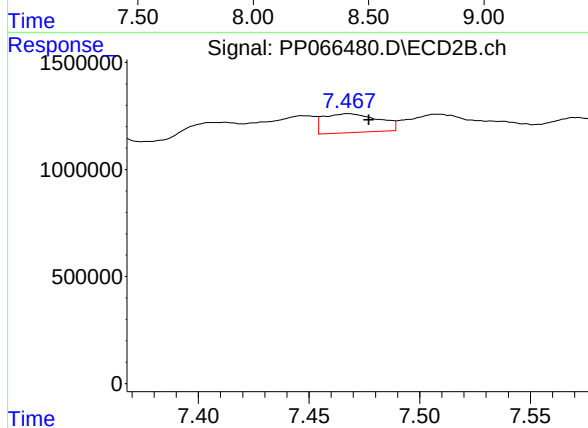

#34 AR-1260-4


R.T.: 7.468 min
Delta R.T.: -0.009 min
Response: 1529391
Conc: 23.53 ng/ml

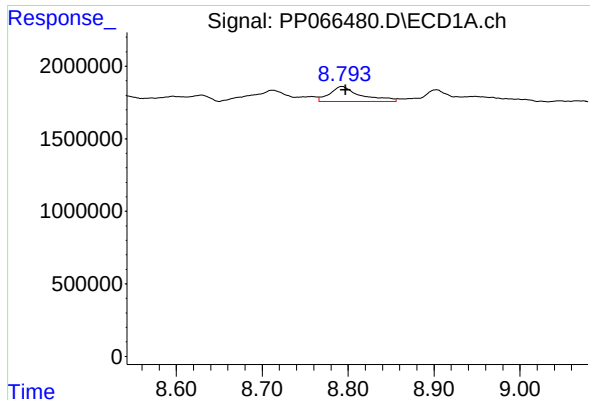

#35 AR-1260-5


R.T.: 8.793 min
Delta R.T.: -0.004 min
Response: 2626880
Conc: 16.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

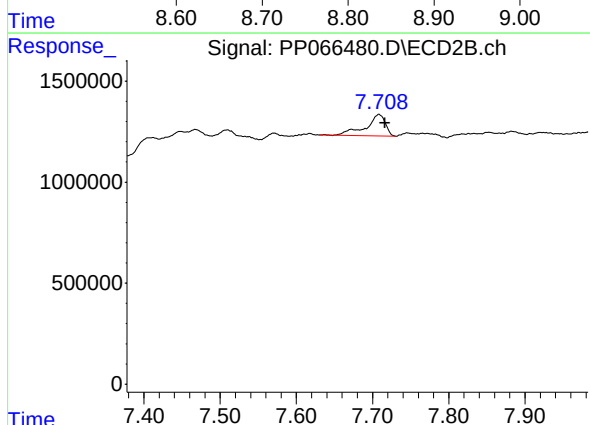


#35 AR-1260-5

R.T.: 7.708 min
Delta R.T.: -0.008 min
Response: 1880469
Conc: 13.38 ng/ml

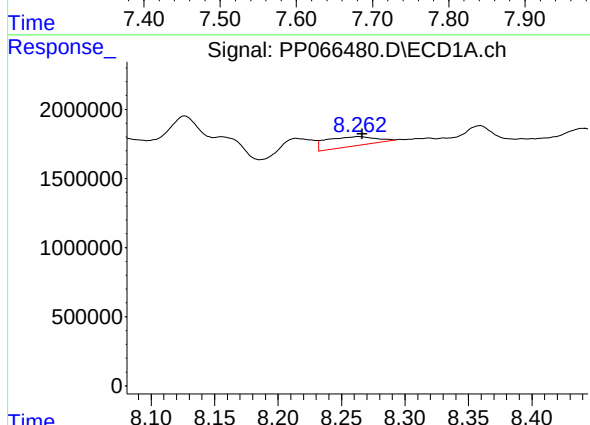


#36 AR-1262-1

R.T.: 8.264 min
Delta R.T.: -0.003 min
Response: 1871408
Conc: 33.19 ng/ml

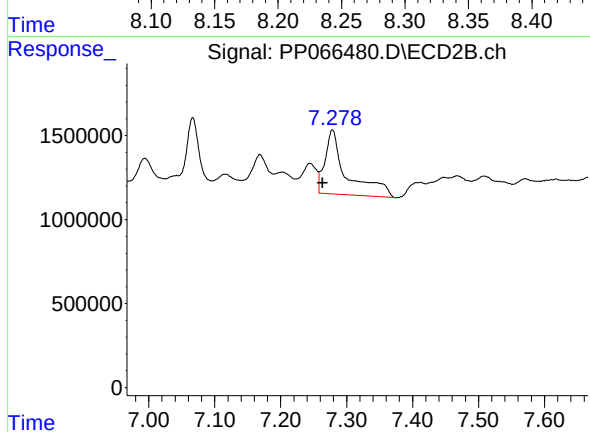

#36 AR-1262-1


R.T.: 7.279 min
Delta R.T.: 0.015 min
Response: 8760743
Conc: 184.10 ng/ml

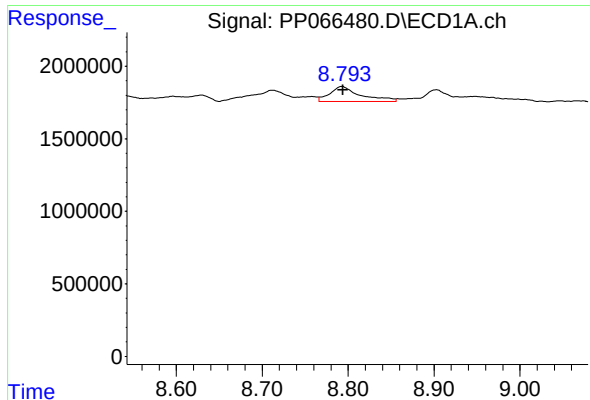

#37 AR-1262-2


R.T.: 8.793 min
Delta R.T.: -0.001 min
Response: 2626880
Conc: 13.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

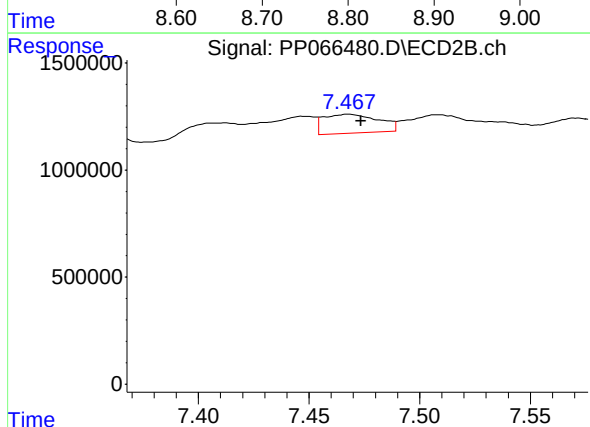


#37 AR-1262-2

R.T.: 7.468 min
Delta R.T.: -0.006 min
Response: 1529391
Conc: 16.35 ng/ml

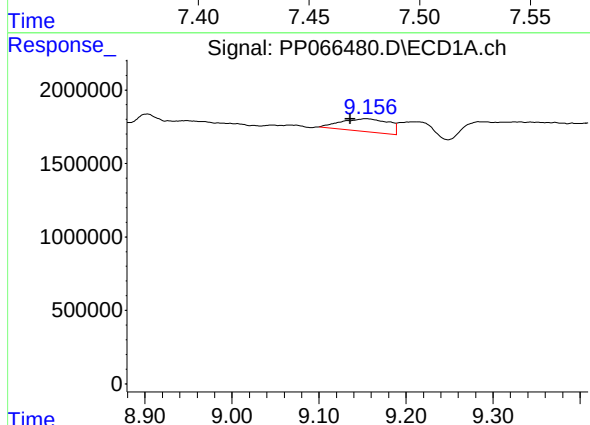


#38 AR-1262-3

R.T.: 9.154 min
Delta R.T.: 0.018 min
Response: 3304927
Conc: 25.32 ng/ml

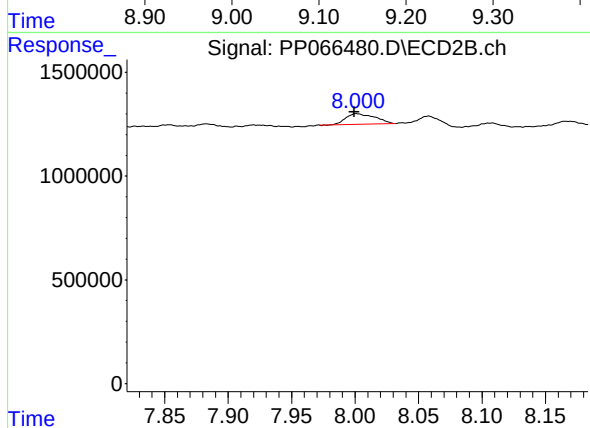

#38 AR-1262-3


R.T.: 8.001 min
Delta R.T.: 0.002 min
Response: 808593
Conc: 11.30 ng/ml

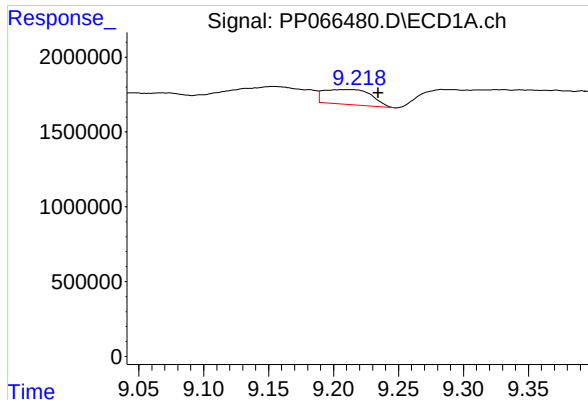

#39 AR-1262-4


R.T.: 9.213 min
Delta R.T.: -0.022 min
Response: 2558114
Conc: 22.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

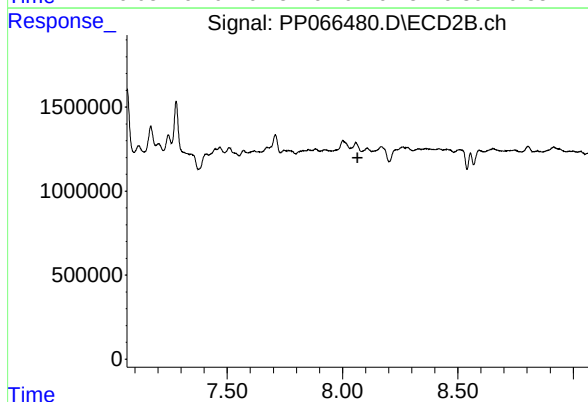


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.065 min
Response: 0
Conc: N.D.

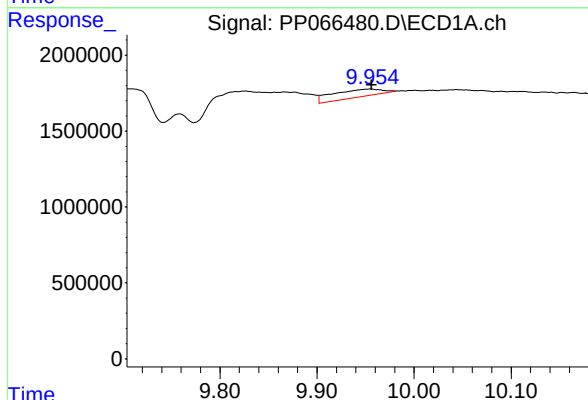


#40 AR-1262-5

R.T.: 9.954 min
Delta R.T.: -0.002 min
Response: 1783630
Conc: 27.39 ng/ml

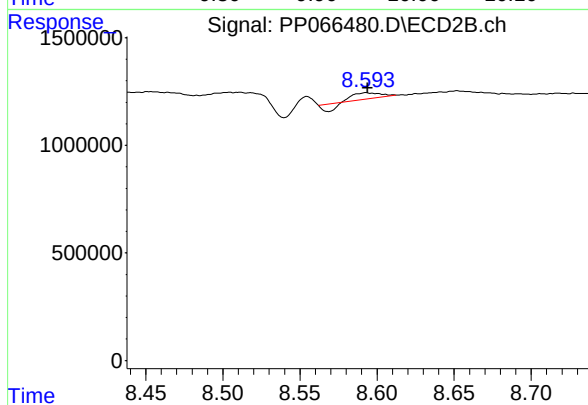

#40 AR-1262-5


R.T.: 8.593 min
Delta R.T.: 0.000 min
Response: 168360
Conc: 2.81 ng/ml

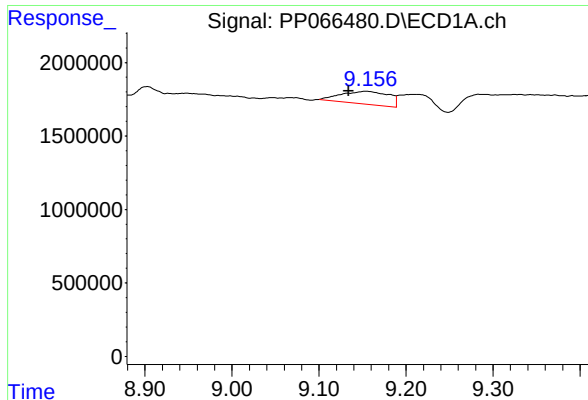

#41 AR-1268-1


R.T.: 9.154 min
Delta R.T.: 0.020 min
Response: 3304927
Conc: 14.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

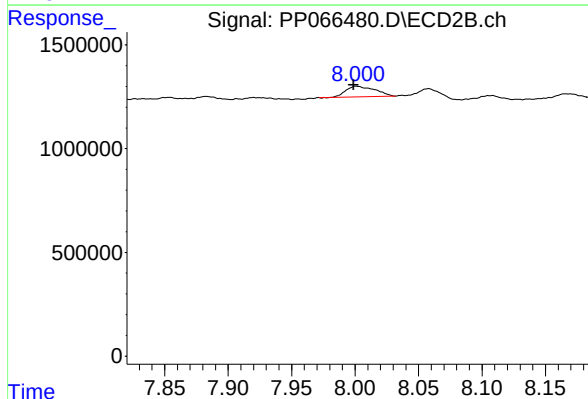


#41 AR-1268-1

R.T.: 8.001 min
Delta R.T.: 0.002 min
Response: 808593
Conc: 4.01 ng/ml

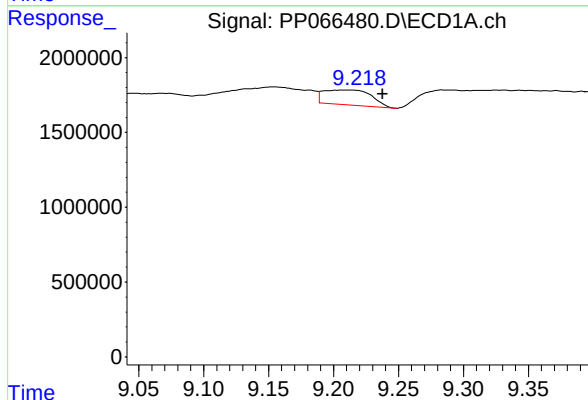


#42 AR-1268-2

R.T.: 9.213 min
Delta R.T.: -0.025 min
Response: 2558114
Conc: 11.99 ng/ml

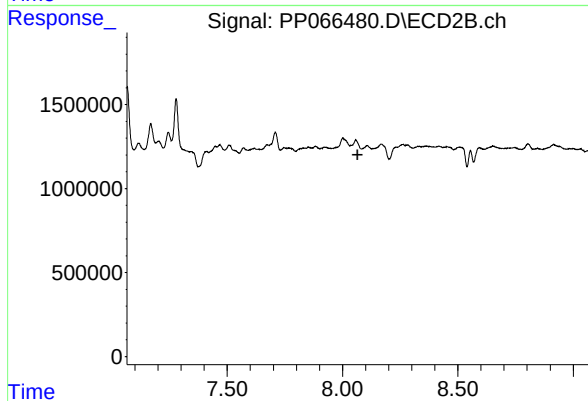

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.065 min
Response: 0
Conc: N.D.

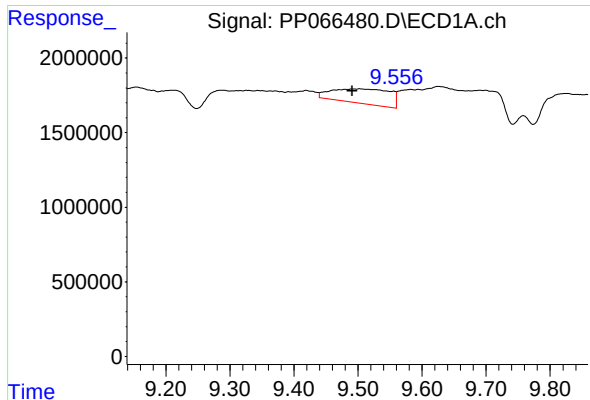

#43 AR-1268-3


R.T.: 9.503 min
Delta R.T.: 0.011 min
Response: 6194535
Conc: 32.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

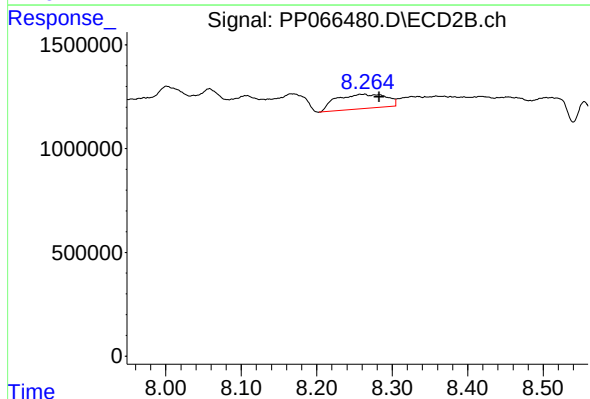


#43 AR-1268-3

R.T.: 8.263 min
Delta R.T.: -0.019 min
Response: 3222485
Conc: 19.93 ng/ml

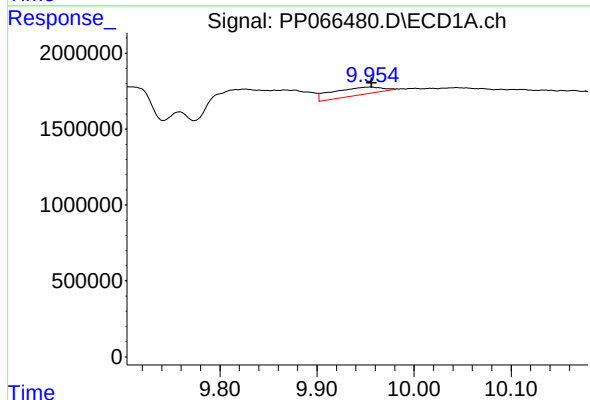


#44 AR-1268-4

R.T.: 9.954 min
Delta R.T.: -0.002 min
Response: 1783630
Conc: 25.57 ng/ml

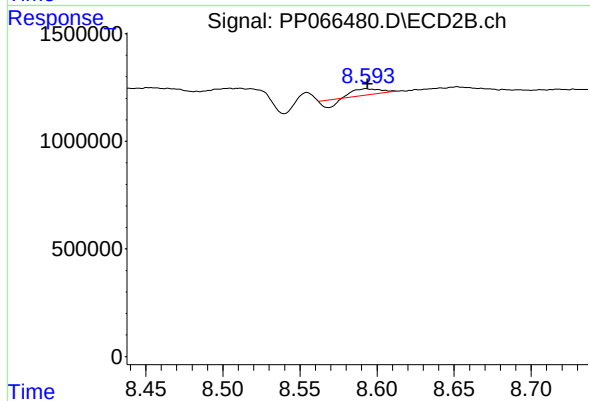

#44 AR-1268-4


R.T.: 8.593 min
Delta R.T.: 0.000 min
Response: 168360
Conc: 2.50 ng/ml

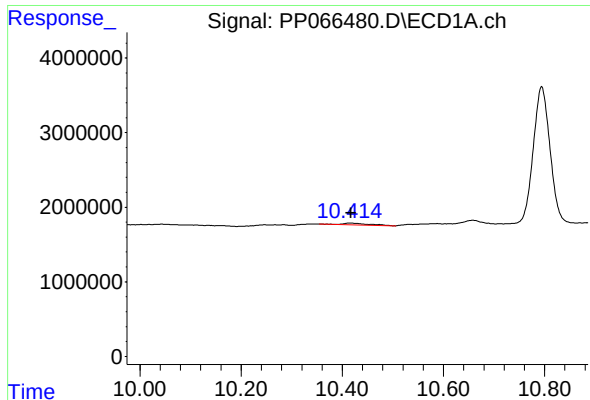

#45 AR-1268-5

R.T.: 10.414 min
Delta R.T.: -0.004 min
Response: 843977
Conc: 1.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVE

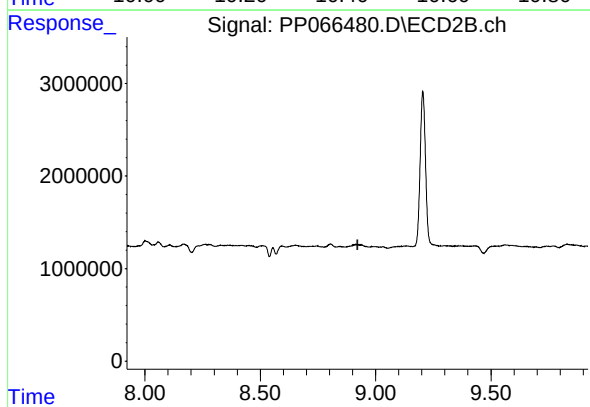

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.921 min
Response: 0
Conc: N.D.