

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072324\
 Data File : PP066481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 13:12
 Operator : YP\AJ
 Sample : P3324-01DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CONRAIL-01-VALVEDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 01:50:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 07:20:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.793	4.029	21918856	23269026	12.441	12.186
2) SA Decachlor...	10.795	9.206	20996899	14313438	11.962	11.218
Target Compounds						
3) L1 AR-1016-1	5.973	5.143	31171811	28101791	425.308	448.585
4) L1 AR-1016-2	5.998	5.163	79422963	41050912	726.268	461.226 #
5) L1 AR-1016-3	6.060	5.344	33645671	24915833	498.443	527.775
6) L1 AR-1016-4	6.159	5.382	33970834	17084772	612.036	447.712 #
7) L1 AR-1016-5	6.455	5.614	35696574	58254845	642.031	1201.946 #
8) L2 AR-1221-1	5.000	4.241	1466147	4711234	66.036	203.841 #
9) L2 AR-1221-2	5.107f	4.335	7225433	1997687	430.472	115.728 #
10) L2 AR-1221-3	5.166	4.412	19424985	21106346	379.181	417.512
11) L3 AR-1232-1	5.166	4.412	19424985	21106346	443.923	494.518
12) L3 AR-1232-2	5.703	5.143	24817863	28101791	960.458	952.841
13) L3 AR-1232-3	5.973	5.344	31171811	24915833	921.751	1118.693
14) L3 AR-1232-4	6.159	5.426	33970834	20813071	1310.535	1035.150
15) L3 AR-1232-5	6.247	5.614	23219062	58254845	1070.951	2734.947 #
16) L4 AR-1242-1	5.973	5.143	31171811	28101791	561.568	537.616
17) L4 AR-1242-2	5.998	5.163	79422963	41050912	887.505	568.322 #
18) L4 AR-1242-3	6.060	5.344	33645671	24915833	612.925	651.201
19) L4 AR-1242-4	6.159	5.426	33970834	20813071	741.910	548.365 #
20) L4 AR-1242-5	6.906	5.958	141.5E6	24968235	2844.215	553.458 #
21) L5 AR-1248-1	5.973	5.143	31171811	28101791	639.570	682.078
22) L5 AR-1248-2	6.247	5.382	23219062	17084772	304.171	300.844
23) L5 AR-1248-3	6.455	5.426	35696574	20813071	438.275	352.968
24) L5 AR-1248-4	6.860	5.614	27812868	58254845	298.602	849.270 #
25) L5 AR-1248-5	6.906	6.001	141.5E6	24680730	1533.348	393.533 #
26) L6 AR-1254-1	6.833	5.958	19542065	24968235	208.961	262.354 #
27) L6 AR-1254-2	7.059	6.108	23143809	8220131	164.076	98.977 #
28) L6 AR-1254-3	7.422	6.519	7543479	7699004	58.163	61.619
29) L6 AR-1254-4	7.707	6.747	3764258	2585745	41.051	37.790
30) L6 AR-1254-5	8.128	7.170	4628688	2244756	46.569	22.358 #
31) L7 AR-1260-1	7.586	6.648	1751000	1845314	16.552	21.585 #
32) L7 AR-1260-2	7.840	6.836	2190853	812878	19.016	8.359 #
33) L7 AR-1260-3	8.220	6.996	1346011	1307594	16.959	14.252
34) L7 AR-1260-4	8.443	7.450f	28542	4113098	0.328	63.289 #
35) L7 AR-1260-5	8.794	7.710	1397610	2351974	9.040	16.732 #
36) L8 AR-1262-1	8.264	7.280f	1949355	7652119	34.576	160.801 #
37) L8 AR-1262-2	8.794	7.450f	1397610	4113098	7.394	43.967 #
38) L8 AR-1262-3	9.161f	0.000	1862496	0	14.270	N.D. #
39) L8 AR-1262-4	9.221	0.000	1135350	0	10.087	N.D. #
40) L8 AR-1262-5	9.963	0.000	1242731	0	19.086	N.D. #
41) L9 AR-1268-1	9.161f	0.000	1862496	0	7.965	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072324\
 Data File : PP066481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 13:12
 Operator : YP\AJ
 Sample : P3324-01DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CONRAIL-01-VALVEDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 01:50:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 07:20:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.221f	0.000	1135350	0	5.321	N.D. #
43) L9	AR-1268-3	0.000	8.284	0	1432733	N.D.	8.860 #
44) L9	AR-1268-4	9.963	0.000	1242731	0	17.818	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072324\
Data File : PP066481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 13:12
Operator : YP\AJ
Sample : P3324-01DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 01:50:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 07:20:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

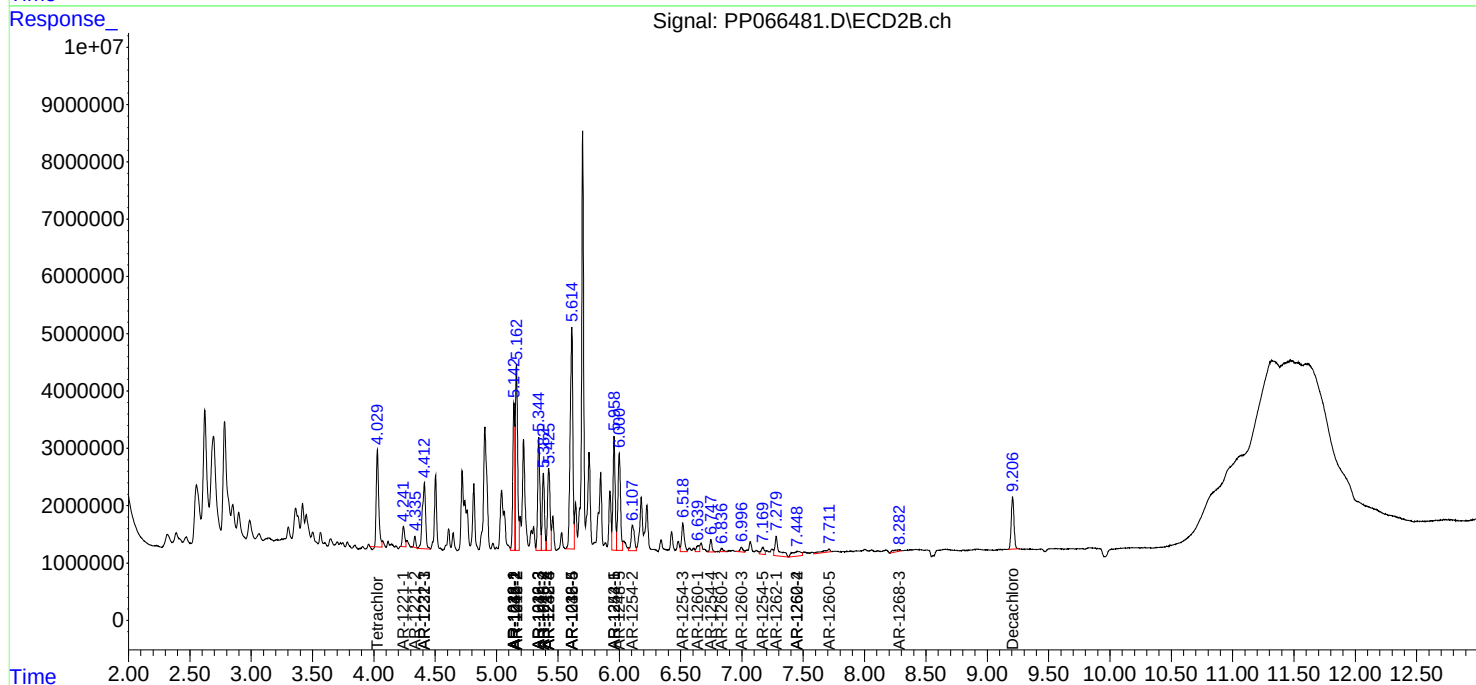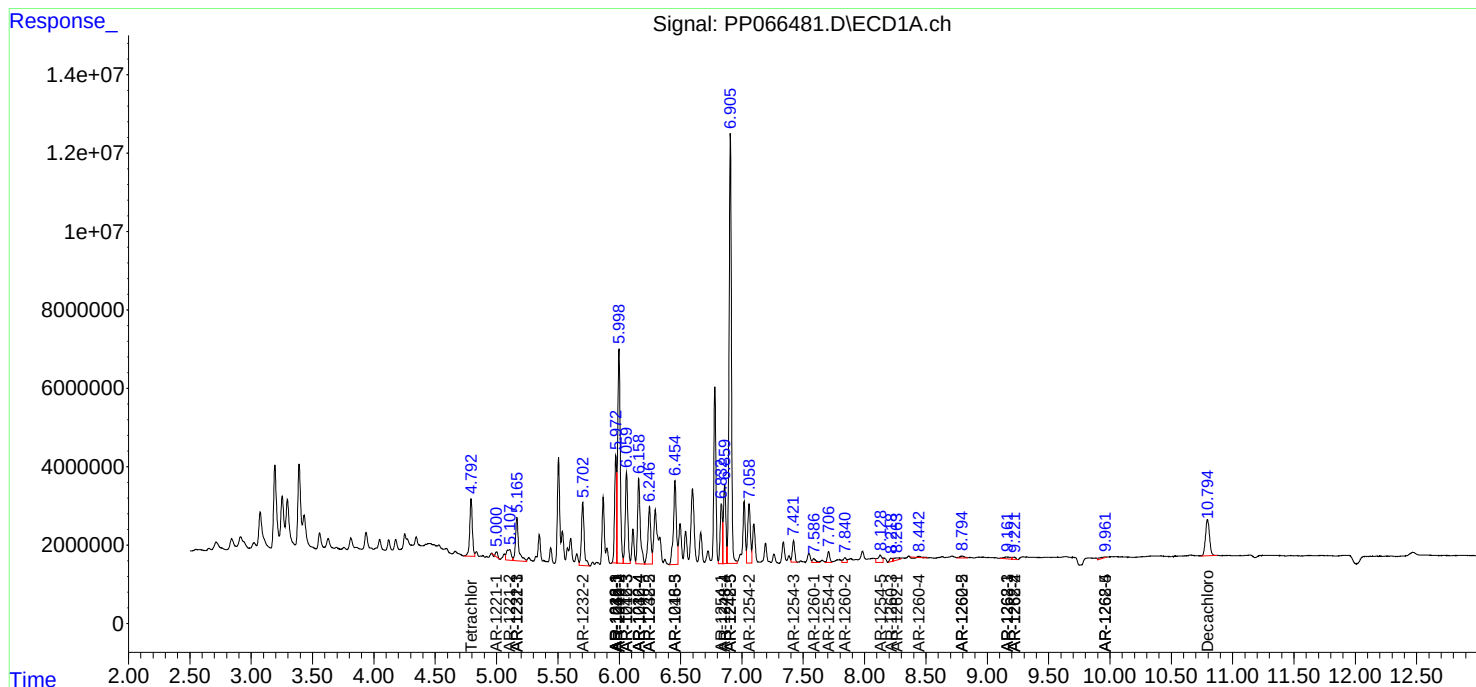


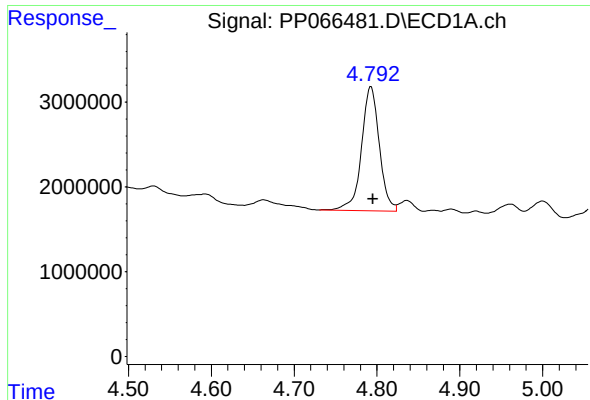

#1 Tetrachloro-m-xylene


R.T.: 4.793 min
Delta R.T.: -0.002 min
Response: 21918856
Conc: 12.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

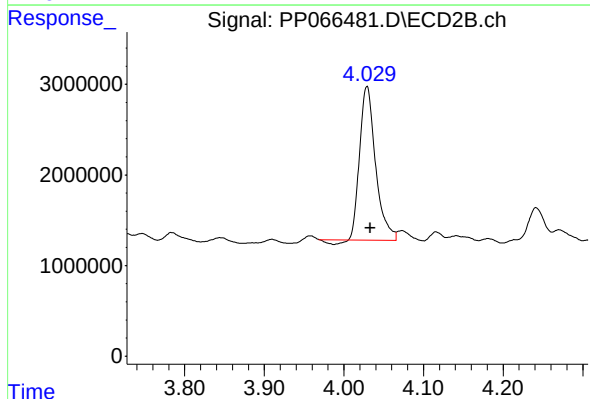


#1 Tetrachloro-m-xylene

R.T.: 4.029 min
Delta R.T.: -0.004 min
Response: 23269026
Conc: 12.19 ng/ml

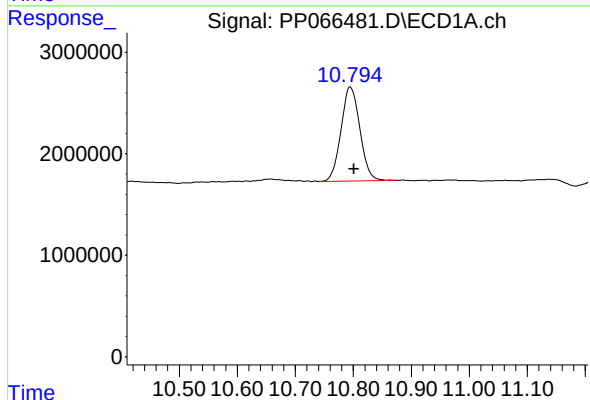


#2 Decachlorobiphenyl

R.T.: 10.795 min
Delta R.T.: -0.006 min
Response: 20996899
Conc: 11.96 ng/ml

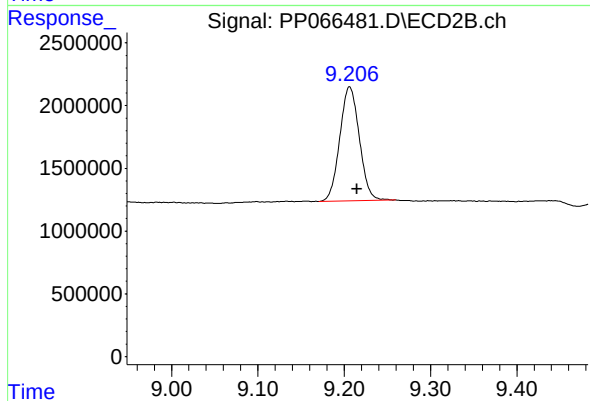

#2 Decachlorobiphenyl


R.T.: 9.206 min
Delta R.T.: -0.008 min
Response: 14313438
Conc: 11.22 ng/ml

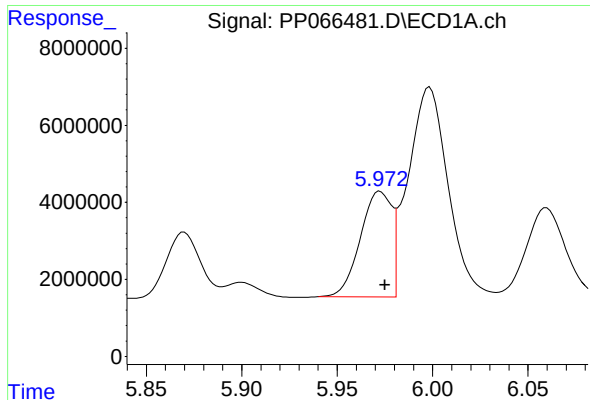

#3 AR-1016-1


R.T.: 5.973 min
Delta R.T.: -0.002 min
Response: 31171811
Conc: 425.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

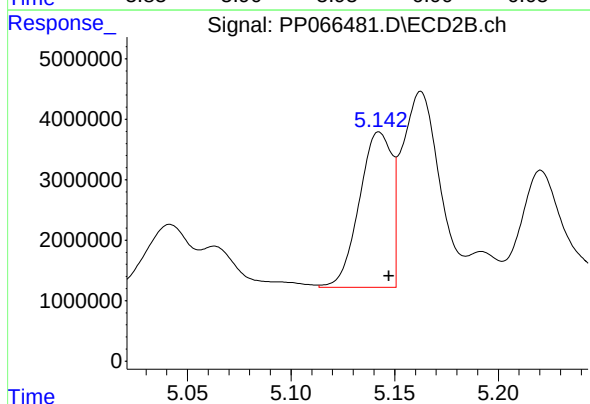


#3 AR-1016-1

R.T.: 5.143 min
Delta R.T.: -0.005 min
Response: 28101791
Conc: 448.59 ng/ml

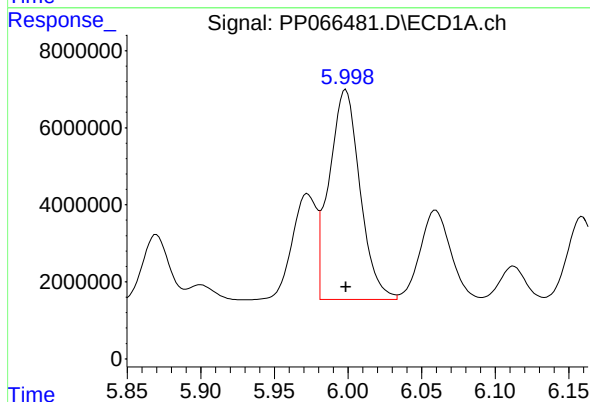


#4 AR-1016-2

R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 79422963
Conc: 726.27 ng/ml

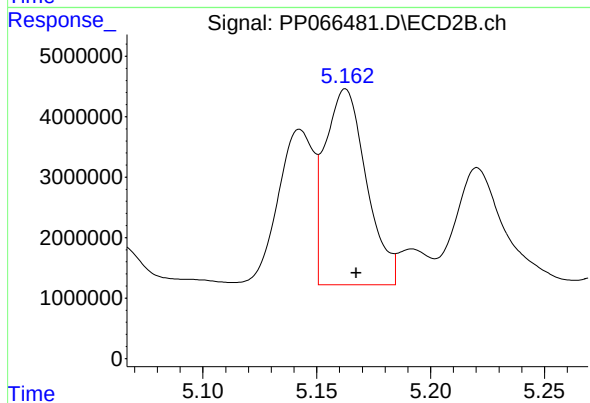

#4 AR-1016-2


R.T.: 5.163 min
Delta R.T.: -0.005 min
Response: 41050912
Conc: 461.23 ng/ml

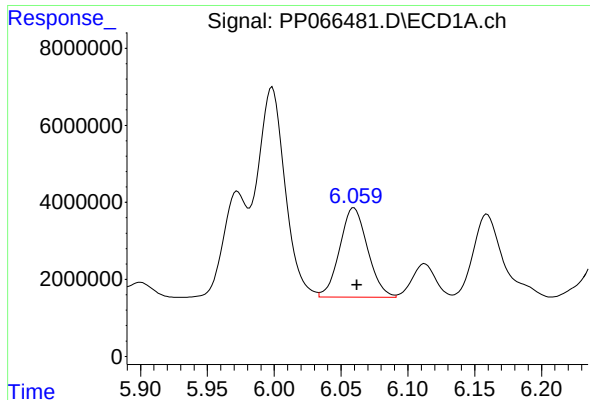

#5 AR-1016-3


R.T.: 6.060 min
Delta R.T.: -0.002 min
Response: 33645671
Conc: 498.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

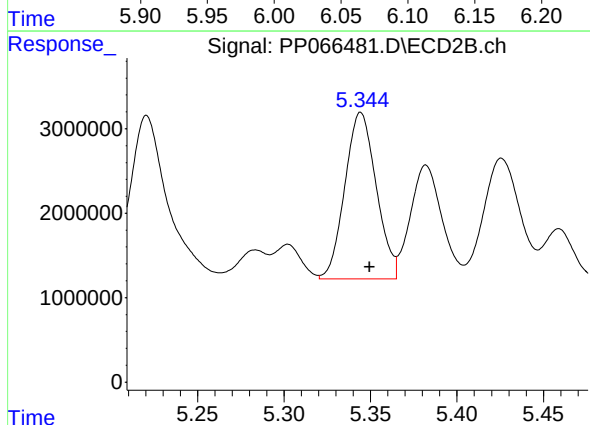


#5 AR-1016-3

R.T.: 5.344 min
Delta R.T.: -0.005 min
Response: 24915833
Conc: 527.77 ng/ml

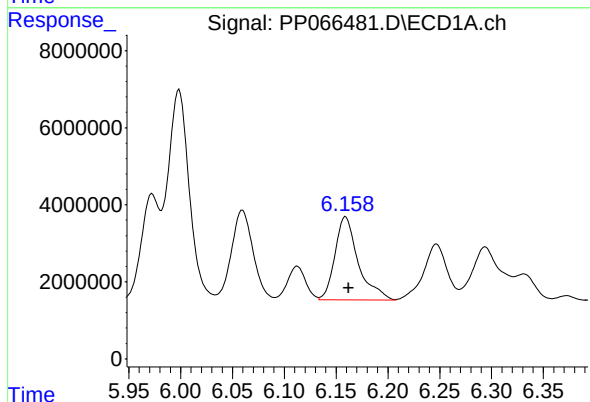


#6 AR-1016-4

R.T.: 6.159 min
Delta R.T.: -0.003 min
Response: 33970834
Conc: 612.04 ng/ml

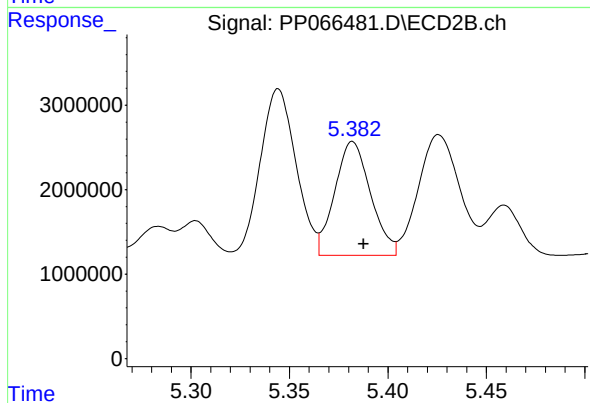

#6 AR-1016-4


R.T.: 5.382 min
Delta R.T.: -0.006 min
Response: 17084772
Conc: 447.71 ng/ml

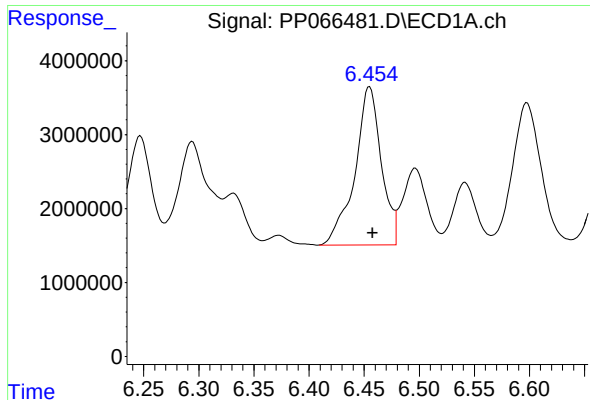

#7 AR-1016-5


R.T.: 6.455 min
Delta R.T.: -0.003 min
Response: 35696574
Conc: 642.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

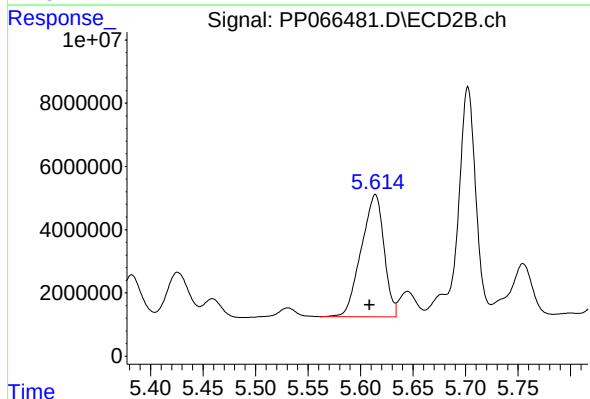


#7 AR-1016-5

R.T.: 5.614 min
Delta R.T.: 0.005 min
Response: 58254845
Conc: 1201.95 ng/ml

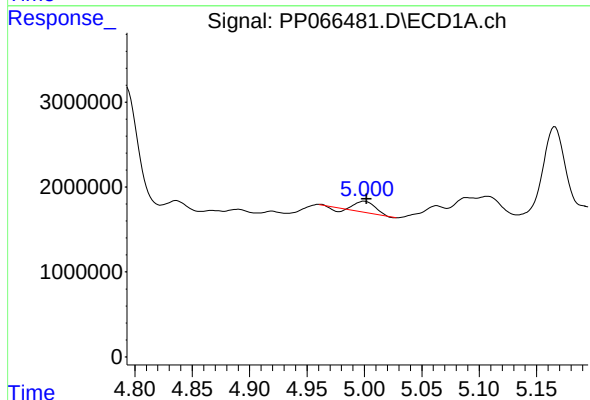


#8 AR-1221-1

R.T.: 5.000 min
Delta R.T.: -0.002 min
Response: 1466147
Conc: 66.04 ng/ml

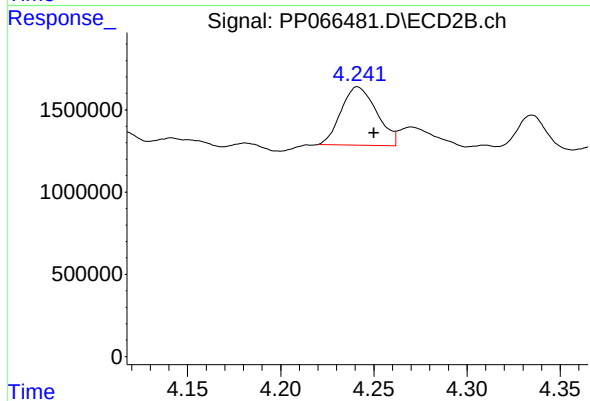

#8 AR-1221-1


R.T.: 4.241 min
Delta R.T.: -0.009 min
Response: 4711234
Conc: 203.84 ng/ml

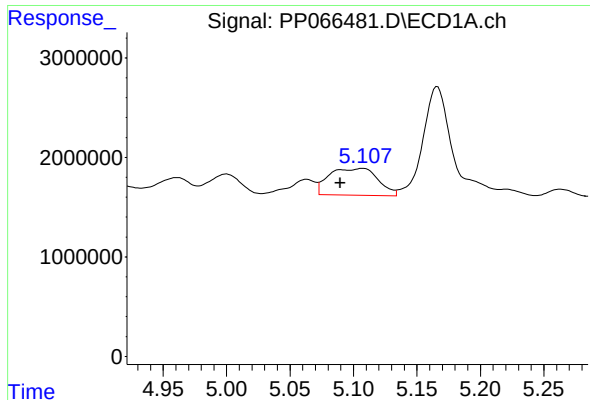

#9 AR-1221-2


R.T.: 5.107 min
Delta R.T.: 0.018 min
Response: 7225433
Conc: 430.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

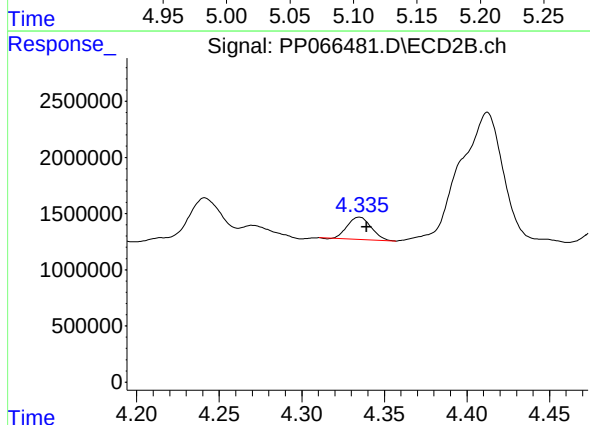


#9 AR-1221-2

R.T.: 4.335 min
Delta R.T.: -0.004 min
Response: 1997687
Conc: 115.73 ng/ml

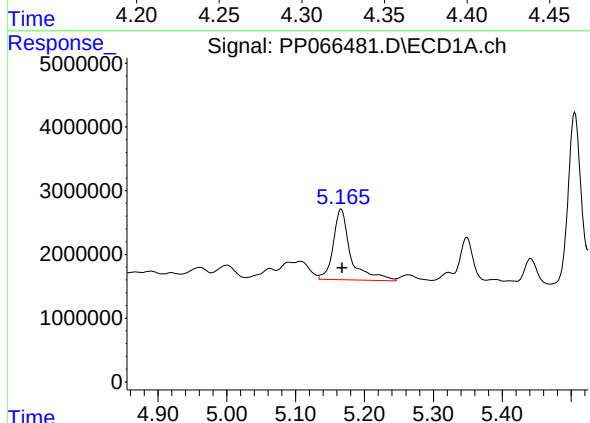


#10 AR-1221-3

R.T.: 5.166 min
Delta R.T.: -0.002 min
Response: 19424985
Conc: 379.18 ng/ml

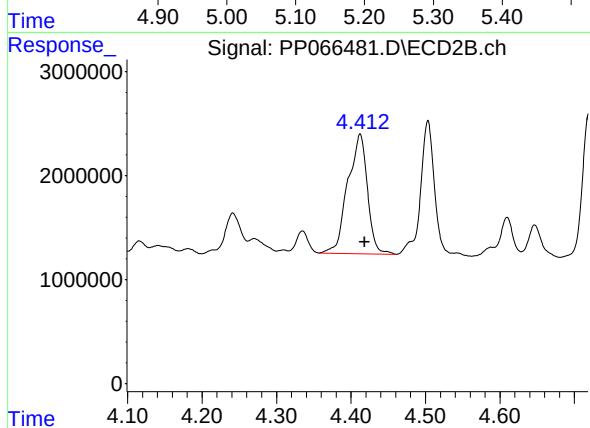

#10 AR-1221-3


R.T.: 4.412 min
Delta R.T.: -0.006 min
Response: 21106346
Conc: 417.51 ng/ml

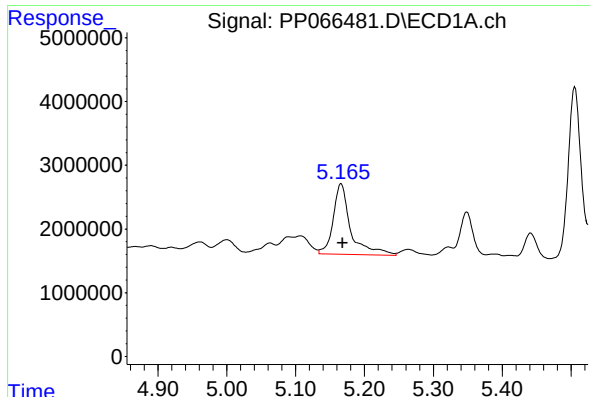

#11 AR-1232-1


R.T.: 5.166 min
Delta R.T.: -0.002 min
Response: 19424985
Conc: 443.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

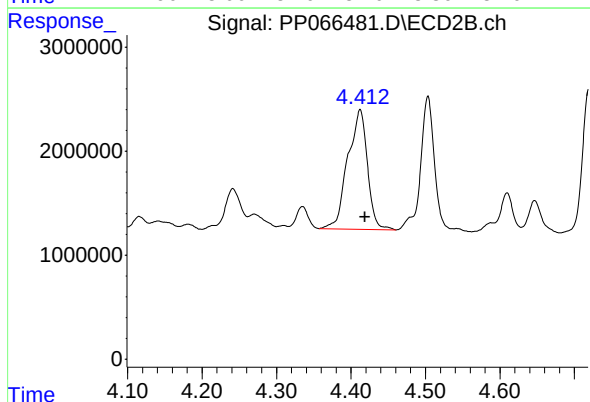


#11 AR-1232-1

R.T.: 4.412 min
Delta R.T.: -0.006 min
Response: 21106346
Conc: 494.52 ng/ml

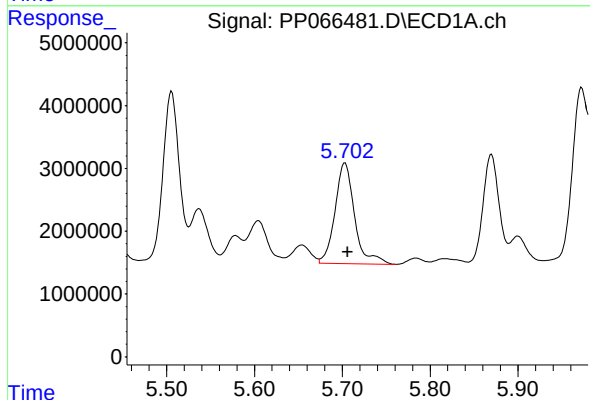


#12 AR-1232-2

R.T.: 5.703 min
Delta R.T.: -0.003 min
Response: 24817863
Conc: 960.46 ng/ml

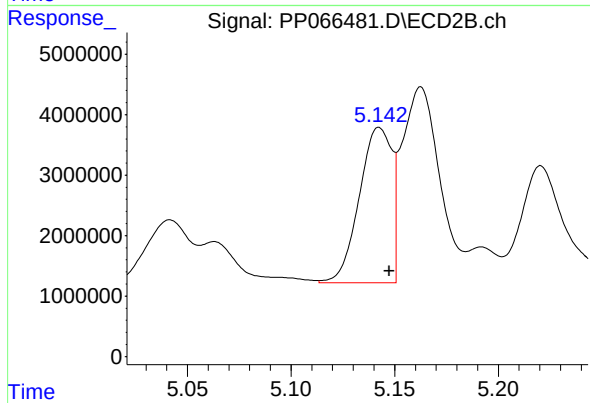

#12 AR-1232-2


R.T.: 5.143 min
Delta R.T.: -0.005 min
Response: 28101791
Conc: 952.84 ng/ml

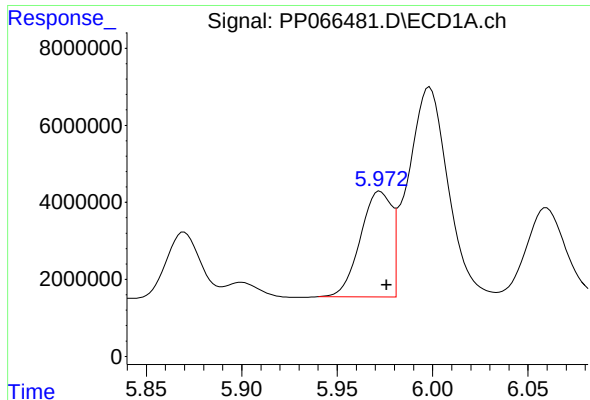

#13 AR-1232-3


R.T.: 5.973 min
Delta R.T.: -0.003 min
Response: 31171811
Conc: 921.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

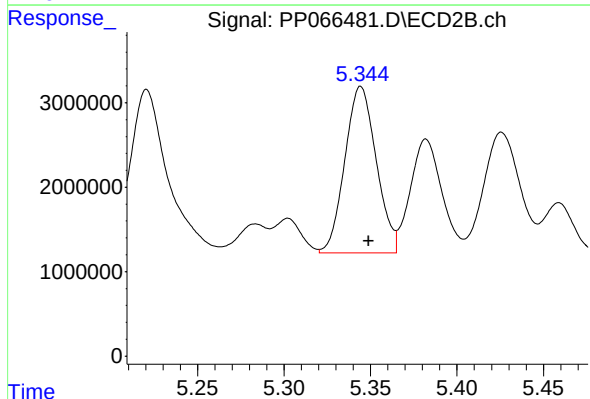


#13 AR-1232-3

R.T.: 5.344 min
Delta R.T.: -0.005 min
Response: 24915833
Conc: 1118.69 ng/ml

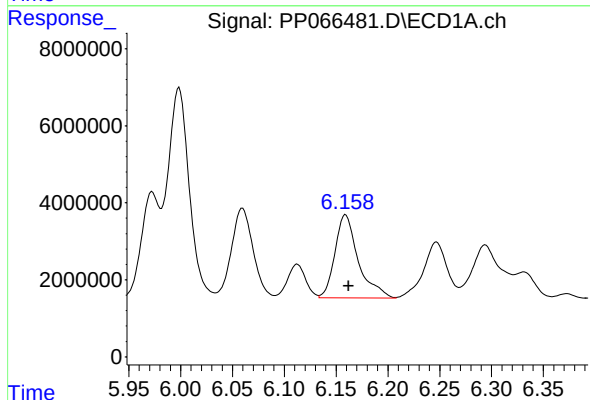


#14 AR-1232-4

R.T.: 6.159 min
Delta R.T.: -0.003 min
Response: 33970834
Conc: 1310.53 ng/ml

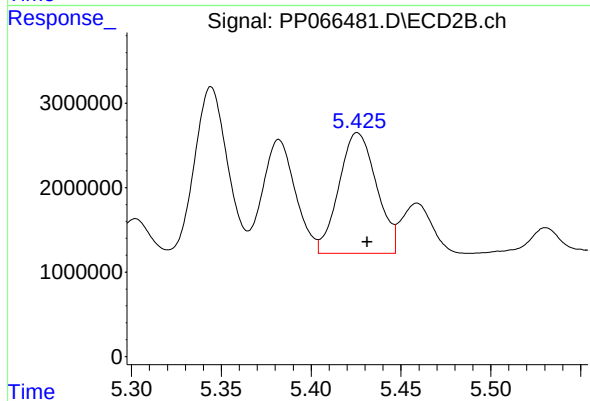

#14 AR-1232-4


R.T.: 5.426 min
Delta R.T.: -0.005 min
Response: 20813071
Conc: 1035.15 ng/ml

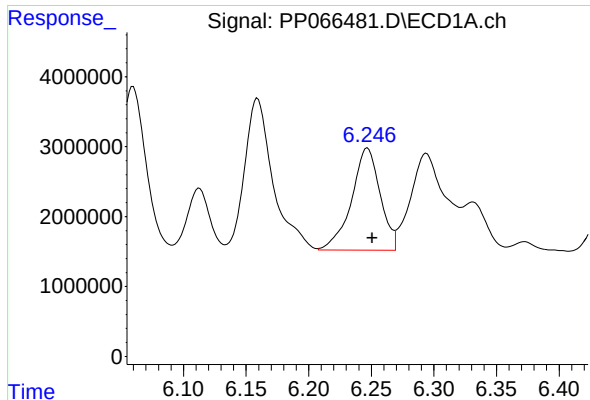

#15 AR-1232-5


R.T.: 6.247 min
Delta R.T.: -0.004 min
Response: 23219062
Conc: 1070.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

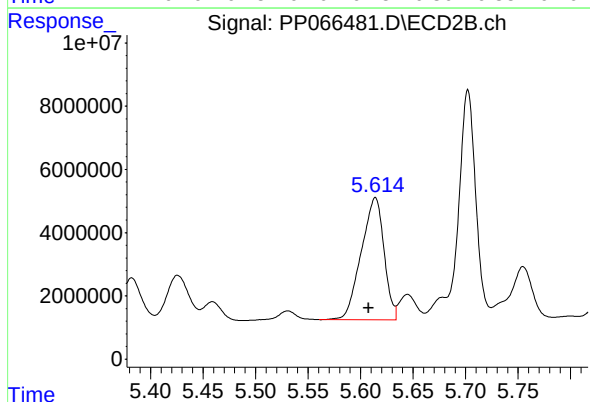


#15 AR-1232-5

R.T.: 5.614 min
Delta R.T.: 0.006 min
Response: 58254845
Conc: 2734.95 ng/ml

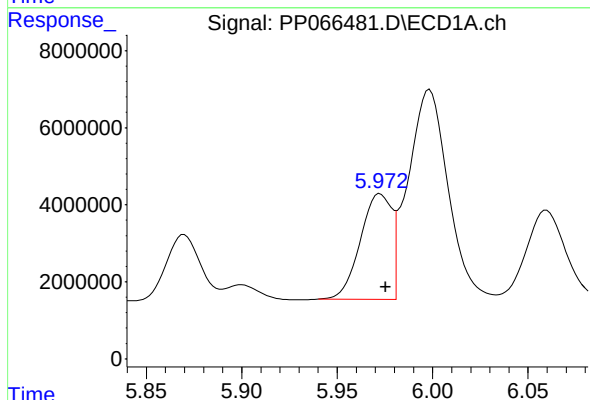


#16 AR-1242-1

R.T.: 5.973 min
Delta R.T.: -0.003 min
Response: 31171811
Conc: 561.57 ng/ml

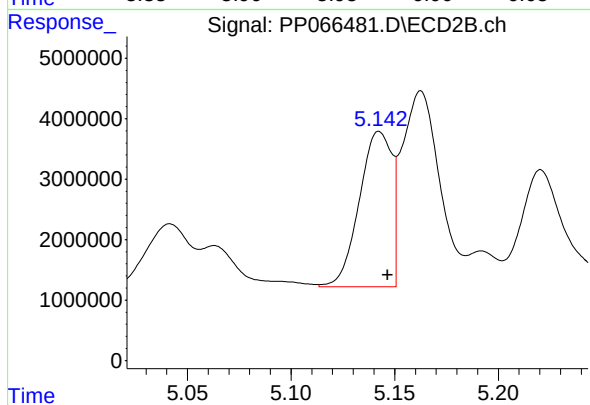

#16 AR-1242-1


R.T.: 5.143 min
Delta R.T.: -0.004 min
Response: 28101791
Conc: 537.62 ng/ml

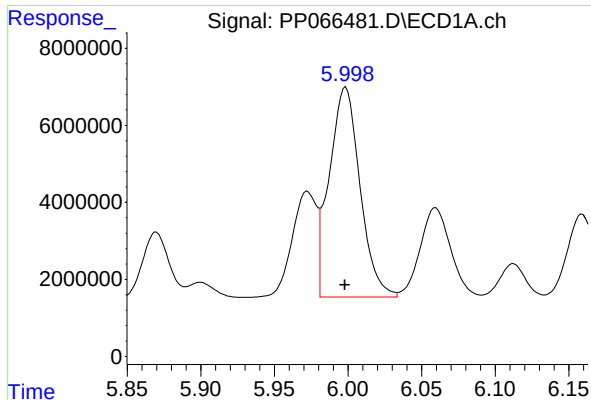

#17 AR-1242-2


R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 79422963
Conc: 887.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

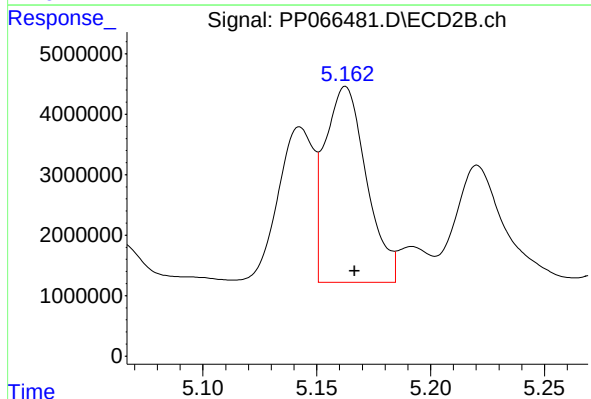


#17 AR-1242-2

R.T.: 5.163 min
Delta R.T.: -0.004 min
Response: 41050912
Conc: 568.32 ng/ml

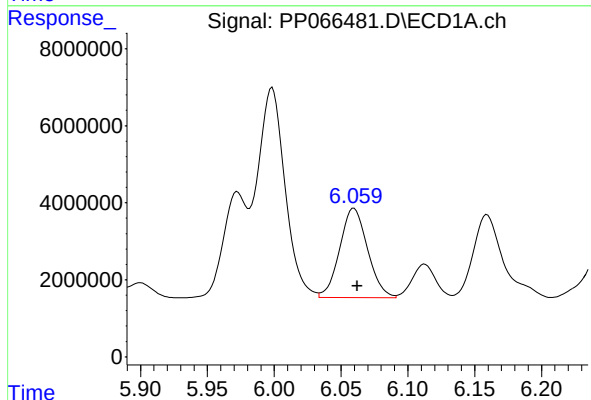


#18 AR-1242-3

R.T.: 6.060 min
Delta R.T.: -0.002 min
Response: 33645671
Conc: 612.93 ng/ml

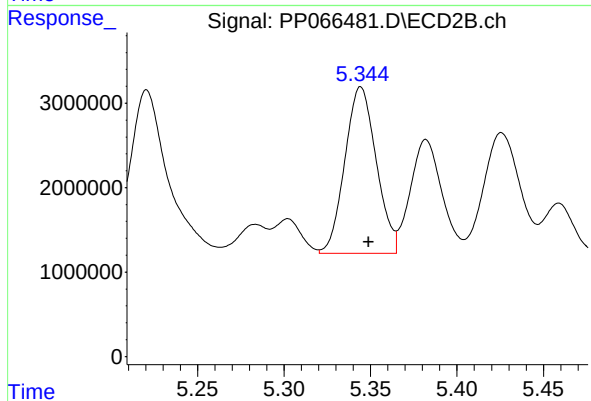

#18 AR-1242-3


R.T.: 5.344 min
Delta R.T.: -0.005 min
Response: 24915833
Conc: 651.20 ng/ml

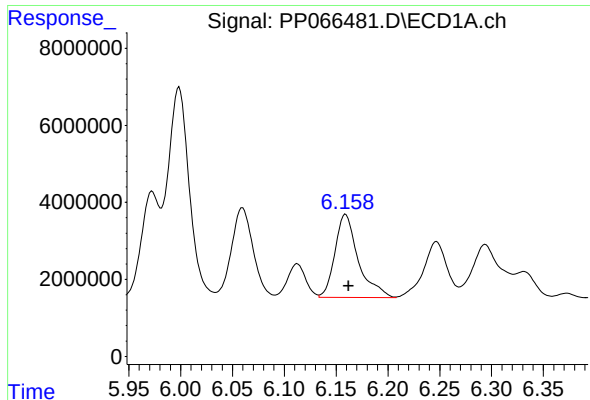

#19 AR-1242-4


R.T.: 6.159 min
Delta R.T.: -0.003 min
Response: 33970834
Conc: 741.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

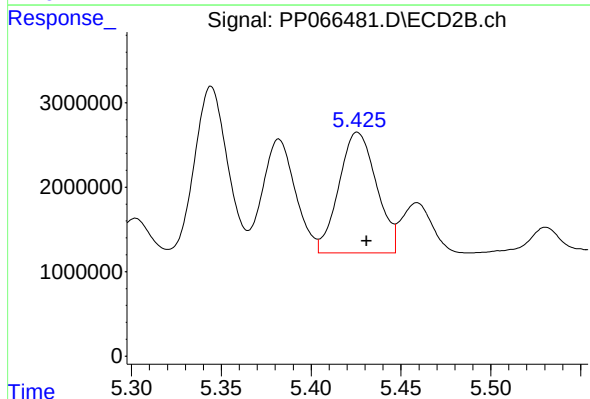


#19 AR-1242-4

R.T.: 5.426 min
Delta R.T.: -0.005 min
Response: 20813071
Conc: 548.36 ng/ml

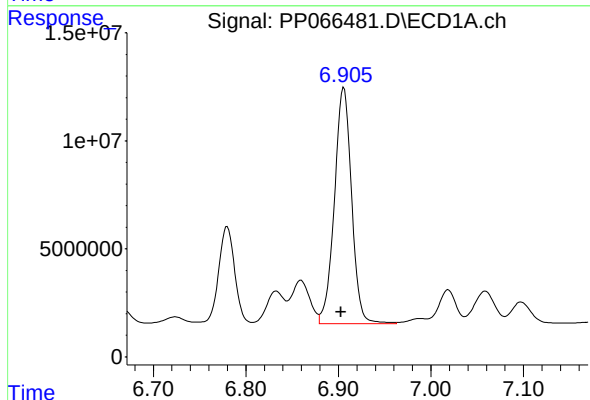


#20 AR-1242-5

R.T.: 6.906 min
Delta R.T.: 0.003 min
Response: 141470364
Conc: 2844.21 ng/ml

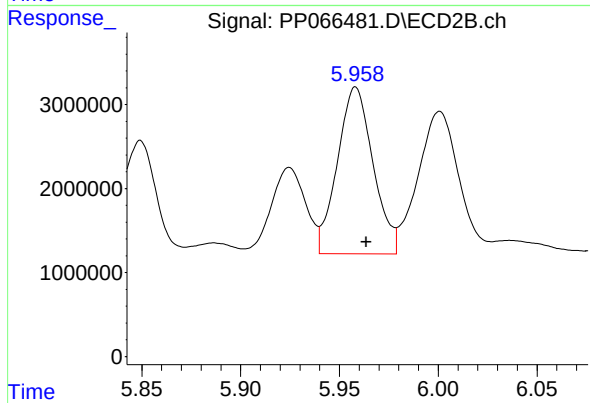

#20 AR-1242-5


R.T.: 5.958 min
Delta R.T.: -0.005 min
Response: 24968235
Conc: 553.46 ng/ml

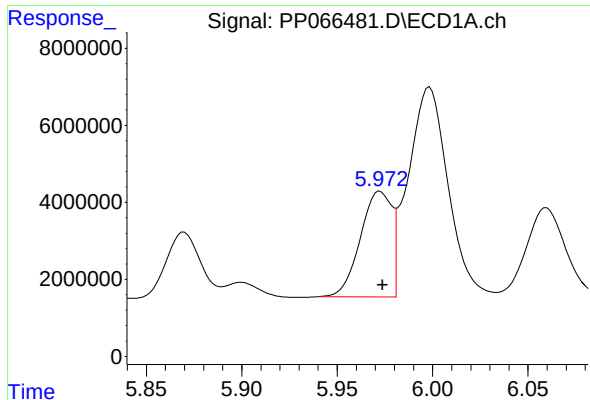

#21 AR-1248-1


R.T.: 5.973 min
Delta R.T.: -0.001 min
Response: 31171811
Conc: 639.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

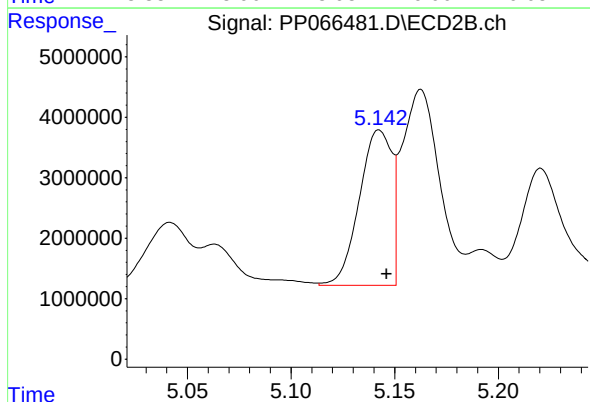


#21 AR-1248-1

R.T.: 5.143 min
Delta R.T.: -0.004 min
Response: 28101791
Conc: 682.08 ng/ml

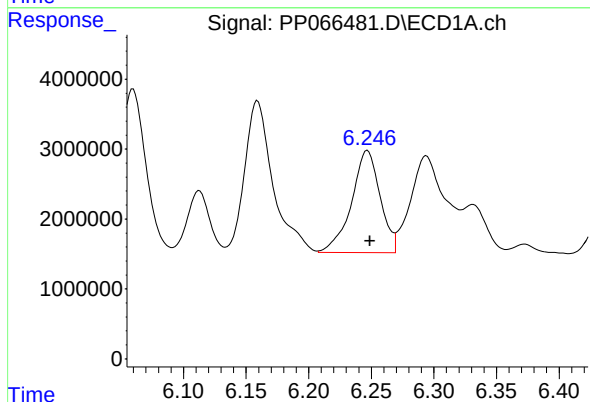


#22 AR-1248-2

R.T.: 6.247 min
Delta R.T.: -0.002 min
Response: 23219062
Conc: 304.17 ng/ml

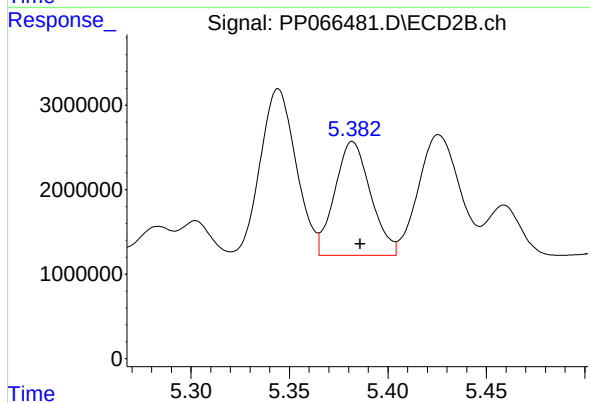

#22 AR-1248-2


R.T.: 5.382 min
Delta R.T.: -0.004 min
Response: 17084772
Conc: 300.84 ng/ml

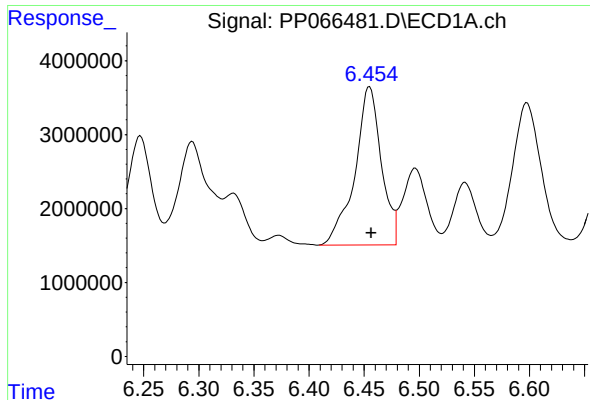

#23 AR-1248-3


R.T.: 6.455 min
Delta R.T.: -0.002 min
Response: 35696574
Conc: 438.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

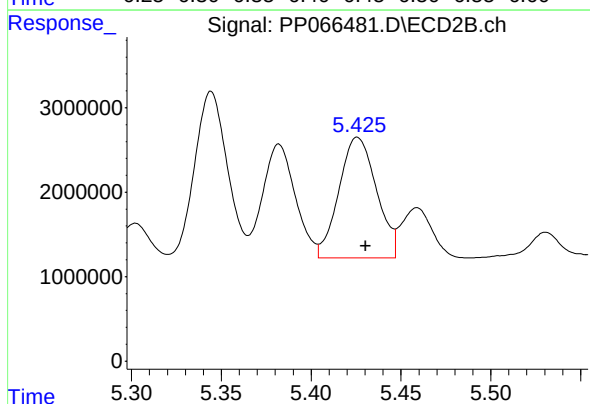


#23 AR-1248-3

R.T.: 5.426 min
Delta R.T.: -0.005 min
Response: 20813071
Conc: 352.97 ng/ml

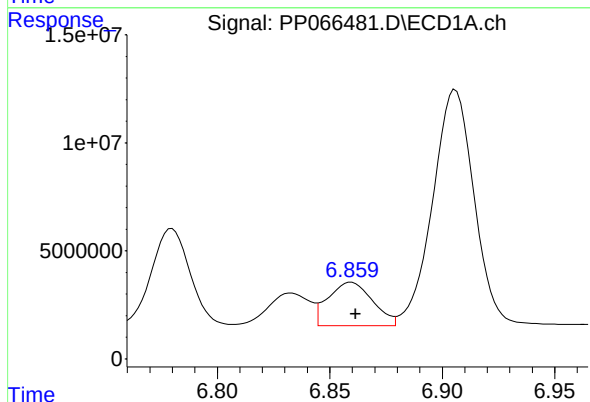


#24 AR-1248-4

R.T.: 6.860 min
Delta R.T.: -0.002 min
Response: 27812868
Conc: 298.60 ng/ml

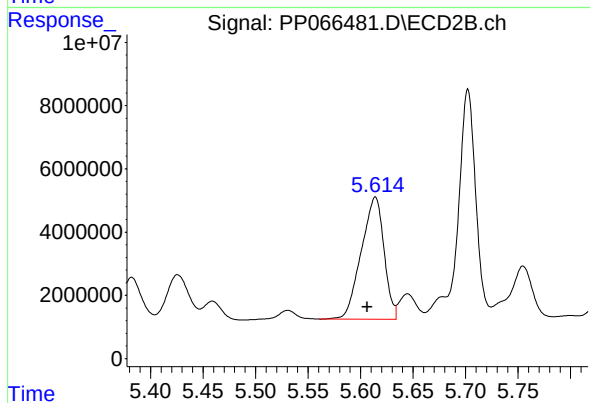

#24 AR-1248-4


R.T.: 5.614 min
Delta R.T.: 0.008 min
Response: 58254845
Conc: 849.27 ng/ml

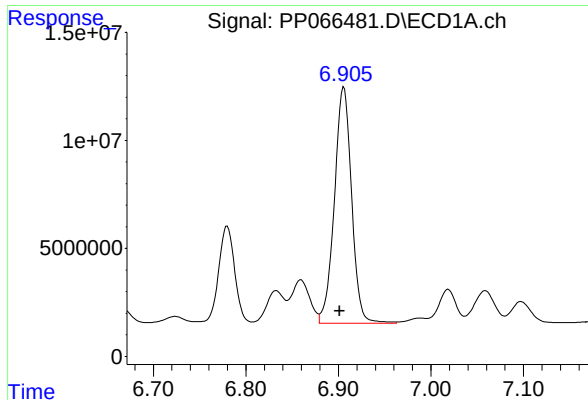

#25 AR-1248-5


R.T.: 6.906 min
Delta R.T.: 0.004 min
Response: 141470364
Conc: 1533.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

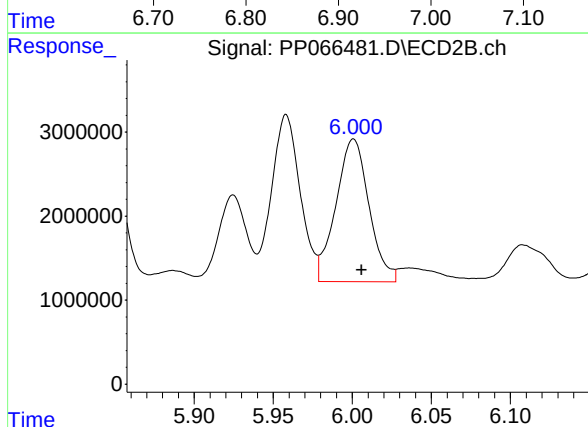


#25 AR-1248-5

R.T.: 6.001 min
Delta R.T.: -0.005 min
Response: 24680730
Conc: 393.53 ng/ml

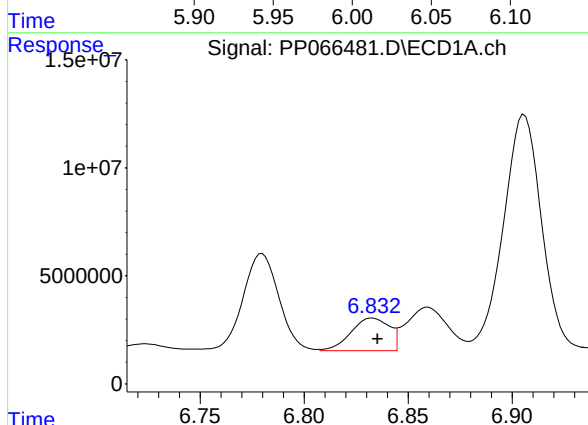


#26 AR-1254-1

R.T.: 6.833 min
Delta R.T.: -0.002 min
Response: 19542065
Conc: 208.96 ng/ml

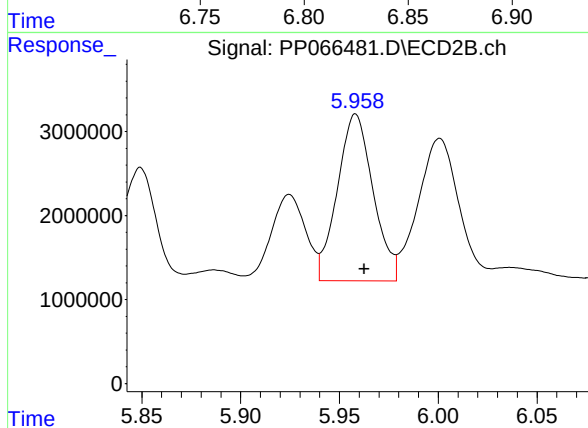

#26 AR-1254-1


R.T.: 5.958 min
Delta R.T.: -0.004 min
Response: 24968235
Conc: 262.35 ng/ml

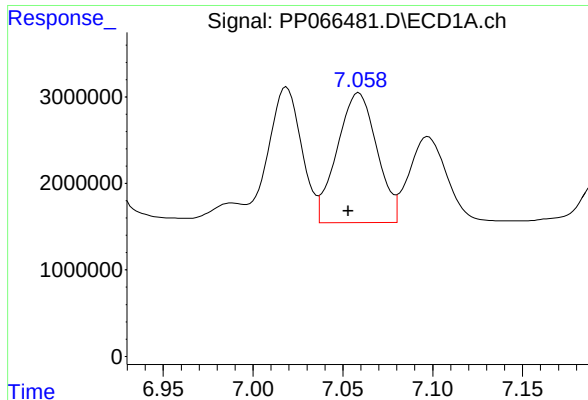

#27 AR-1254-2


R.T.: 7.059 min
Delta R.T.: 0.006 min
Response: 23143809
Conc: 164.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

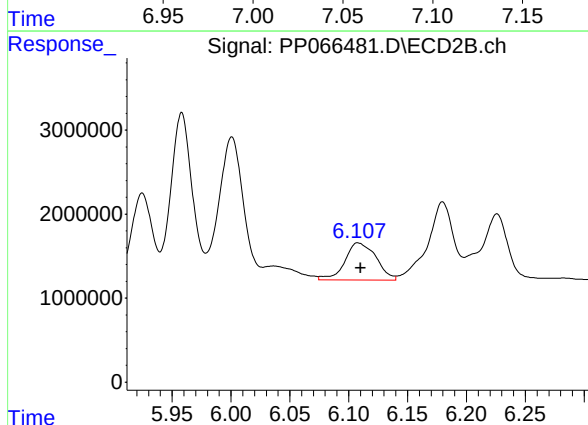


#27 AR-1254-2

R.T.: 6.108 min
Delta R.T.: -0.002 min
Response: 8220131
Conc: 98.98 ng/ml

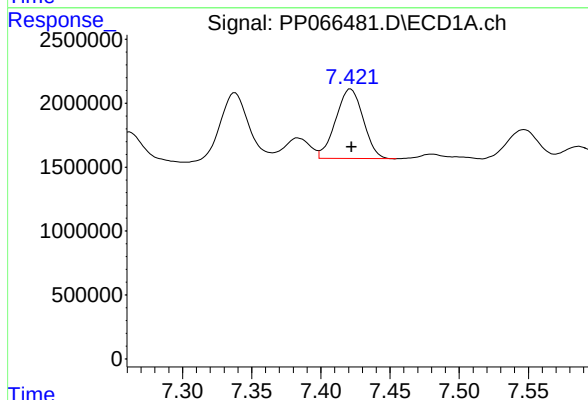


#28 AR-1254-3

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 7543479
Conc: 58.16 ng/ml

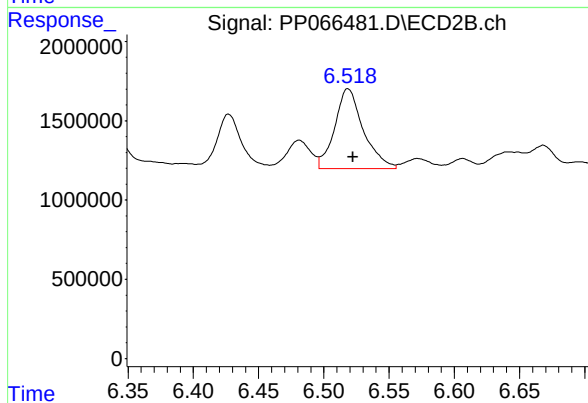

#28 AR-1254-3


R.T.: 6.519 min
Delta R.T.: -0.004 min
Response: 7699004
Conc: 61.62 ng/ml

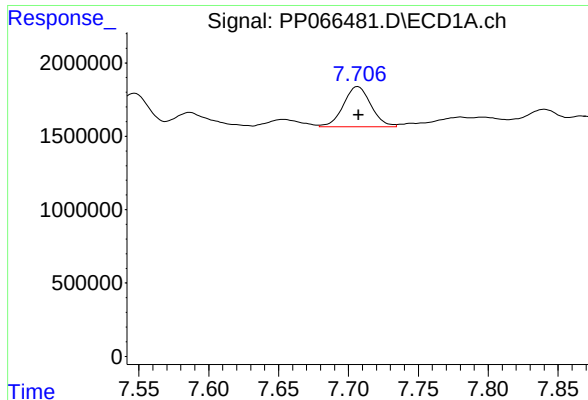

#29 AR-1254-4


R.T.: 7.707 min
Delta R.T.: 0.000 min
Response: 3764258
Conc: 41.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

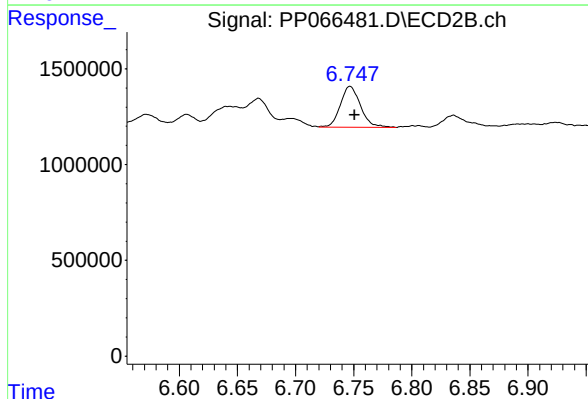


#29 AR-1254-4

R.T.: 6.747 min
Delta R.T.: -0.004 min
Response: 2585745
Conc: 37.79 ng/ml

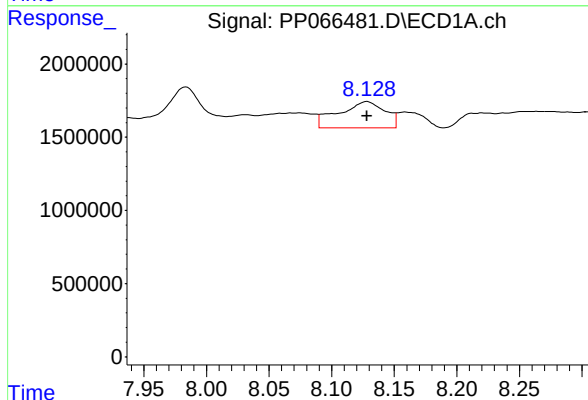


#30 AR-1254-5

R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 4628688
Conc: 46.57 ng/ml

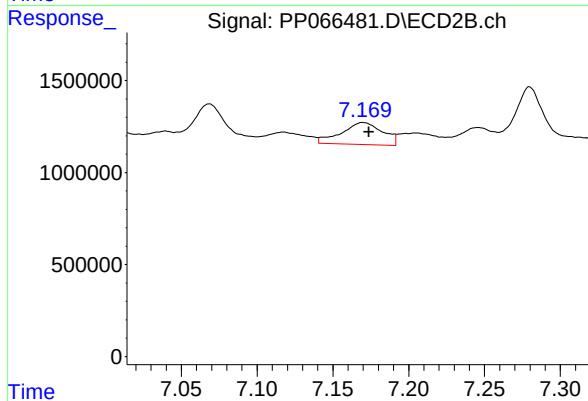

#30 AR-1254-5


R.T.: 7.170 min
Delta R.T.: -0.004 min
Response: 2244756
Conc: 22.36 ng/ml

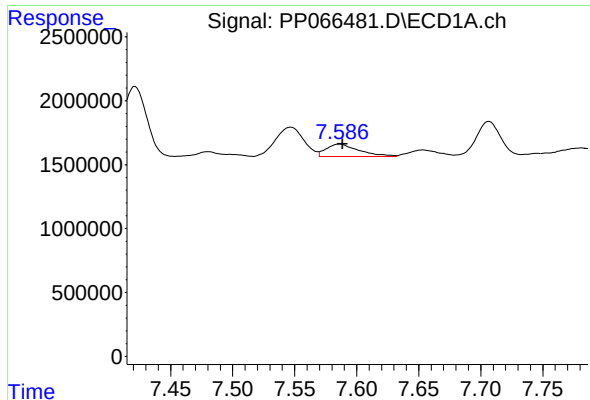

#31 AR-1260-1


R.T.: 7.586 min
Delta R.T.: -0.002 min
Response: 1751000
Conc: 16.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

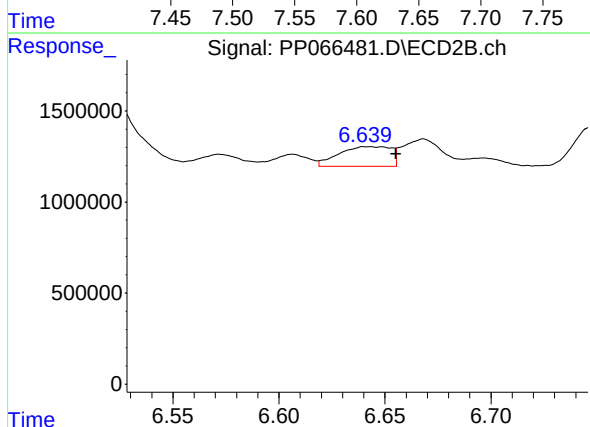


#31 AR-1260-1

R.T.: 6.648 min
Delta R.T.: -0.007 min
Response: 1845314
Conc: 21.59 ng/ml

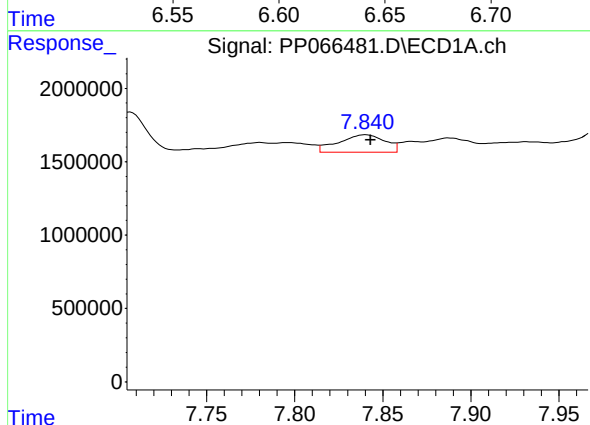


#32 AR-1260-2

R.T.: 7.840 min
Delta R.T.: -0.003 min
Response: 2190853
Conc: 19.02 ng/ml

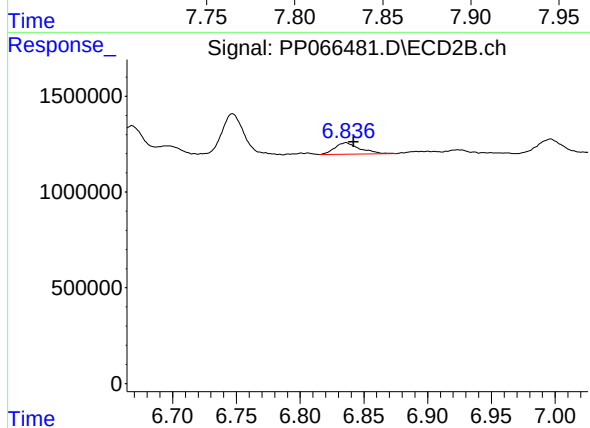

#32 AR-1260-2


R.T.: 6.836 min
Delta R.T.: -0.006 min
Response: 812878
Conc: 8.36 ng/ml

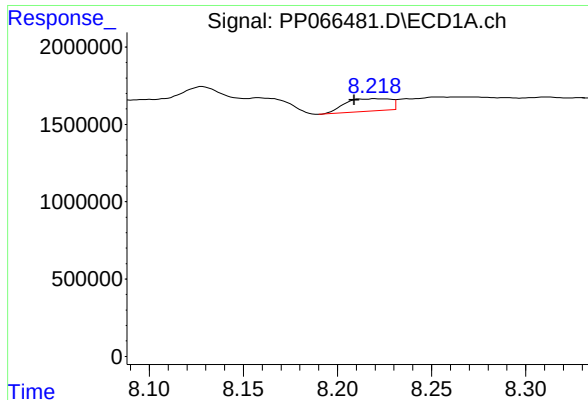

#33 AR-1260-3


R.T.: 8.220 min
Delta R.T.: 0.011 min
Response: 1346011
Conc: 16.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

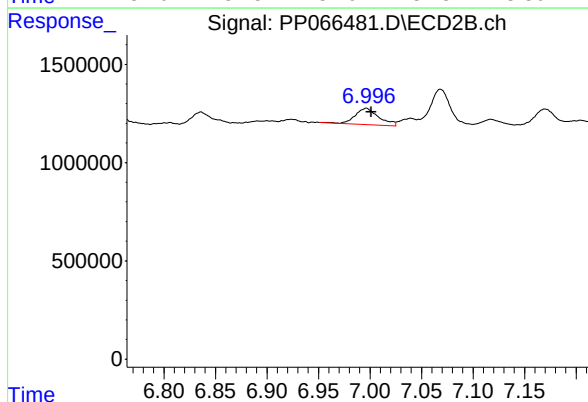


#33 AR-1260-3

R.T.: 6.996 min
Delta R.T.: -0.005 min
Response: 1307594
Conc: 14.25 ng/ml

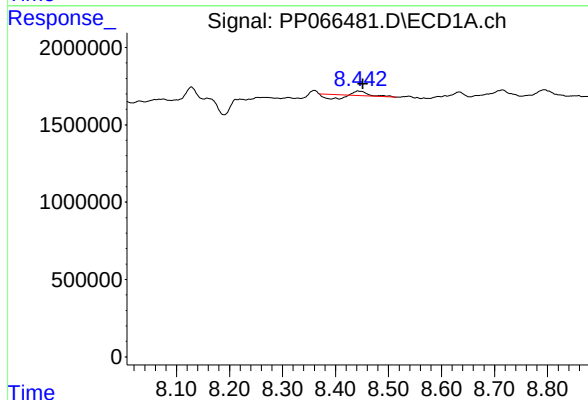


#34 AR-1260-4

R.T.: 8.443 min
Delta R.T.: -0.009 min
Response: 28542
Conc: 0.33 ng/ml

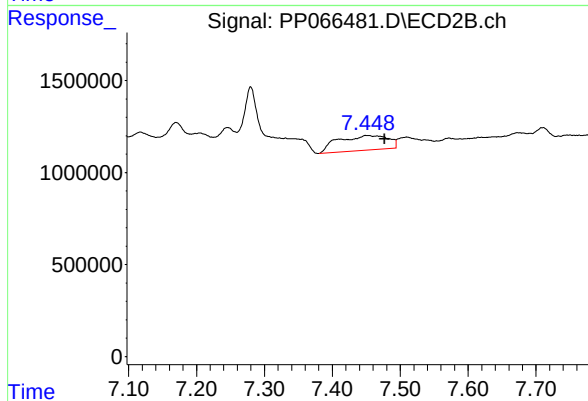

#34 AR-1260-4


R.T.: 7.450 min
Delta R.T.: -0.028 min
Response: 4113098
Conc: 63.29 ng/ml

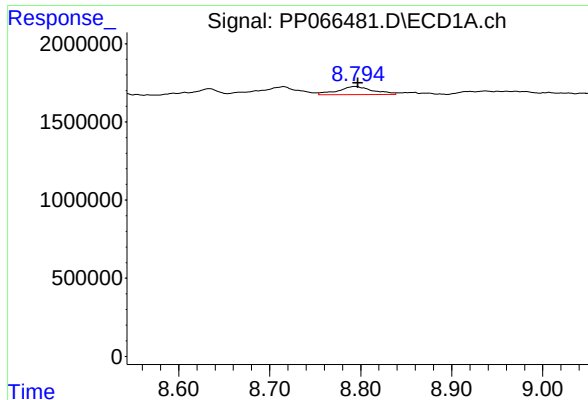

#35 AR-1260-5


R.T.: 8.794 min
Delta R.T.: -0.003 min
Response: 1397610
Conc: 9.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

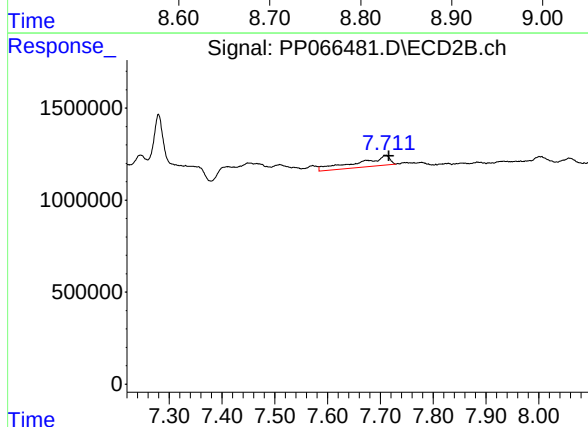


#35 AR-1260-5

R.T.: 7.710 min
Delta R.T.: -0.006 min
Response: 2351974
Conc: 16.73 ng/ml

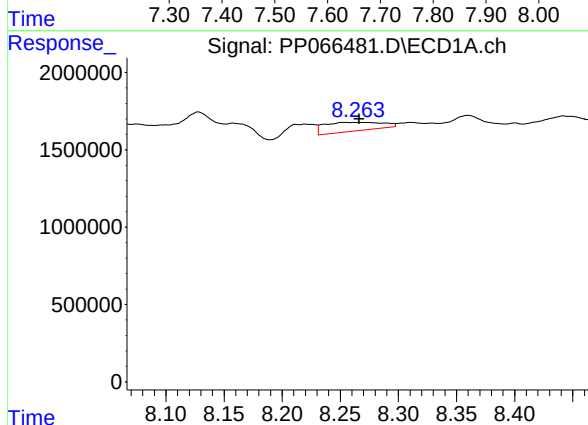


#36 AR-1262-1

R.T.: 8.264 min
Delta R.T.: -0.002 min
Response: 1949355
Conc: 34.58 ng/ml

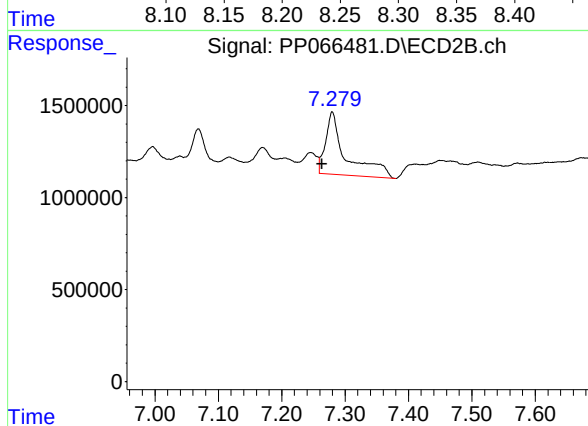

#36 AR-1262-1


R.T.: 7.280 min
Delta R.T.: 0.016 min
Response: 7652119
Conc: 160.80 ng/ml

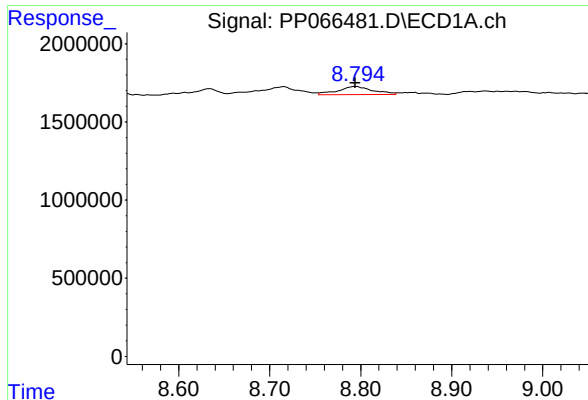

#37 AR-1262-2


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 1397610
Conc: 7.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

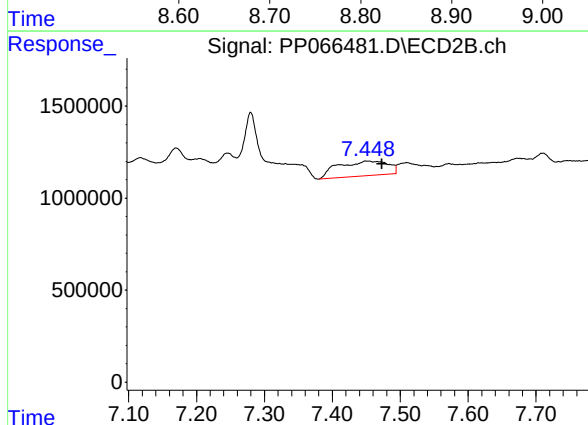


#37 AR-1262-2

R.T.: 7.450 min
Delta R.T.: -0.024 min
Response: 4113098
Conc: 43.97 ng/ml

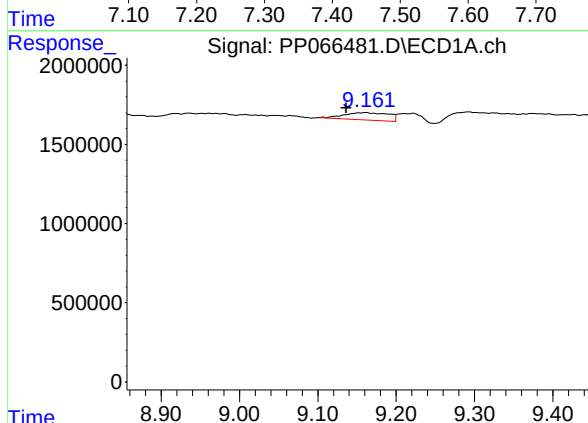


#38 AR-1262-3

R.T.: 9.161 min
Delta R.T.: 0.025 min
Response: 1862496
Conc: 14.27 ng/ml

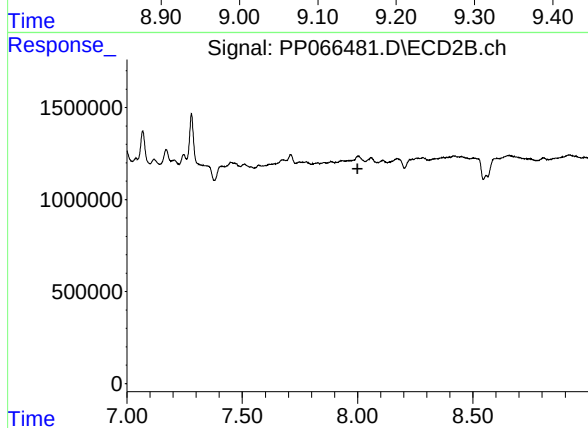

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 7.999 min
Response: 0
Conc: N.D.

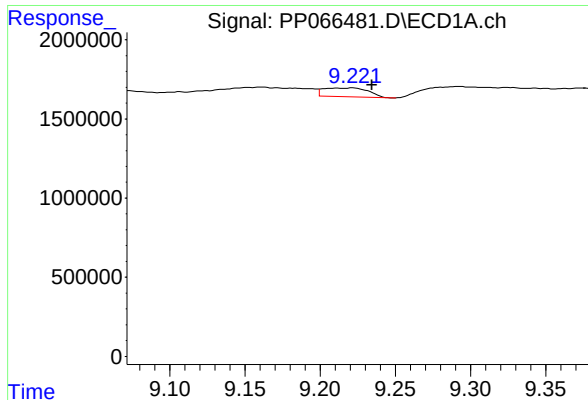

#39 AR-1262-4


R.T.: 9.221 min
Delta R.T.: -0.013 min
Response: 1135350
Conc: 10.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

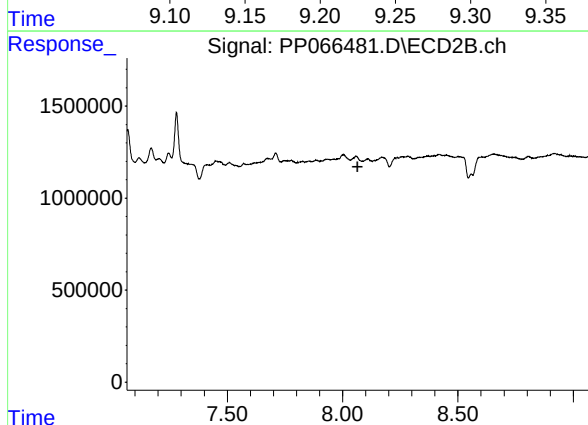


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.065 min
Response: 0
Conc: N.D.

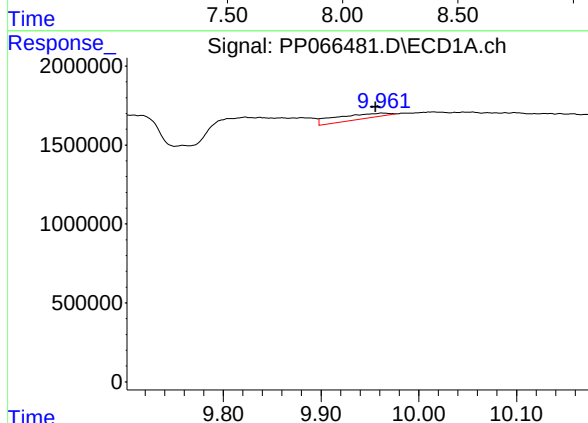


#40 AR-1262-5

R.T.: 9.963 min
Delta R.T.: 0.007 min
Response: 1242731
Conc: 19.09 ng/ml

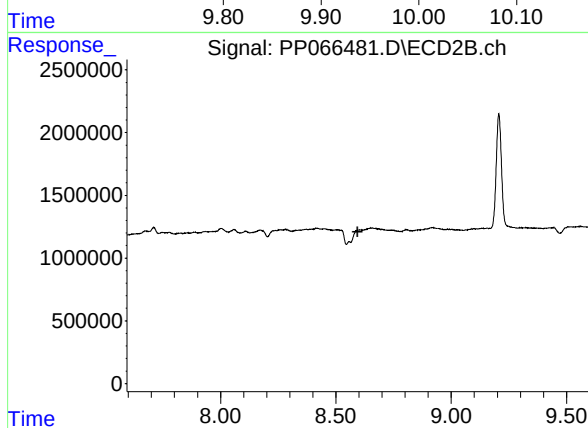

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.594 min
Response: 0
Conc: N.D.

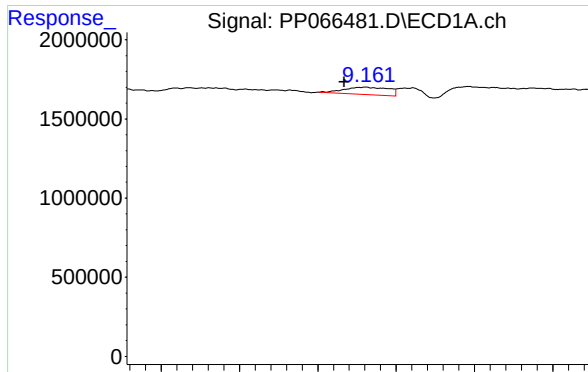

#41 AR-1268-1


R.T.: 9.161 min
Delta R.T.: 0.027 min
Response: 1862496
Conc: 7.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

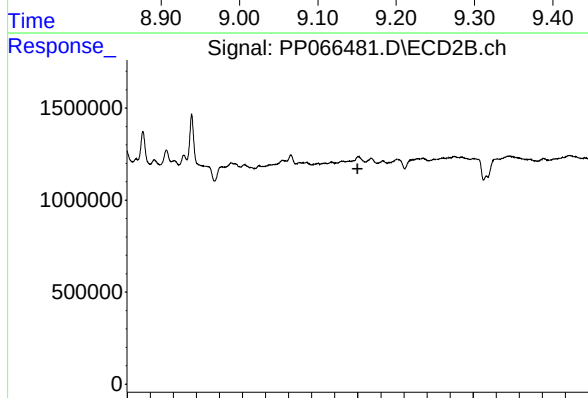


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.999 min
Response: 0
Conc: N.D.

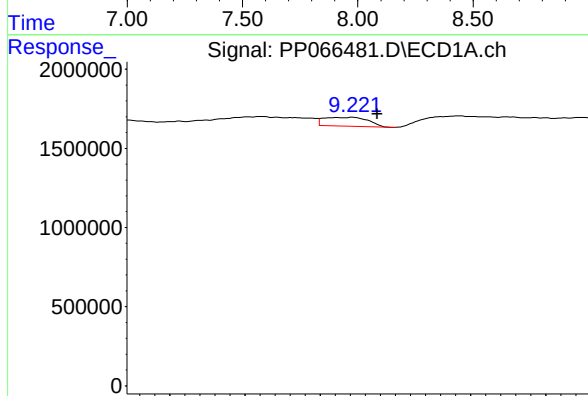


#42 AR-1268-2

R.T.: 9.221 min
Delta R.T.: -0.017 min
Response: 1135350
Conc: 5.32 ng/ml

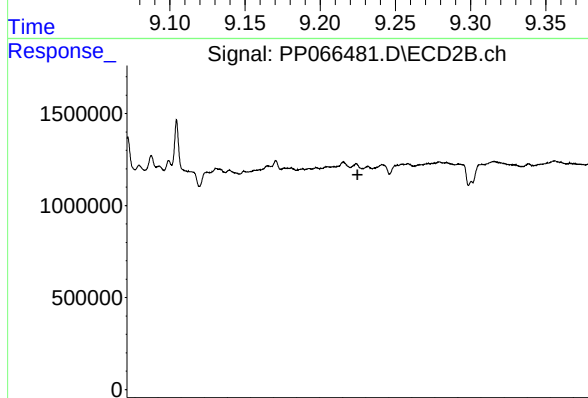

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.065 min
Response: 0
Conc: N.D.

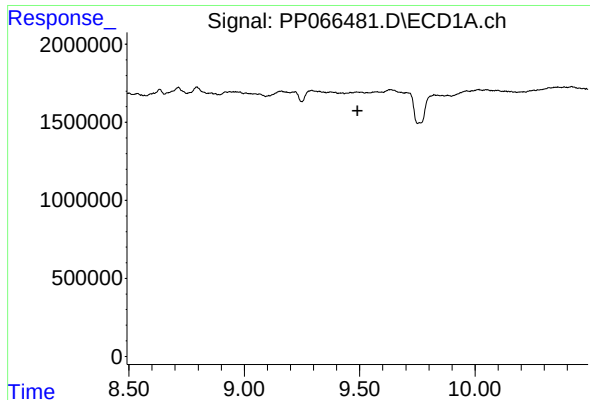

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CONRAIL-01-VALVEDL

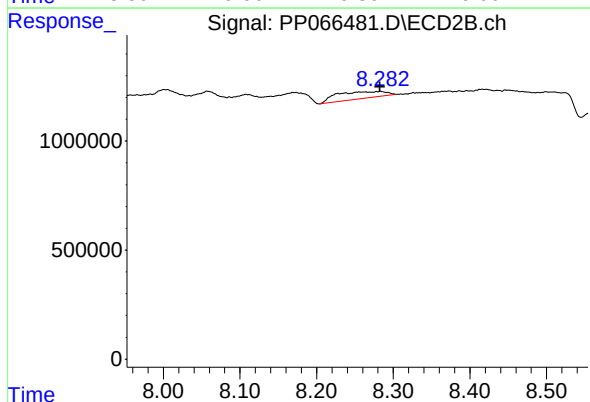


#43 AR-1268-3

R.T.: 8.284 min
Delta R.T.: 0.000 min
Response: 1432733
Conc: 8.86 ng/ml

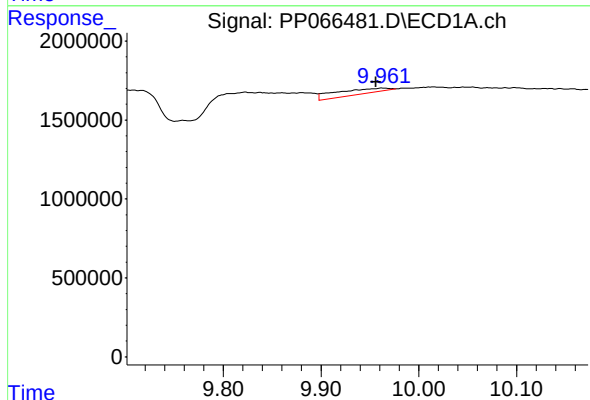

#44 AR-1268-4

R.T.: 9.963 min
Delta R.T.: 0.007 min
Response: 1242731
Conc: 17.82 ng/ml

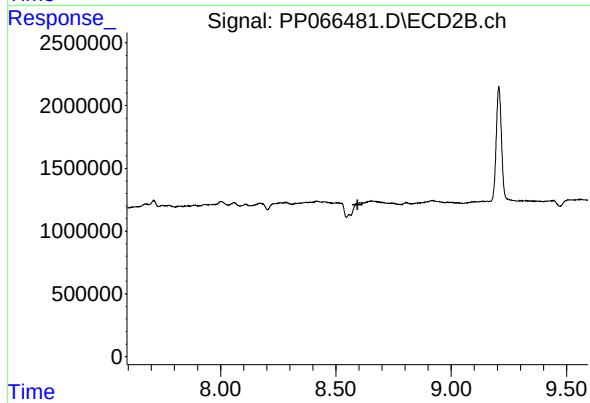

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 8.594 min
Response: 0
Conc: N.D.