

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072324\
 Data File : PP066477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 11:50
 Operator : YP\AJ
 Sample : PB162225BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB162225BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/24/2024
 Supervised By :Ankita Jodhani 07/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 01:48:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 07:20:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.791	4.028	42702632	44329228	24.238	23.214
2) SA Decachlor...	10.791	9.204	41235198	28629628	23.493m	22.437m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072324\
Data File : PP066477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 11:50
Operator : YP\AJ
Sample : PB162225BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB162225BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2024
Supervised By :Ankita Jodhani 07/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 01:48:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071624.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 07:20:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

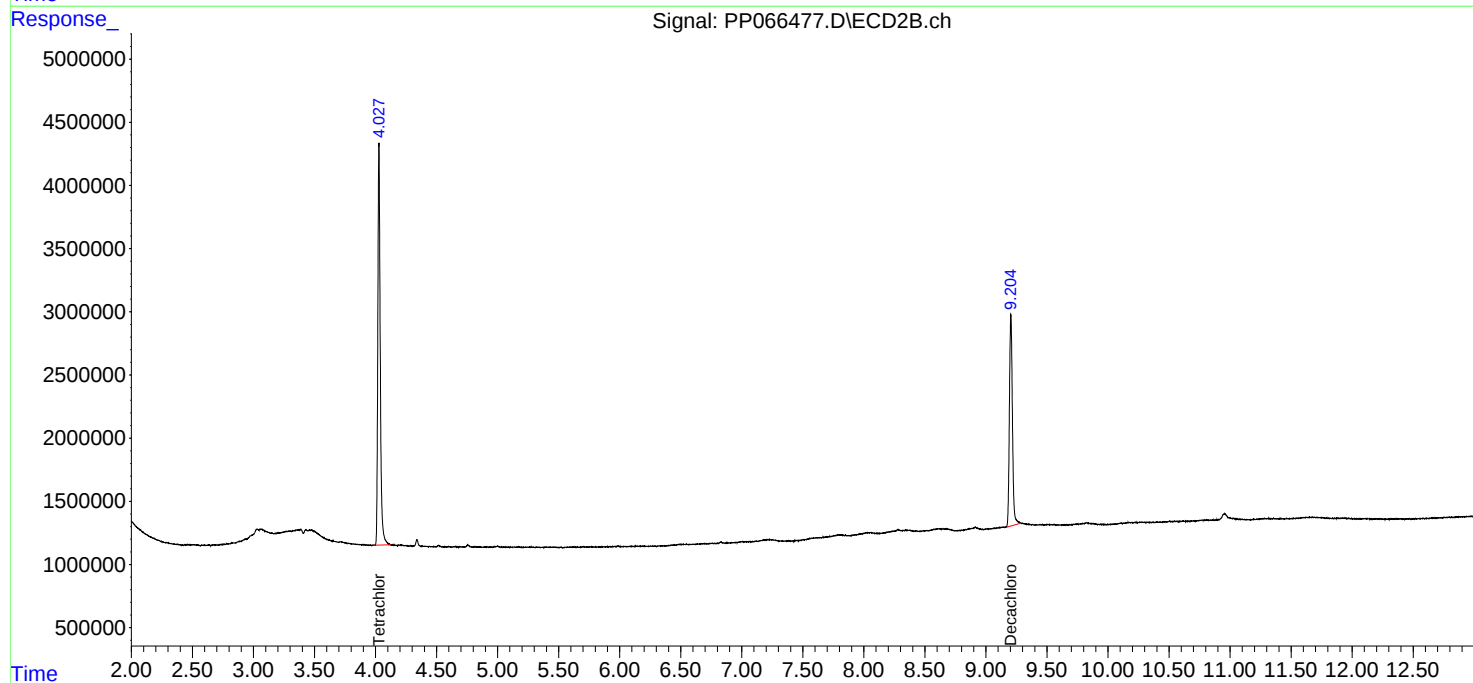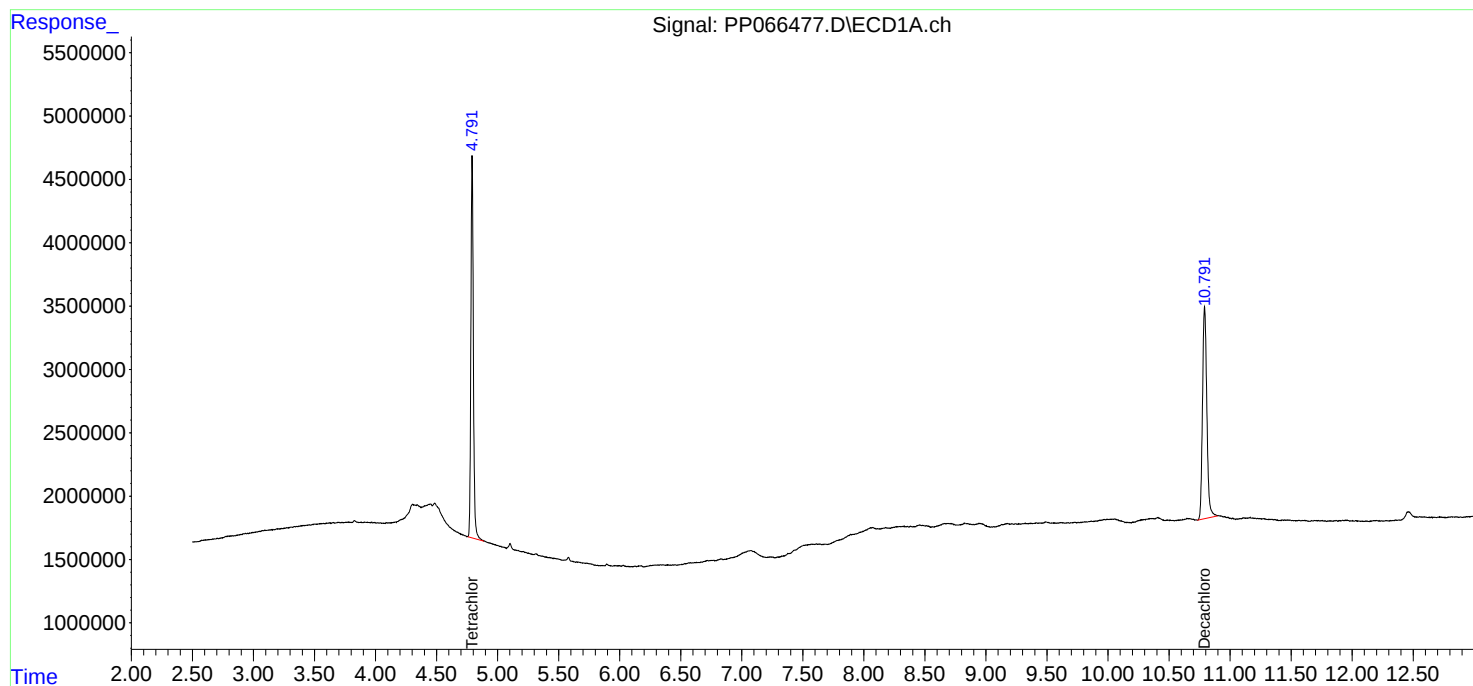

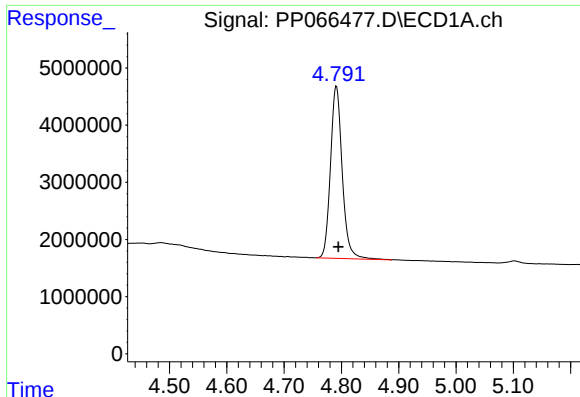


#1 Tetrachloro-m-xylene

R.T.: 4.791 min
Delta R.T.: -0.004 min
Response: 42702632
Conc: 24.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB162225BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2024
Supervised By :Ankita Jodhani 07/24/2024

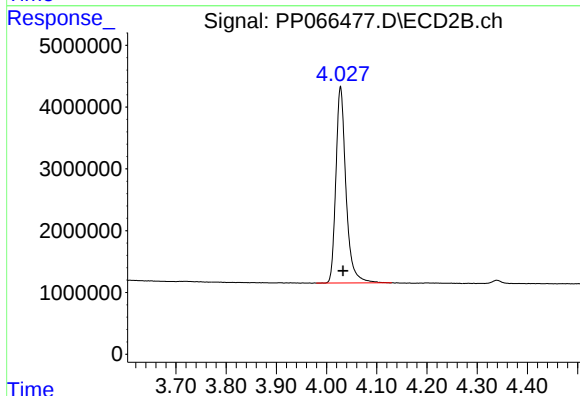


#1 Tetrachloro-m-xylene

R.T.: 4.028 min
Delta R.T.: -0.005 min
Response: 44329228
Conc: 23.21 ng/ml

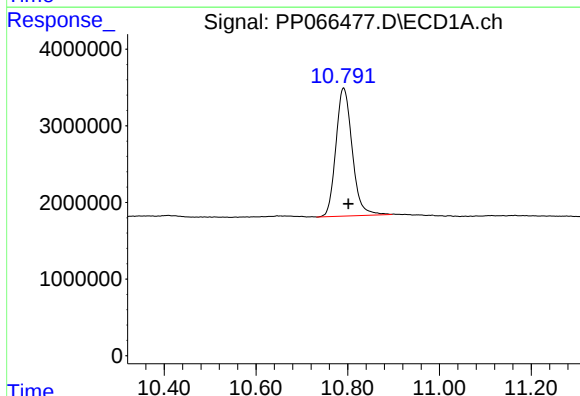

#2 Decachlorobiphenyl

R.T.: 10.791 min
Delta R.T.: -0.011 min
Response: 41235198
Conc: 23.49 ng/ml m

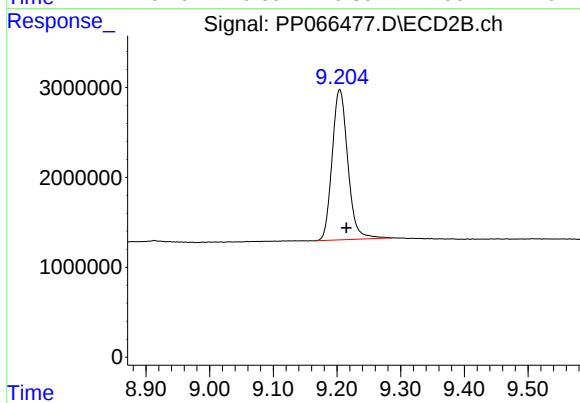

#2 Decachlorobiphenyl

R.T.: 9.204 min
Delta R.T.: -0.011 min
Response: 28629628
Conc: 22.44 ng/ml m