

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072423\
 Data File : PP058910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2023 17:26
 Operator : YP\AJ
 Sample : 03724-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 185465

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 21:47:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 22 02:26:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

07/25/2023
 Supervised By :Ankita
 Jodhani

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	07/25/2023
----------	------	------	--------	--------	-------	-------	------------

System Monitoring Compounds

1) SA Tetrachlo...	4.427	3.666	27552091	39795820	20.013	20.694	
2) SA Decachlor...	10.225	8.711	16889300	26359297	19.605	18.629m	

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072423\
Data File : PP058910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2023 17:26
Operator : YP\AJ
Sample : 03724-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
185465



Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 21:47:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 22 02:26:24 2023
Response via : Initial Calibration
Integrator: ChemStation

07/25/2023
Supervised By :Ankita
Jodhani

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

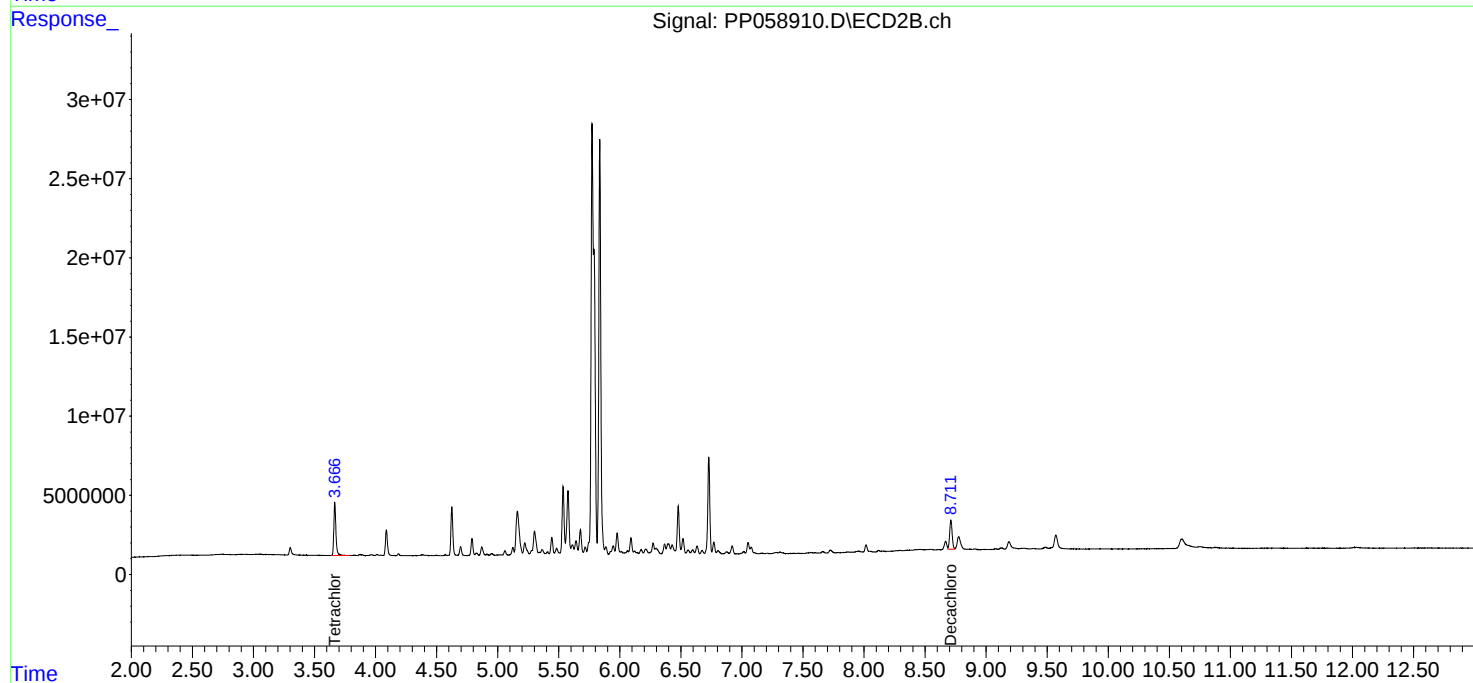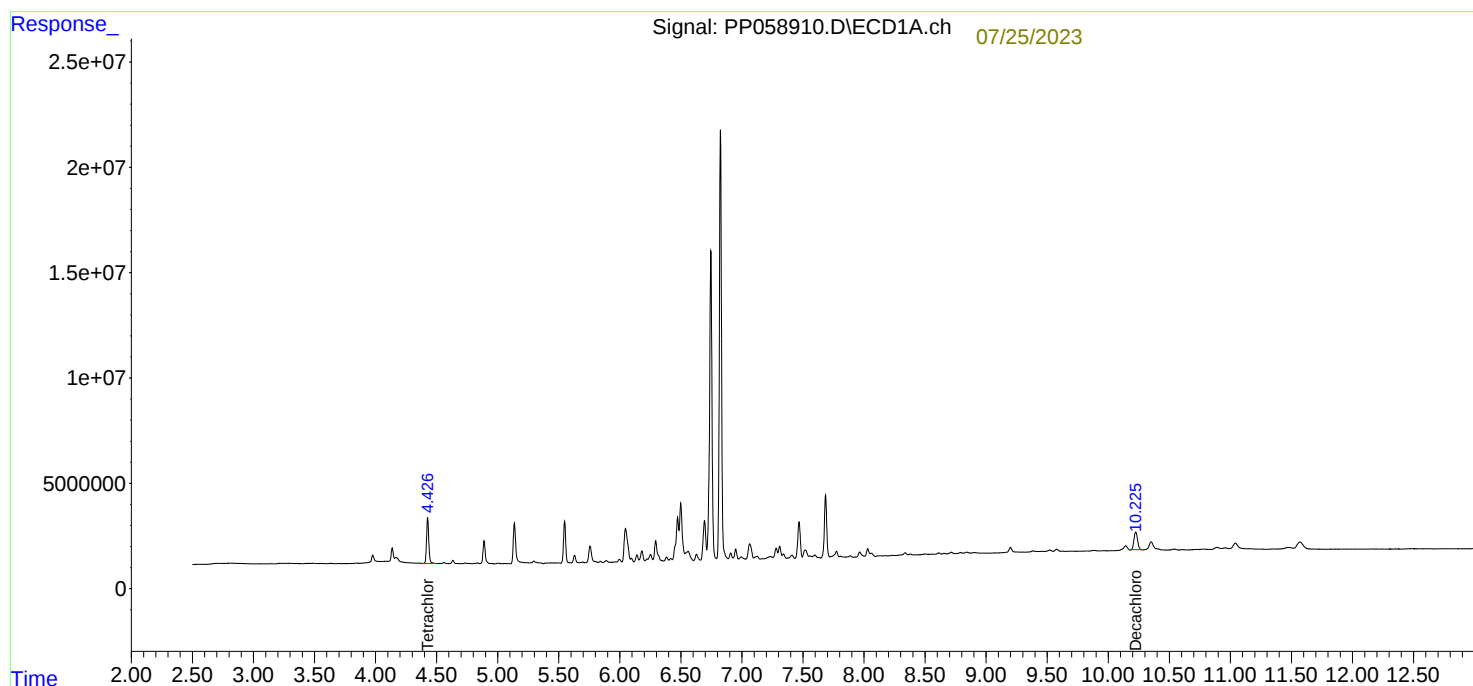

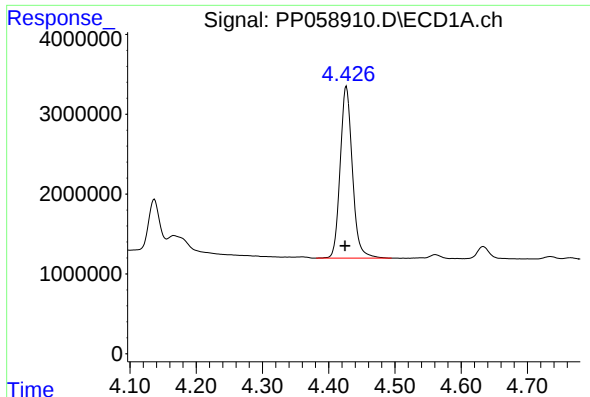


#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: 0.002 min
Response: 27552091
Conc: 20.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
185465

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

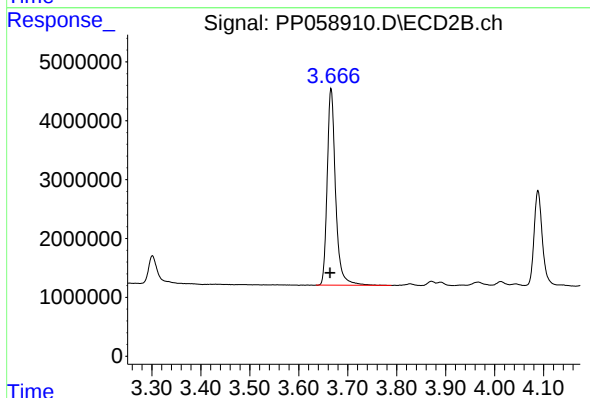


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.002 min
Response: 39795820
Conc: 20.69 ng/ml


07/25/2023
Supervised By :Ankita
Jodhani

07/25/2023

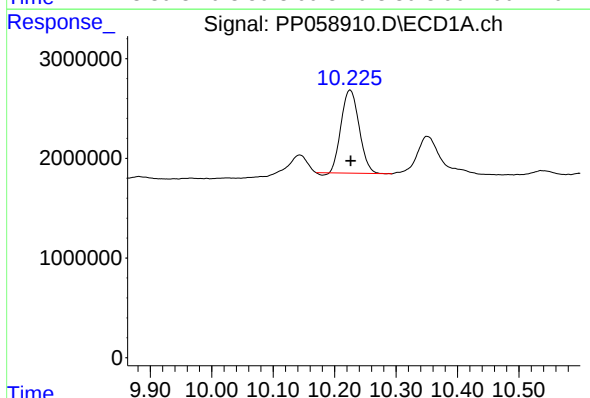

#2 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: 0.000 min
Response: 16889300
Conc: 19.60 ng/ml

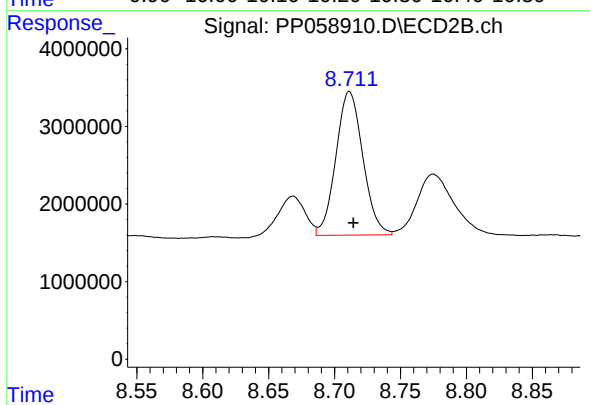

#2 Decachlorobiphenyl

R.T.: 8.711 min
Delta R.T.: -0.004 min
Response: 26359297
Conc: 18.63 ng/ml m