

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072423\
 Data File : PP058921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2023 21:03
 Operator : YP\AJ
 Sample : 03718-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DRIP-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2023
 Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 21:59:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 22 02:26:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.427	3.688	26366267	36794371	19.152	19.133
2) SA Decachlor...	10.221	8.730	12232982	17160301	14.200	12.128
Target Compounds						
21) L5 AR-1248-1	5.601	4.780f	7703517	8422020	278.393	233.800m
22) L5 AR-1248-2	5.878	5.019f	4904215	5892738	114.075	103.981
23) L5 AR-1248-3	6.082	5.061f	6001815	7479285	128.079	130.587
24) L5 AR-1248-4	6.488	5.233f	7977471	8340809	168.698	122.716 #
25) L5 AR-1248-5	6.526	5.587f	7955866	12641749	173.591	207.452

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072423\
Data File : PP058921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2023 21:03
Operator : YP\AJ
Sample : 03718-06
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
DRIP-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 21:59:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 22 02:26:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

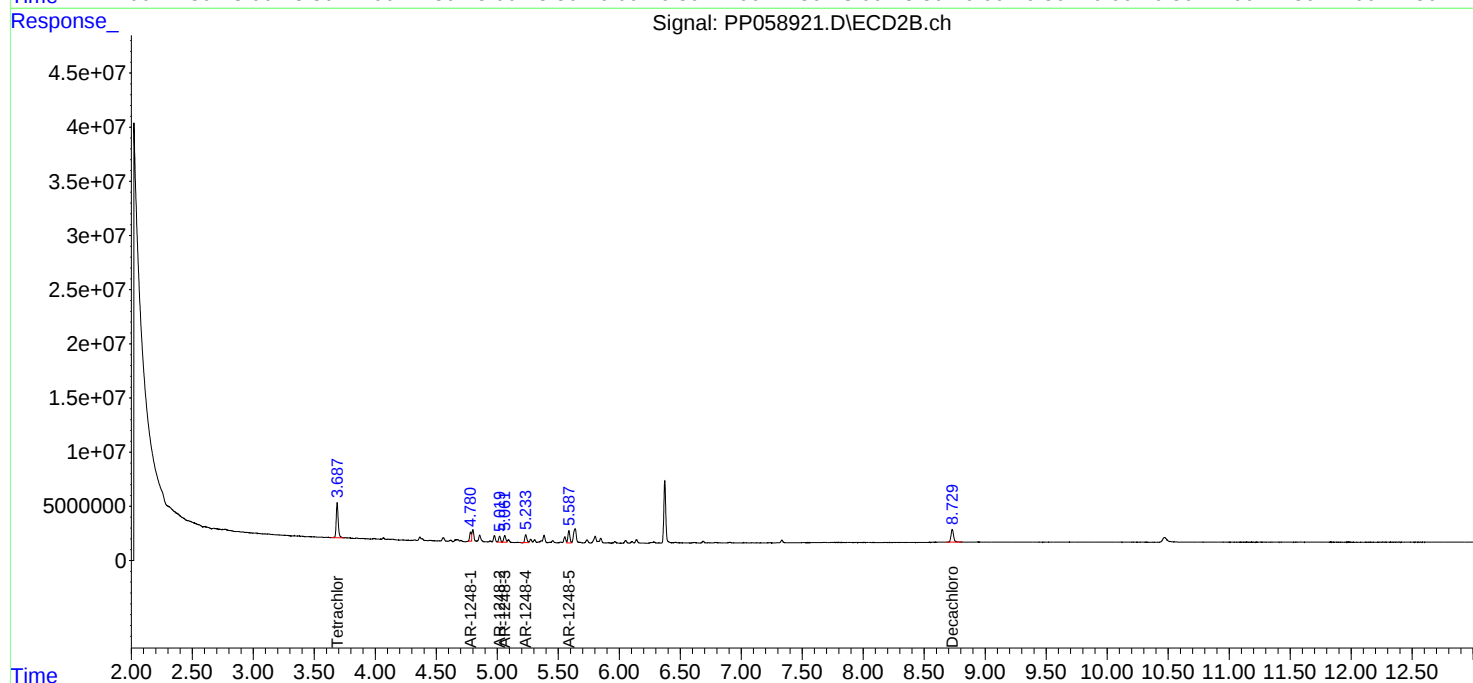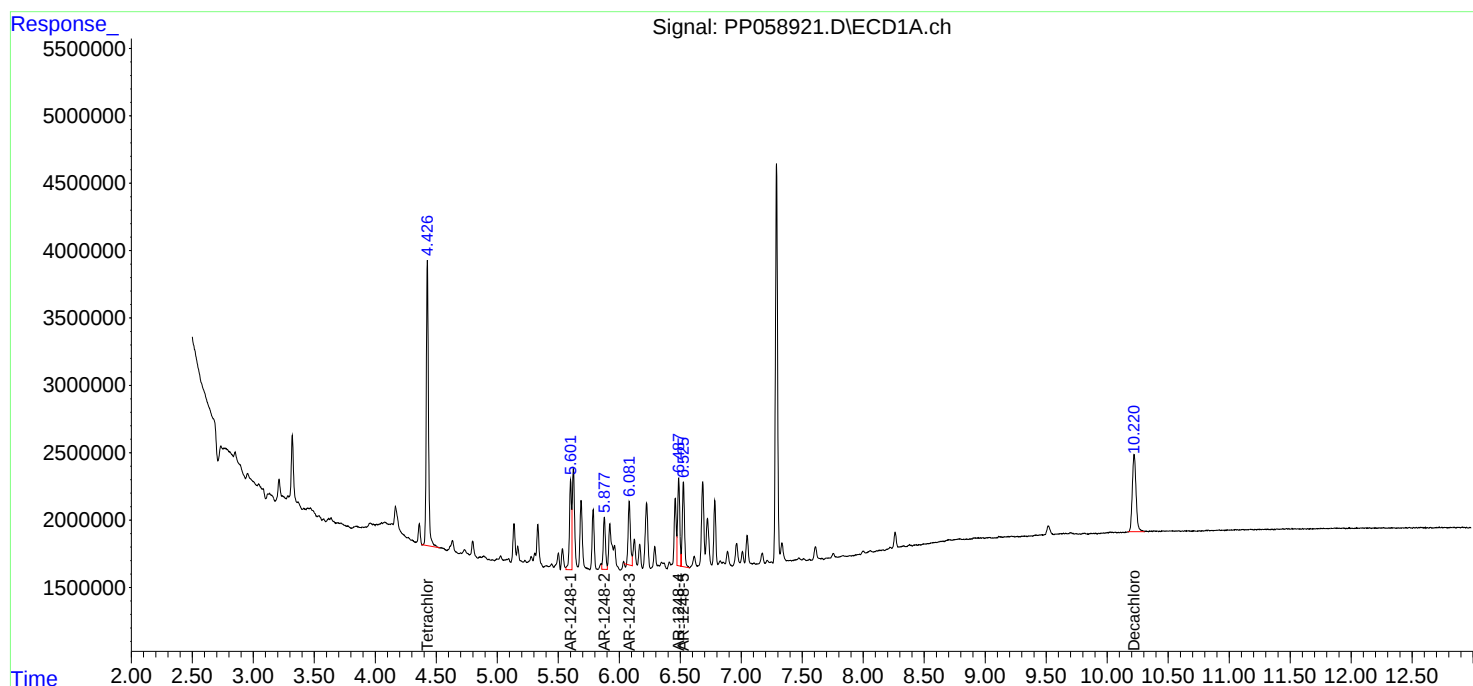

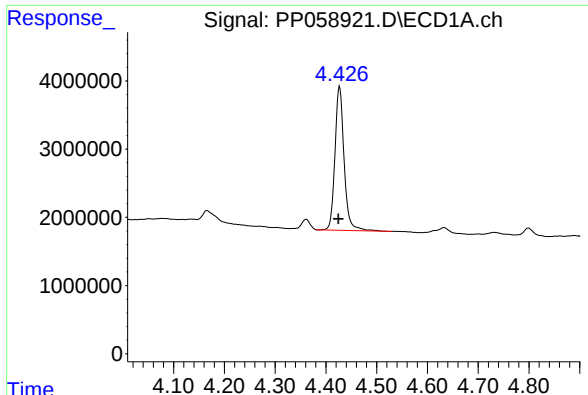


#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: 0.002 min
Response: 26366267
Conc: 19.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
DRIP-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

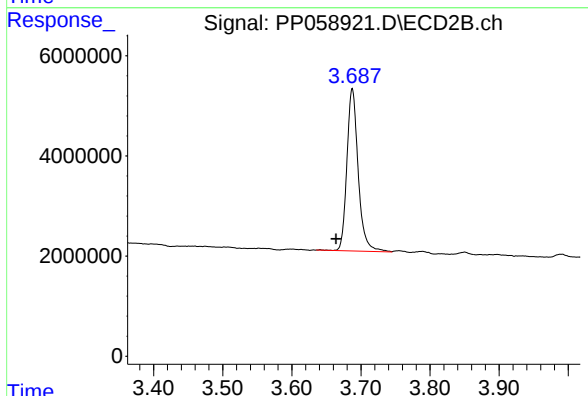


#1 Tetrachloro-m-xylene

R.T.: 3.688 min
Delta R.T.: 0.024 min
Response: 36794371
Conc: 19.13 ng/ml

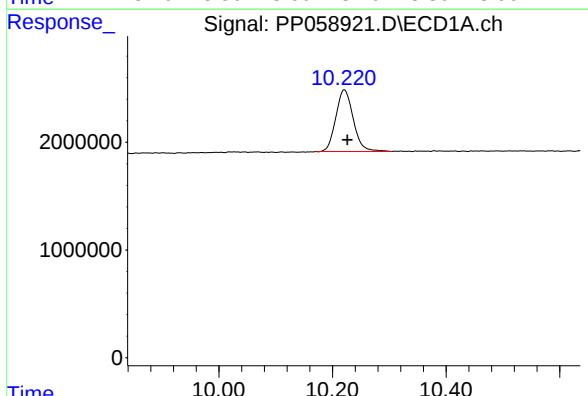


#2 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.005 min
Response: 12232982
Conc: 14.20 ng/ml

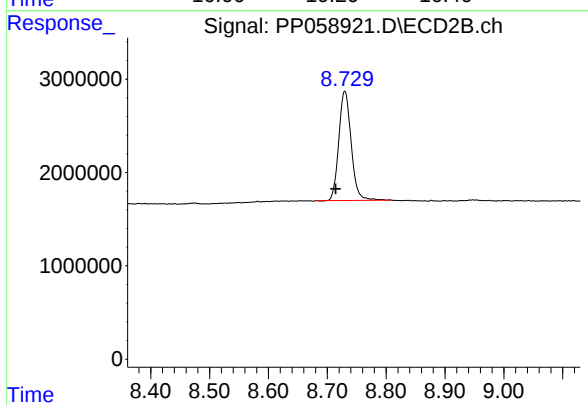

#2 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: 0.016 min
Response: 17160301
Conc: 12.13 ng/ml

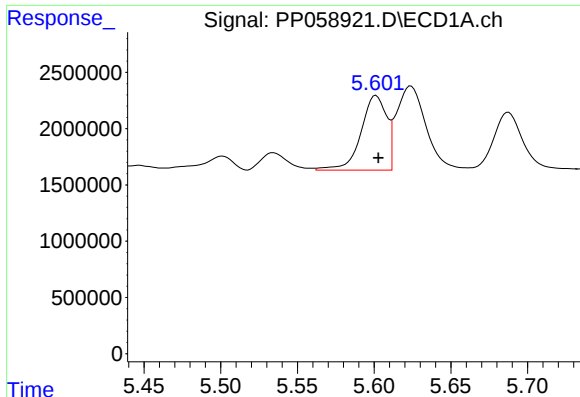


#21 AR-1248-1

R.T.: 5.601 min
Delta R.T.: -0.001 min
Response: 7703517
Conc: 278.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
DRIP-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

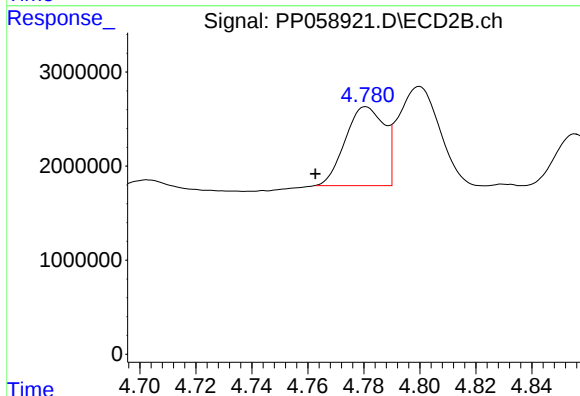


#21 AR-1248-1

R.T.: 4.780 min
Delta R.T.: 0.018 min
Response: 8422020
Conc: 233.80 ng/ml m

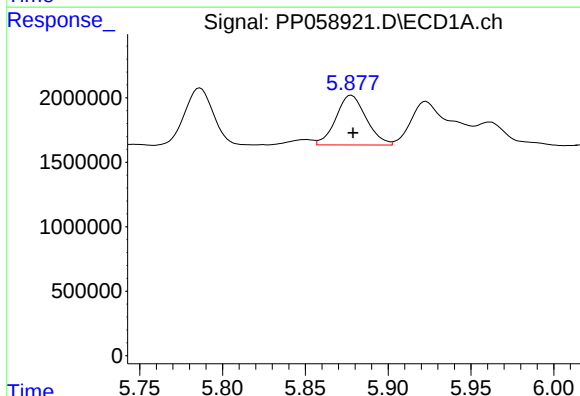


#22 AR-1248-2

R.T.: 5.878 min
Delta R.T.: -0.001 min
Response: 4904215
Conc: 114.08 ng/ml

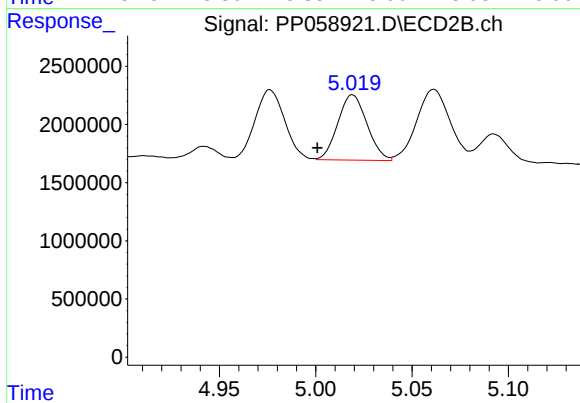

#22 AR-1248-2

R.T.: 5.019 min
Delta R.T.: 0.018 min
Response: 5892738
Conc: 103.98 ng/ml

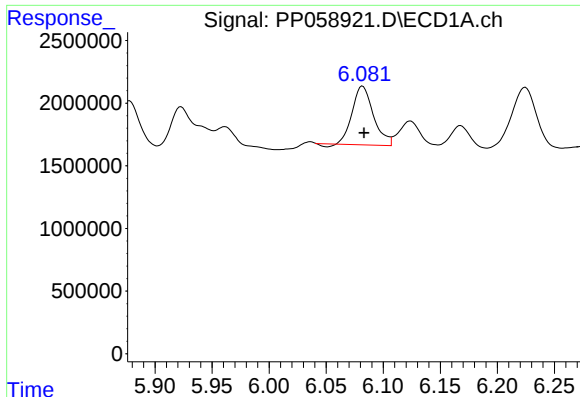


#23 AR-1248-3

R.T.: 6.082 min
Delta R.T.: -0.001 min
Response: 6001815
Conc: 128.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
DRIP-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

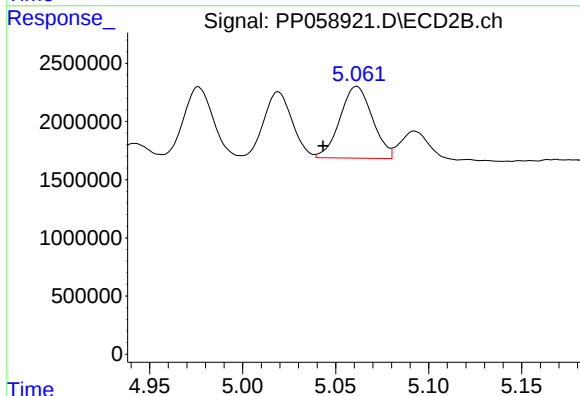


#23 AR-1248-3

R.T.: 5.061 min
Delta R.T.: 0.018 min
Response: 7479285
Conc: 130.59 ng/ml

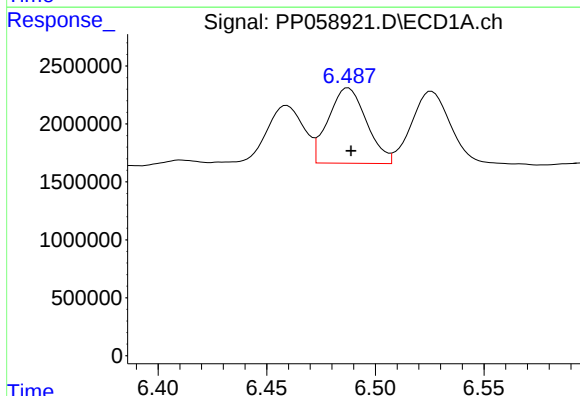


#24 AR-1248-4

R.T.: 6.488 min
Delta R.T.: -0.001 min
Response: 7977471
Conc: 168.70 ng/ml

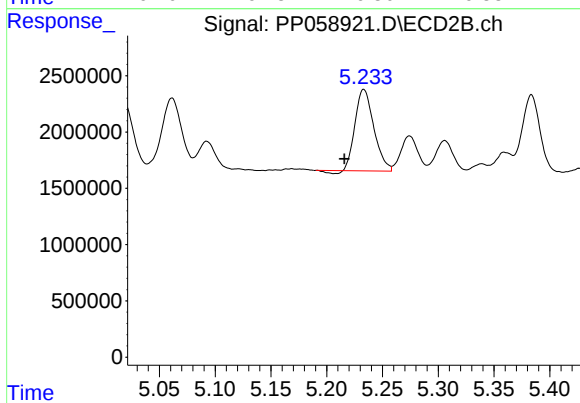

#24 AR-1248-4

R.T.: 5.233 min
Delta R.T.: 0.018 min
Response: 8340809
Conc: 122.72 ng/ml

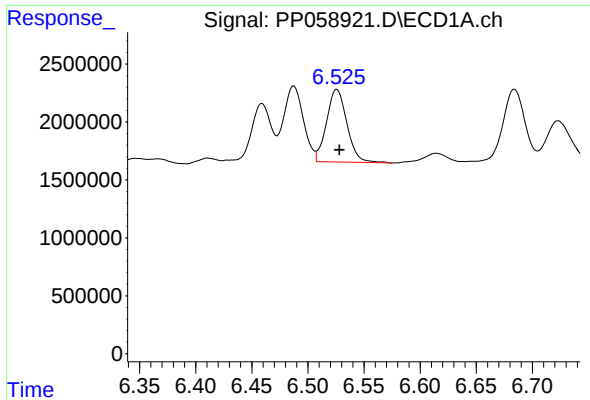


#25 AR-1248-5

R.T.: 6.526 min
Delta R.T.: -0.002 min
Response: 7955866
Conc: 173.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
DRIP-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

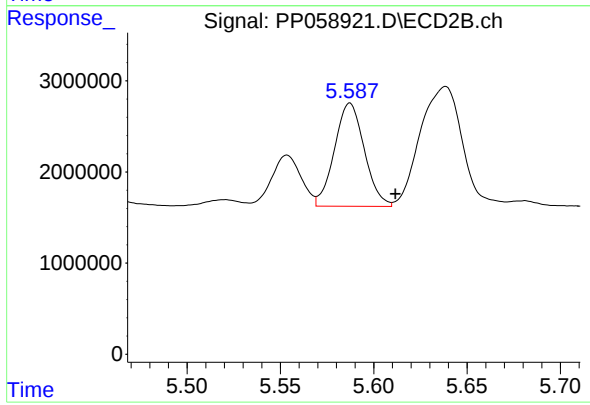

#25 AR-1248-5

R.T.: 5.587 min
Delta R.T.: -0.024 min
Response: 12641749
Conc: 207.45 ng/ml