

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072522\
 Data File : PP049780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 15:34
 Operator : YP\AJ
 Sample : N3859-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S5-03-S3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/26/2022
 Supervised By :Ankita Jodhani 07/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 03:32:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.353	3.601	33098835	58192260	22.809	23.807
2) SA Decachlor...	10.107	8.569	33322736	26411186	23.559	22.678
Target Compounds						
26) L6 AR-1254-1	6.385	5.470	788120	2573469	12.514m	20.291 #
27) L6 AR-1254-2	6.604	5.616	4419232	6028760	45.362	54.544
28) L6 AR-1254-3	6.977	6.019	5237808	9770492	50.693	60.025
29) L6 AR-1254-4	7.264	6.246	6848783	7978736	85.552	82.462
30) L6 AR-1254-5	7.683	6.662	15414526	25956265	173.427m	195.873

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072522\
Data File : PP049780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 15:34
Operator : YP\AJ
Sample : N3859-06
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
S5-03-S3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 03:32:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

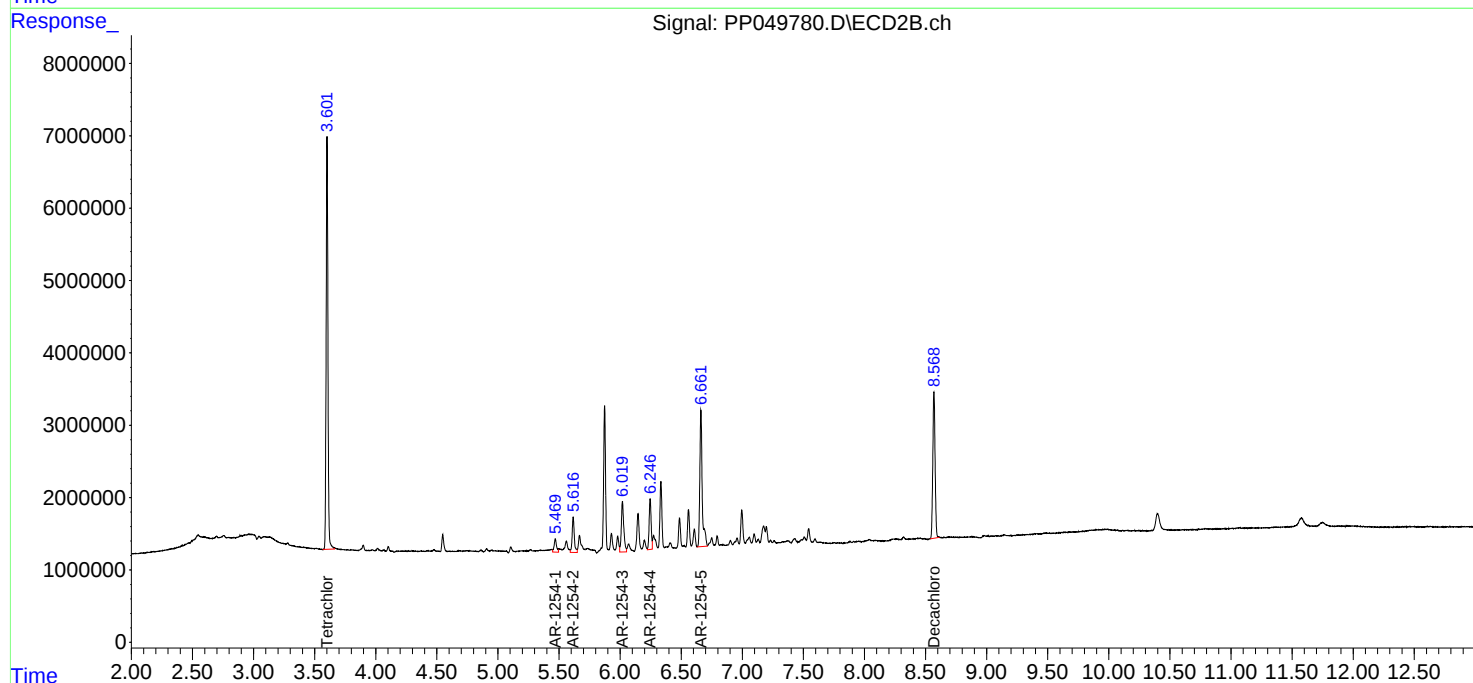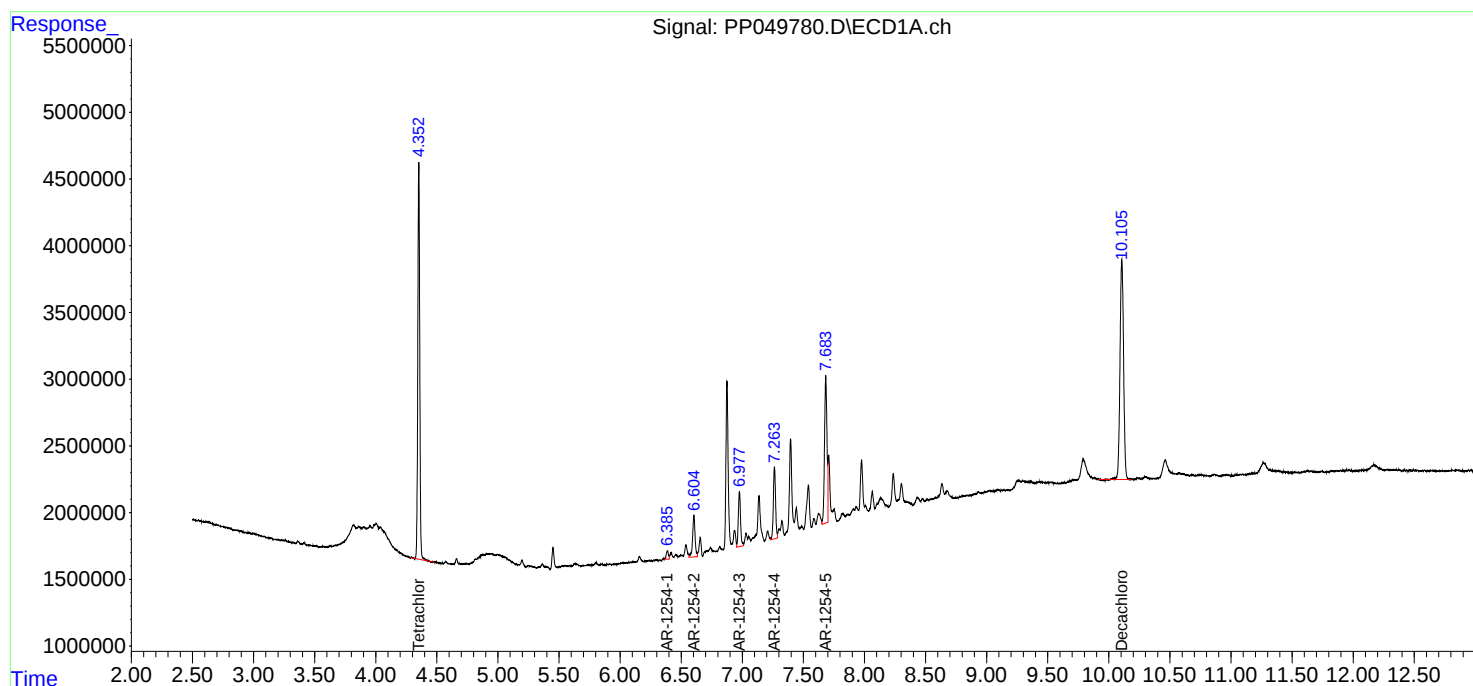

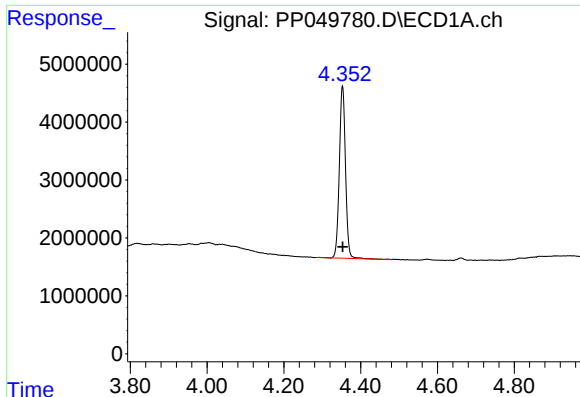


#1 Tetrachloro-m-xylene

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 33098835
Conc: 22.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
S5-03-S3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

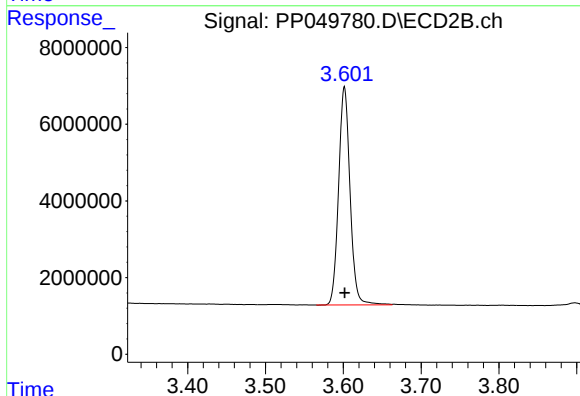


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 58192260
Conc: 23.81 ng/ml

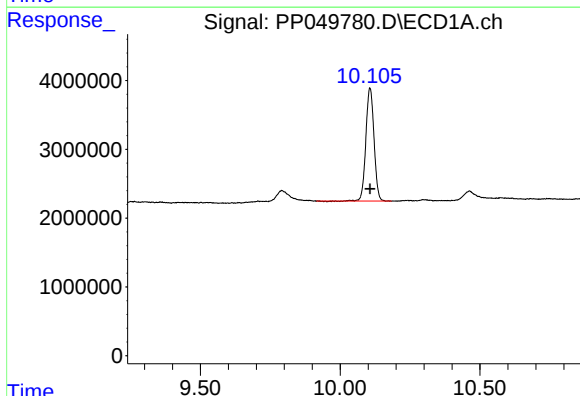


#2 Decachlorobiphenyl

R.T.: 10.107 min
Delta R.T.: 0.000 min
Response: 33322736
Conc: 23.56 ng/ml

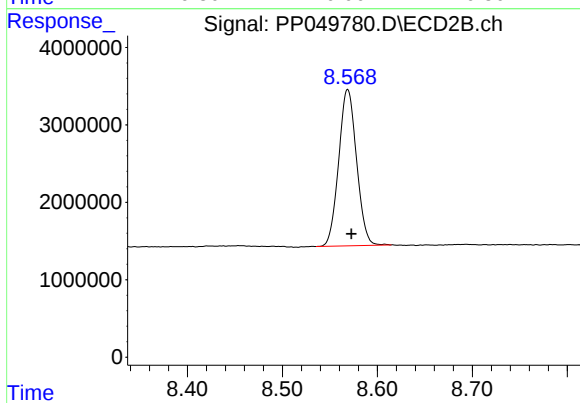

#2 Decachlorobiphenyl

R.T.: 8.569 min
Delta R.T.: -0.004 min
Response: 26411186
Conc: 22.68 ng/ml

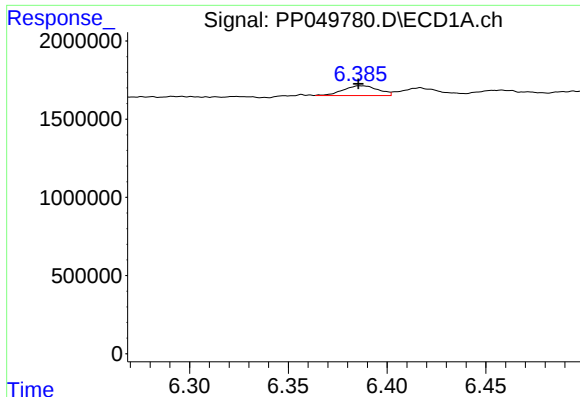


#26 AR-1254-1

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 788120
Conc: 12.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
S5-03-S3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

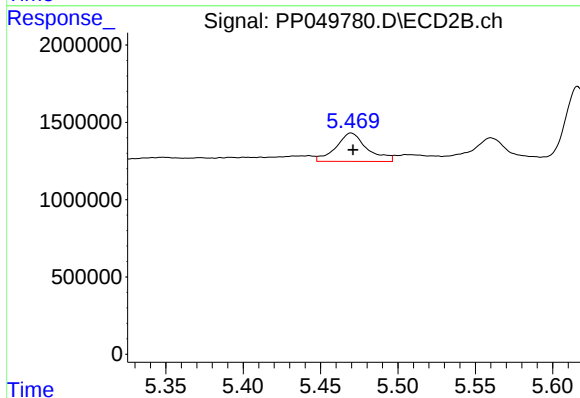


#26 AR-1254-1

R.T.: 5.470 min
Delta R.T.: -0.001 min
Response: 2573469
Conc: 20.29 ng/ml

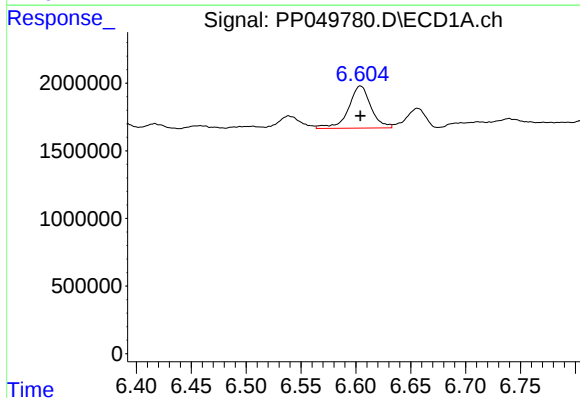


#27 AR-1254-2

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 4419232
Conc: 45.36 ng/ml

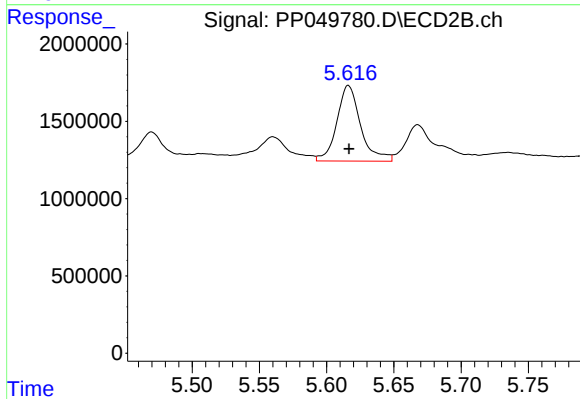

#27 AR-1254-2

R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 6028760
Conc: 54.54 ng/ml

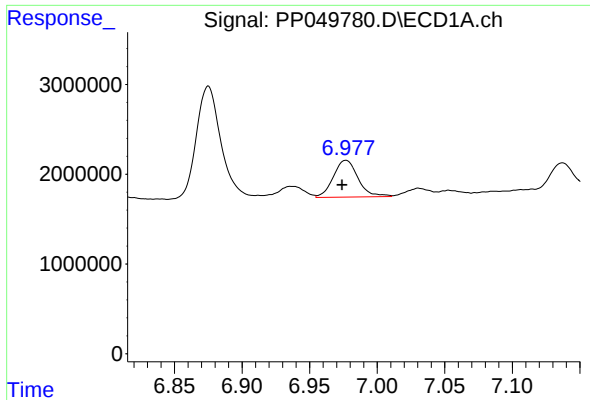


#28 AR-1254-3

R.T.: 6.977 min
Delta R.T.: 0.003 min
Response: 5237808
Conc: 50.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
S5-03-S3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

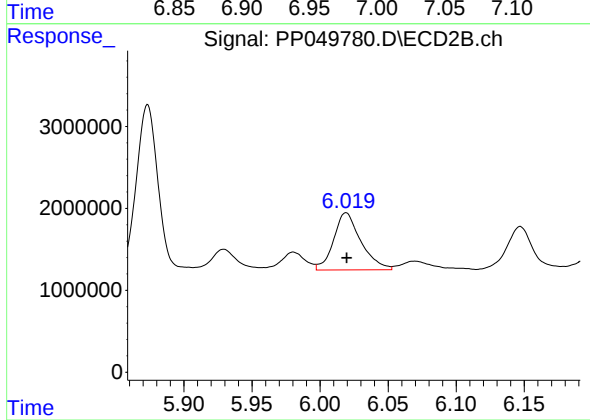


#28 AR-1254-3

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 9770492
Conc: 60.02 ng/ml

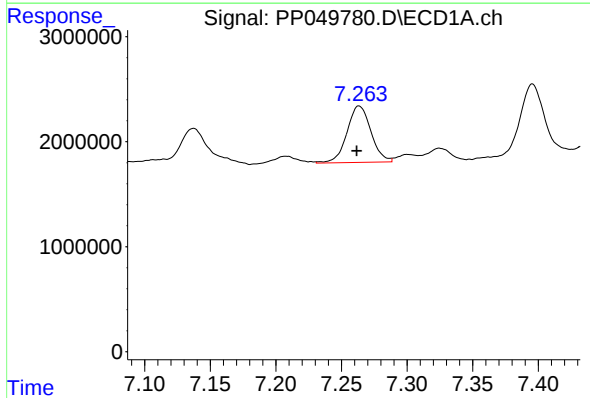


#29 AR-1254-4

R.T.: 7.264 min
Delta R.T.: 0.002 min
Response: 6848783
Conc: 85.55 ng/ml

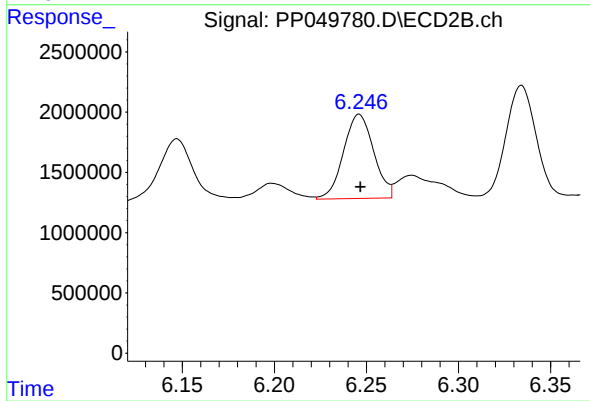

#29 AR-1254-4

R.T.: 6.246 min
Delta R.T.: 0.000 min
Response: 7978736
Conc: 82.46 ng/ml

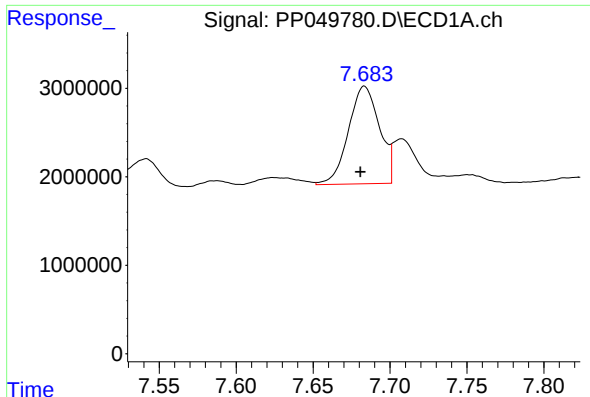


#30 AR-1254-5

R.T.: 7.683 min
Delta R.T.: 0.002 min
Response: 15414526
Conc: 173.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
S5-03-S3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

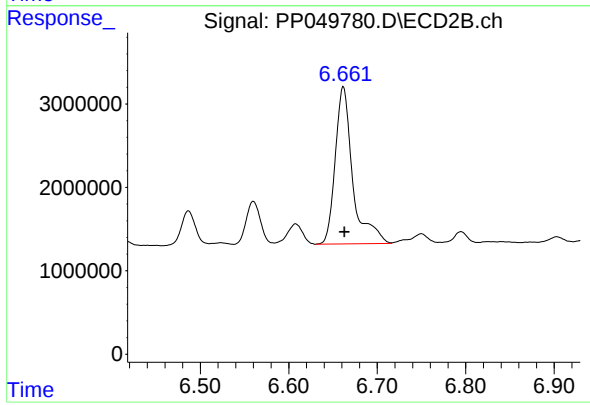

#30 AR-1254-5

R.T.: 6.662 min
Delta R.T.: -0.001 min
Response: 25956265
Conc: 195.87 ng/ml