

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072522\
 Data File : PP049786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 17:14
 Operator : YP\AJ
 Sample : N3860-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S7-02-S

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/26/2022
 Supervised By :Ankita Jodhani 07/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 03:37:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.601	35777362	62641931	24.655	25.627
2) SA Decachlor...	10.101	8.565	39223884	30138864	27.732	25.879m
Target Compounds						
41) L9 AR-1268-1	8.606	7.478	9852730	8917978	48.256	48.553m
42) L9 AR-1268-2	8.702	7.543	6673658	6191315	35.979	35.786
43) L9 AR-1268-3	8.924	7.747	8458778	7465257	53.659	53.061
44) L9 AR-1268-4	9.358	8.034	2658103	1601147	35.511	26.479 #
45) L9 AR-1268-5	9.770	8.318	29534229	20162923	57.357	49.278

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072522\
Data File : PP049786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 17:14
Operator : YP\AJ
Sample : N3860-06
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleID :
S7-02-S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 03:37:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

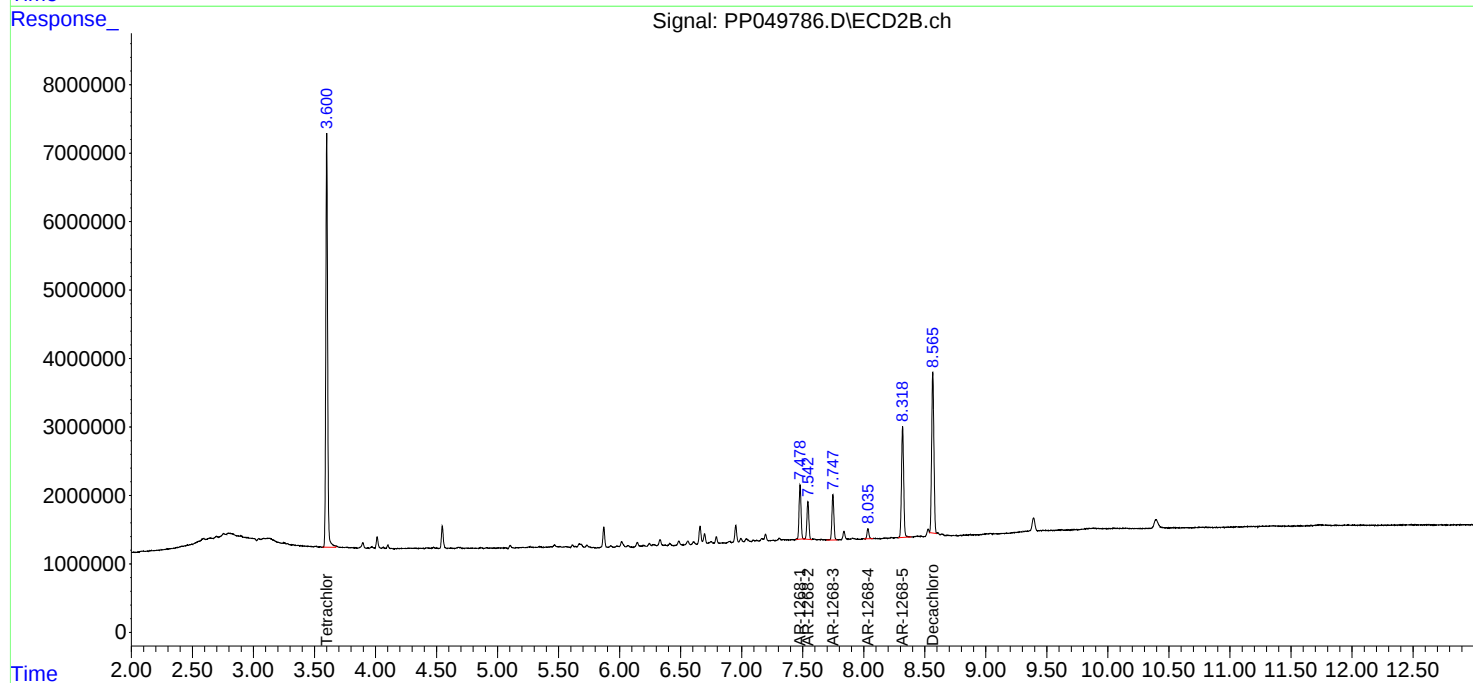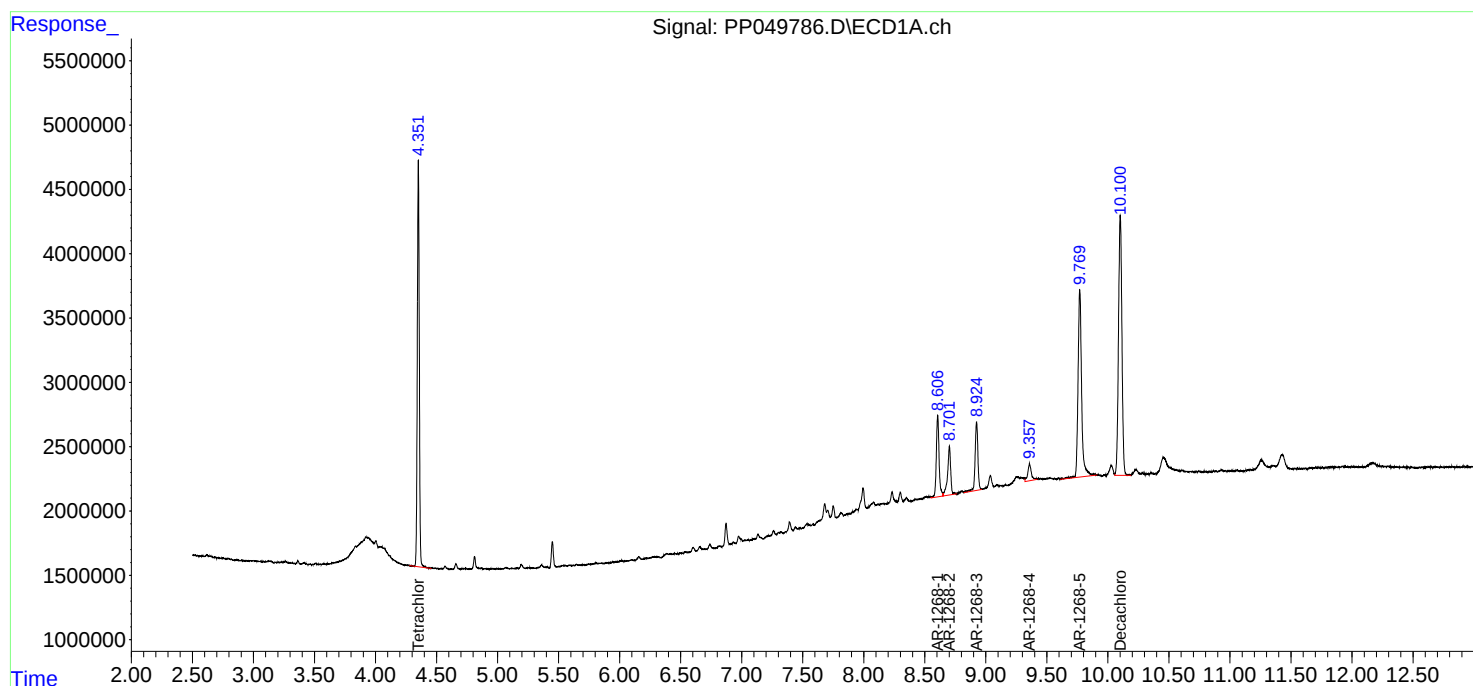

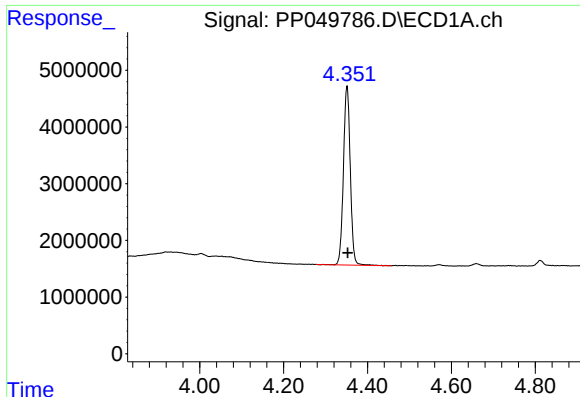


#1 Tetrachloro-m-xylene

R.T.: 4.351 min
Delta R.T.: -0.002 min
Response: 35777362
Conc: 24.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
S7-02-S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

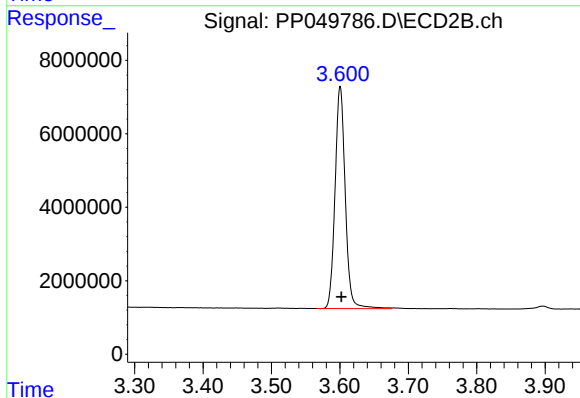


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.001 min
Response: 62641931
Conc: 25.63 ng/ml

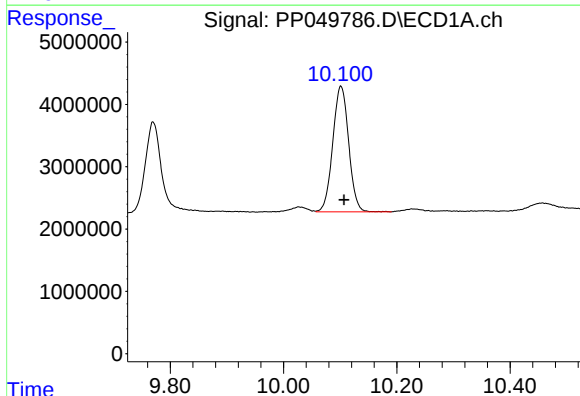


#2 Decachlorobiphenyl

R.T.: 10.101 min
Delta R.T.: -0.006 min
Response: 39223884
Conc: 27.73 ng/ml

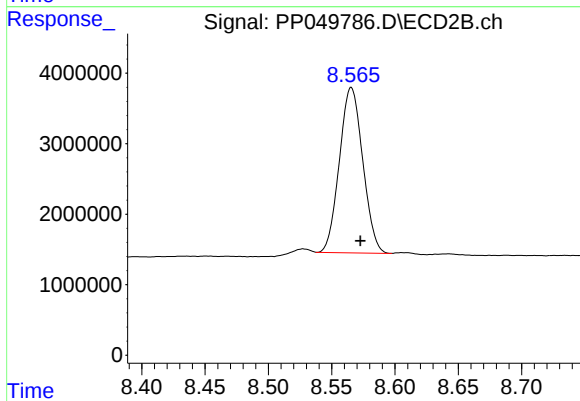

#2 Decachlorobiphenyl

R.T.: 8.565 min
Delta R.T.: -0.008 min
Response: 30138864
Conc: 25.88 ng/ml m

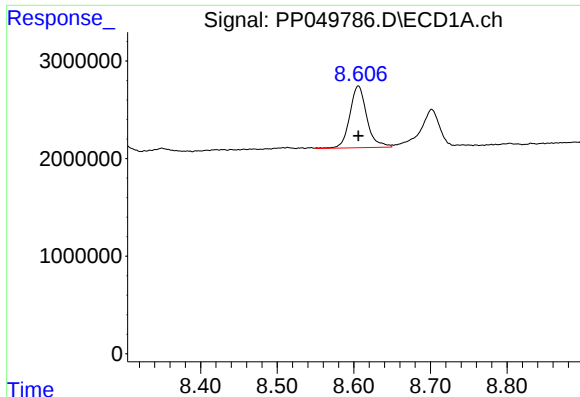


#41 AR-1268-1

R.T.: 8.606 min
Delta R.T.: 0.000 min
Response: 9852730
Conc: 48.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
S7-02-S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

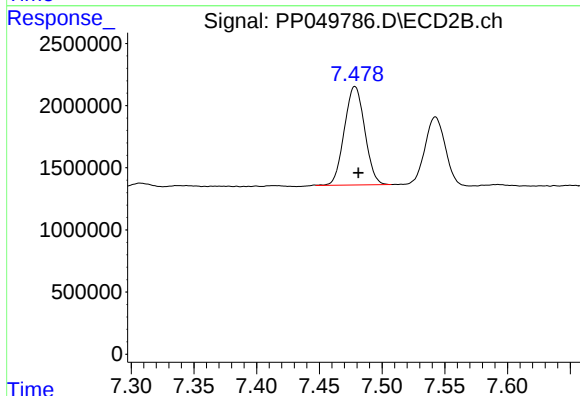


#41 AR-1268-1

R.T.: 7.478 min
Delta R.T.: -0.003 min
Response: 8917978
Conc: 48.55 ng/ml m

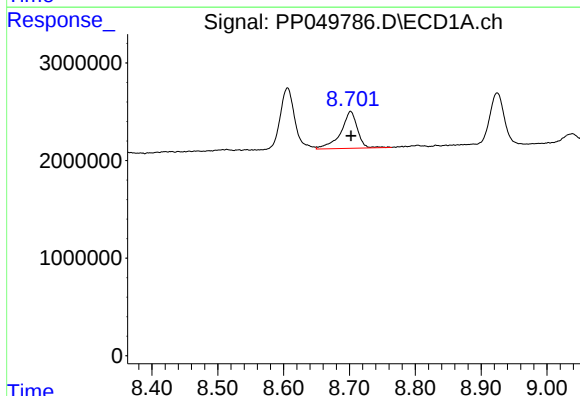


#42 AR-1268-2

R.T.: 8.702 min
Delta R.T.: 0.000 min
Response: 6673658
Conc: 35.98 ng/ml

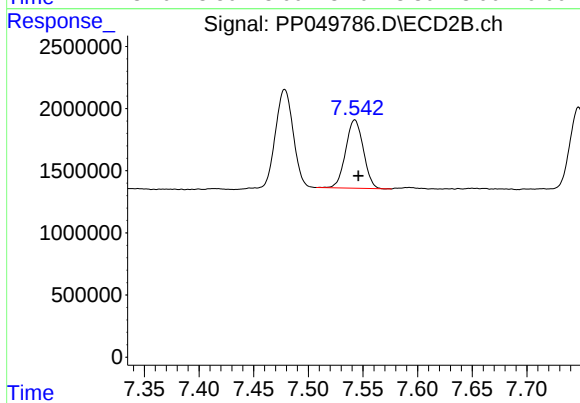

#42 AR-1268-2

R.T.: 7.543 min
Delta R.T.: -0.003 min
Response: 6191315
Conc: 35.79 ng/ml

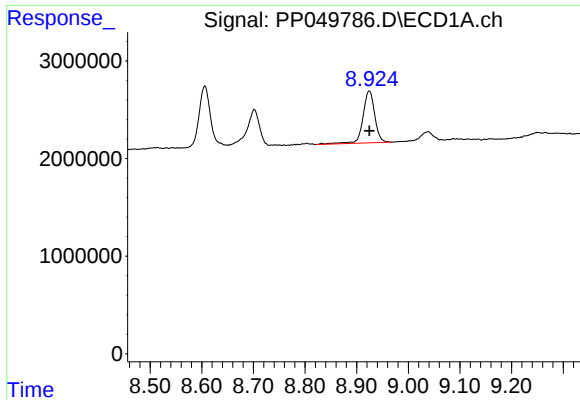


#43 AR-1268-3

R.T.: 8.924 min
Delta R.T.: 0.000 min
Response: 8458778
Conc: 53.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
S7-02-S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

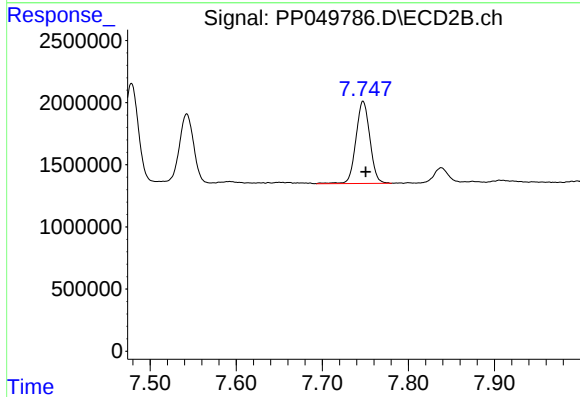


#43 AR-1268-3

R.T.: 7.747 min
Delta R.T.: -0.003 min
Response: 7465257
Conc: 53.06 ng/ml

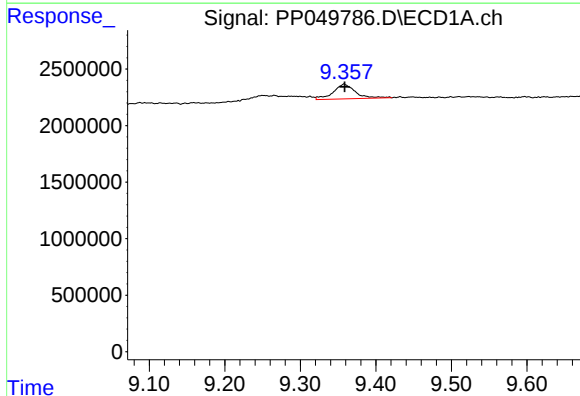


#44 AR-1268-4

R.T.: 9.358 min
Delta R.T.: 0.000 min
Response: 2658103
Conc: 35.51 ng/ml

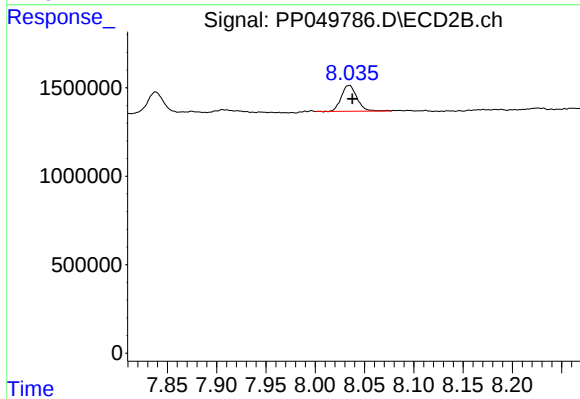

#44 AR-1268-4

R.T.: 8.034 min
Delta R.T.: -0.003 min
Response: 1601147
Conc: 26.48 ng/ml

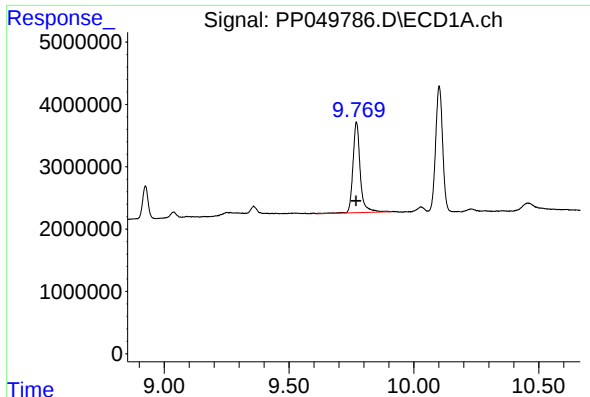


#45 AR-1268-5

R.T.: 9.770 min
Delta R.T.: 0.001 min
Response: 29534229
Conc: 57.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
S7-02-S

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2022
Supervised By :Ankita Jodhani 07/29/2022

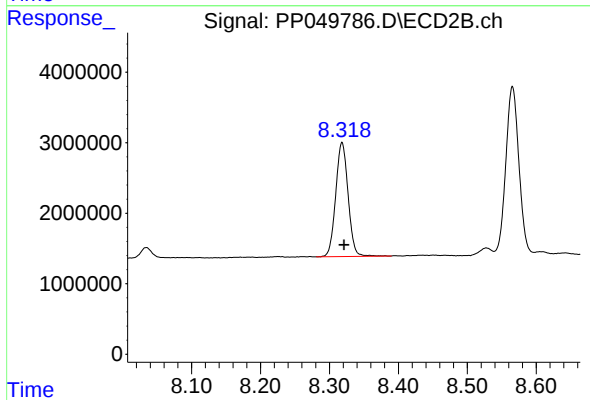

#45 AR-1268-5

R.T.: 8.318 min
Delta R.T.: -0.003 min
Response: 20162923
Conc: 49.28 ng/ml