

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072523\
 Data File : PP058955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2023 18:04
 Operator : YP\AJ
 Sample : 03741-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B-P13A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/26/2023
 Supervised By :Ankita Jodhani 07/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 18:48:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 22 02:26:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.663	26275091	38428006	19.086	19.982
2) SA Decachlor...	10.219	8.705	17560278	28747125	20.384	20.317m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072523\
Data File : PP058955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2023 18:04
Operator : YP\AJ
Sample : 03741-14
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
B-P13A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2023
Supervised By :Ankita Jodhani 07/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 18:48:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 22 02:26:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

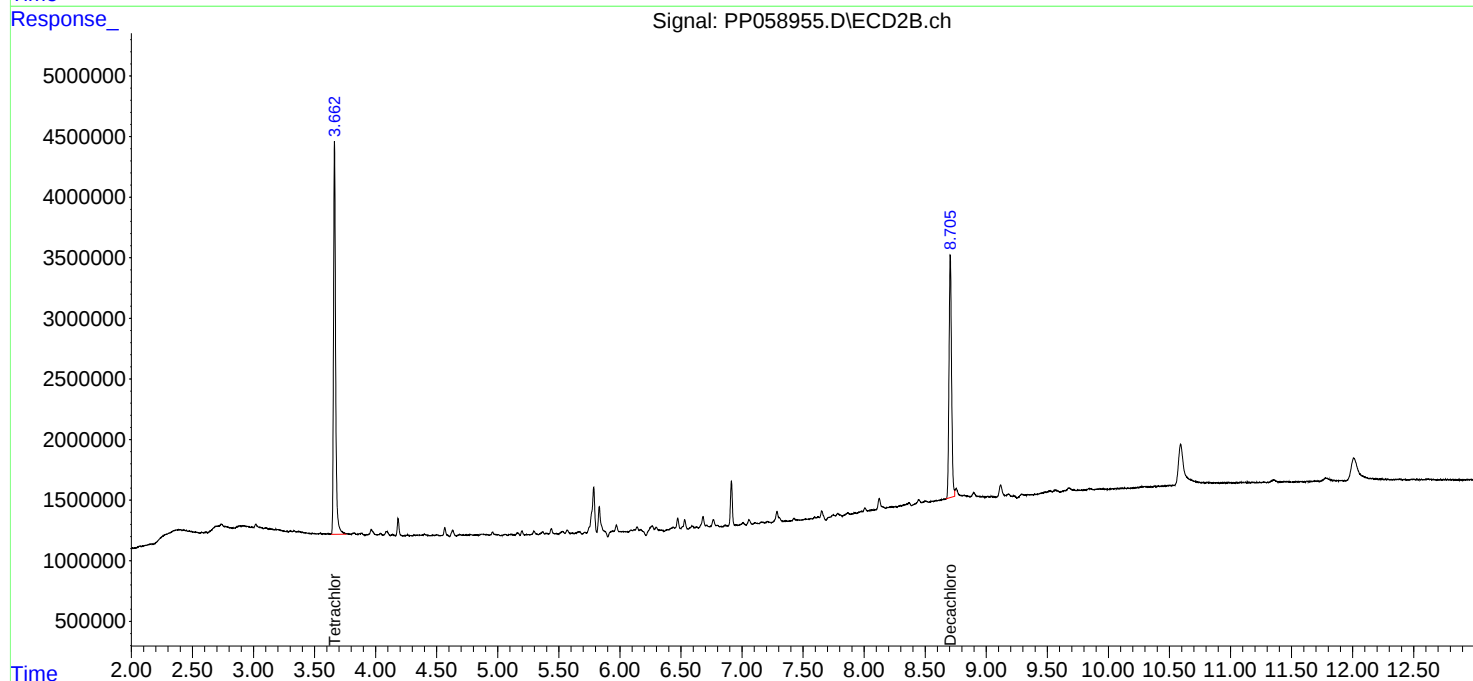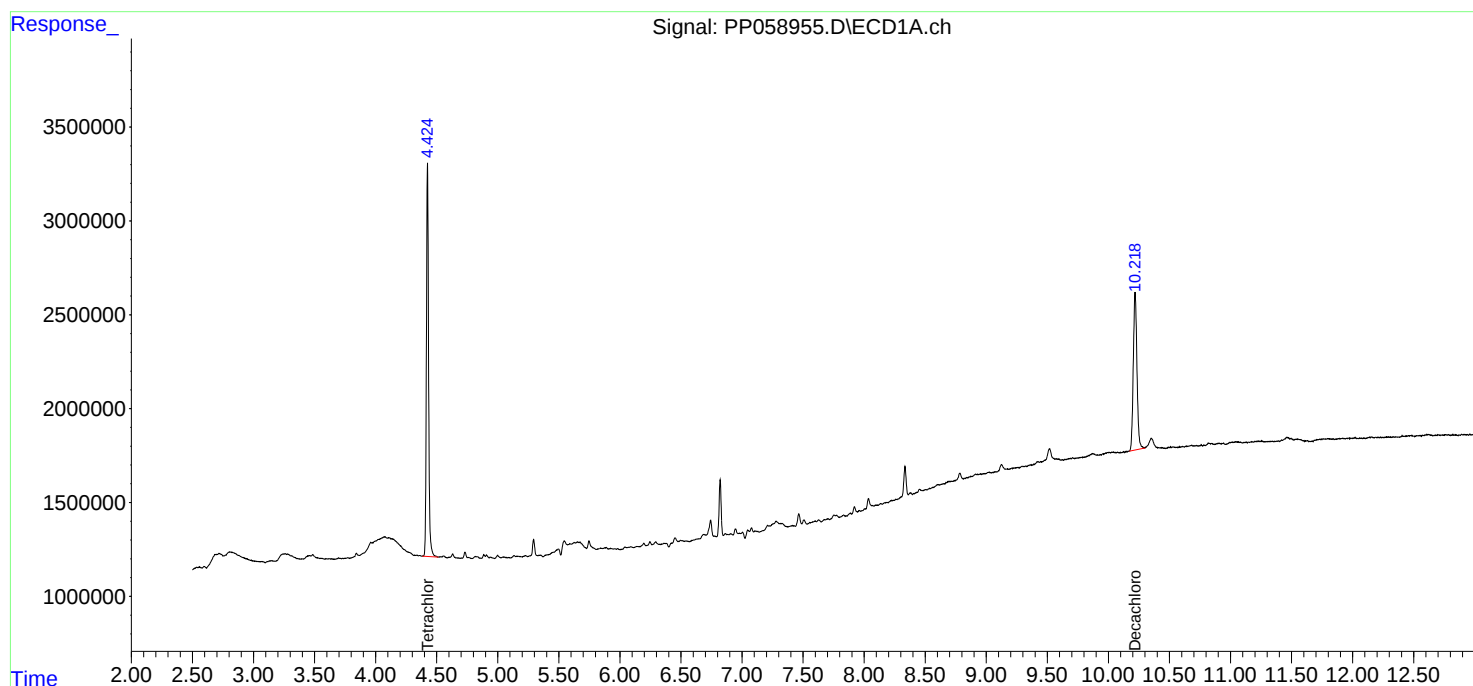

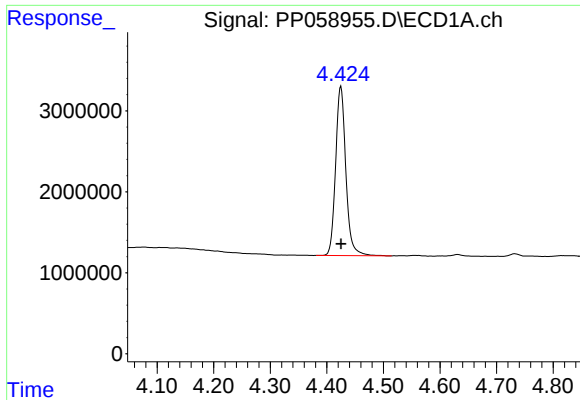


#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: 0.000 min
Response: 26275091
Conc: 19.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
B-P13A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/26/2023
Supervised By :Ankita Jodhani 07/26/2023

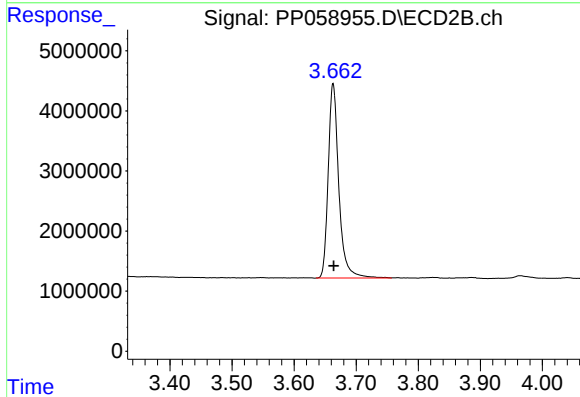


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 38428006
Conc: 19.98 ng/ml

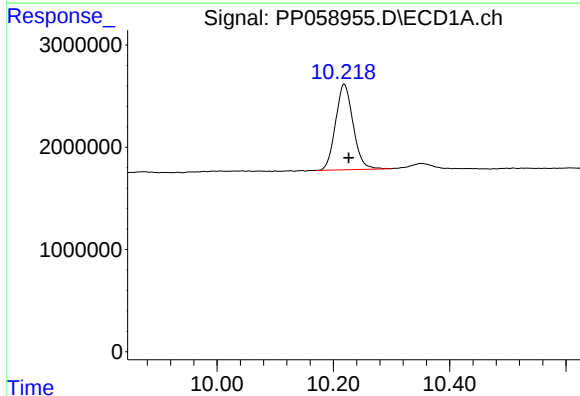

#2 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.007 min
Response: 17560278
Conc: 20.38 ng/ml

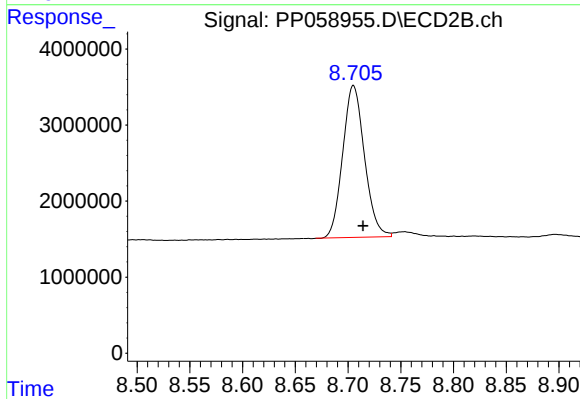

#2 Decachlorobiphenyl

R.T.: 8.705 min
Delta R.T.: -0.010 min
Response: 28747125
Conc: 20.32 ng/ml m