

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072525\
 Data File : PP074072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2025 01:30
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 04:50:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 26 04:44:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.739f	3.894	1570862	256732	1.504	0.028 #
2)	SA Decachlor...	10.619	9.022	128433	1362086	0.191	0.120 #
Target Compounds							
3)	L1 AR-1016-1	5.852	5.016	162893	1922162	4.432	2.263 #
4)	L1 AR-1016-2	5.902	5.063	49799	6200469	0.914	16.529 #
5)	L1 AR-1016-3	5.932	5.196	70874	11163108	2.044	50.652 #
6)	L1 AR-1016-4	6.045	5.249	262980	2569241	9.495	12.289 #
7)	L1 AR-1016-5	6.336	5.435	481862	86427	17.913	0.375 #
8)	L2 AR-1221-1	4.944f	4.108	179822	1038389	11.483	9.273
9)	L2 AR-1221-2	4.980	4.196	403320	917771	33.949	11.984 #
10)	L2 AR-1221-3	5.060	4.271	250904	-79736	7.417	N.D. #
11)	L3 AR-1232-1	5.060	4.271	250904	-79736	9.057	N.D. #
12)	L3 AR-1232-2	5.576	5.016	183242	1922162	13.181	6.323 #
13)	L3 AR-1232-3	5.902	5.196	49799	11163108	1.833	108.628 #
14)	L3 AR-1232-4	6.045	5.284	262980	4510238	18.930	42.749 #
15)	L3 AR-1232-5	6.132	5.435	237912	86427	24.349	0.895 #
16)	L4 AR-1242-1	5.852	5.016	162893	1922162	4.993	2.587 #
17)	L4 AR-1242-2	5.902	5.063	49799	6200469	1.029	18.691 #
18)	L4 AR-1242-3	5.932	5.196	70874	11163108	2.303	57.823 #
19)	L4 AR-1242-4	6.045	5.284	262980	4510238	10.348	19.892 #
20)	L4 AR-1242-5	6.814f	5.789	14823083	6897615	245.793	23.857 #
21)	L5 AR-1248-1	5.852	5.010	162893	1666035	6.371	3.782 #
22)	L5 AR-1248-2	6.132	5.249	237912	2569241	6.840	8.640 #
23)	L5 AR-1248-3	6.336	5.284	481862	4510238	12.242	12.946
24)	L5 AR-1248-4	6.721	5.435	3233036	86427	69.470	0.253 #
25)	L5 AR-1248-5	6.814f	5.866	14823083	834646	195.411	1.554 #
26)	L6 AR-1254-1	6.721	5.789	3233036	6897615	64.364	9.824 #
27)	L6 AR-1254-2	6.933	5.978	9495118	42960102	135.480	80.201 #
28)	L6 AR-1254-3	7.295	6.379	24442007	76470413	334.549	87.376 #
29)	L6 AR-1254-4	7.580	6.548f	1231402	476747	23.588	0.702 #
30)	L6 AR-1254-5	8.021	7.013	895.8E6	12113.2E6	14826.736	15125.195
31)	L7 AR-1260-1	7.420f	6.654	4306288	157.4E6	100.166	200.774 #
32)	L7 AR-1260-2	7.705	0.000	1138.6E6	0	20797.994	N.D. #
33)	L7 AR-1260-3	8.086	7.013f	1789367	12113.2E6	47.145	15245.084 #
34)	L7 AR-1260-4	8.280	7.314	179265	1276101	3.748	2.222 #
35)	L7 AR-1260-5	8.662	7.563	81653	961121	0.957	0.618 #
36)	L8 AR-1262-1	8.280	7.013f	179265	12113.2E6	2.890	10236.207 #
37)	L8 AR-1262-2	8.662	7.314	81653	1276101	0.738	1.520 #
38)	L8 AR-1262-3	8.984	7.865	61437	46492782	0.799	60.245 #
39)	L8 AR-1262-4	9.105f	7.865f	402231	46492782	7.013	33.009 #
40)	L8 AR-1262-5	9.775	8.419	117483	555862	3.016	0.884 #
41)	L9 AR-1268-1	8.984	7.865	61437	46492782	0.480	20.793 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072525\
 Data File : PP074072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2025 01:30
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 04:50:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 26 04:44:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.105	7.865f	402231	46492782	3.439	21.482 #
43) L9	AR-1268-3	9.298	8.125	191911	741246	1.983	0.462 #
44) L9	AR-1268-4	9.775	8.419	117483	555862	2.705	0.838 #
45) L9	AR-1268-5	10.208	8.727	127550	575845	0.444	0.114 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072525\
Data File : PP074072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2025 01:30
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 04:50:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 26 04:44:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

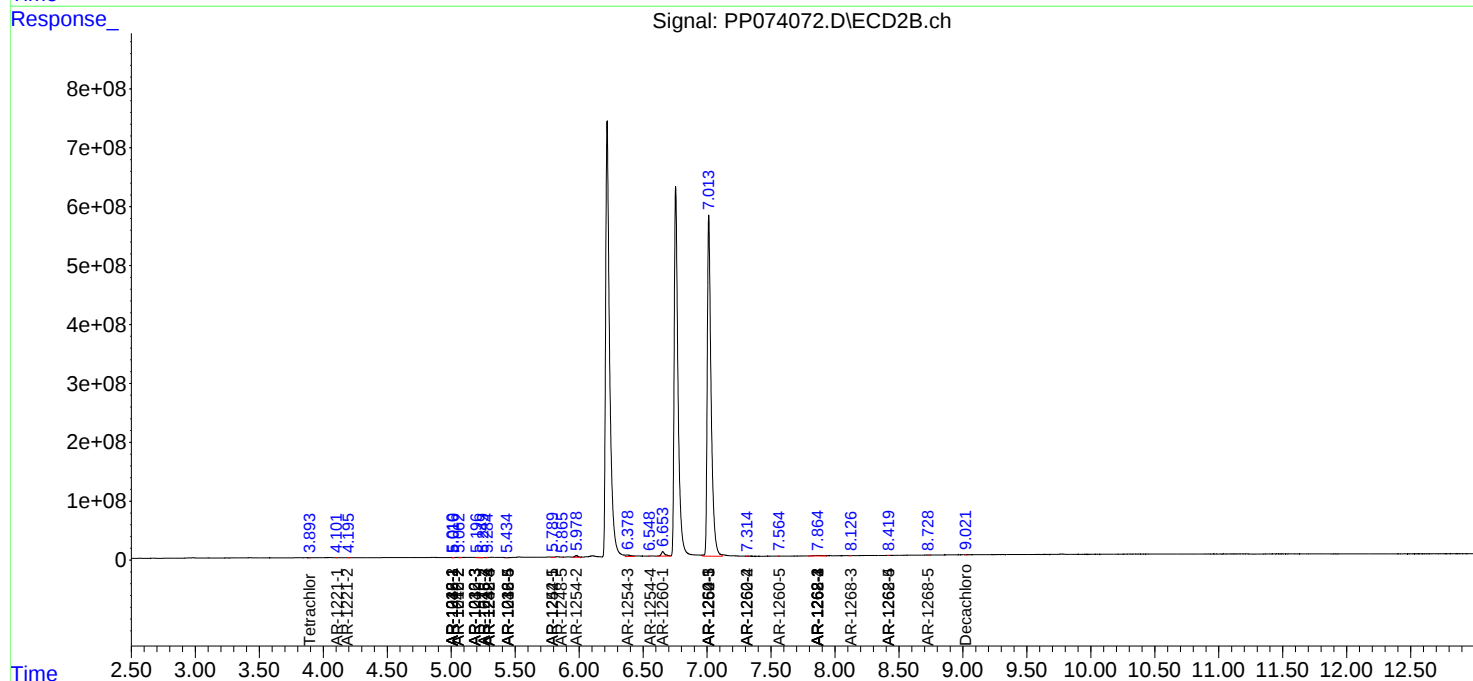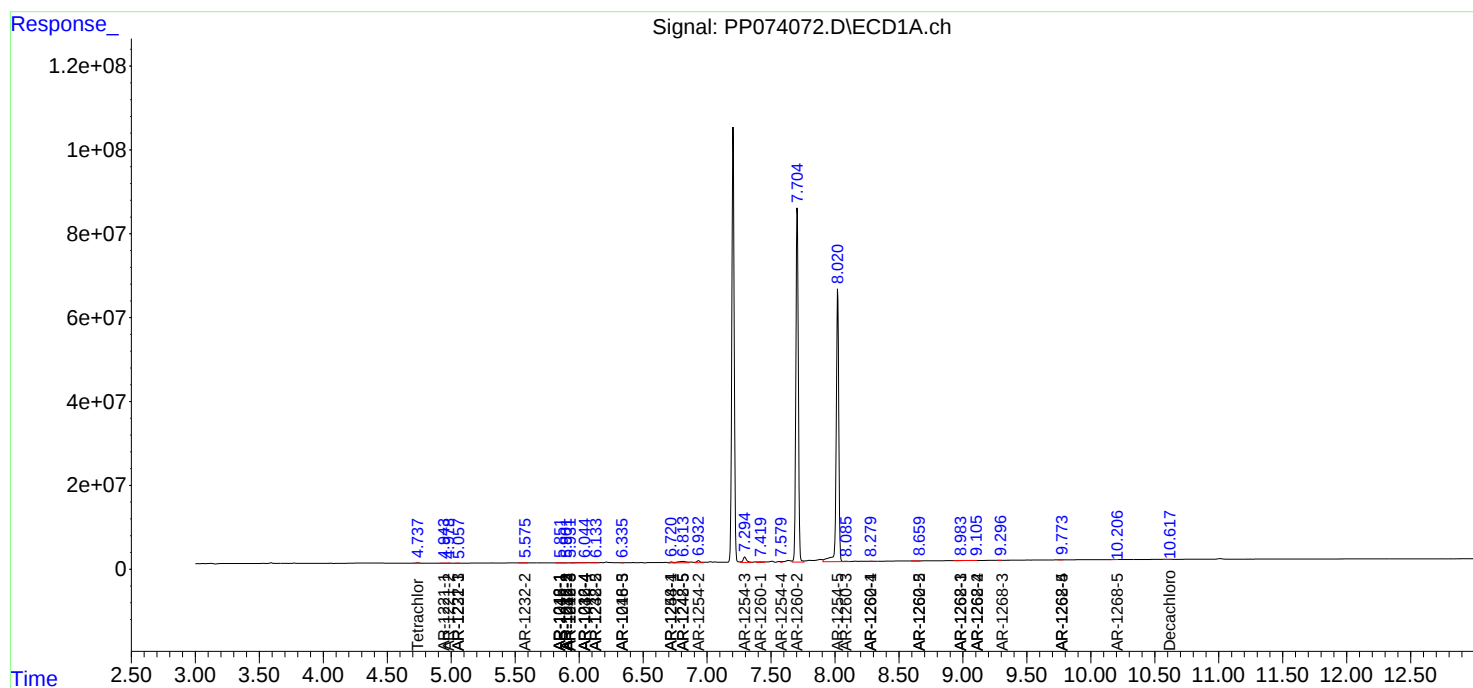


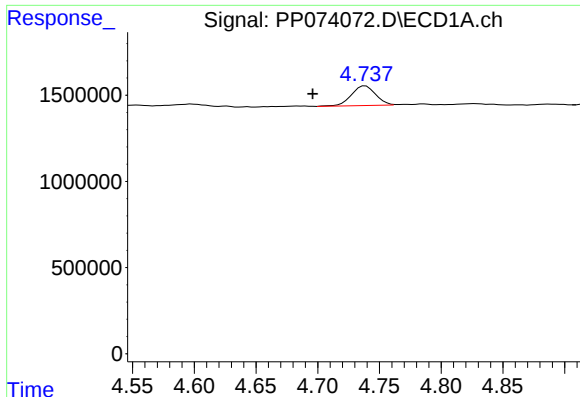

#1 Tetrachloro-m-xylene


R.T.: 4.739 min
Delta R.T.: 0.043 min
Response: 1570862
Conc: 1.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

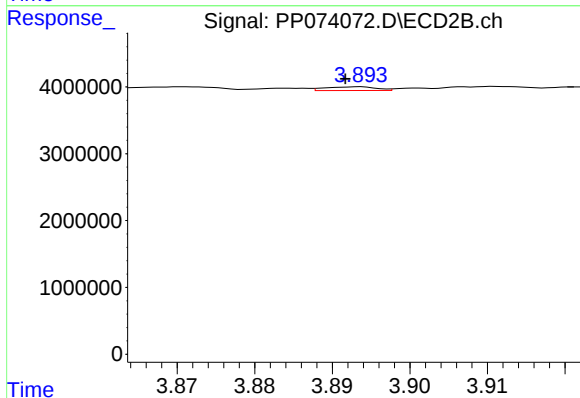


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: 0.002 min
Response: 256732
Conc: 0.03 ng/ml

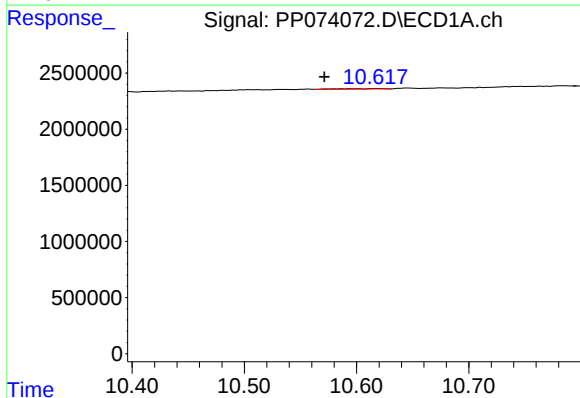


#2 Decachlorobiphenyl

R.T.: 10.619 min
Delta R.T.: 0.047 min
Response: 128433
Conc: 0.19 ng/ml

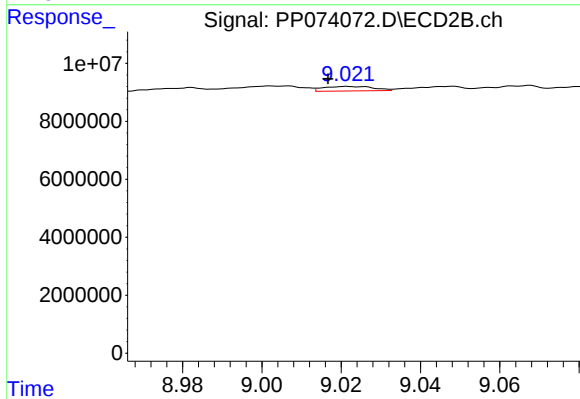

#2 Decachlorobiphenyl


R.T.: 9.022 min
Delta R.T.: 0.005 min
Response: 1362086
Conc: 0.12 ng/ml

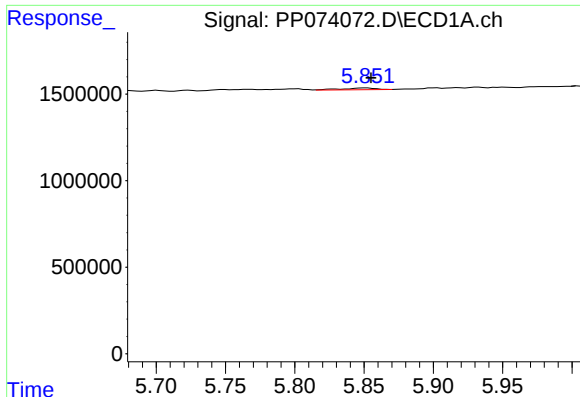

#3 AR-1016-1


R.T.: 5.852 min
Delta R.T.: -0.003 min
Response: 162893
Conc: 4.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

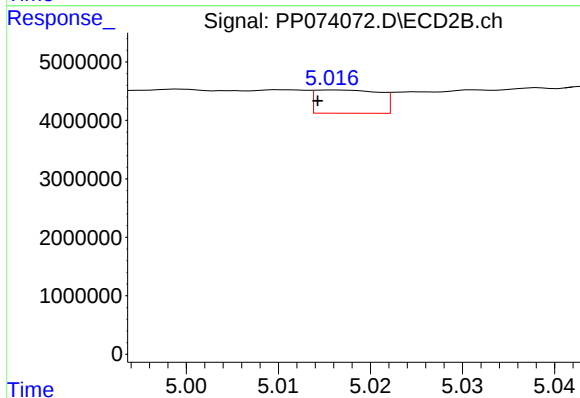


#3 AR-1016-1

R.T.: 5.016 min
Delta R.T.: 0.002 min
Response: 1922162
Conc: 2.26 ng/ml

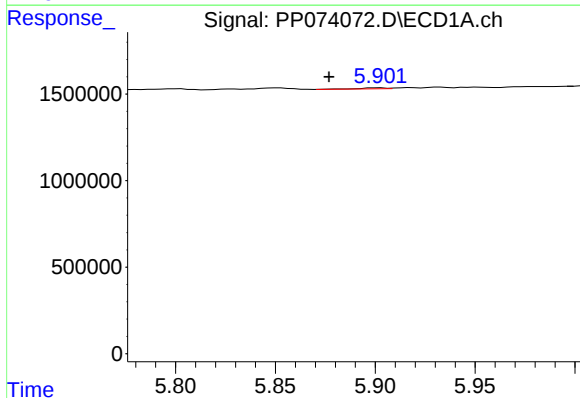


#4 AR-1016-2

R.T.: 5.902 min
Delta R.T.: 0.025 min
Response: 49799
Conc: 0.91 ng/ml

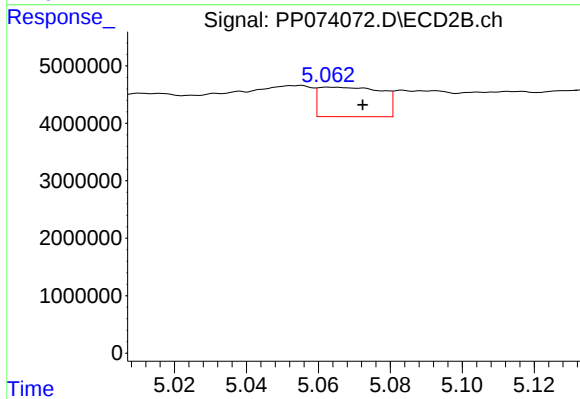

#4 AR-1016-2


R.T.: 5.063 min
Delta R.T.: -0.010 min
Response: 6200469
Conc: 16.53 ng/ml

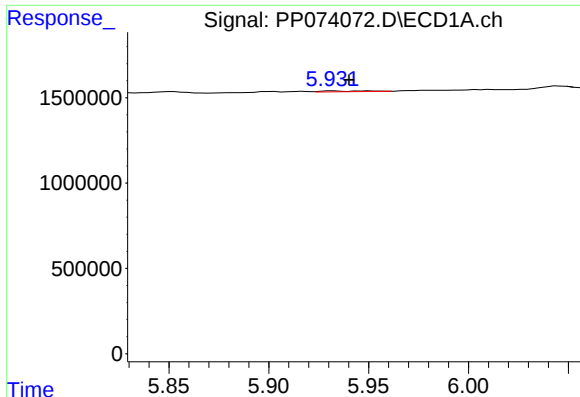

#5 AR-1016-3


R.T.: 5.932 min
Delta R.T.: -0.008 min
Response: 70874
Conc: 2.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

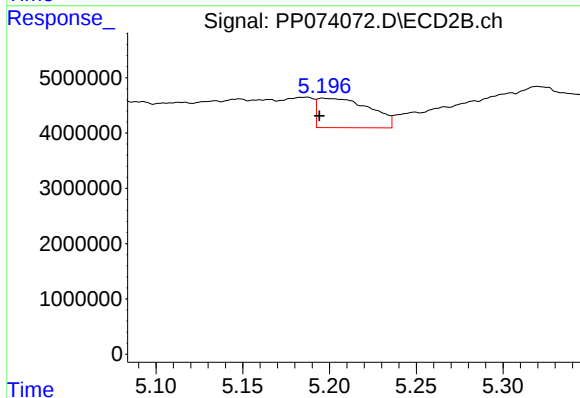


#5 AR-1016-3

R.T.: 5.196 min
Delta R.T.: 0.002 min
Response: 11163108
Conc: 50.65 ng/ml

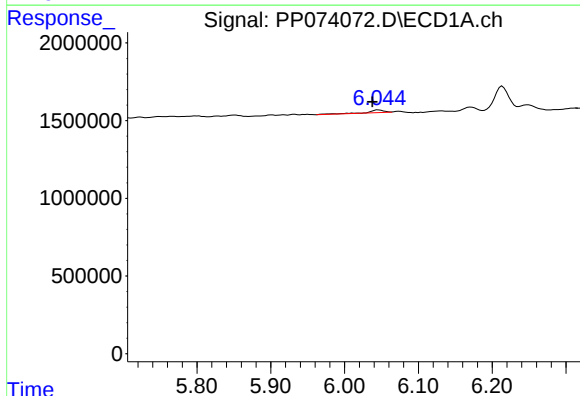


#6 AR-1016-4

R.T.: 6.045 min
Delta R.T.: 0.007 min
Response: 262980
Conc: 9.50 ng/ml

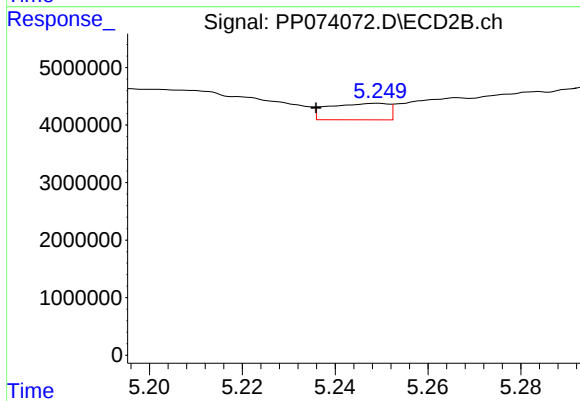

#6 AR-1016-4


R.T.: 5.249 min
Delta R.T.: 0.013 min
Response: 2569241
Conc: 12.29 ng/ml

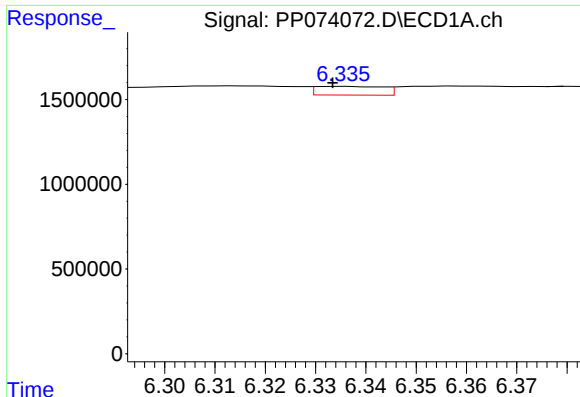

#7 AR-1016-5


R.T.: 6.336 min
Delta R.T.: 0.003 min
Response: 481862
Conc: 17.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

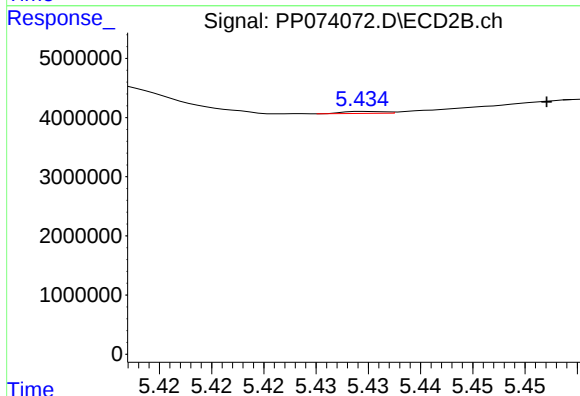


#7 AR-1016-5

R.T.: 5.435 min
Delta R.T.: -0.017 min
Response: 86427
Conc: 0.37 ng/ml

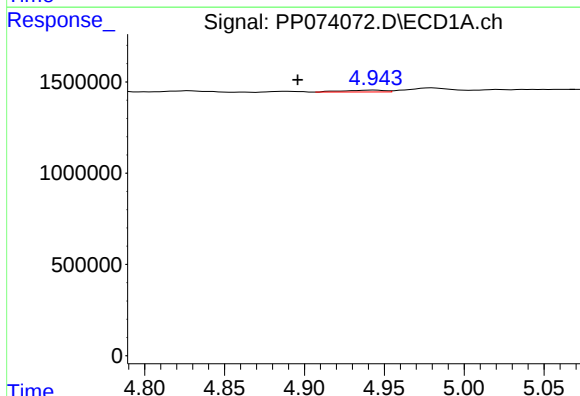


#8 AR-1221-1

R.T.: 4.944 min
Delta R.T.: 0.049 min
Response: 179822
Conc: 11.48 ng/ml

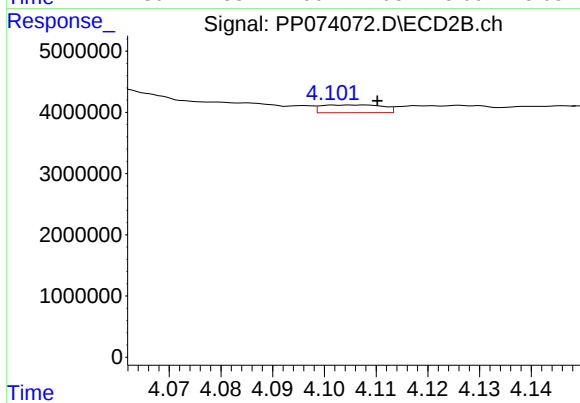

#8 AR-1221-1


R.T.: 4.108 min
Delta R.T.: -0.002 min
Response: 1038389
Conc: 9.27 ng/ml

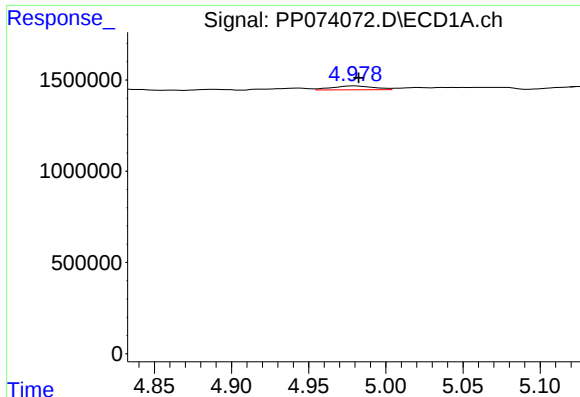

#9 AR-1221-2


R.T.: 4.980 min
Delta R.T.: -0.002 min
Response: 403320
Conc: 33.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

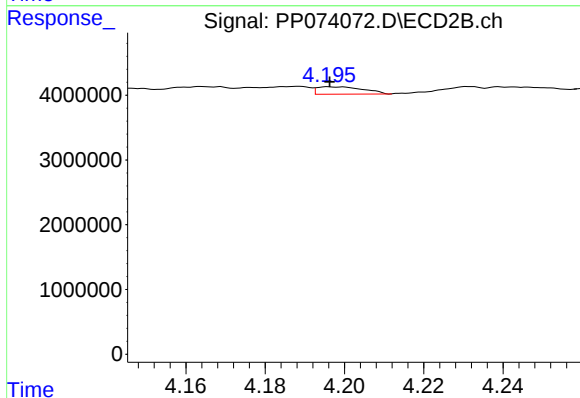


#9 AR-1221-2

R.T.: 4.196 min
Delta R.T.: 0.000 min
Response: 917771
Conc: 11.98 ng/ml

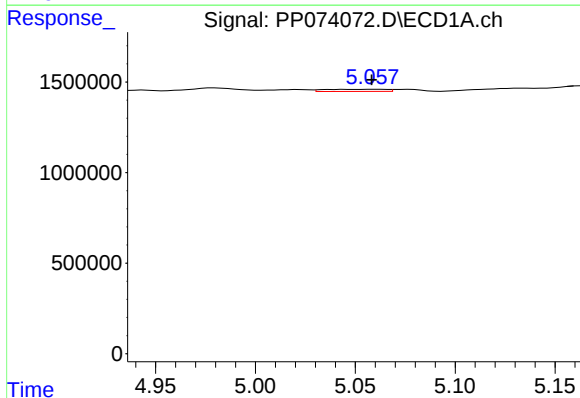


#10 AR-1221-3

R.T.: 5.060 min
Delta R.T.: 0.002 min
Response: 250904
Conc: 7.42 ng/ml

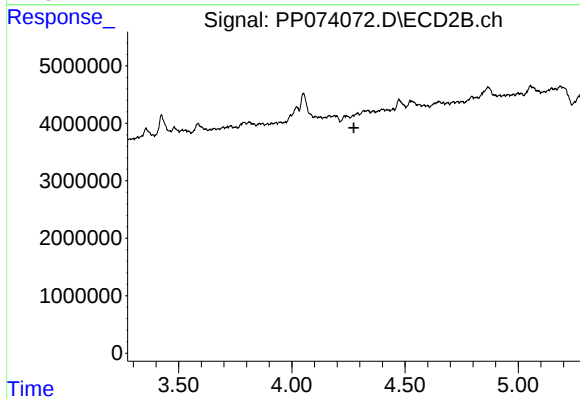

#10 AR-1221-3


R.T.: 4.271 min
Delta R.T.: -0.003 min
Response: -79736
Conc: N.D.

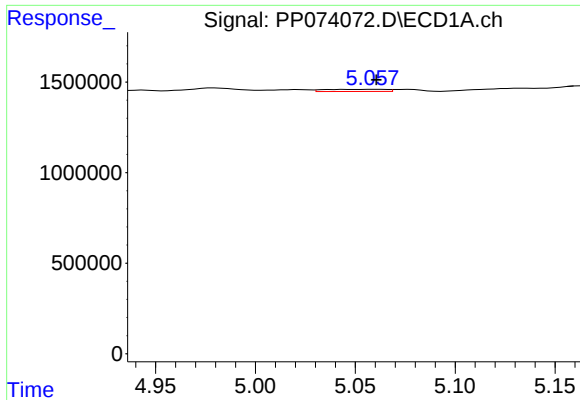

#11 AR-1232-1


R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 250904
Conc: 9.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

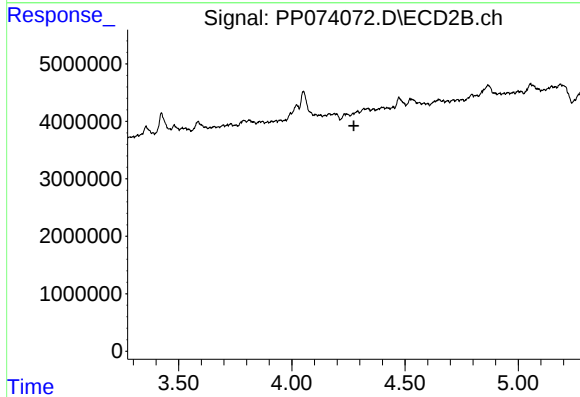


#11 AR-1232-1

R.T.: 4.271 min
Delta R.T.: -0.003 min
Response: -79736
Conc: N.D.

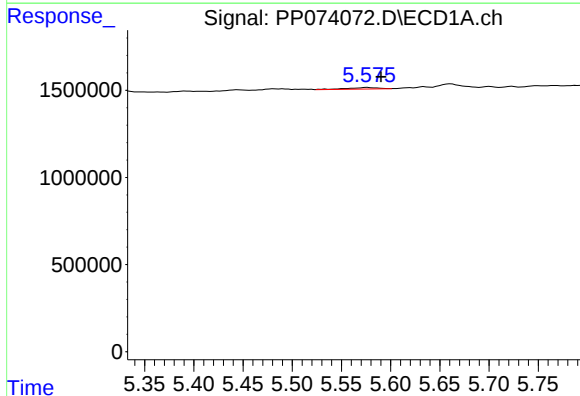


#12 AR-1232-2

R.T.: 5.576 min
Delta R.T.: -0.014 min
Response: 183242
Conc: 13.18 ng/ml

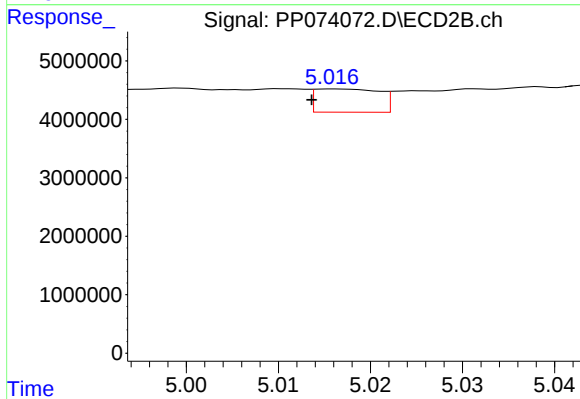

#12 AR-1232-2


R.T.: 5.016 min
Delta R.T.: 0.003 min
Response: 1922162
Conc: 6.32 ng/ml

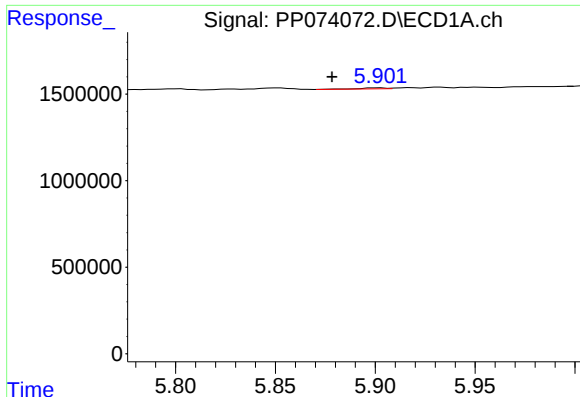

#13 AR-1232-3


R.T.: 5.902 min
Delta R.T.: 0.023 min
Response: 49799
Conc: 1.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

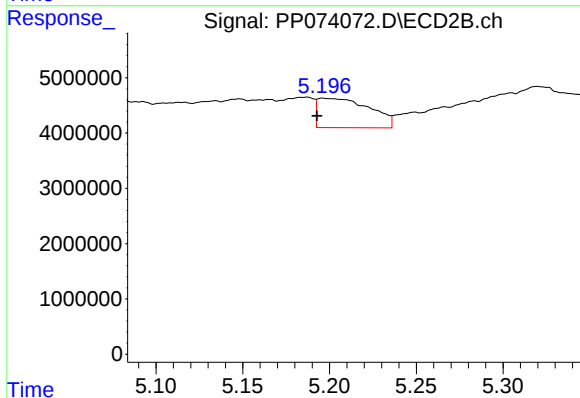


#13 AR-1232-3

R.T.: 5.196 min
Delta R.T.: 0.003 min
Response: 11163108
Conc: 108.63 ng/ml

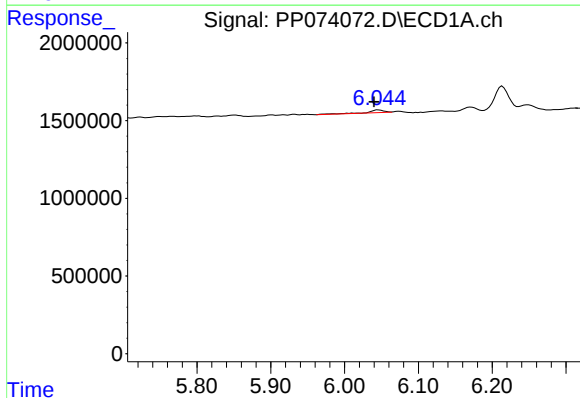


#14 AR-1232-4

R.T.: 6.045 min
Delta R.T.: 0.005 min
Response: 262980
Conc: 18.93 ng/ml

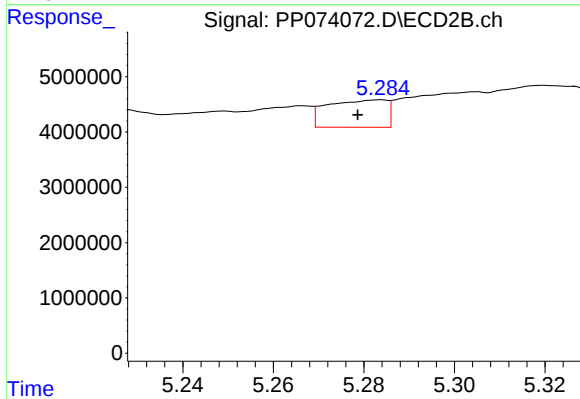

#14 AR-1232-4


R.T.: 5.284 min
Delta R.T.: 0.005 min
Response: 4510238
Conc: 42.75 ng/ml

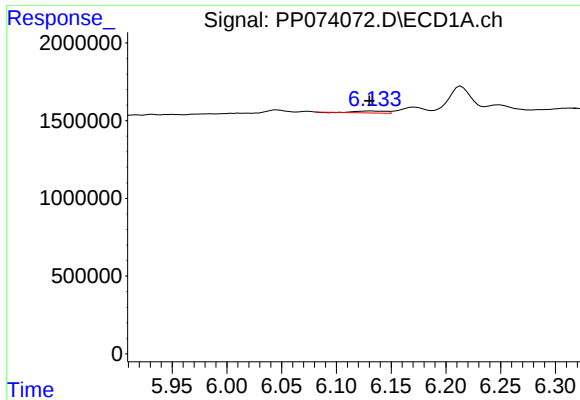

#15 AR-1232-5


R.T.: 6.132 min
Delta R.T.: 0.002 min
Response: 237912
Conc: 24.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

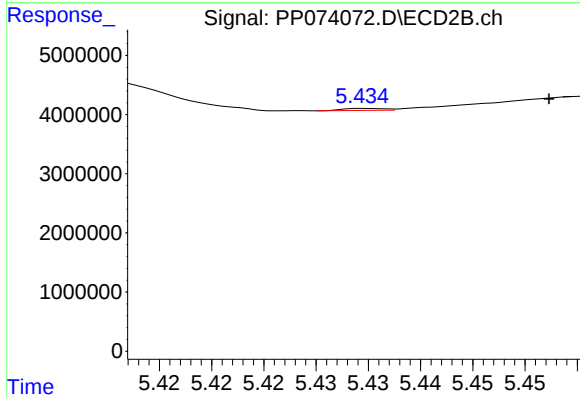


#15 AR-1232-5

R.T.: 5.435 min
Delta R.T.: -0.018 min
Response: 86427
Conc: 0.90 ng/ml

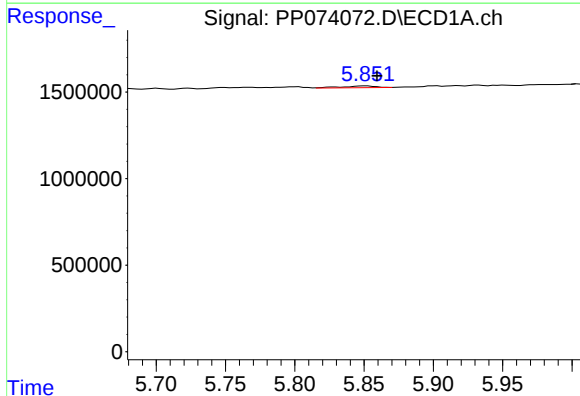


#16 AR-1242-1

R.T.: 5.852 min
Delta R.T.: -0.007 min
Response: 162893
Conc: 4.99 ng/ml

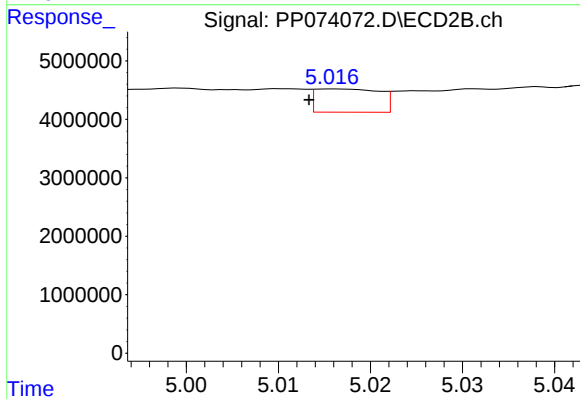

#16 AR-1242-1


R.T.: 5.016 min
Delta R.T.: 0.003 min
Response: 1922162
Conc: 2.59 ng/ml

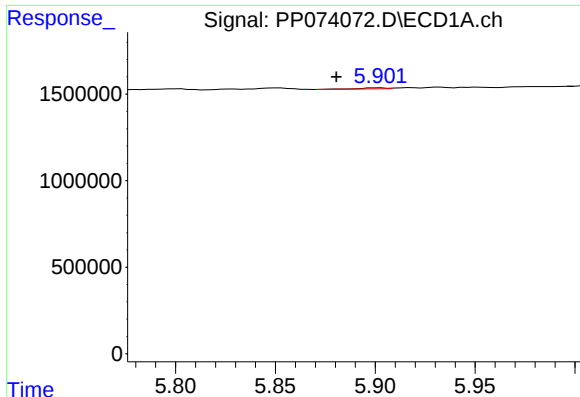

#17 AR-1242-2


R.T.: 5.902 min
Delta R.T.: 0.021 min
Response: 49799
Conc: 1.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

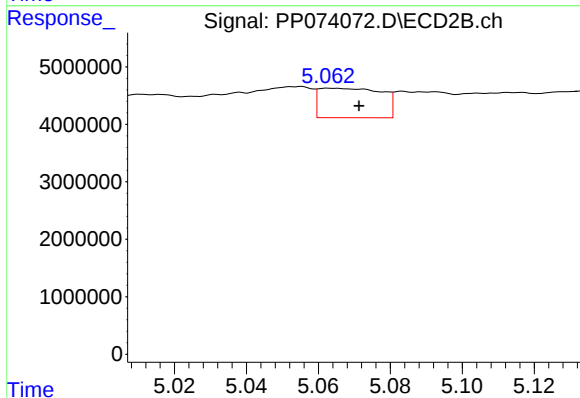


#17 AR-1242-2

R.T.: 5.063 min
Delta R.T.: -0.009 min
Response: 6200469
Conc: 18.69 ng/ml

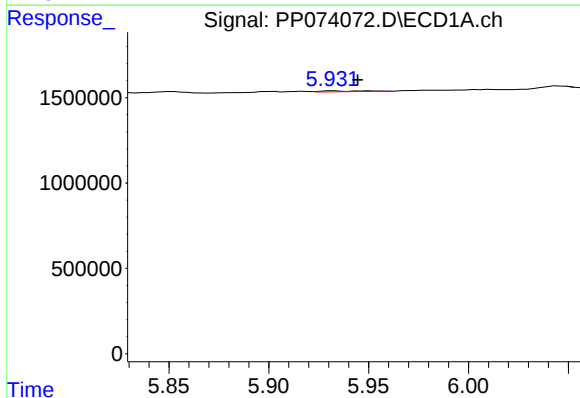


#18 AR-1242-3

R.T.: 5.932 min
Delta R.T.: -0.012 min
Response: 70874
Conc: 2.30 ng/ml

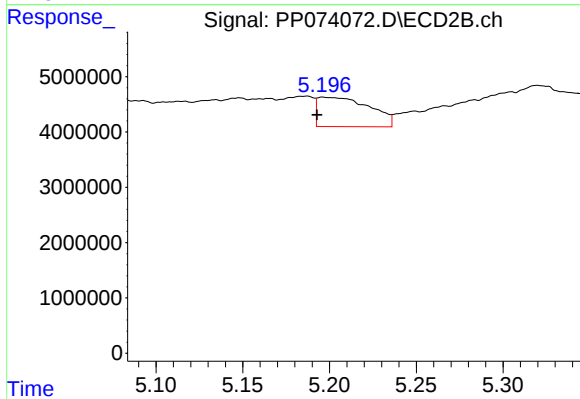

#18 AR-1242-3


R.T.: 5.196 min
Delta R.T.: 0.003 min
Response: 11163108
Conc: 57.82 ng/ml

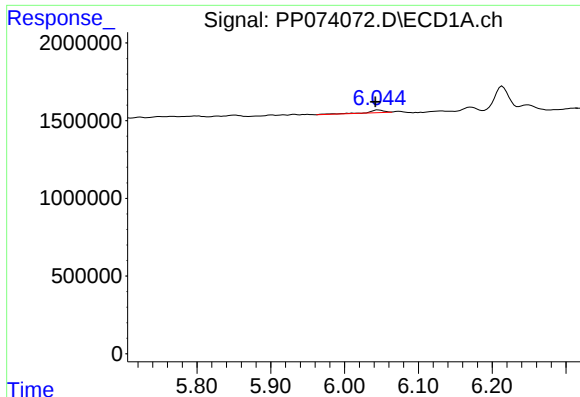

#19 AR-1242-4


R.T.: 6.045 min
Delta R.T.: 0.003 min
Response: 262980
Conc: 10.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

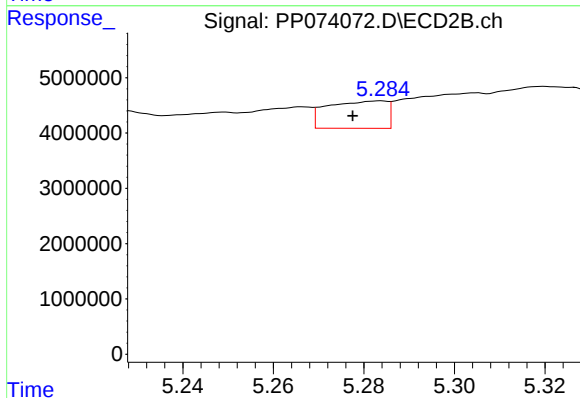


#19 AR-1242-4

R.T.: 5.284 min
Delta R.T.: 0.006 min
Response: 4510238
Conc: 19.89 ng/ml

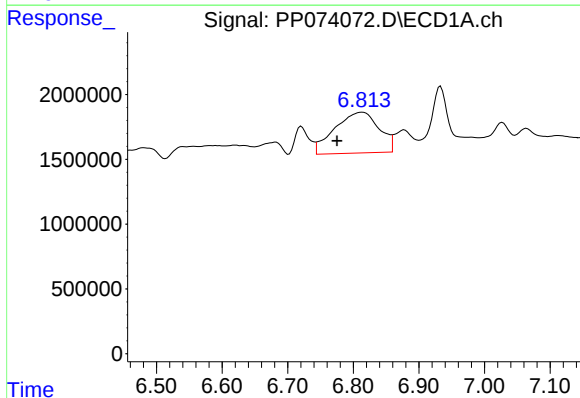


#20 AR-1242-5

R.T.: 6.814 min
Delta R.T.: 0.039 min
Response: 14823083
Conc: 245.79 ng/ml

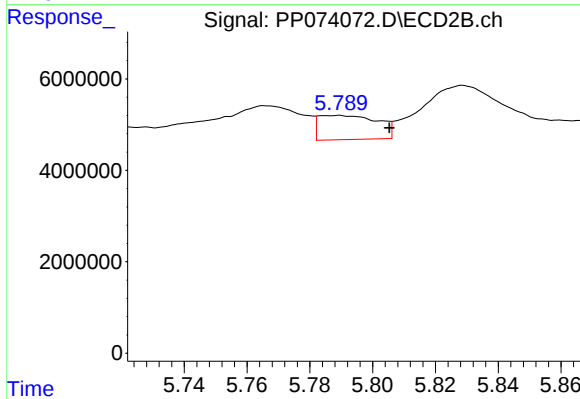

#20 AR-1242-5


R.T.: 5.789 min
Delta R.T.: -0.016 min
Response: 6897615
Conc: 23.86 ng/ml

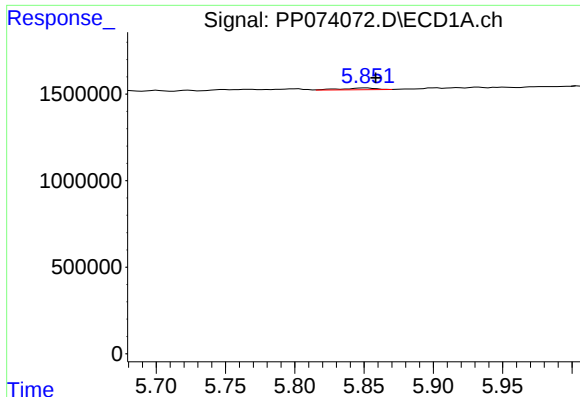

#21 AR-1248-1


R.T.: 5.852 min
Delta R.T.: -0.007 min
Response: 162893
Conc: 6.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

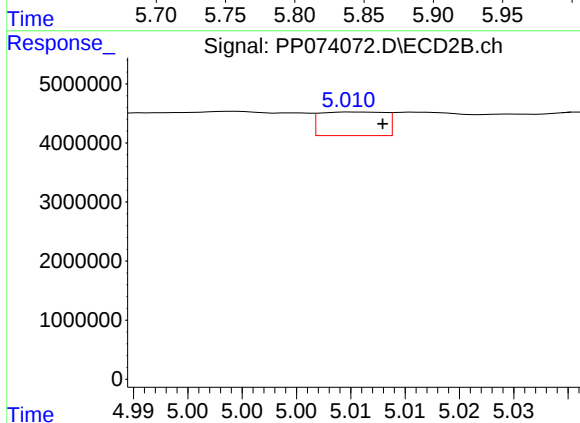


#21 AR-1248-1

R.T.: 5.010 min
Delta R.T.: -0.003 min
Response: 1666035
Conc: 3.78 ng/ml

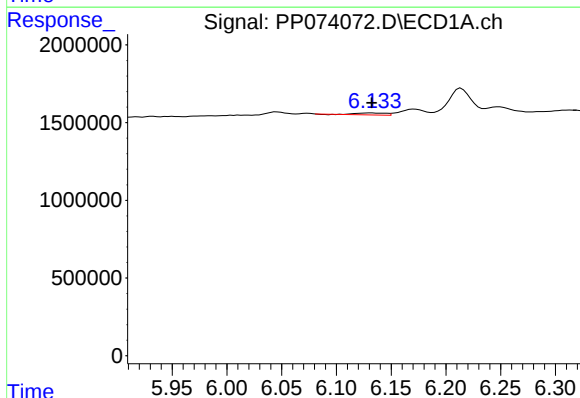


#22 AR-1248-2

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 237912
Conc: 6.84 ng/ml

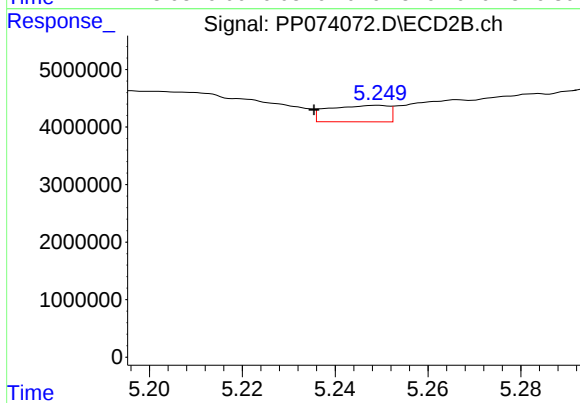

#22 AR-1248-2


R.T.: 5.249 min
Delta R.T.: 0.014 min
Response: 2569241
Conc: 8.64 ng/ml

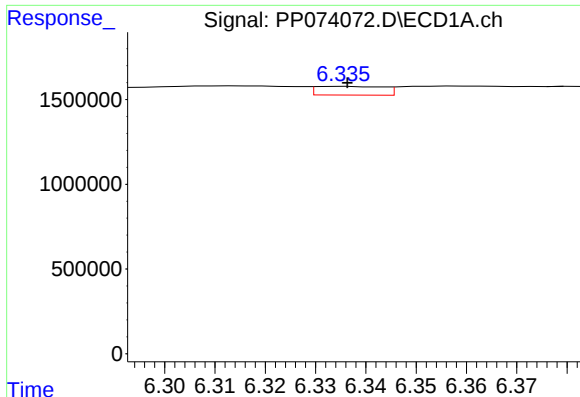

#23 AR-1248-3


R.T.: 6.336 min
Delta R.T.: 0.000 min
Response: 481862
Conc: 12.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

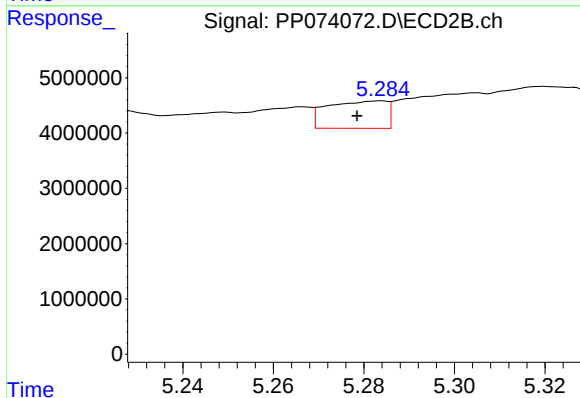


#23 AR-1248-3

R.T.: 5.284 min
Delta R.T.: 0.005 min
Response: 4510238
Conc: 12.95 ng/ml

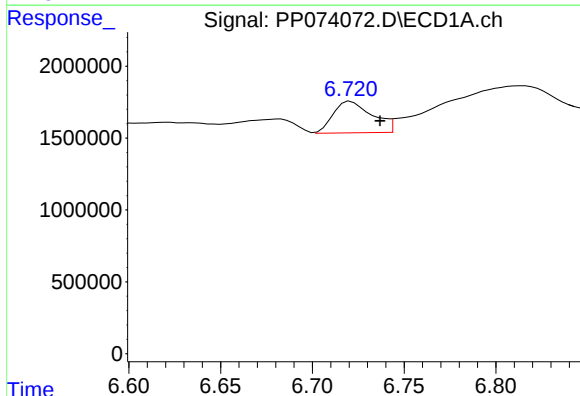


#24 AR-1248-4

R.T.: 6.721 min
Delta R.T.: -0.016 min
Response: 3233036
Conc: 69.47 ng/ml

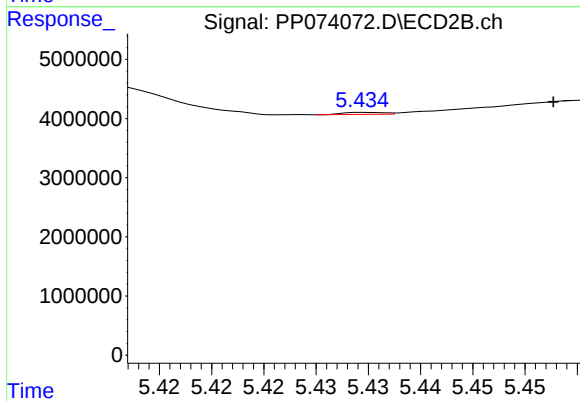

#24 AR-1248-4


R.T.: 5.435 min
Delta R.T.: -0.018 min
Response: 86427
Conc: 0.25 ng/ml

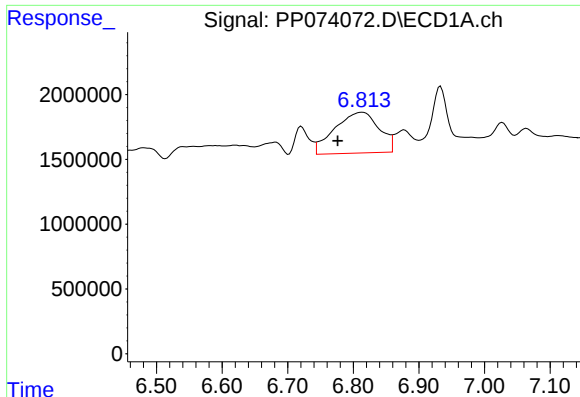

#25 AR-1248-5


R.T.: 6.814 min
Delta R.T.: 0.038 min
Response: 14823083
Conc: 195.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

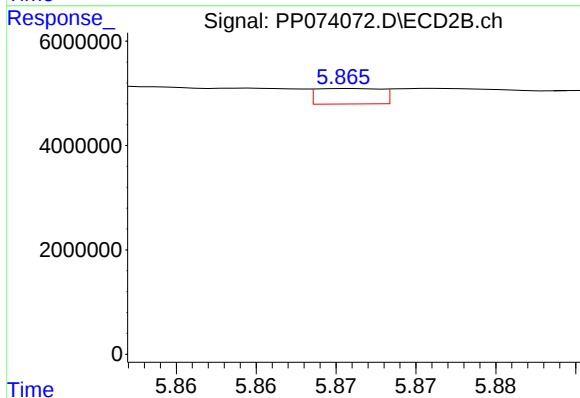


#25 AR-1248-5

R.T.: 5.866 min
Delta R.T.: 0.018 min
Response: 834646
Conc: 1.55 ng/ml

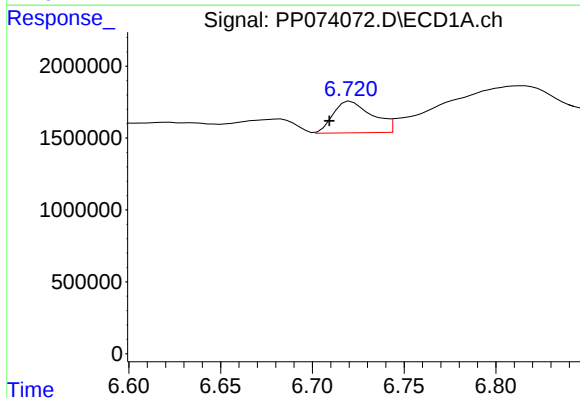


#26 AR-1254-1

R.T.: 6.721 min
Delta R.T.: 0.012 min
Response: 3233036
Conc: 64.36 ng/ml

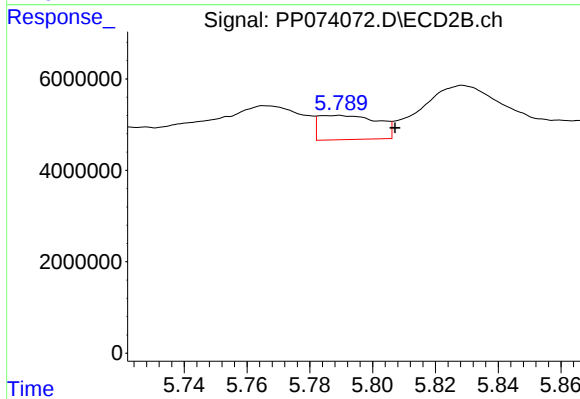

#26 AR-1254-1


R.T.: 5.789 min
Delta R.T.: -0.018 min
Response: 6897615
Conc: 9.82 ng/ml

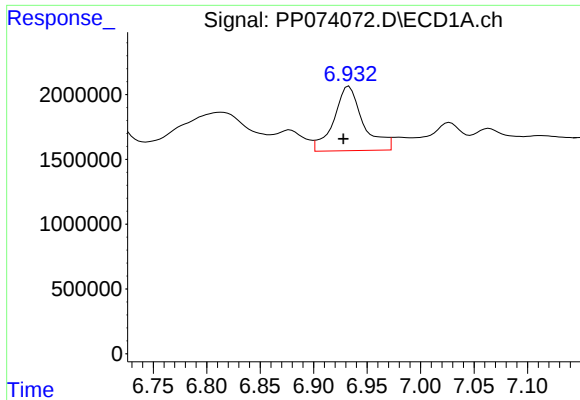

#27 AR-1254-2


R.T.: 6.933 min
Delta R.T.: 0.005 min
Response: 9495118
Conc: 135.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

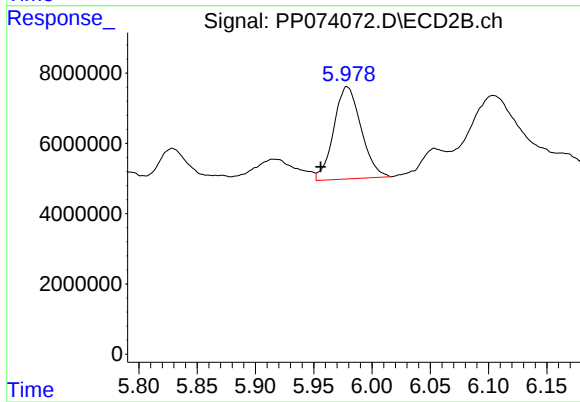


#27 AR-1254-2

R.T.: 5.978 min
Delta R.T.: 0.022 min
Response: 42960102
Conc: 80.20 ng/ml

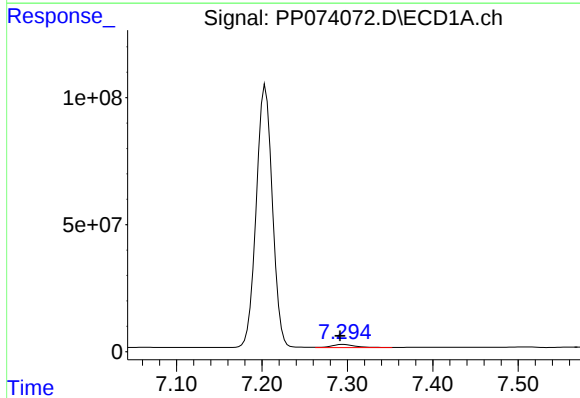


#28 AR-1254-3

R.T.: 7.295 min
Delta R.T.: 0.004 min
Response: 24442007
Conc: 334.55 ng/ml

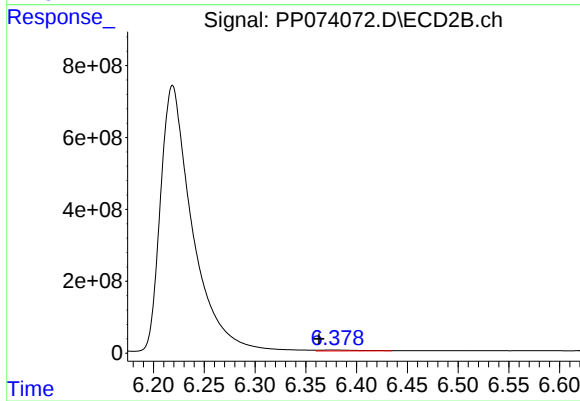

#28 AR-1254-3


R.T.: 6.379 min
Delta R.T.: 0.016 min
Response: 76470413
Conc: 87.38 ng/ml

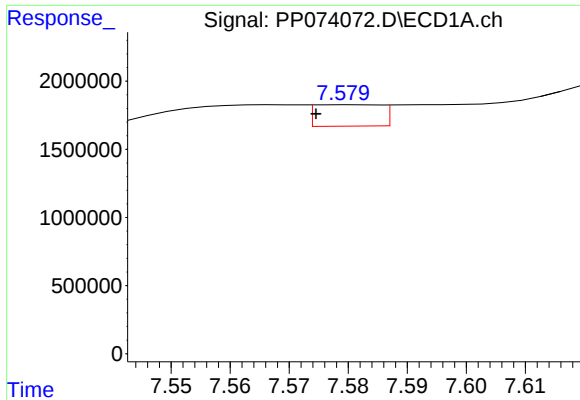

#29 AR-1254-4


R.T.: 7.580 min
Delta R.T.: 0.005 min
Response: 1231402
Conc: 23.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

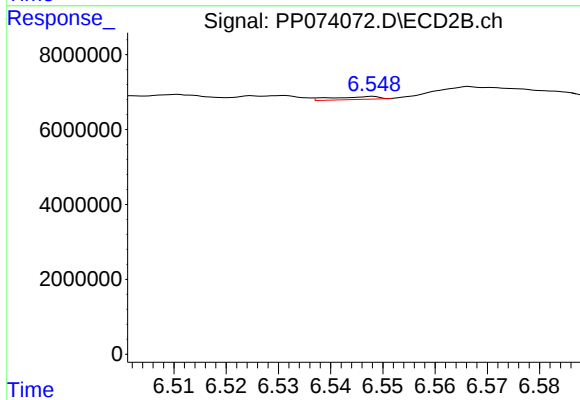


#29 AR-1254-4

R.T.: 6.548 min
Delta R.T.: -0.045 min
Response: 476747
Conc: 0.70 ng/ml

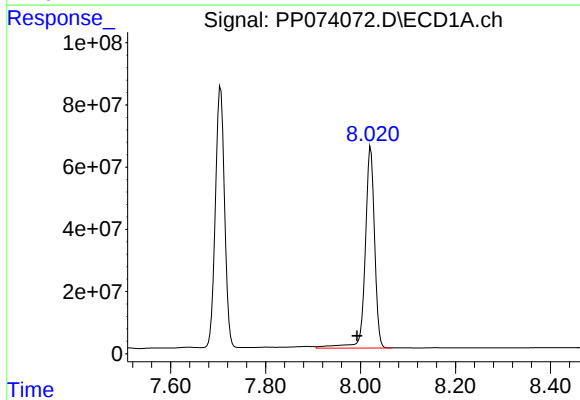


#30 AR-1254-5

R.T.: 8.021 min
Delta R.T.: 0.029 min
Response: 895849943
Conc: 14826.74 ng/ml

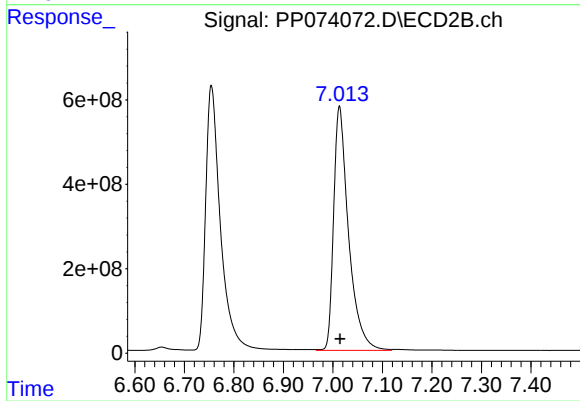

#30 AR-1254-5


R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 12113165638
Conc: 15125.20 ng/ml

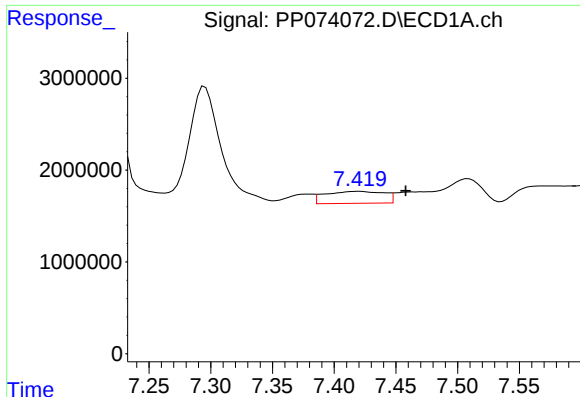

#31 AR-1260-1


R.T.: 7.420 min
Delta R.T.: -0.038 min
Response: 4306288
Conc: 100.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

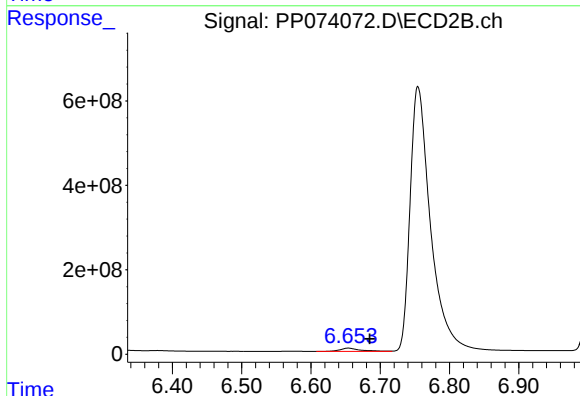


#31 AR-1260-1

R.T.: 6.654 min
Delta R.T.: -0.031 min
Response: 157372193
Conc: 200.77 ng/ml

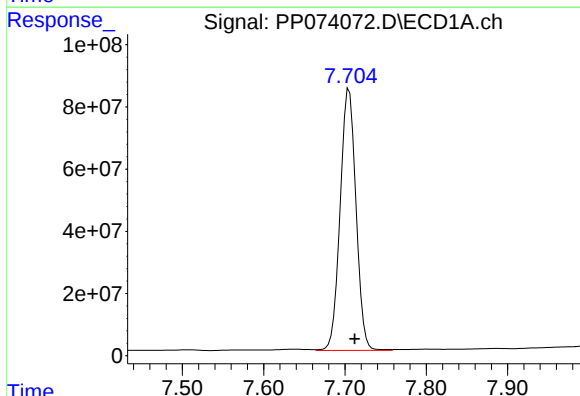


#32 AR-1260-2

R.T.: 7.705 min
Delta R.T.: -0.007 min
Response: 1138571396
Conc: 20797.99 ng/ml

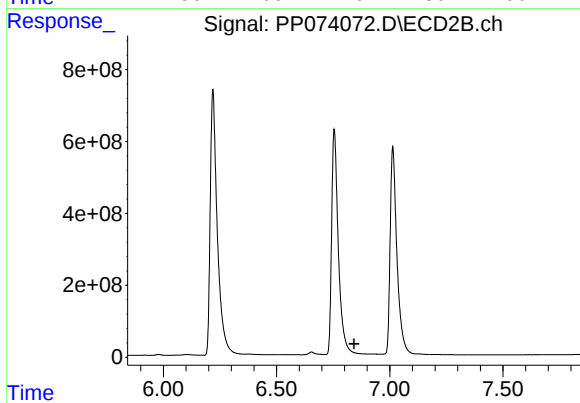

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 6.842 min
Response: 0
Conc: N.D.

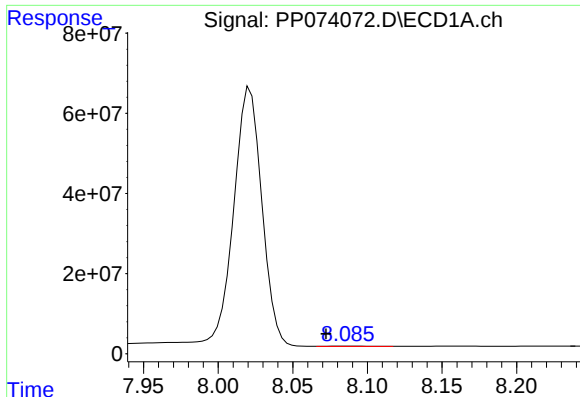

#33 AR-1260-3


R.T.: 8.086 min
Delta R.T.: 0.014 min
Response: 1789367
Conc: 47.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

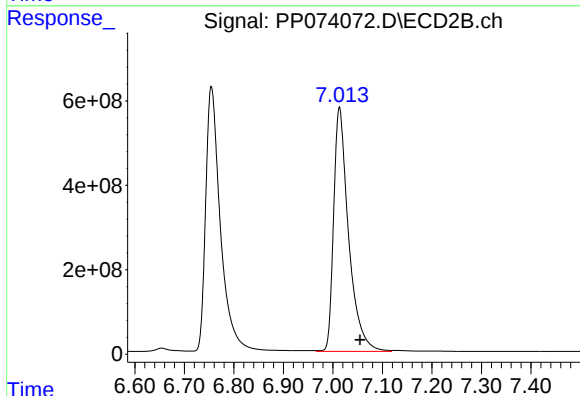


#33 AR-1260-3

R.T.: 7.013 min
Delta R.T.: -0.041 min
Response: 12113165638
Conc: 15245.08 ng/ml

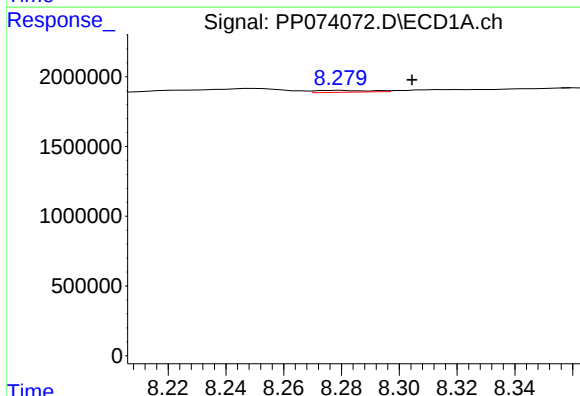


#34 AR-1260-4

R.T.: 8.280 min
Delta R.T.: -0.025 min
Response: 179265
Conc: 3.75 ng/ml

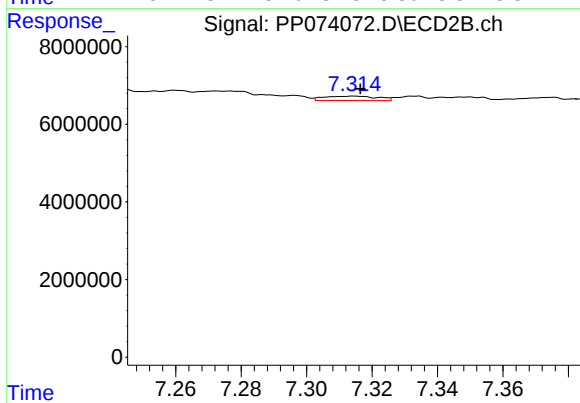

#34 AR-1260-4


R.T.: 7.314 min
Delta R.T.: -0.002 min
Response: 1276101
Conc: 2.22 ng/ml

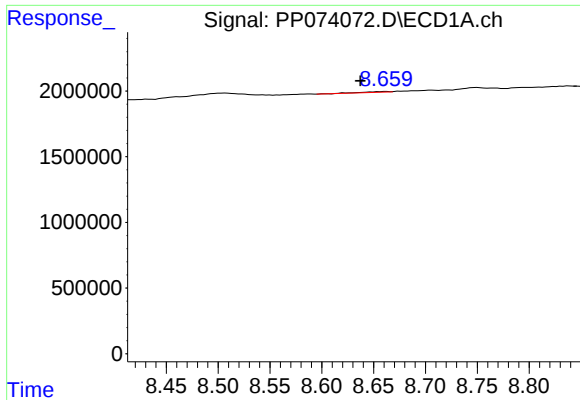

#35 AR-1260-5


R.T.: 8.662 min
Delta R.T.: 0.024 min
Response: 81653
Conc: 0.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

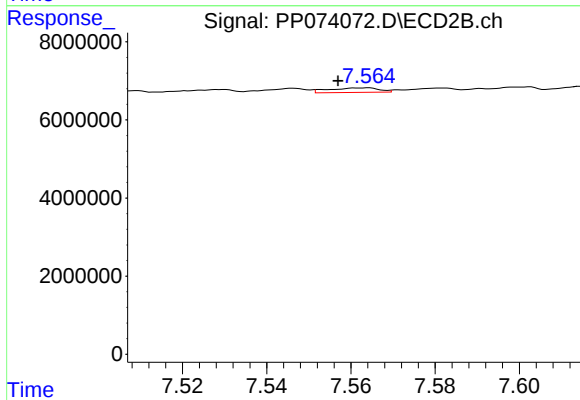


#35 AR-1260-5

R.T.: 7.563 min
Delta R.T.: 0.006 min
Response: 961121
Conc: 0.62 ng/ml

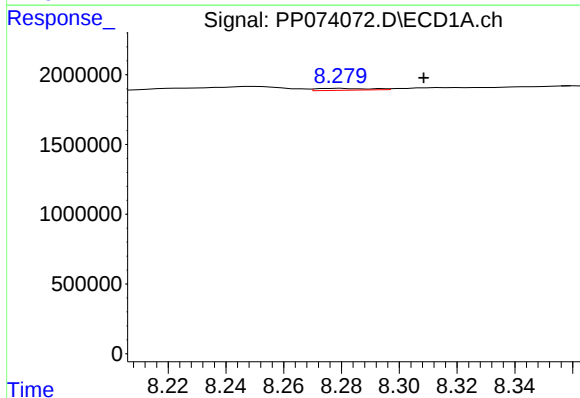


#36 AR-1262-1

R.T.: 8.280 min
Delta R.T.: -0.029 min
Response: 179265
Conc: 2.89 ng/ml

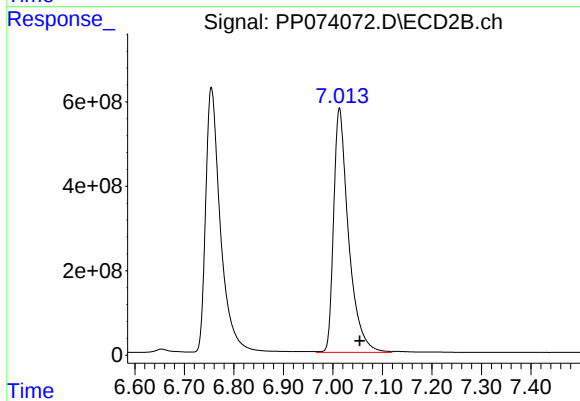

#36 AR-1262-1


R.T.: 7.013 min
Delta R.T.: -0.041 min
Response: 12113165638
Conc: 10236.21 ng/ml

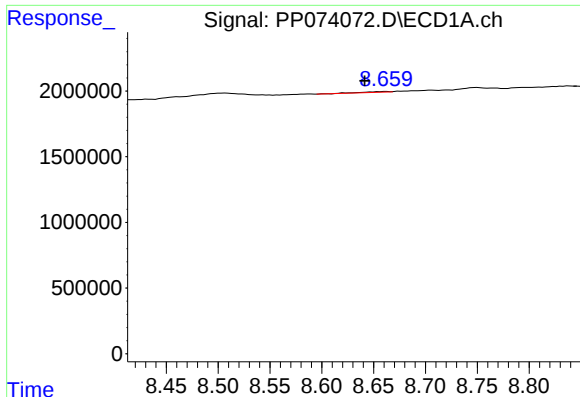

#37 AR-1262-2


R.T.: 8.662 min
Delta R.T.: 0.020 min
Response: 81653
Conc: 0.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

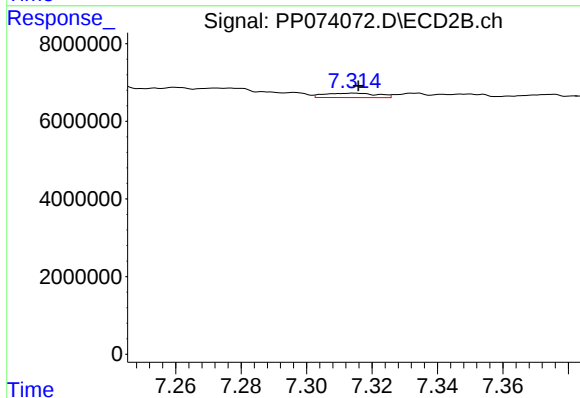


#37 AR-1262-2

R.T.: 7.314 min
Delta R.T.: -0.001 min
Response: 1276101
Conc: 1.52 ng/ml

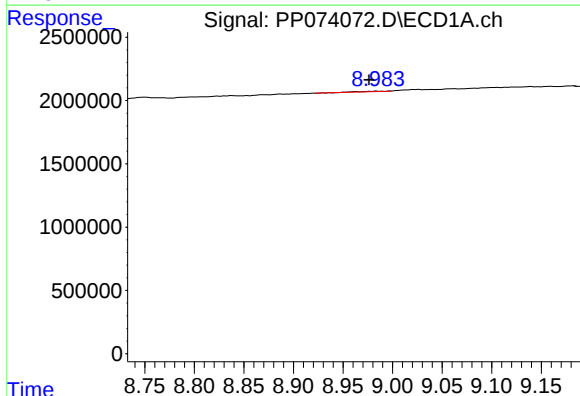


#38 AR-1262-3

R.T.: 8.984 min
Delta R.T.: 0.008 min
Response: 61437
Conc: 0.80 ng/ml

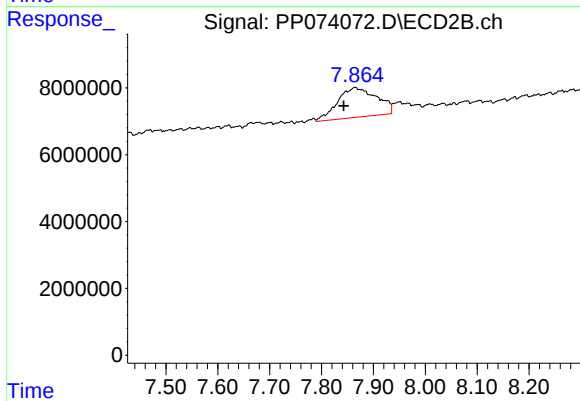

#38 AR-1262-3


R.T.: 7.865 min
Delta R.T.: 0.022 min
Response: 46492782
Conc: 60.24 ng/ml

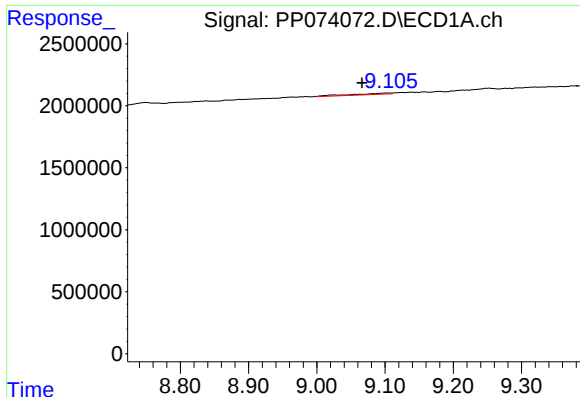

#39 AR-1262-4


R.T.: 9.105 min
Delta R.T.: 0.039 min
Response: 402231
Conc: 7.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

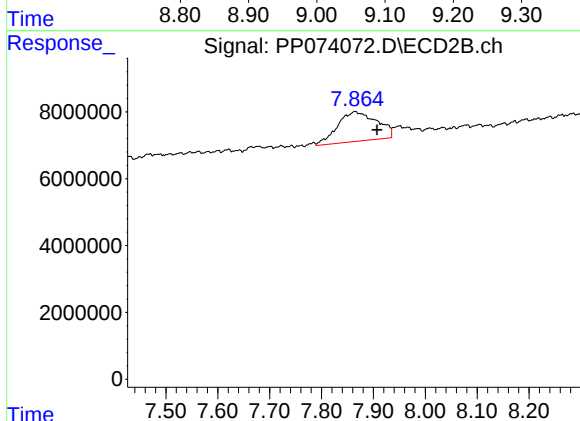


#39 AR-1262-4

R.T.: 7.865 min
Delta R.T.: -0.042 min
Response: 46492782
Conc: 33.01 ng/ml

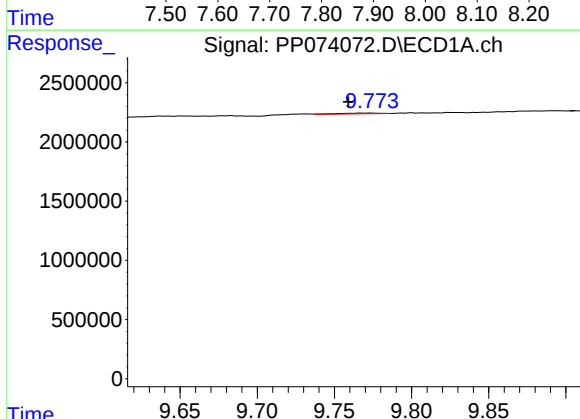


#40 AR-1262-5

R.T.: 9.775 min
Delta R.T.: 0.016 min
Response: 117483
Conc: 3.02 ng/ml

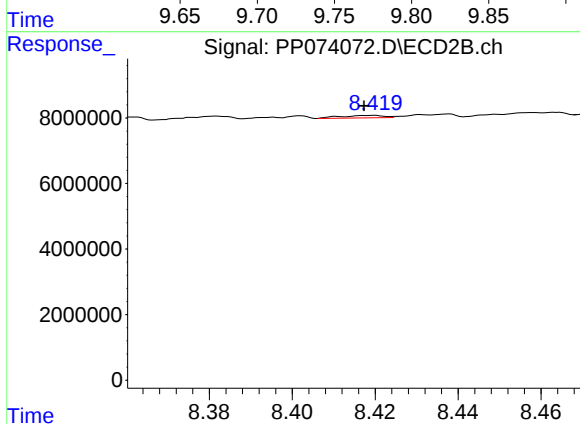

#40 AR-1262-5


R.T.: 8.419 min
Delta R.T.: 0.002 min
Response: 555862
Conc: 0.88 ng/ml

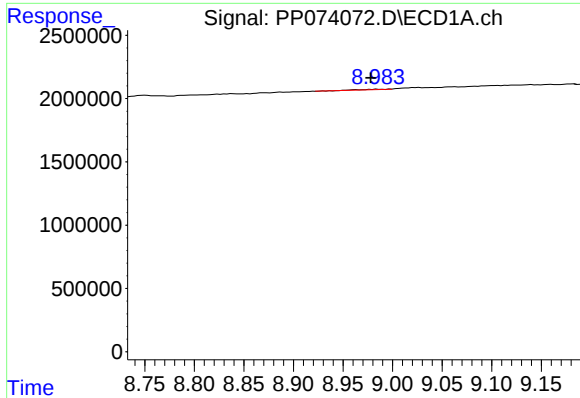

#41 AR-1268-1


R.T.: 8.984 min
Delta R.T.: 0.006 min
Response: 61437
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

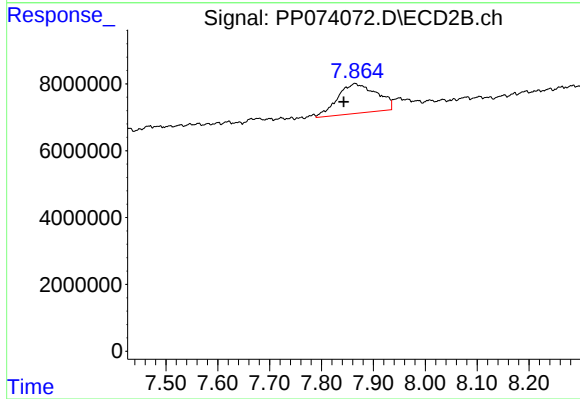


#41 AR-1268-1

R.T.: 7.865 min
Delta R.T.: 0.022 min
Response: 46492782
Conc: 20.79 ng/ml

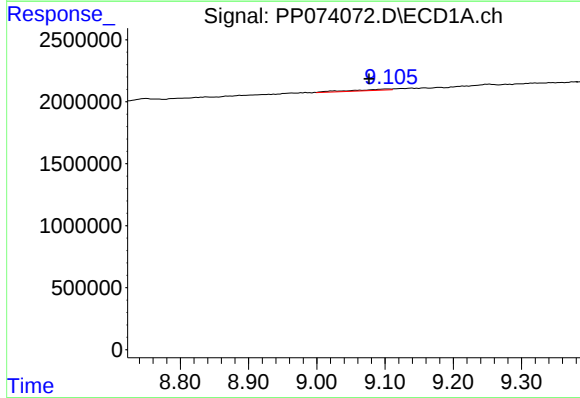


#42 AR-1268-2

R.T.: 9.105 min
Delta R.T.: 0.029 min
Response: 402231
Conc: 3.44 ng/ml

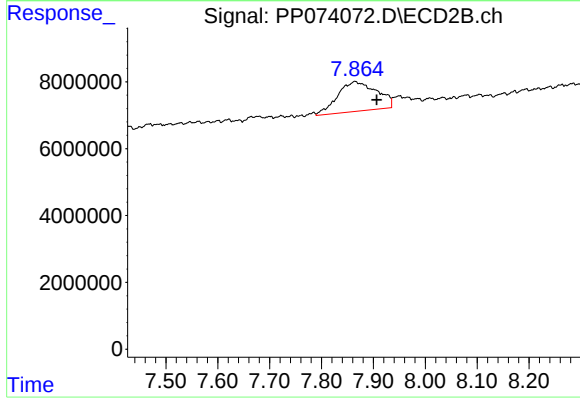

#42 AR-1268-2


R.T.: 7.865 min
Delta R.T.: -0.042 min
Response: 46492782
Conc: 21.48 ng/ml

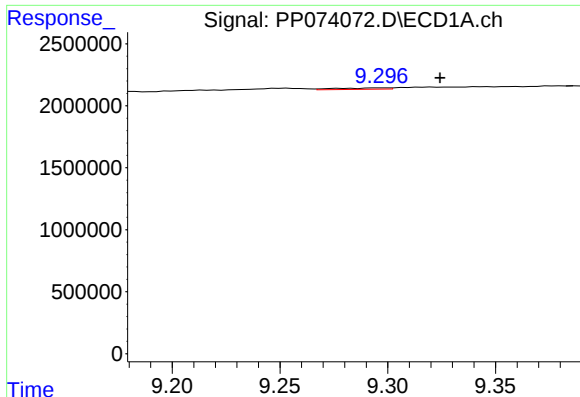

#43 AR-1268-3


R.T.: 9.298 min
Delta R.T.: -0.027 min
Response: 191911
Conc: 1.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

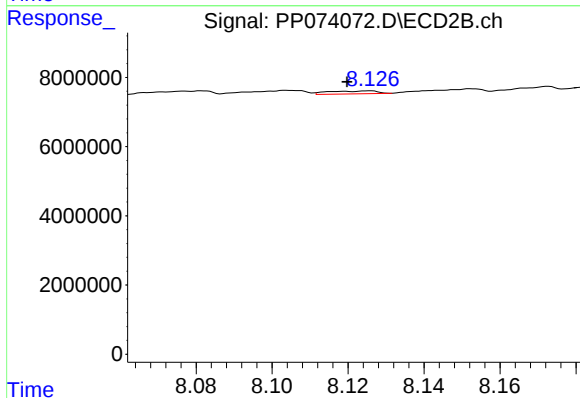


#43 AR-1268-3

R.T.: 8.125 min
Delta R.T.: 0.006 min
Response: 741246
Conc: 0.46 ng/ml

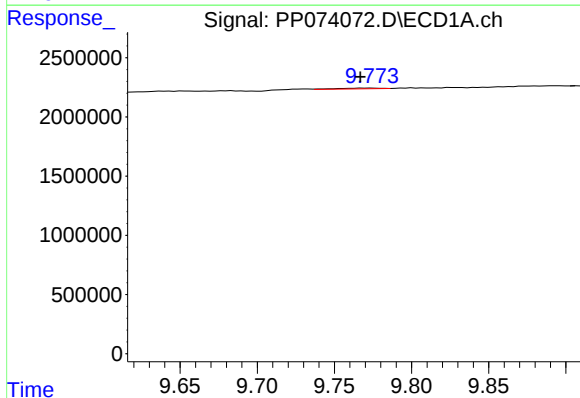


#44 AR-1268-4

R.T.: 9.775 min
Delta R.T.: 0.008 min
Response: 117483
Conc: 2.71 ng/ml

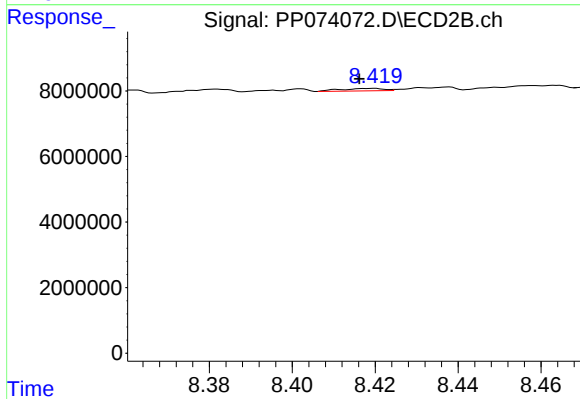

#44 AR-1268-4


R.T.: 8.419 min
Delta R.T.: 0.003 min
Response: 555862
Conc: 0.84 ng/ml

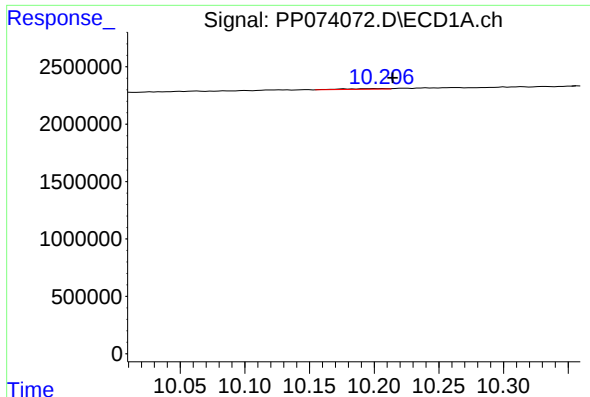

#45 AR-1268-5

R.T.: 10.208 min
Delta R.T.: -0.007 min
Response: 127550
Conc: 0.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

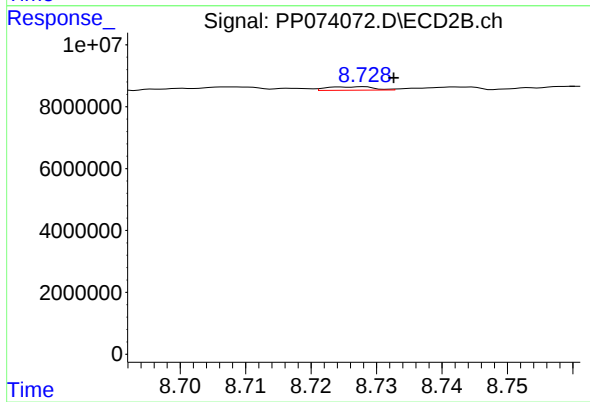

#45 AR-1268-5

R.T.: 8.727 min
Delta R.T.: -0.006 min
Response: 575845
Conc: 0.11 ng/ml