

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072621\
 Data File : PP037689.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jul 2021 20:38
 Operator : DD\AJ
 Sample : M3193-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 01-A-01-B-01-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 04:51:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.956	3.947	1185704	674986	26.088	24.667
2) SA Decachlor...	10.984	9.237	1250043	599490	27.154m	21.537

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072621\
Data File : PP037689.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jul 2021 20:38
Operator : DD\AJ
Sample : M3193-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 04:51:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

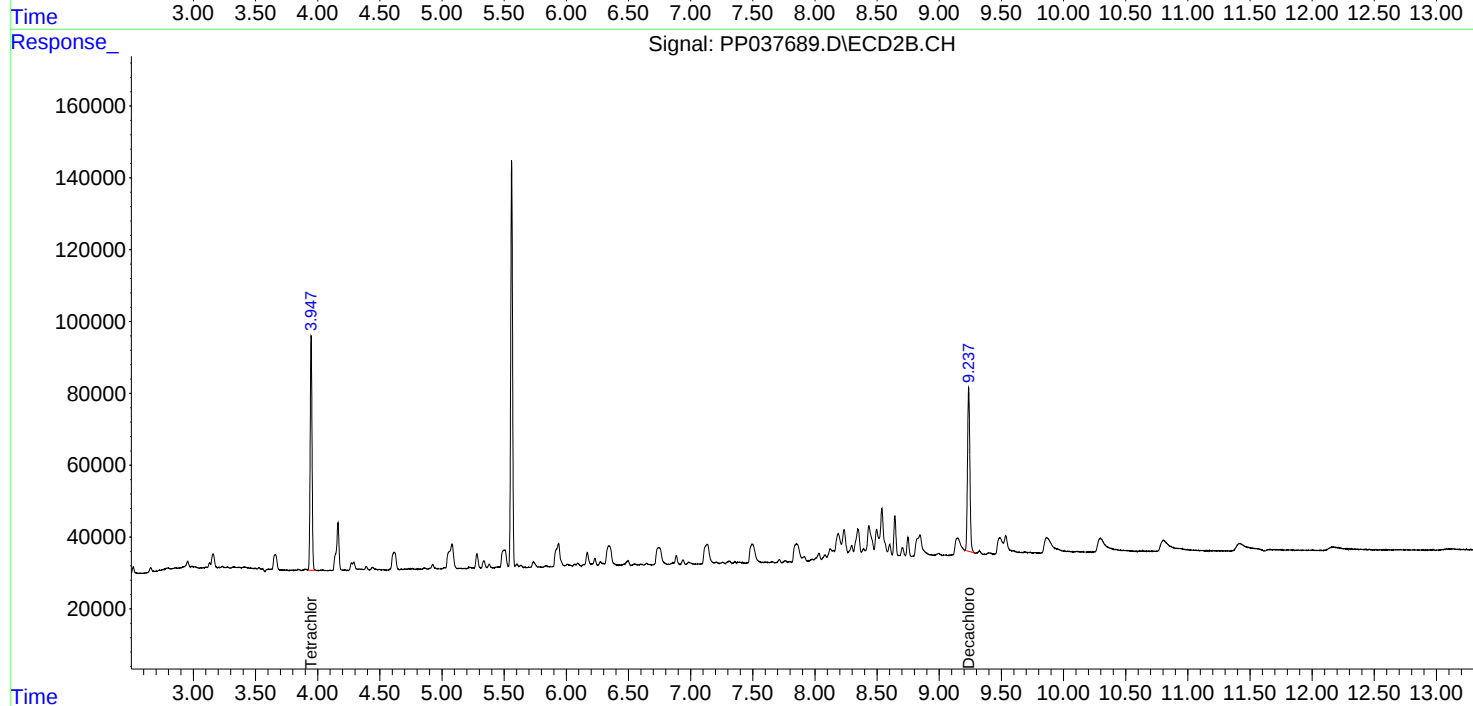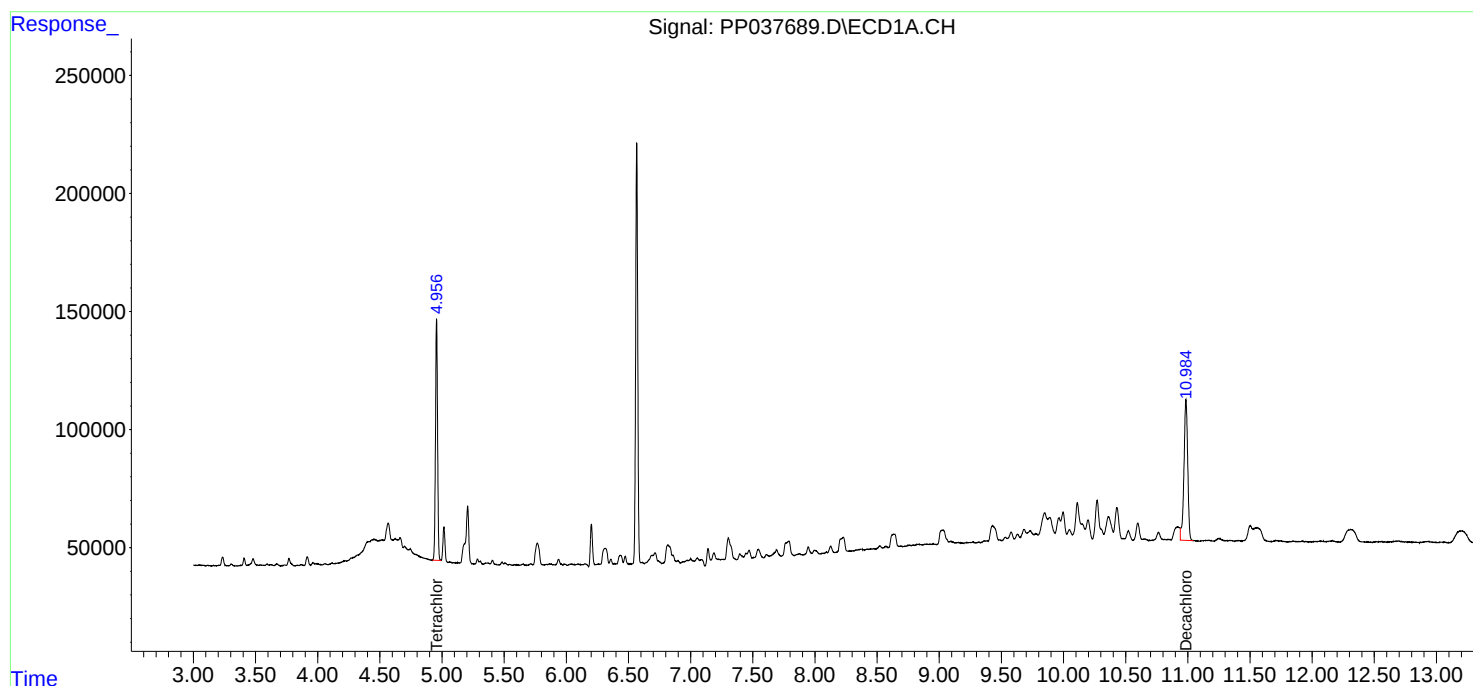


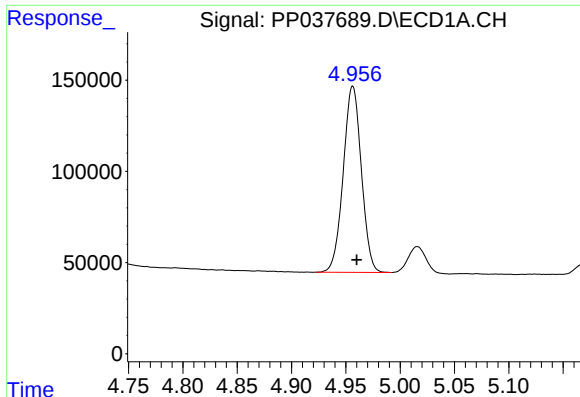

#1 Tetrachloro-m-xylene


R.T.: 4.956 min
Delta R.T.: -0.004 min
Response: 1185704
Conc: 26.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C

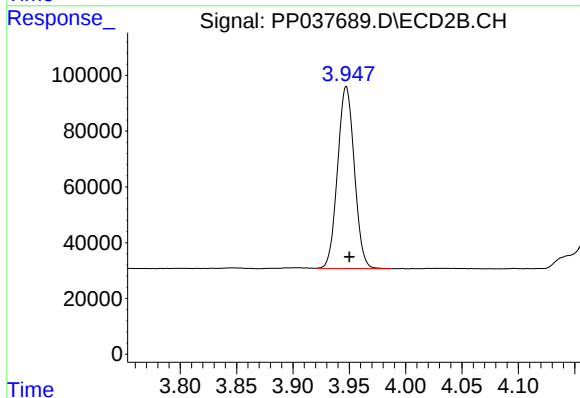


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.003 min
Response: 674986
Conc: 24.67 ng/ml

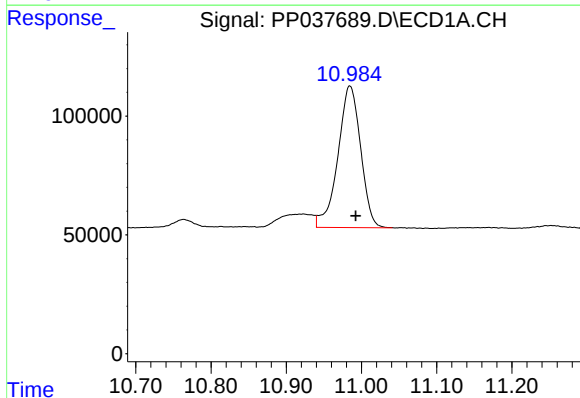

#2 Decachlorobiphenyl

R.T.: 10.984 min
Delta R.T.: -0.008 min
Response: 1250043
Conc: 27.15 ng/ml m

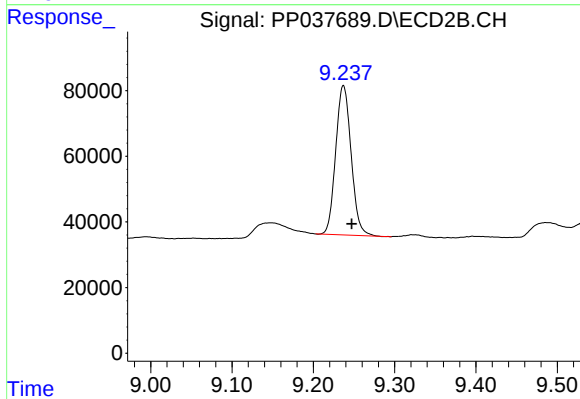

#2 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: -0.010 min
Response: 599490
Conc: 21.54 ng/ml