

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072623\
 Data File : PP058973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2023 20:43
 Operator : YP\AJ
 Sample : PB154458BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB154458BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/27/2023
 Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 03:11:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 22 02:26:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.663	28069140	41589803	20.389	21.627
2) SA Decachlor...	10.221	8.704	23732932	37942146	27.549	26.815m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072623\
Data File : PP058973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2023 20:43
Operator : YP\AJ
Sample : PB154458BL
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB154458BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 03:11:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 22 02:26:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

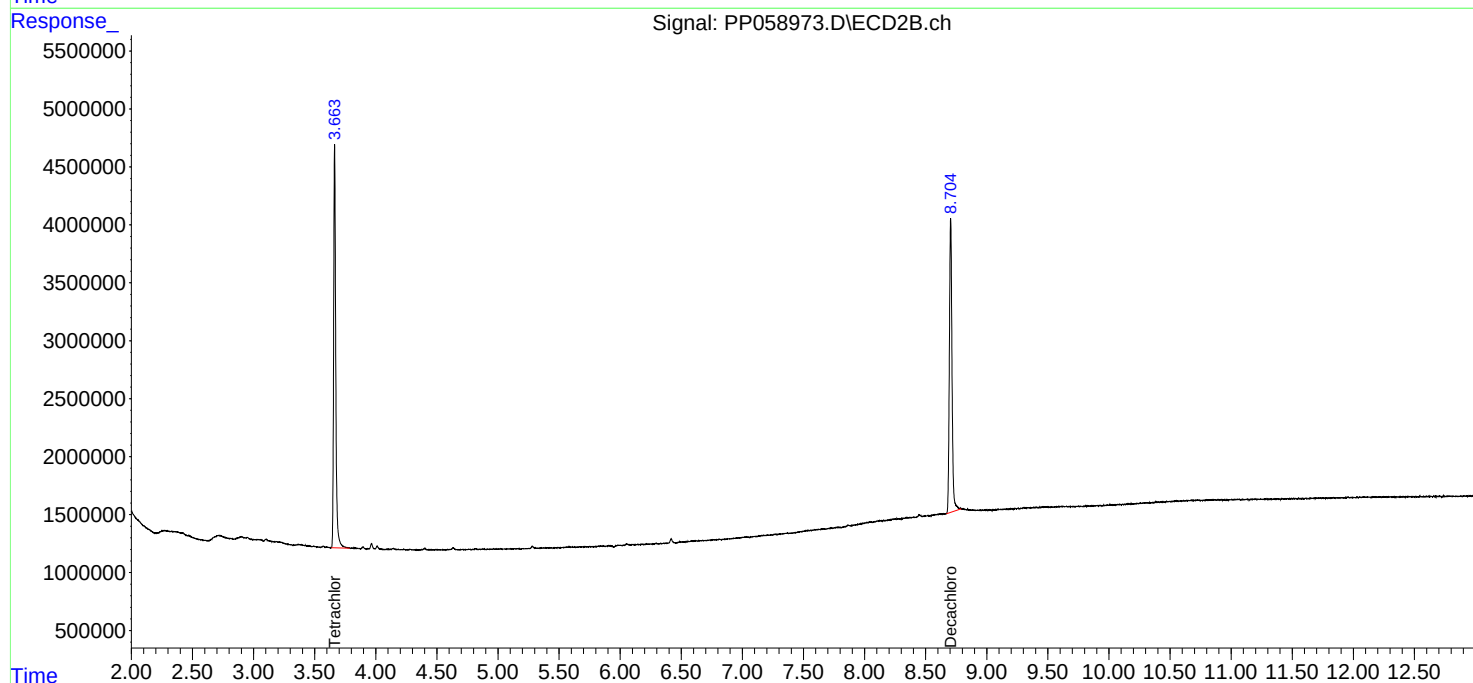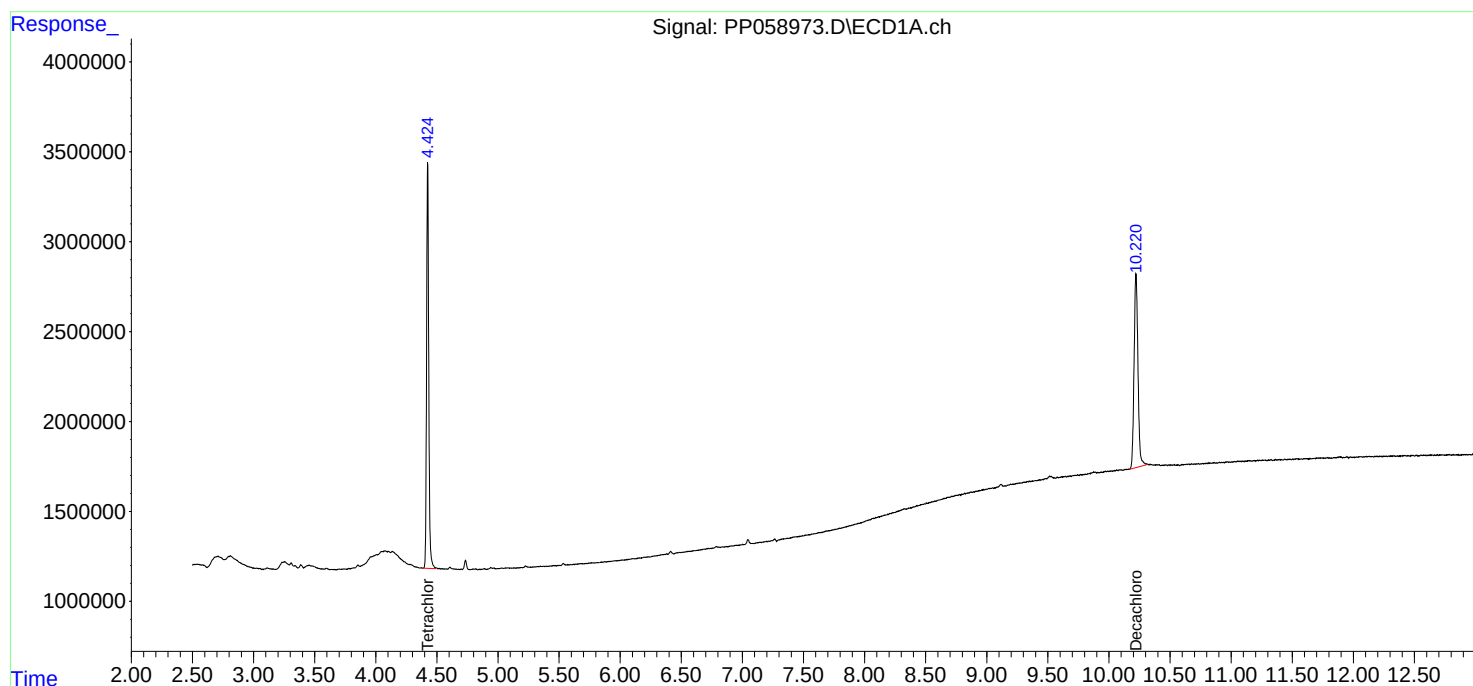

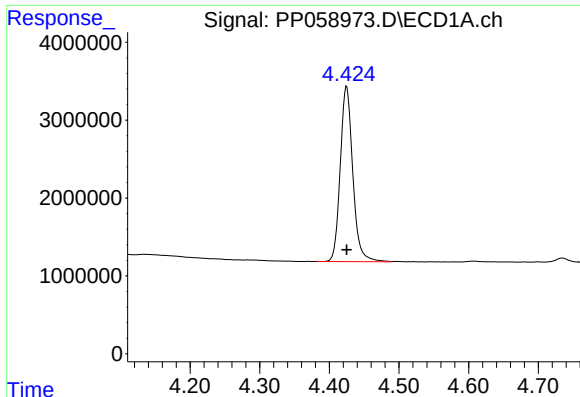


#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: 0.000 min
Response: 28069140
Conc: 20.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB154458BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

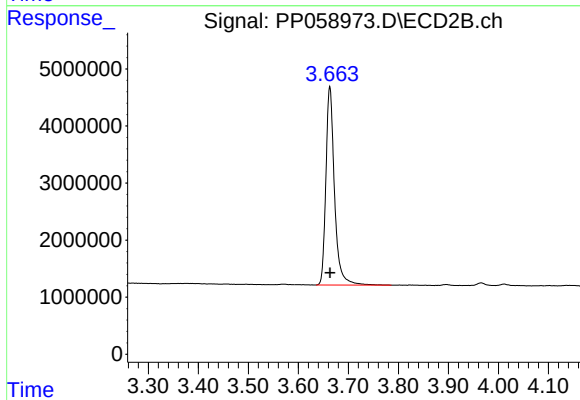


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 41589803
Conc: 21.63 ng/ml

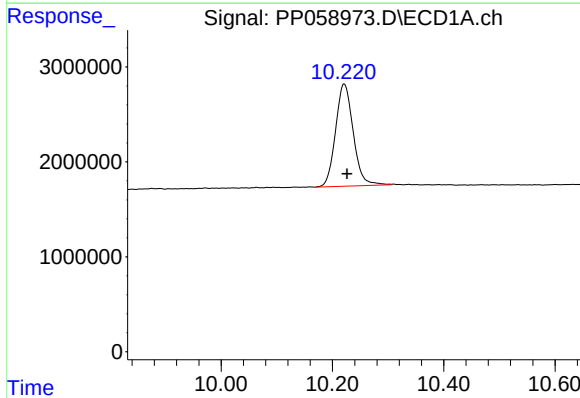

#2 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.005 min
Response: 23732932
Conc: 27.55 ng/ml

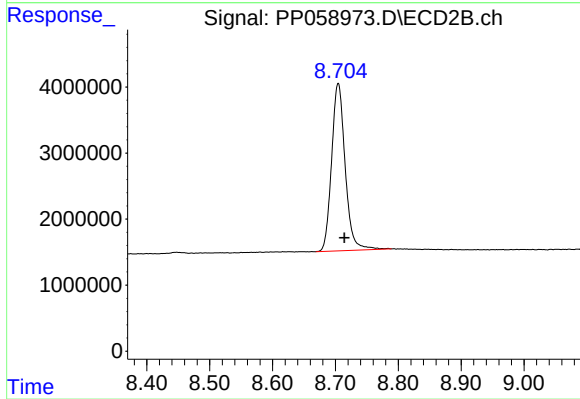

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: -0.010 min
Response: 37942146
Conc: 26.82 ng/ml m