

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072623\
 Data File : PP058993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2023 03:41
 Operator : YP\AJ
 Sample : 03769-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B-P14B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/27/2023
 Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 05:57:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 22 02:26:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.661	26036413	38643517	18.912	20.094
2) SA Decachlor...	10.217	8.703	19150914	28538720	22.230	20.170m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072623\
Data File : PP058993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2023 03:41
Operator : YP\AJ
Sample : 03769-04
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
B-P14B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 05:57:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 22 02:26:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

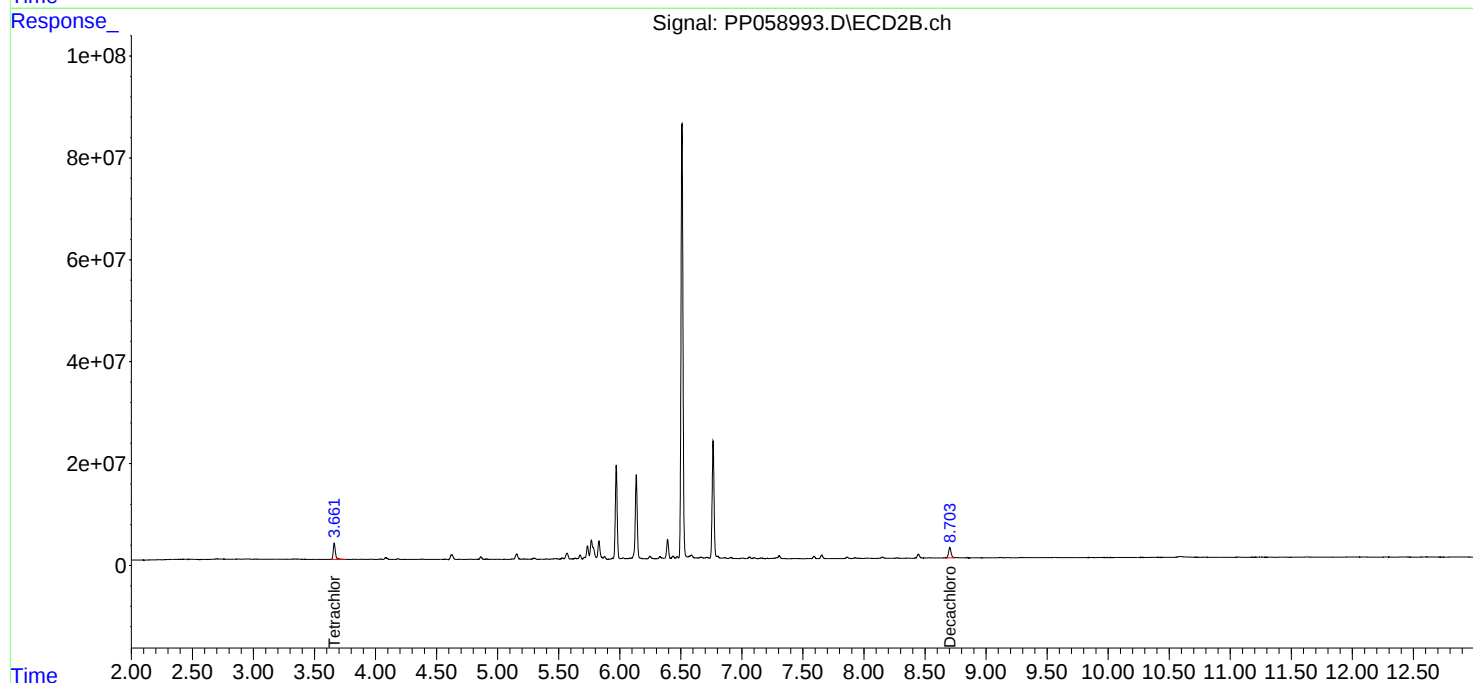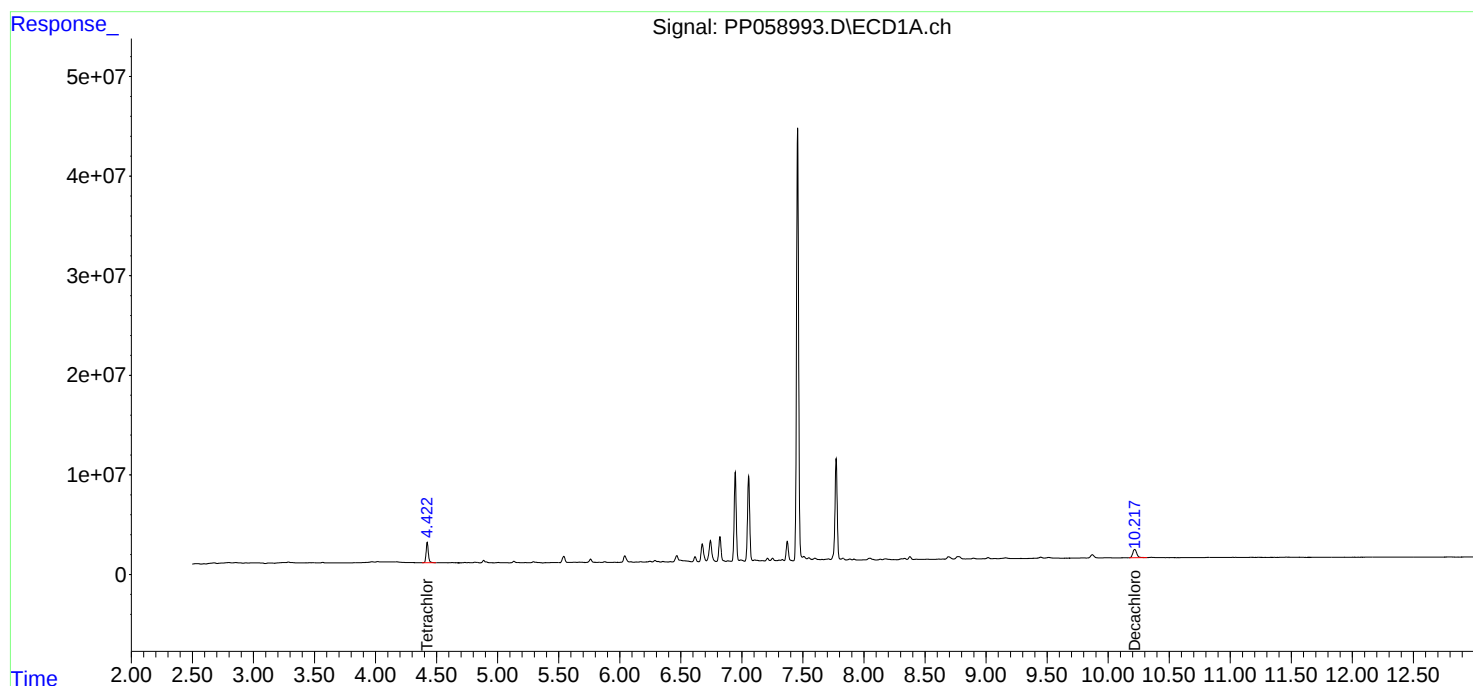

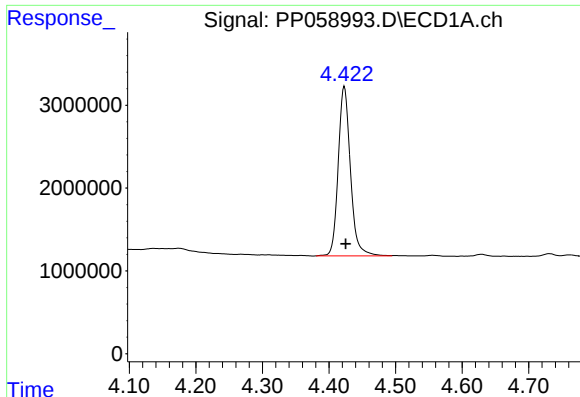


#1 Tetrachloro-m-xylene

R.T.: 4.423 min
Delta R.T.: -0.002 min
Response: 26036413
Conc: 18.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
B-P14B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

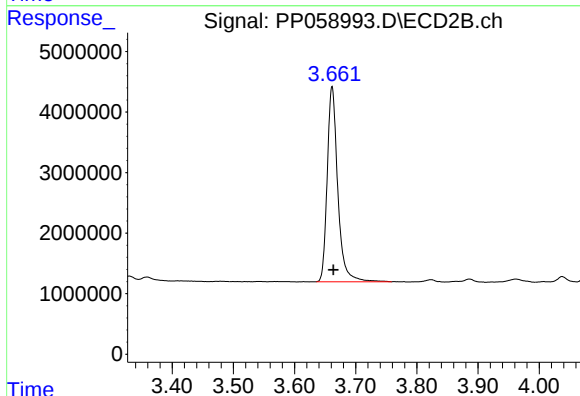


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: -0.002 min
Response: 38643517
Conc: 20.09 ng/ml

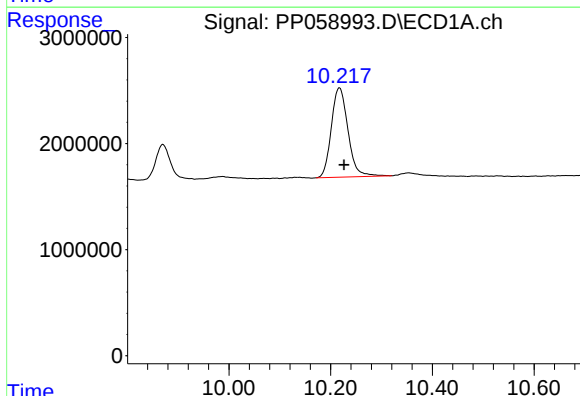

#2 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.009 min
Response: 19150914
Conc: 22.23 ng/ml

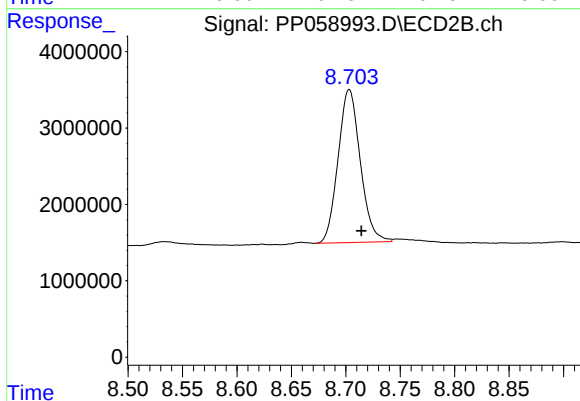

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: -0.012 min
Response: 28538720
Conc: 20.17 ng/ml m