

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072623\
 Data File : PP059006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2023 07:12
 Operator : YP\AJ
 Sample : 03769-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B-P31A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/27/2023
 Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 11:46:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 22 02:26:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.662	27084623	41266179	19.674	21.458
2) SA Decachlor...	10.219	8.702	16283386	26215187	18.902	18.527m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072623\
Data File : PP059006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2023 07:12
Operator : YP\AJ
Sample : 03769-13
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
B-P31A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 11:46:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 22 02:26:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

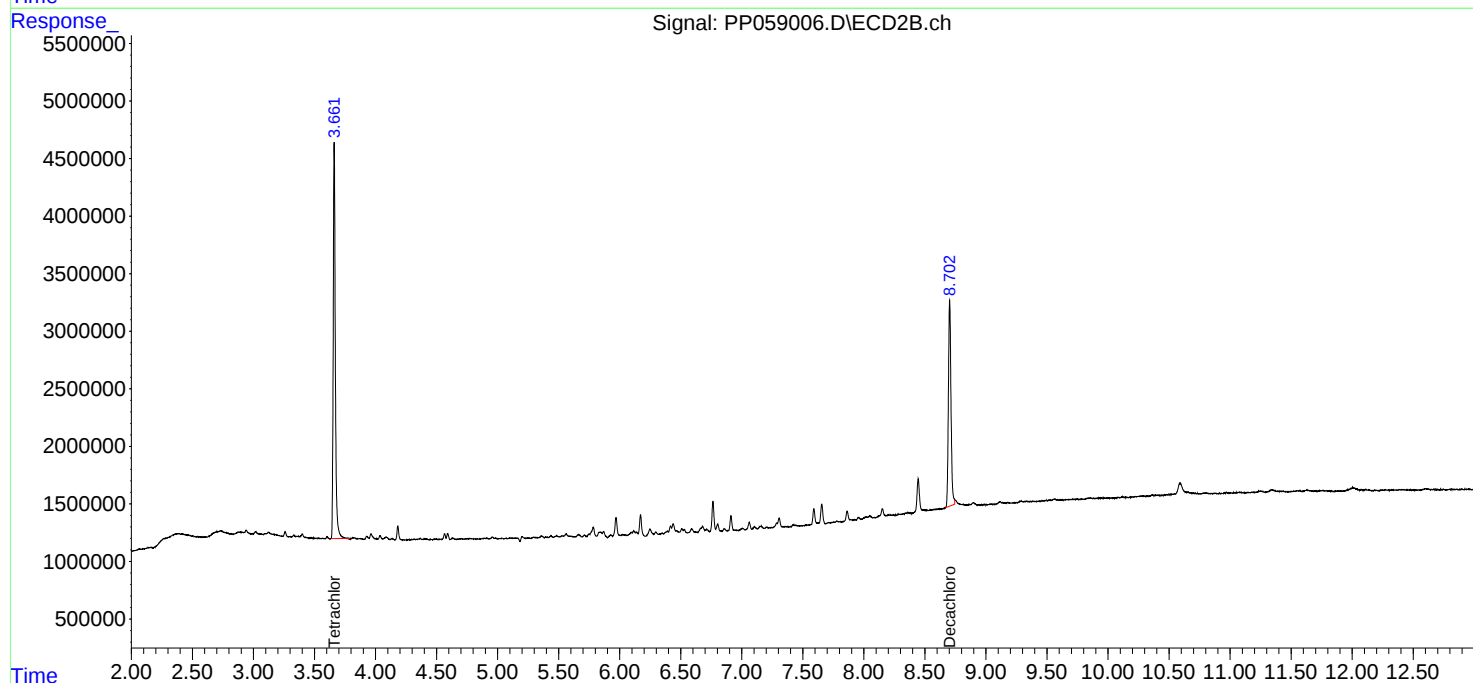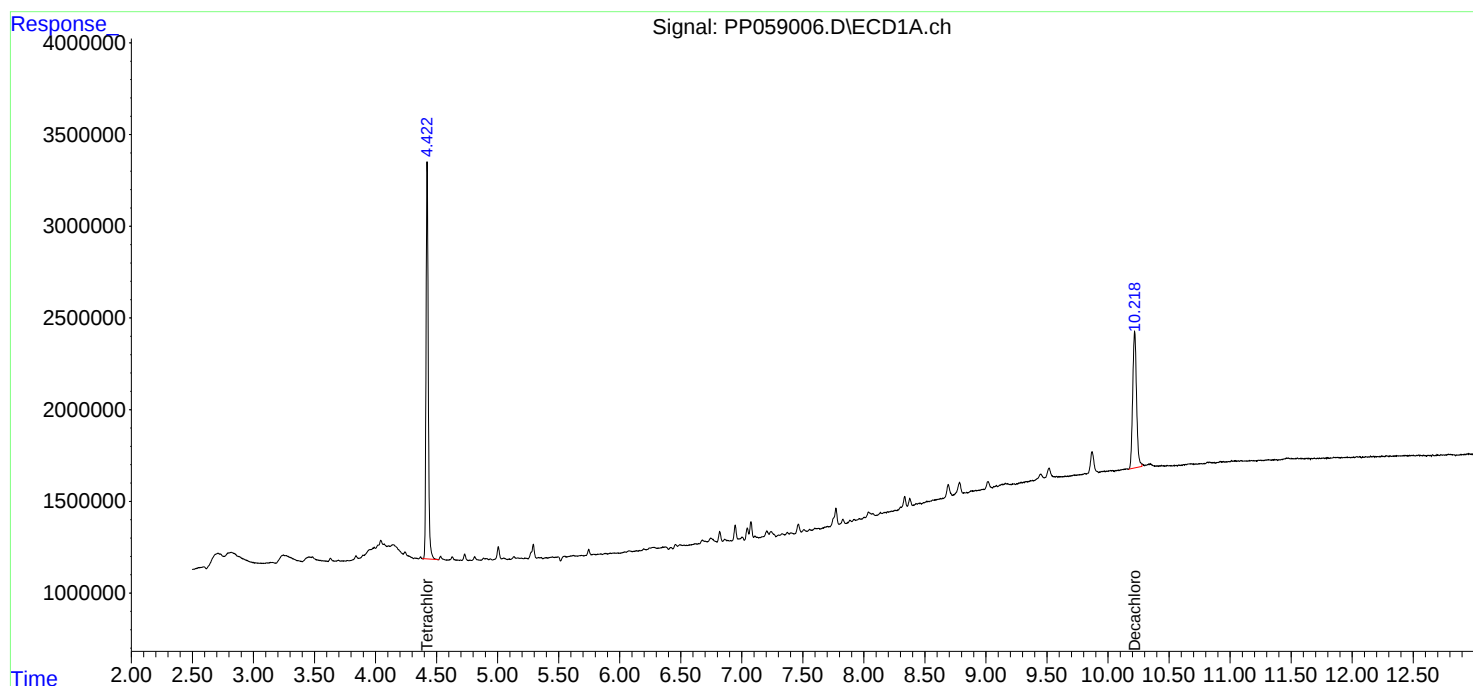

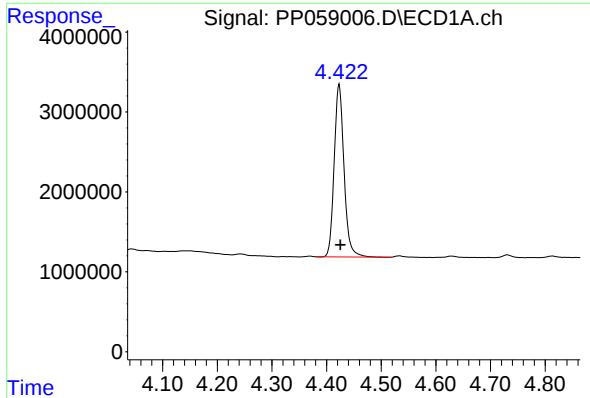

#1 Tetrachloro-m-xylene

R.T.: 4.423 min
Delta R.T.: -0.002 min
Response: 27084623
Conc: 19.67 ng/ml

Instrument :

ECD_P


ClientSampleId :

B-P31A

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

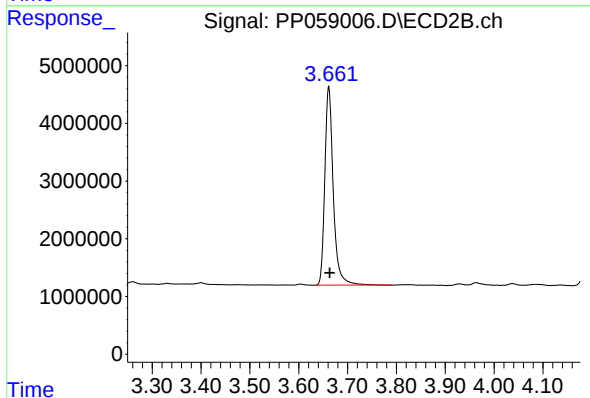


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.002 min
Response: 41266179
Conc: 21.46 ng/ml

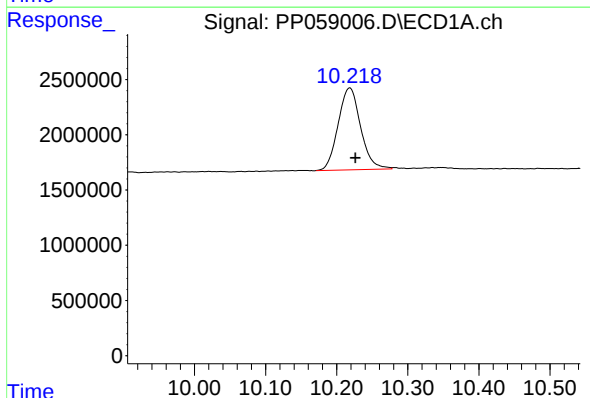

#2 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.008 min
Response: 16283386
Conc: 18.90 ng/ml

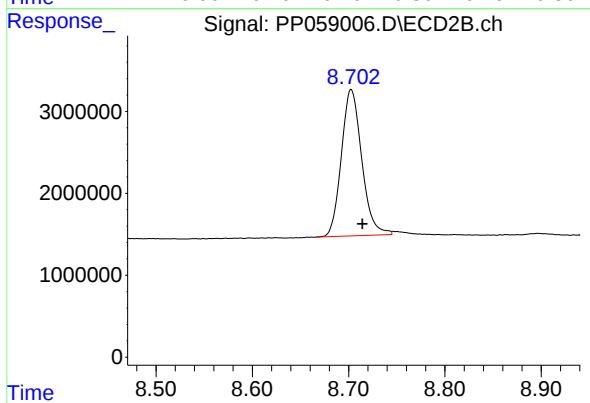

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.012 min
Response: 26215187
Conc: 18.53 ng/ml m