

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072721\
 Data File : PP037726.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jul 2021 15:31
 Operator : DD\AJ
 Sample : M3184-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20210561-COM-34

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 04:32:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.956	3.947	921931	539045	20.285	19.699
2)	SA Decachlor...	10.986	9.236	767286	388401	16.667	13.954

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072721\
Data File : PP037726.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2021 15:31
Operator : DD\AJ
Sample : M3184-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20210561-COM-34

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 04:32:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

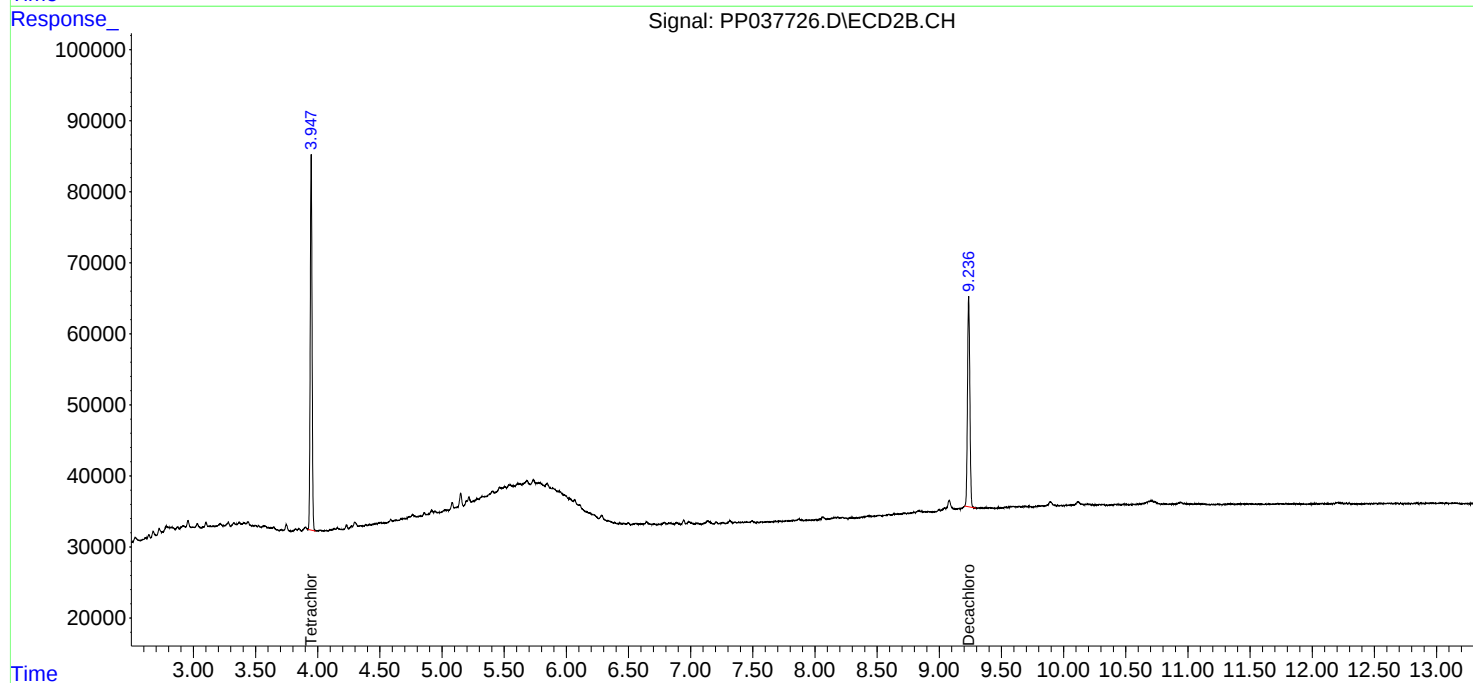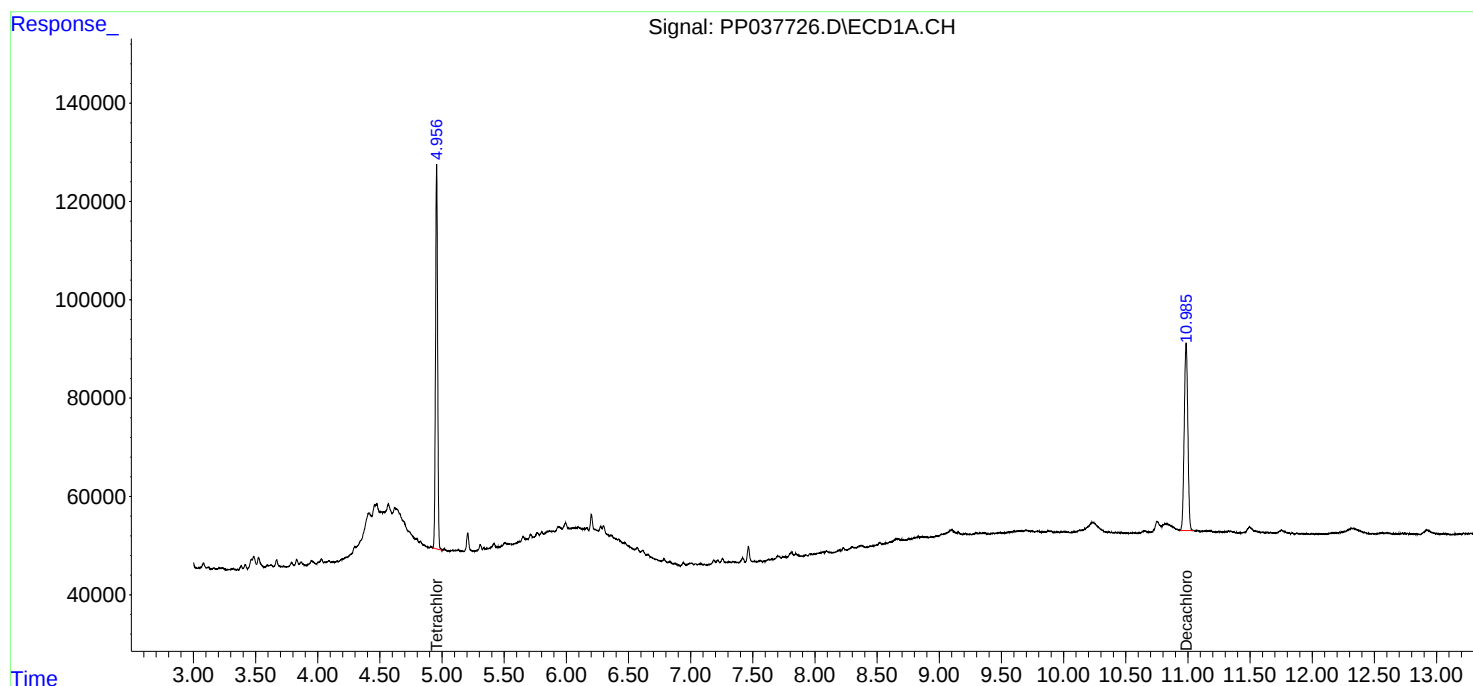


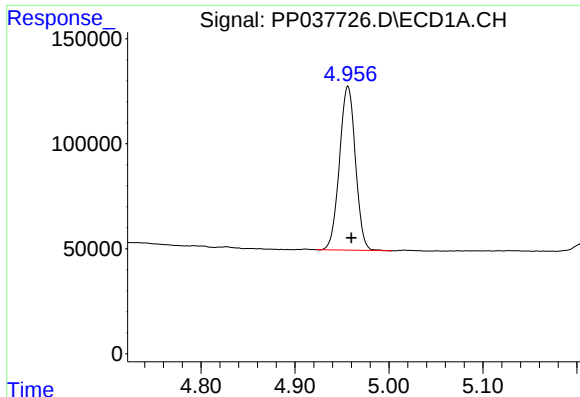

#1 Tetrachloro-m-xylene


R.T.: 4.956 min
Delta R.T.: -0.004 min
Response: 921931
Conc: 20.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
20210561-COM-34

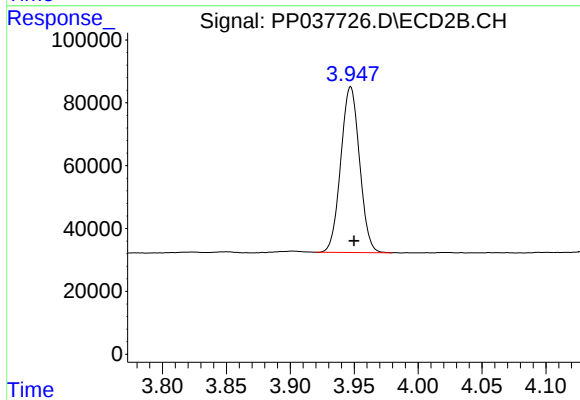


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.003 min
Response: 539045
Conc: 19.70 ng/ml

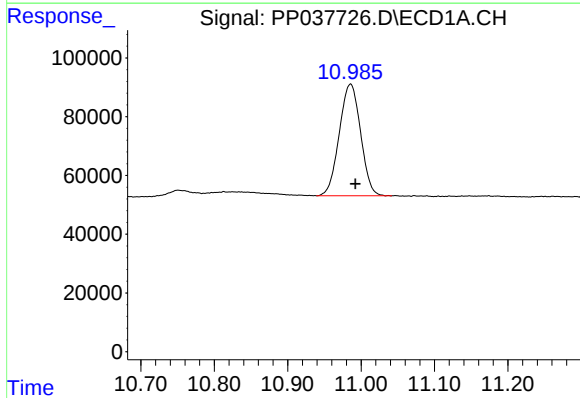

#2 Decachlorobiphenyl

R.T.: 10.986 min
Delta R.T.: -0.007 min
Response: 767286
Conc: 16.67 ng/ml

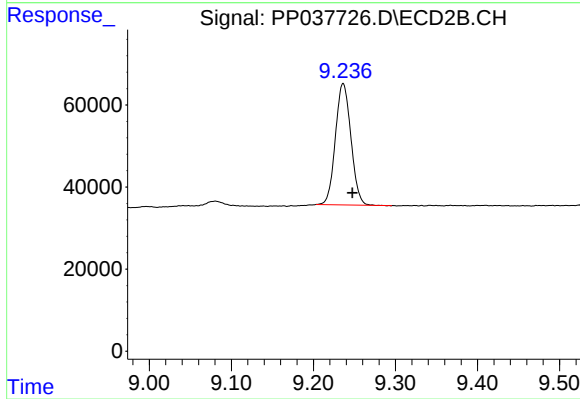

#2 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.011 min
Response: 388401
Conc: 13.95 ng/ml