

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072721\
 Data File : PP037737.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jul 2021 18:39
 Operator : DD\AJ
 Sample : M3199-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HD-02-072621

Manual Integrations
 APPROVED

mohammad
 7/28/2021 2:41:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 04:38:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.956	3.947	851467	515051	18.734m	18.822
2) SA Decachlor...	10.985	9.236	885214	418827	19.229	15.047

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072721\
Data File : PP037737.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2021 18:39
Operator : DD\AJ
Sample : M3199-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HD-02-072621


Manual Integrations
APPROVED

mohammad
7/28/2021 2:41:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 04:38:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

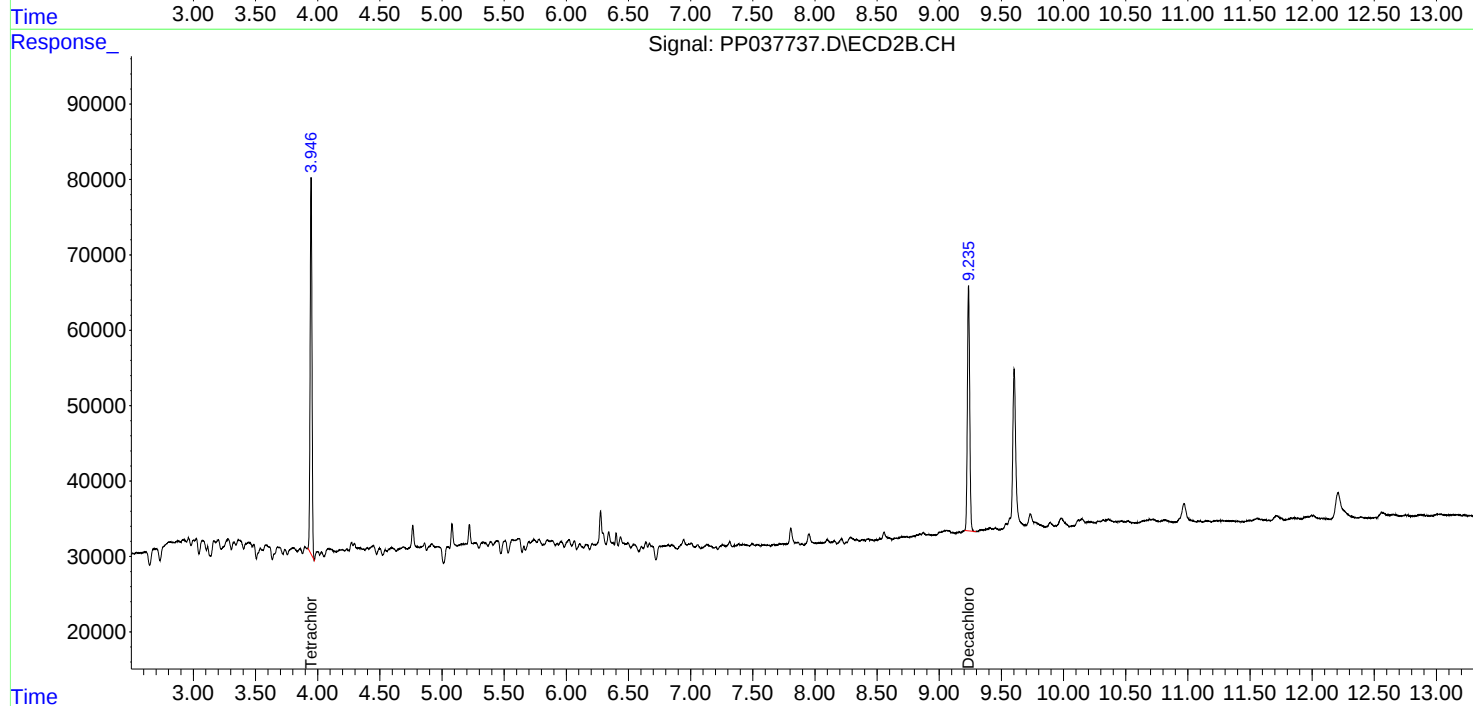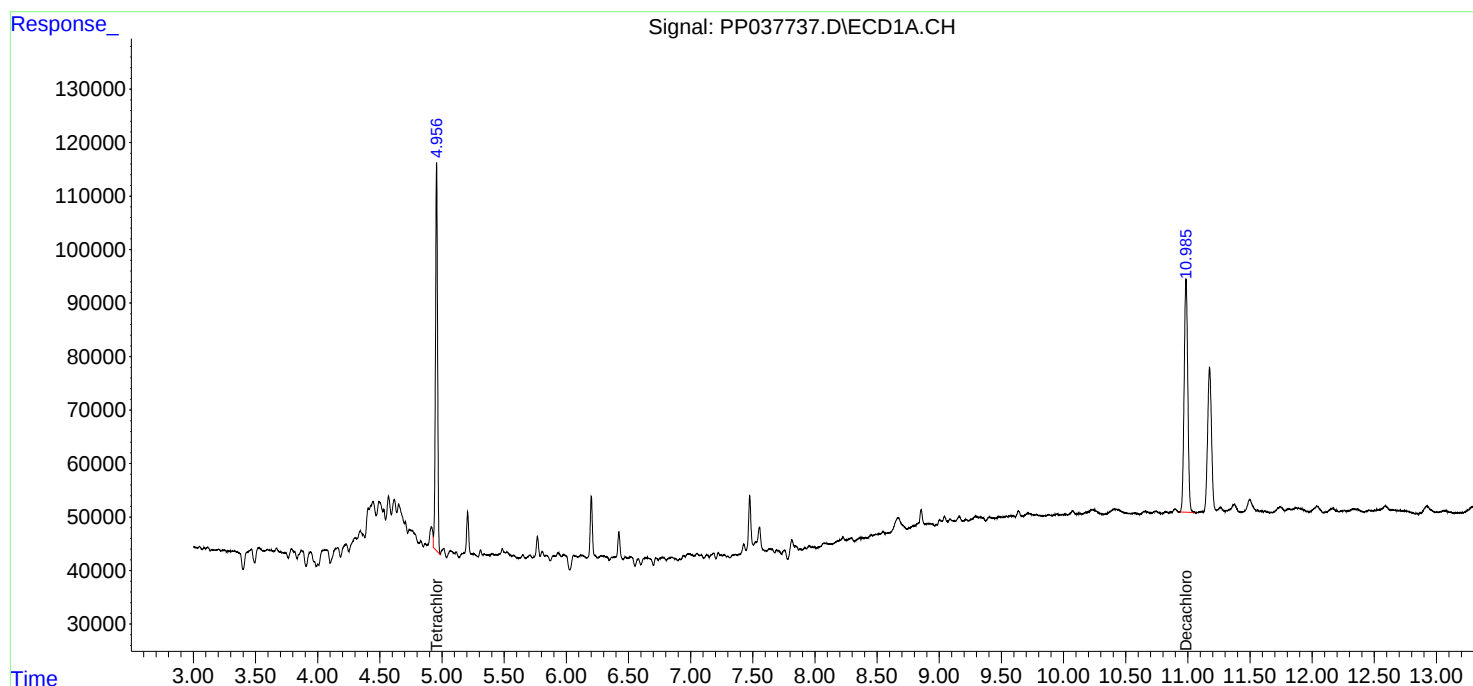

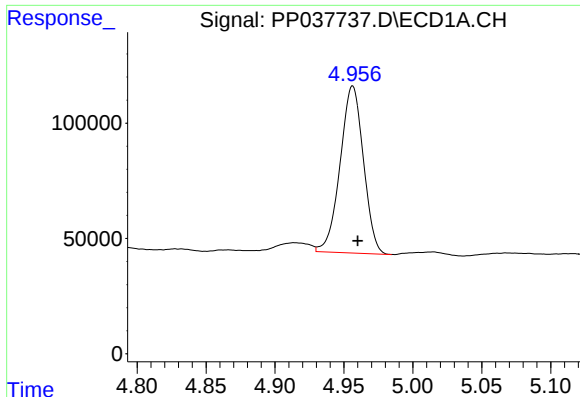


#1 Tetrachloro-m-xylene

R.T.: 4.956 min
Delta R.T.: -0.004 min
Response: 851467
Conc: 18.73 ng/ml m

Instrument :
ECD_P
ClientSampleId :
HD-02-072621


Manual Integrations
APPROVED

mohammad
7/28/2021 2:41:38 PM

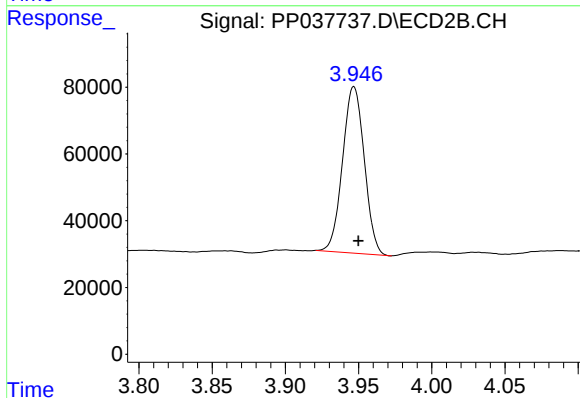


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.003 min
Response: 515051
Conc: 18.82 ng/ml

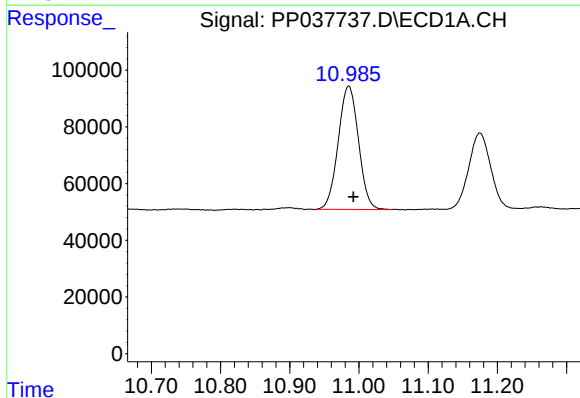

#2 Decachlorobiphenyl

R.T.: 10.985 min
Delta R.T.: -0.007 min
Response: 885214
Conc: 19.23 ng/ml

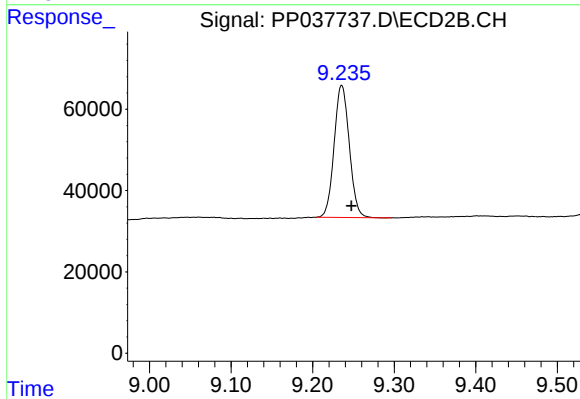

#2 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.012 min
Response: 418827
Conc: 15.05 ng/ml