

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072722\
 Data File : PP049889.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 19:02
 Operator : YP\AJ
 Sample : N3910-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CONCRETE-WALL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 00:24:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.601	31368340	58340550	21.616	23.868
2) SA Decachlor...	10.103	8.566	28867584	24859316	20.410	21.346

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072722\
Data File : PP049889.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 19:02
Operator : YP\AJ
Sample : N3910-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CONCRETE-WALL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 00:24:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

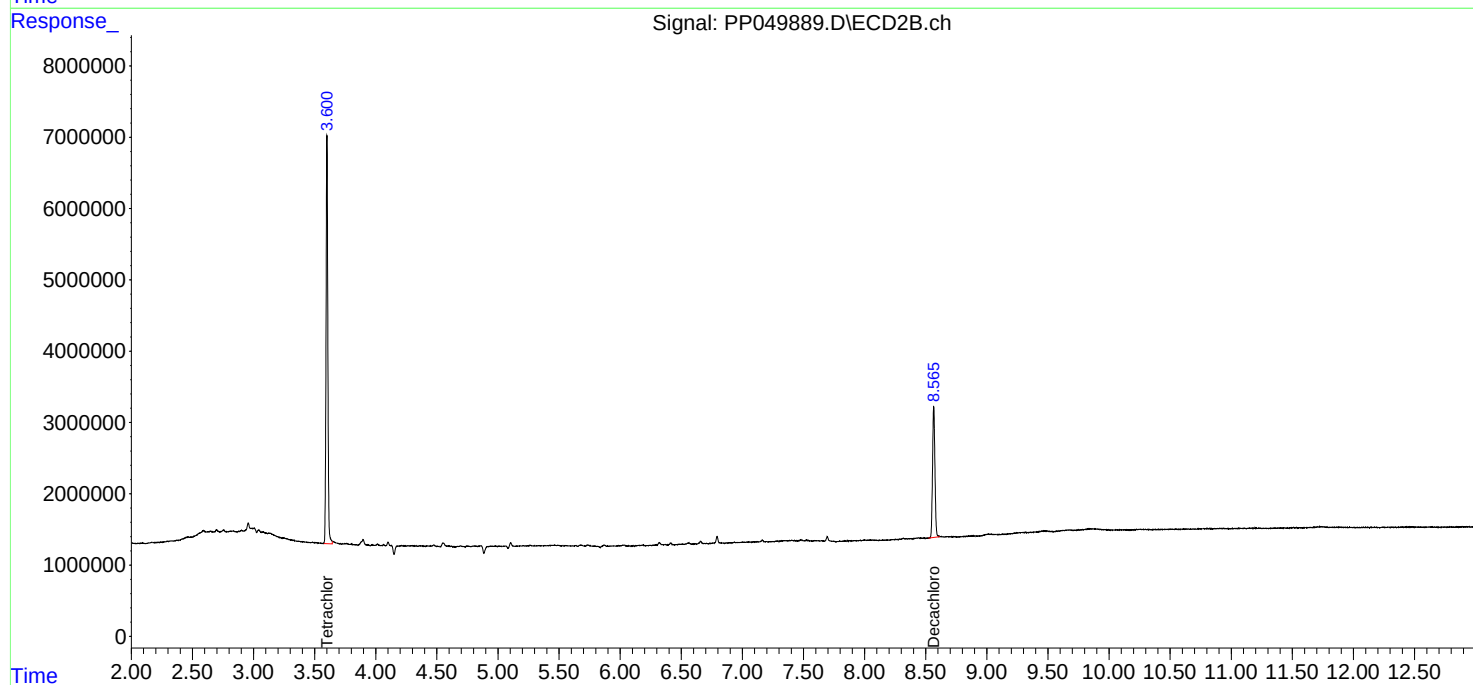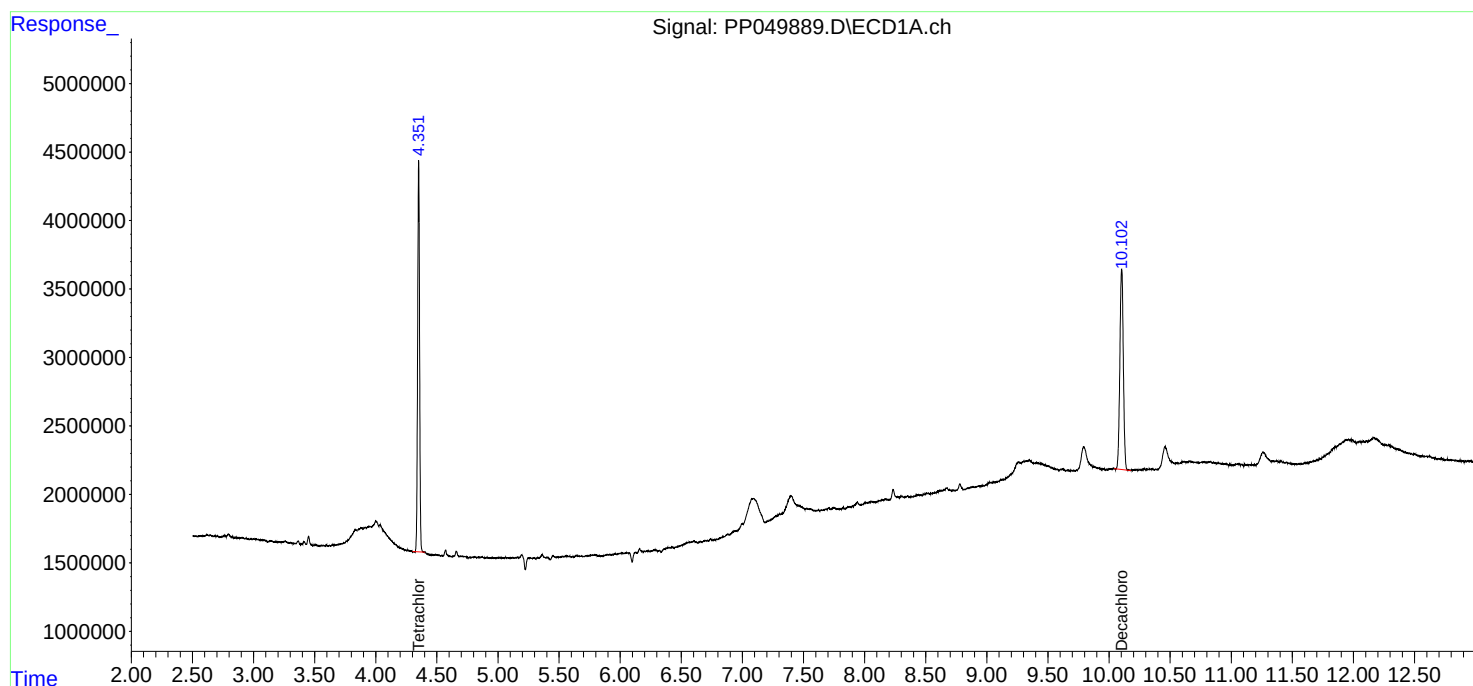


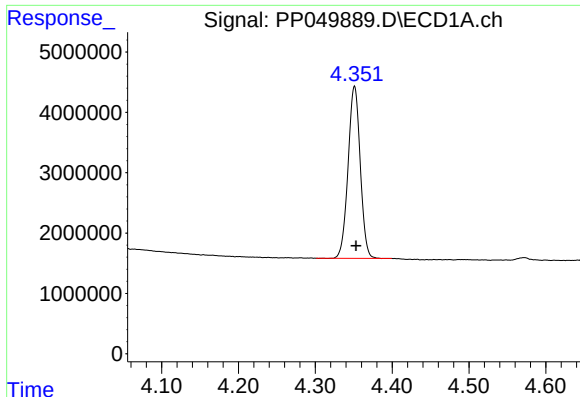

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.002 min
Response: 31368340
Conc: 21.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-WALL

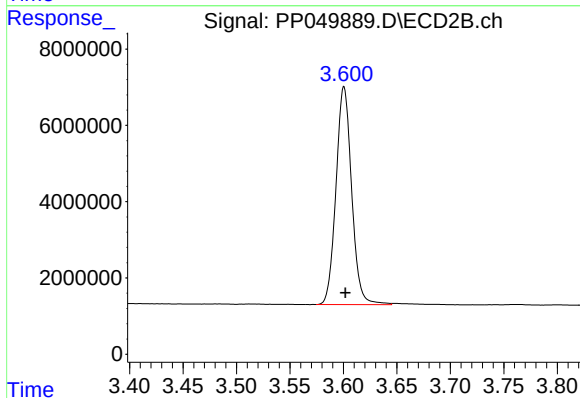


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.001 min
Response: 58340550
Conc: 23.87 ng/ml

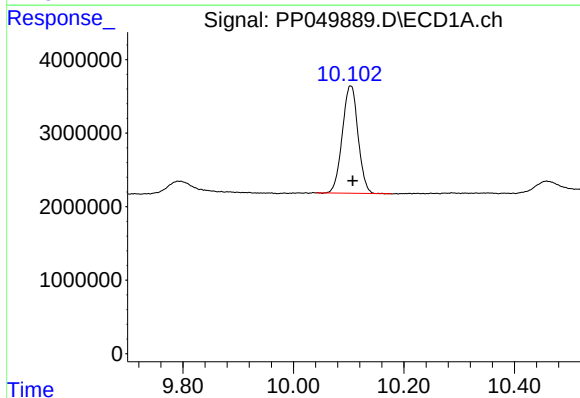

#2 Decachlorobiphenyl

R.T.: 10.103 min
Delta R.T.: -0.004 min
Response: 28867584
Conc: 20.41 ng/ml

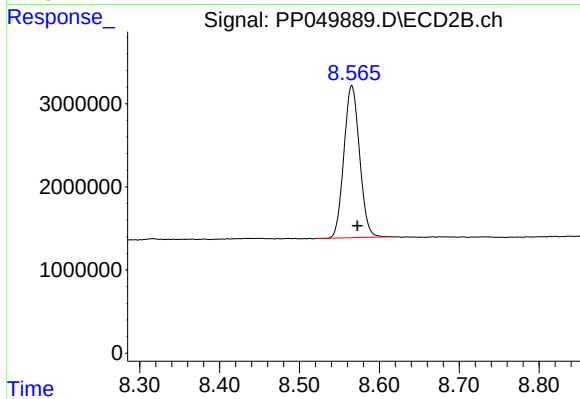

#2 Decachlorobiphenyl

R.T.: 8.566 min
Delta R.T.: -0.007 min
Response: 24859316
Conc: 21.35 ng/ml