

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072722\
 Data File : PP049904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 23:55
 Operator : YP\AJ
 Sample : N3905-05 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KZZ049W-(1-1)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/28/2022
 Supervised By :Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 05:31:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.349	3.599	2963425	4034665	2.042m	1.651m
2) SA Decachlor...	10.101	8.564	2289394	2024103	1.619m	1.738m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072722\
Data File : PP049904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 23:55
Operator : YP\AJ
Sample : N3905-05 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KZZ049W-(1-1)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 05:31:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

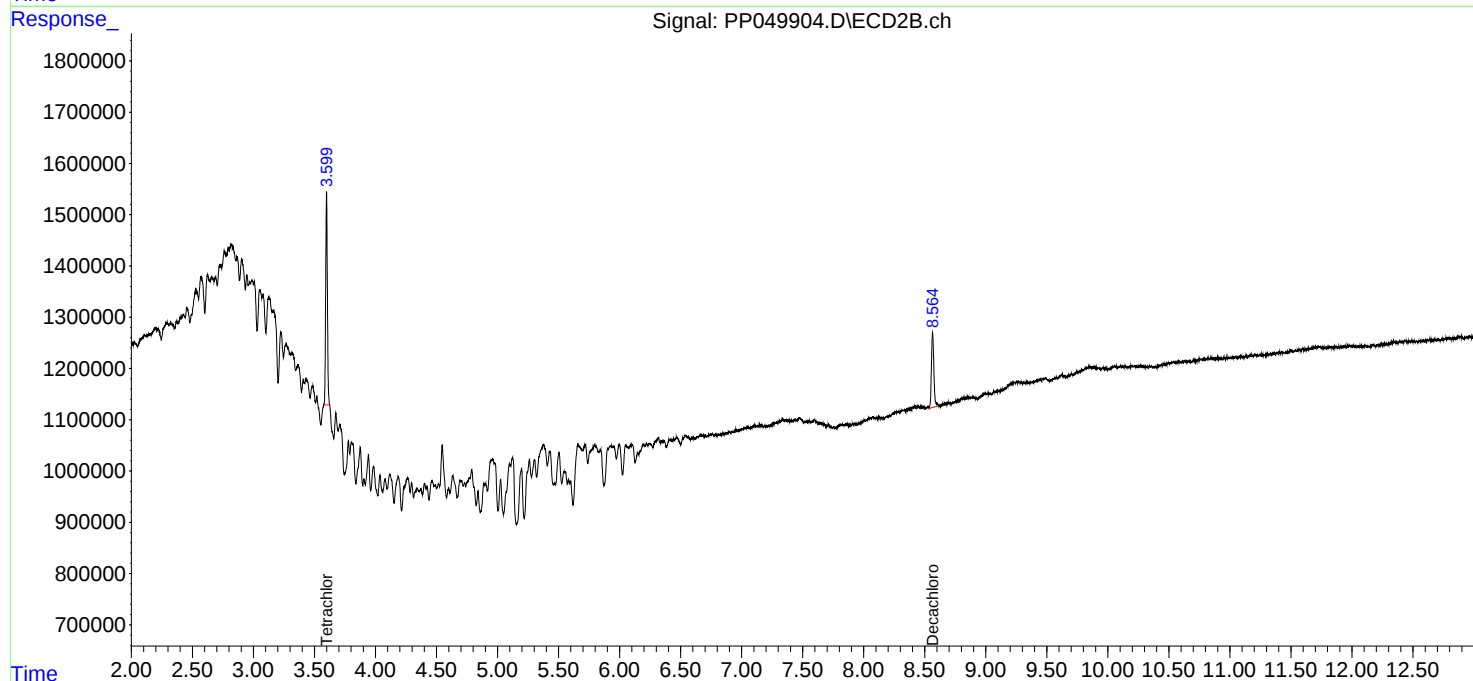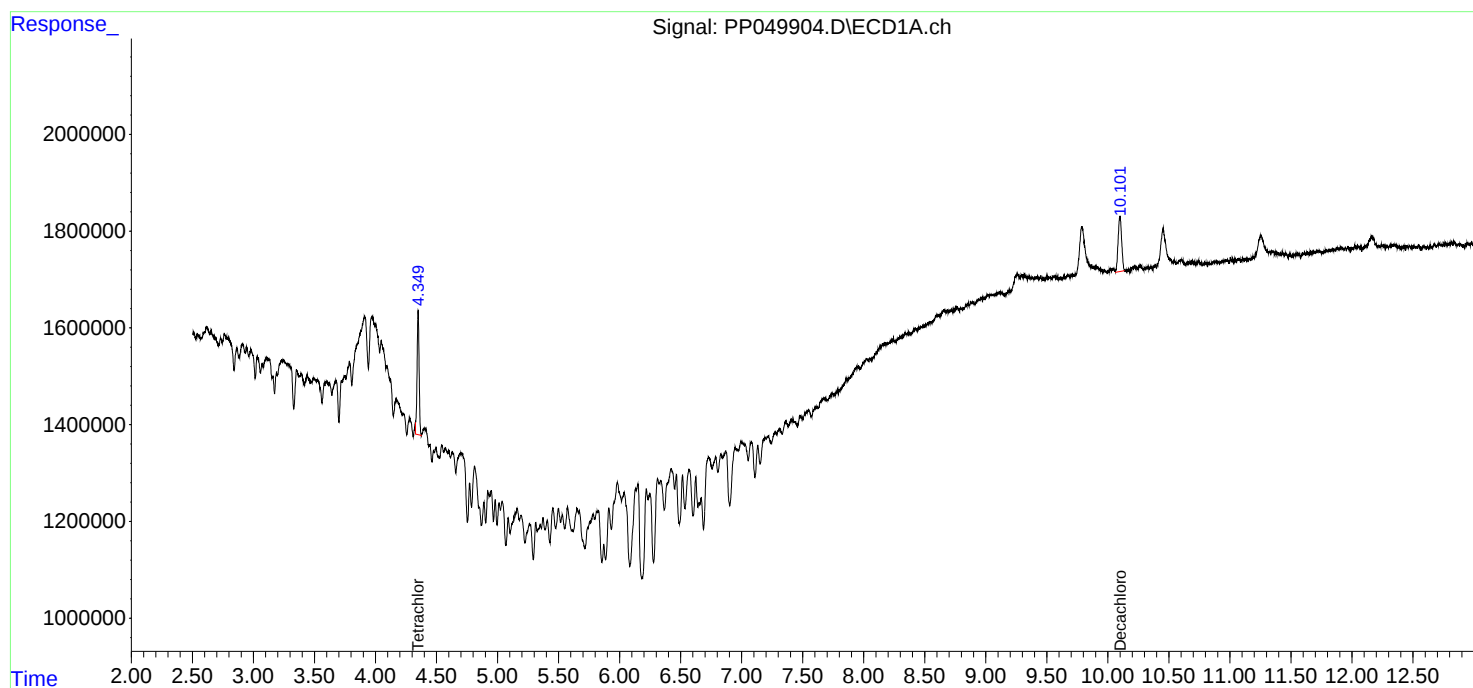

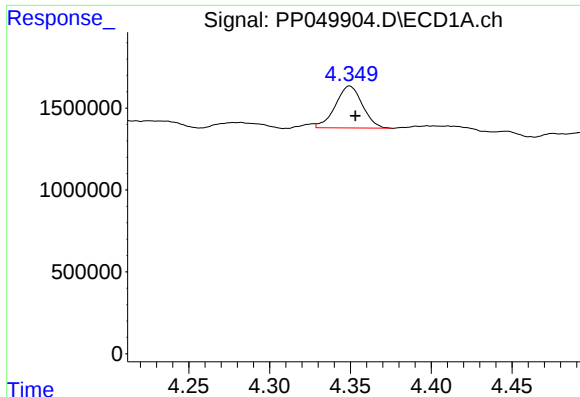


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: -0.004 min
Response: 2963425
Conc: 2.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ049W-(1-1)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

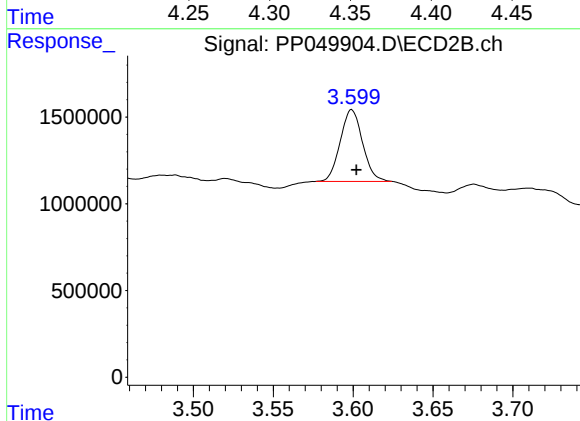


#1 Tetrachloro-m-xylene

R.T.: 3.599 min
Delta R.T.: -0.003 min
Response: 4034665
Conc: 1.65 ng/ml m

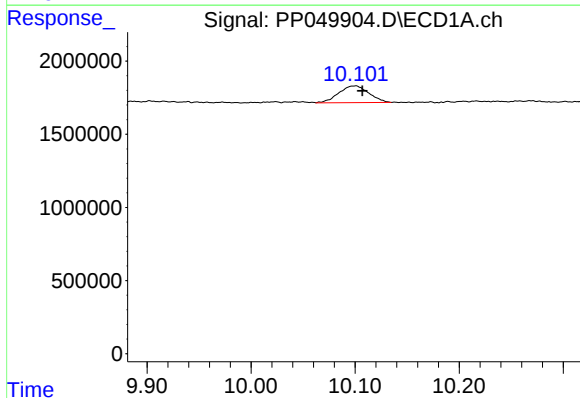

#2 Decachlorobiphenyl

R.T.: 10.101 min
Delta R.T.: -0.006 min
Response: 2289394
Conc: 1.62 ng/ml m

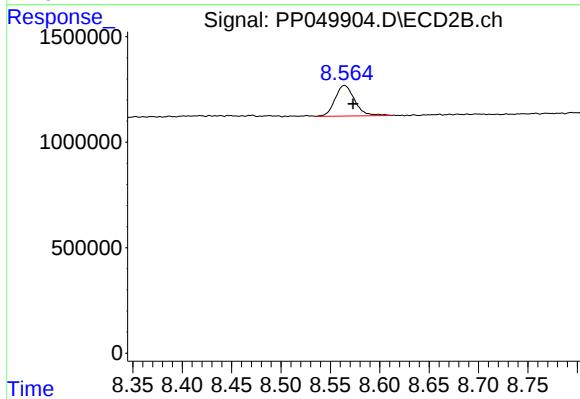

#2 Decachlorobiphenyl

R.T.: 8.564 min
Delta R.T.: -0.009 min
Response: 2024103
Conc: 1.74 ng/ml m