

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072722\
 Data File : PP049909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2022 01:18
 Operator : YP\AJ
 Sample : N3909-02 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-HEH769N-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/28/2022
 Supervised By :Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 05:52:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.349	3.599	2895064	4702279	1.995m	1.924
2) SA Decachlor...	10.100	8.564	2490946	2100579	1.761m	1.804

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072722\
Data File : PP049909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2022 01:18
Operator : YP\AJ
Sample : N3909-02 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-HEH769N-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 05:52:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

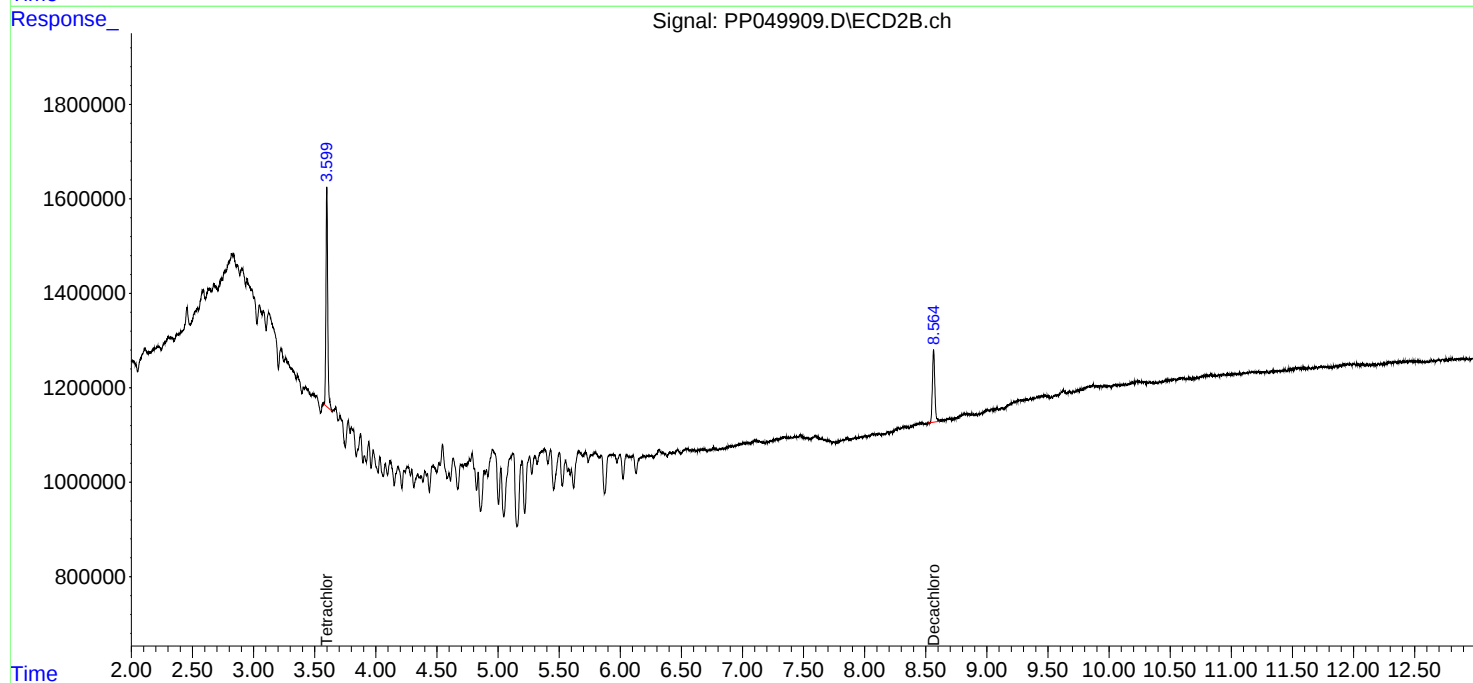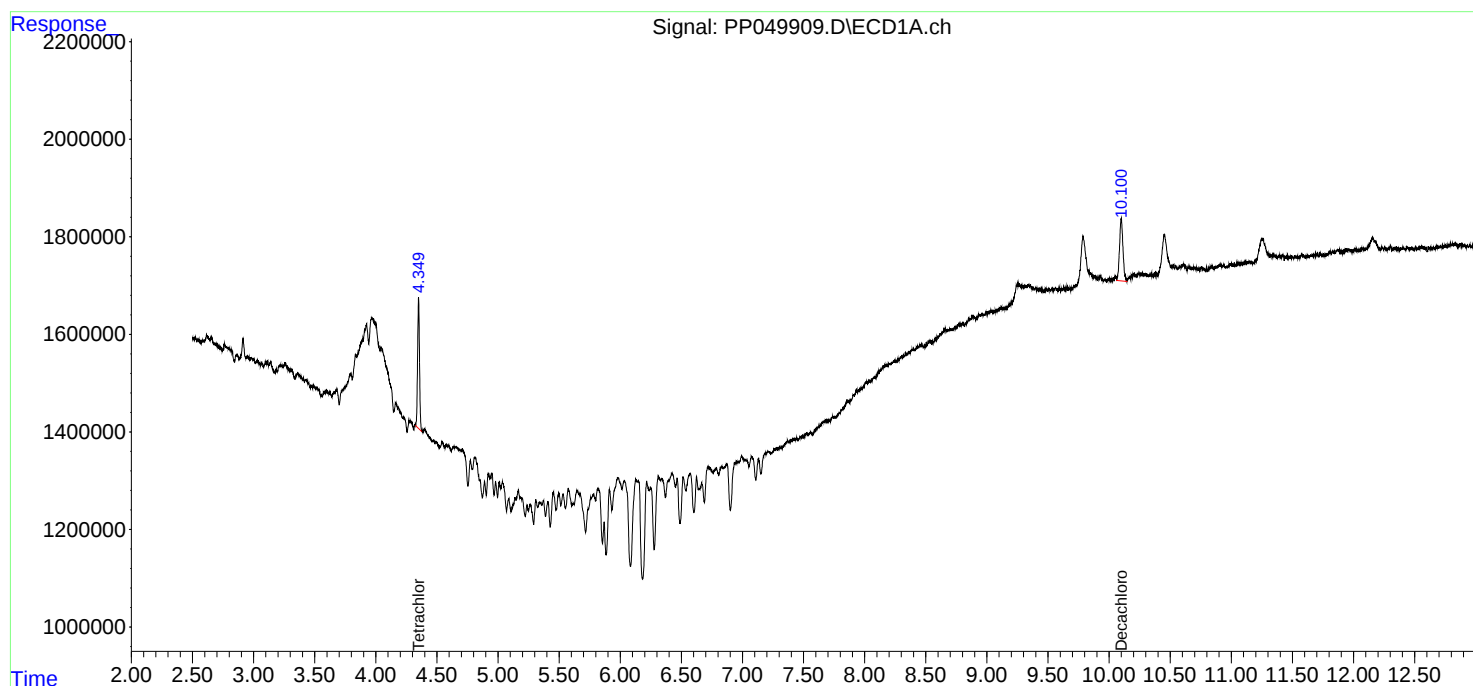

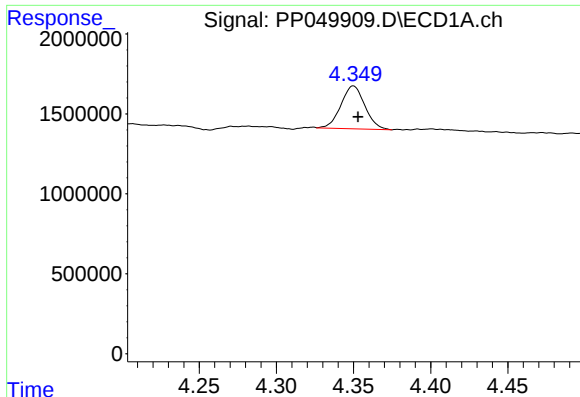


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: -0.004 min
Response: 2895064
Conc: 2.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-HEH769N-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

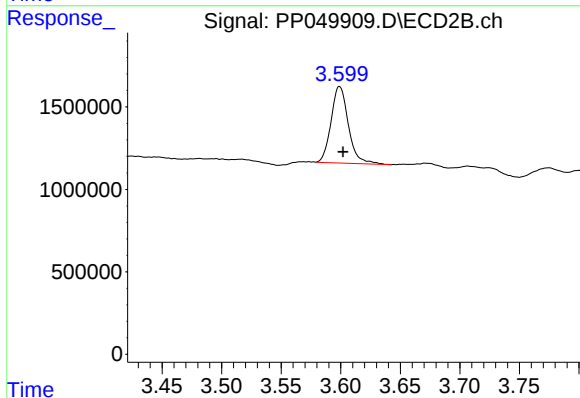


#1 Tetrachloro-m-xylene

R.T.: 3.599 min
Delta R.T.: -0.003 min
Response: 4702279
Conc: 1.92 ng/ml

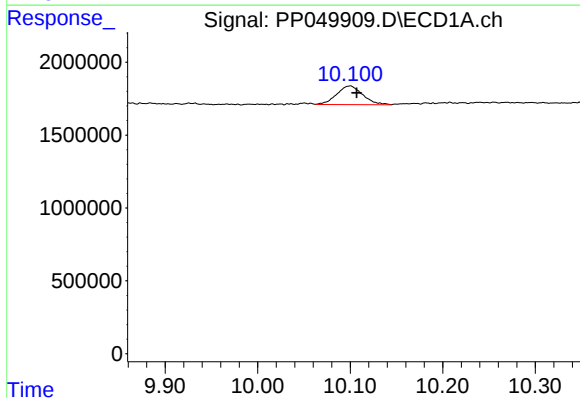

#2 Decachlorobiphenyl

R.T.: 10.100 min
Delta R.T.: -0.007 min
Response: 2490946
Conc: 1.76 ng/ml m

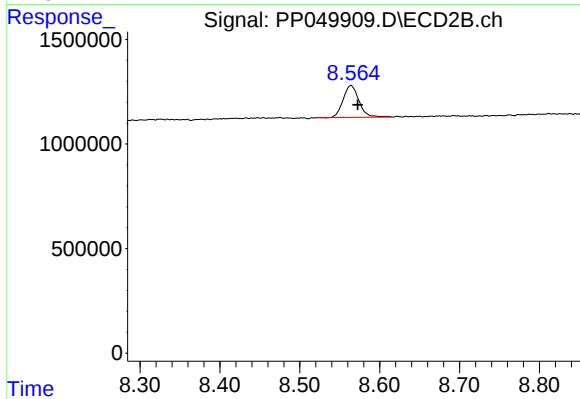

#2 Decachlorobiphenyl

R.T.: 8.564 min
Delta R.T.: -0.009 min
Response: 2100579
Conc: 1.80 ng/ml